


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120224\
Data File : BF140680.D
Acq On : 02 Dec 2024 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

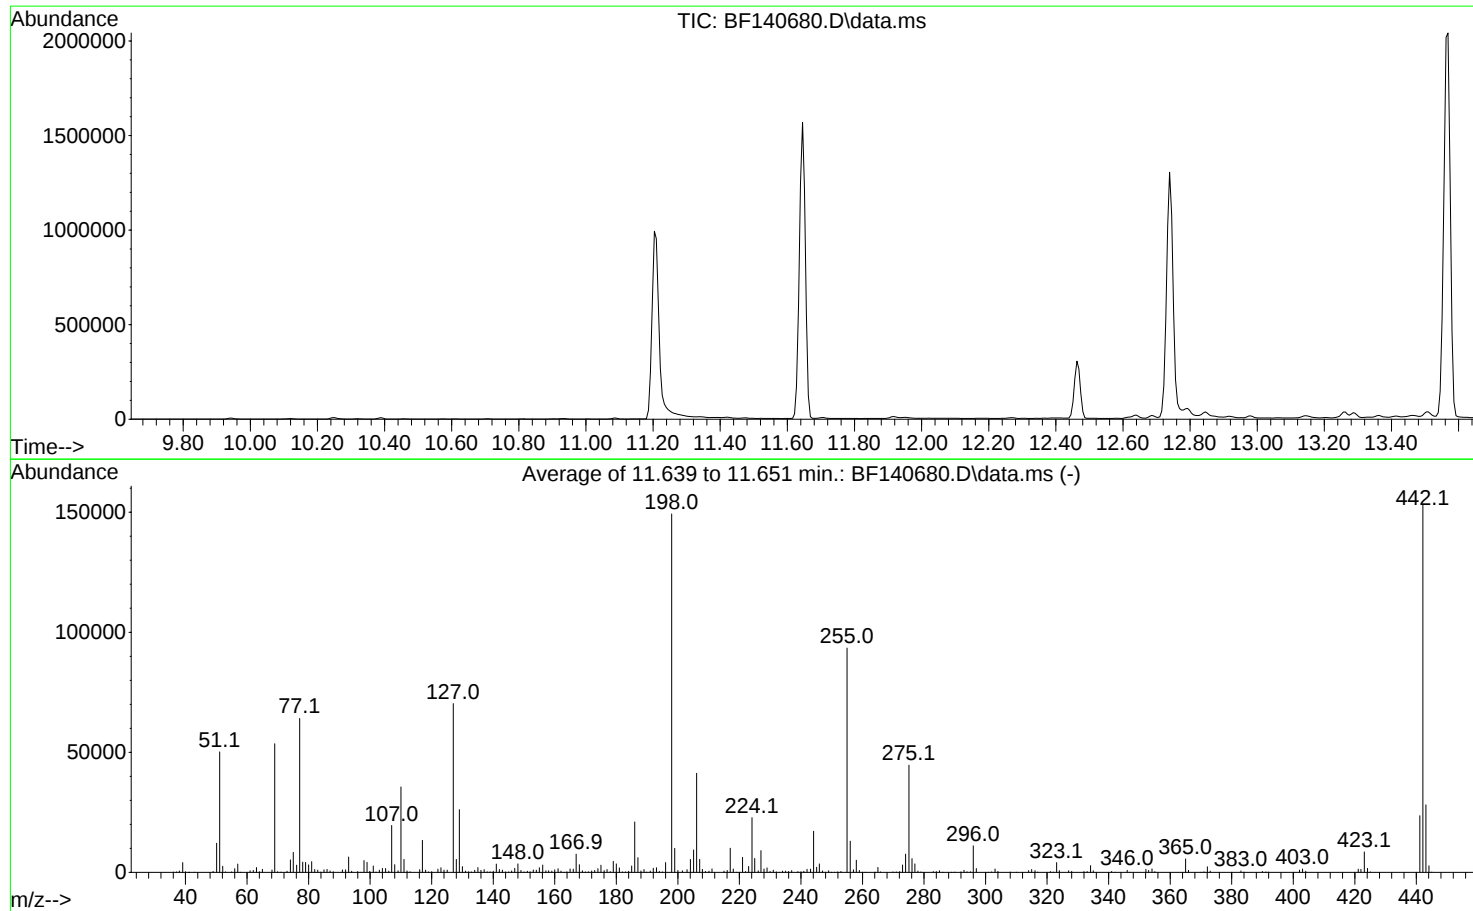

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	50173	PASS
68	69	0.00	2	1.9	999	PASS
69	198	0.00	100	35.9	53580	PASS
70	69	0.00	2	0.5	280	PASS
127	198	10	80	47.1	70339	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	149269	PASS
199	198	5	9	6.7	10008	PASS
275	198	10	60	29.9	44685	PASS
365	198	1	100	3.8	5603	PASS
441	198	0.01	100	15.8	23611	PASS
442	442	50	100	100.0	153221	PASS
443	442	15	24	18.4	28133	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/2/2024	BNA_F	<u>BF140680.D</u>
Compound Name	Response	Retention Time
DDT	546879	13.568
DDD	16061	13.263
DDE	2435	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18496	565375	3.27

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120224\
Data File : BF140680.D
Acq On : 02 Dec 2024 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 02 10:53:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

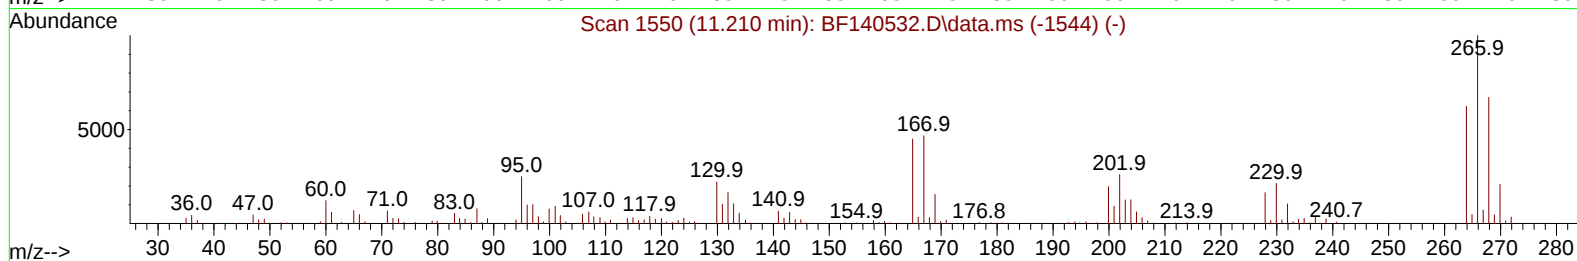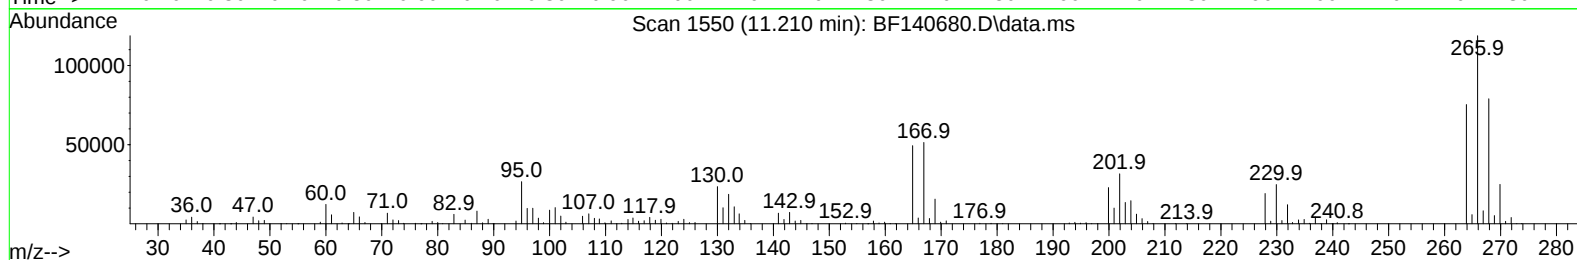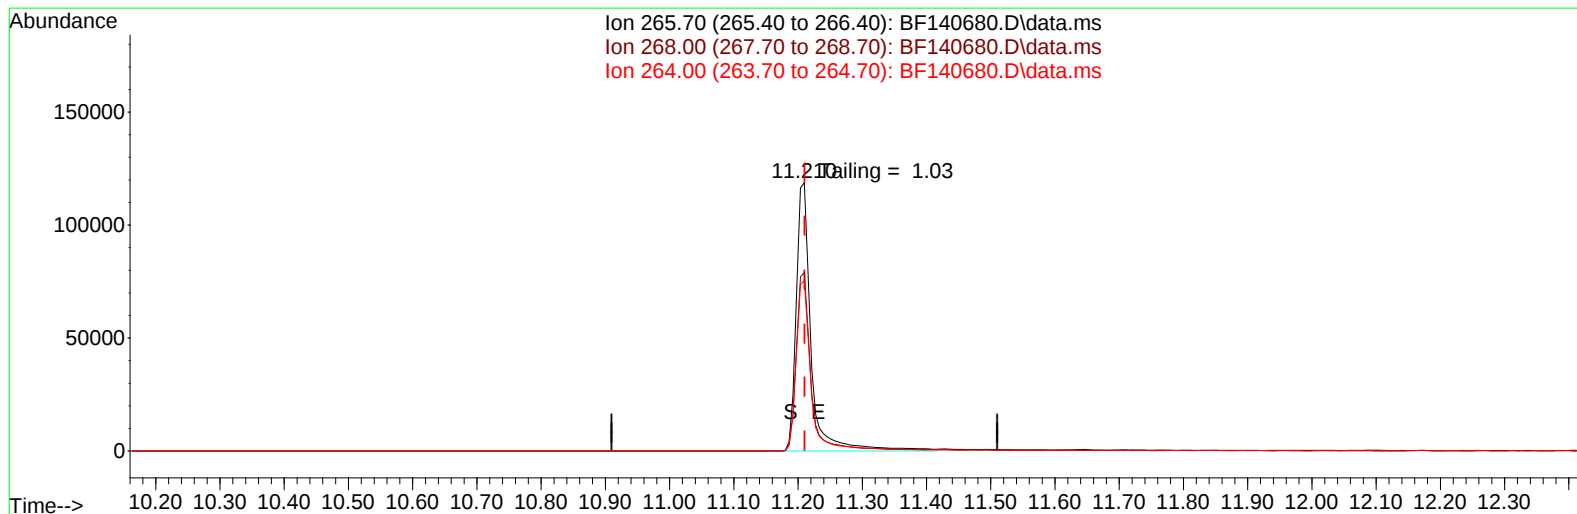

TIC: BF140680.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 19742.67 ng




response 192207

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	66.55
264.00	62.30	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120224\
Data File : BF140680.D
Acq On : 02 Dec 2024 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 02 10:53:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

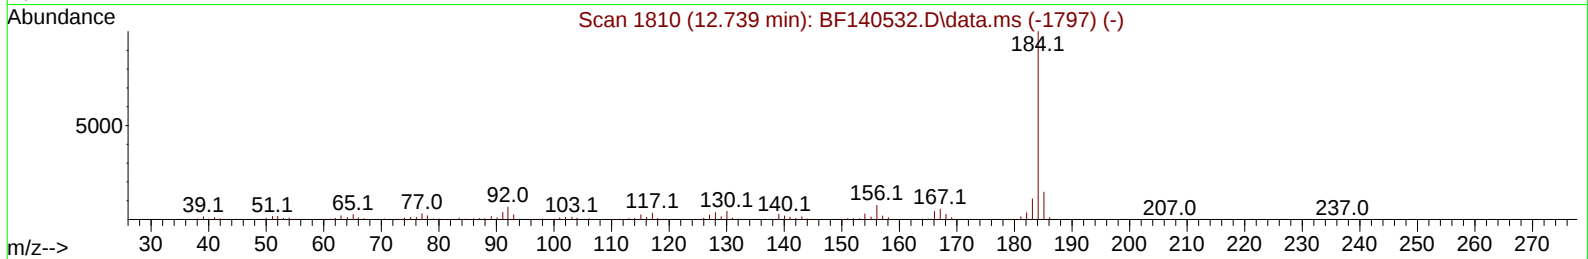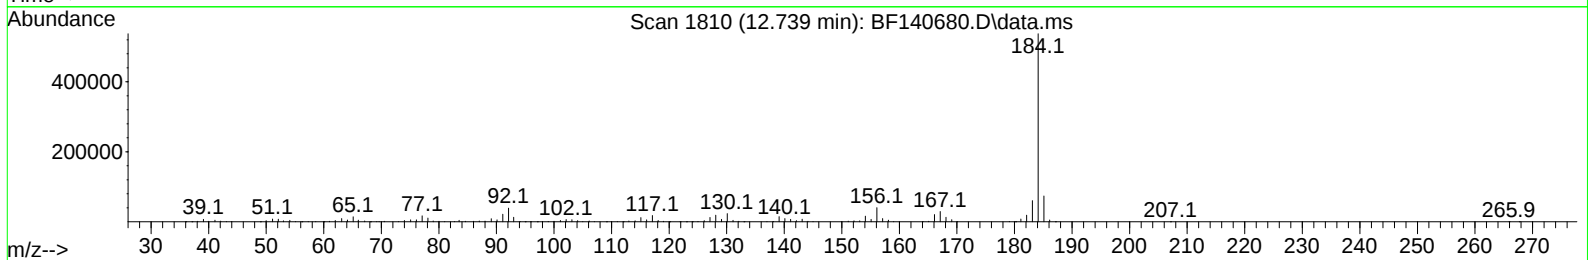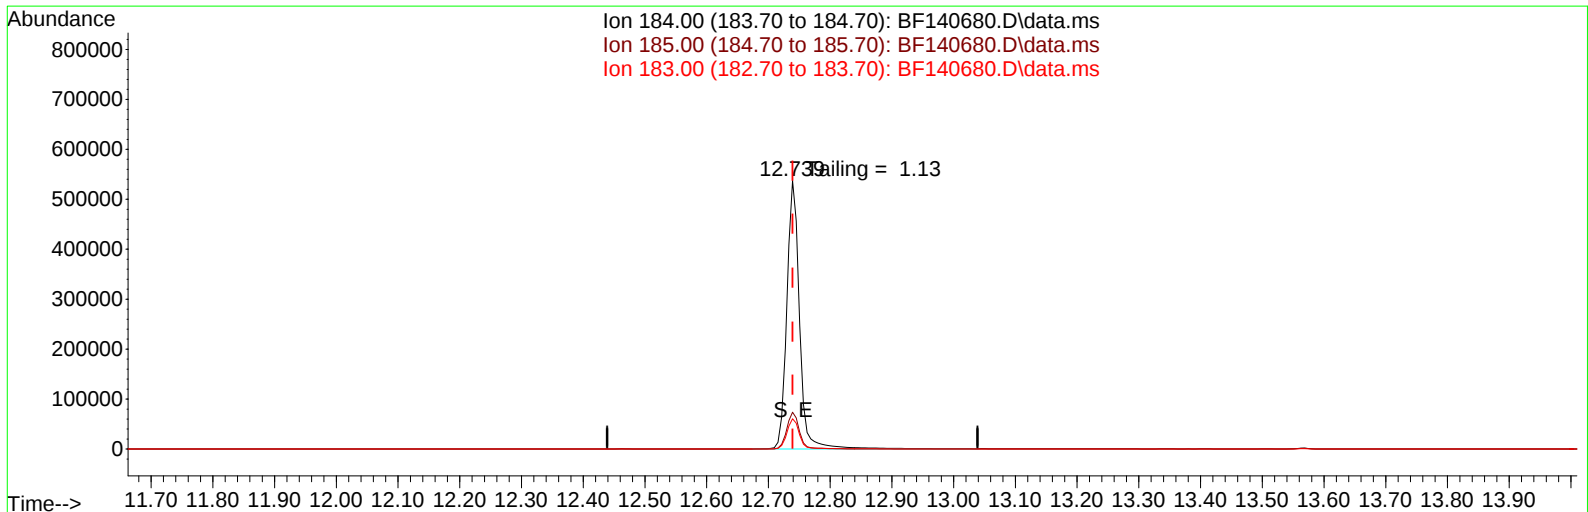

TIC: BF140680.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 18798.86 ng

response 775031

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.73
183.00	11.00	11.31
0.00	0.00	0.00