
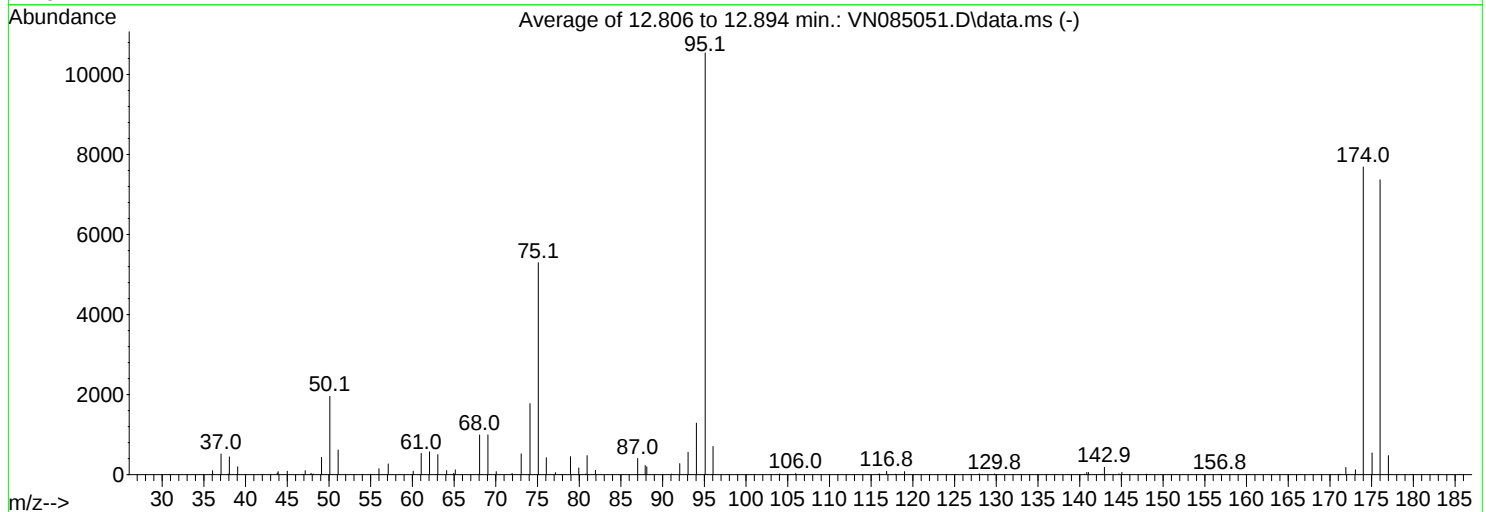


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112724\
Data File : VN085051.D
Acq On : 27 Nov 2024 08:30
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N103124W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Nov 01 02:38:04 2024

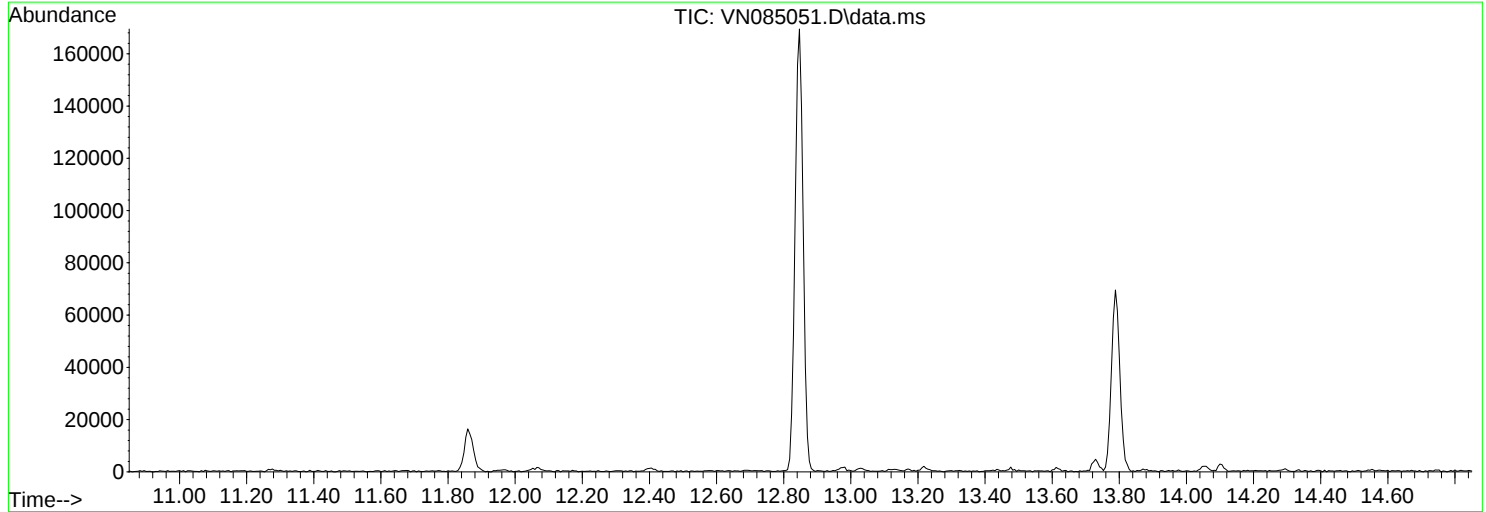

AutoFind: Averaged scan 1845 to 1860; Bkg corrected with scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	1956	PASS
75	95	30	60	50.3	5300	PASS
95	95	100	100	100.0	10541	PASS
96	95	5	9	6.7	704	PASS
173	174	0.00	2	1.6	122	PASS
174	95	50	100	73.0	7691	PASS
175	174	5	9	7.1	544	PASS
176	174	95	101	95.8	7371	PASS
177	176	5	9	6.4	474	PASS