


LB133702

7470A

INSTRUMENT ID: CV1

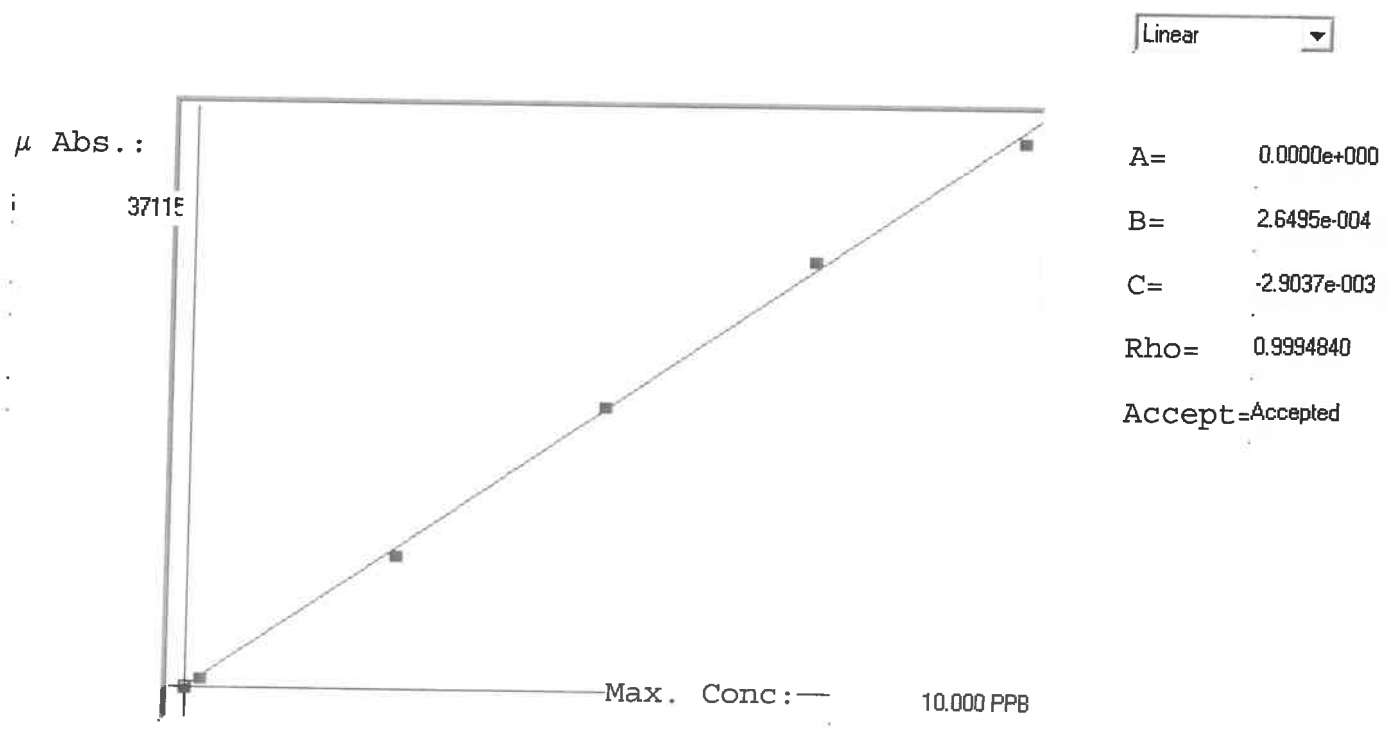

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	Diob
0.0	0.000	0.002	0.002	17	0.000	17	0				1
0.2	0.200	0.195	-0.005	747	0.0 %	747					-3
2.5	2.500	2.395	-0.105	9049	0.0 %	9049					-4
5.0	5.000	5.085	0.085	19203	0.0 %	19203					2
7.5	7.500	7.693	0.193	29047	0.0 %	29047					3
10.0	10.000	9.831	-0.169	37115	0.0 %	37115					-2

LB133702 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 03 Dec 2024 10:22:47

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	17	-	0.0000	7470A	PPB	03 Dec 2024 10:31:09	S	Std
0.2 - 1	50.2	747	-	0.2000	7470A	PPB	03 Dec 2024 10:33:26	S	Std
2.5 - 1	52.5	9049	-	2.5000	7470A	PPB	03 Dec 2024 10:35:43	S	Std
5.0 - 1	55	19203	-	5.0000	7470A	PPB	03 Dec 2024 10:38:00	S	Std
7.5 - 1	57.5	29047	-	7.5000	7470A	PPB	03 Dec 2024 10:50:26	S	Std
10.0 - 1	510	37115	-	10.0000	7470A	PPB	03 Dec 2024 10:55:22	S	Std
ICV109 - 1	ICV109	14324	3.7922	-	7470A	PPB	03 Dec 2024 10:58:11	U	SMPL
ICB109 - 1	ICB109	-231	-0.0641	-	7470A	PPB	03 Dec 2024 11:00:26	U	SMPL
CCV75 - 1	CCV75	19521	5.1692	-	7470A	PPB	03 Dec 2024 11:02:42	U	SMPL
CCB75 - 1	CCB75	-242	-0.0670	-	7470A	PPB	03 Dec 2024 11:04:57	U	SMPL
CRA - 1	CRA	635	0.1653	-	7470A	PPB	03 Dec 2024 11:07:14	U	SMPL
HighStd - 1	HighStd	36867	9.7650	-	7470A	PPB	03 Dec 2024 11:09:29	U	SMPL
ChkStd - 1	ChkStd	24604	6.5159	-	7470A	PPB	03 Dec 2024 11:11:44	U	SMPL
PB165334BL - 1	PBW	-96	-0.0283	-	7470A	PPB	03 Dec 2024 11:14:02	U	SMPL
PB165334BS - 1	LCSW	14228	3.7668	-	7470A	PPB	03 Dec 2024 11:19:37	U	SMPL
P5005-02 - 1	STOCK-PILE	-210	-0.0585	-	7470A	PPB	03 Dec 2024 11:21:52	U	SMPL
P5025-02 - 1	SOIL-WEST	-49	-0.0159	-	7470A	PPB	03 Dec 2024 11:24:10	U	SMPL
P5025-06 - 1	SOIL-EAST	-26	-0.0098	-	7470A	PPB	03 Dec 2024 11:26:27	U	SMPL
P5026-02 - 1	SOIL-1-HAM	134	0.0326	-	7470A	PPB	03 Dec 2024 11:28:43	U	SMPL
P5026-06 - 1	SOIL-1-HAM	43	0.0085	-	7470A	PPB	03 Dec 2024 11:30:58	U	SMPL
CCV76 - 1	CCV76	19043	5.0425	-	7470A	PPB	03 Dec 2024 11:33:14	U	SMPL
CCB76 - 1	CCB76	-246	-0.0681	-	7470A	PPB	03 Dec 2024 11:35:29	U	SMPL
P5048-04 - 1	MH-746-WC	-6	-0.0045	-	7470A	PPB	03 Dec 2024 11:37:47	U	SMPL
P5048-04DUP - 1	MH-746-WCDUP	171	0.0424	-	7470A	PPB	03 Dec 2024 11:40:02	U	SMPL
P5048-04MS - 1	MH-746-WCMS	14461	3.8285	-	7470A	PPB	03 Dec 2024 11:42:17	U	SMPL
P5048-04MSD - 1	MH-746-WCMSD	15414	4.0810	-	7470A	PPB	03 Dec 2024 11:44:32	U	SMPL
PB165335BL - 1	PBW	-277	-0.0763	-	7470A	PPB	03 Dec 2024 11:46:50	U	SMPL
PB165335BS - 1	LCSW	16285	4.3118	-	7470A	PPB	03 Dec 2024 11:49:08	U	SMPL
P5006-18 - 1	TW-WTS-02	-88	-0.0262	-	7470A	PPB	03 Dec 2024 11:51:24	U	SMPL
P5031-01 - 1	286127	960	0.2514	-	7470A	PPB	03 Dec 2024 11:58:41	U	SMPL
P5031-01DUP - 1	286127DUP	818	0.2138	-	7470A	PPB	03 Dec 2024 12:04:00	U	SMPL
P5031-01MS - 1	286127MS	15957	4.2249	-	7470A	PPB	03 Dec 2024 12:06:15	U	SMPL
CCV77 - 1	CCV77	19697	5.2158	-	7470A	PPB	03 Dec 2024 12:08:31	U	SMPL
CCB77 - 1	CCB77	-177	-0.0498	-	7470A	PPB	03 Dec 2024 12:10:48	U	SMPL
P5031-01MSD - 1	286127MSD	16190	4.2866	-	7470A	PPB	03 Dec 2024 12:13:05	U	SMPL
PB165297TB - 1	PB165297TB	-148	-0.0421	-	7470A	PPB	03 Dec 2024 12:15:20	U	SMPL
P5048-04LX5 - 1		-18	-0.0077	-	7470A	PPB	03 Dec 2024 12:17:37	U	SMPL
P5048-04A - 1		14697	3.8911	-	7470A	PPB	03 Dec 2024 12:19:53	U	SMPL
P5031-01LX5 - 1		70	0.0156	-	7470A	PPB	03 Dec 2024 12:22:08	U	SMPL
P5031-01A - 1		14984	3.9671	-	7470A	PPB	03 Dec 2024 12:24:25	U	SMPL
CCV78 - 1	CCV78	20151	5.3361	-	7470A	PPB	03 Dec 2024 12:29:21	U	SMPL
CCB78 - 1	CCB78	-156	-0.0442	-	7470A	PPB	03 Dec 2024 12:31:40	U	SMPL