

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

LAB CHRONICLE

OrderID:	P5026	OrderDate:	11/27/2024 11:24:00 AM
Client:	Tully Construction Co., Inc.	Project:	Hamilton
Contact:	Dean Devoe	Location:	L61,VOA Ref. #2 Soil

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
P5026-01	SOIL-1-HAM	SOIL	PCB	8082A	11/27/24	12/02/24	12/02/24	11/27/24
P5026-03	SOIL-1-HAM-TPH2	SOIL	TPH GC	8015D	11/27/24	12/02/24	12/02/24	11/27/24
P5026-05	SOIL-1-HAM	SOIL	PCB	8082A	11/27/24	12/02/24	12/02/24	11/27/24
P5026-07	SOIL-1-HAM-TPH2	SOIL	TPH GC	8015D	11/27/24	12/02/24	12/02/24	11/27/24



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: P5026

Order ID: P5026

Client: Tully Construction Co., Inc.

Project ID: Hamilton

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------

Client ID :

Total Concentration: 0.000



QC SUMMARY

Surrogate Summary

SDG No.: **P5026**

Client: **Tully Construction Co., Inc.**

Analytical Method: **8082A**

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Rec	Qual	Limits	
								Low	High
I.BLK-PO108037.D	PIBLK-PO108037.D	Tetrachloro-m-xylene	1	20	21.2	106		60	140
		Decachlorobiphenyl	1	20	23.2	116		60	140
		Tetrachloro-m-xylene	2	20	21.0	105		60	140
		Decachlorobiphenyl	2	20	22.5	112		60	140
I.BLK-PO108279.D	PIBLK-PO108279.D	Tetrachloro-m-xylene	1	20	22.8	114		60	140
		Decachlorobiphenyl	1	20	25.1	126		60	140
		Tetrachloro-m-xylene	2	20	24.0	120		60	140
		Decachlorobiphenyl	2	20	22.1	111		60	140
PB165309BL	PB165309BL	Tetrachloro-m-xylene	1	20	21.6	108		32	144
		Decachlorobiphenyl	1	20	23.3	116		32	175
		Tetrachloro-m-xylene	2	20	22.3	111		32	144
		Decachlorobiphenyl	2	20	20.9	105		32	175
PB165309BS	PB165309BS	Tetrachloro-m-xylene	1	20	21.2	106		32	144
		Decachlorobiphenyl	1	20	22.9	115		32	175
		Tetrachloro-m-xylene	2	20	20.6	103		32	144
		Decachlorobiphenyl	2	20	20.6	103		32	175
P5026-01	SOIL-1-HAM	Tetrachloro-m-xylene	1	20	18.9	94		32	144
		Decachlorobiphenyl	1	20	15.5	78		32	175
		Tetrachloro-m-xylene	2	20	21.2	106		32	144
		Decachlorobiphenyl	2	20	12.3	62		32	175
P5026-05		Tetrachloro-m-xylene	1	20	17.4	87		32	144
		Decachlorobiphenyl	1	20	14.3	72		32	175
		Tetrachloro-m-xylene	2	20	20.6	103		32	144
		Decachlorobiphenyl	2	20	12.0	60		32	175
P5026-05MS	SOIL-1-HAMMS	Tetrachloro-m-xylene	1	20	18.6	93		32	144
		Decachlorobiphenyl	1	20	16.5	82		32	175
		Tetrachloro-m-xylene	2	20	20.0	100		32	144
		Decachlorobiphenyl	2	20	13.5	68		32	175
P5026-05MSD	SOIL-1-HAMMSD	Tetrachloro-m-xylene	1	20	19.0	95		32	144
		Decachlorobiphenyl	1	20	16.4	82		32	175
		Tetrachloro-m-xylene	2	20	19.8	99		32	144
		Decachlorobiphenyl	2	20	13.8	69		32	175
I.BLK-PO108294.D	PIBLK-PO108294.D	Tetrachloro-m-xylene	1	20	22.9	115		60	140
		Decachlorobiphenyl	1	20	24.8	124		60	140
		Tetrachloro-m-xylene	2	20	24.4	122		60	140
		Decachlorobiphenyl	2	20	20.8	104		60	140

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: P5026

Client: Tully Construction Co., Inc.

Analytical Method: 8082A

DataFile : PO108286.D

Lab Sample ID:	Parameter	Spike	Sample		Units	Rec	Rec		RPD		Limits	RPD
			Result	Result			Qual	RPD	Qual	Low	High	
Client Sample ID: P5026-05MS	SOIL-1-HAMMS											
	AR1016	214.2	0	200	ug/kg	93				55	146	
	AR1260	214.2	0	165	ug/kg	77				45	144	

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: P5026

Client: Tully Construction Co., Inc.

Analytical Method: 8082A

DataFile : PO108287.D

Lab Sample ID:	Parameter	Spike	Sample		Units	Rec	Rec		RPD		Limits	
			Result	Result			Qual	RPD	Qual	Low	High	RPD
Client Sample ID: P5026-05MSD	SOIL-1-HAMMSD											
	AR1016	213.8	0	199	ug/kg	93		0		55	146	20
	AR1260	213.8	0	168	ug/kg	79		3		45	144	20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: P5026

Client: Tully Construction Co., Inc.

Analytical Method: **8082A** **Datafile :** PO108281.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD		Limits	
								Qual	Low	High	RPD
PB165309BS	AR1016	166.6	166	ug/kg	100				71	120	
	AR1260	166.6	158	ug/kg	95				65	130	

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB165309BL

Lab Name: CHEMTECH

Contract: TULL02

Lab Code: CHEM Case No.: P5026

SAS No.: P5026 SDG NO.: P5026

Lab Sample ID: PB165309BL

Lab File ID: PO108280.D

Matrix: (soil/water) Solid

Extraction: (Type) _____

Sulfur Cleanup: (Y/N) N

Date Extracted: 12/02/2024

Date Analyzed (1): 12/02/2024

Date Analyzed (2): 12/02/2024

Time Analyzed (1): 12:20

Time Analyzed (2): 12:20

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column (1): ZB-MR1 ID: 0.32 (mm)

GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
PB165309BS	PB165309BS	PO108281.D	12/02/2024	12/02/2024
SOIL-1-HAM	P5026-01	PO108284.D	12/02/2024	12/02/2024
SOIL-1-HAM	P5026-05	PO108285.D	12/02/2024	12/02/2024
SOIL-1-HAMMS	P5026-05MS	PO108286.D	12/02/2024	12/02/2024
SOIL-1-HAMMSD	P5026-05MSD	PO108287.D	12/02/2024	12/02/2024

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	Tully Construction Co., Inc.	Date Collected:	11/27/24
Project:	Hamilton	Date Received:	11/27/24
Client Sample ID:	SOIL-1-HAM	SDG No.:	P5026
Lab Sample ID:	P5026-01	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	79.4
Sample Wt/Vol:	30.05	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108284.D	1	12/02/24 08:20	12/02/24 13:26	PB165309

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	0.0043	U	0.0043	0.021	mg/Kg
11104-28-2	Aroclor-1221	0.0081	U	0.0081	0.021	mg/Kg
11141-16-5	Aroclor-1232	0.0043	U	0.0043	0.021	mg/Kg
53469-21-9	Aroclor-1242	0.0043	U	0.0043	0.021	mg/Kg
12672-29-6	Aroclor-1248	0.0099	U	0.0099	0.021	mg/Kg
11097-69-1	Aroclor-1254	0.0034	U	0.0034	0.021	mg/Kg
37324-23-5	Aroclor-1262	0.0057	U	0.0057	0.021	mg/Kg
11100-14-4	Aroclor-1268	0.0043	U	0.0043	0.021	mg/Kg
11096-82-5	Aroclor-1260	0.0037	U	0.0037	0.021	mg/Kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.2		32 - 144	106%	SPK: 20
2051-24-3	Decachlorobiphenyl	15.5		32 - 175	78%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
 Data File : PO108284.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2024 13:26
 Operator : YP/AJ
 Sample : P5026-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SOIL-1-HAM

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/03/2024
 Supervised By :Ankita Jodhani 12/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 00:34:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

 System Monitoring Compounds

1) SA Tetrachlo...	4.371	3.637	164.4E6	71729644	18.884m	21.157
2) SA Decachlor...	10.096	8.632	47354201	41947919	15.505	12.331

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
Data File : PO108284.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2024 13:26
Operator : YP/AJ
Sample : P5026-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SOIL-1-HAM


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/03/2024
Supervised By :Ankita Jodhani 12/03/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 00:34:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

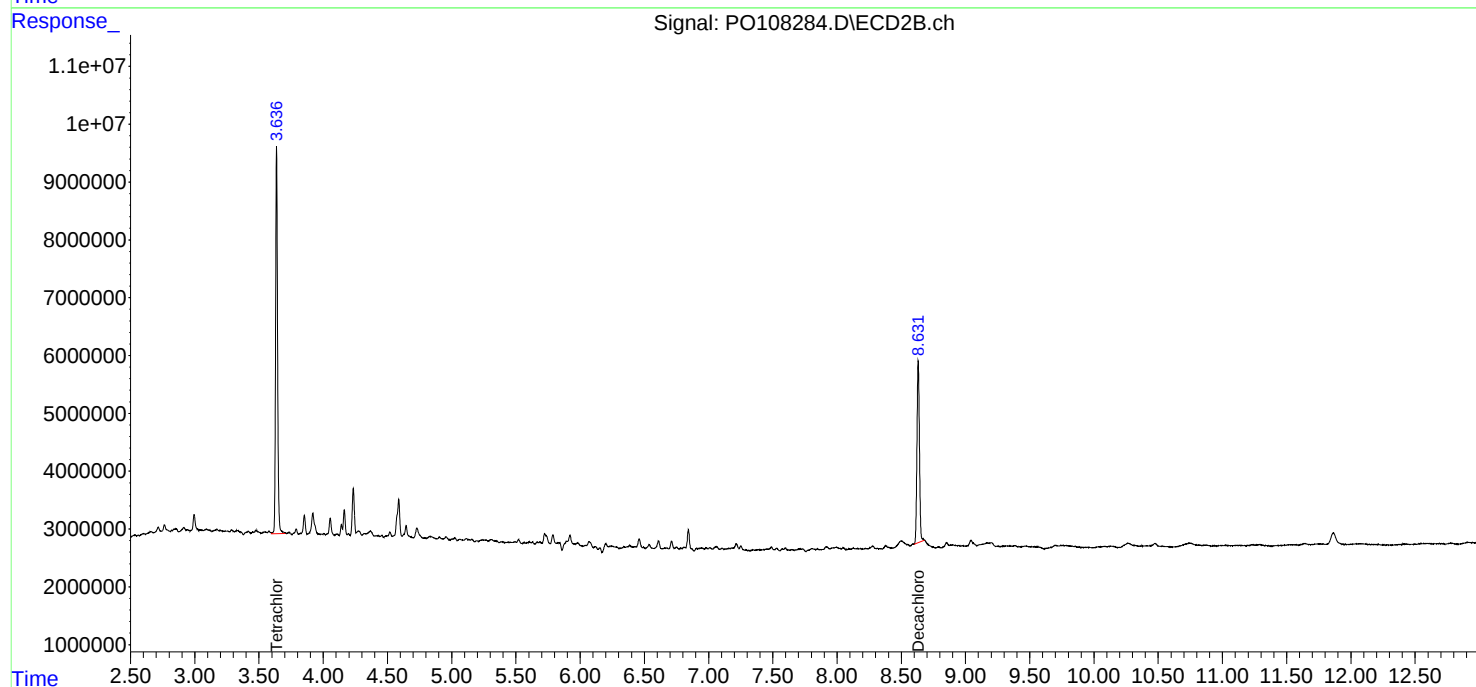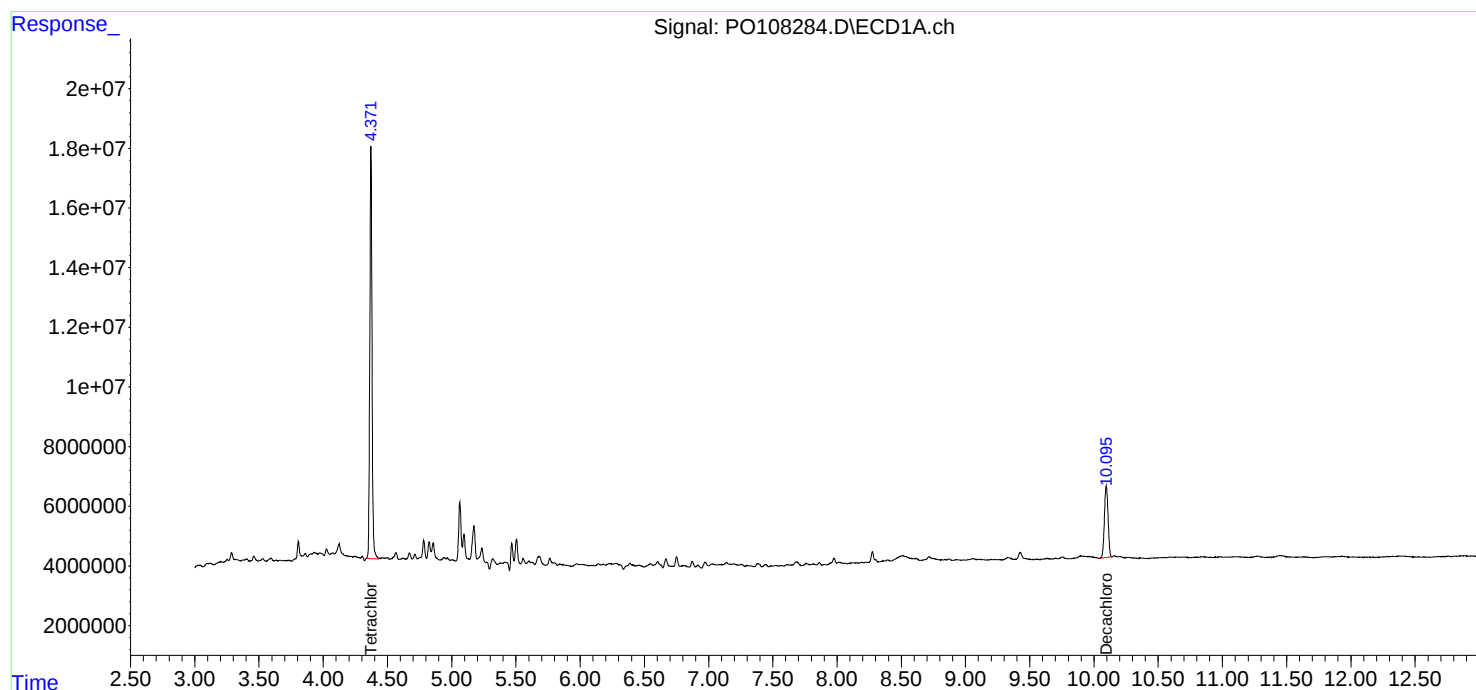

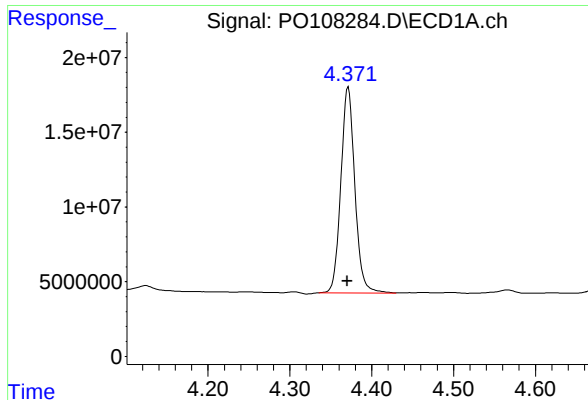


#1 Tetrachloro-m-xylene

R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 164402792
Conc: 18.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
SOIL-1-HAM


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/03/2024
Supervised By :Ankita Jodhani 12/03/2024

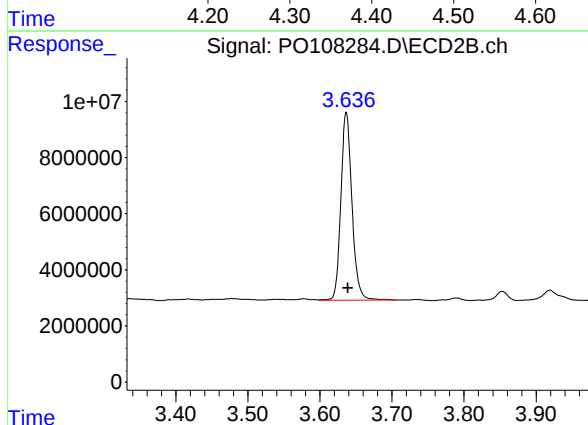


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 71729644
Conc: 21.16 ng/ml

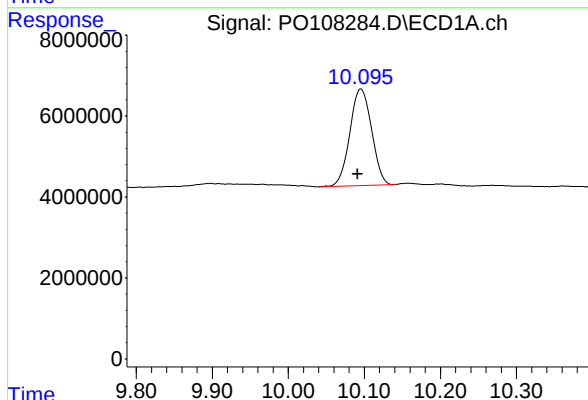

#2 Decachlorobiphenyl

R.T.: 10.096 min
Delta R.T.: 0.004 min
Response: 47354201
Conc: 15.50 ng/ml

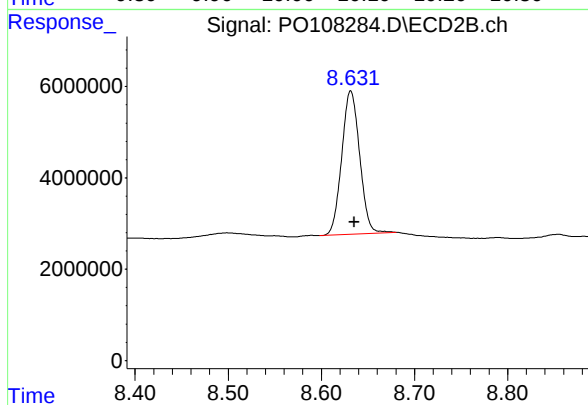

#2 Decachlorobiphenyl

R.T.: 8.632 min
Delta R.T.: -0.004 min
Response: 41947919
Conc: 12.33 ng/ml

Report of Analysis

Client:	Tully Construction Co., Inc.	Date Collected:	11/27/24
Project:	Hamilton	Date Received:	11/27/24
Client Sample ID:	SOIL-1-HAM	SDG No.:	P5026
Lab Sample ID:	P5026-05	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	77.8
Sample Wt/Vol:	30.03	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108285.D	1	12/02/24 08:20	12/02/24 13:43	PB165309

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	0.0044	U	0.0044	0.022	mg/Kg
11104-28-2	Aroclor-1221	0.0082	U	0.0082	0.022	mg/Kg
11141-16-5	Aroclor-1232	0.0044	U	0.0044	0.022	mg/Kg
53469-21-9	Aroclor-1242	0.0044	U	0.0044	0.022	mg/Kg
12672-29-6	Aroclor-1248	0.010	U	0.010	0.022	mg/Kg
11097-69-1	Aroclor-1254	0.0035	U	0.0035	0.022	mg/Kg
37324-23-5	Aroclor-1262	0.0059	U	0.0059	0.022	mg/Kg
11100-14-4	Aroclor-1268	0.0044	U	0.0044	0.022	mg/Kg
11096-82-5	Aroclor-1260	0.0037	U	0.0037	0.022	mg/Kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.6		32 - 144	103%	SPK: 20
2051-24-3	Decachlorobiphenyl	14.3		32 - 175	72%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
 Data File : PO108285.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2024 13:43
 Operator : YP/AJ
 Sample : P5026-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SOIL-1-HAM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 00:34:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.371	3.636	151.5E6	69802908	17.401	20.588
2) SA Decachlor...	10.094	8.631	43694244	40775461	14.306	11.987

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
Data File : PO108285.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2024 13:43
Operator : YP/AJ
Sample : P5026-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SOIL-1-HAM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 00:34:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

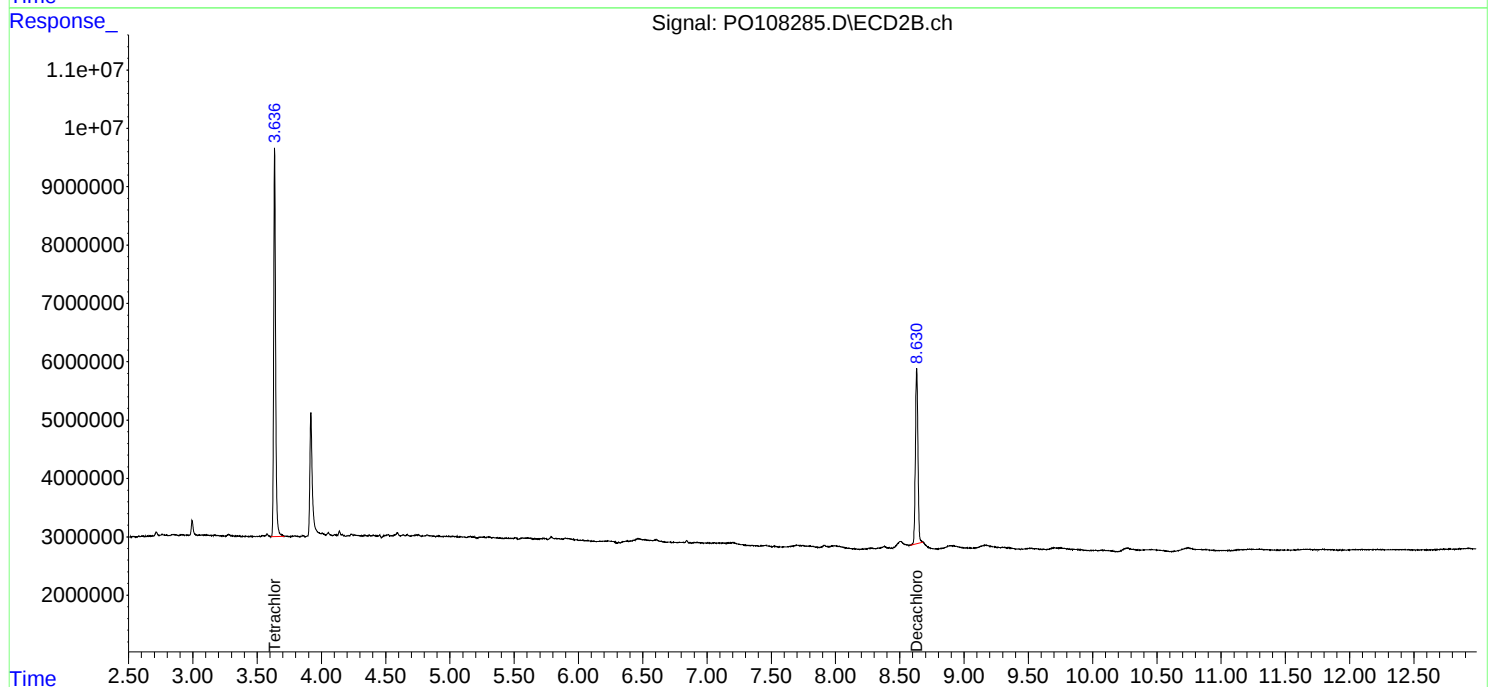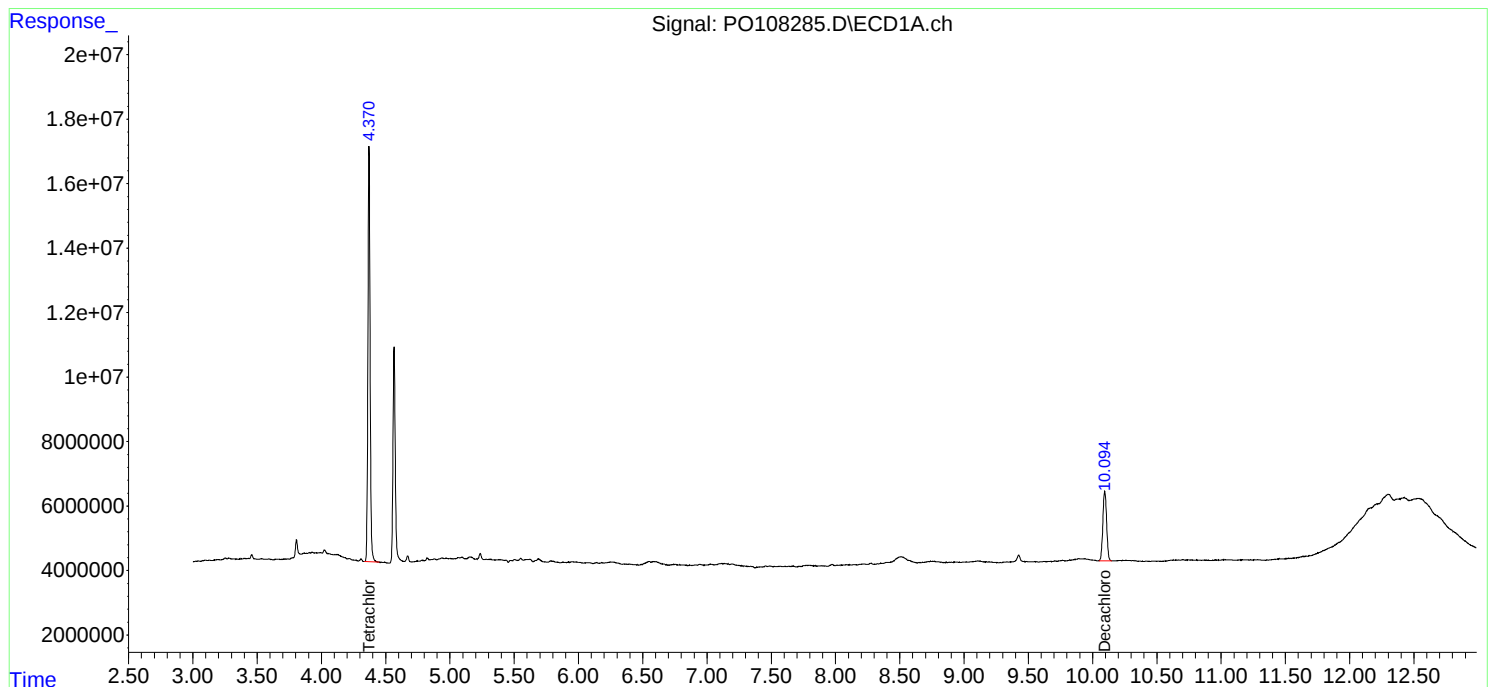


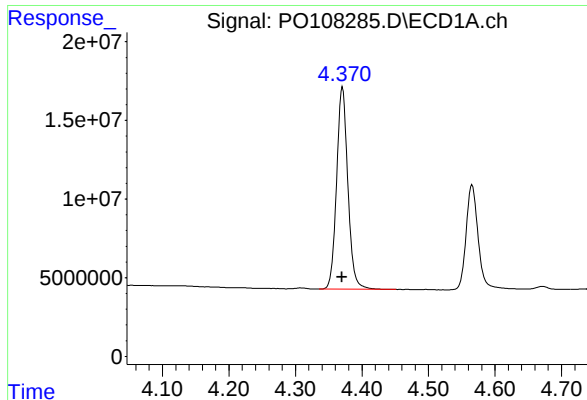

#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 151493794
Conc: 17.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
SOIL-1-HAM

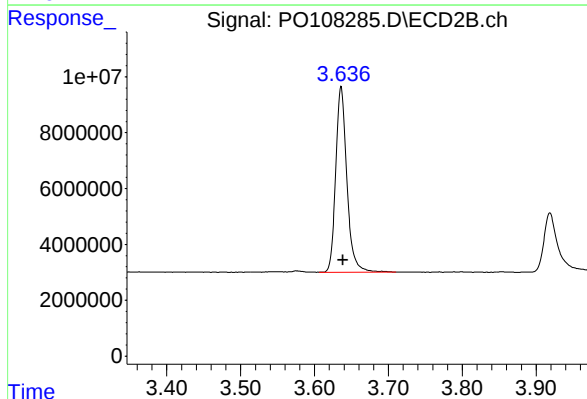


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.003 min
Response: 69802908
Conc: 20.59 ng/ml

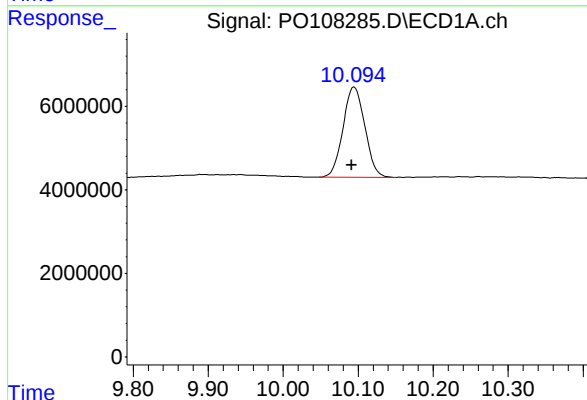

#2 Decachlorobiphenyl

R.T.: 10.094 min
Delta R.T.: 0.003 min
Response: 43694244
Conc: 14.31 ng/ml

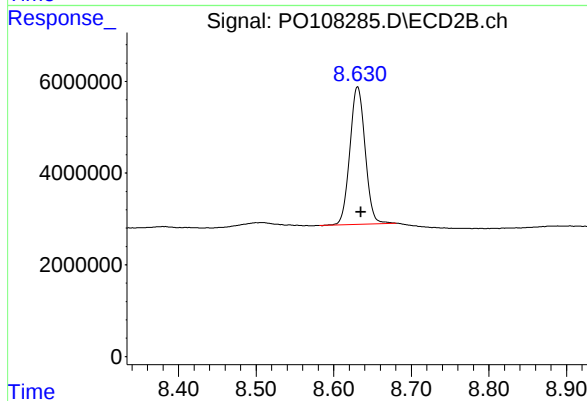

#2 Decachlorobiphenyl

R.T.: 8.631 min
Delta R.T.: -0.005 min
Response: 40775461
Conc: 11.99 ng/ml



CALIBRATION SUMMARY

RETENTION TIMES OF INITIAL CALIBRATION

Contract: TULL02
Lab Code: CHEM **Case No.:** P5026 **SAS No.:** P5026 **SDG NO.:** P5026
Instrument ID: ECD_O **Calibration Date(s):** 11/18/2024 11/18/2024
Calibration Times: 15:32 22:51

GC Column: ZB-MR1 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 = <u>PO108038.D</u>	RT 750 = <u>PO108039.D</u>
RT 500 = <u>PO108040.D</u>	RT 250 = <u>PO108041.D</u>	RT 050 = <u>PO108042.D</u>

COMPOUND		RT 1000	RT 750	RT 500	RT 250	RT 050	MEAN RT	RT WINDOW	
								FROM	TO
Aroclor-1016-1	(1)	5.53	5.53	5.53	5.52	5.53	5.53	5.43	5.63
Aroclor-1016-2	(2)	5.55	5.55	5.55	5.55	5.55	5.55	5.45	5.65
Aroclor-1016-3	(3)	5.61	5.61	5.61	5.61	5.61	5.61	5.51	5.71
Aroclor-1016-4	(4)	5.71	5.71	5.71	5.71	5.71	5.71	5.61	5.81
Aroclor-1016-5	(5)	6.01	6.00	6.00	6.00	6.00	6.00	5.90	6.10
Aroclor-1260-1	(1)	7.14	7.14	7.14	7.14	7.14	7.14	7.04	7.24
Aroclor-1260-2	(2)	7.40	7.39	7.40	7.39	7.39	7.39	7.29	7.49
Aroclor-1260-3	(3)	7.76	7.76	7.76	7.76	7.76	7.76	7.66	7.86
Aroclor-1260-4	(4)	7.98	7.98	7.98	7.98	7.98	7.98	7.88	8.08
Aroclor-1260-5	(5)	8.30	8.30	8.30	8.30	8.30	8.30	8.20	8.40
Decachlorobiphenyl		10.09	10.09	10.09	10.09	10.09	10.09	9.99	10.19
Tetrachloro-m-xylene		4.37	4.37	4.37	4.37	4.37	4.37	4.27	4.47
Aroclor-1242-1	(1)	5.53	5.53	5.53	5.53	5.53	5.53	5.43	5.63
Aroclor-1242-2	(2)	5.55	5.55	5.55	5.55	5.55	5.55	5.45	5.65
Aroclor-1242-3	(3)	5.61	5.61	5.61	5.61	5.61	5.61	5.51	5.71
Aroclor-1242-4	(4)	5.71	5.71	5.71	5.71	5.71	5.71	5.61	5.81
Aroclor-1242-5	(5)	6.45	6.45	6.45	6.45	6.45	6.45	6.35	6.55
Decachlorobiphenyl		10.09	10.09	10.09	10.09	10.09	10.09	9.99	10.19
Tetrachloro-m-xylene		4.37	4.37	4.37	4.37	4.37	4.37	4.27	4.47
Aroclor-1248-1	(1)	5.53	5.52	5.53	5.53	5.53	5.53	5.43	5.63
Aroclor-1248-2	(2)	5.80	5.80	5.80	5.80	5.80	5.80	5.70	5.90
Aroclor-1248-3	(3)	6.00	6.00	6.00	6.00	6.00	6.00	5.90	6.10
Aroclor-1248-4	(4)	6.41	6.41	6.41	6.41	6.41	6.41	6.31	6.51
Aroclor-1248-5	(5)	6.45	6.45	6.45	6.45	6.45	6.45	6.35	6.55
Decachlorobiphenyl		10.09	10.09	10.09	10.09	10.09	10.09	9.99	10.19
Tetrachloro-m-xylene		4.37	4.37	4.37	4.37	4.37	4.37	4.27	4.47
Aroclor-1254-1	(1)	6.38	6.38	6.38	6.38	6.38	6.38	6.28	6.48
Aroclor-1254-2	(2)	6.60	6.60	6.60	6.60	6.60	6.60	6.50	6.70
Aroclor-1254-3	(3)	6.97	6.97	6.97	6.97	6.97	6.97	6.87	7.07
Aroclor-1254-4	(4)	7.26	7.26	7.25	7.26	7.25	7.26	7.16	7.36
Aroclor-1254-5	(5)	7.68	7.68	7.68	7.68	7.68	7.68	7.58	7.78
Decachlorobiphenyl		10.09	10.09	10.09	10.09	10.09	10.09	9.99	10.19
Tetrachloro-m-xylene		4.37	4.37	4.37	4.37	4.37	4.37	4.27	4.47
Aroclor-1268-1	(1)	8.61	8.61	8.61	8.61	8.61	8.61	8.51	8.71
Aroclor-1268-2	(2)	8.70	8.70	8.70	8.70	8.70	8.70	8.60	8.80
Aroclor-1268-3	(3)	8.93	8.93	8.93	8.93	8.93	8.93	8.83	9.03
Aroclor-1268-4	(4)	9.34	9.34	9.34	9.34	9.34	9.34	9.24	9.44
Aroclor-1268-5	(5)	9.76	9.76	9.75	9.75	9.75	9.75	9.65	9.85

[illegible]

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:	RT 1000 =	<u>PO108038.D</u>	RT 750 =	<u>PO108039.D</u>
RT 500 = PO108040.D	RT 250 =	PO108041.D	RT 050 =	PO108042.D

[illegible]

[illegible]

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: TULL02
Lab Code: CHEM **Case No.:** P5026 **SAS No.:** P5026 **SDG NO.:** P5026
Instrument ID: ECD_O **Calibration Date(s):** 11/18/2024 11/18/2024
Calibration Times: 15:32 22:51

GC Column: ZB-MR1 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO108038.D</u>		CF 750 = <u>PO108039.D</u>			
CF 500 = <u>PO108040.D</u>		CF 250 = <u>PO108041.D</u>		CF 050 = <u>PO108042.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	246762638	255183097	267973476	283317680	291399940	7
Aroclor-1016-2	(2)	361906701	371340893	387074982	408562964	409480900	6
Aroclor-1016-3	(3)	222622001	230895227	242997188	262828576	290224400	11
Aroclor-1016-4	(4)	180908655	187263399	196564780	208828236	202781360	6
Aroclor-1016-5	(5)	172054377	178657919	188464708	198508344	189466020	6
Aroclor-1260-1	(1)	247038034	257258523	276155998	300356752	291432540	8
Aroclor-1260-2	(2)	272689813	275156095	291862946	311284092	264022160	7
Aroclor-1260-3	(3)	196571881	200863216	216965512	232635324	227109120	7
Aroclor-1260-4	(4)	206067217	211502581	224665900	236880824	230926000	6
Aroclor-1260-5	(5)	361568828	367344987	386082756	401302256	391367100	4
Decachlorobiphenyl		2788452830	2899237187	3078698780	3257210480	3247383800	7
Tetrachloro-m-xylene		8465605050	8620290680	8898313680	9030365440	8515879800	3
Aroclor-1242-1	(1)	202566328	209266423	216968960	226834060	251201700	9
Aroclor-1242-2	(2)	292414213	300976153	306906846	326944128	345266040	7
Aroclor-1242-3	(3)	180504553	188122379	204296224	206704844	232713180	10
Aroclor-1242-4	(4)	145573082	151871127	147856924	161129744	174130240	7
Aroclor-1242-5	(5)	141458429	150487075	174887798	165575256	171811960	9
Decachlorobiphenyl		2883024050	2993599120	3112238920	3347716960	3290585400	6
Tetrachloro-m-xylene		8474998350	8554163053	8448632340	8865007800	8445940200	2
Aroclor-1248-1	(1)	159118922	161357184	172663464	181852748	193964860	8
Aroclor-1248-2	(2)	223667475	232366575	244148502	257041984	245312320	5
Aroclor-1248-3	(3)	235052357	249913948	255721754	270339584	271390180	6
Aroclor-1248-4	(4)	254865791	270625609	276970026	290980956	271389120	5
Aroclor-1248-5	(5)	250852362	264749787	277140996	291546208	270671600	6
Decachlorobiphenyl		3055844430	3212426880	3323854080	3502784880	3470872200	6
Tetrachloro-m-xylene		8617109190	8960264667	8973068820	9149151720	8598975400	3
Aroclor-1254-1	(1)	252273984	264379132	273757404	293053280	301432280	7
Aroclor-1254-2	(2)	370718764	381771509	401517756	431022924	452397520	8
Aroclor-1254-3	(3)	371029833	378293709	395728354	413498008	404266220	5
Aroclor-1254-4	(4)	258988770	265852057	279911766	295707108	295222320	6
Aroclor-1254-5	(5)	253254357	260982649	273964622	289085188	263893220	5
Decachlorobiphenyl		3053184730	3175475907	3371258020	3559677880	3473166600	6
Tetrachloro-m-xylene		8676286000	8781692213	9032518320	9252845040	8520211800	3
Aroclor-1268-1	(1)	470799605	475917148	498858234	526027740	502833980	5



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	426122965	429724292	449577094	474735796	444314960	444895021	4
Aroclor-1268-3	(3)	347803598	350738465	369541246	388683644	373678420	366089075	5
Aroclor-1268-4	(4)	159396827	162304215	169881814	178873580	168510400	167793367	5
Aroclor-1268-5	(5)	1064152927	1072377252	1107204992	1148173928	1104978940	1099377608	3
Decachlorobiphenyl		5130801040	5235509600	5479770240	5801588440	5574999800	5444533824	5
Tetrachloro-m-xylene		8604281960	8613628107	8840909600	9045256040	8253129800	8671441101	3

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: TULL02
Lab Code: CHEM **Case No.:** P5026 **SAS No.:** P5026 **SDG NO.:** P5026
Instrument ID: ECD_O **Calibration Date(s):** 11/18/2024 11/18/2024
Calibration Times: 15:32 22:51

GC Column: ZB-MR2 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 = <u>PO108038.D</u>		CF 750 = <u>PO108039.D</u>			
CF 500 = <u>PO108040.D</u>		CF 250 = <u>PO108041.D</u>		CF 050 = <u>PO108042.D</u>			
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	% RSD
Aroclor-1016-1	(1)	106788150	108798153	111718164	113509520	105554920	109273781 3
Aroclor-1016-2	(2)	152123024	154097571	158326228	159327316	140638080	152902444 5
Aroclor-1016-3	(3)	80988346	82315700	85055114	86482700	75979360	82164244 5
Aroclor-1016-4	(4)	61290280	63322112	65890902	67513476	60347000	63672754 5
Aroclor-1016-5	(5)	83859555	84976180	88574978	90258120	85814880	86696743 3
Aroclor-1260-1	(1)	157781272	160281296	165675998	168803692	157161680	161940788 3
Aroclor-1260-2	(2)	193178496	195374557	201955632	205123576	188687800	196864012 3
Aroclor-1260-3	(3)	183308515	185530125	190617304	192222592	178946180	186124943 3
Aroclor-1260-4	(4)	158006285	159976592	164422288	165515456	152052260	159994576 3
Aroclor-1260-5	(5)	397600161	398299031	405738120	401770156	360054820	392692458 5
Decachlorobiphenyl		3329333650	3376455133	3495318160	3542281840	3265178400	3401713437 3
Tetrachloro-m-xylene		3460288000	3499045520	3533194380	3490778200	2968782600	3390417740 7
Aroclor-1242-1	(1)	87969741	88248992	87758754	93432100	85060960	88494109 3
Aroclor-1242-2	(2)	124351775	125884719	122342024	129672256	115828860	123615927 4
Aroclor-1242-3	(3)	66089426	66658731	64420492	69305104	64944480	66283647 3
Aroclor-1242-4	(4)	61409091	62399051	61772248	66049176	61264060	62578725 3
Aroclor-1242-5	(5)	80580818	81655216	82065824	87619560	85982300	83580744 4
Decachlorobiphenyl		3376553600	3460953067	3489794800	3599195960	3335440400	3452387565 3
Tetrachloro-m-xylene		3506478780	3524758680	3390143240	3493295680	3130140400	3408963356 5
Aroclor-1248-1	(1)	67026994	69560969	69998122	71628912	68826780	69408355 2
Aroclor-1248-2	(2)	89376189	93801245	94712640	97706412	91207920	93360881 3
Aroclor-1248-3	(3)	94788893	98911040	100115740	103278720	96514280	98721735 3
Aroclor-1248-4	(4)	115527324	120128197	120921898	125233548	119364180	120235029 3
Aroclor-1248-5	(5)	119804627	123323009	123889724	128054636	128073460	124629091 3
Decachlorobiphenyl		3528559440	3596963560	3616896320	3663454400	3377244800	3556623704 3
Tetrachloro-m-xylene		3528541860	3631159893	3583888800	3559804240	3171920200	3495062999 5
Aroclor-1254-1	(1)	174289834	176158589	180893068	186013588	167948420	177060700 4
Aroclor-1254-2	(2)	150108724	152943737	157672006	163048368	154480520	155650671 3
Aroclor-1254-3	(3)	256239069	259520284	265457534	269328112	244789800	259066960 4
Aroclor-1254-4	(4)	157049736	150166115	151648294	150255064	114987000	144821242 12
Aroclor-1254-5	(5)	226514935	228906973	235035164	238147696	216555420	229032038 4
Decachlorobiphenyl		3488739090	3567821253	3665438080	3726867560	3437434800	3577260157 3
Tetrachloro-m-xylene		3561296690	3571149600	3637431600	3609953440	3188991400	3513764546 5
Aroclor-1268-1	(1)	503786717	502542995	506955678	510483304	449116600	494577059 5



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Aroclor-1268-2	(2)	474790608	472331845	474584838	476025240	407711300	461088766	6
Aroclor-1268-3	(3)	398042300	395049041	397077938	397623440	338330320	385224608	7
Aroclor-1268-4	(4)	165026234	165243123	167676480	171057252	157015720	165203762	3
Aroclor-1268-5	(5)	1353304001	1345522504	1338264668	1326360488	1125948300	1297879992	7
Decachlorobiphenyl		6035126950	6057706560	6116207360	6217717120	5517400400	5988831678	5
Tetrachloro-m-xylene		3503890680	3480404160	3510527020	3509133960	2981330200	3397057204	7



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

Instrument ID: ECD_O Date(s) Analyzed: 11/18/2024 11/18/2024

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	4.57	4.47	4.67	108422000
		2	4.66	4.56	4.76	80468200
		3	4.73	4.63	4.83	233076000
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.73	4.63	4.83	171958000
		2	5.26	5.16	5.36	94164000
		3	5.55	5.45	5.65	161766000
		4	5.71	5.61	5.81	76393000
		5	5.80	5.70	5.90	52874400
Aroclor-1262	500	1	7.76	7.66	7.86	323292000
		2	8.30	8.20	8.40	449988000
		3	8.61	8.51	8.71	288986000
		4	8.70	8.60	8.80	223132000
		5	9.34	9.24	9.44	152022000



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

Instrument ID: ECD_O Date(s) Analyzed: 11/18/2024 11/18/2024

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
Aroclor-1221	500	1	3.85	3.75	3.95	35476800
		2	3.94	3.84	4.04	29137000
		3	4.01	3.91	4.11	89032800
		4	0.00			0
		5	0.00			0
Aroclor-1232	500	1	4.01	3.91	4.11	63710600
		2	4.74	4.64	4.84	64827200
		3	4.91	4.81	5.01	33220400
		4	5.00	4.90	5.10	30291200
		5	5.17	5.07	5.27	31376600
Aroclor-1262	500	1	6.75	6.65	6.85	227544000
		2	7.25	7.15	7.35	426902000
		3	7.54	7.44	7.64	165111000
		4	7.60	7.50	7.70	317924000
		5	8.09	7.99	8.19	148021000

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108038.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 15:32
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 16:36:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 18 16:32:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.638	846.6E6	346.0E6	97.508	98.958
2) SA Decachlor...	10.093	8.635	278.8E6	332.9E6	95.053	97.568
Target Compounds						
3) L1 AR-1016-1	5.525	4.719	246.8E6	106.8E6	958.793	977.438
4) L1 AR-1016-2	5.548	4.738	361.9E6	152.1E6	966.397	980.019
5) L1 AR-1016-3	5.611	4.914	222.6E6	80988346	956.241	975.508
6) L1 AR-1016-4	5.708	4.956	180.9E6	61290280	958.524	963.826
7) L1 AR-1016-5	6.005	5.170	172.1E6	83859555	954.481	972.654
31) L7 AR-1260-1	7.138	6.201	247.0E6	157.8E6	944.346	975.593
32) L7 AR-1260-2	7.395	6.389	272.7E6	193.2E6	966.038	977.787
33) L7 AR-1260-3	7.758	6.542	196.6E6	183.3E6	950.685	980.454
34) L7 AR-1260-4	7.983	7.013	206.1E6	158.0E6	956.821	980.101
35) L7 AR-1260-5	8.299	7.253	361.6E6	397.6E6	967.212	989.870



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108038.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 15:32
Operator : YP/AJ
Sample : AR1660ICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 16:36:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 18 16:32:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

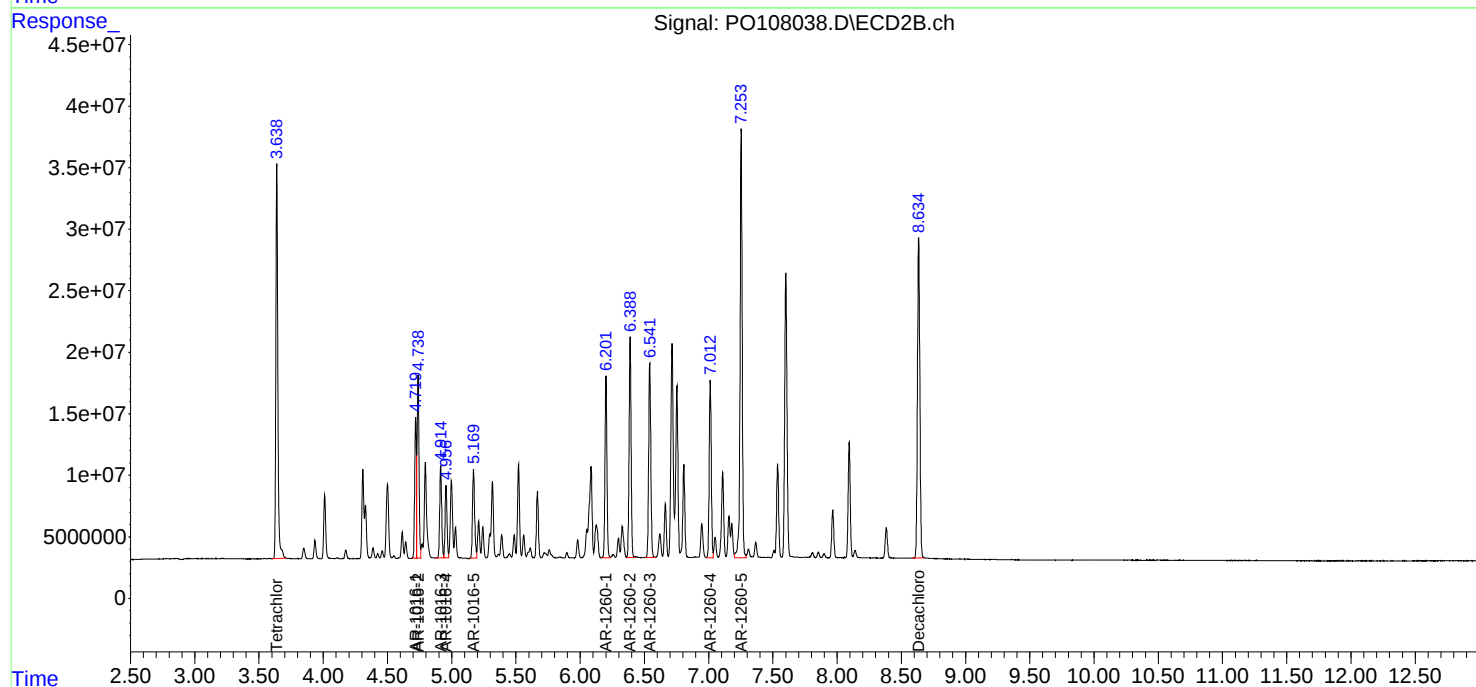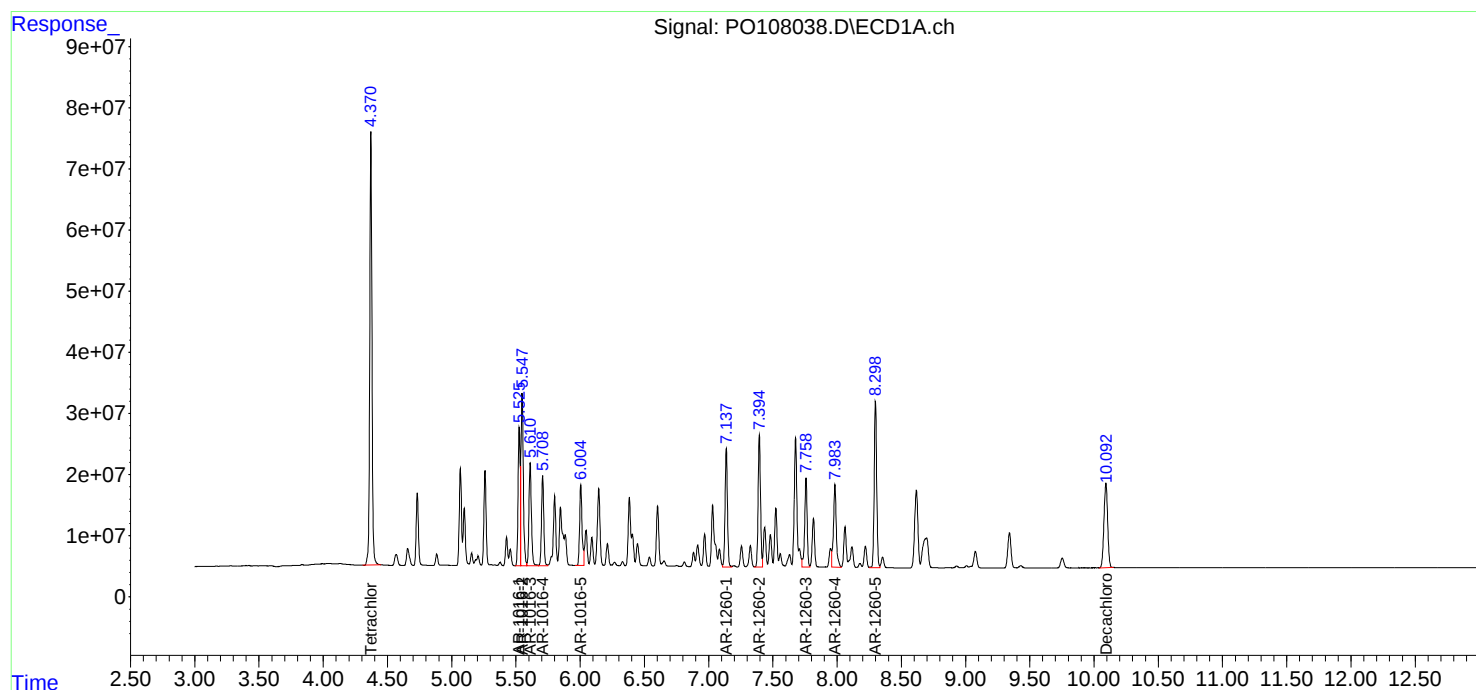

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 15:48
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 16:40:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 18 16:32:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.639	646.5E6	262.4E6	74.644	75.033
2) SA Decachlor...	10.091	8.634	217.4E6	253.2E6	74.412	74.473
Target Compounds						
3) L1 AR-1016-1	5.525	4.720	191.4E6	81598615	745.743	747.915
4) L1 AR-1016-2	5.548	4.738	278.5E6	115.6E6	745.783	746.361
5) L1 AR-1016-3	5.610	4.915	173.2E6	61736775	745.877	745.736
6) L1 AR-1016-4	5.708	4.956	140.4E6	47491584	746.087	747.886
7) L1 AR-1016-5	6.004	5.169	134.0E6	63732135	745.544	742.768
31) L7 AR-1260-1	7.137	6.201	192.9E6	120.2E6	741.662	745.512
32) L7 AR-1260-2	7.394	6.388	206.4E6	146.5E6	737.281	744.431
33) L7 AR-1260-3	7.758	6.541	150.6E6	139.1E6	735.582	746.158
34) L7 AR-1260-4	7.983	7.012	158.6E6	120.0E6	740.975	746.151
35) L7 AR-1260-5	8.299	7.253	275.5E6	298.7E6	741.281	745.793



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 15:48
Operator : YP/AJ
Sample : AR1660ICC750
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 16:40:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 18 16:32:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

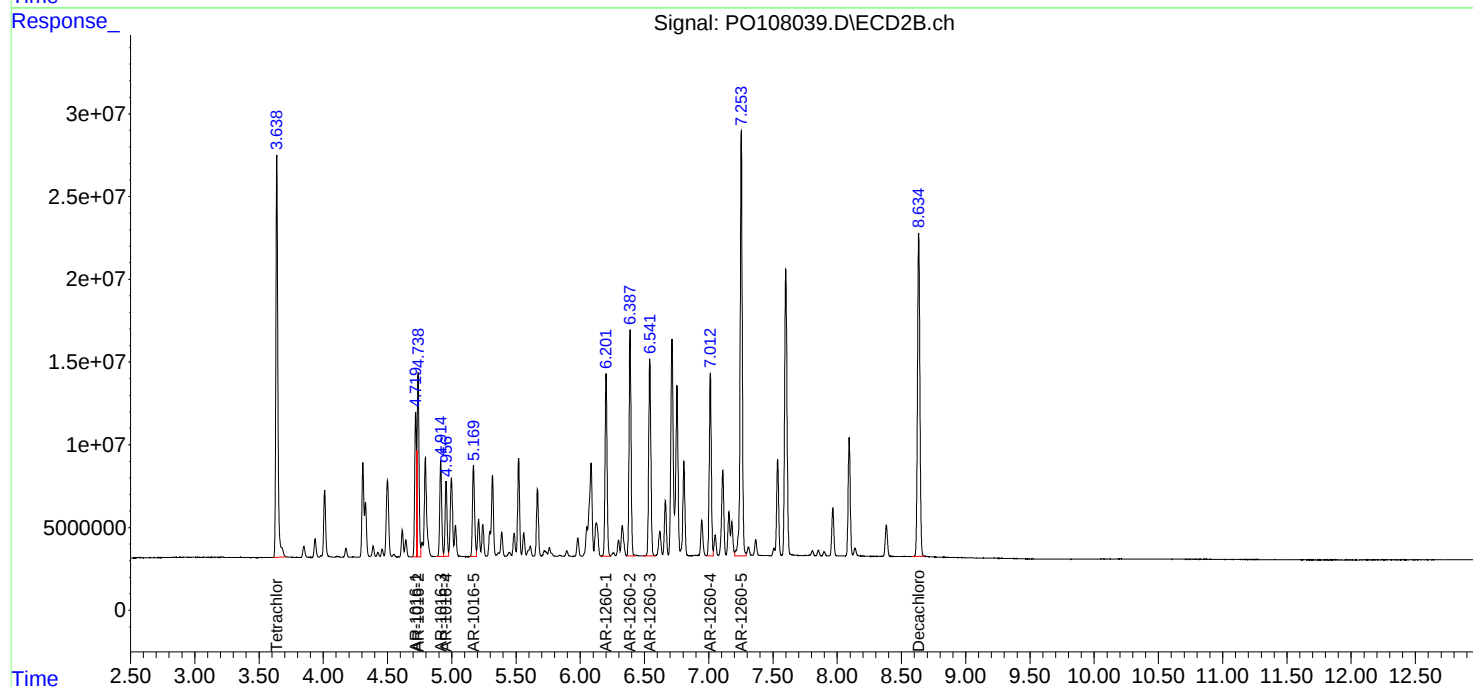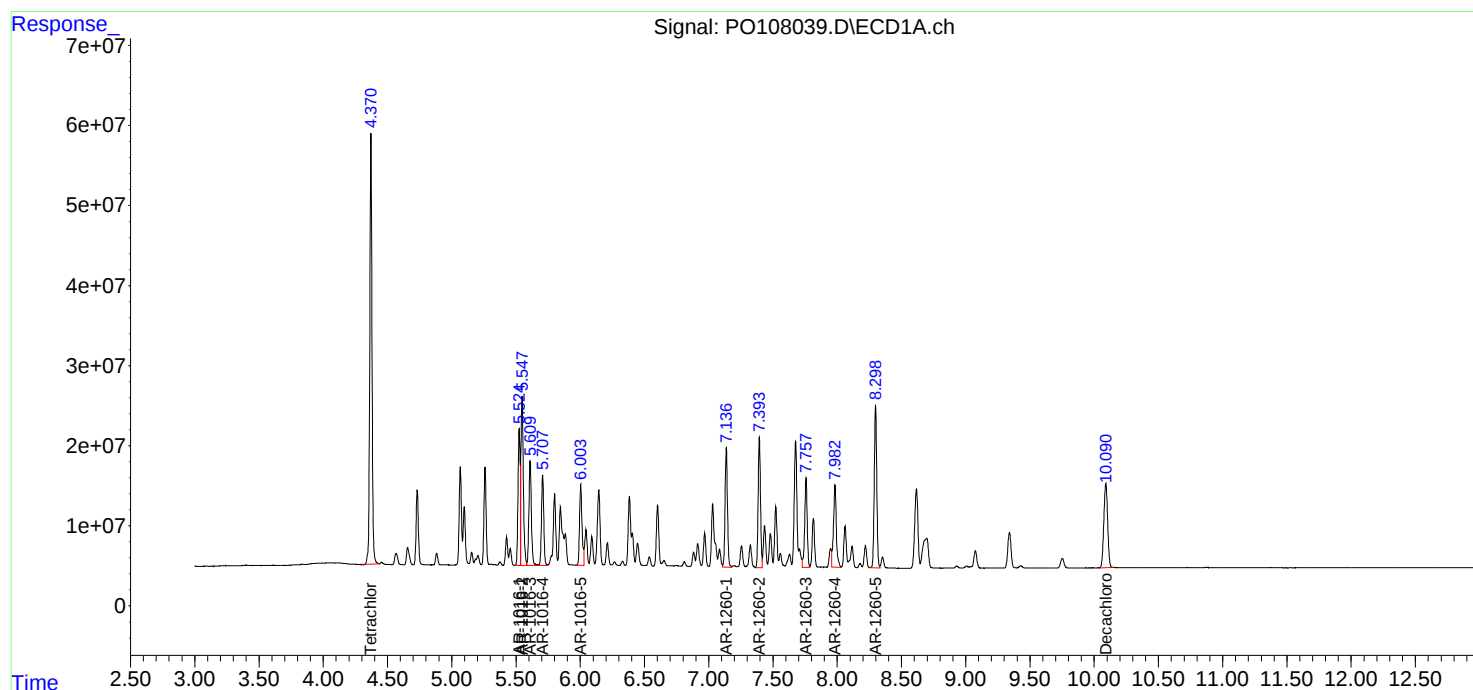

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 16:05
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 16:33:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 18 16:32:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.639	444.9E6	176.7E6	50.000	50.000
2) SA Decachlor...	10.091	8.635	153.9E6	174.8E6	50.000	50.000
Target Compounds						
3) L1 AR-1016-1	5.525	4.720	134.0E6	55859082	500.000	500.000
4) L1 AR-1016-2	5.547	4.739	193.5E6	79163114	500.000	500.000
5) L1 AR-1016-3	5.610	4.915	121.5E6	42527557	500.000	500.000
6) L1 AR-1016-4	5.707	4.956	98282390	32945451	500.000	500.000
7) L1 AR-1016-5	6.004	5.170	94232354	44287489	500.000	500.000
31) L7 AR-1260-1	7.137	6.200	138.1E6	82837999	500.000	500.000
32) L7 AR-1260-2	7.395	6.388	145.9E6	101.0E6	500.000	500.000
33) L7 AR-1260-3	7.758	6.541	108.5E6	95308652	500.000	500.000
34) L7 AR-1260-4	7.984	7.012	112.3E6	82211144	500.000	500.000
35) L7 AR-1260-5	8.298	7.254	193.0E6	202.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 16:05
Operator : YP/AJ
Sample : AR1660ICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 16:33:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 18 16:32:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

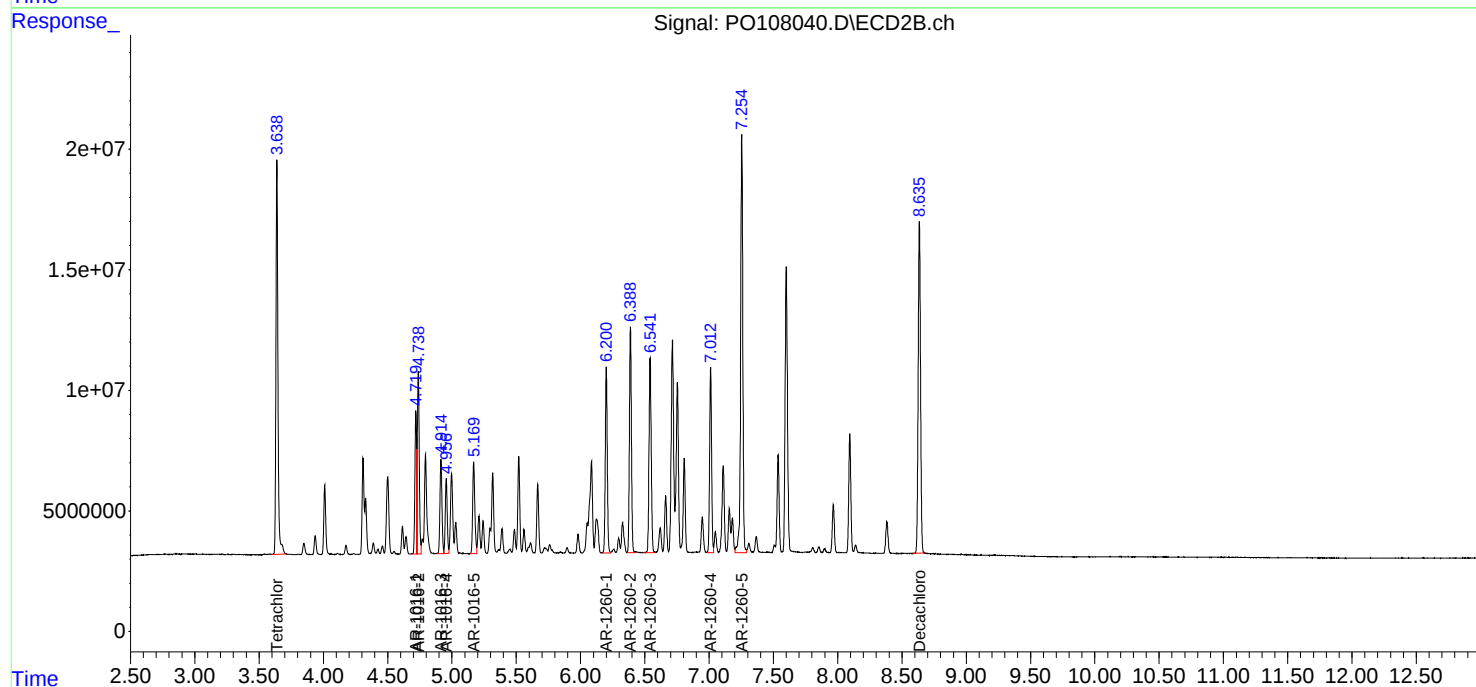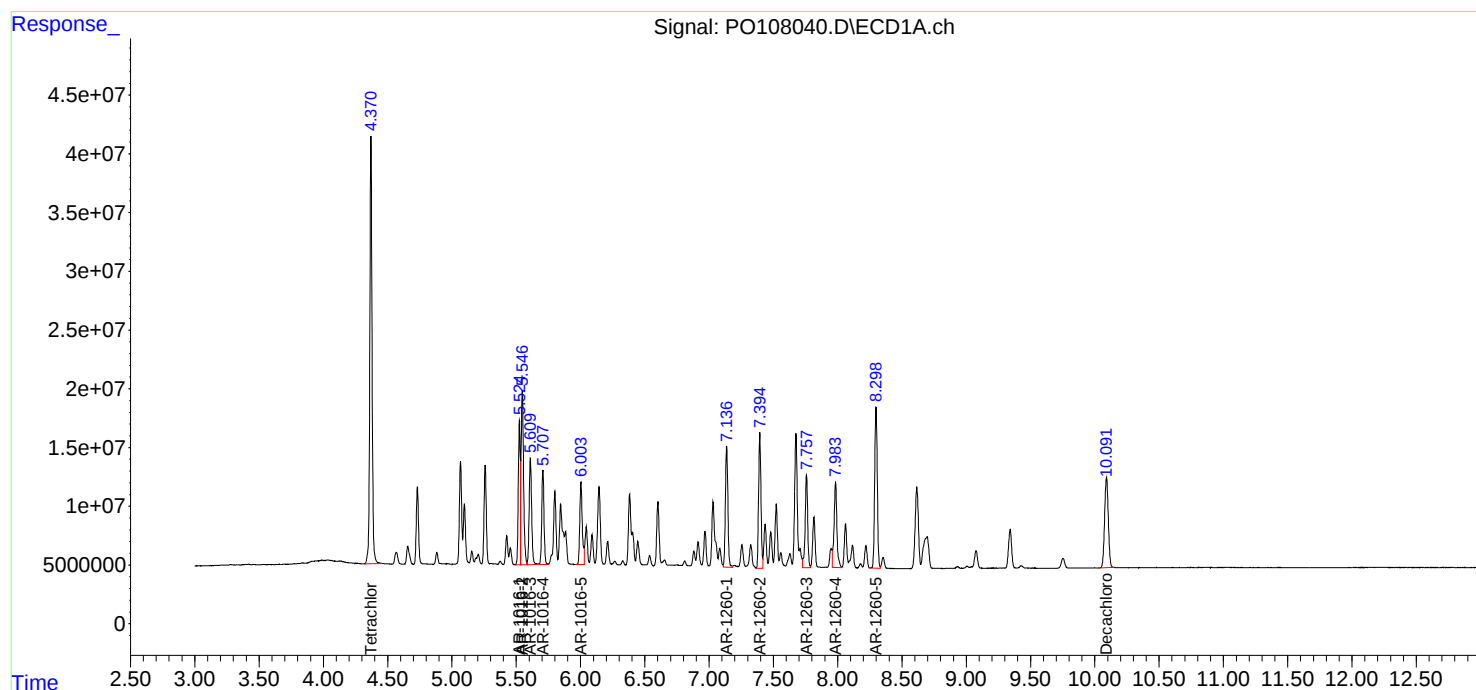

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108041.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 16:21
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 16:43:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 18 16:32:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.638	225.8E6	87269455	25.790	24.964
2) SA Decachlor...	10.089	8.634	81430262	88557046	27.090	25.774
Target Compounds						
3) L1 AR-1016-1	5.524	4.720	70829420	28377380	268.997	257.500
4) L1 AR-1016-2	5.546	4.738	102.1E6	39831829	267.229	255.384
5) L1 AR-1016-3	5.610	4.915	65707144	21620675	273.967	258.279
6) L1 AR-1016-4	5.707	4.956	52207059	16878369	269.956	261.663
7) L1 AR-1016-5	6.003	5.169	49627086	22564530	269.096	259.609
31) L7 AR-1260-1	7.136	6.200	75089188	42200923	277.900	258.686
32) L7 AR-1260-2	7.393	6.388	77821023	51280894	270.448	257.812
33) L7 AR-1260-3	7.756	6.541	58158831	48055648	274.646	255.724
34) L7 AR-1260-4	7.982	7.012	59220206	41378864	269.453	255.456
35) L7 AR-1260-5	8.297	7.254	100.3E6	100.4E6	264.659	250.573



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108041.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 16:21
Operator : YP/AJ
Sample : AR1660ICC250
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 16:43:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 18 16:32:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

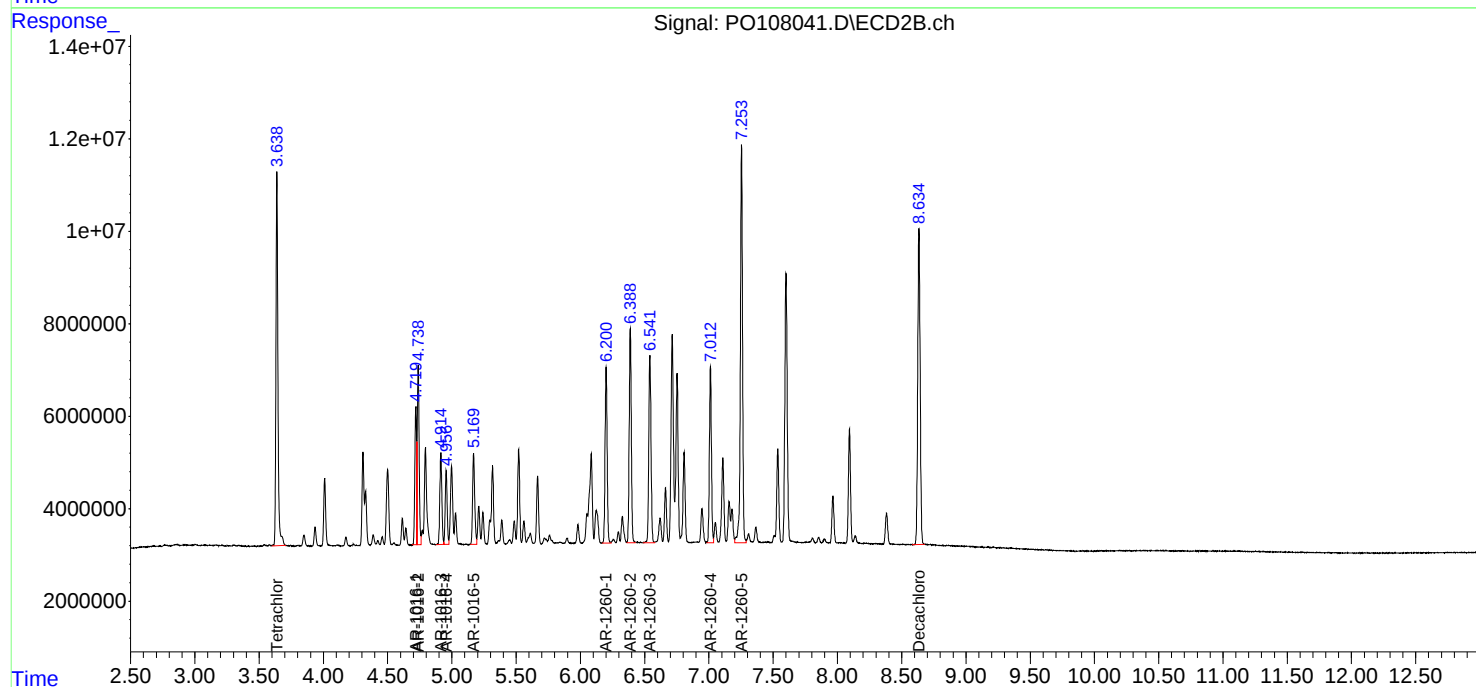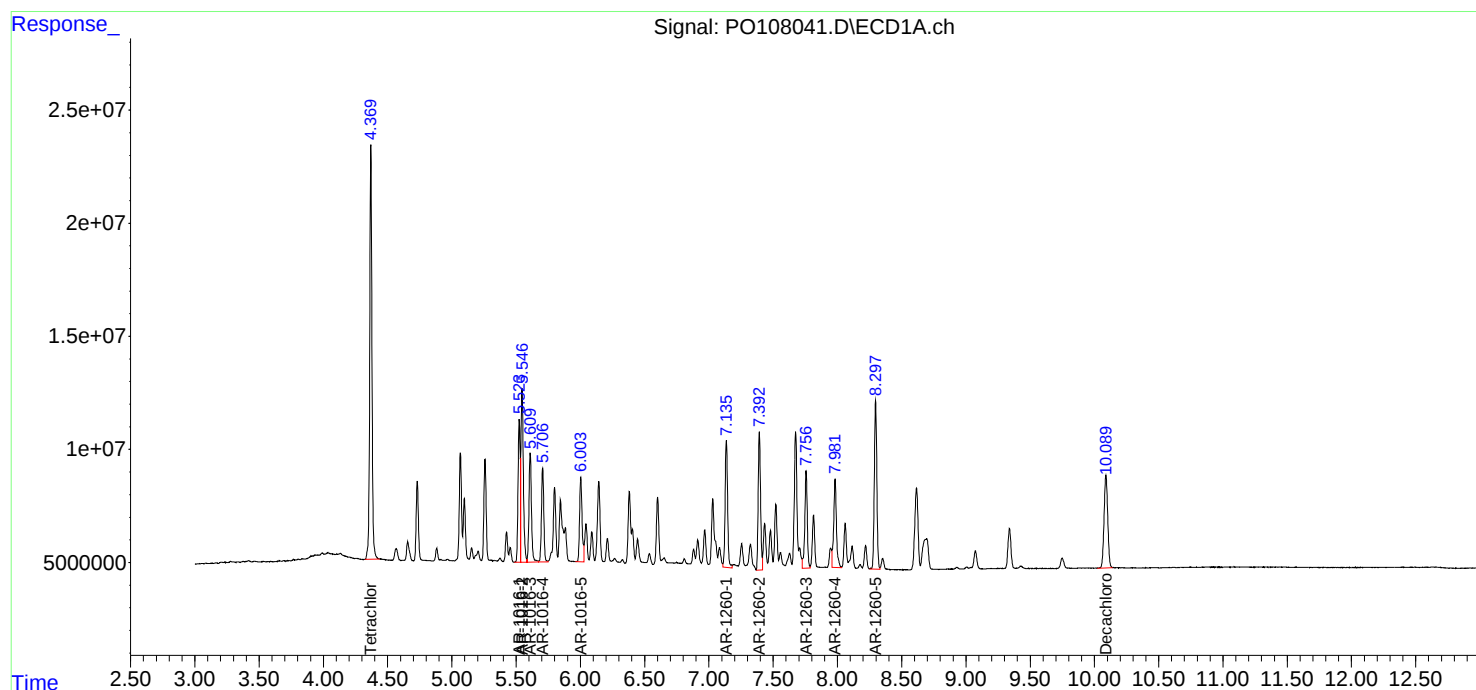

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108042.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 16:37
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 16:51:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 18 16:50:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.638	42579399	14843913	4.891	4.378
2) SA Decachlor...	10.090	8.635	16236919	16325892	5.316	4.799
Target Compounds						
3) L1 AR-1016-1	5.525	4.720	14569997	5277746	54.178	48.298
4) L1 AR-1016-2	5.548	4.739	20474045	7031904	52.813	45.989
5) L1 AR-1016-3	5.610	4.915	14511220	3798968	58.065	46.236
6) L1 AR-1016-4	5.707	4.956	10139068	3017350	51.924	47.388
7) L1 AR-1016-5	6.004	5.170	9473301	4290744	51.088	49.491
31) L7 AR-1260-1	7.135	6.200	14571627	7858084	53.156m	48.838m
32) L7 AR-1260-2	7.392	6.388	13201108	9434390	47.203m	47.725m
33) L7 AR-1260-3	7.756	6.542	11355456	8947309	52.868m	48.072
34) L7 AR-1260-4	7.983	7.012	11546300	7602613	52.008	47.518
35) L7 AR-1260-5	8.297	7.253	19568355	18002741	51.289	45.844

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108042.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 16:37
Operator : YP/AJ
Sample : AR1660ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 16:51:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 18 16:50:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

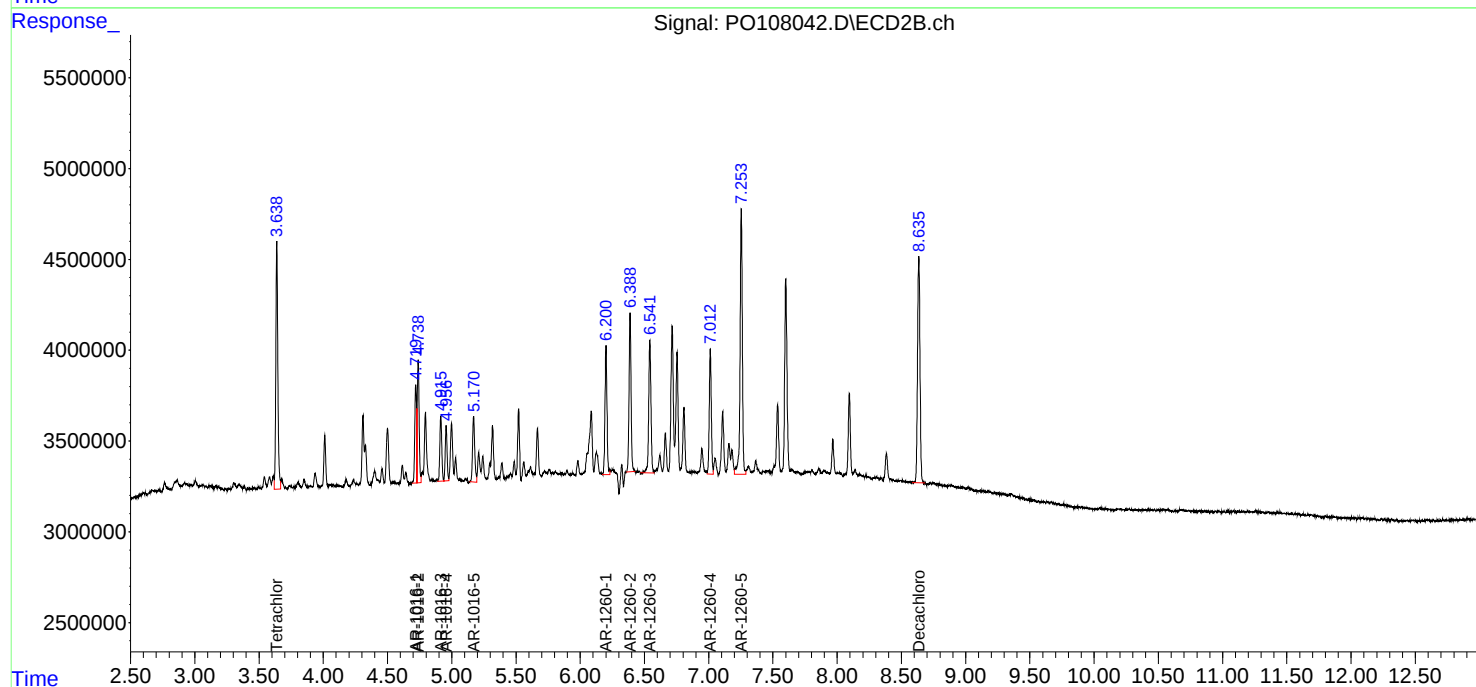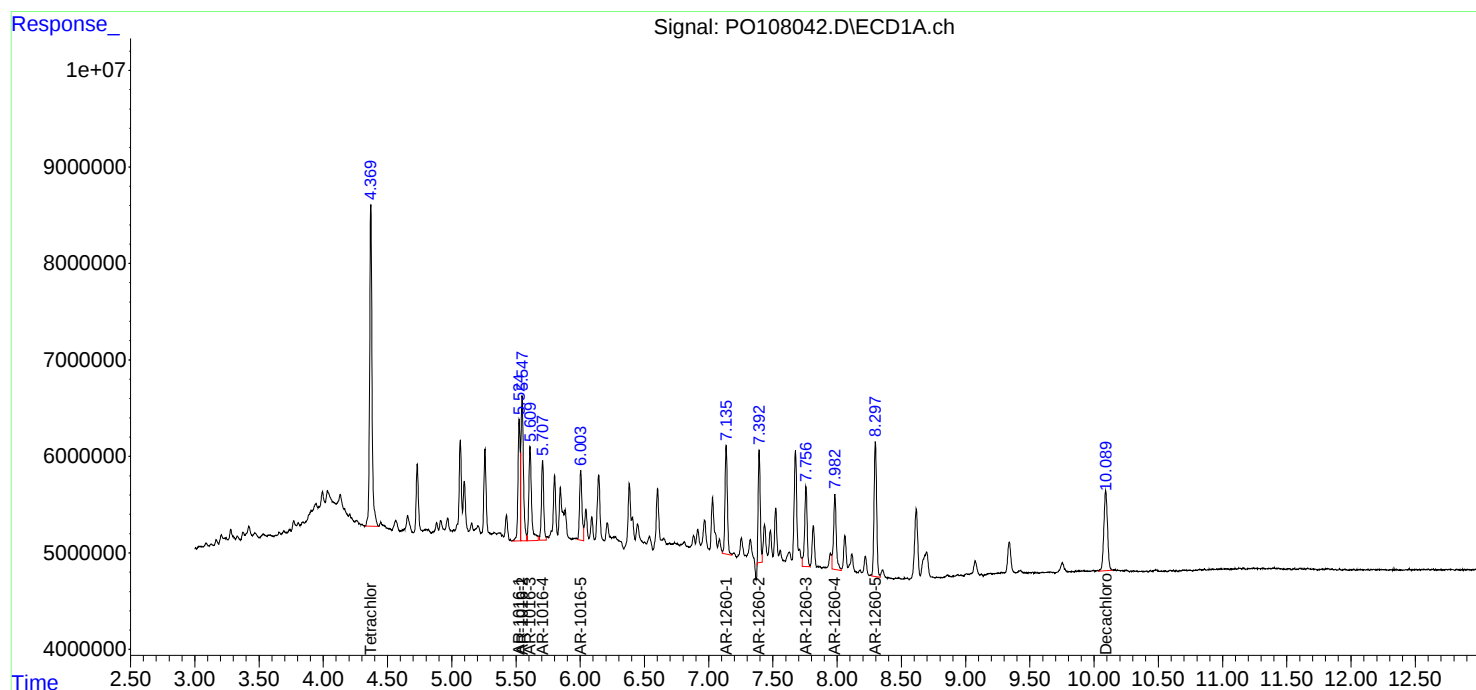

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 16:53
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:32:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 01:31:42 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.639	452.9E6	172.0E6	50.000	50.000
2) SA Decachlor...	10.089	8.634	158.0E6	178.1E6	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	4.571	3.850	54211145	17738379	500.000	500.000
9) L2 AR-1221-2	4.657	3.936	40234141	14568537	500.000	500.000
10) L2 AR-1221-3	4.732	4.011	116.5E6	44516402	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 16:53
Operator : YP/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:32:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 01:31:42 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

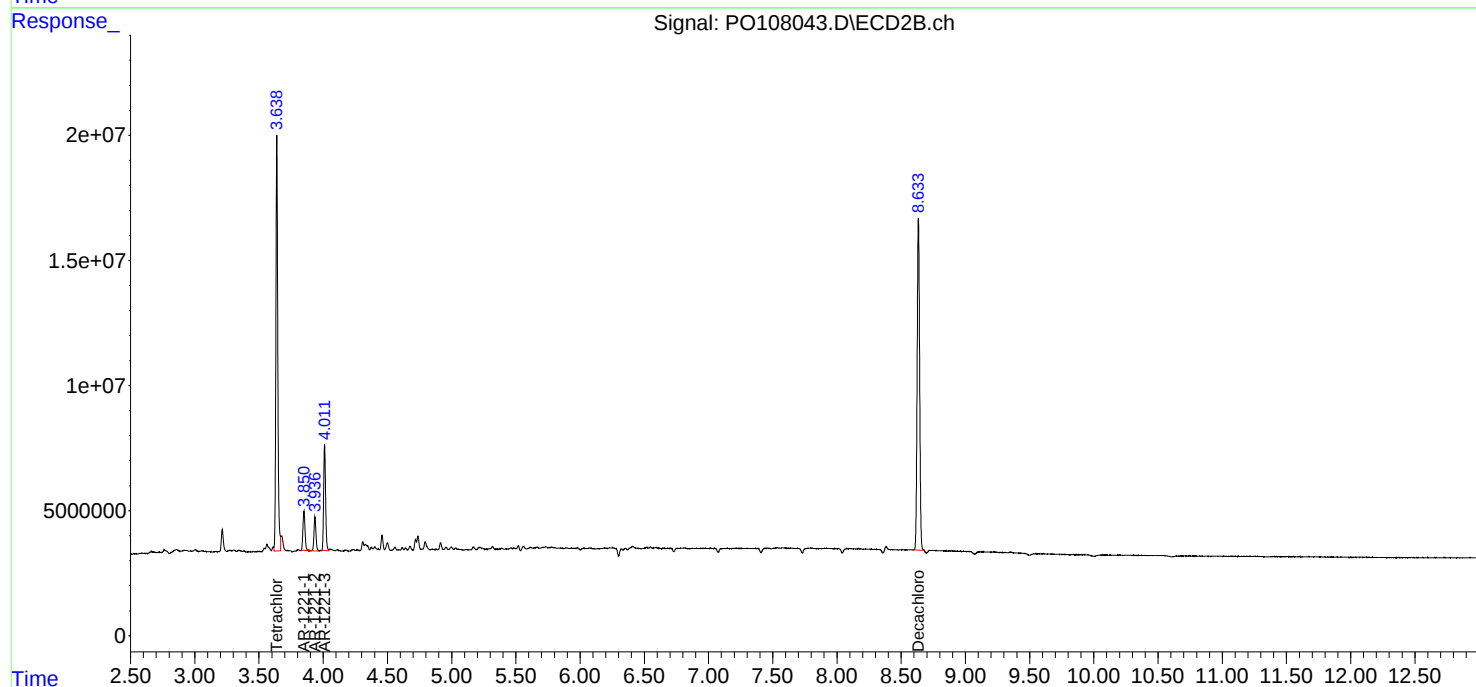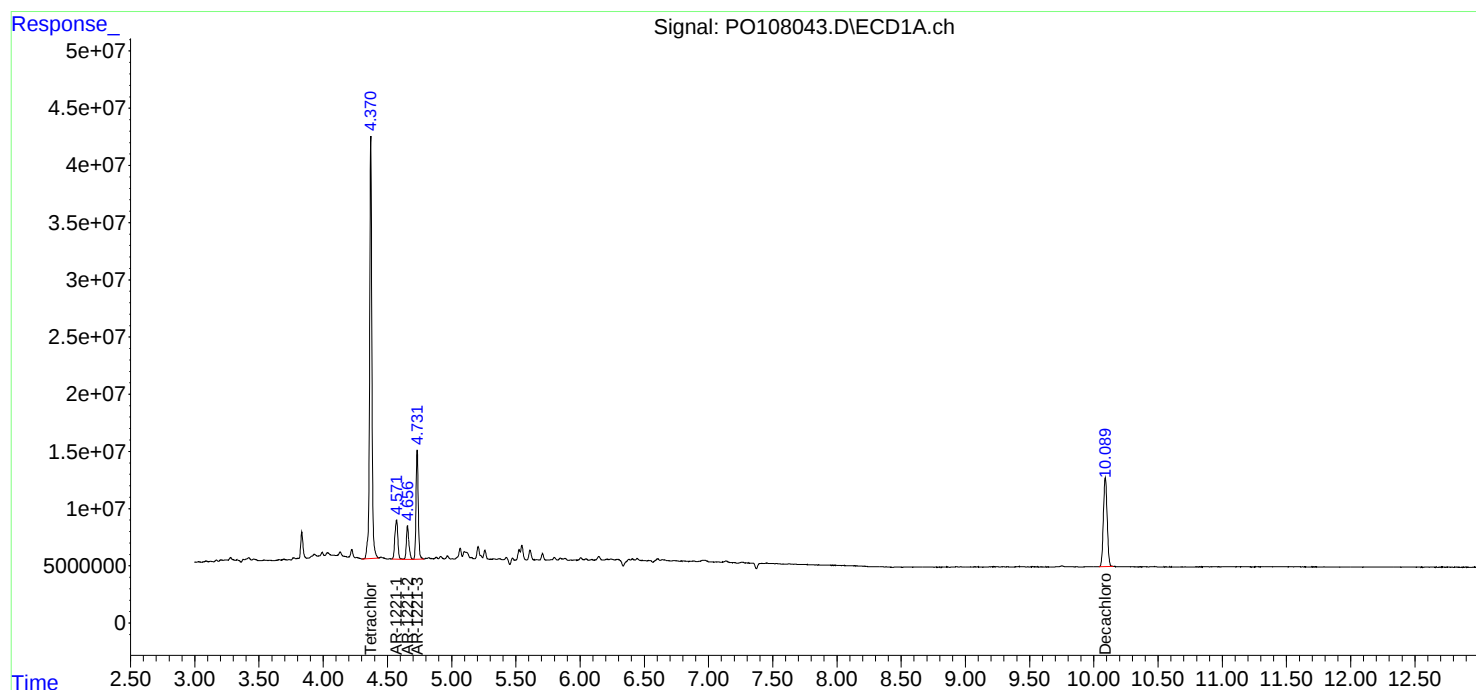

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108044.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 17:09
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:34:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 01:34:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.638	402.5E6	160.7E6	50.000	50.000
2) SA Decachlor...	10.089	8.634	146.9E6	165.2E6	50.000	50.000
Target Compounds						
11) L3 AR-1232-1	4.731	4.010	85979248	31855343	500.000	500.000
12) L3 AR-1232-2	5.258	4.738	47082015	32413612	500.000	500.000
13) L3 AR-1232-3	5.546	4.914	80882831	16610246	500.000	500.000
14) L3 AR-1232-4	5.706	4.997	38196478	15145642	500.000	500.000
15) L3 AR-1232-5	5.800	5.169	26437193	15688296	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108044.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 17:09
Operator : YP/AJ
Sample : AR1232ICC500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:34:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 01:34:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

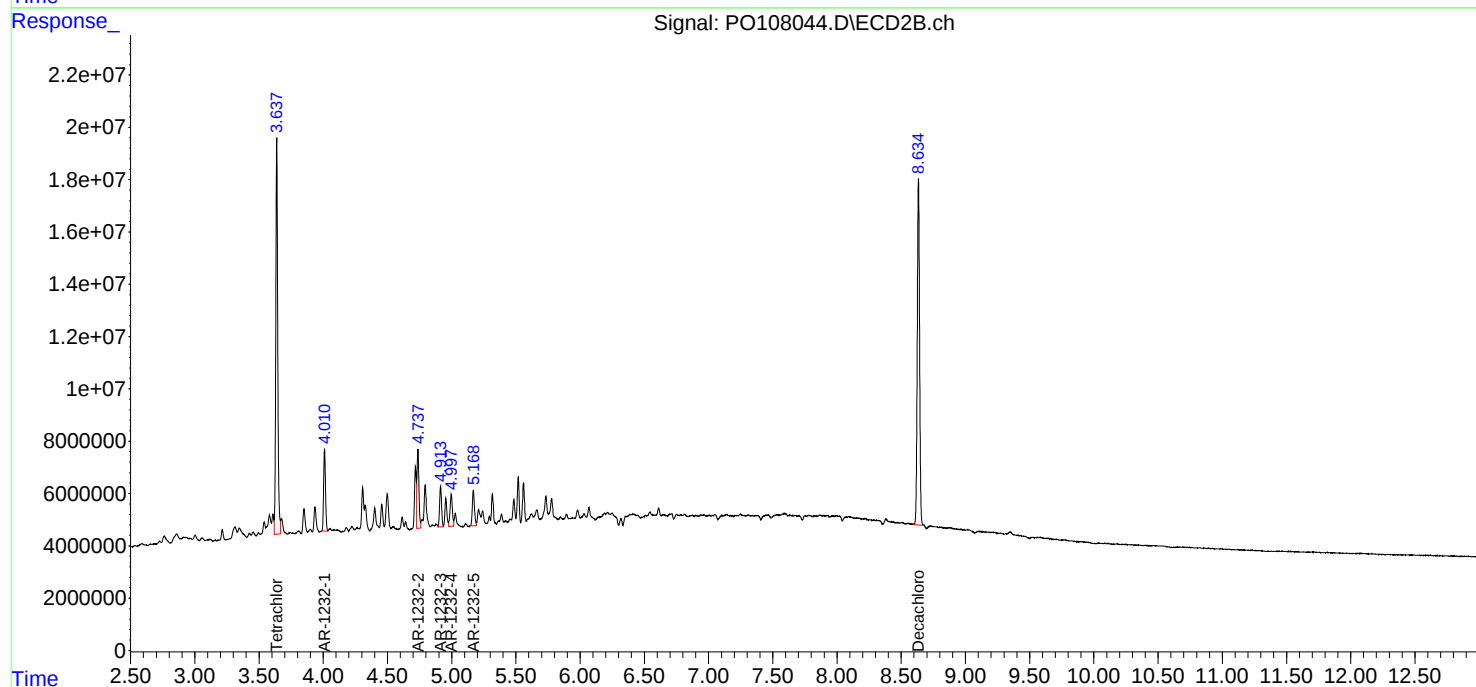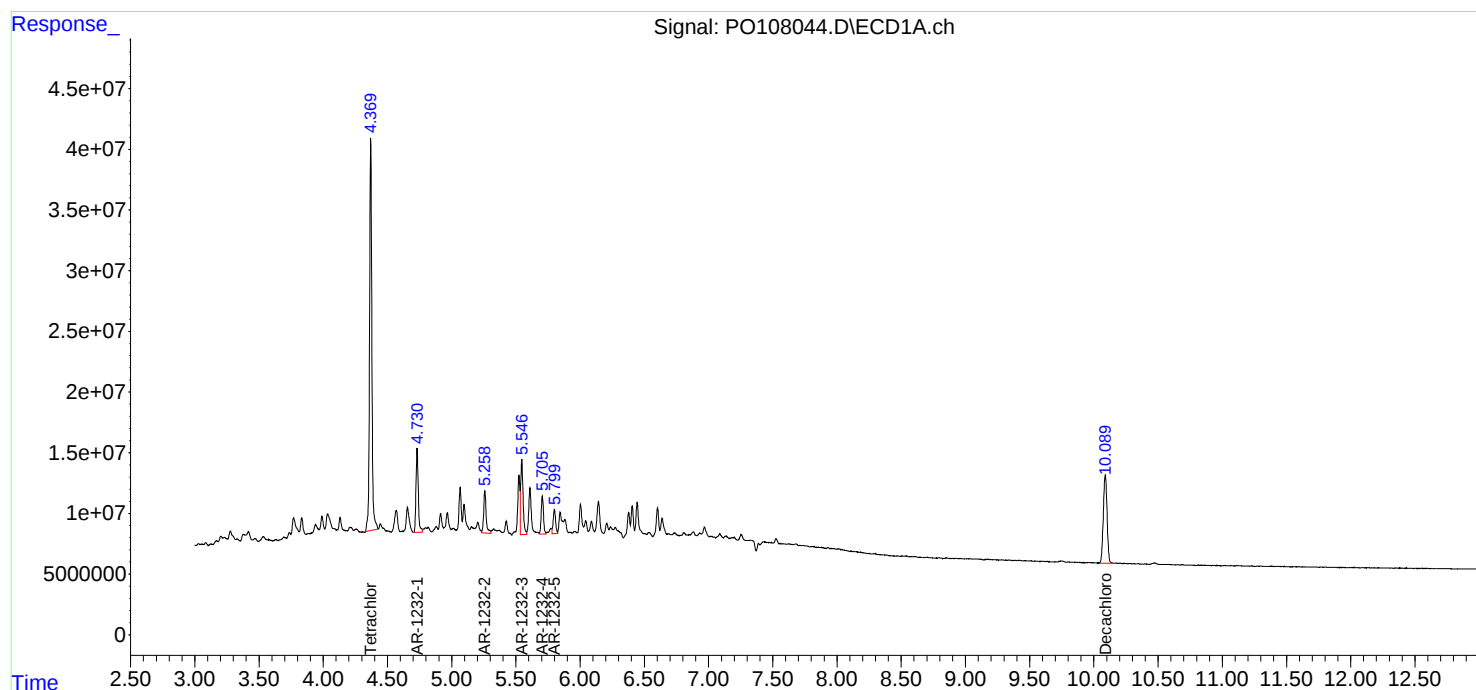

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 17:25
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:40:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 01:39:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.638	847.5E6	350.6E6	100.312	103.432
2) SA Decachlor...	10.092	8.634	288.3E6	337.7E6	92.635	96.755
Target Compounds						
16) L4 AR-1242-1	5.526	4.719	202.6E6	87969741	933.619	1002.404
17) L4 AR-1242-2	5.548	4.738	292.4E6	124.4E6	952.778	1016.427
18) L4 AR-1242-3	5.611	4.914	180.5E6	66089426	883.543	1025.907
19) L4 AR-1242-4	5.708	4.997	145.6E6	61409091	984.554	994.121
20) L4 AR-1242-5	6.446	5.520	141.5E6	80580818	808.852	981.905



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 17:25
Operator : YP/AJ
Sample : AR1242ICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:40:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 01:39:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

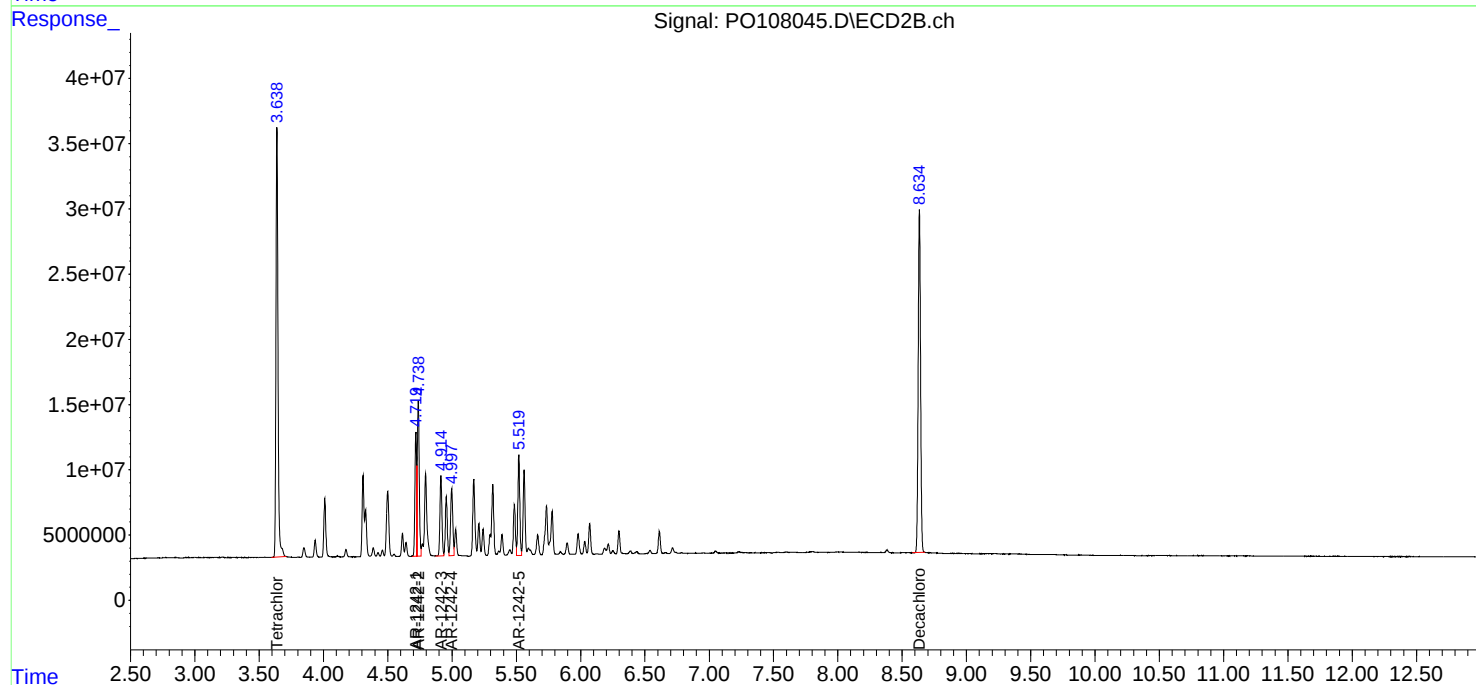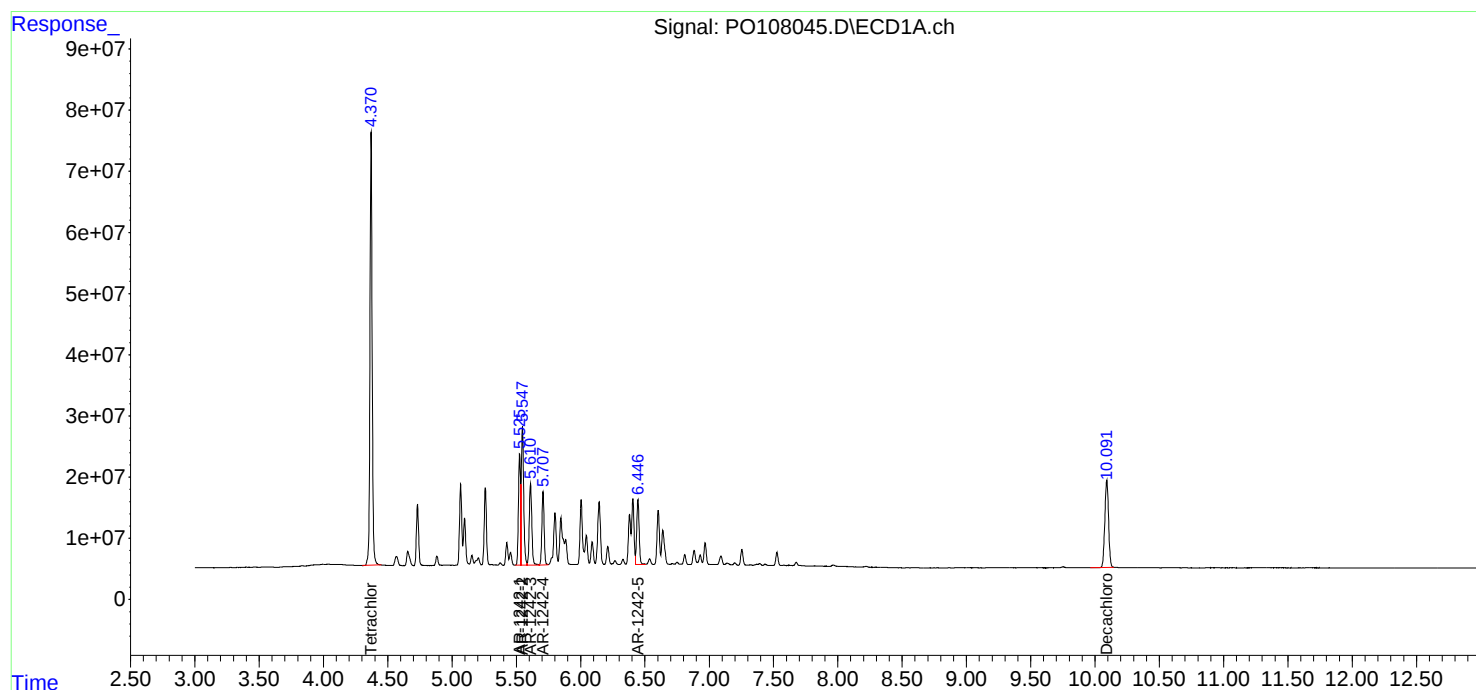

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108046.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 17:42
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:40:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 01:39:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.638	641.6E6	264.4E6	75.937	77.978
2) SA Decachlor...	10.091	8.634	224.5E6	259.6E6	72.141	74.380
Target Compounds						
16) L4 AR-1242-1	5.525	4.719	156.9E6	66186744	723.375	754.190
17) L4 AR-1242-2	5.547	4.738	225.7E6	94413539	735.507	771.718
18) L4 AR-1242-3	5.611	4.914	141.1E6	49994048	690.624	776.058
19) L4 AR-1242-4	5.708	4.997	113.9E6	46799288	770.362	757.610
20) L4 AR-1242-5	6.446	5.519	112.9E6	61241412	645.358	746.247



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108046.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 17:42
Operator : YP/AJ
Sample : AR1242ICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:40:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 01:39:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

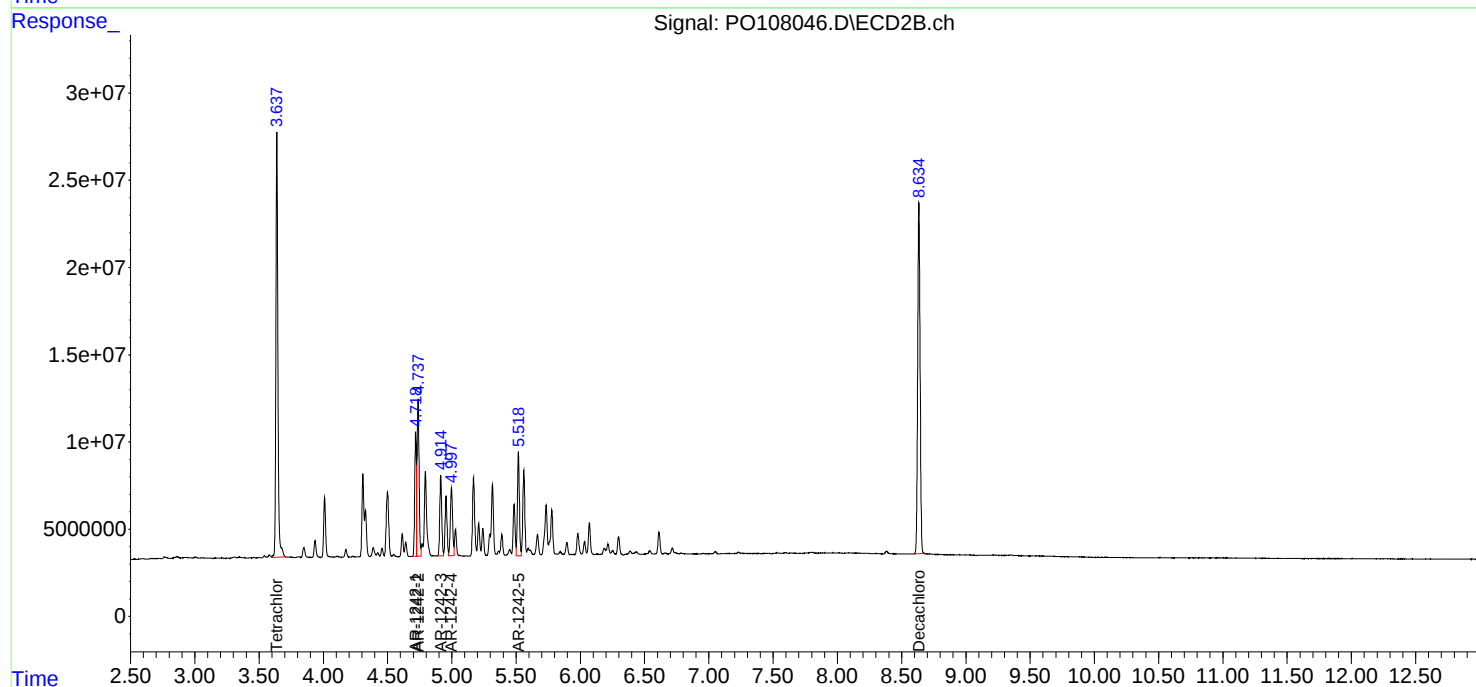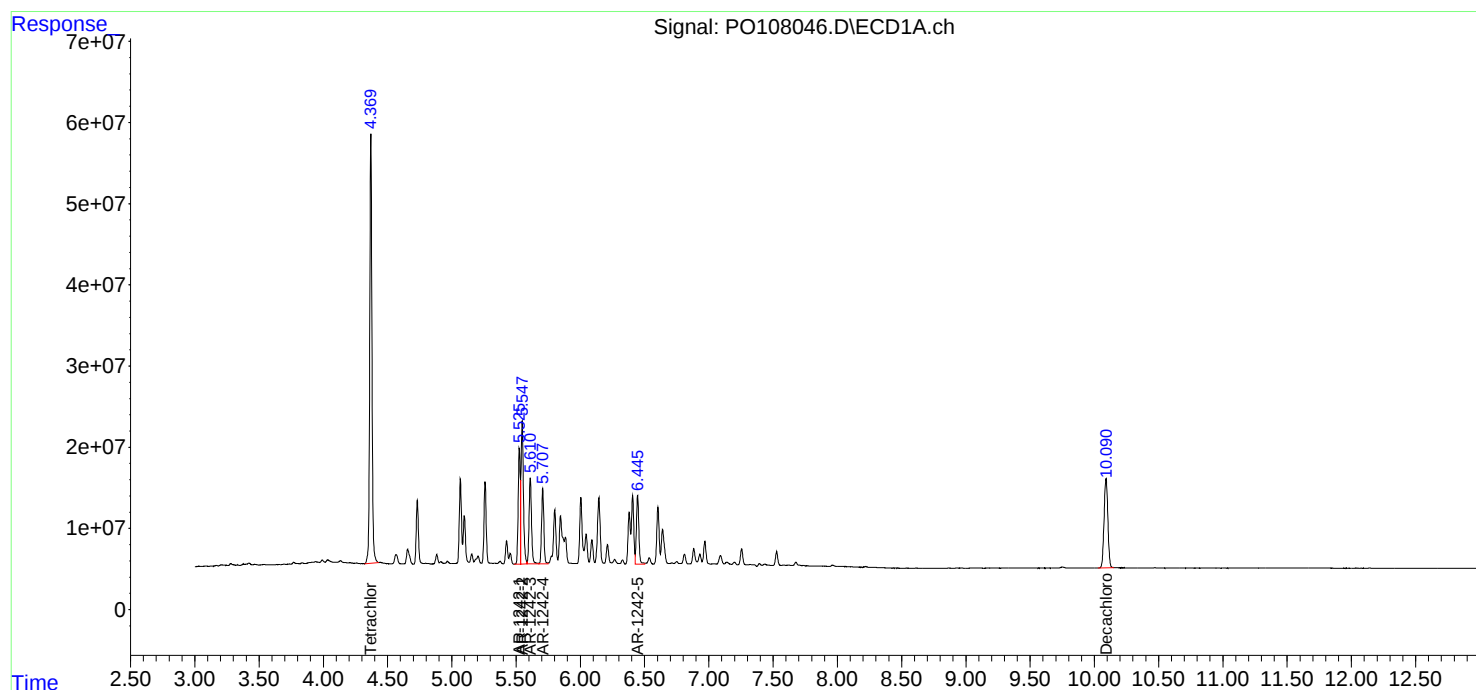

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 17:58
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:40:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 01:39:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.638	422.4E6	169.5E6	50.000	50.000
2) SA Decachlor...	10.087	8.634	155.6E6	174.5E6	50.000	50.000
Target Compounds						
16) L4 AR-1242-1	5.525	4.719	108.5E6	43879377	500.000	500.000
17) L4 AR-1242-2	5.548	4.738	153.5E6	61171012	500.000	500.000
18) L4 AR-1242-3	5.610	4.915	102.1E6	32210246	500.000	500.000
19) L4 AR-1242-4	5.708	4.998	73928462	30886124	500.000	500.000
20) L4 AR-1242-5	6.445	5.520	87443899	41032912	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 17:58
Operator : YP/AJ
Sample : AR1242ICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:40:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 01:39:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

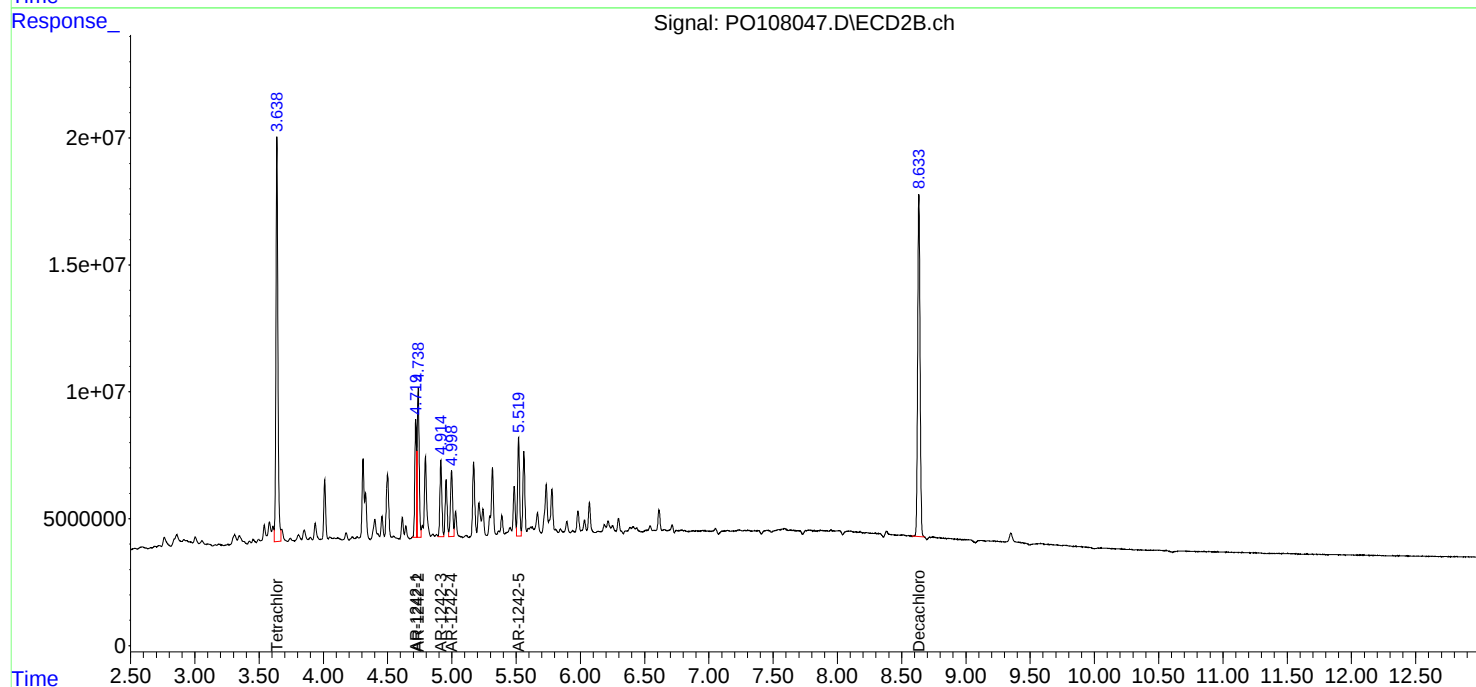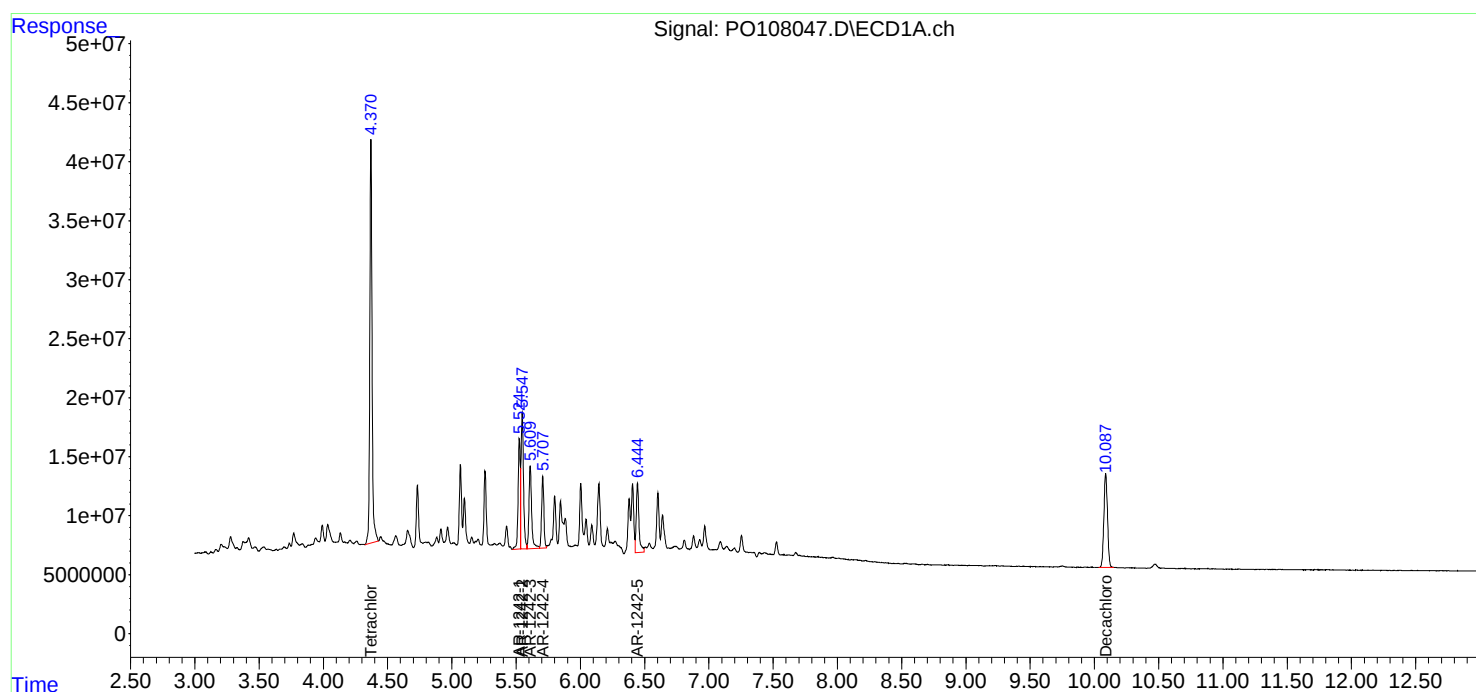

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 18:14
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:41:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 01:39:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.639	221.6E6	87332392	26.232	25.761
2) SA Decachlor...	10.091	8.635	83692924	89979899	26.892	25.784
Target Compounds						
16) L4 AR-1242-1	5.526	4.720	56708515	23358025	261.367	266.162
17) L4 AR-1242-2	5.547	4.739	81736032	32418064	266.322	264.979
18) L4 AR-1242-3	5.610	4.915	51676211	17326276	252.947	268.956
19) L4 AR-1242-4	5.708	4.998	40282436	16512294	272.442	267.309
20) L4 AR-1242-5	6.446	5.520	41393814	21904890	236.688	266.919



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 18:14
Operator : YP/AJ
Sample : AR1242ICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:41:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 01:39:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

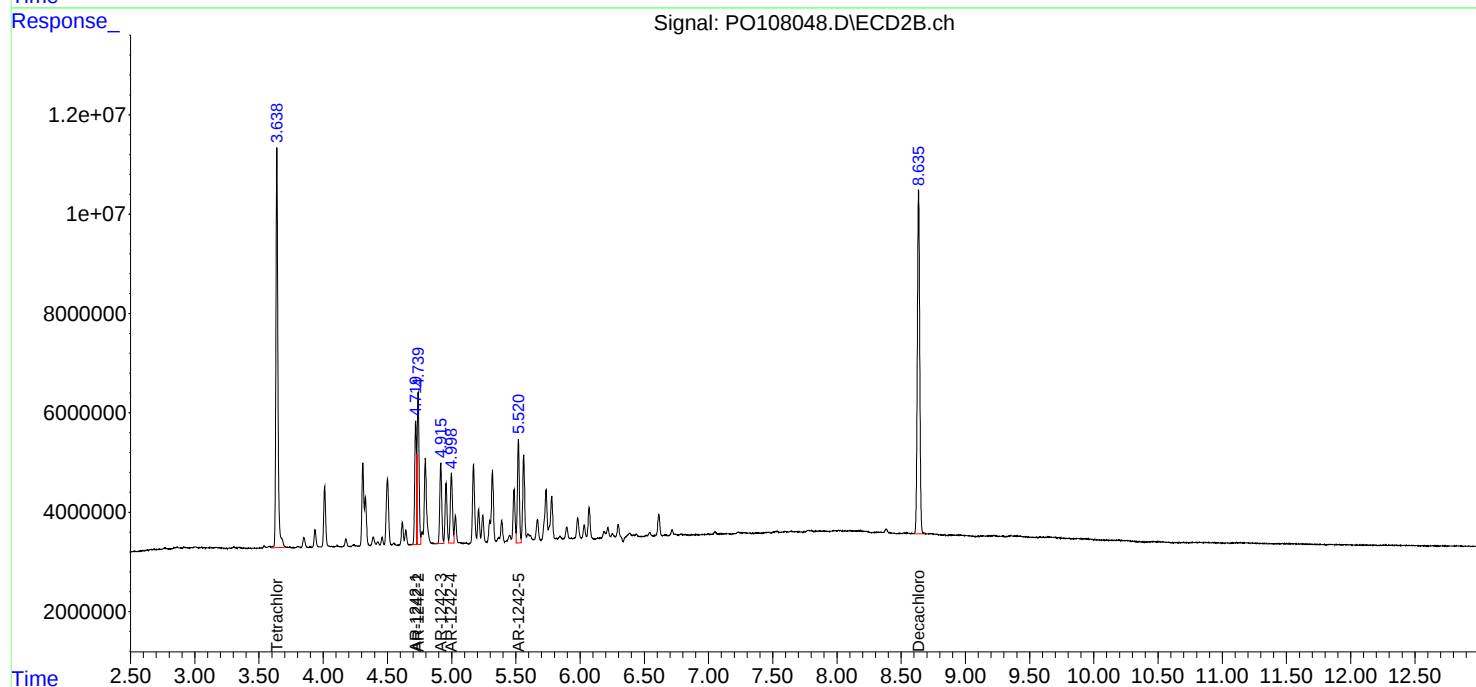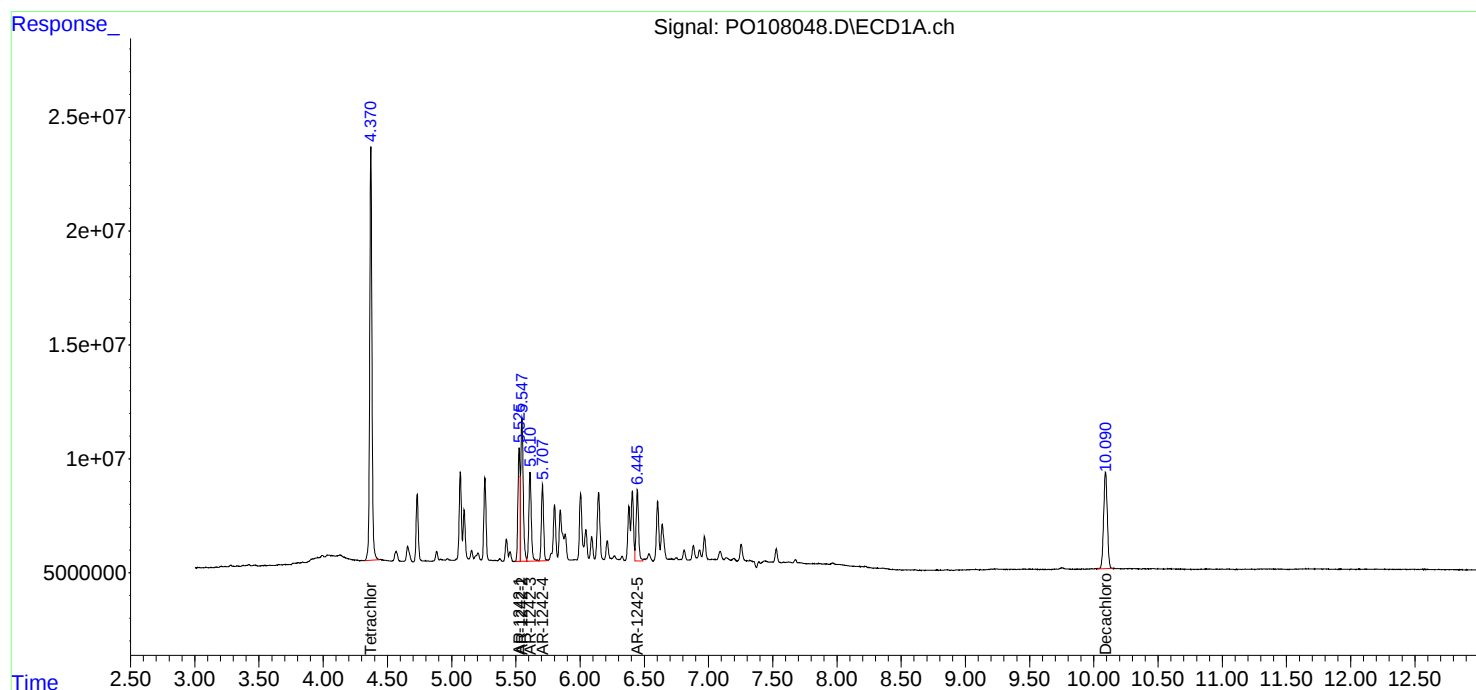

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108049.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 18:30
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:41:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 01:39:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.639	42229701	15650702	4.998	4.617
2) SA Decachlor...	10.091	8.635	16452927	16677202	5.287	4.779
Target Compounds						
16) L4 AR-1242-1	5.525	4.720	12560085	4253048	57.889	48.463
17) L4 AR-1242-2	5.548	4.739	17263302	5791443	56.249	47.338
18) L4 AR-1242-3	5.610	4.915	11635659	3247224	56.955	50.407
19) L4 AR-1242-4	5.708	4.998	8706512	3063203	58.885	49.589
20) L4 AR-1242-5	6.445	5.520	8590598	4299115	49.121m	52.386m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108049.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 18:30
Operator : YP/AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:41:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 01:39:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

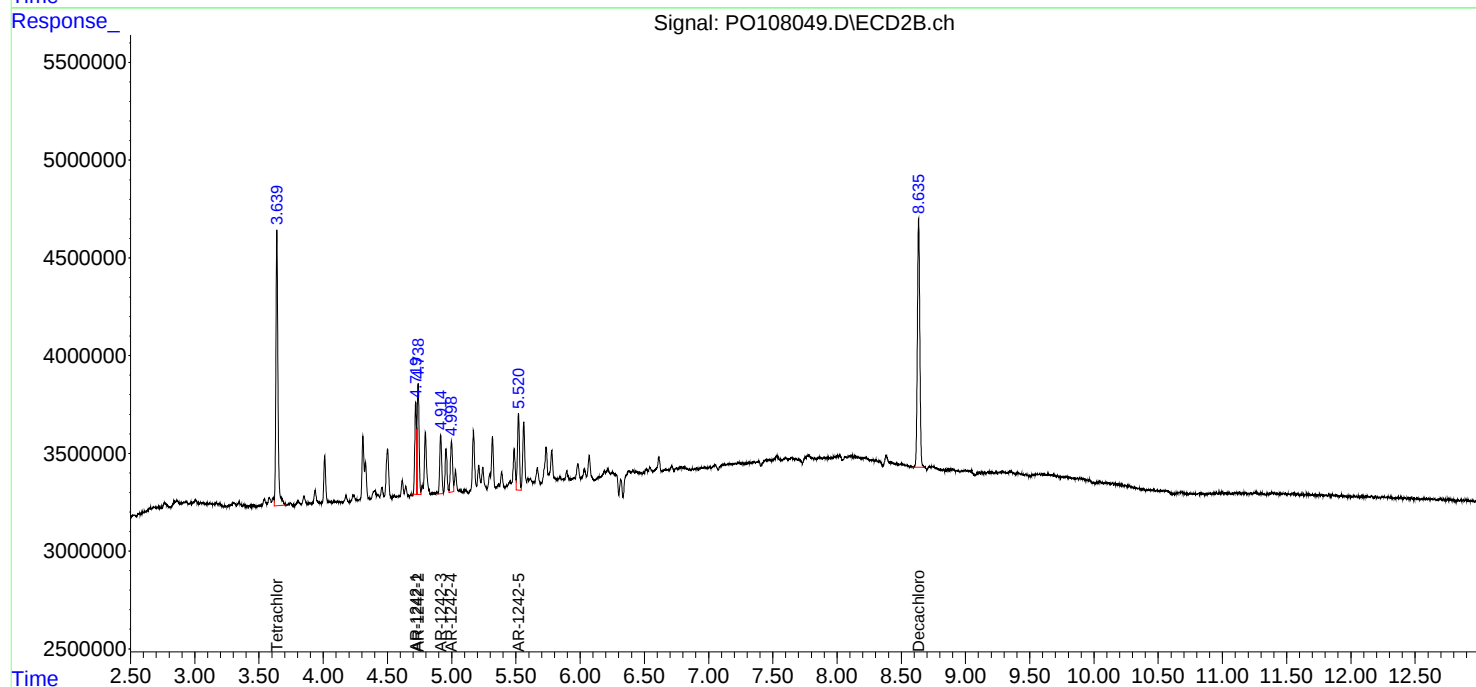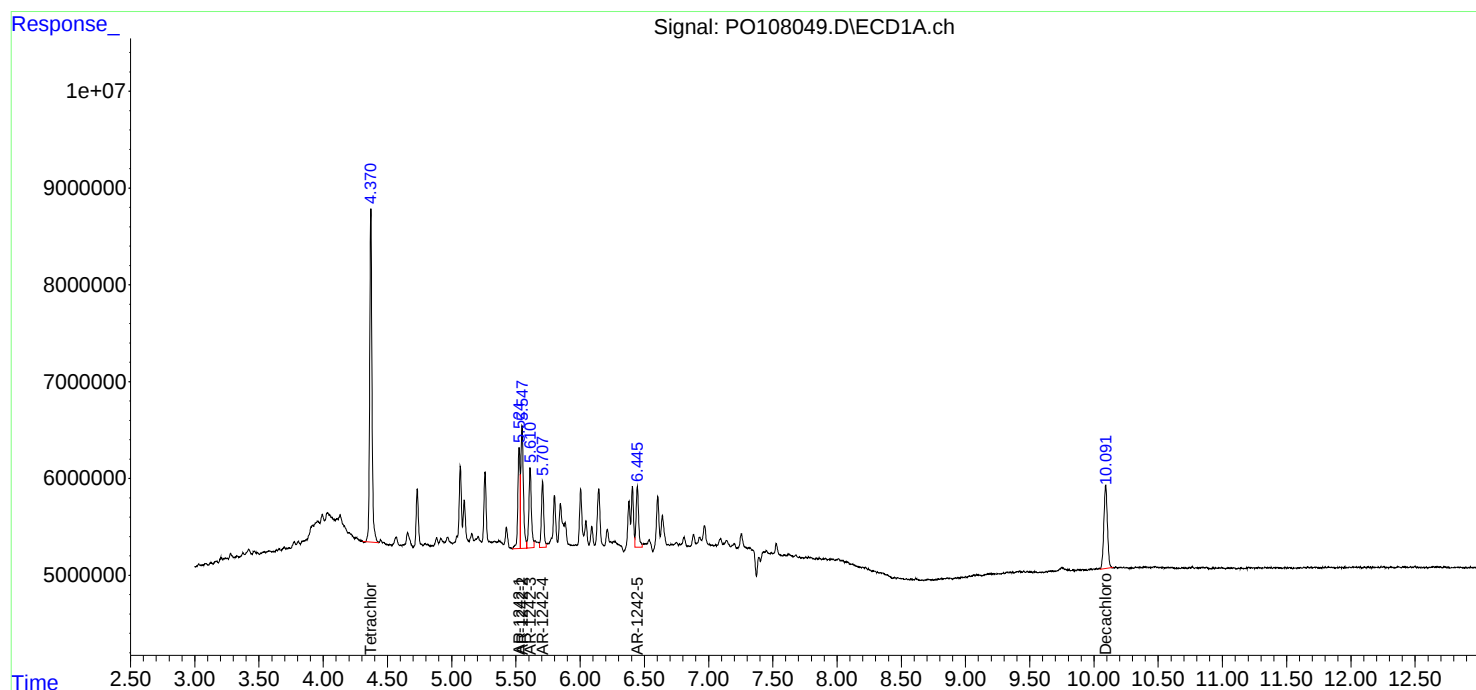

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 18:47
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:10:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:10:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.639	861.7E6	352.9E6	96.033	98.456
2) SA Decachlor...	10.090	8.635	305.6E6	352.9E6	91.937	97.558
Target Compounds						
21) L5 AR-1248-1	5.525	4.720	159.1E6	67026994	921.555	957.554
22) L5 AR-1248-2	5.801	4.956	223.7E6	89376189	916.112	943.656
23) L5 AR-1248-3	6.004	4.998	235.1E6	94788893	919.172	946.793
24) L5 AR-1248-4	6.407	5.170	254.9E6	115.5E6	920.193	955.388
25) L5 AR-1248-5	6.446	5.561	250.9E6	119.8E6	905.143	967.026



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 18:47
Operator : YP/AJ
Sample : AR1248ICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:10:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:10:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

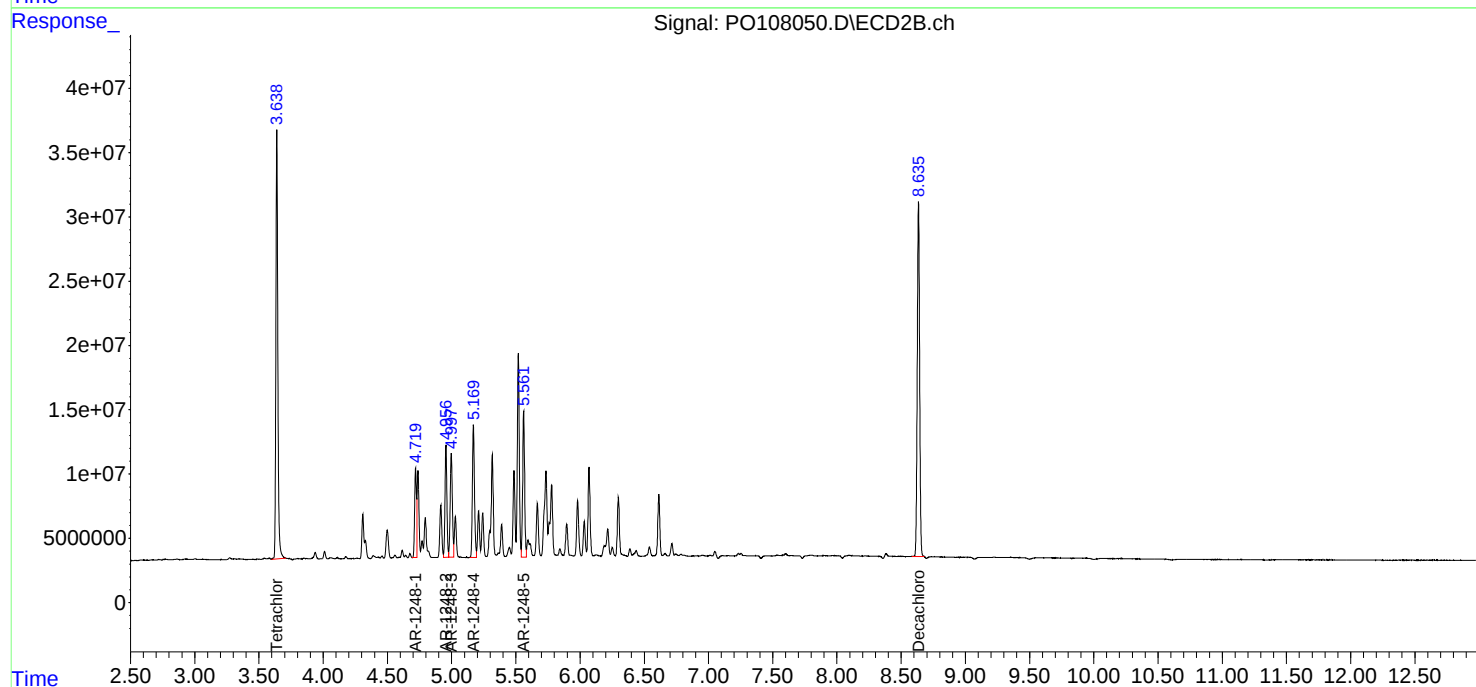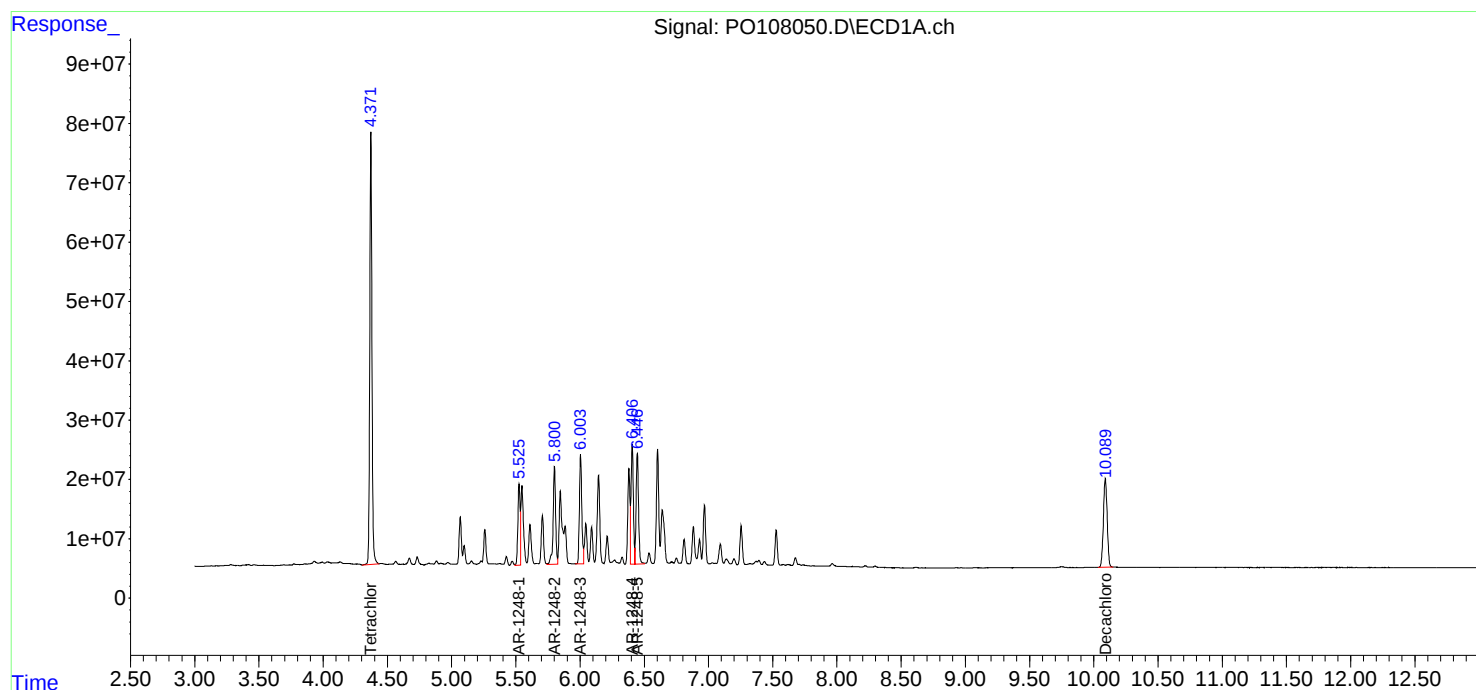

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 19:03
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:11:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:10:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.638	672.0E6	272.3E6	74.893	75.989
2) SA Decachlor...	10.090	8.633	240.9E6	269.8E6	72.486	74.587
Target Compounds						
21) L5 AR-1248-1	5.524	4.719	121.0E6	52170727	700.889	745.316
22) L5 AR-1248-2	5.800	4.956	174.3E6	70350934	713.807	742.783
23) L5 AR-1248-3	6.003	4.997	187.4E6	74183280	732.966	740.975
24) L5 AR-1248-4	6.407	5.169	203.0E6	90096148	732.820	745.077
25) L5 AR-1248-5	6.446	5.561	198.6E6	92492257	716.467	746.569



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 19:03
Operator : YP/AJ
Sample : AR1248ICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:11:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:10:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

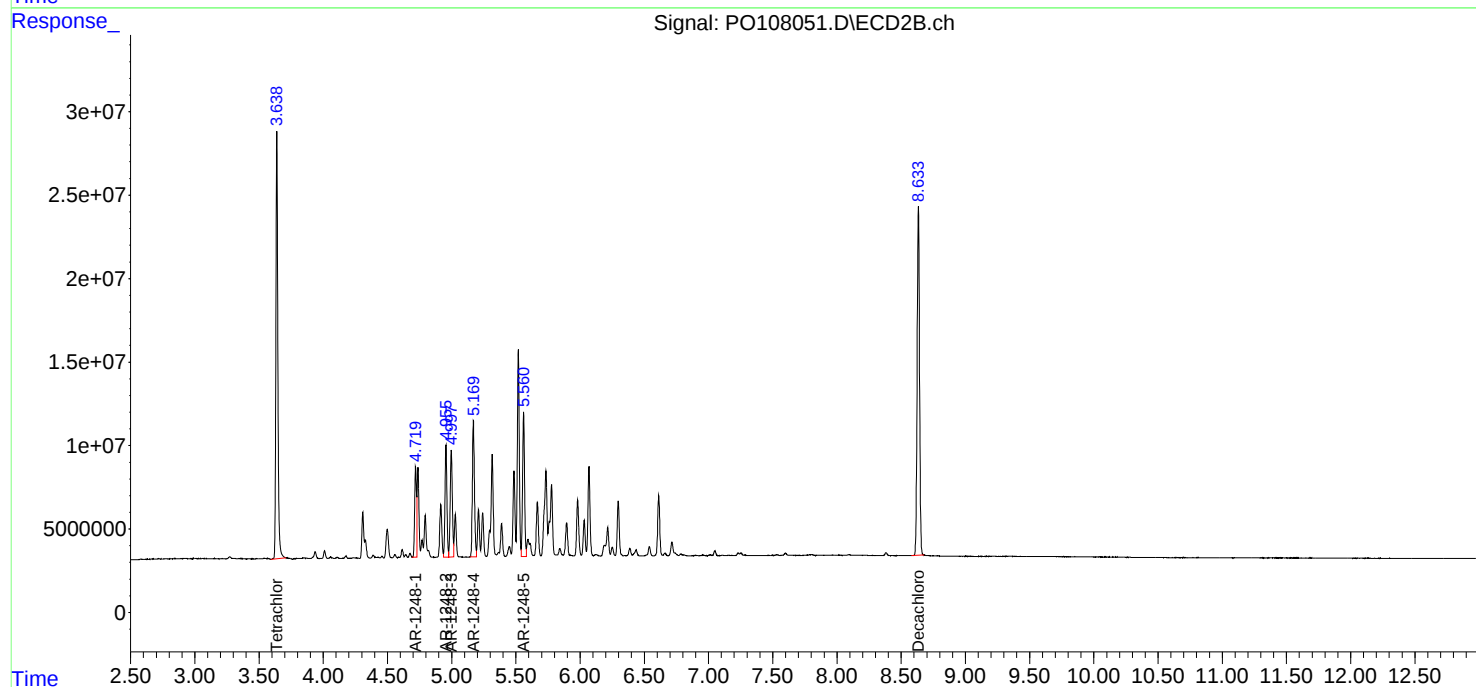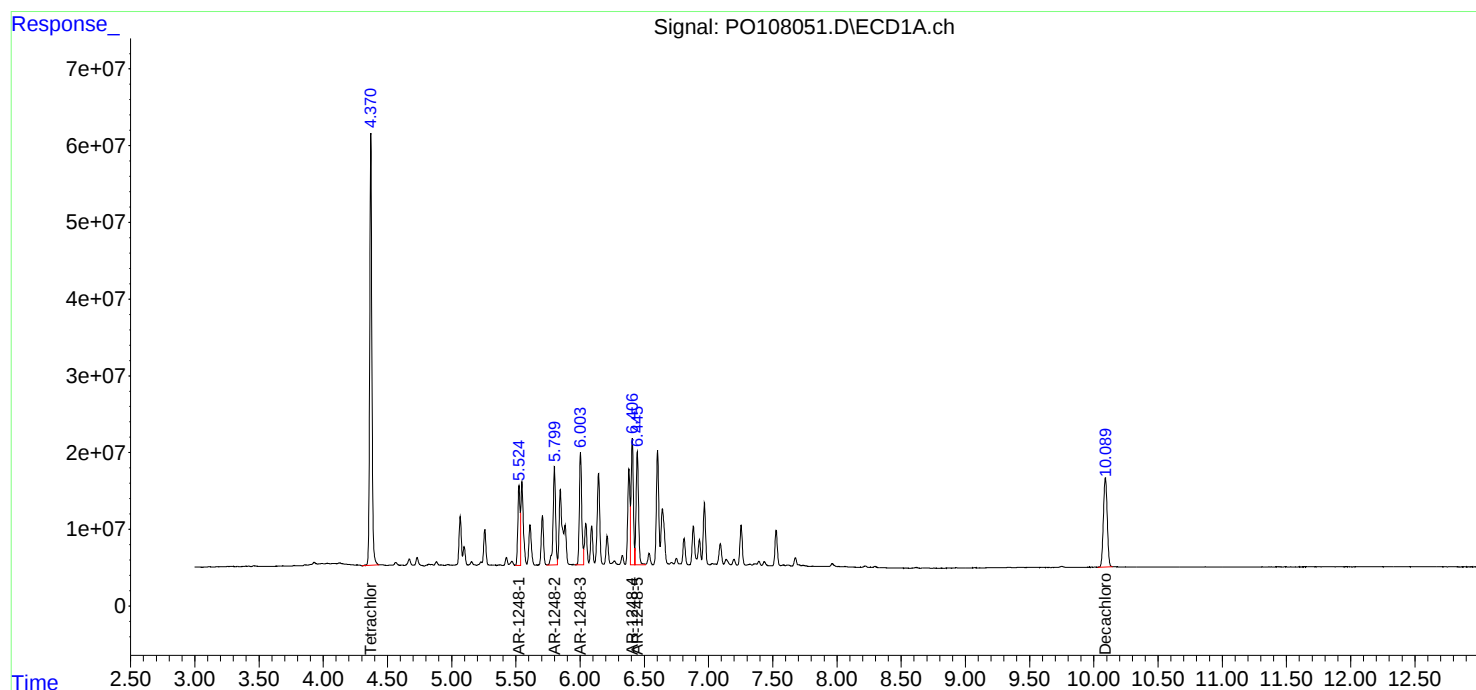

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 19:19
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:11:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:10:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.639	448.7E6	179.2E6	50.000	50.000
2) SA Decachlor...	10.091	8.635	166.2E6	180.8E6	50.000	50.000
Target Compounds						
21) L5 AR-1248-1	5.525	4.720	86331732	34999061	500.000	500.000
22) L5 AR-1248-2	5.801	4.956	122.1E6	47356320	500.000	500.000
23) L5 AR-1248-3	6.004	4.998	127.9E6	50057870	500.000	500.000
24) L5 AR-1248-4	6.406	5.169	138.5E6	60460949	500.000	500.000
25) L5 AR-1248-5	6.446	5.561	138.6E6	61944862	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 19:19
Operator : YP/AJ
Sample : AR1248ICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:11:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:10:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

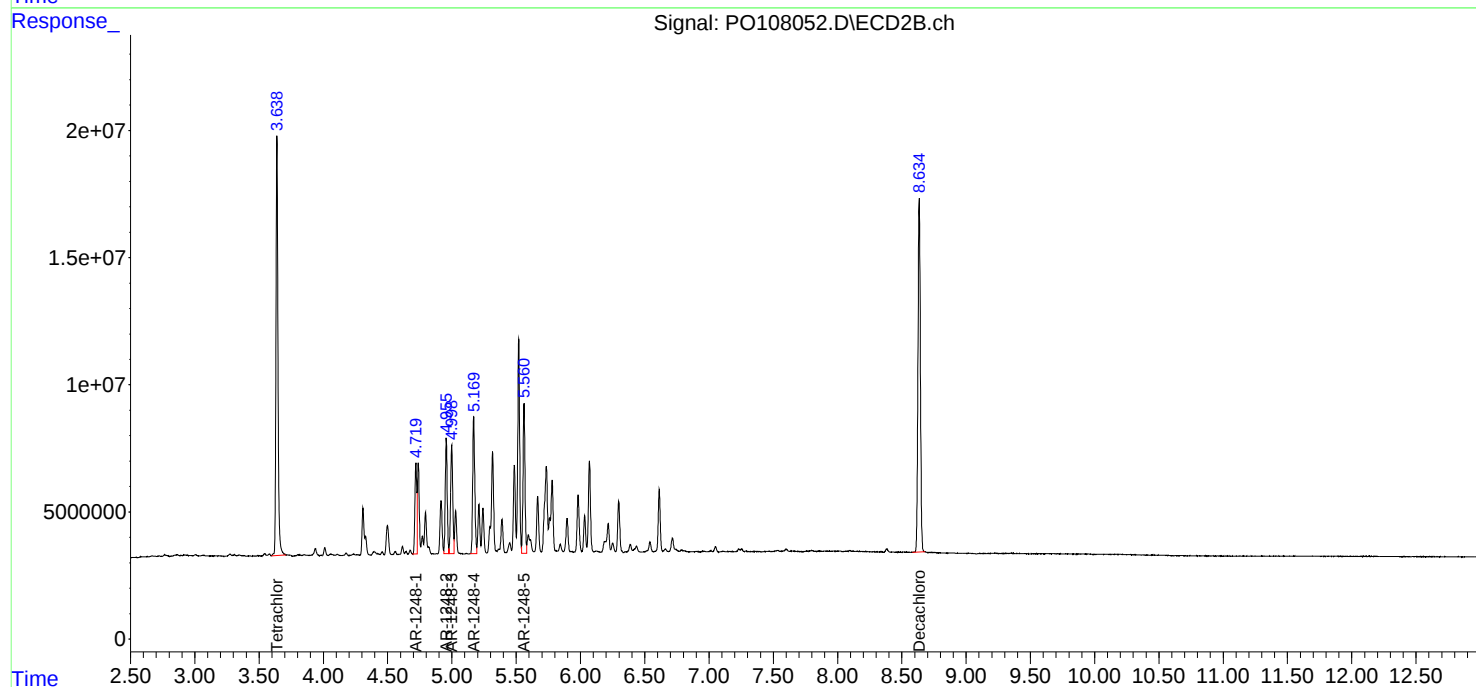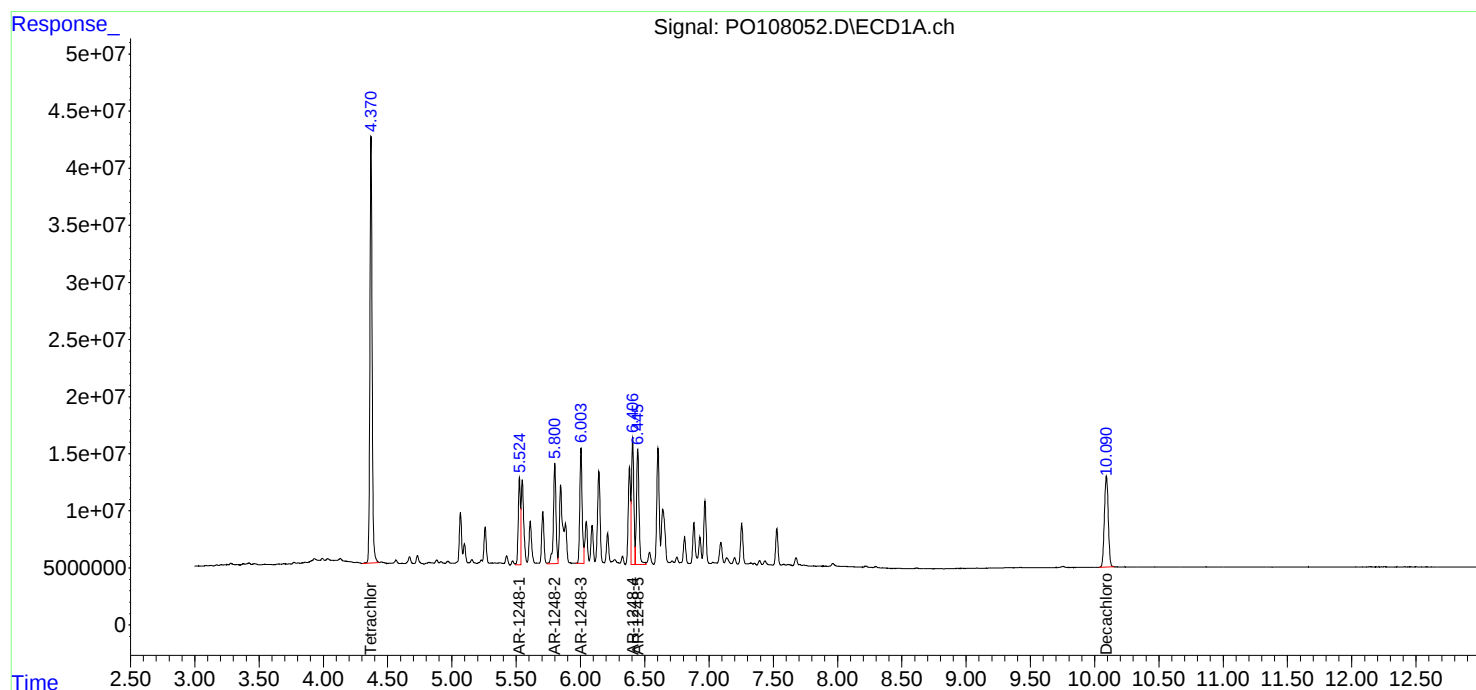

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108053.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 19:35
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:11:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:10:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.639	228.7E6	88995106	25.491	24.832
2) SA Decachlor...	10.092	8.634	87569622	91586360	26.346	25.322
Target Compounds						
21) L5 AR-1248-1	5.525	4.719	45463187	17907228	263.305	255.824
22) L5 AR-1248-2	5.800	4.956	64260496	24426603	263.203	257.902
23) L5 AR-1248-3	6.003	4.998	67584896	25819680	264.291	257.898
24) L5 AR-1248-4	6.407	5.170	72745239	31308387	262.647	258.914
25) L5 AR-1248-5	6.445	5.561	72886552	32013659	262.994	258.404



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108053.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 19:35
Operator : YP/AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:11:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:10:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

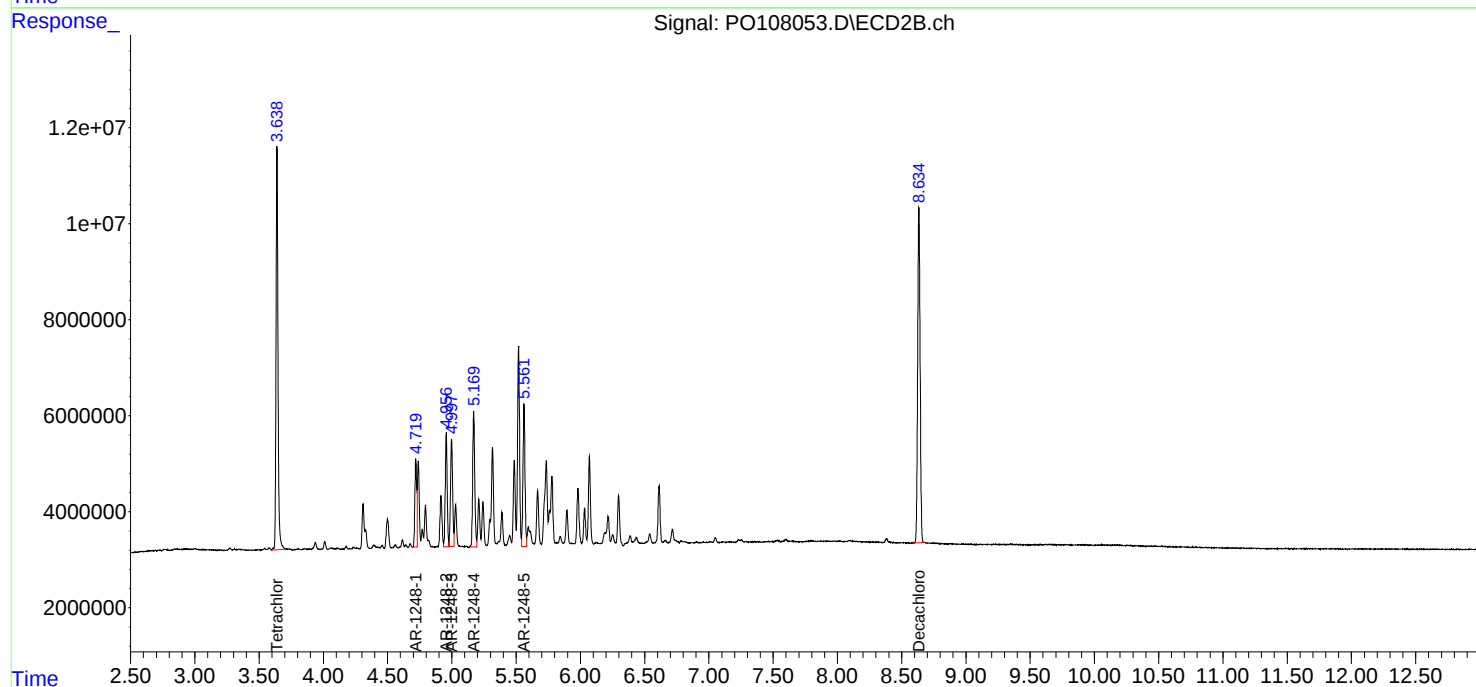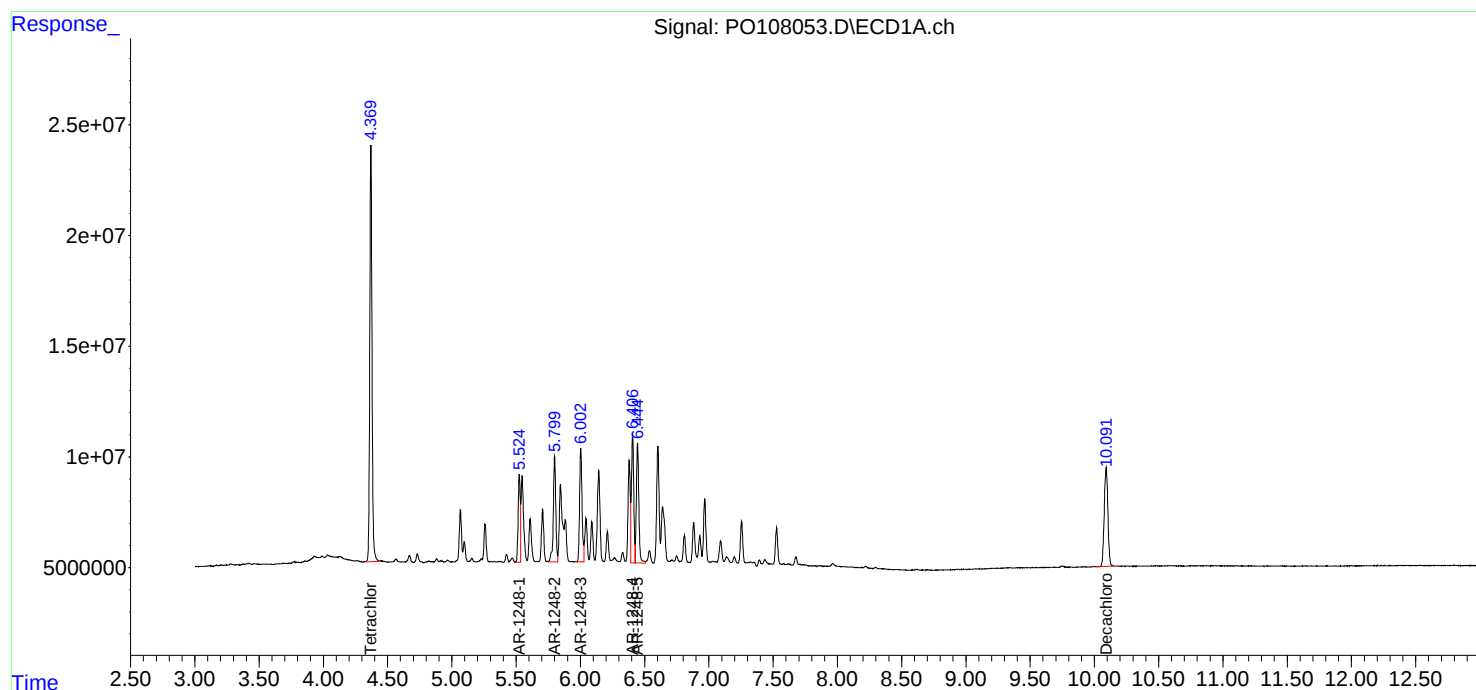

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 19:51
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:11:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:10:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.639	42994877	15859601	4.792	4.425
2) SA Decachlor...	10.092	8.635	17354361	16886224	5.221	4.669
Target Compounds						
21) L5 AR-1248-1	5.525	4.720	9698243	3441339	56.168	49.163
22) L5 AR-1248-2	5.800	4.957	12265616	4560396	50.238	48.150
23) L5 AR-1248-3	6.004	4.998	13569509	4825714	53.064	48.201
24) L5 AR-1248-4	6.406	5.169	13569456	5968209	48.993m	49.356
25) L5 AR-1248-5	6.445	5.561	13533580	6403673	48.833m	51.688m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 19:51
Operator : YP/AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:11:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:10:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

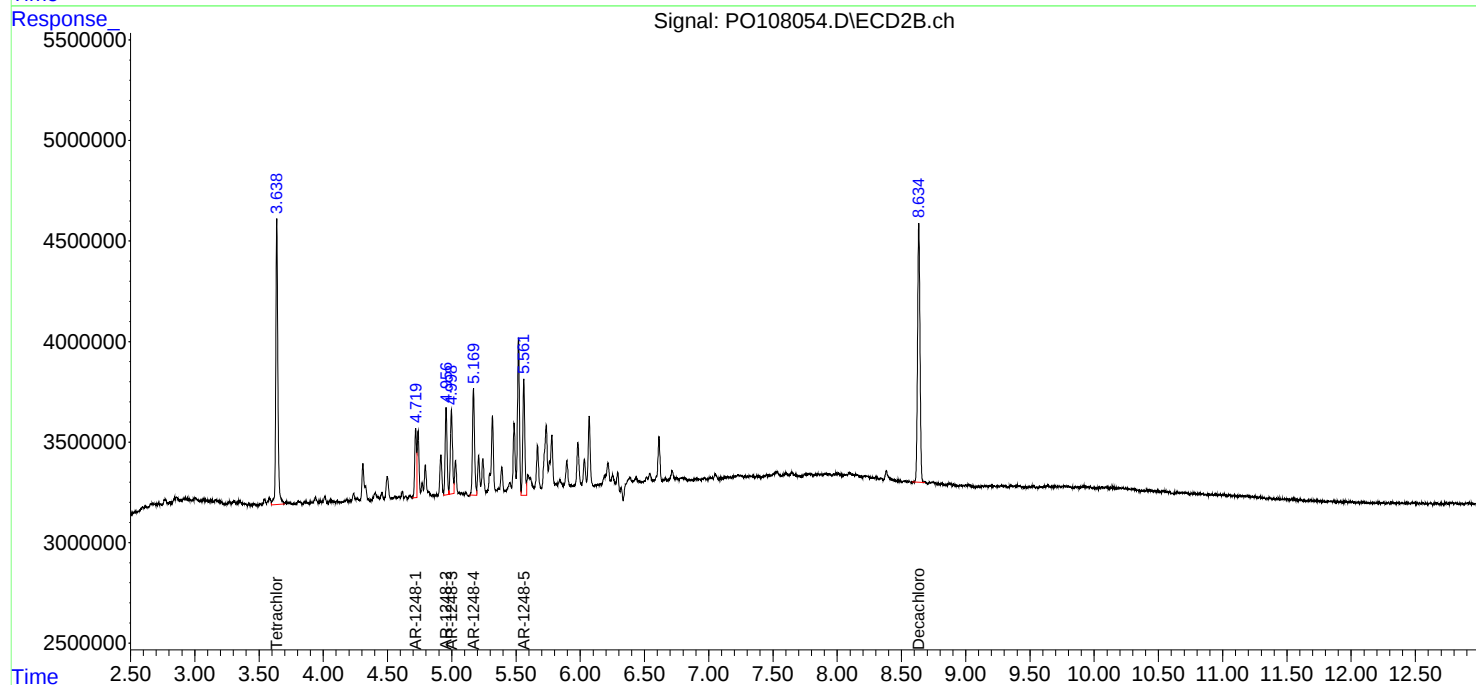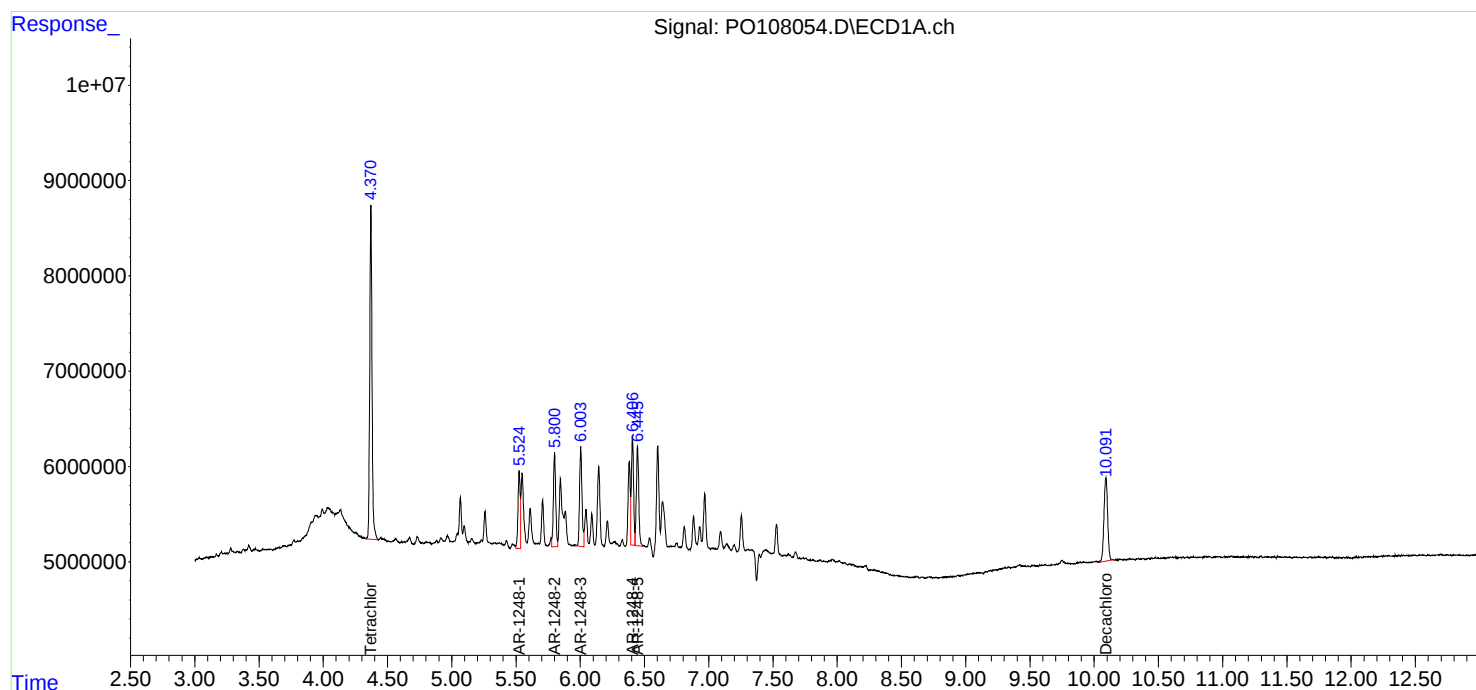

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108055.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 20:07
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:28:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:27:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.639	867.6E6	356.1E6	96.056	97.907
2) SA Decachlor...	10.092	8.635	305.3E6	348.9E6	90.565	95.179
Target Compounds						
26) L6 AR-1254-1	6.383	5.520	252.3E6	174.3E6	921.524	963.496
27) L6 AR-1254-2	6.603	5.668	370.7E6	150.1E6	923.294	952.032
28) L6 AR-1254-3	6.969	6.071	371.0E6	256.2E6	937.587	965.273
29) L6 AR-1254-4	7.255	6.299	259.0E6	157.0E6	925.251	1035.618
30) L6 AR-1254-5	7.678	6.716	253.3E6	226.5E6	924.405	963.749



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108055.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 20:07
Operator : YP/AJ
Sample : AR1254ICC1000
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:28:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:27:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

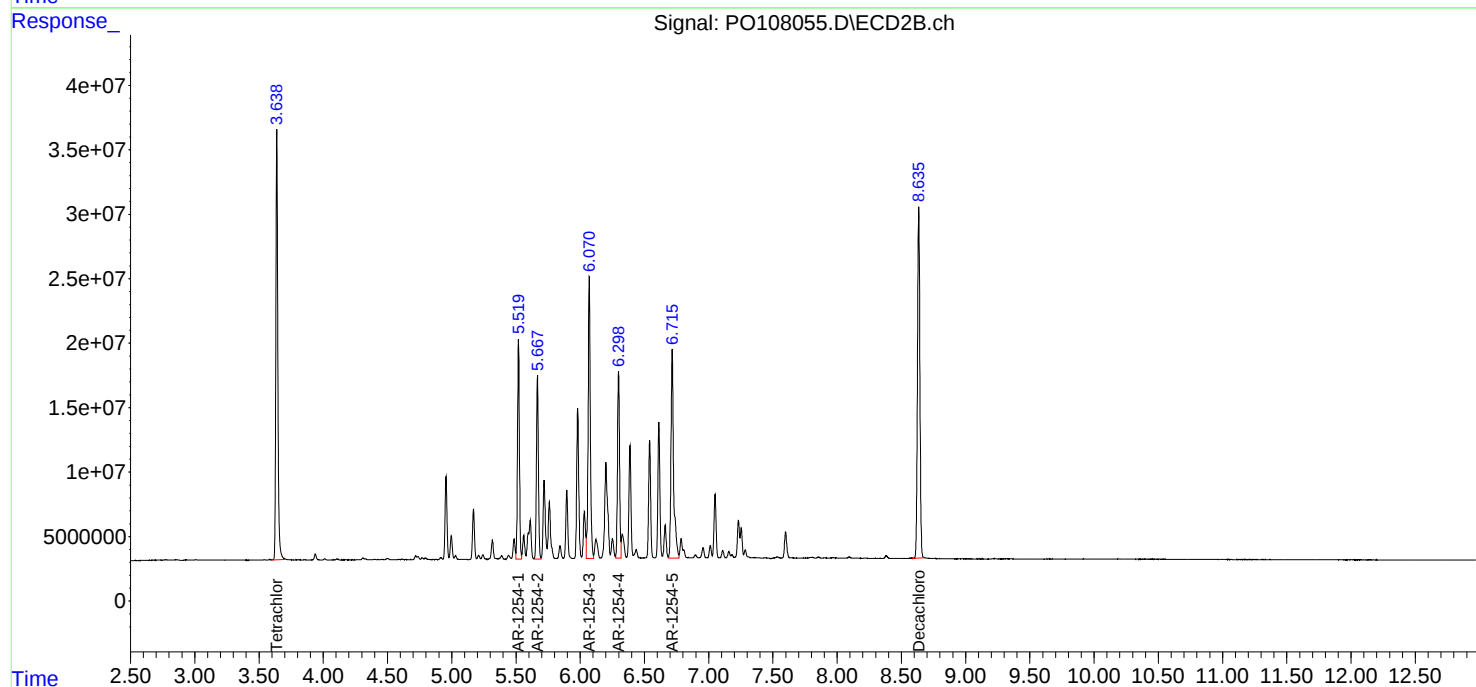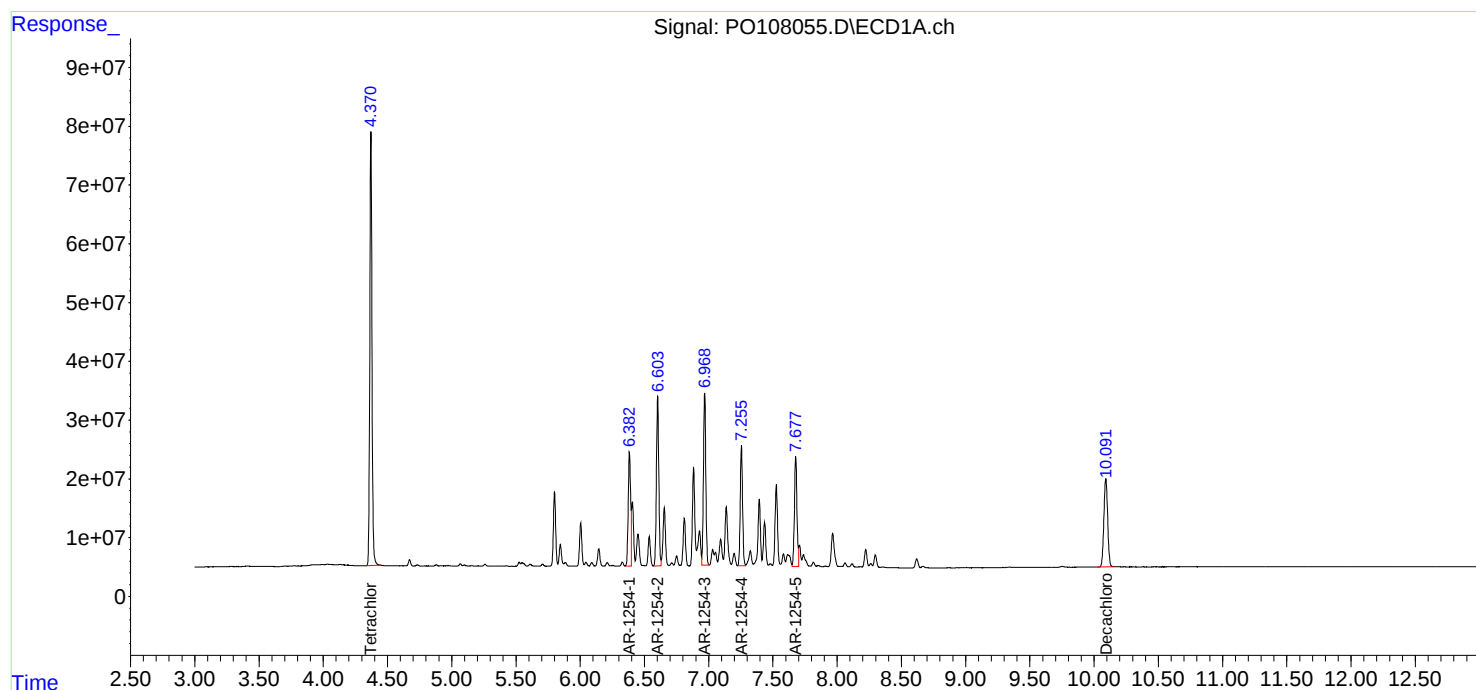

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108056.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 20:24
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:28:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:27:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.639	658.6E6	267.8E6	72.917	73.633
2) SA Decachlor...	10.091	8.635	238.2E6	267.6E6	70.644	73.003
Target Compounds						
26) L6 AR-1254-1	6.384	5.520	198.3E6	132.1E6	724.307	730.370
27) L6 AR-1254-2	6.603	5.668	286.3E6	114.7E6	713.116	727.509
28) L6 AR-1254-3	6.969	6.070	283.7E6	194.6E6	716.957	733.225
29) L6 AR-1254-4	7.256	6.299	199.4E6	112.6E6	712.328	742.670
30) L6 AR-1254-5	7.678	6.716	195.7E6	171.7E6	714.461	730.445



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108056.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 20:24
Operator : YP/AJ
Sample : AR1254ICC750
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:28:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:27:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

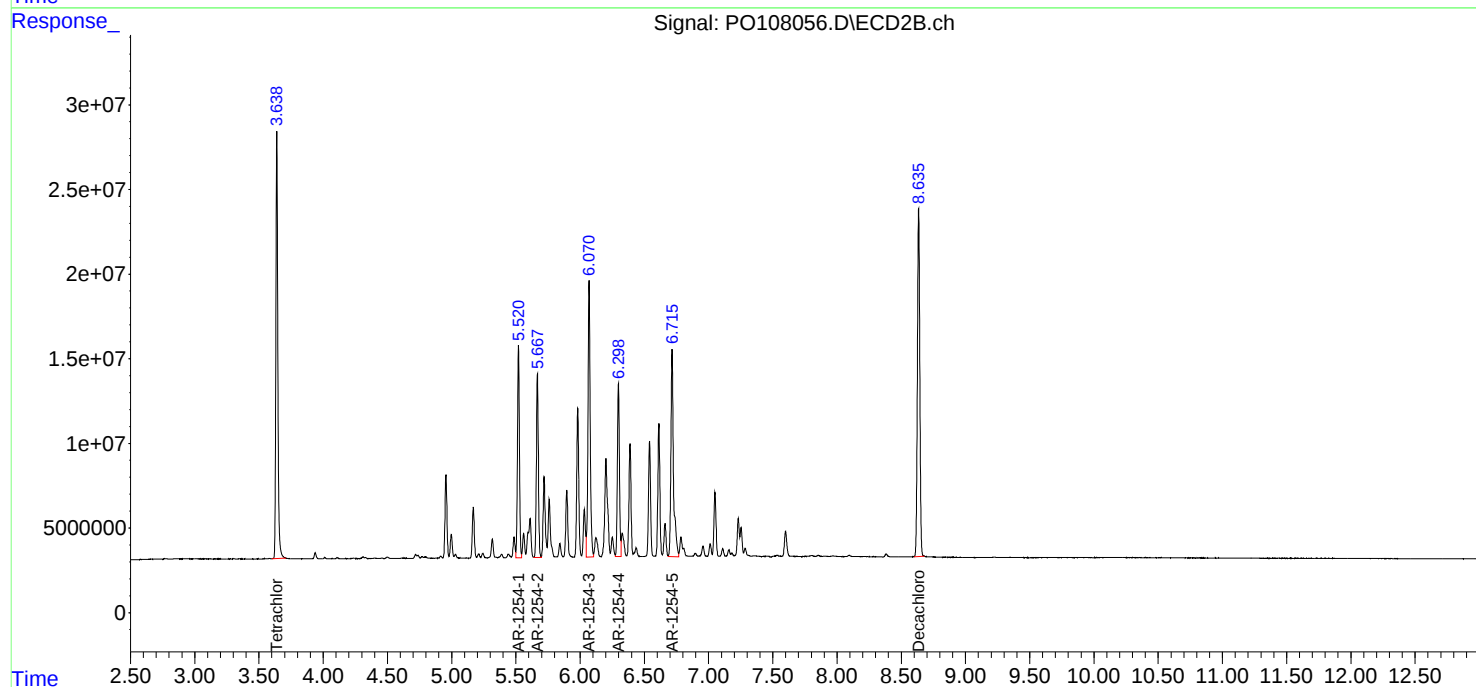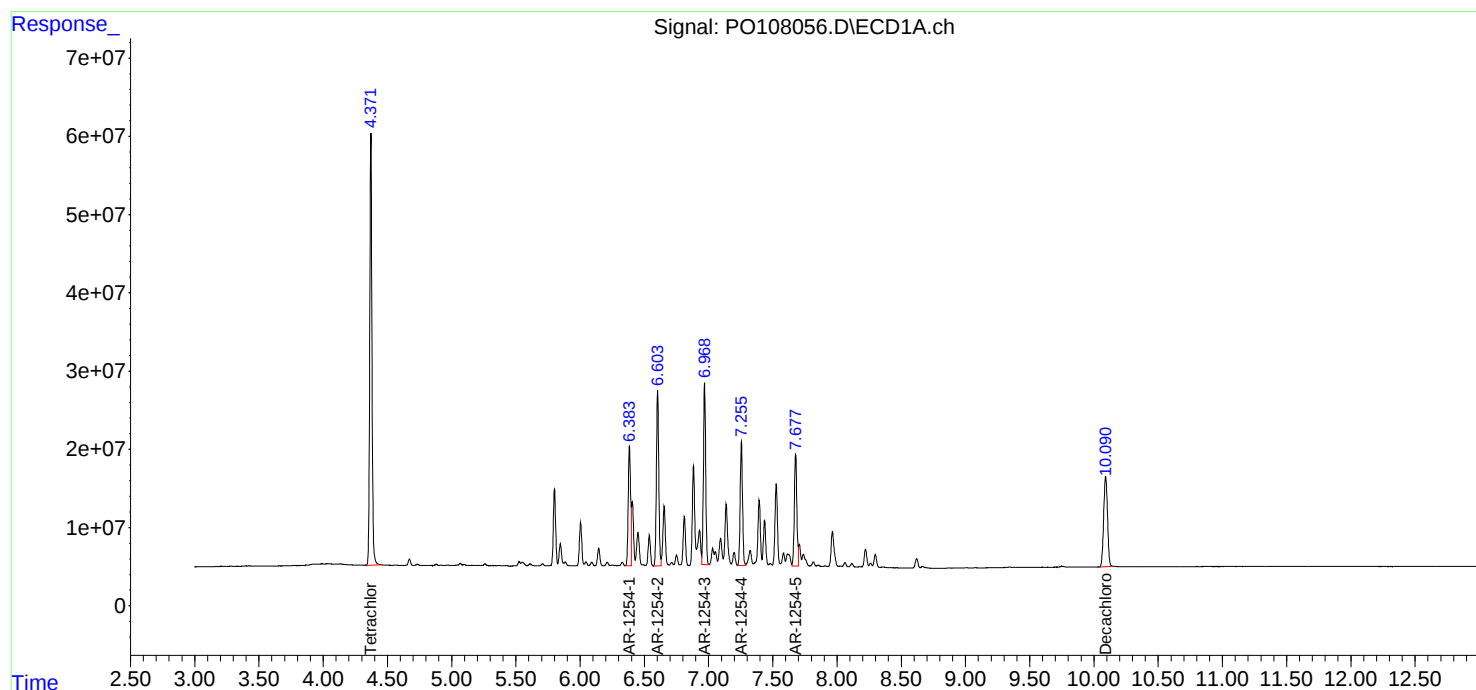

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 20:40
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:28:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:27:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.637	451.6E6	181.9E6	50.000	50.000
2) SA Decachlor...	10.088	8.633	168.6E6	183.3E6	50.000	50.000
Target Compounds						
26) L6 AR-1254-1	6.382	5.519	136.9E6	90446534	500.000	500.000
27) L6 AR-1254-2	6.601	5.667	200.8E6	78836003	500.000	500.000
28) L6 AR-1254-3	6.967	6.069	197.9E6	132.7E6	500.000	500.000
29) L6 AR-1254-4	7.253	6.297	140.0E6	75824147	500.000	500.000
30) L6 AR-1254-5	7.675	6.715	137.0E6	117.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 20:40
Operator : YP/AJ
Sample : AR1254ICC500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:28:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:27:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

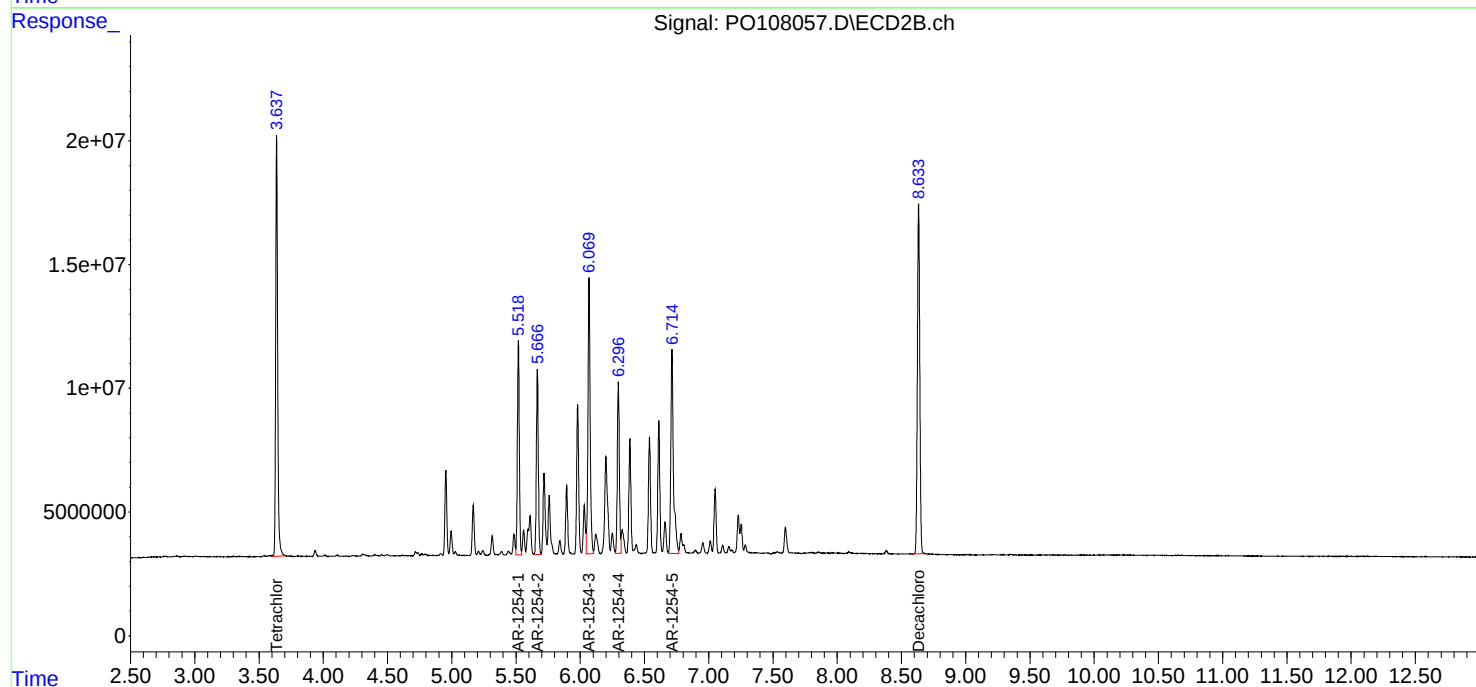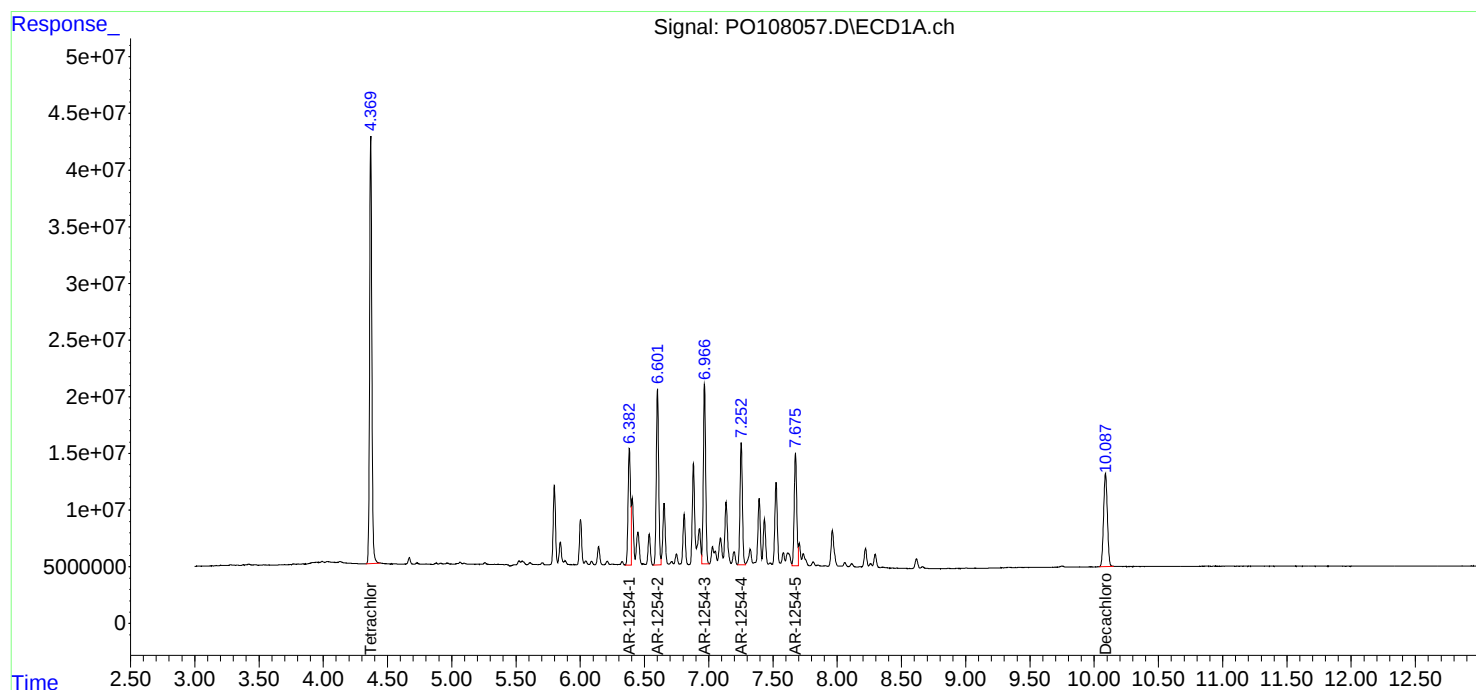

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 20:56
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:29:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:27:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.638	231.3E6	90248836	25.610	24.811
2) SA Decachlor...	10.091	8.635	88991947	93171689	26.397	25.419
Target Compounds						
26) L6 AR-1254-1	6.383	5.520	73263320	46503397	267.621	257.077
27) L6 AR-1254-2	6.603	5.667	107.8E6	40762092	268.371	258.525
28) L6 AR-1254-3	6.969	6.071	103.4E6	67332028	261.226	253.645
29) L6 AR-1254-4	7.255	6.298	73926777	37563766	264.107	247.703
30) L6 AR-1254-5	7.677	6.716	72271297	59536924	263.798	253.311



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 20:56
Operator : YP/AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:29:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:27:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

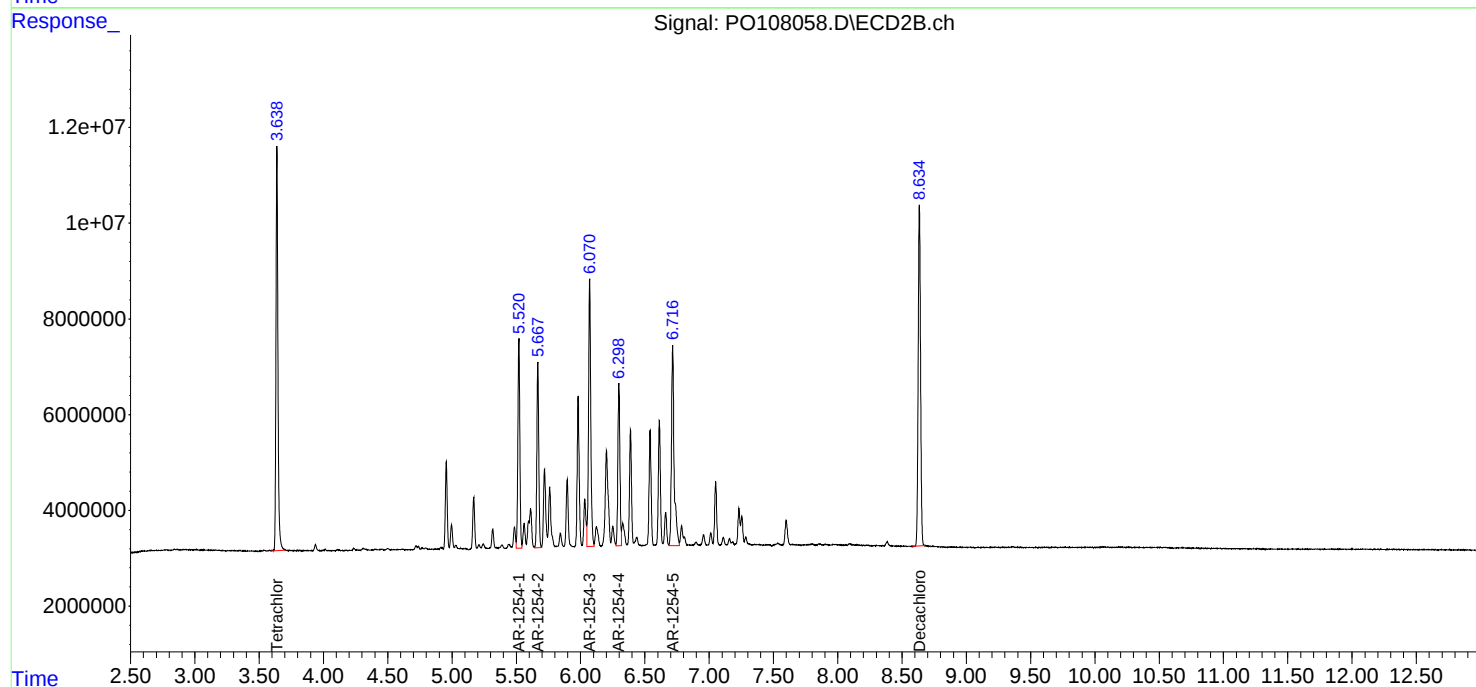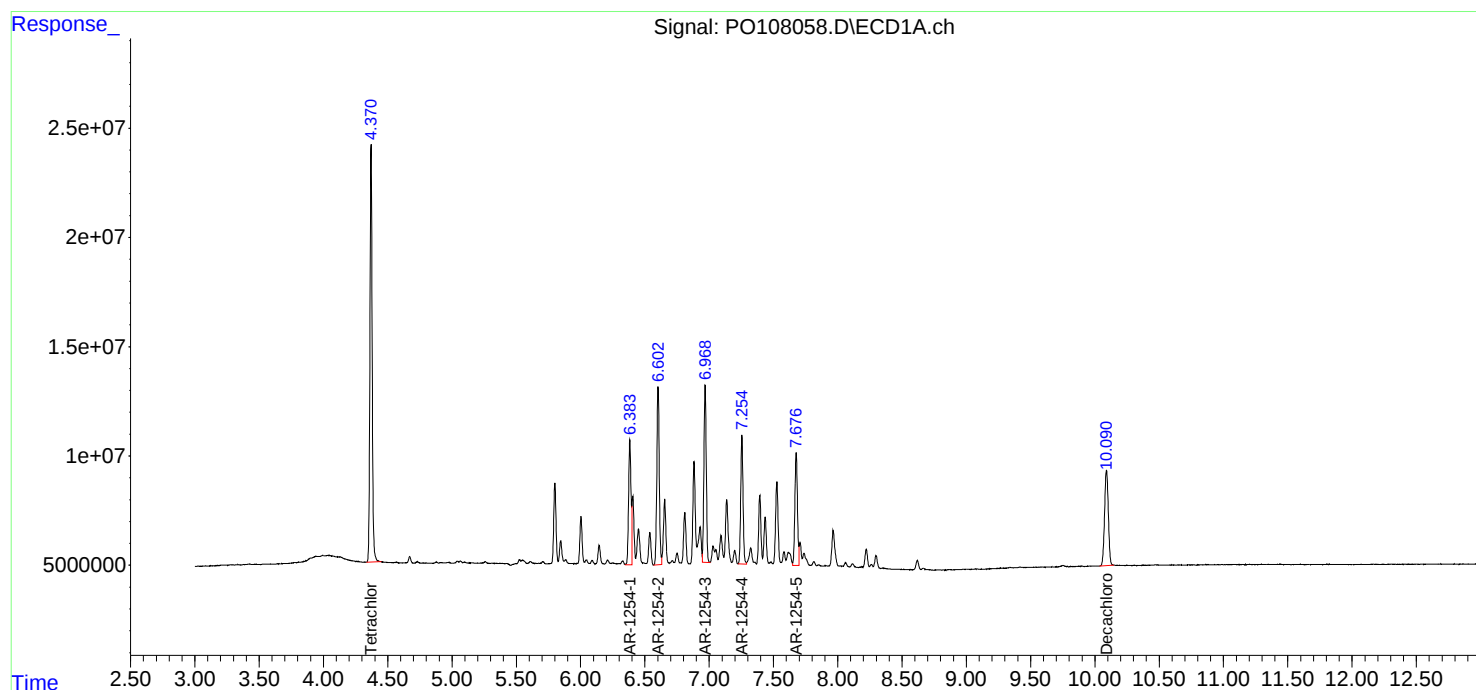

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108059.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 21:12
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:29:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:27:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.639	42601059	15944957	4.716	4.384
2) SA Decachlor...	10.090	8.635	17365833	17187174	5.151	4.689
Target Compounds						
26) L6 AR-1254-1	6.383	5.520	15071614	8397421	55.055	46.422
27) L6 AR-1254-2	6.603	5.668	22619876	7724026	56.336	48.988
28) L6 AR-1254-3	6.968	6.071	20213311	12239490	51.079m	46.107
29) L6 AR-1254-4	7.254	6.297	14761116	5749350	52.735m	37.912m#
30) L6 AR-1254-5	7.676	6.716	13194661	10827771	48.162m	46.069

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108059.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 21:12
Operator : YP/AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:29:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:27:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

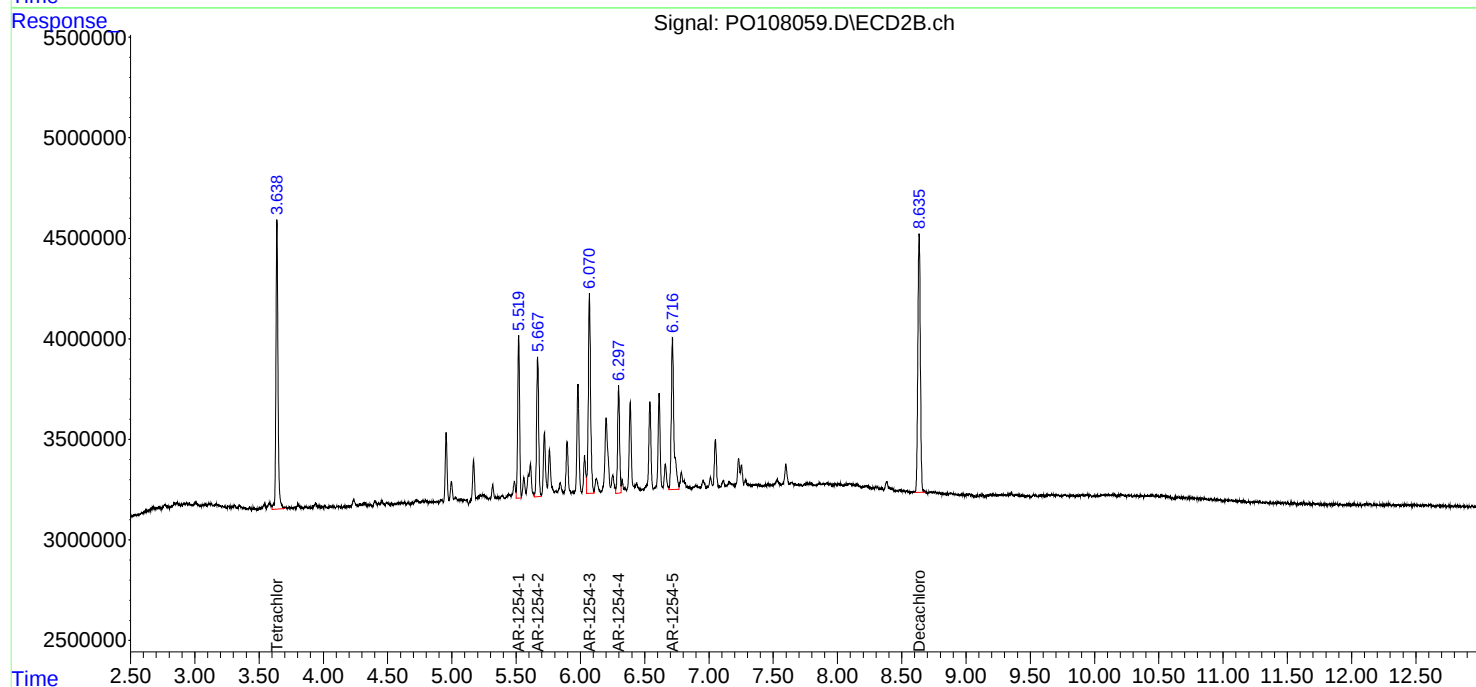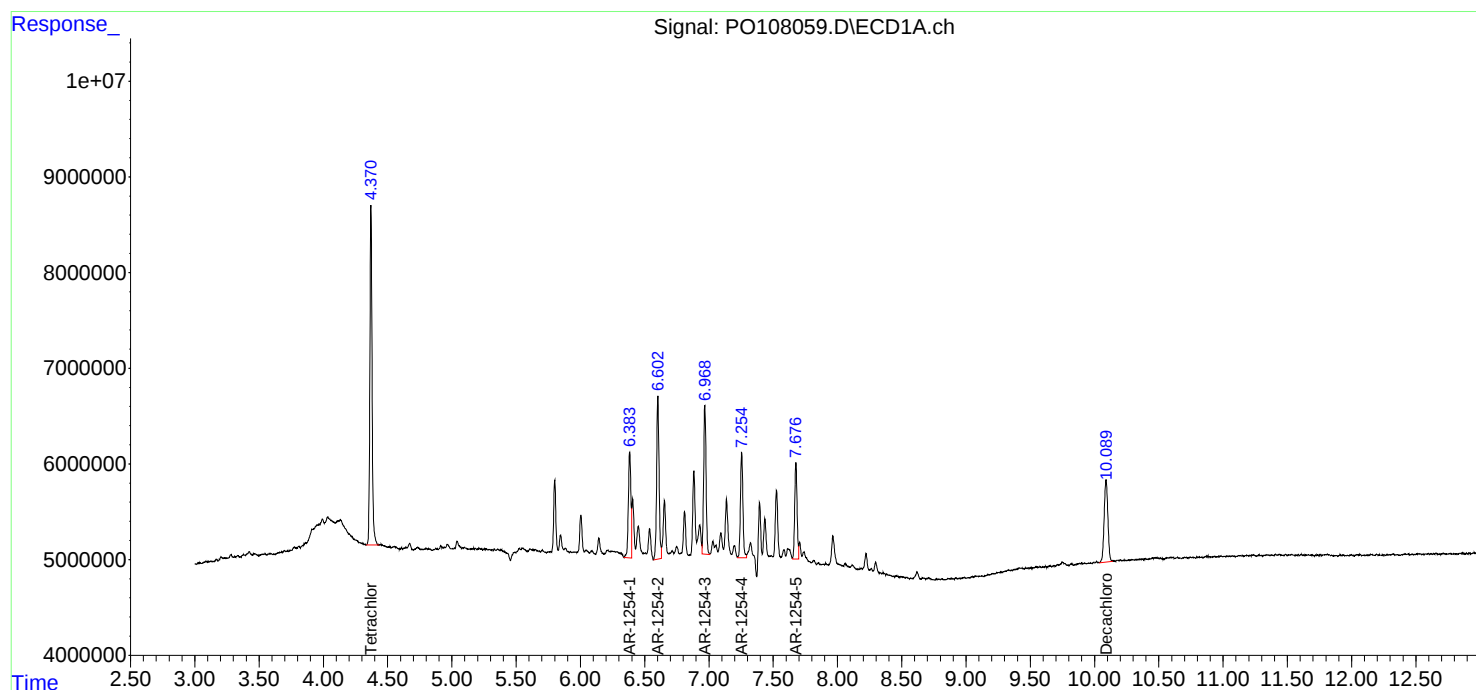

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108060.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 21:28
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:42:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:42:12 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.638	425.1E6	169.1E6	50.000	50.000
2) SA Decachlor...	10.089	8.633	158.6E6	169.0E6	50.000	50.000
Target Compounds						
36) L8 AR-1262-1	7.756	6.753	161.6E6	113.8E6	500.000	500.000
37) L8 AR-1262-2	8.297	7.253	225.0E6	213.5E6	500.000	500.000
38) L8 AR-1262-3	8.612	7.536	144.5E6	82555269	500.000	500.000
39) L8 AR-1262-4	8.697	7.600	111.6E6	159.0E6	500.000	500.000
40) L8 AR-1262-5	9.339	8.093	76010899	74010658	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108060.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 21:28
Operator : YP/AJ
Sample : AR1262ICC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:42:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:42:12 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

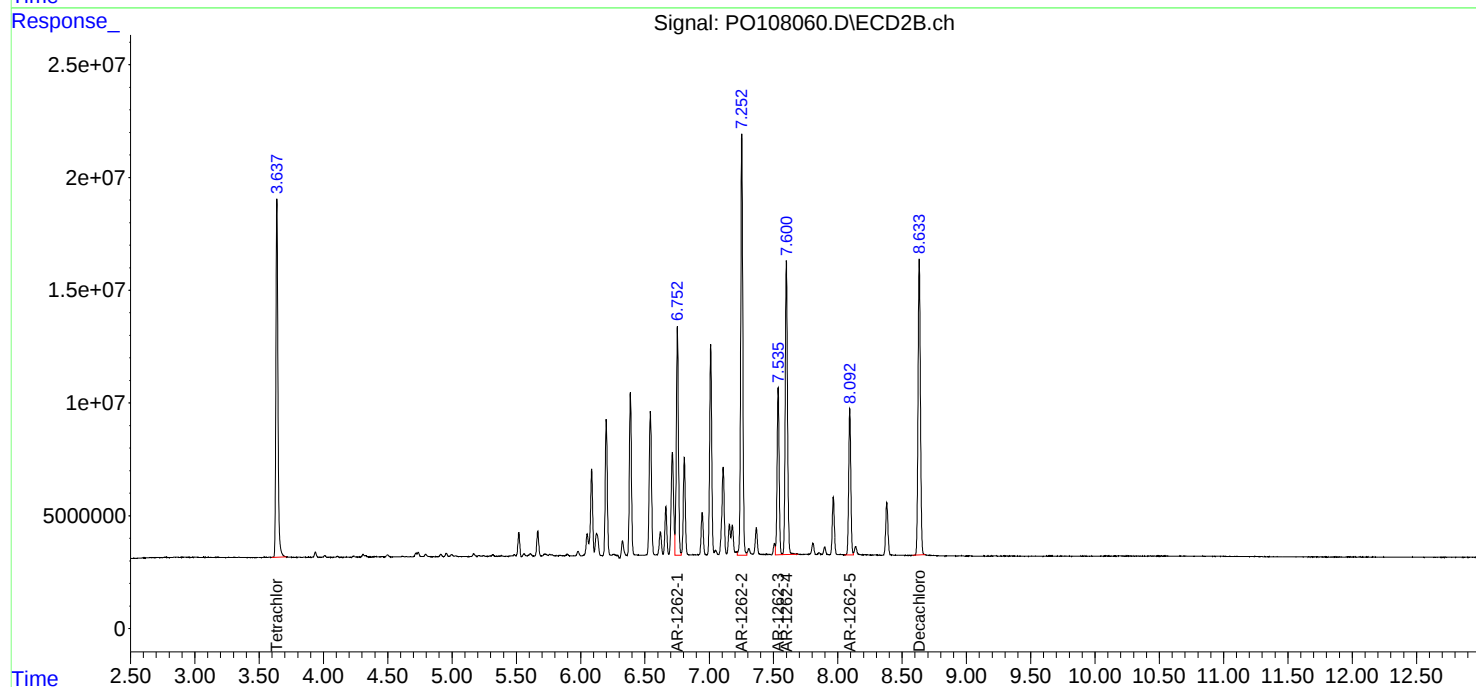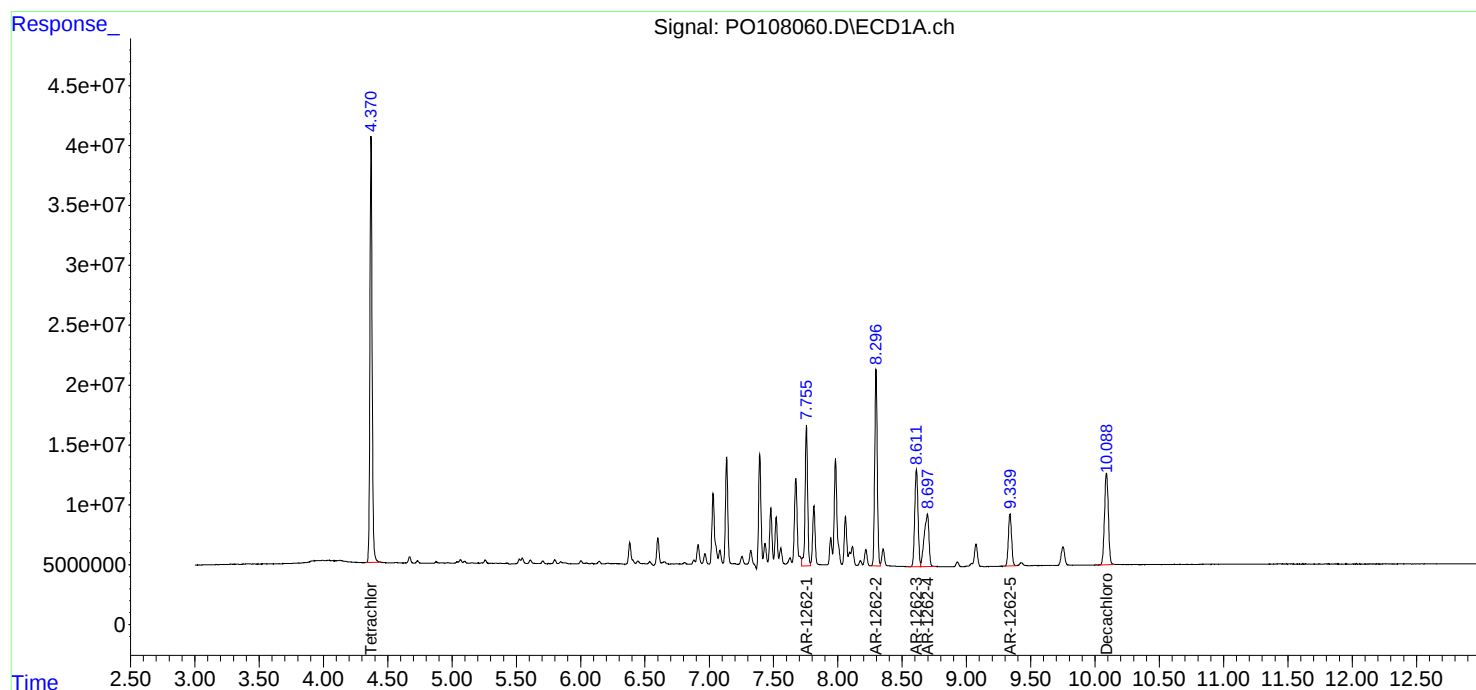

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 21:45
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:49:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:47:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.638	860.4E6	350.4E6	97.323	99.811
2) SA Decachlor...	10.092	8.635	513.1E6	603.5E6	93.632	98.674
Target Compounds						
41) L9 AR-1268-1	8.611	7.537	470.8E6	503.8E6	944.056	993.749
42) L9 AR-1268-2	8.703	7.602	426.1E6	474.8E6	947.831	1000.434
43) L9 AR-1268-3	8.933	7.808	347.8E6	398.0E6	941.177	1002.429
44) L9 AR-1268-4	9.343	8.094	159.4E6	165.0E6	938.281	984.194
45) L9 AR-1268-5	9.755	8.383	1064.2E6	1353.3E6	961.116	1011.238



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 21:45
Operator : YP/AJ
Sample : AR1268ICC1000
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:49:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:47:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

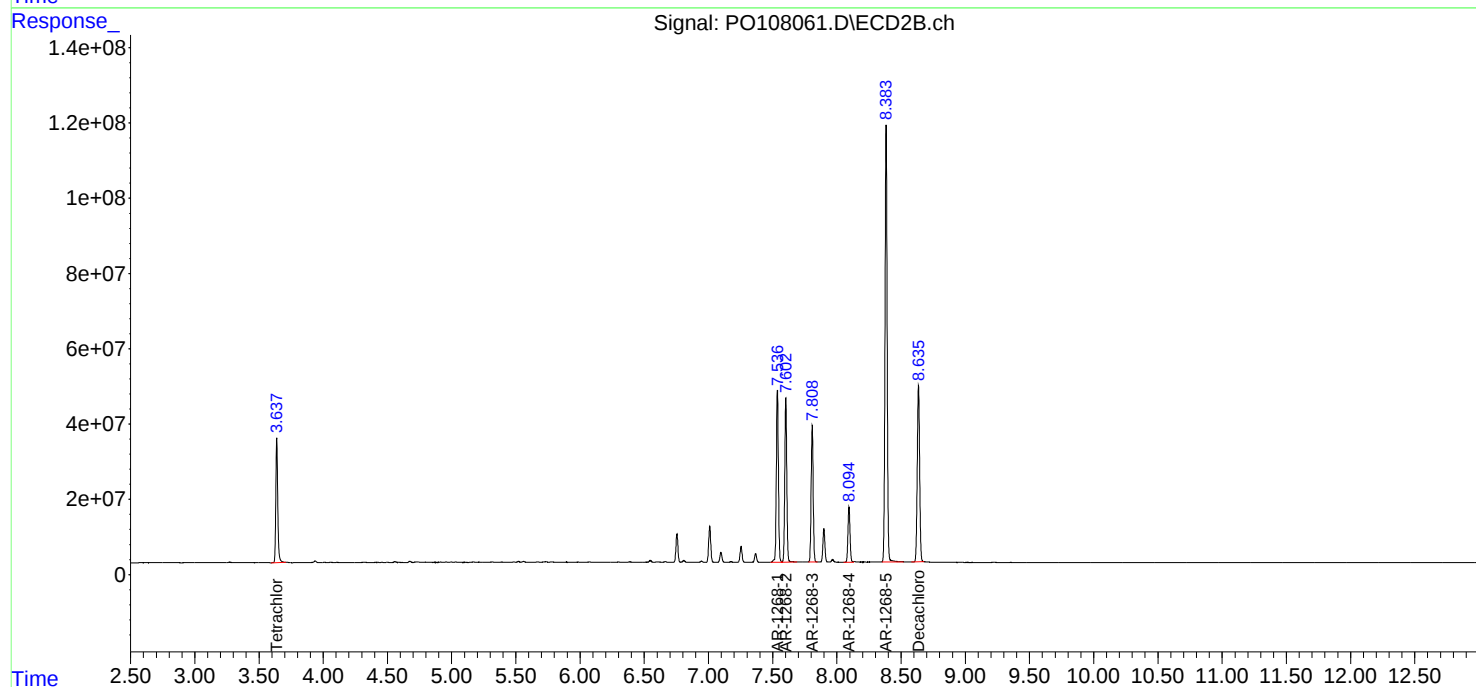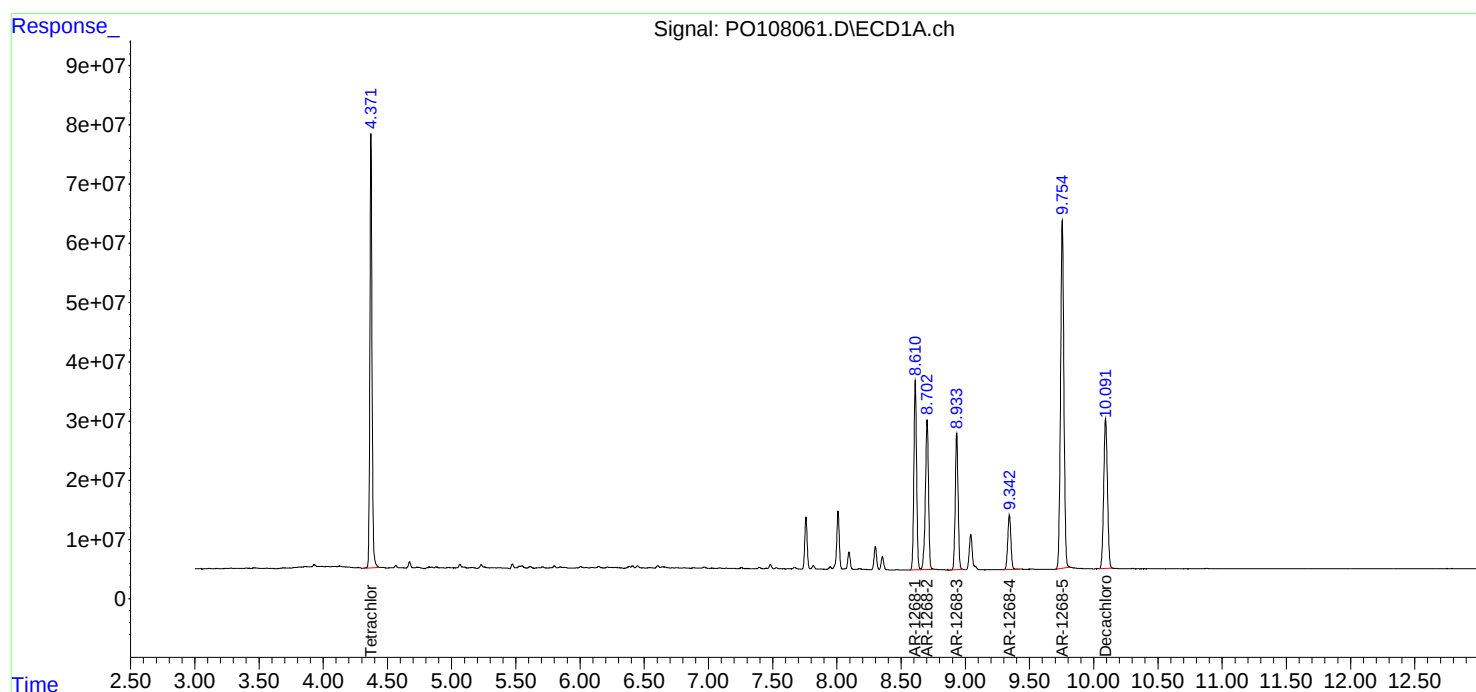

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 22:02
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC750

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:49:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:47:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.638	646.0E6	261.0E6	73.072	74.356
2) SA Decachlor...	10.093	8.635	392.7E6	454.3E6	71.657	74.283
Target Compounds						
41) L9 AR-1268-1	8.609	7.536	356.9E6	376.9E6	715.738m	743.472
42) L9 AR-1268-2	8.702	7.601	322.3E6	354.2E6	716.881	746.440
43) L9 AR-1268-3	8.933	7.807	263.1E6	296.3E6	711.839	746.168
44) L9 AR-1268-4	9.342	8.094	121.7E6	123.9E6	716.546	739.116
45) L9 AR-1268-5	9.755	8.383	804.3E6	1009.1E6	726.408	754.067

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 22:02
Operator : YP/AJ
Sample : AR1268ICC750
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:49:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:47:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

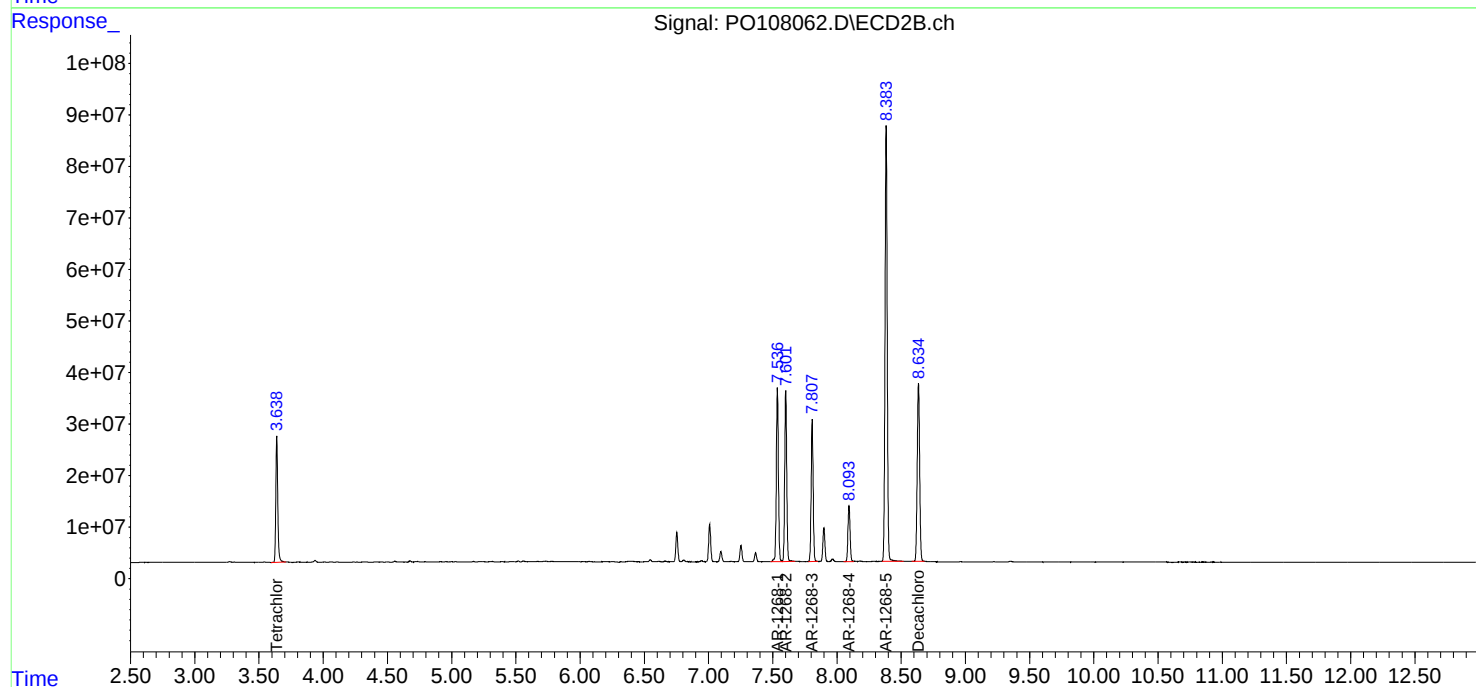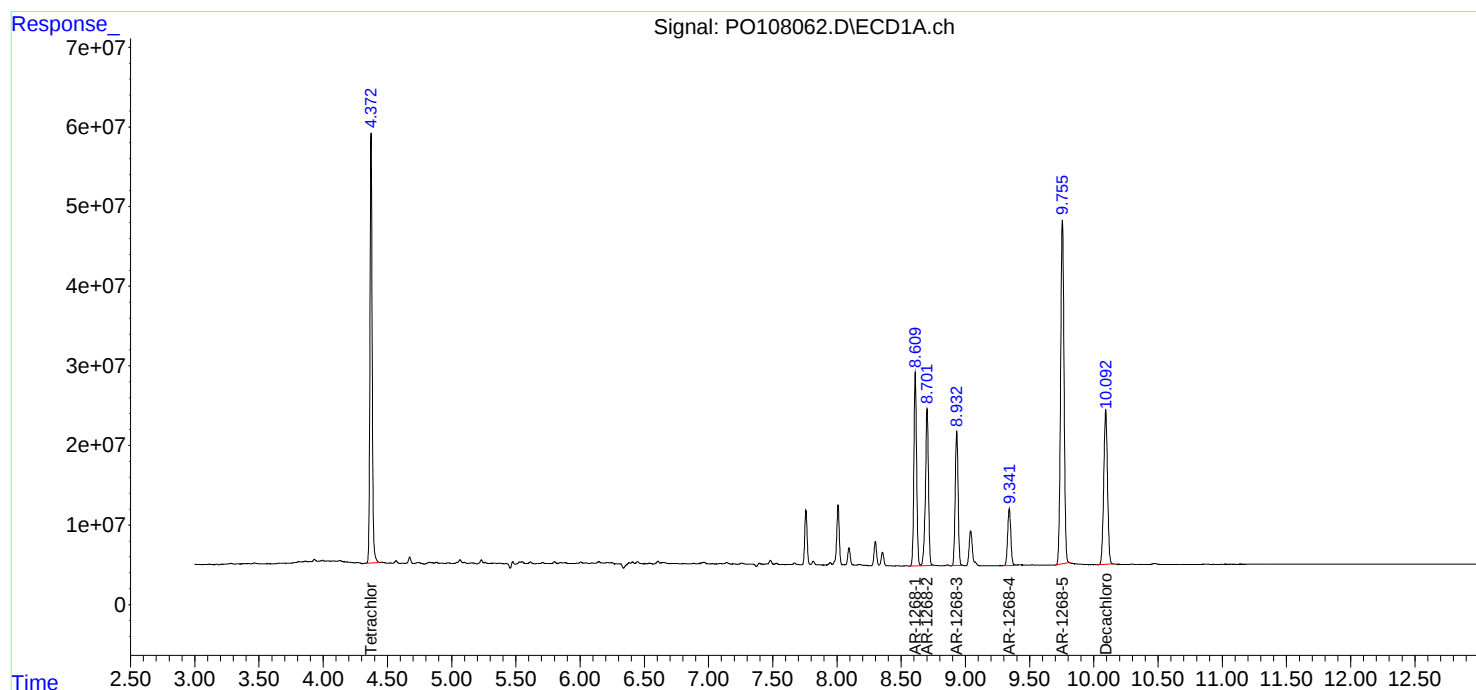

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 22:19
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:49:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:47:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.638	442.0E6	175.5E6	50.000	50.000
2) SA Decachlor...	10.090	8.633	274.0E6	305.8E6	50.000	50.000
Target Compounds						
41) L9 AR-1268-1	8.607	7.535	249.4E6	253.5E6	500.160m	500.000
42) L9 AR-1268-2	8.699	7.600	224.8E6	237.3E6	500.000	500.000
43) L9 AR-1268-3	8.930	7.806	184.8E6	198.5E6	500.000	500.000
44) L9 AR-1268-4	9.338	8.093	84940907	83838240	500.000	500.000
45) L9 AR-1268-5	9.751	8.381	553.6E6	669.1E6	500.000	500.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 22:19
Operator : YP/AJ
Sample : AR1268ICC500
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:49:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:47:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

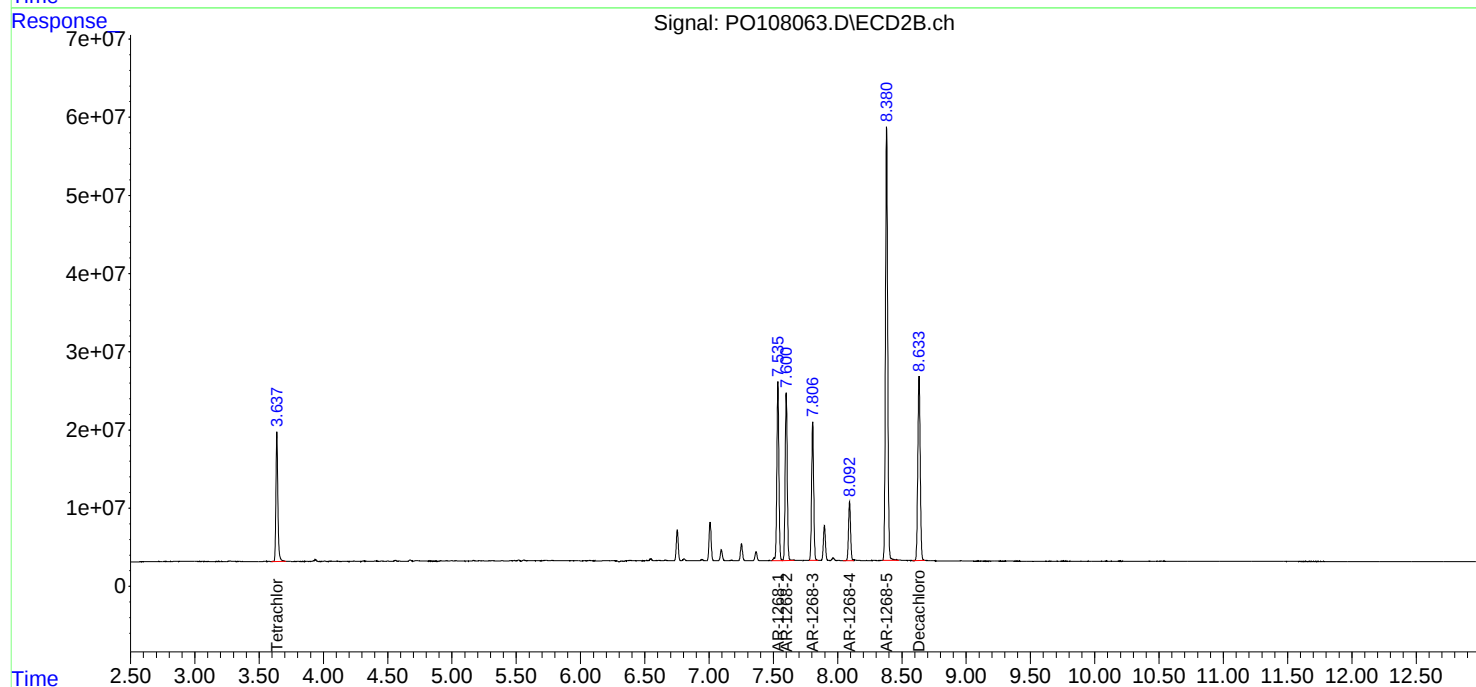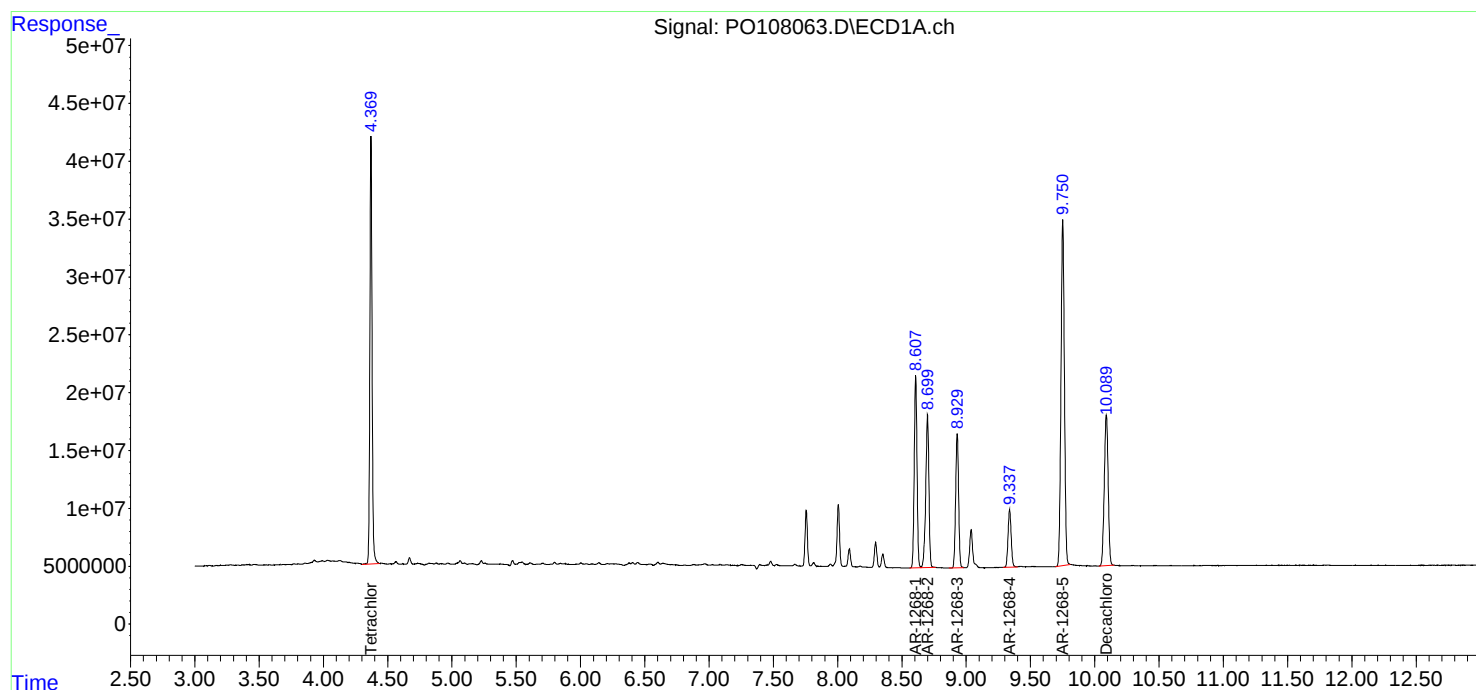

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 22:35
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:50:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:47:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.639	226.1E6	87728349	25.578	24.990
2) SA Decachlor...	10.091	8.634	145.0E6	155.4E6	26.468	25.415
Target Compounds						
41) L9 AR-1268-1	8.609	7.537	131.5E6	127.6E6	263.700	251.740
42) L9 AR-1268-2	8.701	7.601	118.7E6	119.0E6	263.990	250.759
43) L9 AR-1268-3	8.931	7.807	97170911	99405860	262.950	250.343
44) L9 AR-1268-4	9.341	8.094	44718395	42764313	263.232	255.041
45) L9 AR-1268-5	9.753	8.382	287.0E6	331.6E6	259.251	247.776



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 22:35
Operator : YP/AJ
Sample : AR1268ICC250
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:50:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:47:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

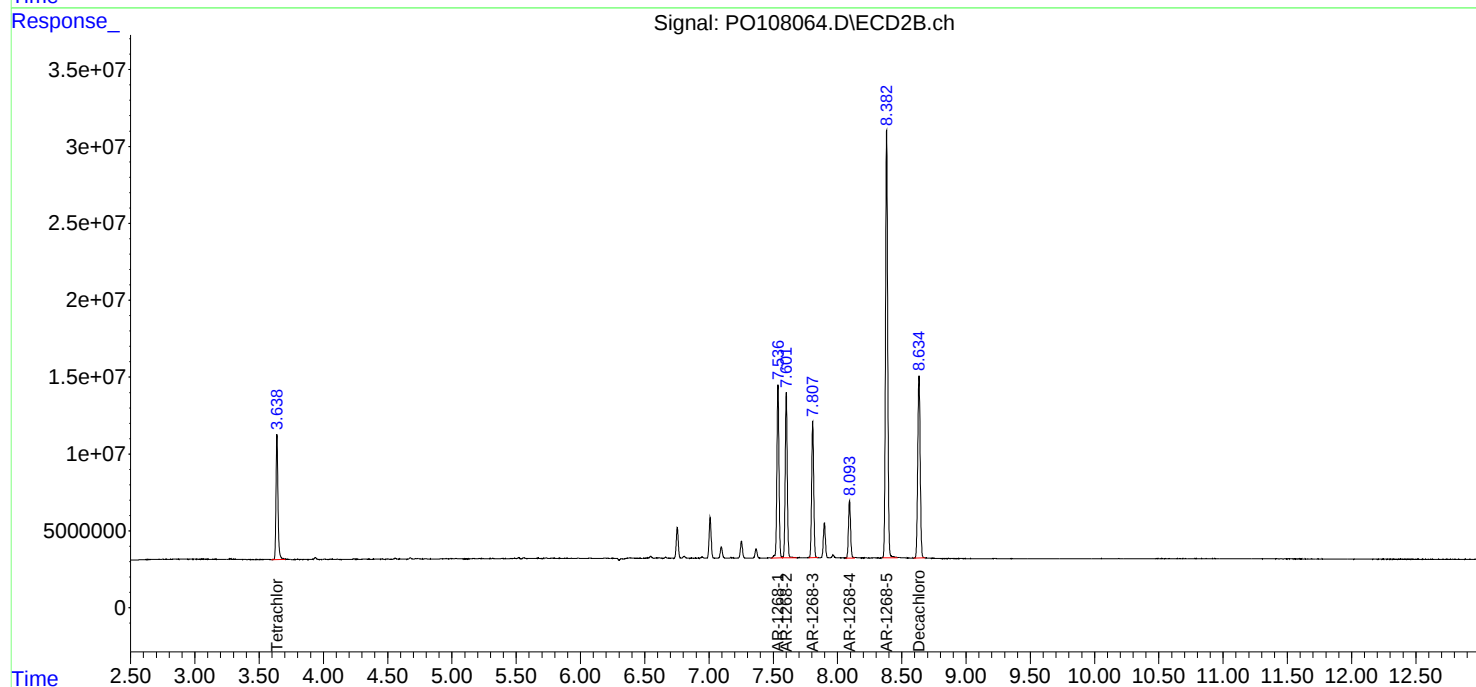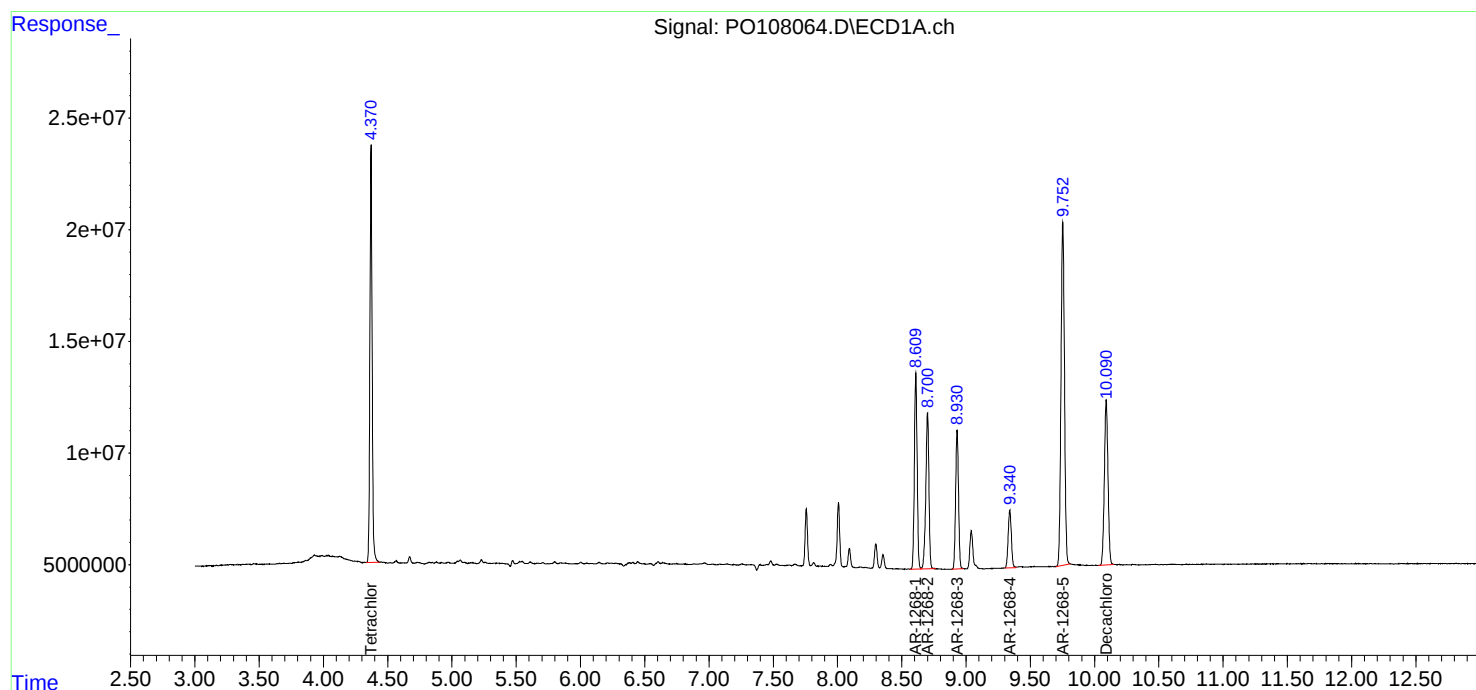

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
 Data File : PO108065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 22:51
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:50:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:47:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.638	41265649	14906651	4.668	4.246
2) SA Decachlor...	10.090	8.634	27874999	27587002	5.087	4.510
Target Compounds						
41) L9 AR-1268-1	8.608	7.536	25141699	22455830	50.415	44.295
42) L9 AR-1268-2	8.699	7.601	22215748	20385565	49.415	42.955
43) L9 AR-1268-3	8.930	7.807	18683921	16916516	50.560	42.603
44) L9 AR-1268-4	9.339	8.093	8425520	7850786	49.596	46.821
45) L9 AR-1268-5	9.752	8.382	55248947	56297415	49.899	42.067



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 22:51
Operator : YP/AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:50:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:47:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

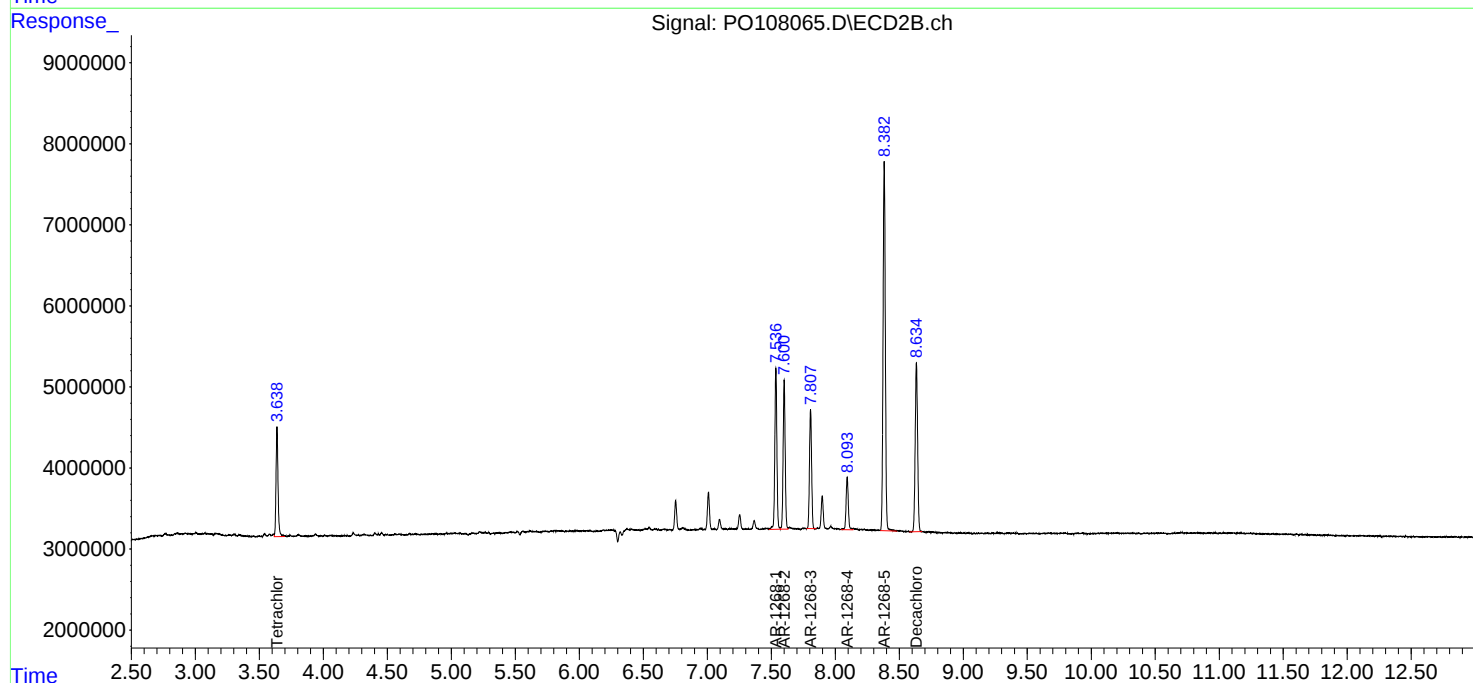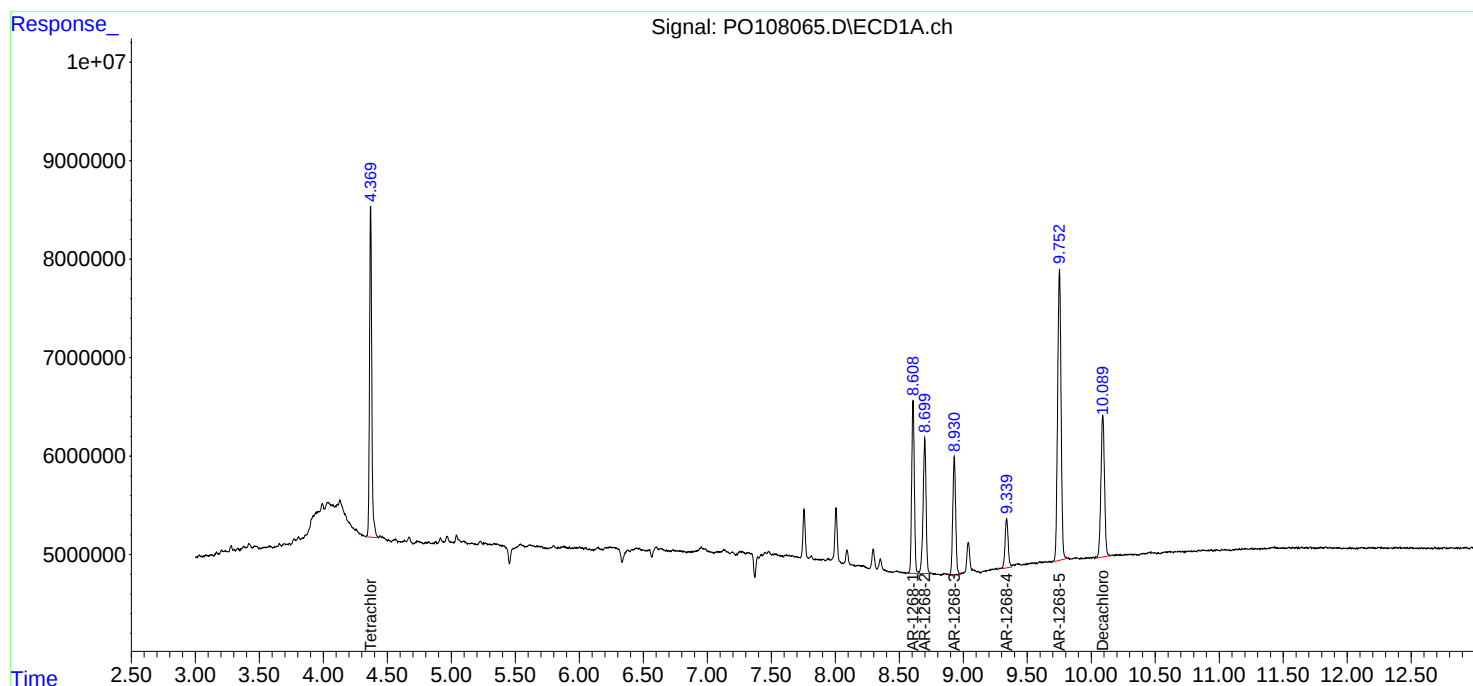

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
 Data File : PO108066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 23:08
 Operator : YP/AJ
 Sample : PO111824ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO111824

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 03:04:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:58:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.638	447.8E6	178.1E6	51.435	52.529
2) SA Decachlor...	10.092	8.635	163.9E6	176.7E6	53.672	51.946
Target Compounds						
3) L1 AR-1016-1	5.527	4.718	135.6E6	56021382	504.261	512.670
4) L1 AR-1016-2	5.550	4.738	194.8E6	80116114	502.442	523.969
5) L1 AR-1016-3	5.612	4.914	123.1E6	42882921	492.655	521.917
6) L1 AR-1016-4	5.709	4.955	98948499	33266198	506.728	522.456
7) L1 AR-1016-5	6.005	5.168	95502205	44630761	515.030	514.792
31) L7 AR-1260-1	7.138	6.200	150.4E6	83950237	547.888	518.401
32) L7 AR-1260-2	7.396	6.388	155.4E6	101.8E6	549.019	517.049
33) L7 AR-1260-3	7.759	6.541	119.2E6	95984927	554.811	515.702
34) L7 AR-1260-4	7.984	7.013	119.9E6	82943761	540.166	518.416
35) L7 AR-1260-5	8.300	7.254	207.4E6	204.3E6	543.596	520.314



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 23:08
Operator : YP/AJ
Sample : PO111824ICV500
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO111824

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 03:04:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:58:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

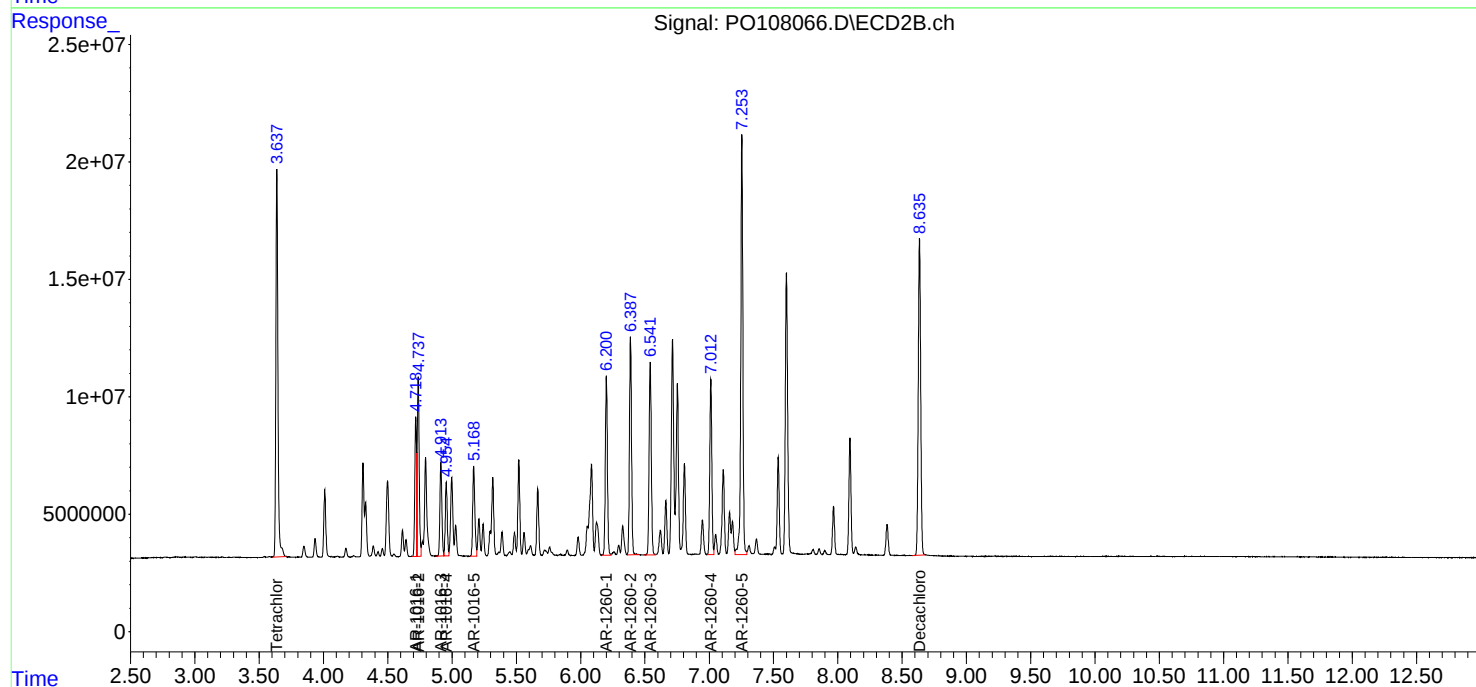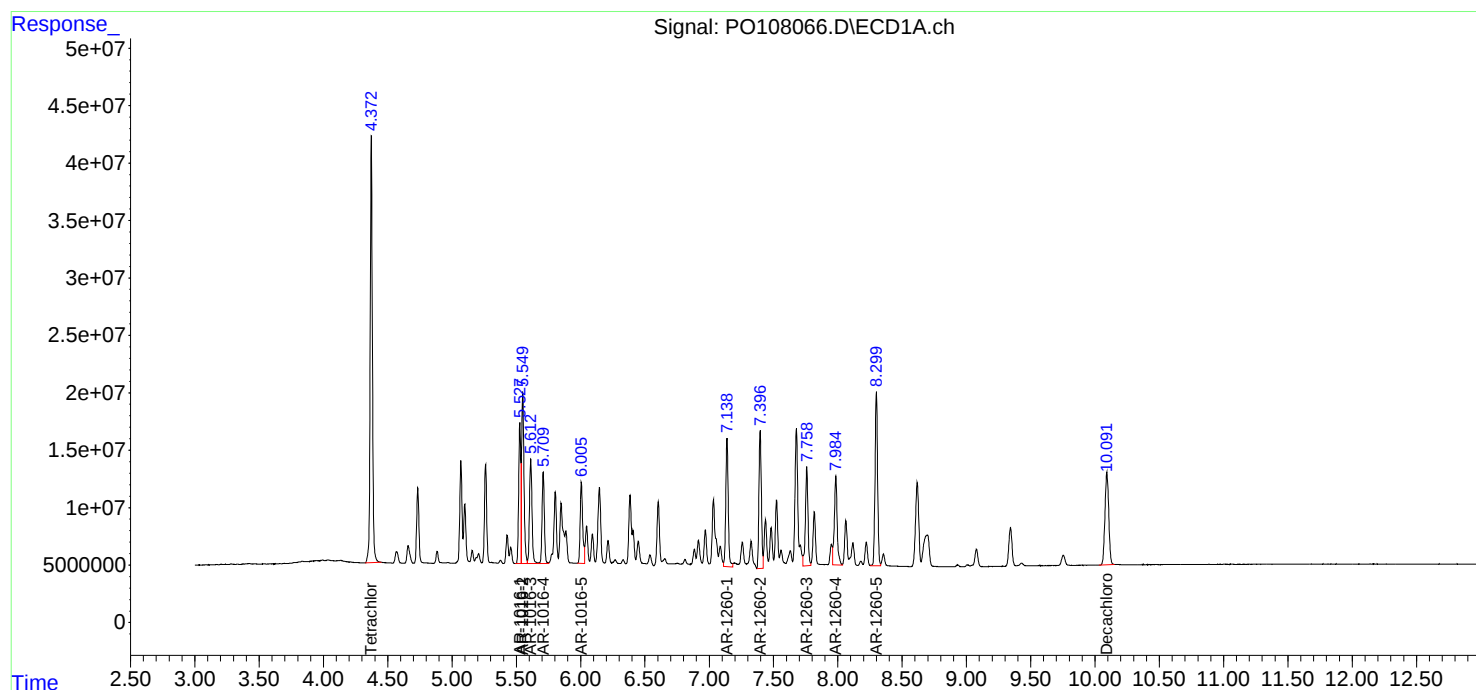

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 23:24
 Operator : YP/AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO111824AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:08:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 01:39:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.638	453.7E6	181.2E6	53.021	53.149
2) SA Decachlor...	10.089	8.634	165.3E6	179.2E6	52.890	51.893
Target Compounds						
16) L4 AR-1242-1	5.525	4.719	113.7E6	47198505	513.844	533.352
17) L4 AR-1242-2	5.547	4.738	164.5E6	66481511	523.001	537.807
18) L4 AR-1242-3	5.610	4.914	103.4E6	35794168	510.930	540.015
19) L4 AR-1242-4	5.707	4.998	82990275	34064861	531.607	544.352
20) L4 AR-1242-5	6.446	5.519	86129155	43591602	535.482	521.551



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 23:24
Operator : YP/AJ
Sample : AR1242ICV500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO111824AR1242

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:08:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 01:39:33 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

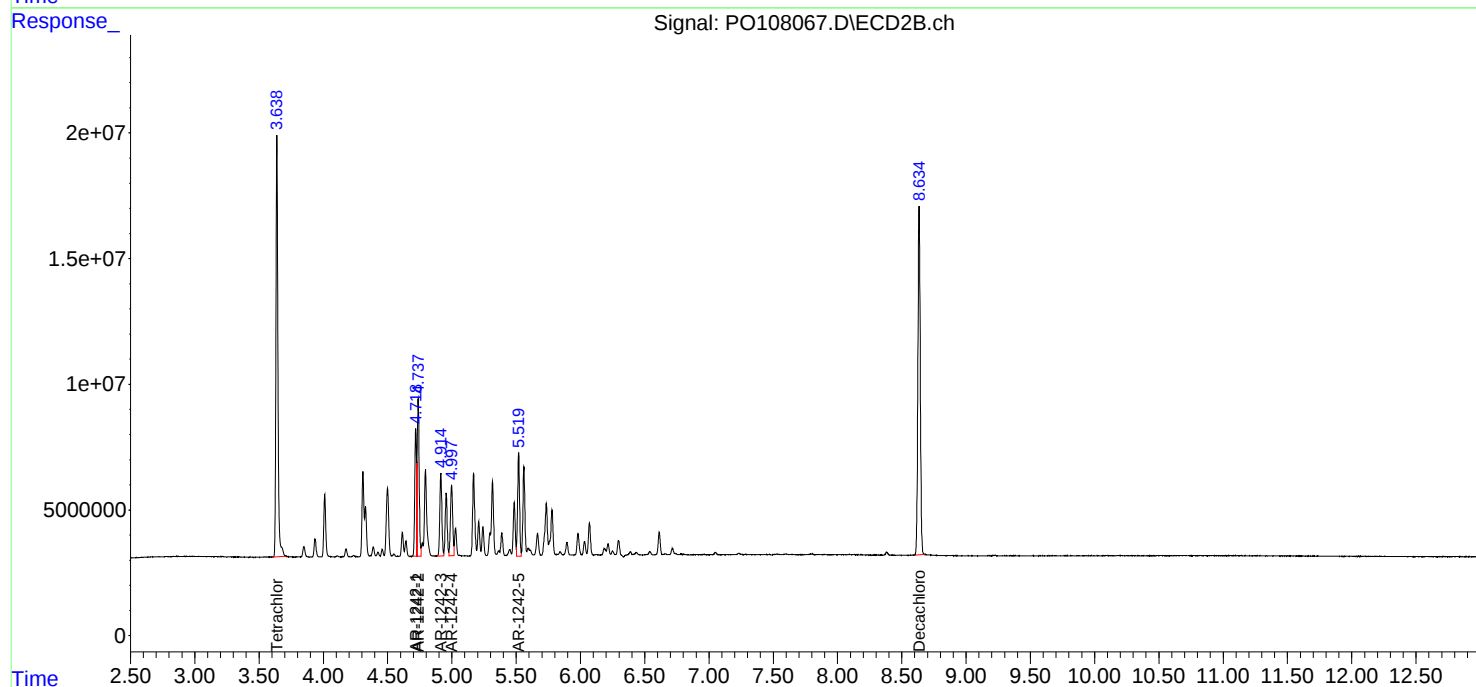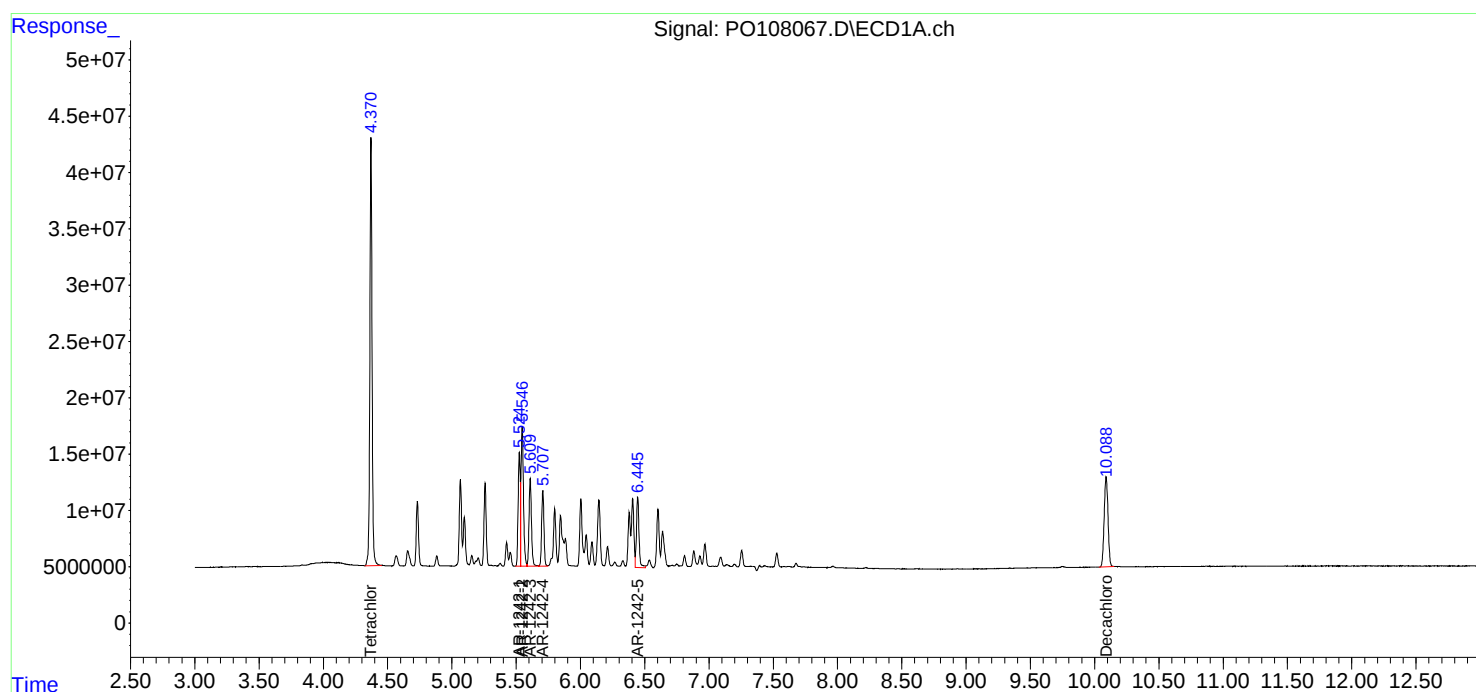

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108068.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 23:41
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO111824AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:12:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:10:25 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.638	460.4E6	183.2E6	51.315	51.130
2) SA Decachlor...	10.093	8.635	172.0E6	184.7E6	51.734	51.072
Target Compounds						
21) L5 AR-1248-1	5.526	4.719	88187110	35657204	510.746	509.402
22) L5 AR-1248-2	5.802	4.956	125.6E6	48485121	514.569	511.918
23) L5 AR-1248-3	6.005	4.998	133.0E6	51234070	520.043	511.748
24) L5 AR-1248-4	6.408	5.169	142.9E6	61969582	516.011	512.476
25) L5 AR-1248-5	6.446	5.561	144.4E6	63236571	520.860	510.426



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108068.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 23:41
Operator : YP/AJ
Sample : AR1248ICV500
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO111824AR1248

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:12:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:10:25 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

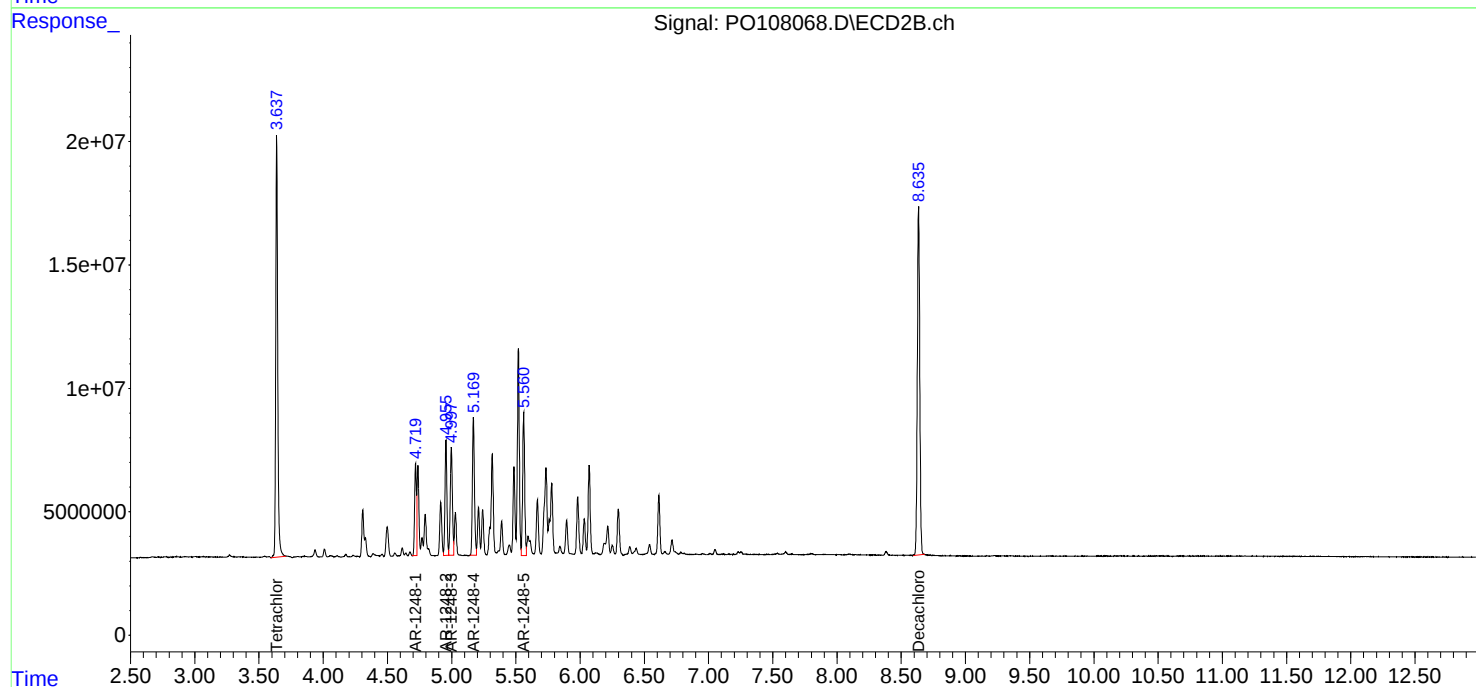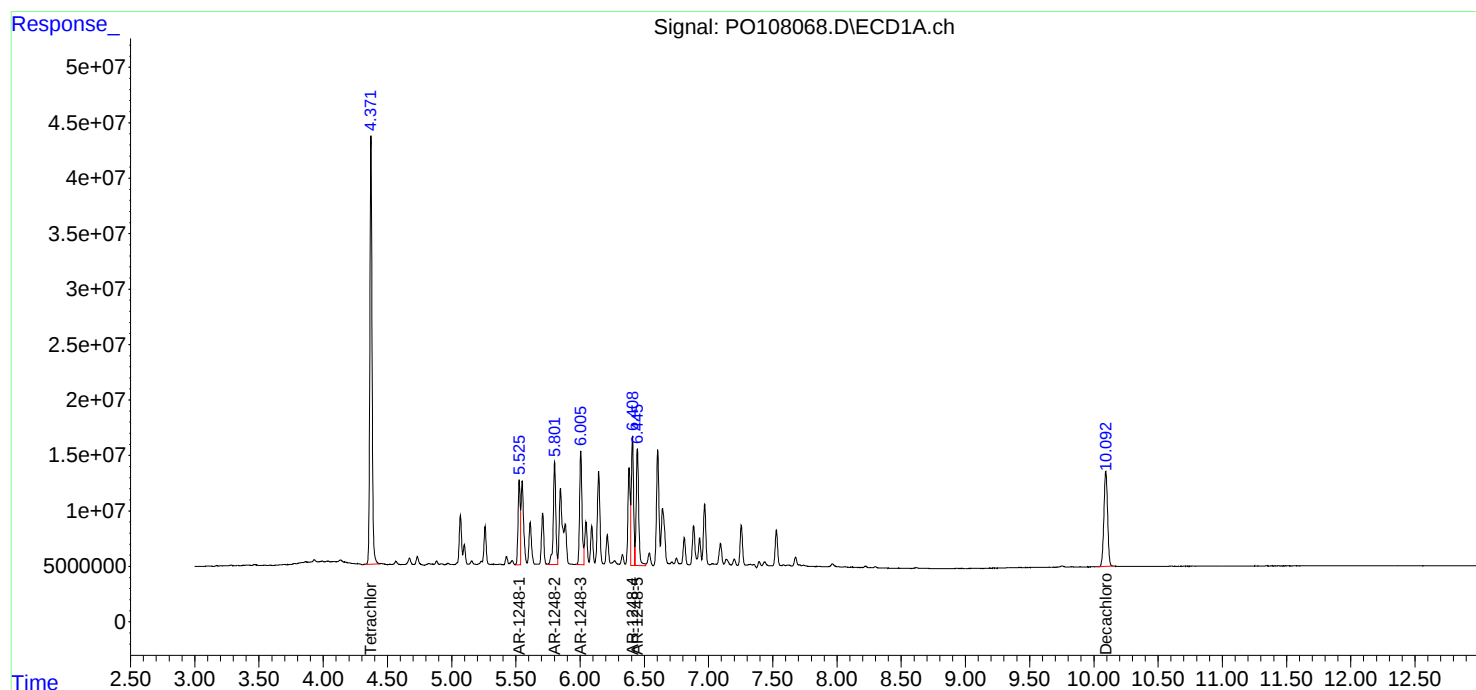

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108069.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 23:58
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO111824AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:29:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:27:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.638	454.2E6	181.4E6	50.289	49.875
2) SA Decachlor...	10.093	8.634	171.6E6	181.9E6	50.888	49.622
Target Compounds						
26) L6 AR-1254-1	6.385	5.520	138.9E6	88718453	507.323	490.447
27) L6 AR-1254-2	6.605	5.667	203.5E6	78333103	506.802	496.810
28) L6 AR-1254-3	6.971	6.071	198.2E6	130.7E6	500.900	492.256
29) L6 AR-1254-4	7.257	6.298	138.7E6	69782489	495.535	460.160
30) L6 AR-1254-5	7.678	6.716	137.8E6	115.0E6	503.106	489.288



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108069.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 23:58
Operator : YP/AJ
Sample : AR1254ICV500
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO111824AR1254

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:29:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:27:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

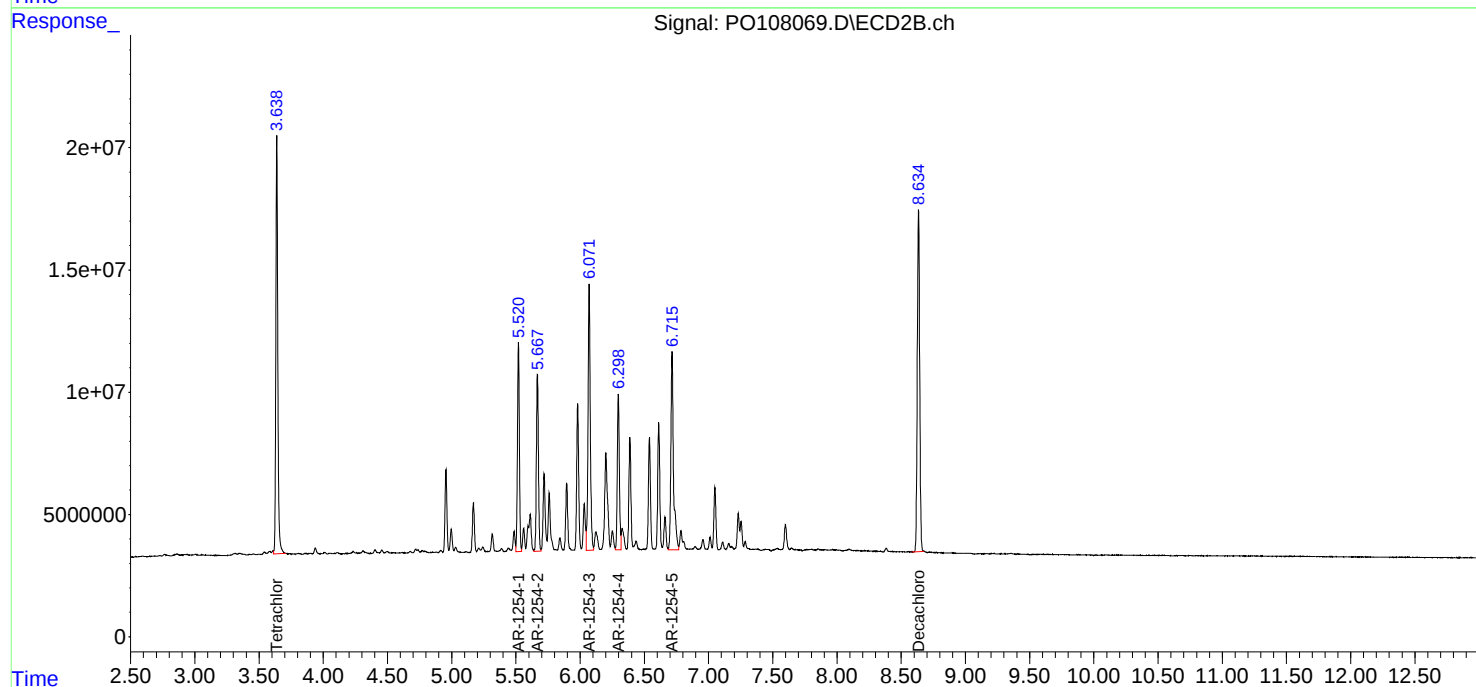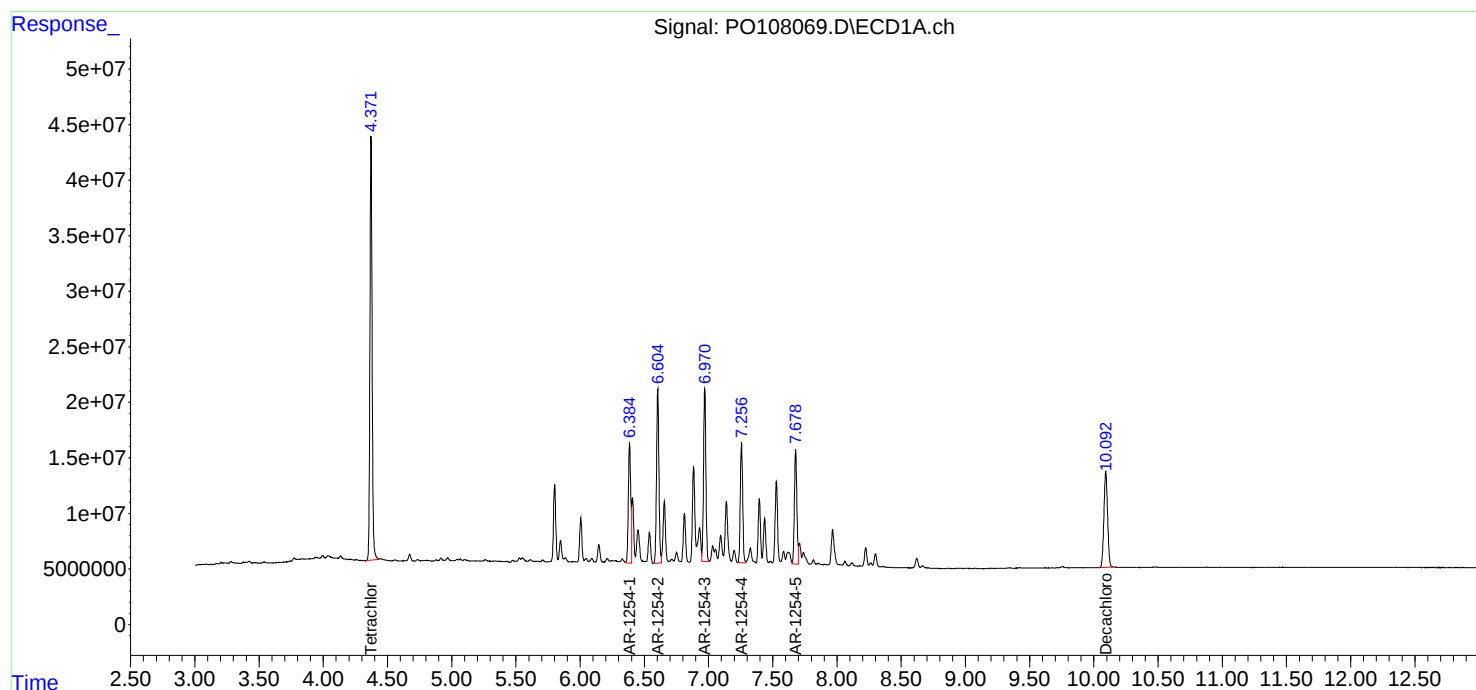

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111824\
 Data File : P0108070.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2024 00:14
 Operator : YP/AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO111824AR1268

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 03:00:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 02:47:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.638	455.1E6	180.1E6	52.485	53.017
2) SA Decachlor...	10.091	8.634	280.7E6	310.0E6	51.562	51.760
Target Compounds						
41) L9 AR-1268-1	8.608	7.536	257.3E6	256.8E6	519.955m	519.212
42) L9 AR-1268-2	8.701	7.601	232.3E6	240.8E6	522.064	522.172
43) L9 AR-1268-3	8.930	7.807	189.1E6	201.1E6	516.673	521.984
44) L9 AR-1268-4	9.341	8.093	86718741	84948088	516.819	514.202
45) L9 AR-1268-5	9.752	8.383	568.1E6	679.2E6	516.704	523.301

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 00:14
Operator : YP/AJ
Sample : AR1268ICV500
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ICVPO111824AR1268

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 03:00:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 02:47:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

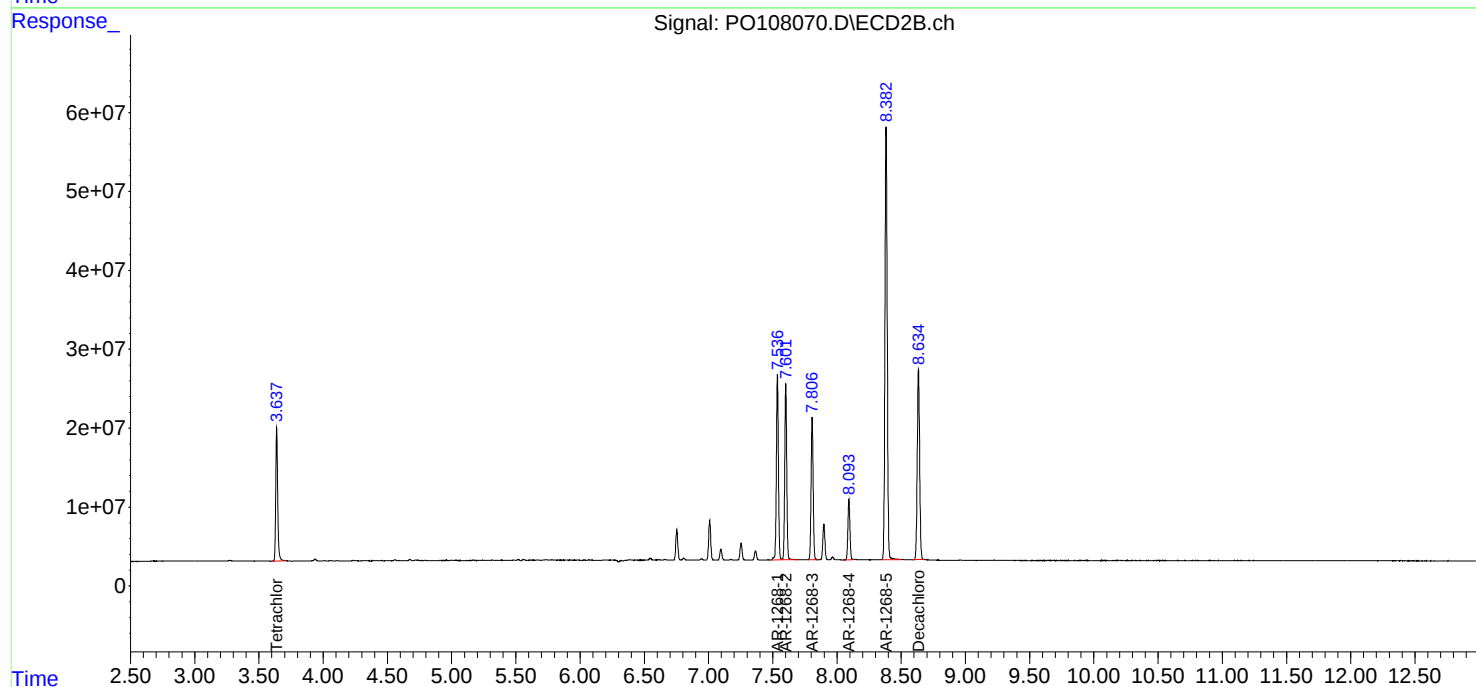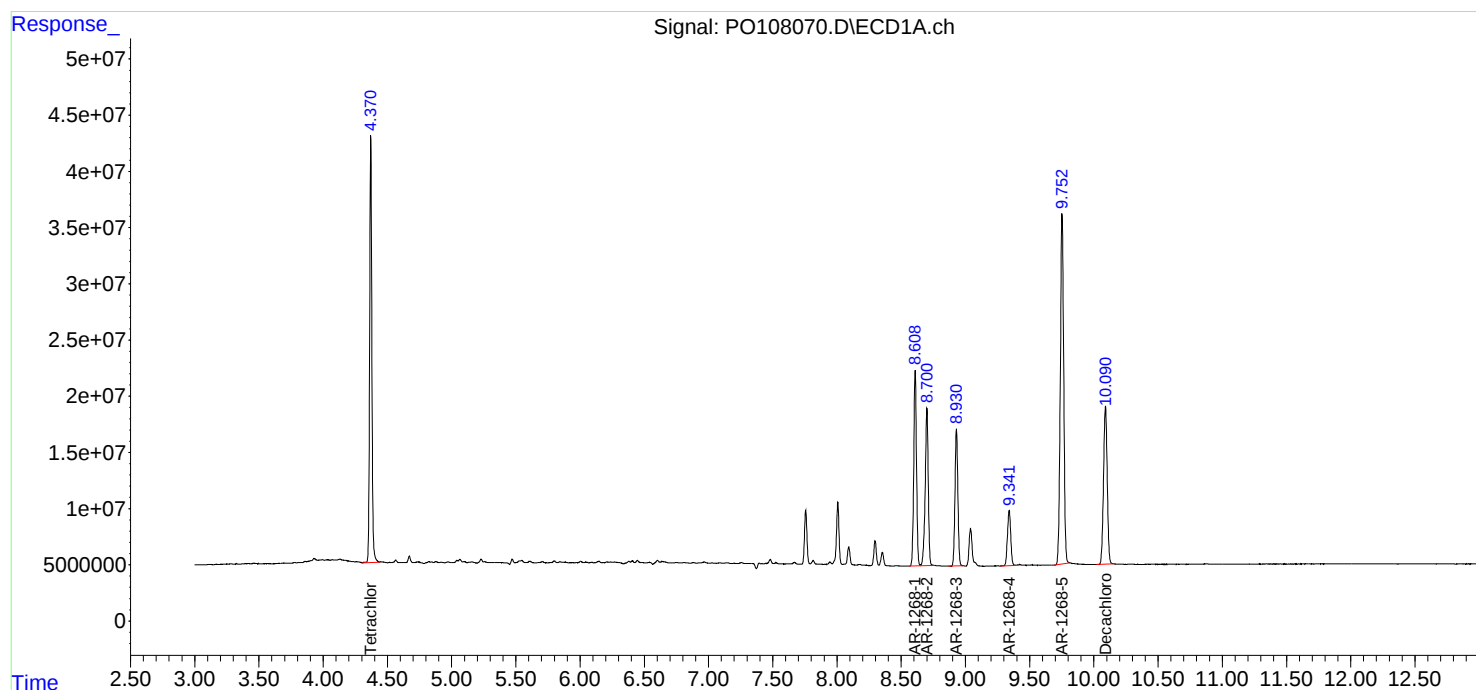



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

Continuing Calib Date: 12/02/2024 Initial Calibration Date(s): 11/18/2024 11/18/2024

Continuing Calib Time: 10:02 Initial Calibration Time(s): 15:32 22:51

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Aroclor-1016-1	(1)	5.53	5.53	5.43	5.63	0.00
Aroclor-1016-2	(2)	5.55	5.55	5.45	5.65	0.00
Aroclor-1016-3	(3)	5.62	5.61	5.51	5.71	0.00
Aroclor-1016-4	(4)	5.71	5.71	5.61	5.81	0.00
Aroclor-1016-5	(5)	6.01	6.00	5.90	6.10	-0.01
Aroclor-1260-1	(1)	7.14	7.14	7.04	7.24	0.00
Aroclor-1260-2	(2)	7.40	7.40	7.30	7.50	0.00
Aroclor-1260-3	(3)	7.76	7.76	7.66	7.86	0.00
Aroclor-1260-4	(4)	7.99	7.98	7.88	8.08	-0.01
Aroclor-1260-5	(5)	8.30	8.30	8.20	8.40	0.00
Tetrachloro-m-xylene		4.37	4.37	4.27	4.47	0.00
Decachlorobiphenyl		10.10	10.09	9.99	10.19	-0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

Continuing Calib Date: 12/02/2024 Initial Calibration Date(s): 11/18/2024 11/18/2024

Continuing Calib Time: 10:02 Initial Calibration Time(s): 15:32 22:51

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.72	4.72	4.62	4.82	0.00
Aroclor-1016-2	(2)	4.74	4.74	4.64	4.84	0.00
Aroclor-1016-3	(3)	4.91	4.92	4.82	5.02	0.01
Aroclor-1016-4	(4)	4.96	4.96	4.86	5.06	0.00
Aroclor-1016-5	(5)	5.17	5.17	5.07	5.27	0.00
Aroclor-1260-1	(1)	6.20	6.20	6.10	6.30	0.00
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.54	6.54	6.44	6.64	0.00
Aroclor-1260-4	(4)	7.01	7.01	6.91	7.11	0.00
Aroclor-1260-5	(5)	7.25	7.25	7.15	7.35	0.00
Tetrachloro-m-xylene		3.64	3.64	3.54	3.74	0.00
Decachlorobiphenyl		8.63	8.64	8.54	8.74	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 11/18/2024 11/18/2024

Client Sample No.: CCAL01 Date Analyzed: 12/02/2024

Lab Sample No.: AR1660CCC500 Data File : PO108275.D Time Analyzed: 10:02

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	5.530	5.425	5.625	496.620	500.000	-0.7
Aroclor-1016-2	5.552	5.447	5.647	500.300	500.000	0.1
Aroclor-1016-3	5.615	5.510	5.710	493.010	500.000	-1.4
Aroclor-1016-4	5.712	5.607	5.807	504.490	500.000	0.9
Aroclor-1016-5	6.008	5.904	6.104	496.090	500.000	-0.8
Aroclor-1260-1	7.143	7.037	7.237	451.790	500.000	-9.6
Aroclor-1260-2	7.400	7.295	7.495	512.580	500.000	2.5
Aroclor-1260-3	7.764	7.658	7.858	509.460	500.000	1.9
Aroclor-1260-4	7.988	7.884	8.084	542.430	500.000	8.5
Aroclor-1260-5	8.304	8.198	8.398	544.180	500.000	8.8
Decachlorobiphenyl	10.100	9.991	10.191	52.240	50.000	4.5
Tetrachloro-m-xylene	4.374	4.270	4.470	52.880	50.000	5.8



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 11/18/2024 11/18/2024

Client Sample No.: CCAL01 Date Analyzed: 12/02/2024

Lab Sample No.: AR1660CCC500 Data File : PO108275.D Time Analyzed: 10:02

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.720	4.620	4.820	546.000	500.000	9.2
Aroclor-1016-2	4.738	4.639	4.839	552.240	500.000	10.4
Aroclor-1016-3	4.914	4.815	5.015	556.490	500.000	11.3
Aroclor-1016-4	4.956	4.856	5.056	559.120	500.000	11.8
Aroclor-1016-5	5.169	5.070	5.270	546.670	500.000	9.3
Aroclor-1260-1	6.200	6.100	6.300	529.460	500.000	5.9
Aroclor-1260-2	6.388	6.288	6.488	526.080	500.000	5.2
Aroclor-1260-3	6.541	6.441	6.641	527.020	500.000	5.4
Aroclor-1260-4	7.012	6.912	7.112	520.110	500.000	4.0
Aroclor-1260-5	7.253	7.154	7.354	510.030	500.000	2.0
Decachlorobiphenyl	8.634	8.535	8.735	44.990	50.000	-10.0
Tetrachloro-m-xylene	3.639	3.539	3.739	57.590	50.000	15.2

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
 Data File : PO108275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2024 10:02
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 00:31:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.374	3.639	460.4E6	195.3E6	52.880	57.595
2) SA Decachlor...	10.100	8.634	159.6E6	153.0E6	52.244	44.987
Target Compounds						
3) L1 AR-1016-1	5.530	4.720	133.6E6	59663466	496.623	546.000
4) L1 AR-1016-2	5.552	4.738	194.0E6	84439430	500.297	552.244
5) L1 AR-1016-3	5.615	4.914	123.2E6	45723588	493.013	556.490
6) L1 AR-1016-4	5.712	4.956	98511742	35600874	504.492	559.123
7) L1 AR-1016-5	6.008	5.169	91989232	47394377	496.085	546.668
31) L7 AR-1260-1	7.143	6.200	124.0E6	85740742	451.785	529.457
32) L7 AR-1260-2	7.400	6.388	145.1E6	103.6E6	512.583	526.080
33) L7 AR-1260-3	7.764	6.541	109.4E6	98091445	509.457	527.019
34) L7 AR-1260-4	7.988	7.012	120.4E6	83215283	542.430	520.113
35) L7 AR-1260-5	8.304	7.253	207.6E6	200.3E6	544.184	510.034



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
Data File : PO108275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2024 10:02
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 00:31:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

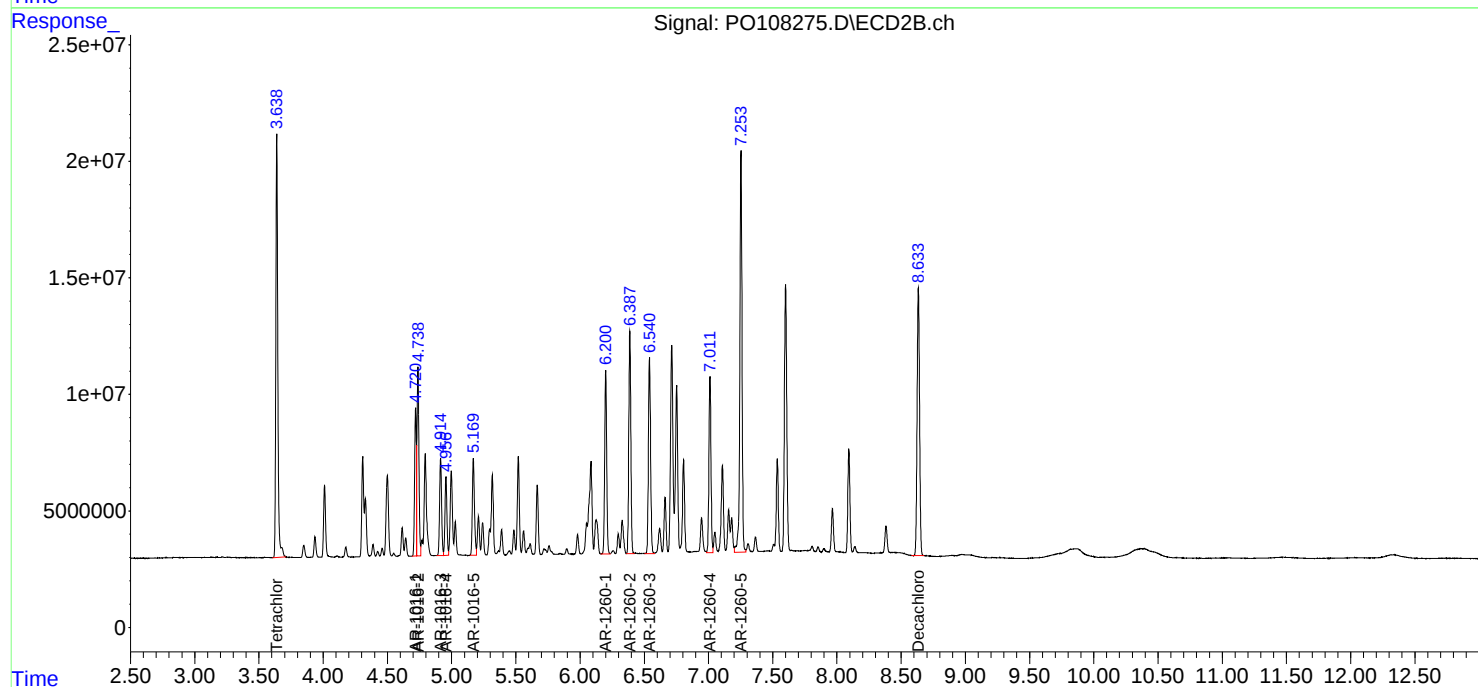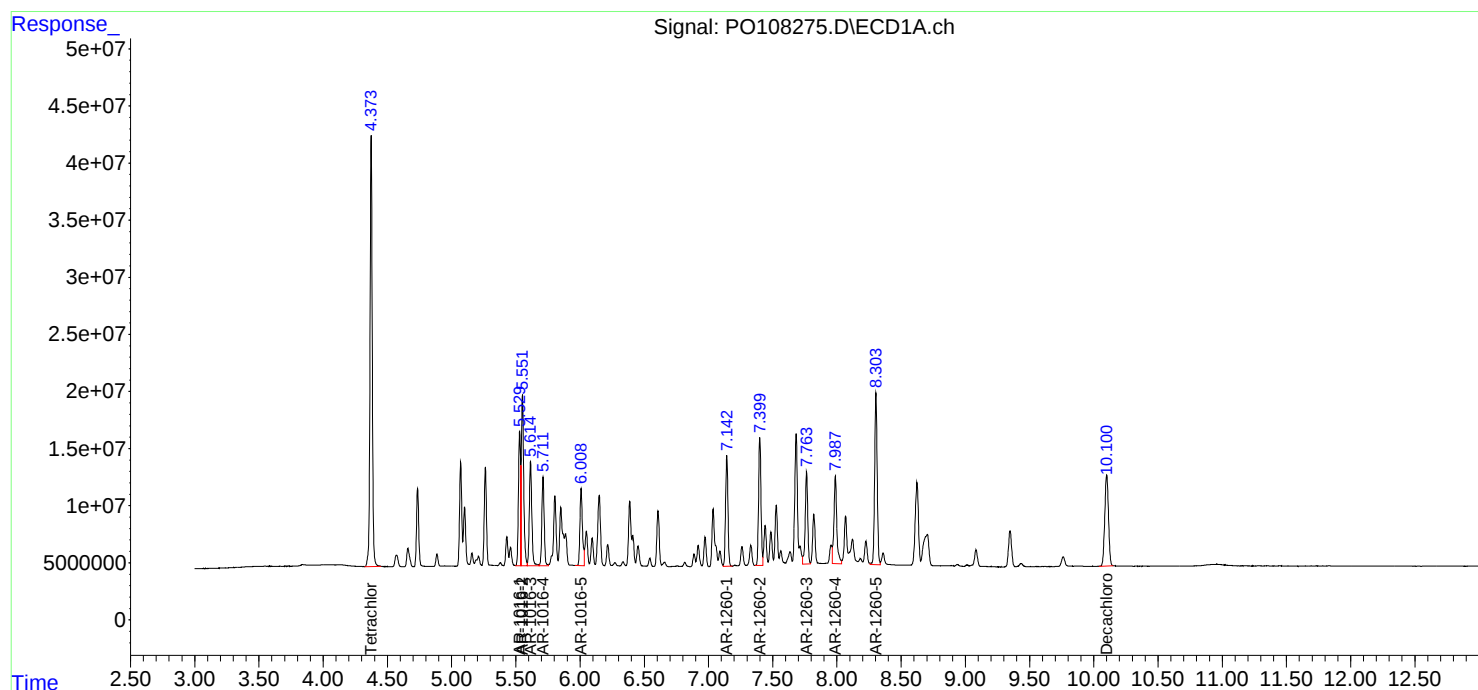



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

Continuing Calib Date: 12/02/2024 Initial Calibration Date(s): 11/18/2024 11/18/2024

Continuing Calib Time: 15:36 Initial Calibration Time(s): 15:32 22:51

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Aroclor-1016-1	(1)	5.53	5.53	5.43	5.63	0.00
Aroclor-1016-2	(2)	5.55	5.55	5.45	5.65	0.00
Aroclor-1016-3	(3)	5.61	5.61	5.51	5.71	0.00
Aroclor-1016-4	(4)	5.71	5.71	5.61	5.81	0.00
Aroclor-1016-5	(5)	6.00	6.00	5.90	6.10	0.00
Aroclor-1260-1	(1)	7.14	7.14	7.04	7.24	0.00
Aroclor-1260-2	(2)	7.40	7.40	7.30	7.50	0.01
Aroclor-1260-3	(3)	7.76	7.76	7.66	7.86	0.00
Aroclor-1260-4	(4)	7.98	7.98	7.88	8.08	0.00
Aroclor-1260-5	(5)	8.30	8.30	8.20	8.40	0.00
Tetrachloro-m-xylene		4.37	4.37	4.27	4.47	0.00
Decachlorobiphenyl		10.09	10.09	9.99	10.19	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

Continuing Calib Date: 12/02/2024 Initial Calibration Date(s): 11/18/2024 11/18/2024

Continuing Calib Time: 15:36 Initial Calibration Time(s): 15:32 22:51

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Aroclor-1016-1	(1)	4.72	4.72	4.62	4.82	0.00
Aroclor-1016-2	(2)	4.74	4.74	4.64	4.84	0.00
Aroclor-1016-3	(3)	4.91	4.92	4.82	5.02	0.01
Aroclor-1016-4	(4)	4.95	4.96	4.86	5.06	0.01
Aroclor-1016-5	(5)	5.17	5.17	5.07	5.27	0.00
Aroclor-1260-1	(1)	6.20	6.20	6.10	6.30	0.00
Aroclor-1260-2	(2)	6.39	6.39	6.29	6.49	0.00
Aroclor-1260-3	(3)	6.54	6.54	6.44	6.64	0.00
Aroclor-1260-4	(4)	7.01	7.01	6.91	7.11	0.00
Aroclor-1260-5	(5)	7.25	7.25	7.15	7.35	0.00
Tetrachloro-m-xylene		3.64	3.64	3.54	3.74	0.00
Decachlorobiphenyl		8.63	8.64	8.54	8.74	0.01



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 11/18/2024 11/18/2024

Client Sample No.: CCAL02 Date Analyzed: 12/02/2024

Lab Sample No.: AR1660CCC500 Data File : PO108290.D Time Analyzed: 15:36

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	5.525	5.425	5.625	487.990	500.000	-2.4
Aroclor-1016-2	5.548	5.447	5.647	481.260	500.000	-3.7
Aroclor-1016-3	5.610	5.510	5.710	473.120	500.000	-5.4
Aroclor-1016-4	5.707	5.607	5.807	480.870	500.000	-3.8
Aroclor-1016-5	6.003	5.904	6.104	473.480	500.000	-5.3
Aroclor-1260-1	7.138	7.037	7.237	468.790	500.000	-6.2
Aroclor-1260-2	7.395	7.295	7.495	494.770	500.000	-1.0
Aroclor-1260-3	7.758	7.658	7.858	467.760	500.000	-6.4
Aroclor-1260-4	7.983	7.884	8.084	478.740	500.000	-4.3
Aroclor-1260-5	8.299	8.198	8.398	492.810	500.000	-1.4
Decachlorobiphenyl	10.091	9.991	10.191	49.340	50.000	-1.3
Tetrachloro-m-xylene	4.370	4.270	4.470	50.680	50.000	1.4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 11/18/2024 11/18/2024

Client Sample No.: CCAL02 Date Analyzed: 12/02/2024

Lab Sample No.: AR1660CCC500 Data File : PO108290.D Time Analyzed: 15:36

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.717	4.620	4.820	545.260	500.000	9.1
Aroclor-1016-2	4.736	4.639	4.839	551.390	500.000	10.3
Aroclor-1016-3	4.912	4.815	5.015	552.780	500.000	10.6
Aroclor-1016-4	4.953	4.856	5.056	549.950	500.000	10.0
Aroclor-1016-5	5.167	5.070	5.270	547.430	500.000	9.5
Aroclor-1260-1	6.198	6.100	6.300	522.810	500.000	4.6
Aroclor-1260-2	6.385	6.288	6.488	515.130	500.000	3.0
Aroclor-1260-3	6.538	6.441	6.641	511.790	500.000	2.4
Aroclor-1260-4	7.009	6.912	7.112	492.000	500.000	-1.6
Aroclor-1260-5	7.250	7.154	7.354	475.990	500.000	-4.8
Decachlorobiphenyl	8.630	8.535	8.735	41.760	50.000	-16.5
Tetrachloro-m-xylene	3.637	3.539	3.739	57.370	50.000	14.7

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
 Data File : PO108290.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2024 15:36
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 00:36:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.637	441.2E6	194.5E6	50.682	57.374
2) SA Decachlor...	10.091	8.630	150.7E6	142.0E6	49.345	41.756
Target Compounds						
3) L1 AR-1016-1	5.525	4.717	131.2E6	59582391	487.992	545.258
4) L1 AR-1016-2	5.548	4.736	186.6E6	84309159	481.262	551.392
5) L1 AR-1016-3	5.610	4.912	118.2E6	45418646	473.125	552.779
6) L1 AR-1016-4	5.707	4.953	93899361	35016932	480.871	549.952
7) L1 AR-1016-5	6.003	5.167	87798114	47460202	473.483	547.428
31) L7 AR-1260-1	7.138	6.198	128.7E6	84663591	468.790	522.806
32) L7 AR-1260-2	7.395	6.385	140.0E6	101.4E6	494.768	515.128
33) L7 AR-1260-3	7.758	6.538	100.5E6	95257610	467.759	511.794
34) L7 AR-1260-4	7.983	7.009	106.3E6	78717928	478.741	492.004
35) L7 AR-1260-5	8.299	7.250	188.0E6	186.9E6	492.813	475.989



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
Data File : PO108290.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2024 15:36
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 00:36:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

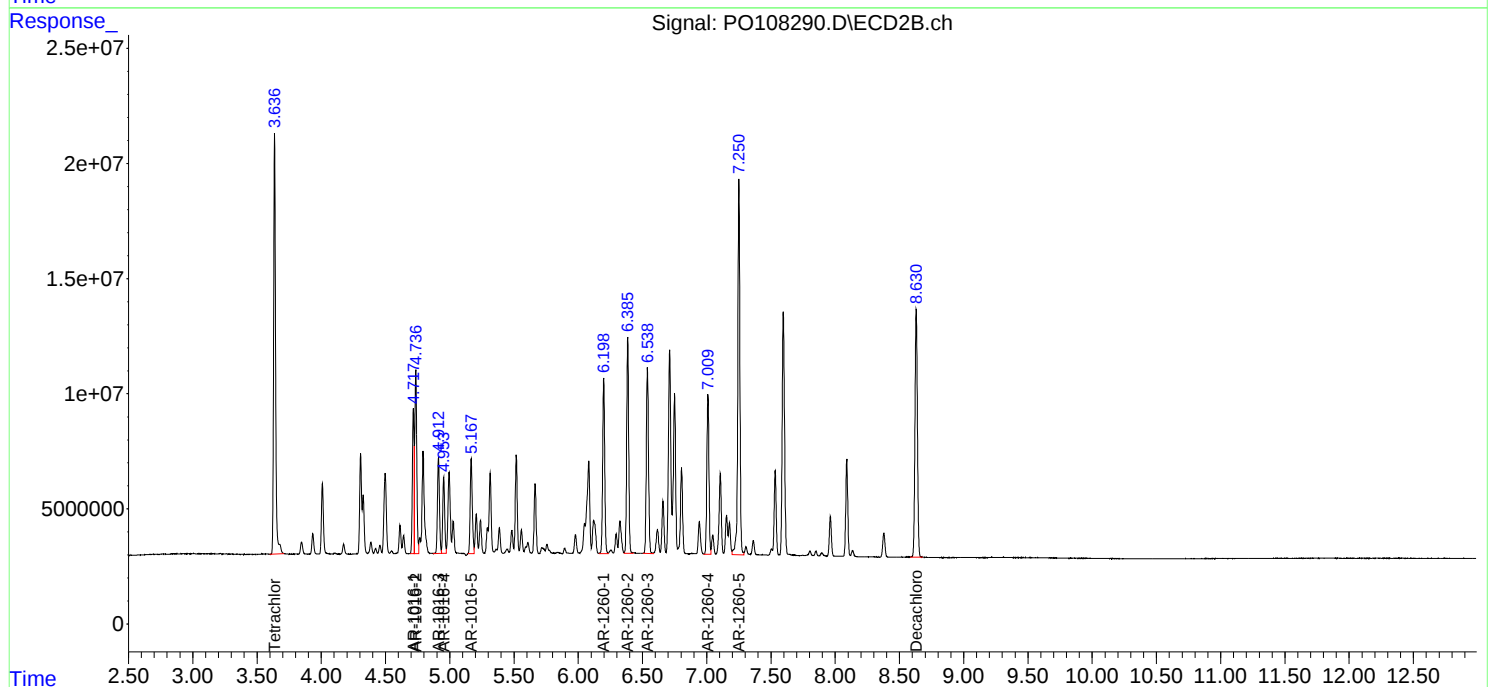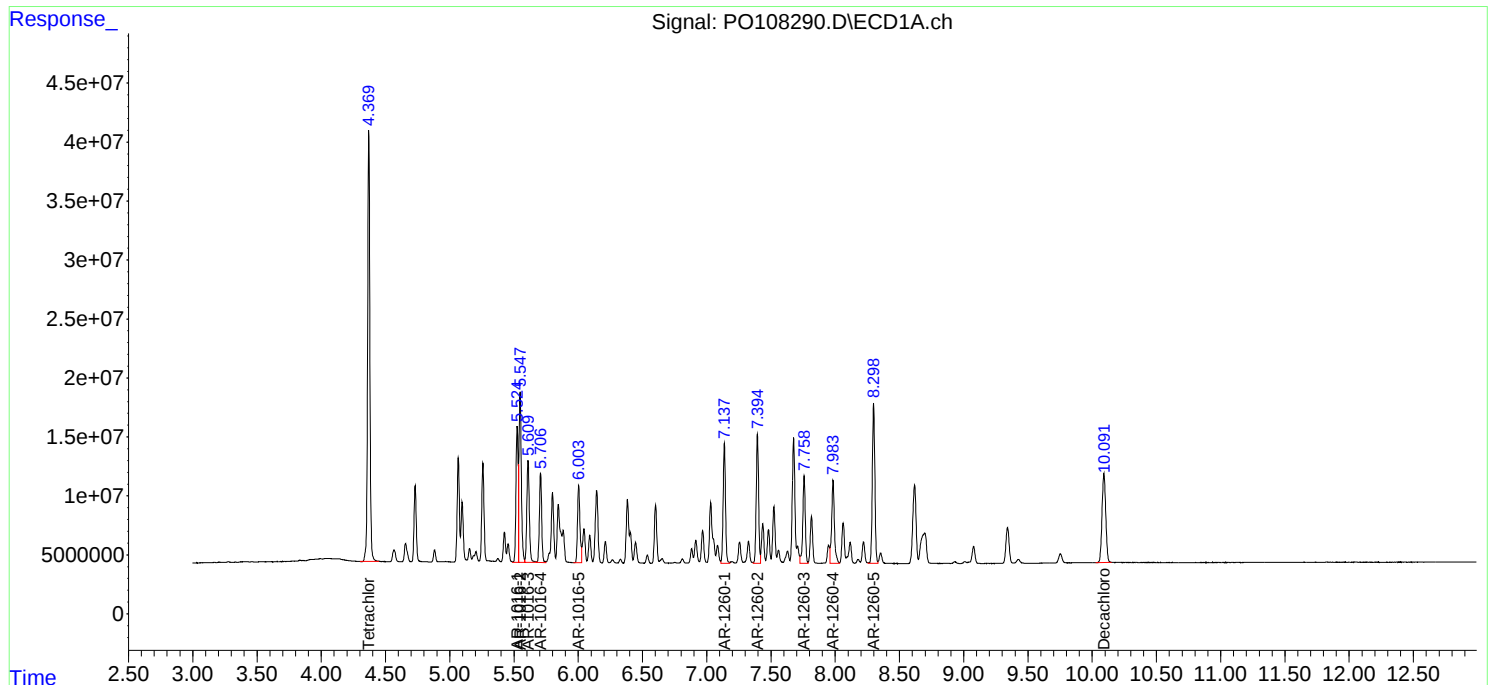

Analytical Sequence

Client: Tully Construction Co., Inc.

SDG No.: P5026

Project: Hamilton

Instrument ID: ECD_O

GC Column: ZB-MR1

ID: 0.32 (mm)

Inst. Calib. Date(s): 11/18/2024

11/18/2024

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	11/18/2024	15:16	PO108037.D	10.09	4.37
AR1660ICC1000	AR1660ICC1000	11/18/2024	15:32	PO108038.D	10.09	4.37
AR1660ICC750	AR1660ICC750	11/18/2024	15:48	PO108039.D	10.09	4.37
AR1660ICC500	AR1660ICC500	11/18/2024	16:05	PO108040.D	10.09	4.37
AR1660ICC250	AR1660ICC250	11/18/2024	16:21	PO108041.D	10.09	4.37
AR1660ICC050	AR1660ICC050	11/18/2024	16:37	PO108042.D	10.09	4.37
AR1221ICC500	AR1221ICC500	11/18/2024	16:53	PO108043.D	10.09	4.37
AR1232ICC500	AR1232ICC500	11/18/2024	17:09	PO108044.D	10.09	4.37
AR1242ICC1000	AR1242ICC1000	11/18/2024	17:25	PO108045.D	10.09	4.37
AR1242ICC750	AR1242ICC750	11/18/2024	17:42	PO108046.D	10.09	4.37
AR1242ICC500	AR1242ICC500	11/18/2024	17:58	PO108047.D	10.09	4.37
AR1242ICC250	AR1242ICC250	11/18/2024	18:14	PO108048.D	10.09	4.37
AR1242ICC050	AR1242ICC050	11/18/2024	18:30	PO108049.D	10.09	4.37
AR1248ICC1000	AR1248ICC1000	11/18/2024	18:47	PO108050.D	10.09	4.37
AR1248ICC750	AR1248ICC750	11/18/2024	19:03	PO108051.D	10.09	4.37
AR1248ICC500	AR1248ICC500	11/18/2024	19:19	PO108052.D	10.09	4.37
AR1248ICC250	AR1248ICC250	11/18/2024	19:35	PO108053.D	10.09	4.37
AR1248ICC050	AR1248ICC050	11/18/2024	19:51	PO108054.D	10.09	4.37
AR1254ICC1000	AR1254ICC1000	11/18/2024	20:07	PO108055.D	10.09	4.37
AR1254ICC750	AR1254ICC750	11/18/2024	20:24	PO108056.D	10.09	4.37
AR1254ICC500	AR1254ICC500	11/18/2024	20:40	PO108057.D	10.09	4.37
AR1254ICC250	AR1254ICC250	11/18/2024	20:56	PO108058.D	10.09	4.37
AR1254ICC050	AR1254ICC050	11/18/2024	21:12	PO108059.D	10.09	4.37
AR1262ICC500	AR1262ICC500	11/18/2024	21:28	PO108060.D	10.09	4.37
AR1268ICC1000	AR1268ICC1000	11/18/2024	21:45	PO108061.D	10.09	4.37
AR1268ICC750	AR1268ICC750	11/18/2024	22:02	PO108062.D	10.09	4.37
AR1268ICC500	AR1268ICC500	11/18/2024	22:19	PO108063.D	10.09	4.37
AR1268ICC250	AR1268ICC250	11/18/2024	22:35	PO108064.D	10.09	4.37
AR1268ICC050	AR1268ICC050	11/18/2024	22:51	PO108065.D	10.09	4.37
AR1660CCC500	AR1660CCC500	12/02/2024	10:02	PO108275.D	10.10	4.37
IBLK	IBLK	12/02/2024	11:07	PO108279.D	10.10	4.37
PB165309BL	PB165309BL	12/02/2024	12:20	PO108280.D	10.10	4.37
PB165309BS	PB165309BS	12/02/2024	12:37	PO108281.D	10.10	4.37
SOIL-1-HAM	P5026-01	12/02/2024	13:26	PO108284.D	10.10	4.37
SOIL-1-HAM	P5026-05	12/02/2024	13:43	PO108285.D	10.09	4.37
SOIL-1-HAMMS	P5026-05MS	12/02/2024	14:00	PO108286.D	10.10	4.37
SOIL-1-HAMMSD	P5026-05MSD	12/02/2024	14:16	PO108287.D	10.10	4.37
AR1660CCC500	AR1660CCC500	12/02/2024	15:36	PO108290.D	10.09	4.37
IBLK	IBLK	12/02/2024	17:11	PO108294.D	10.10	4.37

Analytical Sequence

Client: Tully Construction Co., Inc.

SDG No.: P5026

Project: Hamilton

Instrument ID: ECD_O

GC Column: ZB-MR2

ID: 0.32 (mm)

Inst. Calib. Date(s): 11/18/2024

11/18/2024

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	11/18/2024	15:16	PO108037.D	8.64	3.64
AR1660ICC1000	AR1660ICC1000	11/18/2024	15:32	PO108038.D	8.64	3.64
AR1660ICC750	AR1660ICC750	11/18/2024	15:48	PO108039.D	8.63	3.64
AR1660ICC500	AR1660ICC500	11/18/2024	16:05	PO108040.D	8.64	3.64
AR1660ICC250	AR1660ICC250	11/18/2024	16:21	PO108041.D	8.63	3.64
AR1660ICC050	AR1660ICC050	11/18/2024	16:37	PO108042.D	8.64	3.64
AR1221ICC500	AR1221ICC500	11/18/2024	16:53	PO108043.D	8.63	3.64
AR1232ICC500	AR1232ICC500	11/18/2024	17:09	PO108044.D	8.63	3.64
AR1242ICC1000	AR1242ICC1000	11/18/2024	17:25	PO108045.D	8.63	3.64
AR1242ICC750	AR1242ICC750	11/18/2024	17:42	PO108046.D	8.63	3.64
AR1242ICC500	AR1242ICC500	11/18/2024	17:58	PO108047.D	8.63	3.64
AR1242ICC250	AR1242ICC250	11/18/2024	18:14	PO108048.D	8.64	3.64
AR1242ICC050	AR1242ICC050	11/18/2024	18:30	PO108049.D	8.64	3.64
AR1248ICC1000	AR1248ICC1000	11/18/2024	18:47	PO108050.D	8.64	3.64
AR1248ICC750	AR1248ICC750	11/18/2024	19:03	PO108051.D	8.63	3.64
AR1248ICC500	AR1248ICC500	11/18/2024	19:19	PO108052.D	8.64	3.64
AR1248ICC250	AR1248ICC250	11/18/2024	19:35	PO108053.D	8.63	3.64
AR1248ICC050	AR1248ICC050	11/18/2024	19:51	PO108054.D	8.64	3.64
AR1254ICC1000	AR1254ICC1000	11/18/2024	20:07	PO108055.D	8.64	3.64
AR1254ICC750	AR1254ICC750	11/18/2024	20:24	PO108056.D	8.64	3.64
AR1254ICC500	AR1254ICC500	11/18/2024	20:40	PO108057.D	8.63	3.64
AR1254ICC250	AR1254ICC250	11/18/2024	20:56	PO108058.D	8.64	3.64
AR1254ICC050	AR1254ICC050	11/18/2024	21:12	PO108059.D	8.64	3.64
AR1262ICC500	AR1262ICC500	11/18/2024	21:28	PO108060.D	8.63	3.64
AR1268ICC1000	AR1268ICC1000	11/18/2024	21:45	PO108061.D	8.64	3.64
AR1268ICC750	AR1268ICC750	11/18/2024	22:02	PO108062.D	8.64	3.64
AR1268ICC500	AR1268ICC500	11/18/2024	22:19	PO108063.D	8.63	3.64
AR1268ICC250	AR1268ICC250	11/18/2024	22:35	PO108064.D	8.63	3.64
AR1268ICC050	AR1268ICC050	11/18/2024	22:51	PO108065.D	8.63	3.64
AR1660CCC500	AR1660CCC500	12/02/2024	10:02	PO108275.D	8.63	3.64
IBLK	IBLK	12/02/2024	11:07	PO108279.D	8.63	3.64
PB165309BL	PB165309BL	12/02/2024	12:20	PO108280.D	8.63	3.64
PB165309BS	PB165309BS	12/02/2024	12:37	PO108281.D	8.63	3.64
SOIL-1-HAM	P5026-01	12/02/2024	13:26	PO108284.D	8.63	3.64
SOIL-1-HAM	P5026-05	12/02/2024	13:43	PO108285.D	8.63	3.64
SOIL-1-HAMMS	P5026-05MS	12/02/2024	14:00	PO108286.D	8.63	3.64
SOIL-1-HAMMSD	P5026-05MSD	12/02/2024	14:16	PO108287.D	8.63	3.64
AR1660CCC500	AR1660CCC500	12/02/2024	15:36	PO108290.D	8.63	3.64
IBLK	IBLK	12/02/2024	17:11	PO108294.D	8.63	3.64

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB165309BS

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

Lab Sample ID: PB165309BS Date(s) Analyzed: 12/02/2024 12/02/2024

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO108281.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.528	5.478	5.578	158	157	5.57
COLUMN 1	2	5.55	5.5	5.6	157		
	3	5.613	5.563	5.663	154		
	4	5.711	5.661	5.761	157		
	5	6.008	5.958	6.058	157		
	1	4.718	4.668	4.768	165		
COLUMN 2	2	4.737	4.687	4.787	168	166	
	3	4.913	4.863	4.963	168		
	4	4.954	4.904	5.004	166		
	5	5.167	5.117	5.217	161		
Aroclor-1260	1	7.141	7.091	7.191	156	153	3.22
COLUMN 1	2	7.398	7.348	7.448	165		
	3	7.763	7.713	7.813	137		
	4	7.988	7.938	8.038	154		
	5	8.303	8.253	8.353	153		
	1	6.199	6.149	6.249	168	158	
COLUMN 2	2	6.386	6.336	6.436	167		
	3	6.54	6.49	6.59	167		
	4	7.011	6.961	7.061	144		
	5	7.252	7.202	7.302	142		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

SOIL-1-HAMMS

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

Lab Sample ID: P5026-05MS Date(s) Analyzed: 12/02/2024 12/02/2024

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO108286.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.526	5.476	5.576	187	184	8.33
COLUMN 1	2	5.549	5.499	5.599	185		
	3	5.611	5.561	5.661	180		
	4	5.709	5.659	5.759	193		
	5	6.005	5.955	6.055	175		
	1	4.716	4.666	4.766	203		
COLUMN 2	2	4.735	4.685	4.785	203	200	
	3	4.911	4.861	4.961	203		
	4	4.953	4.903	5.003	199		
	5	5.166	5.116	5.216	191		
Aroclor-1260	1	7.139	7.089	7.189	166	156	5.61
COLUMN 1	2	7.397	7.347	7.447	171		
	3	7.761	7.711	7.811	138		
	4	7.985	7.935	8.035	153		
	5	8.301	8.251	8.351	151		
	1	6.198	6.148	6.248	183		
COLUMN 2	2	6.386	6.336	6.436	178	165	
	3	6.538	6.488	6.588	177		
	4	7.01	6.96	7.06	148		
	5	7.251	7.201	7.301	139		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

SOIL-1-HAMMSD

Contract: TULL02

Lab Code: CHEM Case No.: P5026 SAS No.: P5026 SDG NO.: P5026

Lab Sample ID: P5026-05MSD Date(s) Analyzed: 12/02/2024 12/02/2024

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO108287.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	5.525	5.475	5.575	172	174	13.4
COLUMN 1	2	5.548	5.498	5.598	170		
	3	5.61	5.56	5.66	167		
	4	5.707	5.657	5.757	182		
	5	6.005	5.955	6.055	179		
	1	4.717	4.667	4.767	202		
COLUMN 2	2	4.736	4.686	4.786	202	199	
	3	4.912	4.862	4.962	202		
	4	4.953	4.903	5.003	199		
	5	5.167	5.117	5.217	192		
Aroclor-1260	1	7.138	7.088	7.188	166	156	7.41
COLUMN 1	2	7.395	7.345	7.445	170		
	3	7.76	7.71	7.81	139		
	4	7.985	7.935	8.035	153		
	5	8.301	8.251	8.351	152		
	1	6.198	6.148	6.248	187		
COLUMN 2	2	6.385	6.335	6.435	180	168	
	3	6.538	6.488	6.588	181		
	4	7.009	6.959	7.059	149		
	5	7.25	7.2	7.3	142		



QC SAMPLE DATA

Report of Analysis

Client:	Tully Construction Co., Inc.		Date Collected:		
Project:	Hamilton		Date Received:		
Client Sample ID:	PB165309BL		SDG No.:	P5026	
Lab Sample ID:	PB165309BL		Matrix:	SOIL	
Analytical Method:	SW8082A		% Solid:	100	Decanted:
Sample Wt/Vol:	30.02	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108280.D	1	12/02/24 08:20	12/02/24 12:20	PB165309

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	0.0034	U	0.0034	0.017	mg/Kg
11104-28-2	Aroclor-1221	0.0064	U	0.0064	0.017	mg/Kg
11141-16-5	Aroclor-1232	0.0034	U	0.0034	0.017	mg/Kg
53469-21-9	Aroclor-1242	0.0034	U	0.0034	0.017	mg/Kg
12672-29-6	Aroclor-1248	0.0079	U	0.0079	0.017	mg/Kg
11097-69-1	Aroclor-1254	0.0027	U	0.0027	0.017	mg/Kg
37324-23-5	Aroclor-1262	0.0046	U	0.0046	0.017	mg/Kg
11100-14-4	Aroclor-1268	0.0034	U	0.0034	0.017	mg/Kg
11096-82-5	Aroclor-1260	0.0029	U	0.0029	0.017	mg/Kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	22.3		32 - 144	111%	SPK: 20
2051-24-3	Decachlorobiphenyl	23.3		32 - 175	116%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
 Data File : PO108280.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2024 12:20
 Operator : YP/AJ
 Sample : PB165309BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB165309BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 00:33:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.637	188.4E6	75553375	21.644	22.284
2) SA Decachlor...	10.101	8.633	71115897	71113876	23.285	20.905

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
Data File : PO108280.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2024 12:20
Operator : YP/AJ
Sample : PB165309BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB165309BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 00:33:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

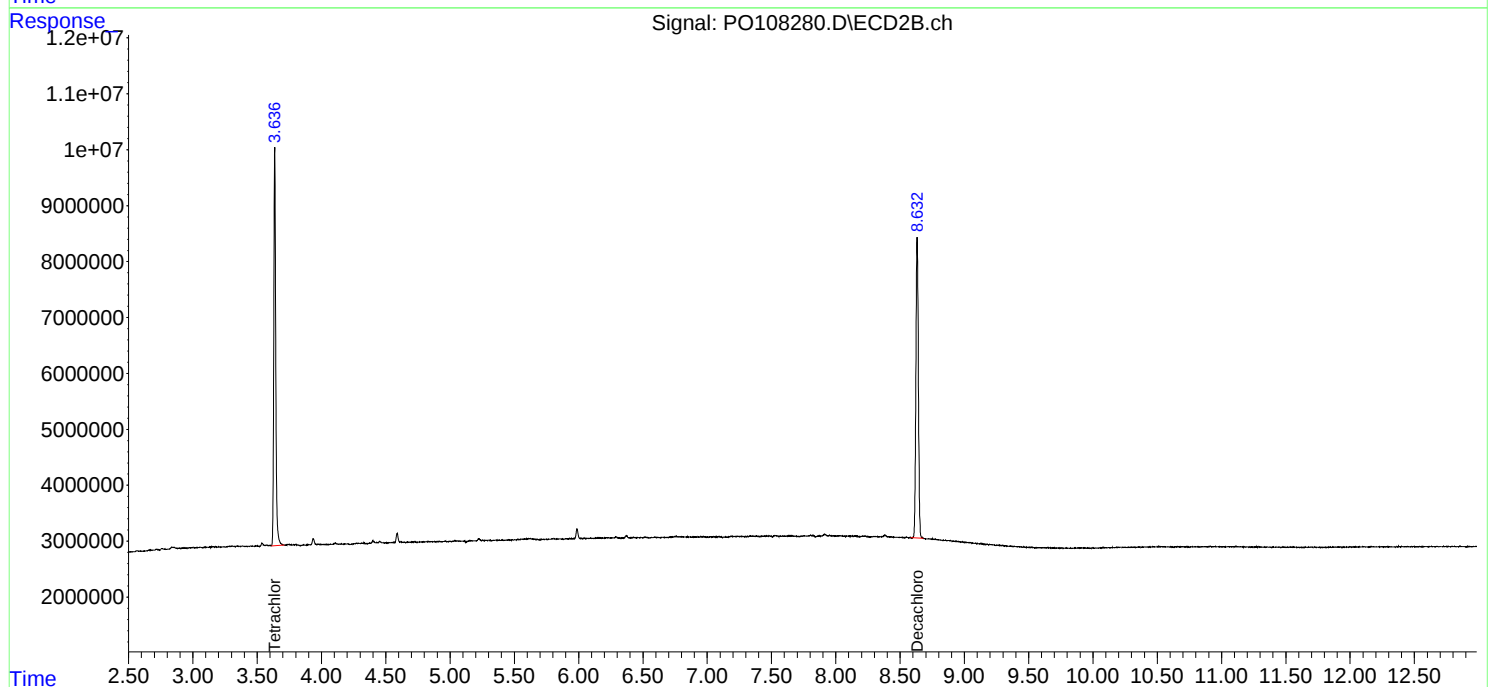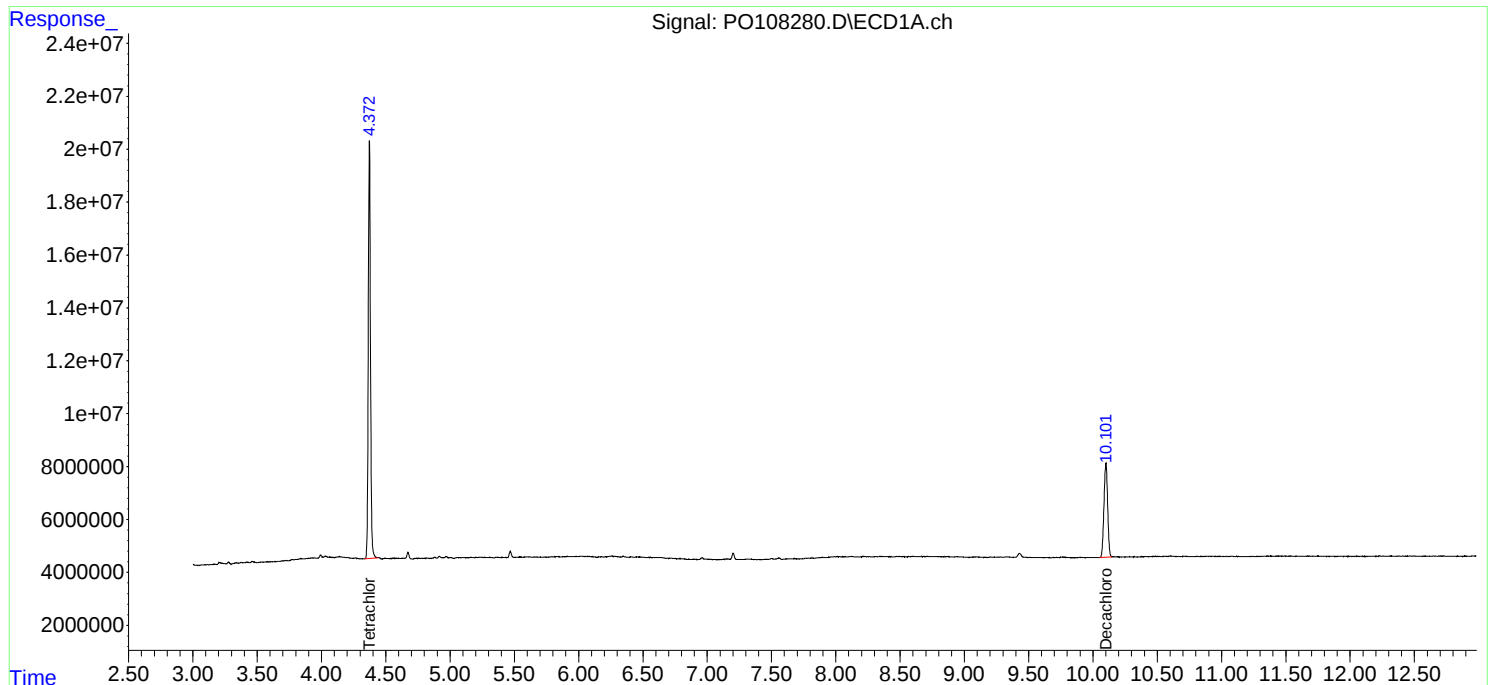


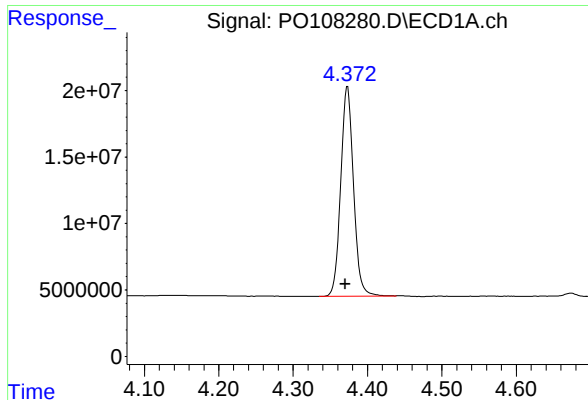

#1 Tetrachloro-m-xylene


R.T.: 4.373 min
Delta R.T.: 0.003 min
Response: 188435581
Conc: 21.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB165309BL

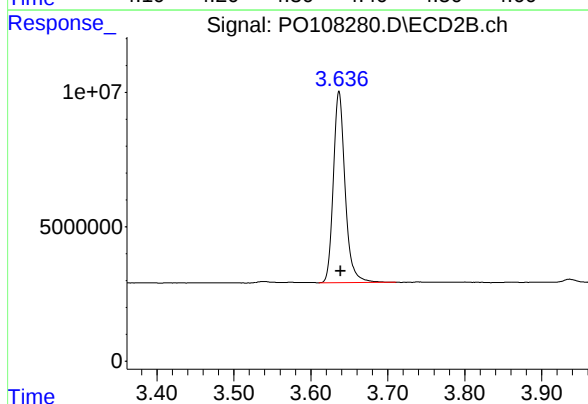


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 75553375
Conc: 22.28 ng/ml

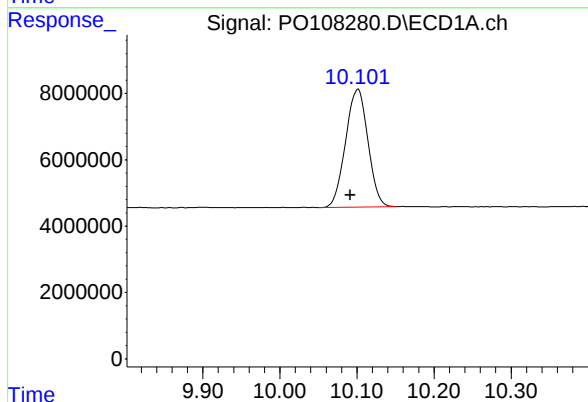

#2 Decachlorobiphenyl

R.T.: 10.101 min
Delta R.T.: 0.010 min
Response: 71115897
Conc: 23.28 ng/ml

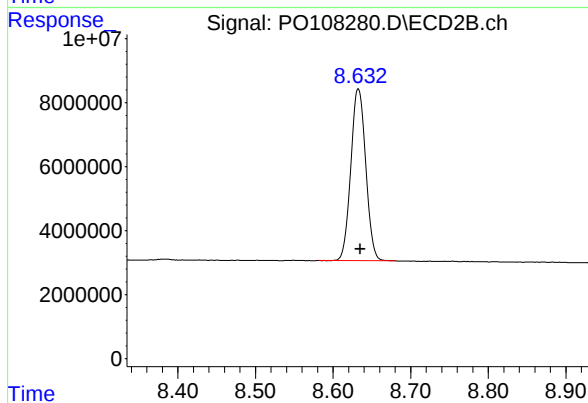

#2 Decachlorobiphenyl

R.T.: 8.633 min
Delta R.T.: -0.003 min
Response: 71113876
Conc: 20.91 ng/ml

Report of Analysis

Client:	Tully Construction Co., Inc.		Date Collected:	11/18/24	
Project:	Hamilton		Date Received:	11/18/24	
Client Sample ID:	PIBLK-PO108037.D		SDG No.:	P5026	
Lab Sample ID:	I.BLK-PO108037.D		Matrix:	WATER	
Analytical Method:	SW8082A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	5030				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108037.D	1		11/18/24	PO111824

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.00015	U	0.00015	0.00050	mg/L
11104-28-2	Aroclor-1221	0.00023	U	0.00023	0.00050	mg/L
11141-16-5	Aroclor-1232	0.00037	U	0.00037	0.00050	mg/L
53469-21-9	Aroclor-1242	0.00016	U	0.00016	0.00050	mg/L
12672-29-6	Aroclor-1248	0.00012	U	0.00012	0.00050	mg/L
11097-69-1	Aroclor-1254	0.00011	U	0.00011	0.00050	mg/L
11096-82-5	Aroclor-1260	0.00015	U	0.00015	0.00050	mg/L
37324-23-5	Aroclor-1262	0.00014	U	0.00014	0.00050	mg/L
11100-14-4	Aroclor-1268	0.00012	U	0.00012	0.00050	mg/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.0		60 - 140	105%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.5		60 - 140	112%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
 Data File : PO108037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 15:16
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 16:53:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 18 16:52:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.638	184.5E6	71172641	21.187	20.992
2) SA Decachlor...	10.090	8.636	70888561	76430464	23.210	22.468

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111824\
Data File : PO108037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 15:16
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 16:53:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 18 16:52:46 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

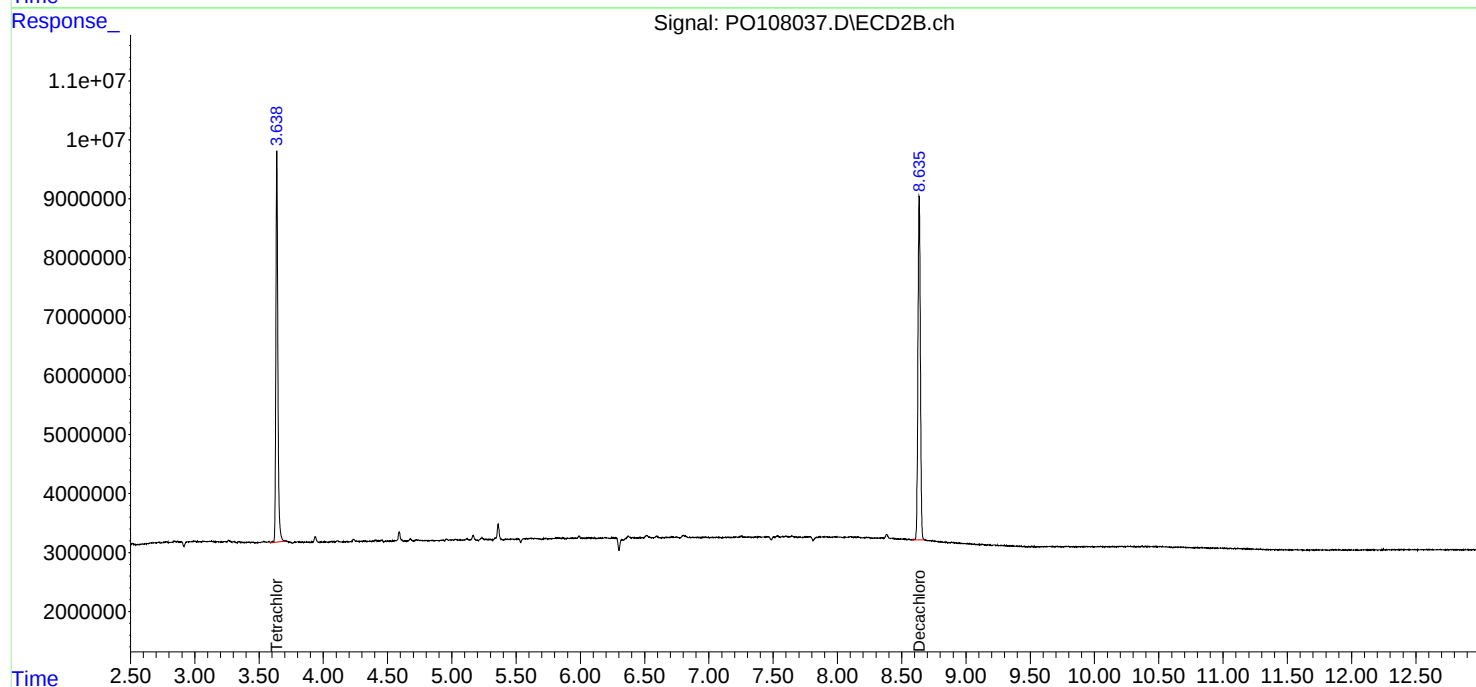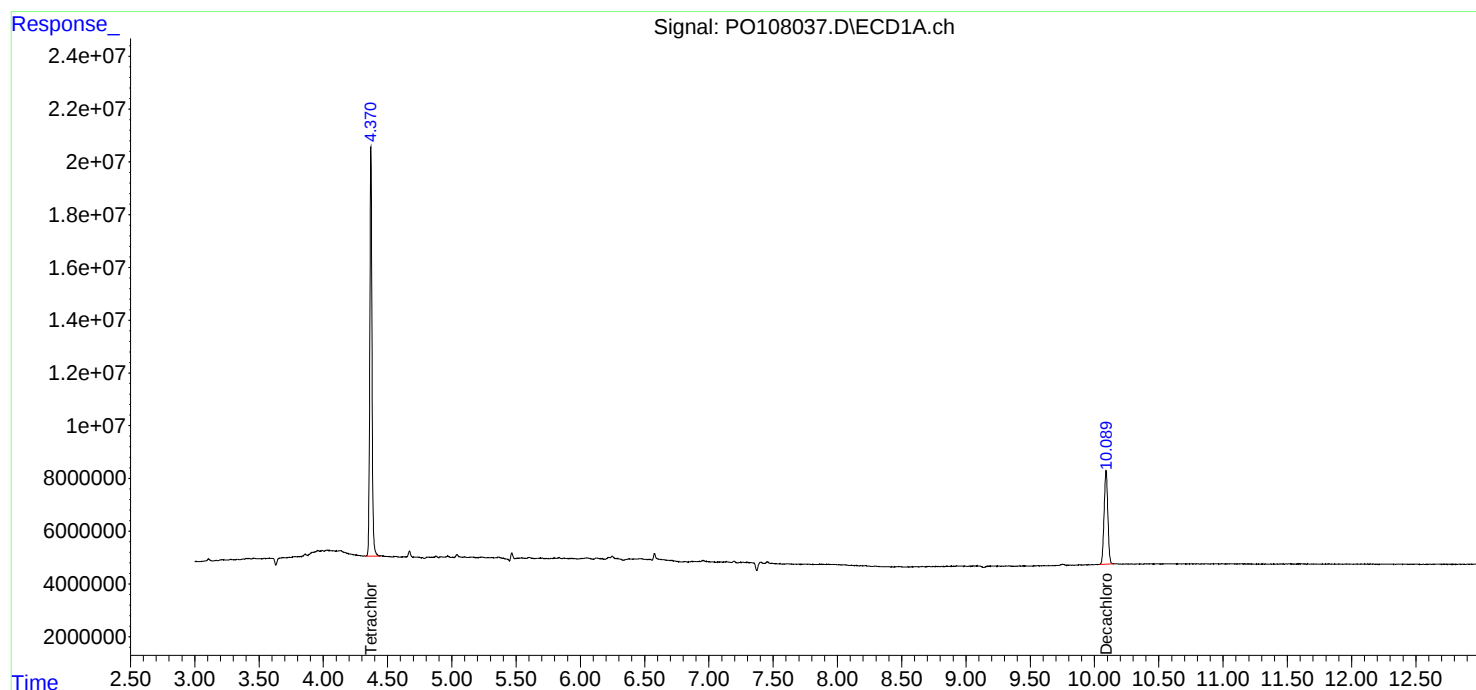


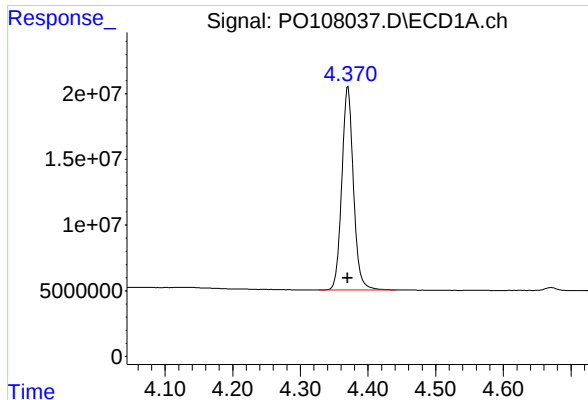

#1 Tetrachloro-m-xylene


R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 184453457
Conc: 21.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

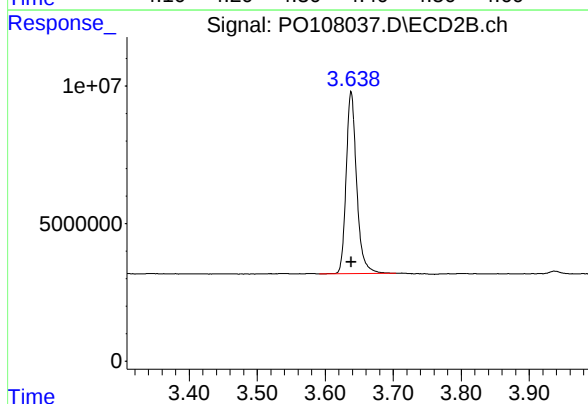


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: 0.000 min
Response: 71172641
Conc: 20.99 ng/ml

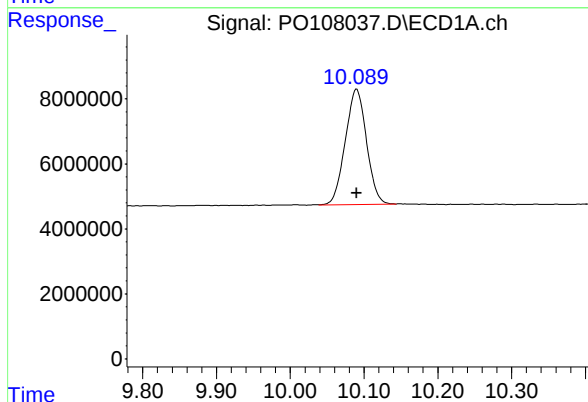

#2 Decachlorobiphenyl

R.T.: 10.090 min
Delta R.T.: 0.000 min
Response: 70888561
Conc: 23.21 ng/ml

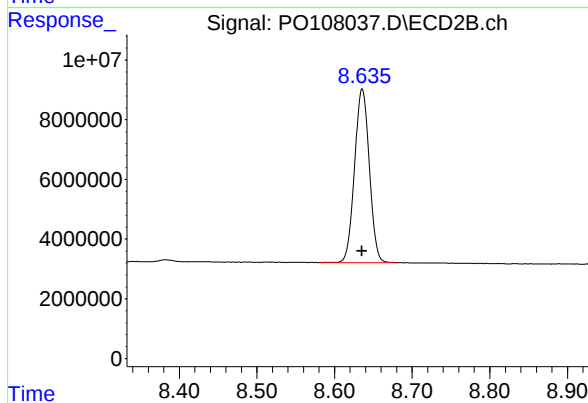

#2 Decachlorobiphenyl

R.T.: 8.636 min
Delta R.T.: 0.000 min
Response: 76430464
Conc: 22.47 ng/ml

Report of Analysis

Client:	Tully Construction Co., Inc.	Date Collected:	12/02/24
Project:	Hamilton	Date Received:	12/02/24
Client Sample ID:	PIBLK-PO108279.D	SDG No.:	P5026
Lab Sample ID:	I.BLK-PO108279.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108279.D	1		12/02/24	PO120224

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.00015	U	0.00015	0.00050	mg/L
11104-28-2	Aroclor-1221	0.00023	U	0.00023	0.00050	mg/L
11141-16-5	Aroclor-1232	0.00037	U	0.00037	0.00050	mg/L
53469-21-9	Aroclor-1242	0.00016	U	0.00016	0.00050	mg/L
12672-29-6	Aroclor-1248	0.00012	U	0.00012	0.00050	mg/L
11097-69-1	Aroclor-1254	0.00011	U	0.00011	0.00050	mg/L
11096-82-5	Aroclor-1260	0.00015	U	0.00015	0.00050	mg/L
37324-23-5	Aroclor-1262	0.00014	U	0.00014	0.00050	mg/L
11100-14-4	Aroclor-1268	0.00012	U	0.00012	0.00050	mg/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	22.8		60 - 140	114%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.1		60 - 140	111%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
Data File : PO108279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2024 11:07
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 00:32:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.637	198.8E6	81336760	22.838	23.990
2) SA Decachlor...	10.095	8.632	76740935	75290625	25.126	22.133

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
Data File : PO108279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2024 11:07
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 00:32:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

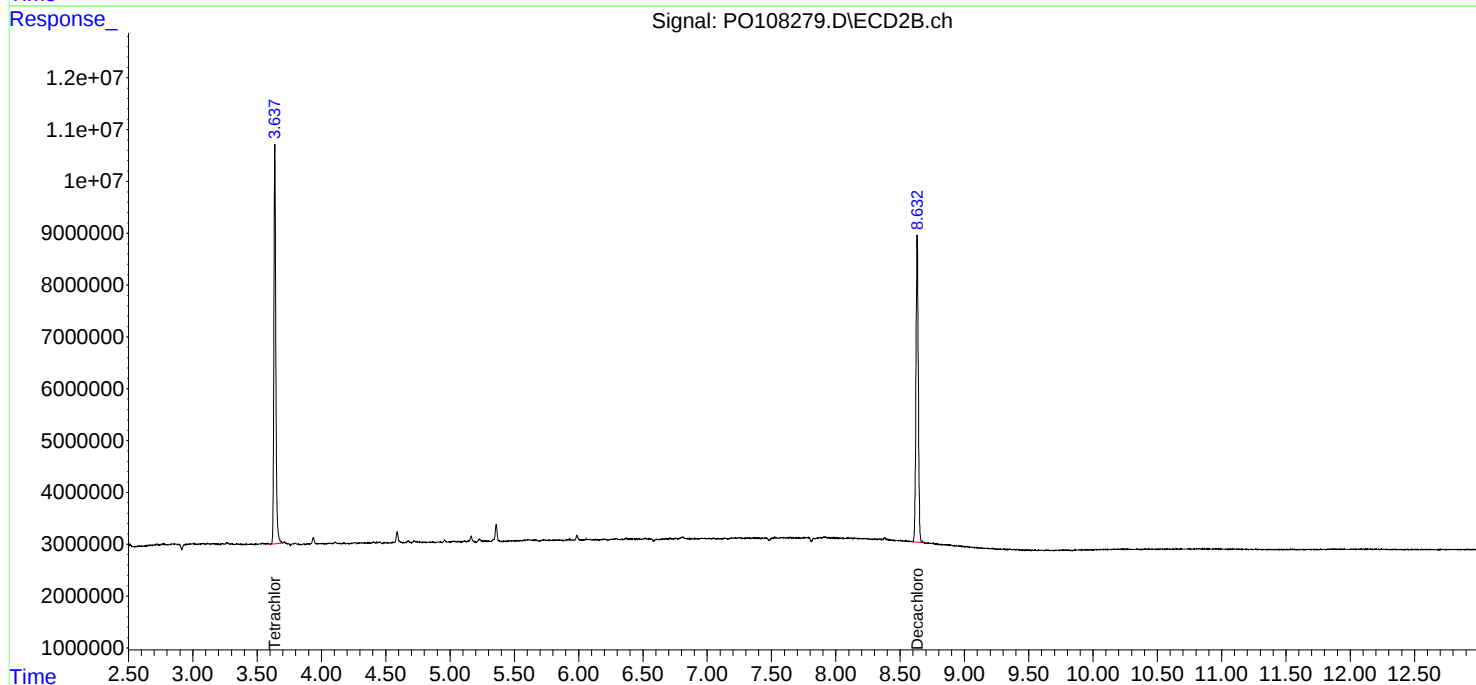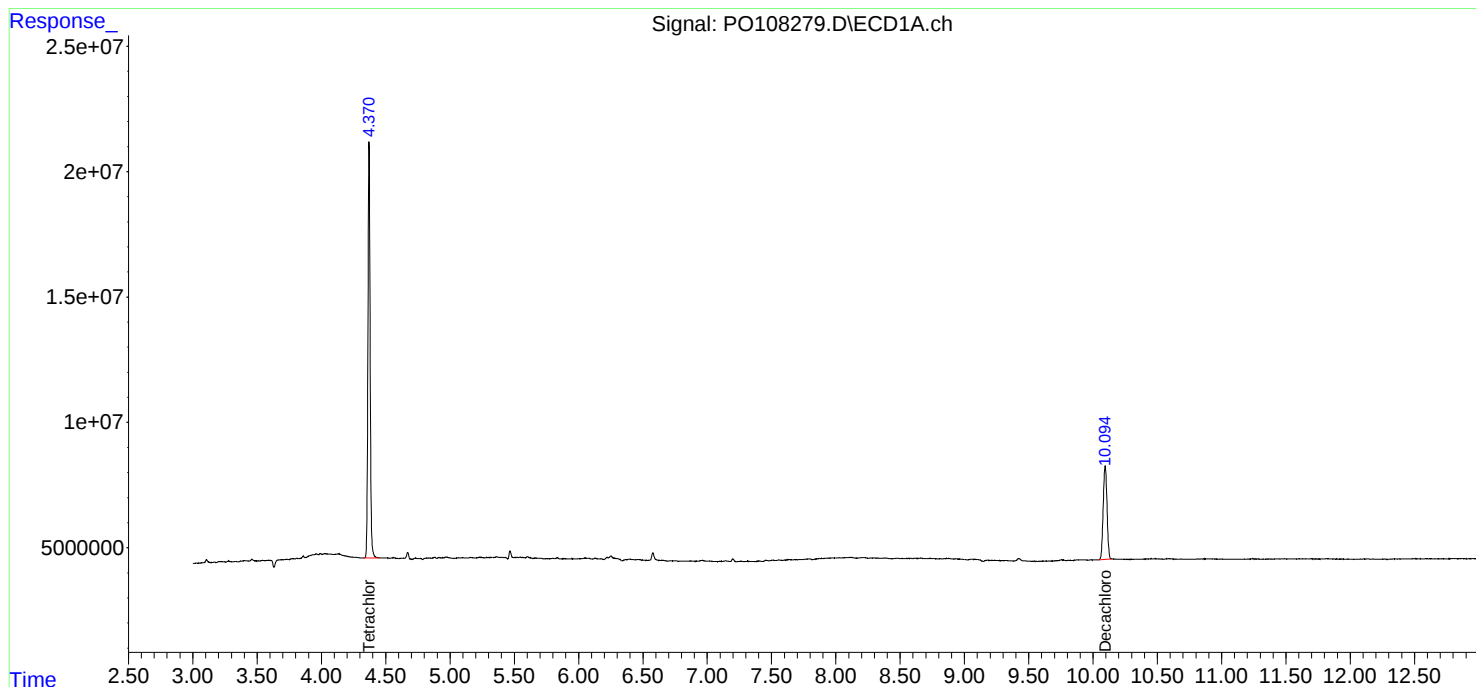


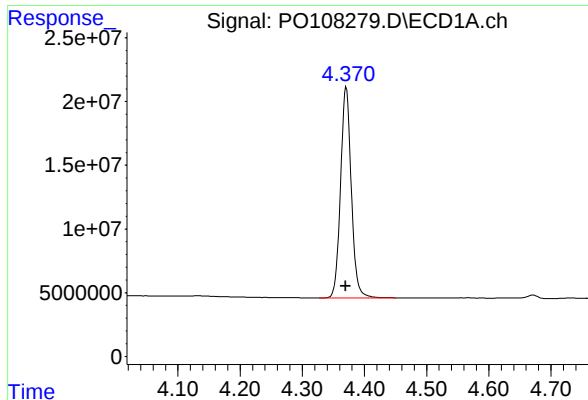

#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 198833273
Conc: 22.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

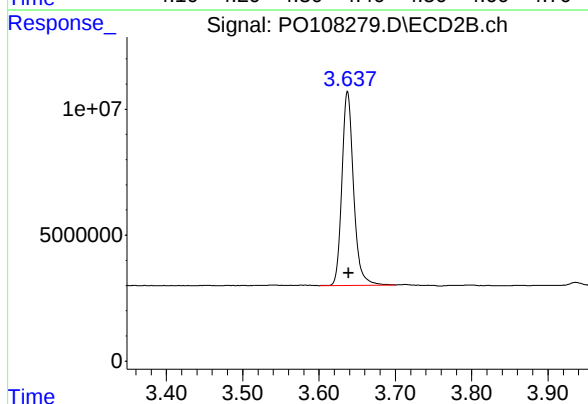


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 81336760
Conc: 23.99 ng/ml

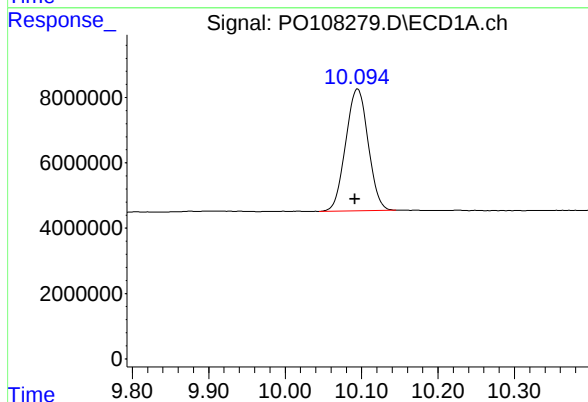

#2 Decachlorobiphenyl

R.T.: 10.095 min
Delta R.T.: 0.003 min
Response: 76740935
Conc: 25.13 ng/ml

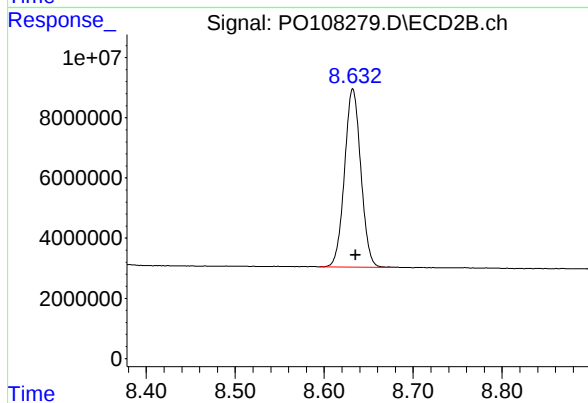

#2 Decachlorobiphenyl

R.T.: 8.632 min
Delta R.T.: -0.003 min
Response: 75290625
Conc: 22.13 ng/ml

Report of Analysis

Client:	Tully Construction Co., Inc.		Date Collected:	12/02/24	
Project:	Hamilton		Date Received:	12/02/24	
Client Sample ID:	PIBLK-PO108294.D		SDG No.:	P5026	
Lab Sample ID:	I.BLK-PO108294.D		Matrix:	WATER	
Analytical Method:	SW8082A		% Solid:	0	Decanted:
Sample Wt/Vol:	1000	Units: mL	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	5030				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108294.D	1		12/02/24	PO120224

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.00015	U	0.00015	0.00050	mg/L
11104-28-2	Aroclor-1221	0.00023	U	0.00023	0.00050	mg/L
11141-16-5	Aroclor-1232	0.00037	U	0.00037	0.00050	mg/L
53469-21-9	Aroclor-1242	0.00016	U	0.00016	0.00050	mg/L
12672-29-6	Aroclor-1248	0.00012	U	0.00012	0.00050	mg/L
11097-69-1	Aroclor-1254	0.00011	U	0.00011	0.00050	mg/L
11096-82-5	Aroclor-1260	0.00015	U	0.00015	0.00050	mg/L
37324-23-5	Aroclor-1262	0.00014	U	0.00014	0.00050	mg/L
11100-14-4	Aroclor-1268	0.00012	U	0.00012	0.00050	mg/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	22.9		60 - 140	115%	SPK: 20
2051-24-3	Decachlorobiphenyl	20.8		60 - 140	104%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
 Data File : PO108294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2024 17:11
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 00:37:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.636	199.7E6	82845560	22.934	24.435
2) SA Decachlor...	10.095	8.631	75749808	70849348	24.802	20.828

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
Data File : PO108294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2024 17:11
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 00:37:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

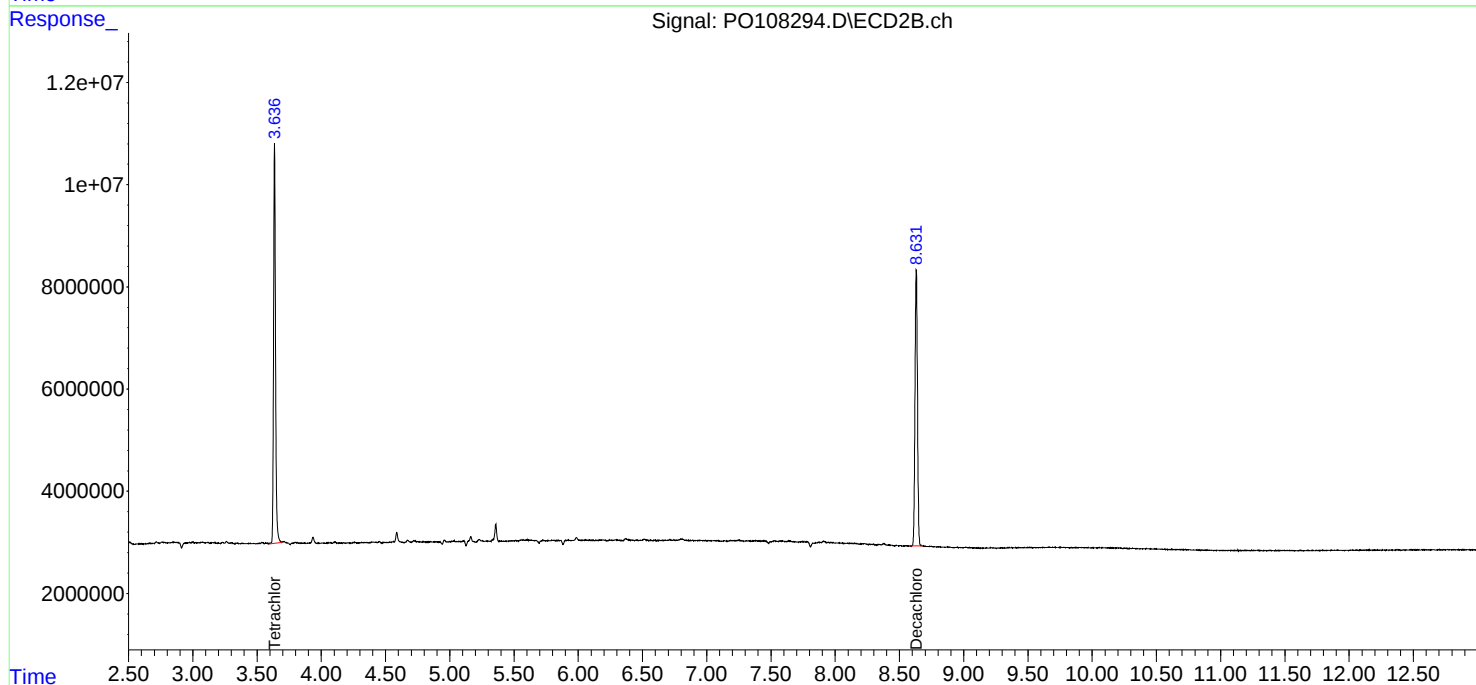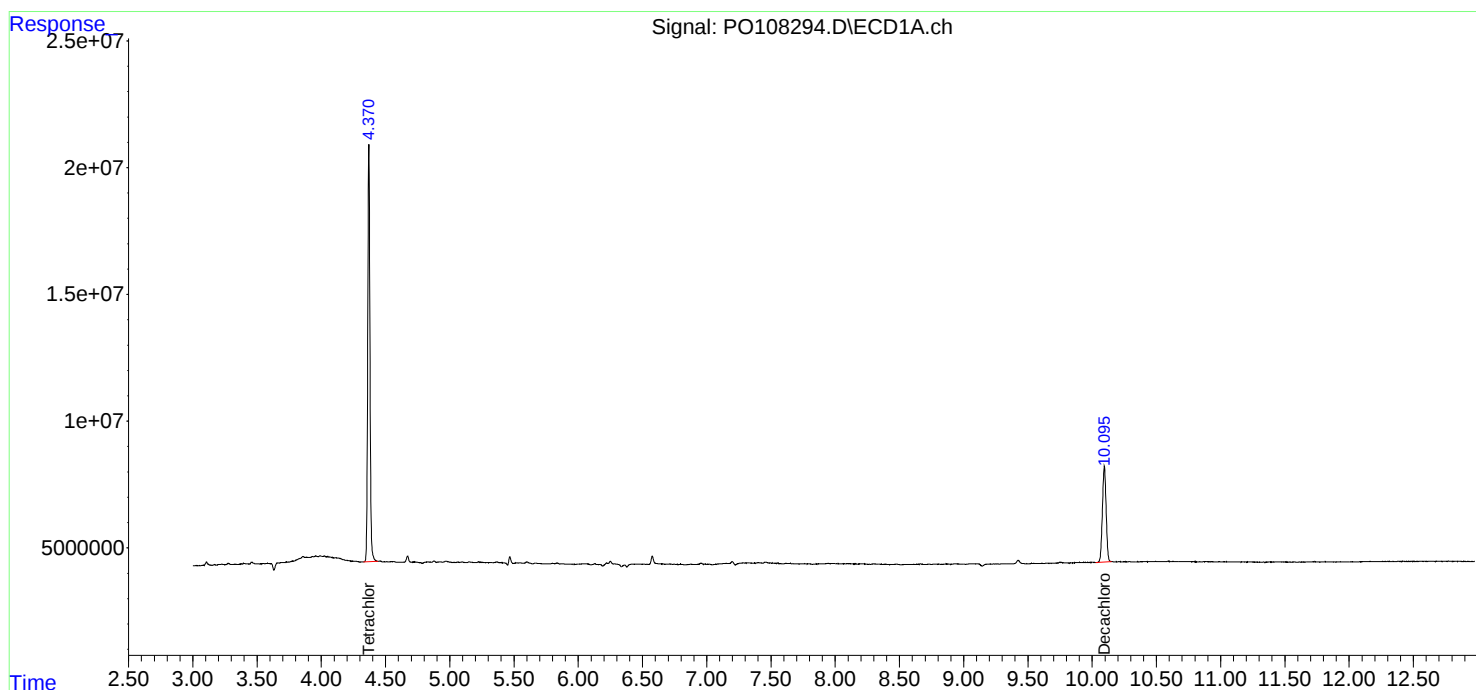


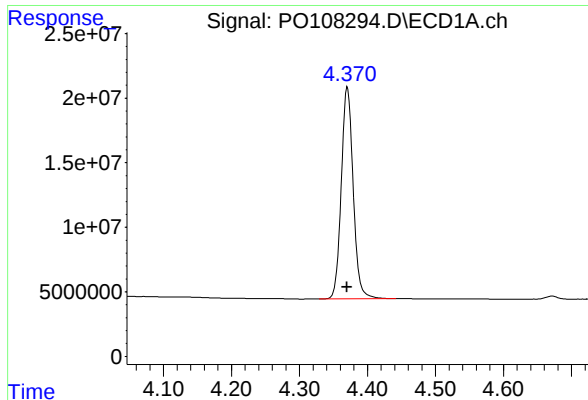

#1 Tetrachloro-m-xylene


R.T.: 4.371 min
Delta R.T.: 0.000 min
Response: 199665565
Conc: 22.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

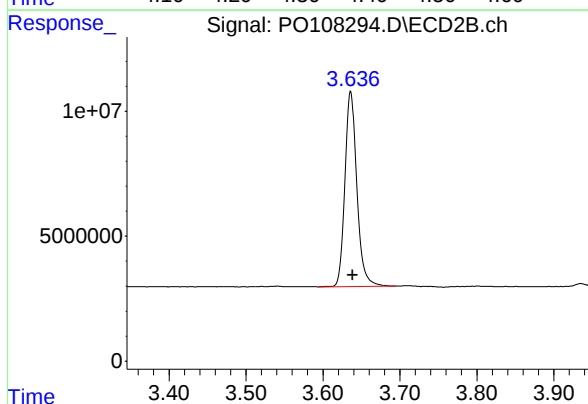


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.003 min
Response: 82845560
Conc: 24.44 ng/ml

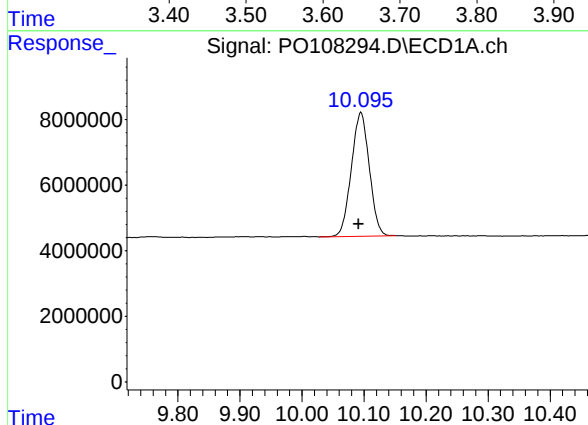

#2 Decachlorobiphenyl

R.T.: 10.095 min
Delta R.T.: 0.004 min
Response: 75749808
Conc: 24.80 ng/ml

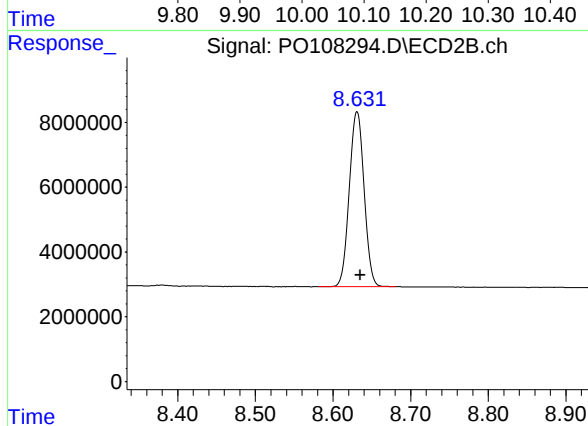

#2 Decachlorobiphenyl

R.T.: 8.631 min
Delta R.T.: -0.004 min
Response: 70849348
Conc: 20.83 ng/ml

Report of Analysis

Client:	Tully Construction Co., Inc.		Date Collected:		
Project:	Hamilton		Date Received:		
Client Sample ID:	PB165309BS		SDG No.:	P5026	
Lab Sample ID:	PB165309BS		Matrix:	SOIL	
Analytical Method:	SW8082A		% Solid:	100	Decanted:
Sample Wt/Vol:	30.01	Units: g	Final Vol:	10000	uL
Soil Aliquot Vol:		uL	Test:	PCB	
Extraction Type:			Injection Volume :		
GPC Factor :	1.0	PH :			
Prep Method :	SW3541B				

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108281.D	1	12/02/24 08:20	12/02/24 12:37	PB165309

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	0.17		0.0034	0.017	mg/Kg
11104-28-2	Aroclor-1221	0.0064	U	0.0064	0.017	mg/Kg
11141-16-5	Aroclor-1232	0.0034	U	0.0034	0.017	mg/Kg
53469-21-9	Aroclor-1242	0.0034	U	0.0034	0.017	mg/Kg
12672-29-6	Aroclor-1248	0.0079	U	0.0079	0.017	mg/Kg
11097-69-1	Aroclor-1254	0.0027	U	0.0027	0.017	mg/Kg
37324-23-5	Aroclor-1262	0.0046	U	0.0046	0.017	mg/Kg
11100-14-4	Aroclor-1268	0.0034	U	0.0034	0.017	mg/Kg
11096-82-5	Aroclor-1260	0.16		0.0029	0.017	mg/Kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.2		32 - 144	106%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.9		32 - 175	115%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
 Data File : PO108281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2024 12:37
 Operator : YP/AJ
 Sample : PB165309BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB165309BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 00:33:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.637	184.2E6	69845663	21.155	20.601
2) SA Decachlor...	10.099	8.632	70013162	69892306	22.924	20.546
Target Compounds						
3) L1 AR-1016-1	5.528	4.718	127.4E6	54200324	473.637	496.005
4) L1 AR-1016-2	5.550	4.737	182.8E6	76946983	471.559	503.242
5) L1 AR-1016-3	5.613	4.913	115.3E6	41408331	461.326	503.970
6) L1 AR-1016-4	5.711	4.954	92138315	31647792	471.853	497.038
7) L1 AR-1016-5	6.008	5.167	87275202	41961959	470.663	484.008
31) L7 AR-1260-1	7.141	6.199	128.5E6	81804560	468.317	505.151
32) L7 AR-1260-2	7.398	6.386	140.5E6	98689253	496.336	501.307
33) L7 AR-1260-3	7.763	6.540	88200679	93546653	410.562	502.601
34) L7 AR-1260-4	7.988	7.011	102.7E6	68947625	462.676	430.937
35) L7 AR-1260-5	8.303	7.252	175.2E6	167.9E6	459.114	427.641



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
Data File : PO108281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2024 12:37
Operator : YP/AJ
Sample : PB165309BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB165309BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 00:33:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

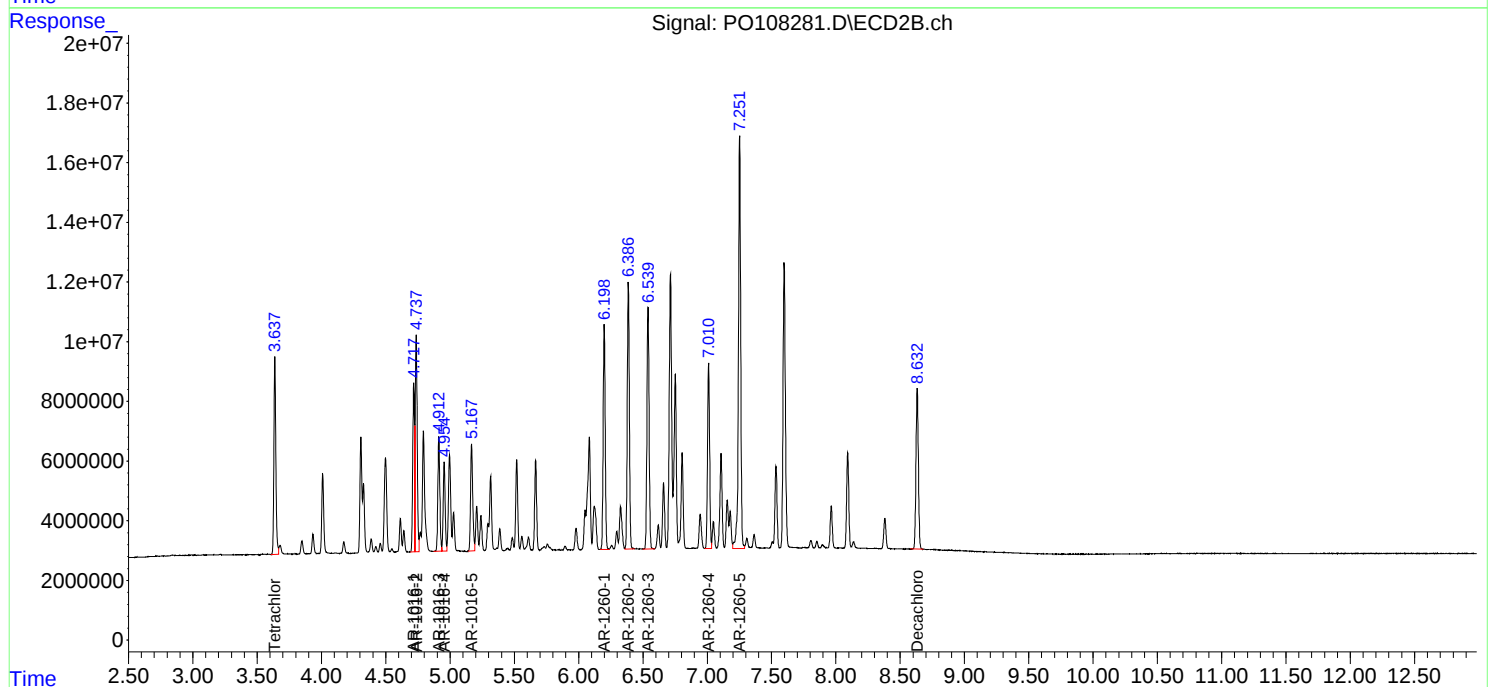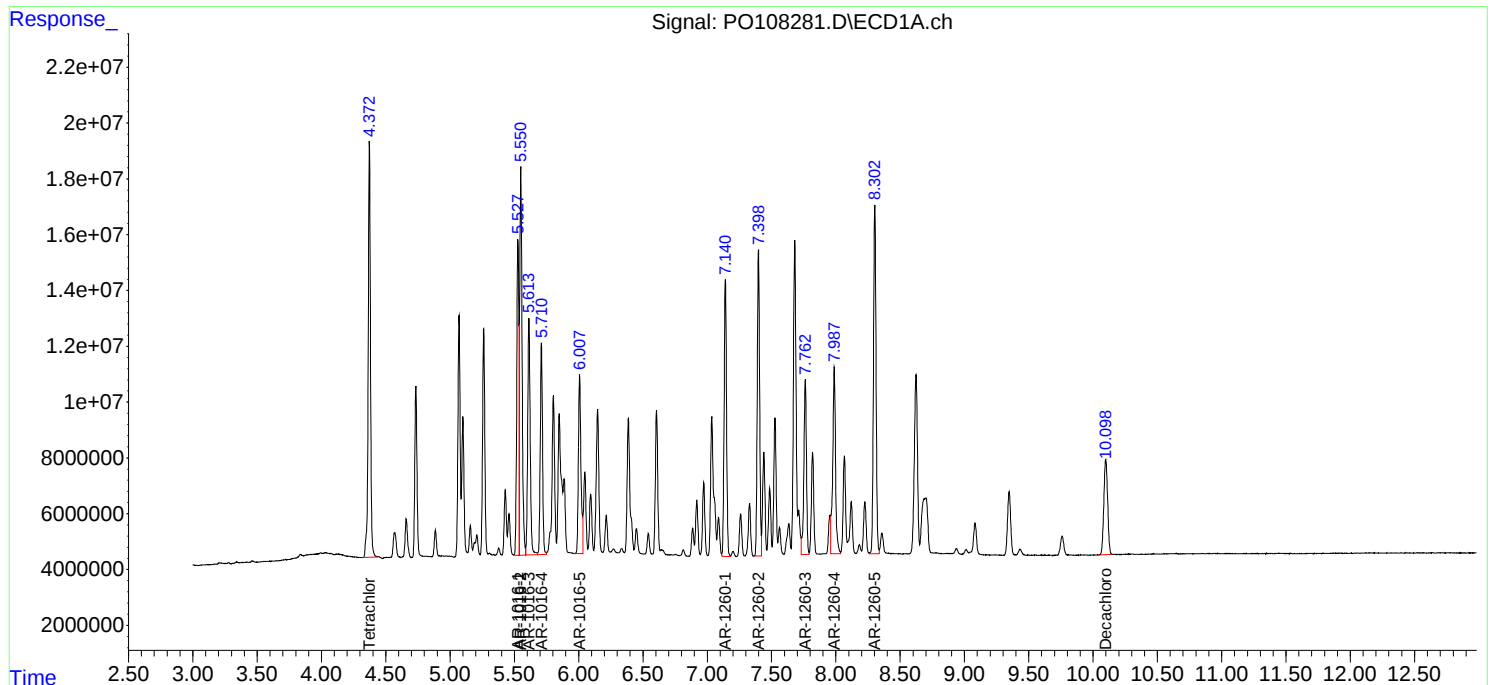

Report of Analysis

Client:	Tully Construction Co., Inc.	Date Collected:	11/27/24
Project:	Hamilton	Date Received:	11/27/24
Client Sample ID:	SOIL-1-HAMMS	SDG No.:	P5026
Lab Sample ID:	P5026-05MS	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	77.8
Sample Wt/Vol:	30.01	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108286.D	1	12/02/24 08:20	12/02/24 14:00	PB165309

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	0.20		0.0044	0.022	mg/Kg
11104-28-2	Aroclor-1221	0.0082	U	0.0082	0.022	mg/Kg
11141-16-5	Aroclor-1232	0.0044	U	0.0044	0.022	mg/Kg
53469-21-9	Aroclor-1242	0.0044	U	0.0044	0.022	mg/Kg
12672-29-6	Aroclor-1248	0.010	U	0.010	0.022	mg/Kg
11097-69-1	Aroclor-1254	0.0035	U	0.0035	0.022	mg/Kg
37324-23-5	Aroclor-1262	0.0059	U	0.0059	0.022	mg/Kg
11100-14-4	Aroclor-1268	0.0044	U	0.0044	0.022	mg/Kg
11096-82-5	Aroclor-1260	0.17		0.0037	0.022	mg/Kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.0		32 - 144	100%	SPK: 20
2051-24-3	Decachlorobiphenyl	16.5		32 - 175	82%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
 Data File : PO108286.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2024 14:00
 Operator : YP/AJ
 Sample : P5026-05MS
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SOIL-1-HAMMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 00:34:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.635	162.4E6	67752358	18.654	19.983
2) SA Decachlor...	10.095	8.631	50375827	46042931	16.494	13.535
Target Compounds						
3) L1 AR-1016-1	5.526	4.716	117.1E6	51674949	435.581	472.894
4) L1 AR-1016-2	5.549	4.735	167.1E6	72493312	431.159	474.115
5) L1 AR-1016-3	5.611	4.911	104.9E6	38987770	419.809	474.510
6) L1 AR-1016-4	5.709	4.953	87943590	29517109	450.371	463.575
7) L1 AR-1016-5	6.005	5.166	75676728	38728311	408.114	446.710
31) L7 AR-1260-1	7.139	6.198	106.7E6	69281718	388.679	427.821
32) L7 AR-1260-2	7.397	6.386	113.0E6	81585667	399.280	414.427
33) L7 AR-1260-3	7.761	6.538	69417826	76797435	323.131	412.612 #
34) L7 AR-1260-4	7.985	7.010	79280542	55191062	357.106	344.956
35) L7 AR-1260-5	8.301	7.251	134.2E6	127.6E6	351.622	324.981



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
Data File : PO108286.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2024 14:00
Operator : YP/AJ
Sample : P5026-05MS
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SOIL-1-HAMMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 00:34:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

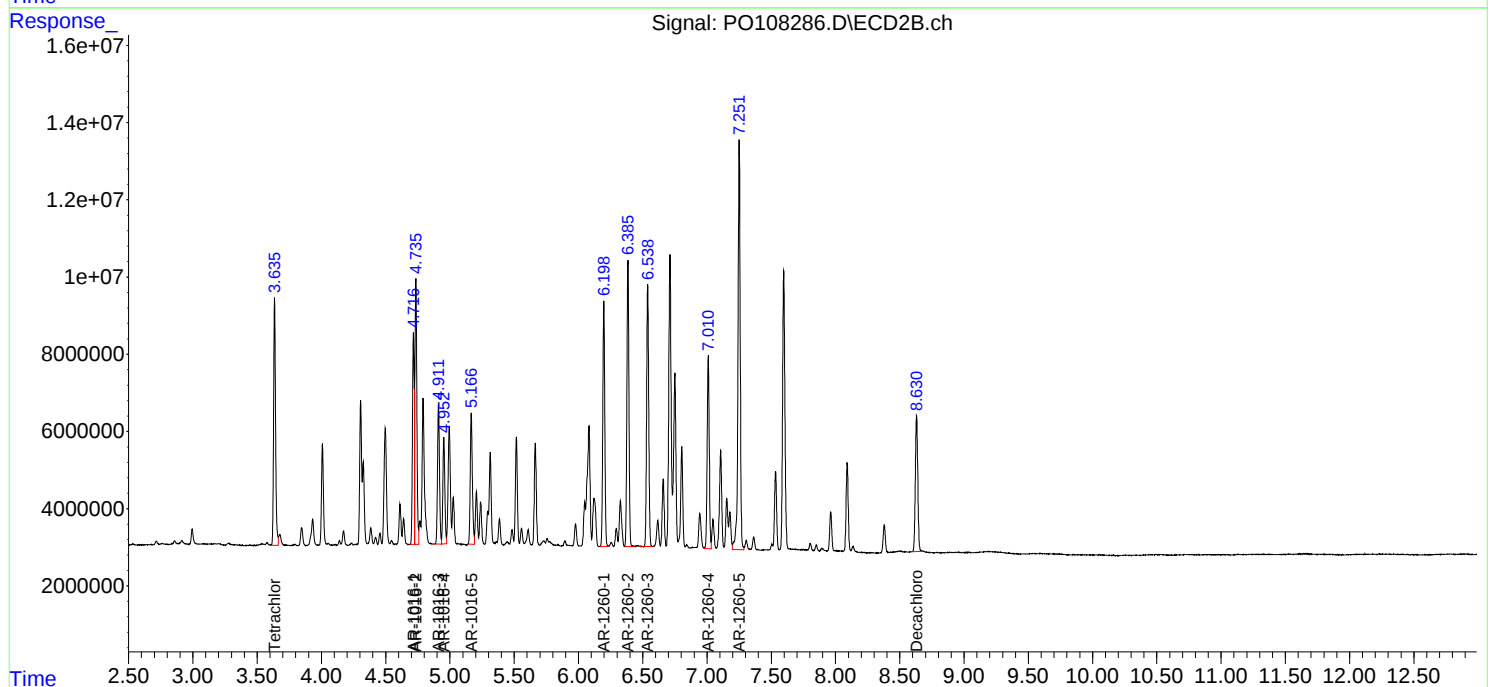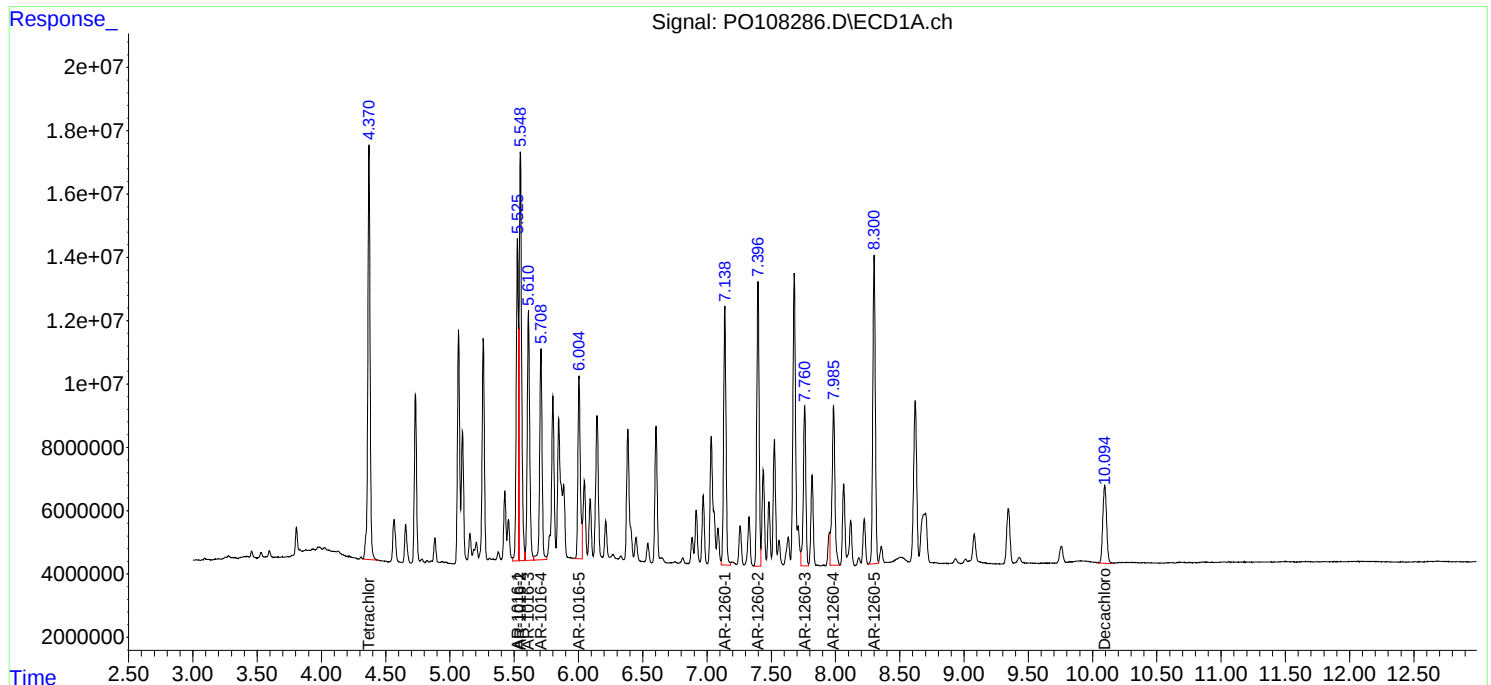

Report of Analysis

Client:	Tully Construction Co., Inc.	Date Collected:	11/27/24
Project:	Hamilton	Date Received:	11/27/24
Client Sample ID:	SOIL-1-HAMMSD	SDG No.:	P5026
Lab Sample ID:	P5026-05MSD	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	77.8
Sample Wt/Vol:	30.06	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108287.D	1	12/02/24 08:20	12/02/24 14:16	PB165309

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	0.20		0.0043	0.022	mg/Kg
11104-28-2	Aroclor-1221	0.0082	U	0.0082	0.022	mg/Kg
11141-16-5	Aroclor-1232	0.0044	U	0.0044	0.022	mg/Kg
53469-21-9	Aroclor-1242	0.0043	U	0.0043	0.022	mg/Kg
12672-29-6	Aroclor-1248	0.010	U	0.010	0.022	mg/Kg
11097-69-1	Aroclor-1254	0.0035	U	0.0035	0.022	mg/Kg
37324-23-5	Aroclor-1262	0.0059	U	0.0059	0.022	mg/Kg
11100-14-4	Aroclor-1268	0.0044	U	0.0044	0.022	mg/Kg
11096-82-5	Aroclor-1260	0.17		0.0037	0.022	mg/Kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.8		32 - 144	99%	SPK: 20
2051-24-3	Decachlorobiphenyl	16.4		32 - 175	82%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
 Data File : PO108287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Dec 2024 14:16
 Operator : YP/AJ
 Sample : P5026-05MSD
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SOIL-1-HAMMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 00:35:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 19 03:13:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.636	165.1E6	67082482	18.958	19.786
2) SA Decachlor...	10.095	8.630	50097083	46837196	16.403	13.769
Target Compounds						
3) L1 AR-1016-1	5.525	4.717	108.3E6	51548033	402.542	471.733
4) L1 AR-1016-2	5.548	4.736	154.2E6	72086292	397.770	471.453
5) L1 AR-1016-3	5.610	4.912	97447577	38906149	389.925	473.517
6) L1 AR-1016-4	5.707	4.953	82979341	29563769	424.948	464.308
7) L1 AR-1016-5	6.005	5.167	77687478	38983969	418.958	449.659
31) L7 AR-1260-1	7.138	6.198	106.6E6	70665447	388.280	436.366
32) L7 AR-1260-2	7.395	6.385	112.5E6	82887040	397.643	421.037
33) L7 AR-1260-3	7.760	6.538	69971425	78655687	325.708	422.596 #
34) L7 AR-1260-4	7.985	7.009	79461352	55771830	357.920	348.586
35) L7 AR-1260-5	8.301	7.250	135.5E6	130.6E6	355.185	332.561



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120224\
Data File : PO108287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Dec 2024 14:16
Operator : YP/AJ
Sample : P5026-05MSD
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SOIL-1-HAMMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 00:35:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 19 03:13:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

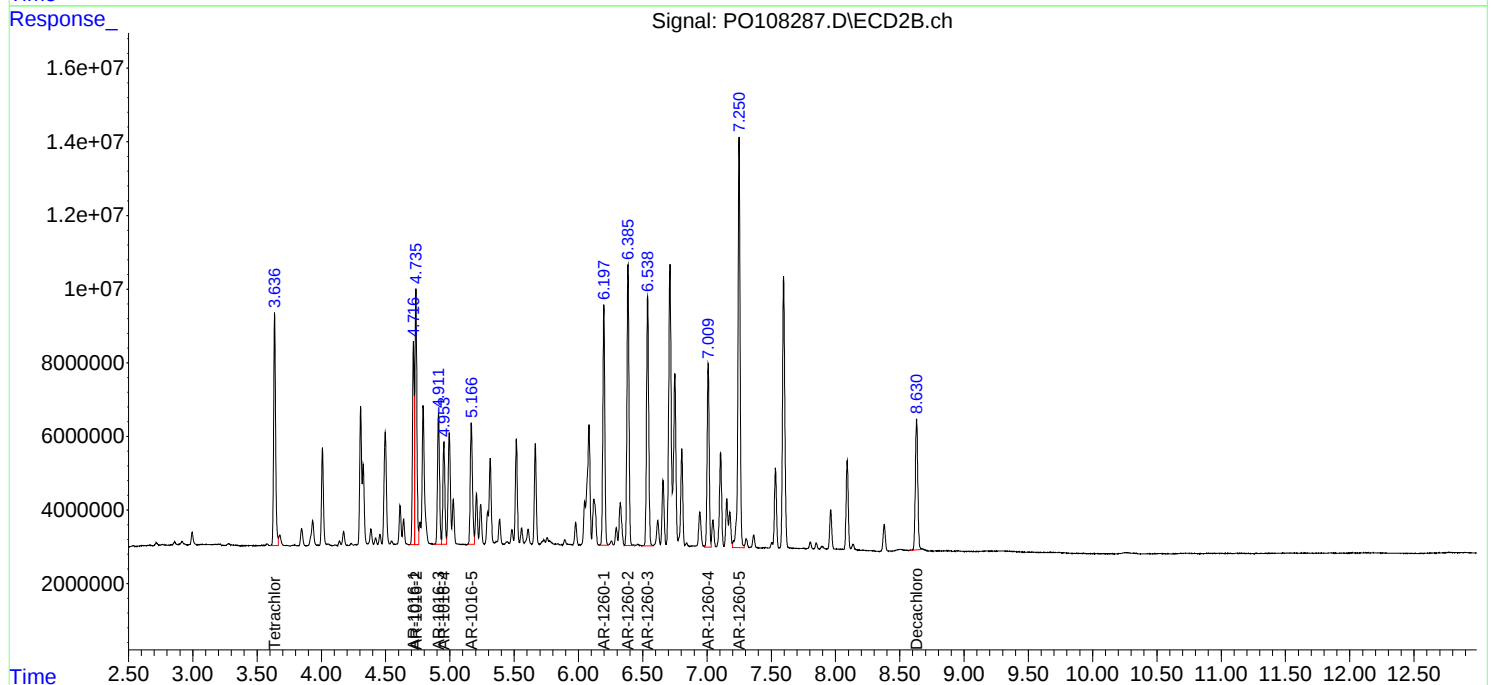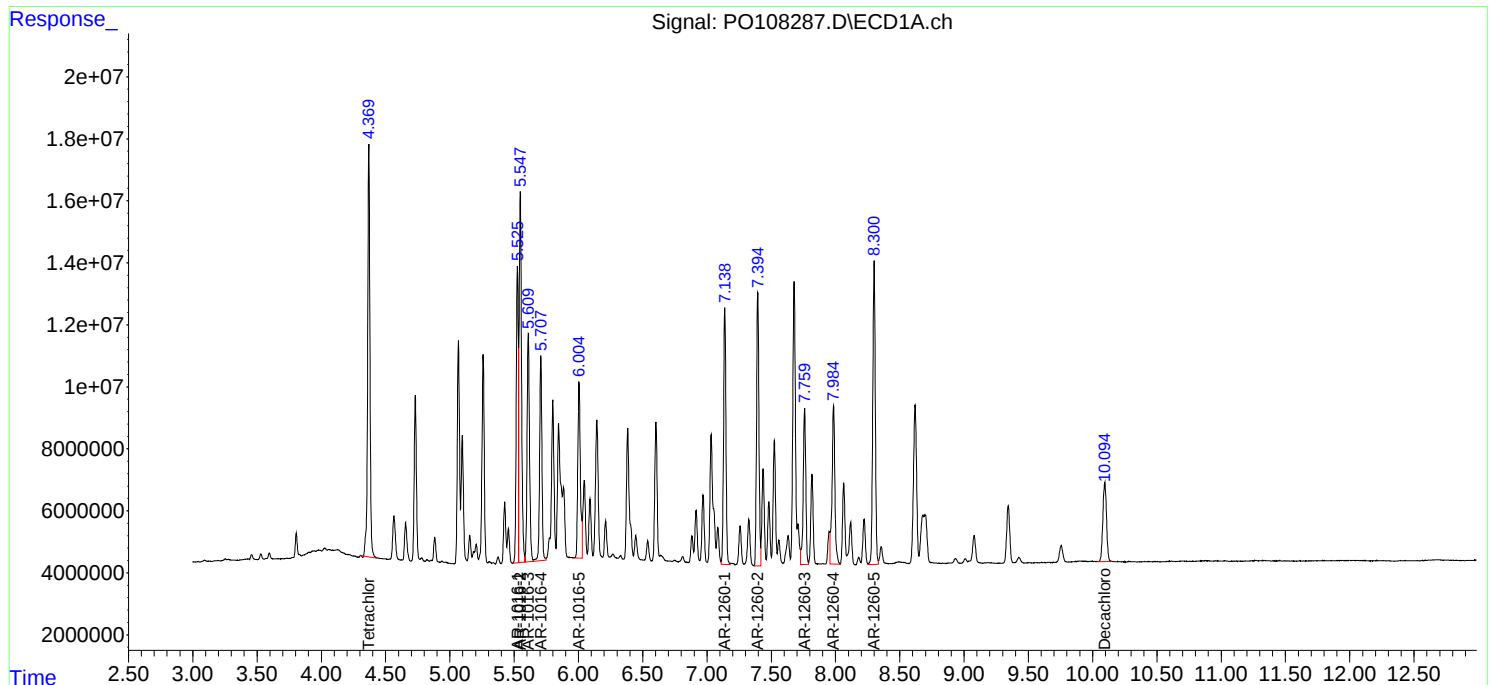

Manual Integration Report

Sequence:	PO111824	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC050	PO108042.D	AR-1260-1	yogesh	11/19/2024 9:13:44 AM	Ankita	11/19/2024 11:25:21	Peak Integrated by Software
AR1660ICC050	PO108042.D	AR-1260-1 #2	yogesh	11/19/2024 9:13:44 AM	Ankita	11/19/2024 11:25:21	Peak Integrated by Software
AR1660ICC050	PO108042.D	AR-1260-2	yogesh	11/19/2024 9:13:44 AM	Ankita	11/19/2024 11:25:21	Peak Integrated by Software
AR1660ICC050	PO108042.D	AR-1260-2 #2	yogesh	11/19/2024 9:13:44 AM	Ankita	11/19/2024 11:25:21	Peak Integrated by Software
AR1660ICC050	PO108042.D	AR-1260-3	yogesh	11/19/2024 9:13:44 AM	Ankita	11/19/2024 11:25:21	Peak Integrated by Software
AR1242ICC050	PO108049.D	AR-1242-5	yogesh	11/19/2024 9:13:45 AM	Ankita	11/19/2024 11:25:23	Peak Integrated by Software
AR1242ICC050	PO108049.D	AR-1242-5 #2	yogesh	11/19/2024 9:13:45 AM	Ankita	11/19/2024 11:25:23	Peak Integrated by Software
AR1248ICC050	PO108054.D	AR-1248-4	yogesh	11/19/2024 9:13:47 AM	Ankita	11/19/2024 11:25:25	Peak Integrated by Software
AR1248ICC050	PO108054.D	AR-1248-5	yogesh	11/19/2024 9:13:47 AM	Ankita	11/19/2024 11:25:25	Peak Integrated by Software
AR1248ICC050	PO108054.D	AR-1248-5 #2	yogesh	11/19/2024 9:13:47 AM	Ankita	11/19/2024 11:25:25	Peak Integrated by Software
AR1254ICC050	PO108059.D	AR-1254-3	yogesh	11/19/2024 9:13:49 AM	Ankita	11/19/2024 11:25:26	Peak Integrated by Software
AR1254ICC050	PO108059.D	AR-1254-4	yogesh	11/19/2024 9:13:49 AM	Ankita	11/19/2024 11:25:26	Peak Integrated by Software
AR1254ICC050	PO108059.D	AR-1254-4 #2	yogesh	11/19/2024 9:13:49 AM	Ankita	11/19/2024 11:25:26	Peak Integrated by Software

Manual Integration Report

Sequence:

PO111824

Instrument

ECD_o

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1254ICC050	PO108059.D	AR-1254-5	yogesh	11/19/2024 9:13:49 AM	Ankita	11/19/2024 11:25:26	Peak Integrated by Software
AR1268ICC750	PO108062.D	AR-1268-1	yogesh	11/19/2024 9:13:50 AM	Ankita	11/19/2024 11:25:27	Peak Integrated by Software
AR1268ICC500	PO108063.D	AR-1268-1	yogesh	11/19/2024 9:13:52 AM	Ankita	11/19/2024 11:25:29	Peak Integrated by Software
AR1268ICV500	PO108070.D	AR-1268-1	yogesh	11/19/2024 9:13:54 AM	Ankita	11/19/2024 11:25:30	Peak Integrated by Software

Manual Integration Report

Sequence:	PO120224	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
P5026-01	PO108284.D	Tetrachloro-m-xylene	yogesh	12/3/2024 8:42:14 AM	Ankita	12/3/2024 9:04:03	Peak Integrated by Software
AR1242CCC500	PO108291.D	AR-1242-1 #2	yogesh	12/3/2024 11:20:07 AM	Ankita	12/3/2024 11:23:28	Peak Integrated by Software
AR1242CCC500	PO108291.D	AR-1242-2 #2	yogesh	12/3/2024 11:20:07 AM	Ankita	12/3/2024 11:23:28	Peak Integrated by Software
AR1242CCC500	PO108291.D	AR-1242-3 #2	yogesh	12/3/2024 11:20:07 AM	Ankita	12/3/2024 11:23:28	Peak Integrated by Software
AR1242CCC500	PO108291.D	AR-1242-4 #2	yogesh	12/3/2024 11:20:07 AM	Ankita	12/3/2024 11:23:28	Peak Integrated by Software
AR1242CCC500	PO108291.D	AR-1242-5 #2	yogesh	12/3/2024 11:20:07 AM	Ankita	12/3/2024 11:23:28	Peak Integrated by Software
AR1242CCC500	PO108291.D	Decachlorobiphenyl #2	yogesh	12/3/2024 11:20:07 AM	Ankita	12/3/2024 11:23:28	Peak Integrated by Software
AR1242CCC500	PO108291.D	Tetrachloro-m-xylene #2	yogesh	12/3/2024 11:20:07 AM	Ankita	12/3/2024 11:23:28	Peak Integrated by Software

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO111824

Review By	yogesh	Review On	11/19/2024 9:14:18 AM
Supervise By	Ankita	Supervise On	11/19/2024 11:25:53 AM
SubDirectory	PO111824	HP Acquire Method	HP Processing Method PO111824
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO108034.D	18 Nov 2024 09:01	YP/AJ	Ok
2	AR1660CCC500	PO108035.D	18 Nov 2024 10:59	YP/AJ	Not Ok
3	HEXANE	PO108036.D	18 Nov 2024 15:00	YP/AJ	Ok
4	I.BLK	PO108037.D	18 Nov 2024 15:16	YP/AJ	Ok
5	AR1660ICC1000	PO108038.D	18 Nov 2024 15:32	YP/AJ	Ok
6	AR1660ICC750	PO108039.D	18 Nov 2024 15:48	YP/AJ	Ok
7	AR1660ICC500	PO108040.D	18 Nov 2024 16:05	YP/AJ	Ok
8	AR1660ICC250	PO108041.D	18 Nov 2024 16:21	YP/AJ	Ok
9	AR1660ICC050	PO108042.D	18 Nov 2024 16:37	YP/AJ	Ok,M
10	AR1221ICC500	PO108043.D	18 Nov 2024 16:53	YP/AJ	Ok
11	AR1232ICC500	PO108044.D	18 Nov 2024 17:09	YP/AJ	Ok
12	AR1242ICC1000	PO108045.D	18 Nov 2024 17:25	YP/AJ	Ok
13	AR1242ICC750	PO108046.D	18 Nov 2024 17:42	YP/AJ	Ok
14	AR1242ICC500	PO108047.D	18 Nov 2024 17:58	YP/AJ	Ok
15	AR1242ICC250	PO108048.D	18 Nov 2024 18:14	YP/AJ	Ok
16	AR1242ICC050	PO108049.D	18 Nov 2024 18:30	YP/AJ	Ok,M
17	AR1248ICC1000	PO108050.D	18 Nov 2024 18:47	YP/AJ	Ok
18	AR1248ICC750	PO108051.D	18 Nov 2024 19:03	YP/AJ	Ok
19	AR1248ICC500	PO108052.D	18 Nov 2024 19:19	YP/AJ	Ok
20	AR1248ICC250	PO108053.D	18 Nov 2024 19:35	YP/AJ	Ok
21	AR1248ICC050	PO108054.D	18 Nov 2024 19:51	YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO111824

Review By	yogesh	Review On	11/19/2024 9:14:18 AM
Supervise By	Ankita	Supervise On	11/19/2024 11:25:53 AM
SubDirectory	PO111824	HP Acquire Method	HP Processing Method PO111824
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	AR1254ICC1000	PO108055.D	18 Nov 2024 20:07	YP/AJ	Ok
23	AR1254ICC750	PO108056.D	18 Nov 2024 20:24	YP/AJ	Ok
24	AR1254ICC500	PO108057.D	18 Nov 2024 20:40	YP/AJ	Ok
25	AR1254ICC250	PO108058.D	18 Nov 2024 20:56	YP/AJ	Ok
26	AR1254ICC050	PO108059.D	18 Nov 2024 21:12	YP/AJ	Ok,M
27	AR1262ICC500	PO108060.D	18 Nov 2024 21:28	YP/AJ	Ok
28	AR1268ICC1000	PO108061.D	18 Nov 2024 21:45	YP/AJ	Ok
29	AR1268ICC750	PO108062.D	18 Nov 2024 22:02	YP/AJ	Ok,M
30	AR1268ICC500	PO108063.D	18 Nov 2024 22:19	YP/AJ	Ok,M
31	AR1268ICC250	PO108064.D	18 Nov 2024 22:35	YP/AJ	Ok
32	AR1268ICC050	PO108065.D	18 Nov 2024 22:51	YP/AJ	Ok
33	PO111824ICV500	PO108066.D	18 Nov 2024 23:08	YP/AJ	Ok
34	AR1242ICV500	PO108067.D	18 Nov 2024 23:24	YP/AJ	Ok
35	AR1248ICV500	PO108068.D	18 Nov 2024 23:41	YP/AJ	Ok
36	AR1254ICV500	PO108069.D	18 Nov 2024 23:58	YP/AJ	Ok
37	AR1268ICV500	PO108070.D	19 Nov 2024 00:14	YP/AJ	Ok,M
38	AR1660CCC500	PO108071.D	19 Nov 2024 00:31	YP/AJ	Ok
39	I.BLK	PO108072.D	19 Nov 2024 00:48	YP/AJ	Ok
40	PB165043BL	PO108073.D	19 Nov 2024 01:04	YP/AJ	Ok
41	PB165043BS	PO108074.D	19 Nov 2024 01:20	YP/AJ	Ok
42	P4860-01	PO108075.D	19 Nov 2024 01:37	YP/AJ	Ok,M
43	P4860-01MS	PO108076.D	19 Nov 2024 01:54	YP/AJ	Ok,M
44	P4860-01MSD	PO108077.D	19 Nov 2024 02:10	YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO111824

Review By	yogesh	Review On	11/19/2024 9:14:18 AM
Supervise By	Ankita	Supervise On	11/19/2024 11:25:53 AM
SubDirectory	PO111824	HP Acquire Method	HP Processing Method PO111824
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

45	P4860-02	PO108078.D	19 Nov 2024 02:26	YP/AJ	Ok,M
46	P4860-03	PO108079.D	19 Nov 2024 02:42	YP/AJ	Ok,M
47	P4860-04	PO108080.D	19 Nov 2024 02:59	YP/AJ	Ok
48	P4860-05	PO108081.D	19 Nov 2024 03:16	YP/AJ	Ok
49	P4860-06	PO108082.D	19 Nov 2024 03:33	YP/AJ	Ok
50	P4860-07	PO108083.D	19 Nov 2024 03:49	YP/AJ	Ok
51	P4860-08	PO108084.D	19 Nov 2024 04:06	YP/AJ	Ok
52	P4860-09	PO108085.D	19 Nov 2024 04:23	YP/AJ	Ok
53	P4860-10	PO108086.D	19 Nov 2024 04:39	YP/AJ	Ok
54	AR1660CCC500	PO108087.D	19 Nov 2024 04:56	YP/AJ	Ok
55	I.BLK	PO108088.D	19 Nov 2024 05:12	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO120224

Review By	yogesh	Review On	12/3/2024 8:42:36 AM
Supervise By	Ankita	Supervise On	12/3/2024 9:04:16 AM
SubDirectory	PO120224	HP Acquire Method	HP Processing Method PO111824
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO108274.D	02 Dec 2024 09:45	YP/AJ	Ok
2	AR1660CCC500	PO108275.D	02 Dec 2024 10:02	YP/AJ	Ok
3	AR1242CCC500	PO108276.D	02 Dec 2024 10:18	YP/AJ	Ok
4	AR1248CCC500	PO108277.D	02 Dec 2024 10:35	YP/AJ	Ok
5	AR1254CCC500	PO108278.D	02 Dec 2024 10:51	YP/AJ	Ok
6	I.BLK	PO108279.D	02 Dec 2024 11:07	YP/AJ	Ok
7	PB165309BL	PO108280.D	02 Dec 2024 12:20	YP/AJ	Ok
8	PB165309BS	PO108281.D	02 Dec 2024 12:37	YP/AJ	Ok
9	P5025-01	PO108282.D	02 Dec 2024 12:53	YP/AJ	Ok,M
10	P5025-05	PO108283.D	02 Dec 2024 13:09	YP/AJ	Ok
11	P5026-01	PO108284.D	02 Dec 2024 13:26	YP/AJ	Ok,M
12	P5026-05	PO108285.D	02 Dec 2024 13:43	YP/AJ	Ok
13	P5026-05MS	PO108286.D	02 Dec 2024 14:00	YP/AJ	Ok
14	P5026-05MSD	PO108287.D	02 Dec 2024 14:16	YP/AJ	Ok
15	P5045-01	PO108288.D	02 Dec 2024 14:33	YP/AJ	Ok,M
16	P5046-01	PO108289.D	02 Dec 2024 14:49	YP/AJ	Ok
17	AR1660CCC500	PO108290.D	02 Dec 2024 15:36	YP/AJ	Ok
18	AR1242CCC500	PO108291.D	02 Dec 2024 16:21	YP/AJ	Ok,M
19	AR1248CCC500	PO108292.D	02 Dec 2024 16:38	YP/AJ	Ok
20	AR1254CCC500	PO108293.D	02 Dec 2024 16:54	YP/AJ	Ok
21	I.BLK	PO108294.D	02 Dec 2024 17:11	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO120224

Review By	yogesh	Review On	12/3/2024 8:42:36 AM
Supervise By	Ankita	Supervise On	12/3/2024 9:04:16 AM
SubDirectory	PO120224	HP Acquire Method	HP Processing Method PO111824
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	P5048-01	PO108295.D	02 Dec 2024 17:27	YP/AJ	Ok,M
23	PB165315BL	PO108296.D	02 Dec 2024 17:44	YP/AJ	Ok
24	PB165315BS	PO108297.D	02 Dec 2024 18:00	YP/AJ	Ok
25	PB165315BSD	PO108298.D	02 Dec 2024 18:16	YP/AJ	Ok
26	P5031-01	PO108299.D	02 Dec 2024 18:33	YP/AJ	Ok
27	AR1660CCC500	PO108300.D	02 Dec 2024 19:19	YP/AJ	Ok
28	AR1242CCC500	PO108301.D	02 Dec 2024 19:35	YP/AJ	Ok
29	AR1248CCC500	PO108302.D	02 Dec 2024 19:52	YP/AJ	Ok
30	AR1254CCC500	PO108303.D	02 Dec 2024 20:08	YP/AJ	Ok
31	I.BLK	PO108304.D	02 Dec 2024 20:24	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO111824

Review By	yogesh	Review On	11/19/2024 9:14:18 AM
Supervise By	Ankita	Supervise On	11/19/2024 11:25:53 AM
SubDirectory	PO111824	HP Acquire Method	HP Processing Method PO111824

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773
Internal Standard/PEM	
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO108034.D	18 Nov 2024 09:01		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO108035.D	18 Nov 2024 10:59		YP/AJ	Not Ok
3	HEXANE	HEXANE	PO108036.D	18 Nov 2024 15:00		YP/AJ	Ok
4	I.BLK	I.BLK	PO108037.D	18 Nov 2024 15:16		YP/AJ	Ok
5	AR1660ICC1000	AR1660ICC1000	PO108038.D	18 Nov 2024 15:32		YP/AJ	Ok
6	AR1660ICC750	AR1660ICC750	PO108039.D	18 Nov 2024 15:48		YP/AJ	Ok
7	AR1660ICC500	AR1660ICC500	PO108040.D	18 Nov 2024 16:05		YP/AJ	Ok
8	AR1660ICC250	AR1660ICC250	PO108041.D	18 Nov 2024 16:21		YP/AJ	Ok
9	AR1660ICC050	AR1660ICC050	PO108042.D	18 Nov 2024 16:37		YP/AJ	Ok,M
10	AR1221ICC500	AR1221ICC500	PO108043.D	18 Nov 2024 16:53		YP/AJ	Ok
11	AR1232ICC500	AR1232ICC500	PO108044.D	18 Nov 2024 17:09		YP/AJ	Ok
12	AR1242ICC1000	AR1242ICC1000	PO108045.D	18 Nov 2024 17:25		YP/AJ	Ok
13	AR1242ICC750	AR1242ICC750	PO108046.D	18 Nov 2024 17:42		YP/AJ	Ok
14	AR1242ICC500	AR1242ICC500	PO108047.D	18 Nov 2024 17:58		YP/AJ	Ok
15	AR1242ICC250	AR1242ICC250	PO108048.D	18 Nov 2024 18:14		YP/AJ	Ok
16	AR1242ICC050	AR1242ICC050	PO108049.D	18 Nov 2024 18:30		YP/AJ	Ok,M
17	AR1248ICC1000	AR1248ICC1000	PO108050.D	18 Nov 2024 18:47		YP/AJ	Ok
18	AR1248ICC750	AR1248ICC750	PO108051.D	18 Nov 2024 19:03		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO111824

Review By	yogesh	Review On	11/19/2024 9:14:18 AM
Supervise By	Ankita	Supervise On	11/19/2024 11:25:53 AM
SubDirectory	PO111824	HP Acquire Method	HP Processing Method PO111824
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248ICC500	AR1248ICC500	PO108052.D	18 Nov 2024 19:19		YP/AJ	Ok
20	AR1248ICC250	AR1248ICC250	PO108053.D	18 Nov 2024 19:35		YP/AJ	Ok
21	AR1248ICC050	AR1248ICC050	PO108054.D	18 Nov 2024 19:51		YP/AJ	Ok,M
22	AR1254ICC1000	AR1254ICC1000	PO108055.D	18 Nov 2024 20:07		YP/AJ	Ok
23	AR1254ICC750	AR1254ICC750	PO108056.D	18 Nov 2024 20:24		YP/AJ	Ok
24	AR1254ICC500	AR1254ICC500	PO108057.D	18 Nov 2024 20:40		YP/AJ	Ok
25	AR1254ICC250	AR1254ICC250	PO108058.D	18 Nov 2024 20:56		YP/AJ	Ok
26	AR1254ICC050	AR1254ICC050	PO108059.D	18 Nov 2024 21:12		YP/AJ	Ok,M
27	AR1262ICC500	AR1262ICC500	PO108060.D	18 Nov 2024 21:28		YP/AJ	Ok
28	AR1268ICC1000	AR1268ICC1000	PO108061.D	18 Nov 2024 21:45		YP/AJ	Ok
29	AR1268ICC750	AR1268ICC750	PO108062.D	18 Nov 2024 22:02		YP/AJ	Ok,M
30	AR1268ICC500	AR1268ICC500	PO108063.D	18 Nov 2024 22:19		YP/AJ	Ok,M
31	AR1268ICC250	AR1268ICC250	PO108064.D	18 Nov 2024 22:35		YP/AJ	Ok
32	AR1268ICC050	AR1268ICC050	PO108065.D	18 Nov 2024 22:51		YP/AJ	Ok
33	PO111824ICV500	ICVPO111824	PO108066.D	18 Nov 2024 23:08		YP/AJ	Ok
34	AR1242ICV500	ICVPO111824AR1242	PO108067.D	18 Nov 2024 23:24		YP/AJ	Ok
35	AR1248ICV500	ICVPO111824AR1248	PO108068.D	18 Nov 2024 23:41		YP/AJ	Ok
36	AR1254ICV500	ICVPO111824AR1254	PO108069.D	18 Nov 2024 23:58		YP/AJ	Ok
37	AR1268ICV500	ICVPO111824AR1268	PO108070.D	19 Nov 2024 00:14		YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO111824

Review By	yogesh	Review On	11/19/2024 9:14:18 AM
Supervise By	Ankita	Supervise On	11/19/2024 11:25:53 AM
SubDirectory	PO111824	HP Acquire Method	HP Processing Method PO111824
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

38	AR1660CCC500	AR1660CCC500	PO108071.D	19 Nov 2024 00:31		YP/AJ	Ok
39	I.BLK	I.BLK	PO108072.D	19 Nov 2024 00:48		YP/AJ	Ok
40	PB165043BL	PB165043BL	PO108073.D	19 Nov 2024 01:04		YP/AJ	Ok
41	PB165043BS	PB165043BS	PO108074.D	19 Nov 2024 01:20		YP/AJ	Ok
42	P4860-01	DUP-01	PO108075.D	19 Nov 2024 01:37		YP/AJ	Ok,M
43	P4860-01MS	DUP-01MS	PO108076.D	19 Nov 2024 01:54		YP/AJ	Ok,M
44	P4860-01MSD	DUP-01MSD	PO108077.D	19 Nov 2024 02:10		YP/AJ	Ok,M
45	P4860-02	PH2-BOT-001	PO108078.D	19 Nov 2024 02:26		YP/AJ	Ok,M
46	P4860-03	PH2-BOT-002	PO108079.D	19 Nov 2024 02:42		YP/AJ	Ok,M
47	P4860-04	PH2-BOT-003	PO108080.D	19 Nov 2024 02:59		YP/AJ	Ok
48	P4860-05	PH2-BOT-004	PO108081.D	19 Nov 2024 03:16		YP/AJ	Ok
49	P4860-06	PH2-BOT-009	PO108082.D	19 Nov 2024 03:33		YP/AJ	Ok
50	P4860-07	PH2-BOT-008	PO108083.D	19 Nov 2024 03:49		YP/AJ	Ok
51	P4860-08	PH2-BOT-007	PO108084.D	19 Nov 2024 04:06		YP/AJ	Ok
52	P4860-09	PH2-BOT-006	PO108085.D	19 Nov 2024 04:23		YP/AJ	Ok
53	P4860-10	PH2-BOT-005	PO108086.D	19 Nov 2024 04:39		YP/AJ	Ok
54	AR1660CCC500	AR1660CCC500	PO108087.D	19 Nov 2024 04:56		YP/AJ	Ok
55	I.BLK	I.BLK	PO108088.D	19 Nov 2024 05:12		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO120224

Review By	yogesh	Review On	12/3/2024 8:42:36 AM
Supervise By	Ankita	Supervise On	12/3/2024 9:04:16 AM
SubDirectory	PO120224	HP Acquire Method	HP Processing Method PO111824
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO108274.D	02 Dec 2024 09:45		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO108275.D	02 Dec 2024 10:02		YP/AJ	Ok
3	AR1242CCC500	AR1242CCC500	PO108276.D	02 Dec 2024 10:18		YP/AJ	Ok
4	AR1248CCC500	AR1248CCC500	PO108277.D	02 Dec 2024 10:35		YP/AJ	Ok
5	AR1254CCC500	AR1254CCC500	PO108278.D	02 Dec 2024 10:51		YP/AJ	Ok
6	I.BLK	I.BLK	PO108279.D	02 Dec 2024 11:07		YP/AJ	Ok
7	PB165309BL	PB165309BL	PO108280.D	02 Dec 2024 12:20		YP/AJ	Ok
8	PB165309BS	PB165309BS	PO108281.D	02 Dec 2024 12:37		YP/AJ	Ok
9	P5025-01	SOIL-WEST	PO108282.D	02 Dec 2024 12:53		YP/AJ	Ok,M
10	P5025-05	SOIL-EAST	PO108283.D	02 Dec 2024 13:09		YP/AJ	Ok
11	P5026-01	SOIL-1-HAM	PO108284.D	02 Dec 2024 13:26		YP/AJ	Ok,M
12	P5026-05	SOIL-1-HAM	PO108285.D	02 Dec 2024 13:43		YP/AJ	Ok
13	P5026-05MS	SOIL-1-HAMMS	PO108286.D	02 Dec 2024 14:00		YP/AJ	Ok
14	P5026-05MSD	SOIL-1-HAMMSD	PO108287.D	02 Dec 2024 14:16		YP/AJ	Ok
15	P5045-01	SU-04-11222024	PO108288.D	02 Dec 2024 14:33		YP/AJ	Ok,M
16	P5046-01	HD-01-11272024	PO108289.D	02 Dec 2024 14:49		YP/AJ	Ok
17	AR1660CCC500	AR1660CCC500	PO108290.D	02 Dec 2024 15:36		YP/AJ	Ok
18	AR1242CCC500	AR1242CCC500	PO108291.D	02 Dec 2024 16:21		YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO120224

Review By	yogesh	Review On	12/3/2024 8:42:36 AM
Supervise By	Ankita	Supervise On	12/3/2024 9:04:16 AM
SubDirectory	PO120224	HP Acquire Method	HP Processing Method PO111824
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248CCC500	AR1248CCC500	PO108292.D	02 Dec 2024 16:38		YP/AJ	Ok
20	AR1254CCC500	AR1254CCC500	PO108293.D	02 Dec 2024 16:54		YP/AJ	Ok
21	I.BLK	I.BLK	PO108294.D	02 Dec 2024 17:11		YP/AJ	Ok
22	P5048-01	MH-746-WC	PO108295.D	02 Dec 2024 17:27		YP/AJ	Ok,M
23	PB165315BL	PB165315BL	PO108296.D	02 Dec 2024 17:44		YP/AJ	Ok
24	PB165315BS	PB165315BS	PO108297.D	02 Dec 2024 18:00		YP/AJ	Ok
25	PB165315BSD	PB165315BSD	PO108298.D	02 Dec 2024 18:16		YP/AJ	Ok
26	P5031-01	286127	PO108299.D	02 Dec 2024 18:33		YP/AJ	Ok
27	AR1660CCC500	AR1660CCC500	PO108300.D	02 Dec 2024 19:19		YP/AJ	Ok
28	AR1242CCC500	AR1242CCC500	PO108301.D	02 Dec 2024 19:35		YP/AJ	Ok
29	AR1248CCC500	AR1248CCC500	PO108302.D	02 Dec 2024 19:52		YP/AJ	Ok
30	AR1254CCC500	AR1254CCC500	PO108303.D	02 Dec 2024 20:08		YP/AJ	Ok
31	I.BLK	I.BLK	PO108304.D	02 Dec 2024 20:24		YP/AJ	Ok

M : Manual Integration



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 12/2/2024

OVENTEMP IN Celsius(°C): 107
Time IN: 17:15
In Date: 11/27/2024
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 103
Time OUT: 08:15
Out Date: 11/28/2024
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID- OVEN

QC:LB133667

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
P5022-01	TAPIAL2-SB02D-13-11242 4-00-T1	1	1.15	8.70	9.85	9.23	92.9	
P5025-01	SOIL-WEST	2	1.18	8.43	9.61	8.41	85.8	
P5025-03	SOIL-WEST-TPH2	3	1.17	8.60	9.77	8.54	85.7	
P5025-04	SOIL-WEST-GRAB	4	1.16	8.49	9.65	8.43	85.6	
P5025-05	SOIL-EAST	5	1.15	8.73	9.88	7.85	76.7	
P5025-07	SOIL-EAST-TPH2	6	1.11	8.70	9.81	7.76	76.4	
P5025-08	SOIL-EAST-GRAB	7	1.15	8.82	9.97	9.39	93.4	
P5026-01	SOIL-1-HAM	8	1.13	8.65	9.78	8.00	79.4	
P5026-03	SOIL-1-HAM-TPH2	9	1.17	8.50	9.67	8.72	88.8	
P5026-04	SOIL-1-HAM-GRAB	10	1.18	8.42	9.6	8.66	88.8	
P5026-05	SOIL-1-HAM	11	1.15	8.81	9.96	8.00	77.8	
P5026-07	SOIL-1-HAM-TPH2	12	1.19	8.50	9.69	7.51	74.4	
P5026-08	SOIL-1-HAM-GRAB	13	1.14	8.75	9.89	7.7	75.0	
P5045-01	SU-04-11222024	14	1.19	8.50	9.69	8.96	91.4	
P5045-02	SU-04-11222024-E2	15	1.13	8.74	9.87	8.49	84.2	
P5046-01	HD-01-11272024	16	1.17	8.57	9.74	8.8	89.0	
P5046-02	HD-01-11272024-E2	17	1.16	8.83	9.99	9.00	88.8	
P5048-01	MH-746-WC	18	1.17	8.65	9.82	9.18	92.6	
P5048-02	MH-746-EPH	19	1.15	8.80	9.95	8.91	88.2	
P5048-03	MH-746--VOC	20	1.15	8.36	9.51	8.48	87.7	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

133667

WorkList Name : %1-112724

WorkList ID : 185820

Department : Wet-Chemistry

Date : 11-27-2024 08:06:01

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P5022-01	TAPIAL2-SB02D-13-112424-00.	Solid	Percent Solids	Cool 4 deg C	WEST04	L41	11/24/2024	Chemtech -SO
P5025-01	SOIL-WEST	Solid	Percent Solids	Cool 4 deg C	TULL02	L61	11/27/2024	Chemtech -SO
P5025-03	SOIL-WEST-TPH2	Solid	Percent Solids	Cool 4 deg C	TULL02	L61	11/27/2024	Chemtech -SO
P5025-04	SOIL-WEST-GRAB	Solid	Percent Solids	Cool 4 deg C	TULL02	L61	11/27/2024	Chemtech -SO
P5025-05	SOIL-EAST	Solid	Percent Solids	Cool 4 deg C	TULL02	L61	11/27/2024	Chemtech -SO
P5025-07	SOIL-EAST-TPH2	Solid	Percent Solids	Cool 4 deg C	TULL02	L61	11/27/2024	Chemtech -SO
P5025-08	SOIL-EAST-GRAB	Solid	Percent Solids	Cool 4 deg C	TULL02	L61	11/27/2024	Chemtech -SO
P5026-01	SOIL-1-HAM	Solid	Percent Solids	Cool 4 deg C	TULL02	L61	11/27/2024	Chemtech -SO
P5026-03	SOIL-1-HAM-TPH2	Solid	Percent Solids	Cool 4 deg C	TULL02	L61	11/27/2024	Chemtech -SO
P5026-04	SOIL-1-HAM-GRAB	Solid	Percent Solids	Cool 4 deg C	TULL02	L61	11/27/2024	Chemtech -SO
P5026-05	SOIL-1-HAM	Solid	Percent Solids	Cool 4 deg C	TULL02	L61	11/27/2024	Chemtech -SO
P5026-07	SOIL-1-HAM-TPH2	Solid	Percent Solids	Cool 4 deg C	TULL02	L61	11/27/2024	Chemtech -SO
P5026-08	SOIL-1-HAM-GRAB	Solid	Percent Solids	Cool 4 deg C	TULL02	L61	11/27/2024	Chemtech -SO
P5045-01	SU-04-11222024	Solid	Percent Solids	Cool 4 deg C	PSEG05	L51	11/27/2024	Chemtech -SO
P5045-02	SU-04-11222024-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	L51	11/27/2024	Chemtech -SO
P5046-01	HD-01-11272024	Solid	Percent Solids	Cool 4 deg C	PSEG05	L51	11/27/2024	Chemtech -SO
P5046-02	HD-01-11272024-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	L51	11/27/2024	Chemtech -SO
P5048-01	MH-746-WC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L61	11/27/2024	Chemtech -SO
P5048-02	MH-746-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	L61	11/27/2024	Chemtech -SO
P5048-03	MH-746-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	L61	11/27/2024	Chemtech -SO

Date/Time 11/27/24 16:10

Raw Sample Received by: go woc

Raw Sample Relinquished by: [Signature]

Date/Time 11/27/24

Raw Sample Received by: [Signature]

Raw Sample Relinquished by: go woc

SOP ID: M3541-ASE Extraction-14

Clean Up SOP #: Acid Cleanup

Matrix : Solid

Weigh By: RJ **Extraction By:** RJ

Balance check: RJ **Filter By:** RJ

Balance ID: EX-SC-2 **pH Meter ID:** N/A

pH Strip Lot#: N/A **Hood ID:** 3,7

Extraction Start Date : 12/02/2024

Extraction Start Time : 08:20

Extraction End Date : 12/02/2024

Extraction End Time : 11:30

Concentration By: EH

Supervisor By : rajesh

Extraction Method: ☐ Separatory Funnel ☐ Continuous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☒ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP23913
Surrogate	1.0ML	200 PPB	PP23985
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Hexane	N/A	E3826
Baked Na2SO4	N/A	EP2566
H2SO4 1:1	N/A	EP2565
Sand	N/A	E2865
Hexane/Acetone/1:1	N/A	EP2561
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40 ML Vial lot# 03-40BTS721.

KD Bath ID: N/A **Envap ID:** NEVAP-02

KD Bath Temperature: N/A **Envap Temperature:** 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
12/2/24	Rp (Ext 104)	Y.P. pest-PCB.
11:35	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-14

Concentration Date: 12/02/2024

Sample ID	Client Sample ID	Test	g/mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB165309BL	ABLK309	PCB	30.02	N/A	ritesh	Evelyn	10			U7-1
PB165309BS	ALCS309	PCB	30.01	N/A	ritesh	Evelyn	10			2
P5025-01	SOIL-WEST	PCB	30.06	N/A	ritesh	Evelyn	10	D		3
P5025-05	SOIL-EAST	PCB	30.02	N/A	ritesh	Evelyn	10	D		4
P5026-01	SOIL-1-HAM	PCB	30.05	N/A	ritesh	Evelyn	10	D		5
P5026-05	SOIL-1-HAM	PCB	30.03	N/A	ritesh	Evelyn	10	E		6
P5026-05MS	SOIL-1-HAMMS	PCB	30.01	N/A	ritesh	Evelyn	10	E		U6-1
P5026-05MS D	SOIL-1-HAMMSD	PCB	30.06	N/A	ritesh	Evelyn	10	E		2
P5045-01	SU-04-11222024	PCB	30.08	N/A	ritesh	Evelyn	10	E		3
P5046-01	HD-01-11272024	PCB	30.04	N/A	ritesh	Evelyn	10	D		4
P5048-01	MH-746-WC	PCB	30.03	N/A	ritesh	Evelyn	10	D		5

* Extracts relinquished on the same date as received.

12/2/24

11/26/24

WORKLIST(Hardcopy Internal Chain)

WorkList Name : P5025 WorkList ID : 185872 Department : Extraction Date : 12-02-2024 08:13:17

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P5025-01	SOIL-WEST	Solid	PCB	Cool 4 deg C	TULL02	L61	11/27/2024	8082A
P5025-05	SOIL-EAST	Solid	PCB	Cool 4 deg C	TULL02	L61	11/27/2024	8082A
P5026-01	SOIL-1-HAM	Solid	PCB	Cool 4 deg C	TULL02	L61	11/27/2024	8082A
P5026-05	SOIL-1-HAM	Solid	PCB	Cool 4 deg C	TULL02	L61	11/27/2024	8082A
P5045-01	SU-04-11222024	Solid	PCB	Cool 4 deg C	PSEG05	L51	11/27/2024	8082A
P5046-01	HD-01-11272024	Solid	PCB	Cool 4 deg C	PSEG05	L51	11/27/2024	8082A
P5048-01	MH-746-WC	Solid	PCB	Cool 4 deg C	PSEG03	L61	11/27/2024	8082A

Date/Time 12/2/24 8:15
Raw Sample Received by: RJ (Ed 10/21) Of 6
Raw Sample Relinquished by: Of 6

Date/Time 12/2/24 8:45
Raw Sample Received by: Of 5
Raw Sample Relinquished by: RJ (Ed 10/21)

Prep Standard - Chemical Standard Summary

Order ID : P5026

Test : PCB

Prepbatch ID : PB165309,

Sequence ID/Qc Batch ID: PO120224,

Standard ID :

EP2561,EP2565,EP2566,PP23733,PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775,PP23776,PP23777,PP23778,PP23779,PP23780,PP23781,PP23782,PP23783,PP23784,PP23785,PP23786,PP23787,PP23788,PP23789,PP23790,PP23913,PP23946,PP23947,PP23985,

Chemical ID :

E2865,E3551,E3804,E3805,E3822,E3825,E3826,E3827,M5173,P10483,P10500,P11507,P11512,P11521,P11581,P11587,P11590,P11597,P12698,P12929,P12934,P12947,P12957,P13033,P13104,P13109,P13350,P13352,P13372,W3112,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	EP2561	11/14/2024	05/08/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 11/14/2024

FROM 8000.00000ml of E3826 + 8000.00000ml of E3827 = Final Quantity: 8000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2565	11/20/2024	05/20/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 11/20/2024

FROM 1000.00000ml of M5173 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2566	11/22/2024	01/03/2025	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	Evelyn Huang 11/22/2024
<u>FROM</u> 4000.00000gram of E3551 = Final Quantity: 4000.000 gram								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP23733	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel 10/03/2024
<u>FROM</u> 1.00000ml of P13350 + 9.00000ml of E3805 = Final Quantity: 10.000 ml								

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
202	AR1660 1000/100 ppb working solution 1st source	PP23735	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P10483 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
203	AR1660 750 PPB STD	PP23736	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23735 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
204	AR1660 500 PPB STD	PP23737	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23735 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
205	AR1660 250 PPB STD	PP23738	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23735 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
206	AR1660 50 PPB STD	PP23739	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23737 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
213	AR1221 1000 PPB WORKING SOLUTION	PP23740	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11581 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1079	AR1221 750 PPB STD	PP23741	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23740 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
222	AR1221 500 PPB STD	PP23742	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23740 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1080	AR1221 250 PPB STD	PP23743	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23740 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1081	AR1221 50 PPB STD	PP23744	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23742 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
214	AR1232 1000 PPB WORKING SOLUTION	PP23745	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11587 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1063	AR1232 750 PPB STD	PP23747	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23745 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
223	AR1232 500 PPB STD	PP23748	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23745 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1064	AR1232 250 PPB STD	PP23749	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23745 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1065	AR1232 50 PPB STD	PP23750	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23748 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
215	AR1242 1000 PPB WORKING STD	PP23751	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P12929 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1067	AR1242 750 PPB STD	PP23752	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23751 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
224	AR1242 500 PPB STD	PP23753	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23751 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1068	AR1242 250 PPB STD	PP23754	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23751 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1069	AR1242 50 PPB STD	PP23755	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23753 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
216	AR1248 1000 PPB WORKING STD	PP23756	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P12934 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1075	AR1248 750 PPB STD	PP23757	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23756 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
225	AR1248 500 PPB STD	PP23758	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23756 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1076	AR1248 250 PPB STD	PP23759	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23756 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1077	AR1248 50 PPB STD	PP23760	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23758 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
217	AR1254 1000 PPB WORKING STD	PP23761	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11590 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1071	AR1254 750 PPB STD	PP23762	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23761 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
226	AR1254 500 PPB STD	PP23763	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23761 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1072	AR1254 250 PPB STD	PP23764	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23761 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1073	AR1254 50 PPB STD	PP23765	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23763 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1529	AR1262 1000 PPB Working Solution	PP23766	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P10500 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3753	AR1262 750 PPB STD	PP23767	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23766 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1530	AR1262 500 PPB STD	PP23768	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23766 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3754	AR1262 250 PPB STD	PP23769	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23766 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3755	AR1262 50 PPB STD	PP23770	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23768 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1532	AR1268 1000 PPB Working Solution	PP23771	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11597 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3820	AR1268 750 PPB STD	PP23772	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23771 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1533	AR1268 500 PPB STD	PP23773	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23771 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3821	AR1268 250 PPB STD	PP23774	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23771 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3822	AR1268 50 PPB STD	PP23775	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23773 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
404	AR1660 100 PPM Stock Solution 2nd Source	PP23776	10/03/2024	04/01/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12947 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
405	AR1660 1000/100 PPB ICV STD	PP23777	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 98.50000ml of E3805 + 0.50000ml of PP23733 + 1.00000ml of PP23776 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
406	AR1660 500 PPB ICV	PP23778	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23777 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3789	AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT)	PP23779	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P13372 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3790	AR1221 500 PPB ICV(AGILENT)	PP23780	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23779 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1887	AR1232 1000 PPB Working Sol. 2nd Source	PP23781	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12698 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1889	AR1242 1000 PPB Working Sol. 2nd Source	PP23782	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel 10/03/2024

FROM 1.00000ml of P11507 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1888	AR1232 500 PPB ICV	PP23783	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel 10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23781 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1891	AR1242 500 PPB ICV	PP23784	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23782 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1890	AR1248 1000 PPB Working Sol. 2nd Source	PP23785	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11512 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1892	AR1248 500 PPB ICV	PP23786	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23785 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1893	AR1254 1000 PPB Working Sol. 2nd Source	PP23787	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12957 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1894	AR1254 500 PPB ICV	PP23788	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23787 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3757	AR1262 1000 PPB Working Solution second source	PP23789	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P13033 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3758	AR1262 500 PPB STD ICV	PP23790	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23789 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3609	20 PPM DRO SPIKE SOLUTION (RESTEK)	PP23913	10/25/2024	04/23/2025	Yogesh Patel	None	None	Ankita Jodhani
								10/25/2024

FROM 1.00000ml of P13104 + 1.00000ml of P13109 + 48.00000ml of E3822 = Final Quantity: 50.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3817	AR1268 1000 ppb Working Soln. 2nd source	PP23946	11/07/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								11/13/2024

FROM 1.00000ml of P11521 + 98.50000ml of E3825 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3823	AR1268 500 PPB STD ICV	PP23947	11/07/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								11/13/2024

FROM 0.50000ml of E3825 + 0.50000ml of PP23946 = Final Quantity: 1.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP23985	11/15/2024	05/08/2025	Ankita Jodhani	None	None	Yogesh Patel
<u>FROM</u> 1.00000ml of P13352 + 999.00000ml of E3827 = Final Quantity: 1000.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	12/31/2024	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	01/03/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	11/05/2025	10/01/2024 / Rajesh	09/25/2024 / Rajesh	E3804

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	03/30/2025	09/30/2024 / Rajesh	09/25/2024 / Rajesh	E3805

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24I2662006	04/23/2025	10/24/2024 / Rajesh	10/24/2024 / Rajesh	E3822

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	11/06/2025	11/06/2024 / Rajesh	11/01/2024 / Rajesh	E3825

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	05/09/2025	11/09/2024 / Rajesh	11/07/2024 / Rajesh	E3826

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	05/08/2025	11/08/2024 / Rajesh	11/07/2024 / Rajesh	E3827

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	0000281827	06/02/2025	06/01/2022 /	04/05/2022 / william	M5173

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul	A0163157	04/03/2025	10/03/2024 / Ankita	03/19/2021 / Abdul	P10483

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane	A0167722	04/03/2025	10/03/2024 / Ankita	03/19/2021 / Ankita	P10500

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-312-1 / Aroclor 1242	0006665550	04/03/2025	10/03/2024 / Ankita	02/21/2022 / Ankita	P11507

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-342-1 / Aroclor 1248	0006626997	04/03/2025	10/03/2024 / Ankita	02/21/2022 / Ankita	P11512

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-382-1 / Aroclor 1268	0006587800	05/07/2025	11/07/2024 / Ankita	02/21/2022 / Ankita	P11521

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul	A0175456	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11581

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul	A0173309	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11587

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	A0175403	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11590

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane	A0181782	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11597

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	91867 / Aroclor 1232 100 ug/mL	020823	04/03/2025	10/03/2024 / Ankita	08/07/2023 / Ankita	P12698

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul	a0203672	04/03/2025	10/03/2024 / Ankita	12/07/2023 / Ankita	P12929

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul	a0202803	04/03/2025	10/03/2024 / Ankita	12/07/2023 / Ankita	P12934

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12947

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ Aroclor 1254	121823	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12957

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	90165 / Aroclor 1262	112322	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P13033

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0204859	04/25/2025	10/25/2024 / yogesh	01/12/2024 / Yogesh	P13104

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0204859	04/25/2025	10/25/2024 / yogesh	01/12/2024 / Yogesh	P13109

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	04/03/2025	10/03/2024 / Ankita	04/22/2024 / Abdul	P13350

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	05/15/2025	11/15/2024 / Ankita	04/22/2024 / Abdul	P13352

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-292-1 / Aroclor 1221	0006783205	04/03/2025	10/03/2024 / Ankita	05/02/2024 / Ankita	P13372

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1


Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865

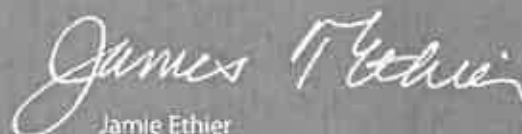
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use

Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC



Michelle Bales
Sr. Manager, Quality Assurance

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

avantor™



Material No.: 9262-03
Batch No.: 24C1862008
Manufactured Date: 2024-01-30
Expiration Date: 2025-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.4 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 9/25/24

E 3805

Jamie Croak
Director Quality Operations, Bioscience Production

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4

Batch No.: 24I2662006

Manufactured Date: 2024-08-29

Expiration Date: 2025-11-28

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	3
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	99.9 %
Color (APHA)	≤ 10	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.2 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	$< 5 \text{ ppm}$
Water (by KF, coulometric)	$\leq 0.02 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3822

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

£3825

Jamie Croak
Director Quality Operations, Bioscience Production

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3826

Rec'd by RP on 11/7/24

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone

BAKER RESI-ANALYZED® Reagent

For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3827

Recd. by RS on ~~11/8/24~~ 11/7/24
RS
11/7

Jamie Croak

Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Hydrochloric Acid, 36.5–38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis



Material No.: 9530-33
Batch No.: 0000281827
Manufactured Date: 2021/03/30
Retest Date: 2026/03/29
Revision No: 1

Certificate of Analysis

Test	Specification	Result
ACS – Assay (as HCl) (by acid–base titrn)	36.5 – 38.0 %	37.6
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	1
ACS – Specific Gravity at 60°/60°F	1.185 – 1.192	1.189
ACS – Bromide (Br)	<= 0.005 %	< 0.005
ACS – Extractable Organic Substances	<= 5 ppm	< 1
ACS – Free Chlorine (as Cl ₂)	<= 0.5 ppm	< 0.5
Phosphate (PO ₄)	<= 0.05 ppm	< 0.03
Sulfate (SO ₄)	<= 0.5 ppm	< 0.3
Sulfite (SO ₃)	<= 0.8 ppm	0.3
Ammonium (NH ₄)	<= 3 ppm	< 1
Trace Impurities – Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities – Aluminum (Al)	<= 10.0 ppb	0.5
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities – Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities – Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities – Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities – Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities – Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities – Calcium (Ca)	<= 50.0 ppb	15.0
Trace Impurities – Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities – Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities – Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities – Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	3.0
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	1.0
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	< 0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	< 0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.2
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	18.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	< 0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.4
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use

Product Information (not specifications):

Appearance (clear, fuming liquid)

Meets ACS Specifications

Country of Origin: US

Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32039 Lot No.: A0163157
Description : Aroclor® 1016/1260 Mix
Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2026 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1016 CAS # 12674-11-2 (Lot 04) Purity ----%	1,007.0 µg/mL	+/- 5.8683 µg/mL Gravimetric +/- 31.9082 µg/mL Unstressed +/- 41.6868 µg/mL Stressed
2	Aroclor 1260 CAS # 11096-82-5 (Lot 07) Purity ----%	1,008.0 µg/mL	+/- 5.8741 µg/mL Gravimetric +/- 31.9399 µg/mL Unstressed +/- 41.7282 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 10476

P 10480

AR
02/19/21

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

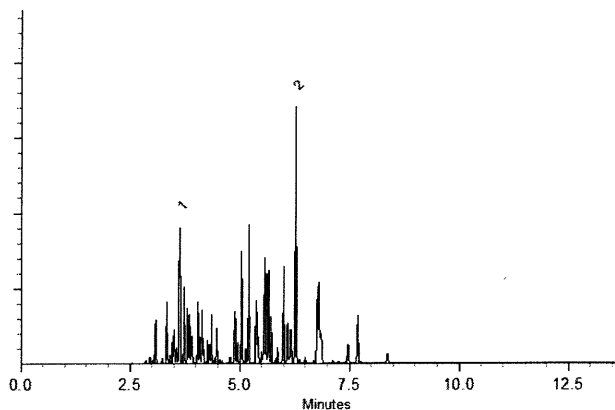

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar - Mix Technician

Date Mixed: 03-Aug-2020

Balance: B442140311

Justine Albertson - Operations Tech-ARM QC

Date Passed: 05-Aug-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32409 Lot No.: A0167722
Description : Aroclor® 1262 Standard
Aroclor® 1262 Standard 1,000 µg/mL, 1mL/ampul, Hexane
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : April 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1262	1,004.0 µg/mL	+/- 5.9635 µg/mL Gravimetric
	CAS # 37324-23-5 (Lot 10849100)		+/- 31.8340 µg/mL Unstressed
	Purity ----%		+/- 41.5787 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P10496
↓
P10500

AJ
09/19/21

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

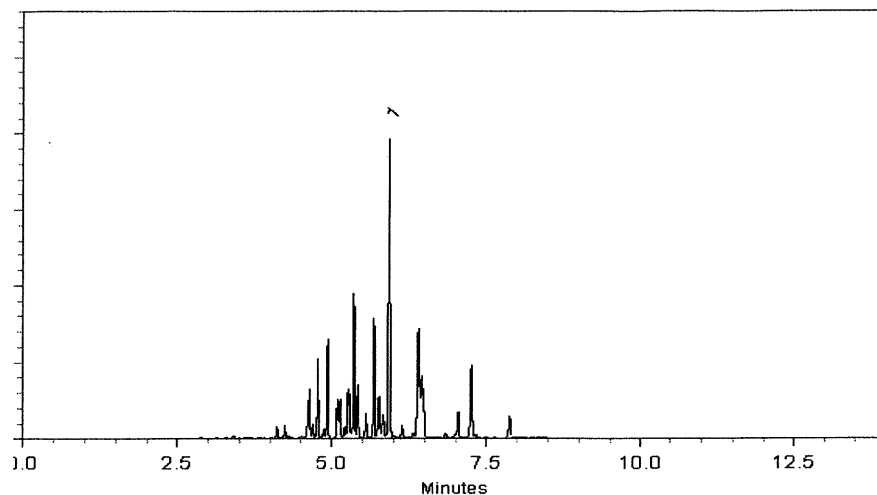

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 03-Jan-2021


Balance: B707717271

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 05-Jan-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1242 Standard

Lot Number: 0006665550

Product Number: PP-312-1

Lot Issue Date: 08-Feb-2022

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 31-Jan-2027

Component Name	CERTIFIED VALUES			CAS#	Analyte Lot
	Concentration	Expanded Uncertainty			
Aroclor 1242	100.4	± 0.5 µg/mL		053469-21-9	NT01020

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P11503
↓
P11507A7
02/21/22

Page: 1 of 2

CSD-QA-015.1

ISO 17034



Agilent

Trusted Answers

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2


www.agilent.com/quality/

CSD-QA-015.1



ISO 17025
Cert No. AT-

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1248 Standard

Lot Number: 0006626997

Product Number: PP-342-1

Lot Issue Date: 17-Aug-2021

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 30-Sep-2025

Component Name	CERTIFIED VALUES		CAS#	Analyte Lot
	Concentration	Expanded Uncertainty		
Aroclor 1248	100.3	± 0.5 µg/mL	012672-29-6	NT01582

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P11508


↓

P11512

AJ

2/21/22

ISO 17034



Agilent

Trusted Answers

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



Certificate of Analysis

P11518
↓
P11522
AJ
02/21/22

Product Name: Aroclor 1268 Standard

Product Number: PP-382-1

Lot Issue Date: 09-Feb-2021

Lot Number: 0006587800

Expiration Date: 31-Mar-2029

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration ± Uncertainty
Aroclor 1268	011100-14-4	RM00937	100.0 ± 0.5 µg/mL

Matrix: isooctane (2,2,4-trimethylpentane)

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.


Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026
Page: 1 of 1

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32007 Lot No.: A0175456
Description : Aroclor® 1221 Standard
Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1221	1,002.0 µg/mL	+/- 5.9516 µg/mL Gravimetric
	CAS # 11104-28-2 (Lot 10210500)		+/- 31.7706 µg/mL Unstressed
	Purity ----%		+/- 41.4958 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 11578
↓
P 11582 / (S)

AR
04/30/22

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

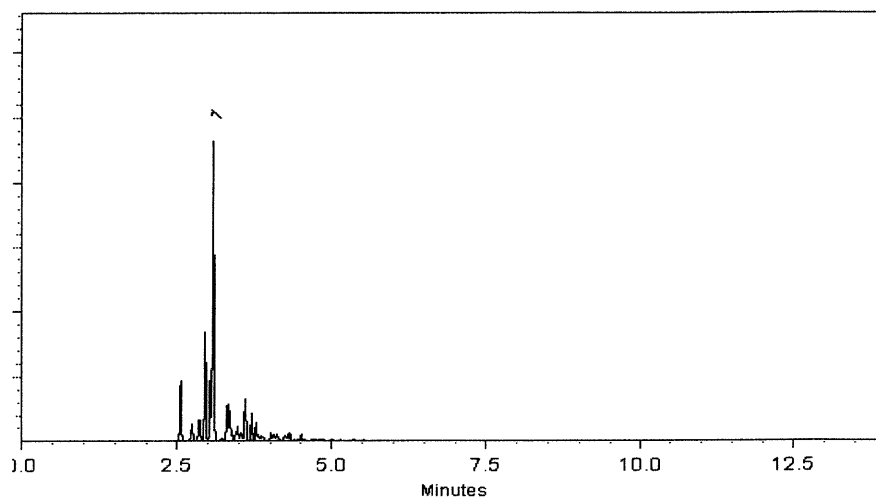

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 16-Aug-2021 **Balance:** B442140311

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 18-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11578
↓
P11582 / (S)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32008 Lot No.: A0173309
Description : Aroclor® 1232 Standard
Aroclor® 1232 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : September 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1232	1,001.0 µg/mL	+/- 5.9456 µg/mL Gravimetric
	CAS # 11141-16-5 (Lot 15665-01)		+/- 31.7389 µg/mL Unstressed
	Purity ----%		+/- 41.4544 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11583
↓
P11587 / (S)

AR
04/30/22

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

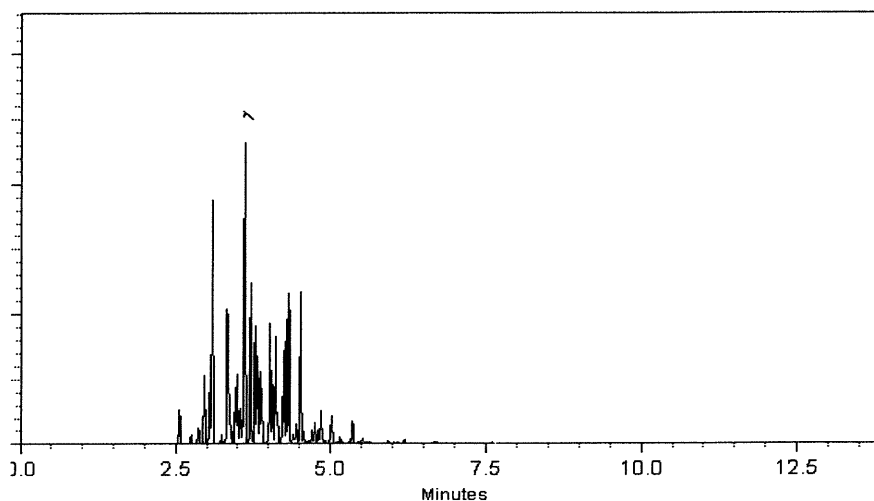

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 13-Jun-2021 **Balance:** B442140311

Alexis Shelow
Alexis Shelow - Operations Tech I

Date Passed: 16-Jun-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11583
↓
P11587 | (5)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011 Lot No.: A0175403
Description : Aroclor® 1254 Standard
Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1254 CAS # 11097-69-1 (Lot 124-191-B) Purity ----%	1,000.7 µg/mL	+/- 5.9437 µg/mL Gravimetric +/- 31.7284 µg/mL Unstressed +/- 41.4406 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11588
↓
P11592 / (S)

AR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

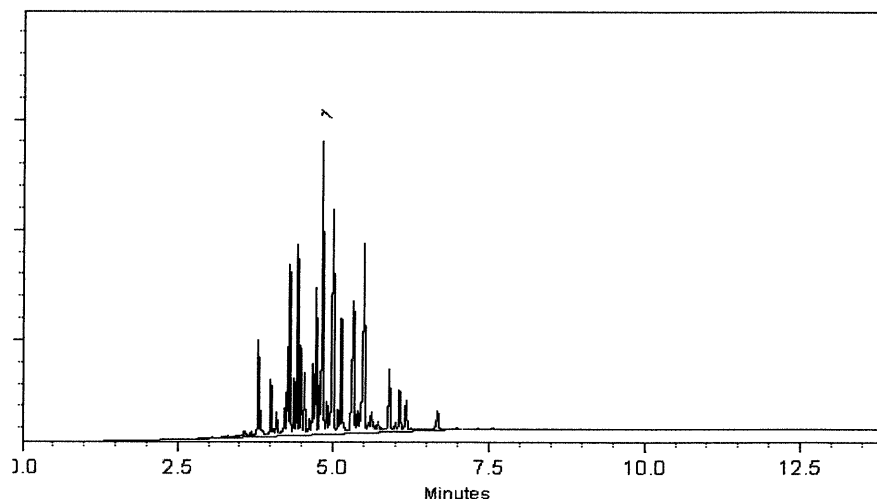

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Cathleen Soltis

Cathleen Soltis - Mix Technician

Date Mixed: 15-Aug-2021

Balance: 1128360905

Alexis Shelow

Alexis Shelow - Operations Tech I

Date Passed: 17-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11588
↓
P11592 / (5)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32410 **Lot No.:** A0181782

Description : Aroclor® 1268 Standard

Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : May 31, 2028 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1268	1,001.4 µg/mL	+/- 5.9480 µg/mL Gravimetric
	CAS # 11100-14-4 (Lot 10947000)		+/- 31.7516 µg/mL Unstressed
	Purity ----%		+/- 41.4710 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 11593
↓
P 11597

UAR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

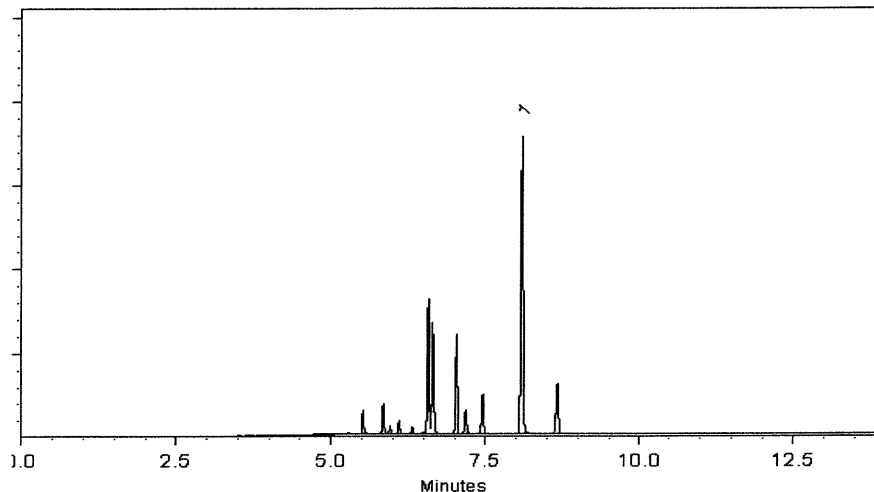

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Penelope S. Riglin
Penelope Riglin - Operations Tech I

Date Mixed: 14-Feb-2022

Balance: 1128360905

Clara Windle
Clara Windle - Operations Technician I

Date Passed: 17-Feb-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 11593 / (5)
↓
P 11597
[Signature]
04/30/2022



CERTIFIED WEIGHT REPORT

Part Number: **91867**
 Lot Number: **020823**
 Description: **WP 037 - Aroclor 1232**
PCB Technical Mixture
 Expiration Date: **020833**
 Recommended Storage: **Ambient (20 °C)**
 Nominal Concentration ($\mu\text{g/mL}$): **100**
 NIST Test ID#: **6UTB**

Solvent(
Aceton


Weight(s) shown below were combined and diluted to (mL): **100.0**
 5E-05 Balance Uncertainty
 0.057 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight (g)
1. Aroclor 1232	17	45-6A	100	100	0.5	0.01000

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measure Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stonier
 Column ID SPB-608 30 meter X 0.53mm X 5 μm film thickness
 Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
 Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
 Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
 Rate = 8°C/min, Total run time = 35 min
 Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
 Standard injection = 1.5 μL , Range=3

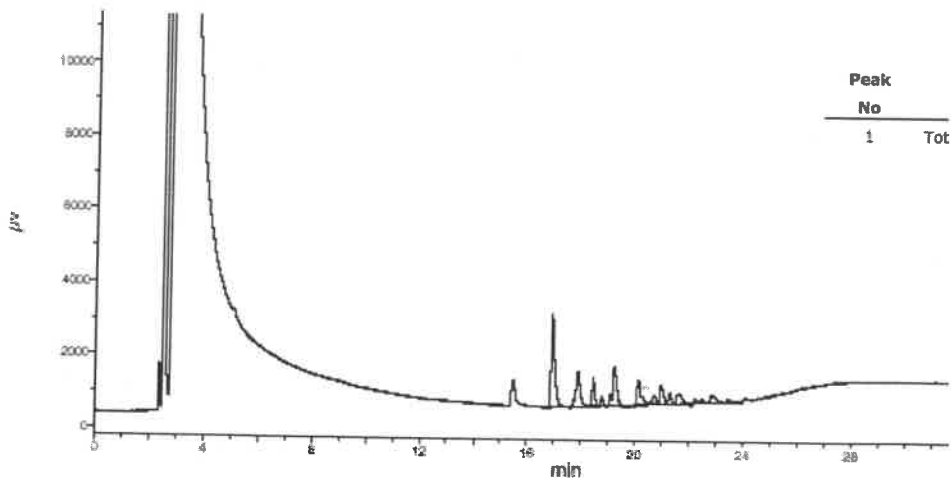




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32009 **Lot No.:** A0203672

Description: Aroclor® 1242 Standard

Aroclor® 1242 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

p12928

→

p12932

AJ

12/27/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Aroclor 1242	53469-21-9	01141	—%	1,004.7 µg/mL	+/- 55.7515

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

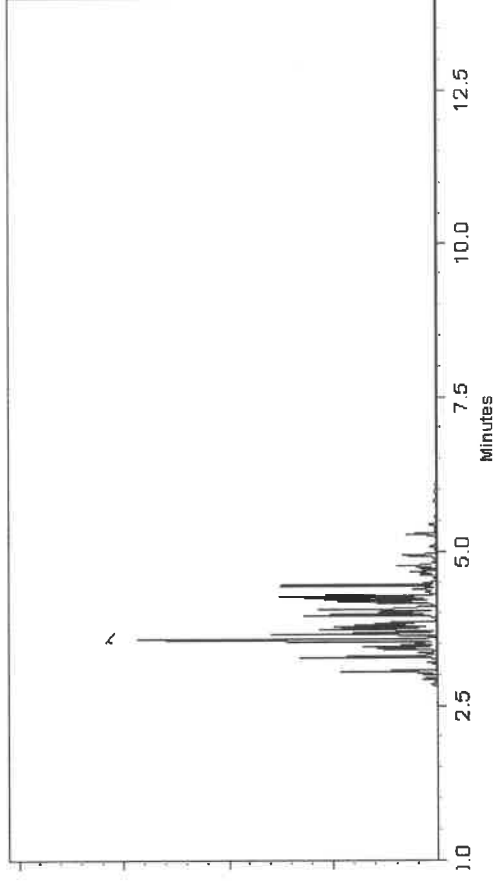

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Boothamer

Russ Boothamer - Operations Technician I

Date Mixed: 26-Oct-2023

Balance Serial #

B442140311

Jennifer Polino

Jennifer Polino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32010 **Lot No.:** A0202803

Description: Aroclor® 1248 Standard

Aroclor® 1248 Standard 1,000µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P1219697
P1219697
AF
12104123

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1248	12672-29-6	13897600	---%	1,001.7 µg/mL	+/- 55.5850

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

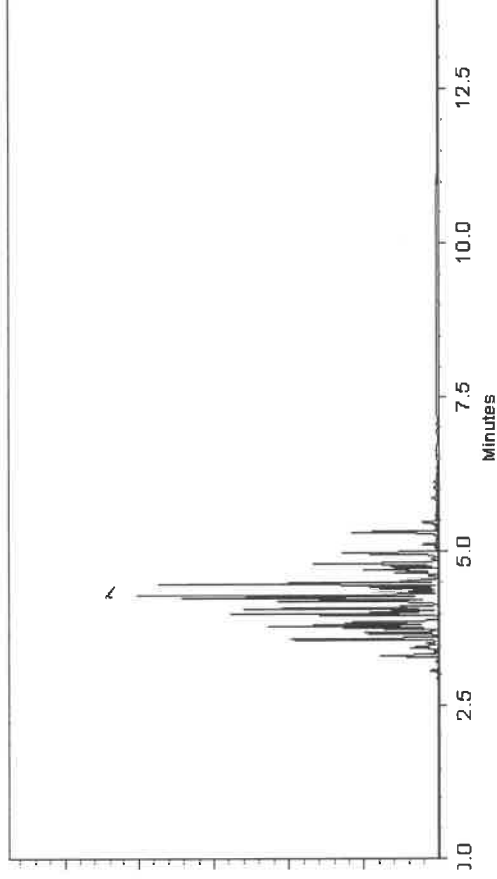

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

[Signature]
Laith Clemente - Operations Technician I

Date Mixed: 03-Oct-2023

Balance Serial # 1128360905

[Signature]
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20084

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Part Number:
20084

Lot Number:
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Expiration Date:
022033

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):
1000

NIST Test ID#:
6UTB

Solvent(s):
Hexane

Lot#
273615

Formulated By:
Benson Chan

Reviewed By:
Pedro L. Rentas

DATE
022023

DATE
022023

5E-05 Balance Uncertainty
0.010 Flask Uncertainty


Nominal Conc (µg/mL):
200.0

Weight(s) shown below were combined and diluted to (mL):

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

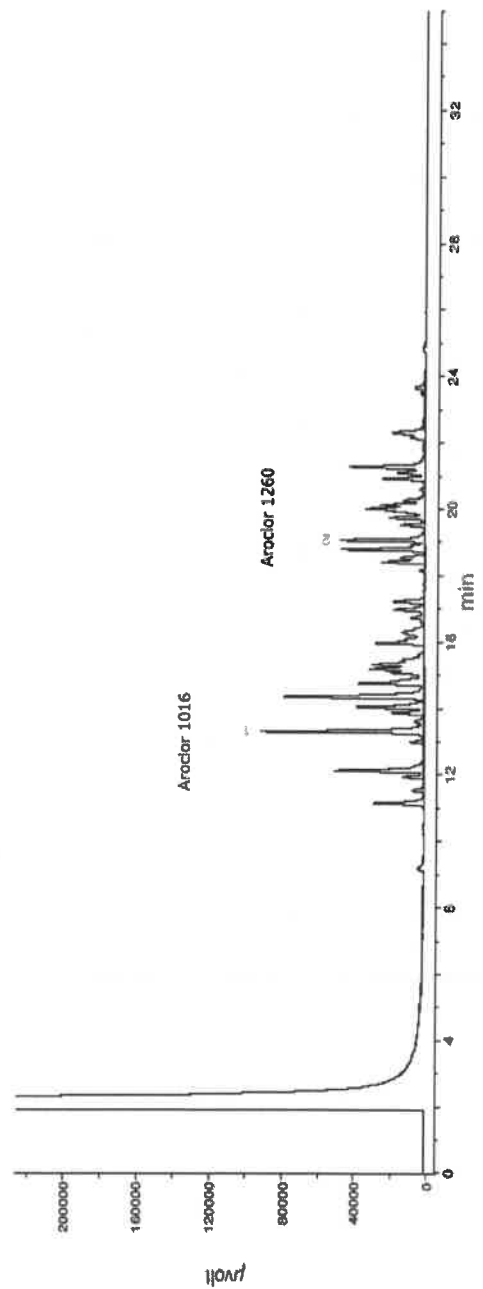



CERTIFIED WEIGHT REPORT

Part Number: 99139
Lot Number: 121823
Description: Aroclor 1254

Expiration Date: 121833
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 100
NIST Test ID#: 6UTB

Volume(s) shown below were combined and diluted to (mL): 20.0
Note: Aroclor 1254 is a mix of isomers.

Solvent(s): Iso-octane
Lot#: 82227

Formulated By: Anthony Mahoney	121823	DATE
Reviewed By: Pedro L. Rentas	121823	DATE

P12956 / Y.P.
12/18/23
P12957


Note: Aroclor 1254 is a mix of isomers.

Compound		Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Initial Uncertainty	Pipette (mL)	Conc.(µg/mL)	Initial Conc.(µg/mL)	Final Conc.(µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1254		79100	121823	0.10	2.00	0.017	0.017	1003.3	100.1	11097-69-1	1.8	0.5mg/m3 (skin)	or-rat 1295mg/kg	

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X 5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150 °C (Time 1 = 4 min), Temp 2 = 280 °C (Time 2 = 13.5 min)
Rate = 8 °C/min, Total run time = 35 min
Injector temp. = 200 °C, FID Temp. = 300 °C, FID Signal = EDAQ Channel 1
Standard injection = 1.5µL, Range=3

Peak No.	Name	FID RT (min.)
1	Total Aroclor 1254	18.12

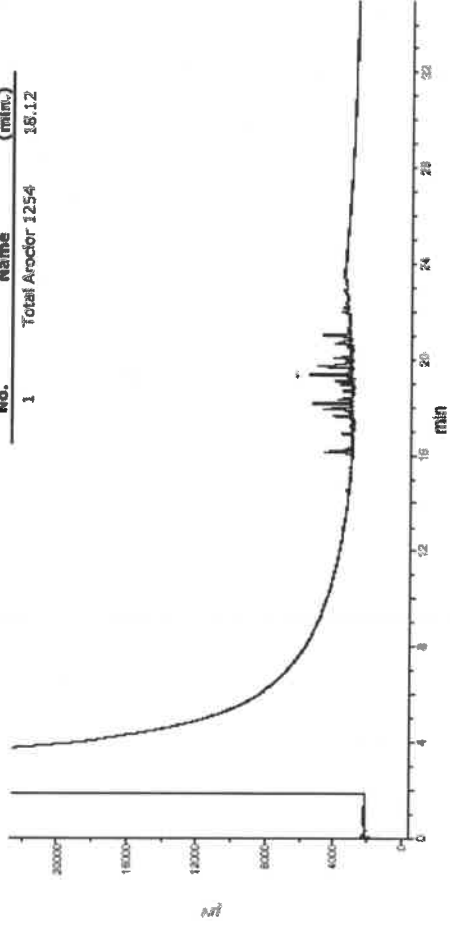



CERTIFIED WEIGHT REPORT

Part Number: 90165
Lot Number: 112322
Description: Atrocior 1262
Expiration Date: 112332
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 6LUTB
Weight(s) shown were combined and diluted to (mL): 50.0

Solvent(s): Hexane
Lot# 273615


SE-05 Balance Uncertainty
0.005 Flask Uncertainty

Formulated By:	Prashant Chauhan	112322	DATE
Reviewed By:	Pedro L. Rentes	112322	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	--------------------	-------------------	-------------------	---------------------	----------------------------------	------	----------------	------

1. Atrocior 1262 444 W-130-05 1000 100 0.2 0.05003 0.05016 1002.7 4.5 37324-23-5 N/A or-ral 11300mg/kg

Method GC/MSD-7.M: Column:(30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (0min.), Temp 2 = 290°C (12.5 min.), Rate = 8°C/min., Injector B = 200°C, Detector B = 290°C.

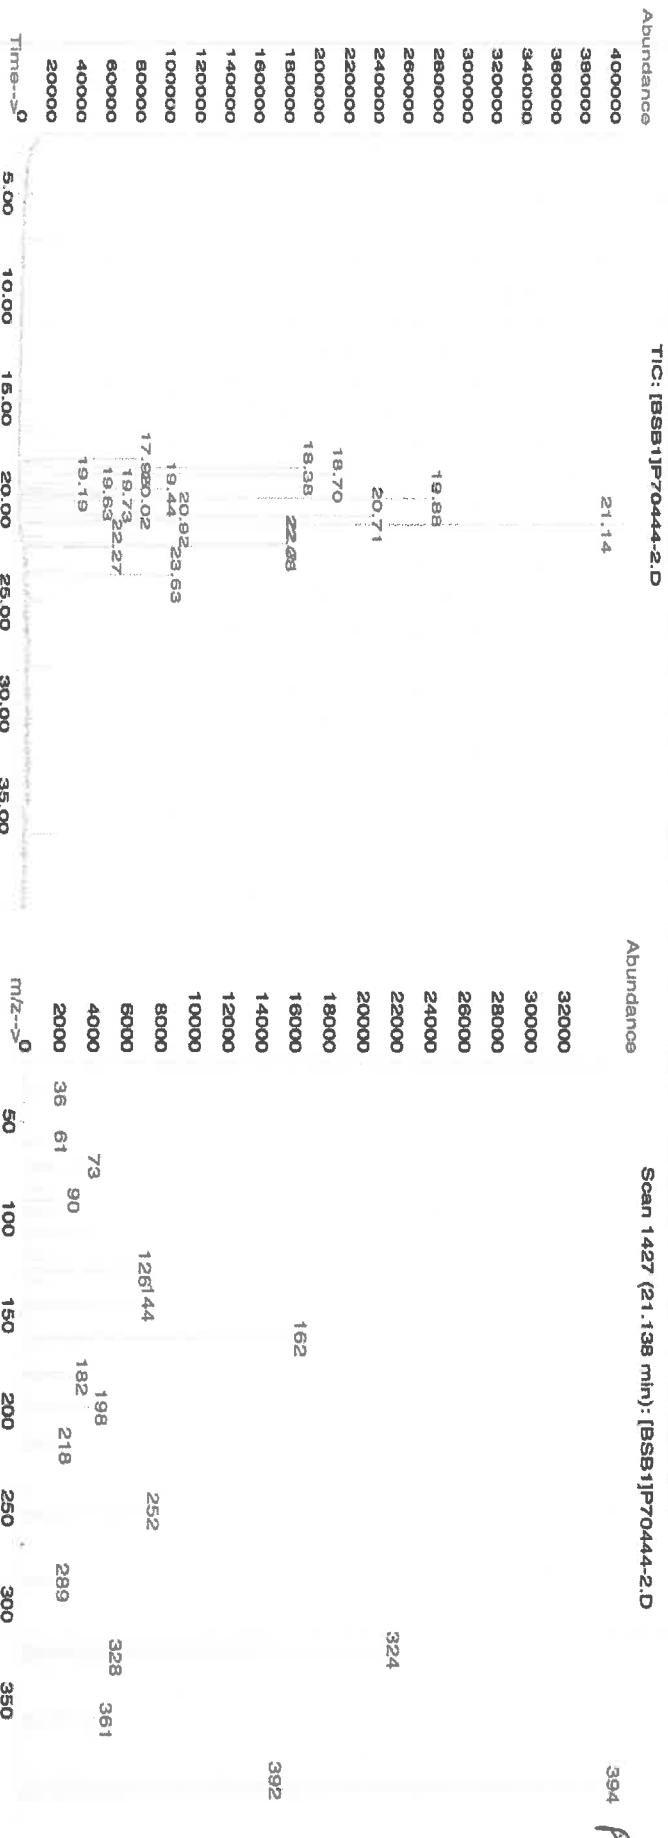

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




Run 20, "P90165 L112322 [1000µg/mL in hexane]"

Run Length: 35.00 min, 21000 points at 10 points/second.
Created: Thu, Dec 8, 2022 at 2:31:02 AM.
Sampled: Sequence "120722-GC3M1", Method "GC3-M1".
Analyzed using Method "GC3-M1".

Comments

GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
Standard injection = 1.5µL, Range=3

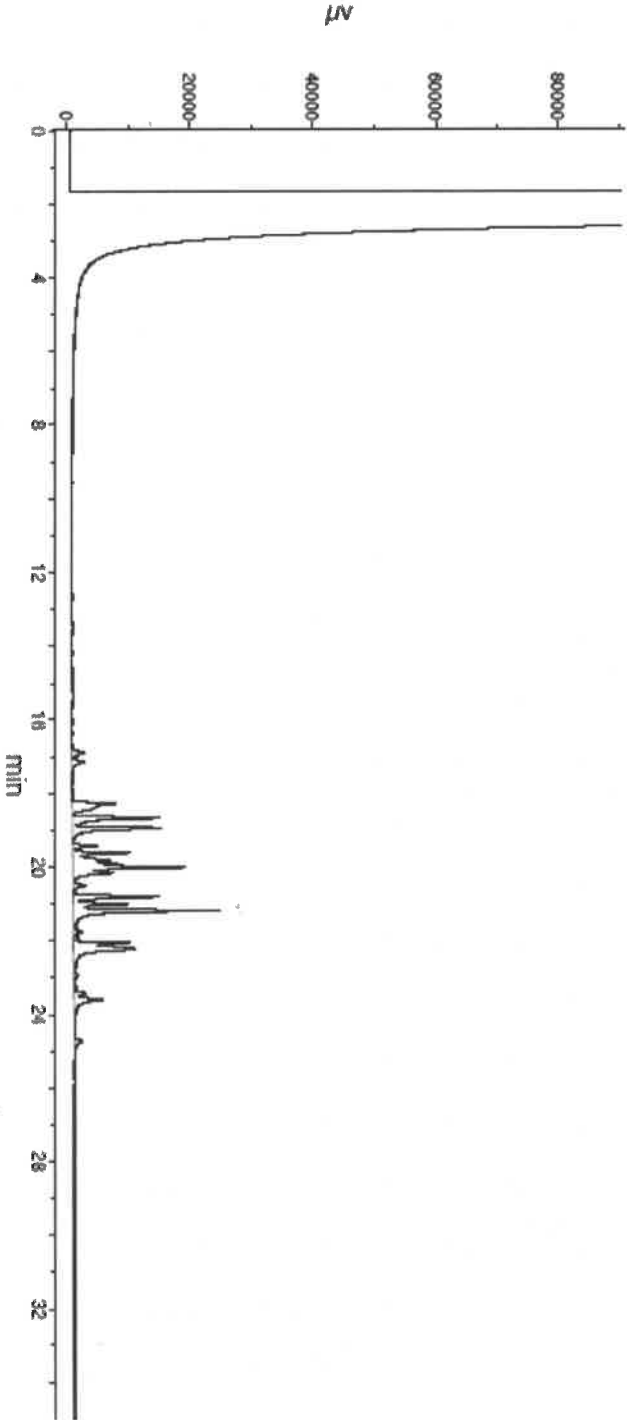



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266 **Lot No.:** A0204859

Description : Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2030 **Storage:** 25°C nominal

Handling: Sonicate prior to use. **Ship:** Ambient

P13103 } Y.P.
↓
P13112 } 01/12/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Octane (C8)	111-65-9	SHBP9758	99%	504.4 µg/mL	+/- 13.0305
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	503.6 µg/mL	+/- 13.0098
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	503.6 µg/mL	+/- 13.0098
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	504.0 µg/mL	+/- 13.0201
5	n-Hexadecane (C16)	544-76-3	SHBP8192	99%	504.0 µg/mL	+/- 13.0201
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	504.1 µg/mL	+/- 13.0230
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	504.0 µg/mL	+/- 13.0204
8	n-Docosane (C22)	629-97-0	MKCQ3882	99%	503.6 µg/mL	+/- 13.0098
9	n-Tetracosane (C24)	646-31-1	MKCQ8345	99%	504.0 µg/mL	+/- 13.0201
10	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	504.0 µg/mL	+/- 13.0201
11	n-Octacosane (C28)	630-02-4	BCCG0084	99%	504.0 µg/mL	+/- 13.0201
12	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	504.0 µg/mL	+/- 13.0204
13	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	504.0 µg/mL	+/- 13.0201
14	n-Tetratriacontane (C34)	14167-59-0	OML4N	99%	504.4 µg/mL	+/- 13.0305
15	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	504.0 µg/mL	+/- 13.0201
16	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	503.8 µg/mL	+/- 13.0152
17	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	503.6 µg/mL	+/- 13.0098

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

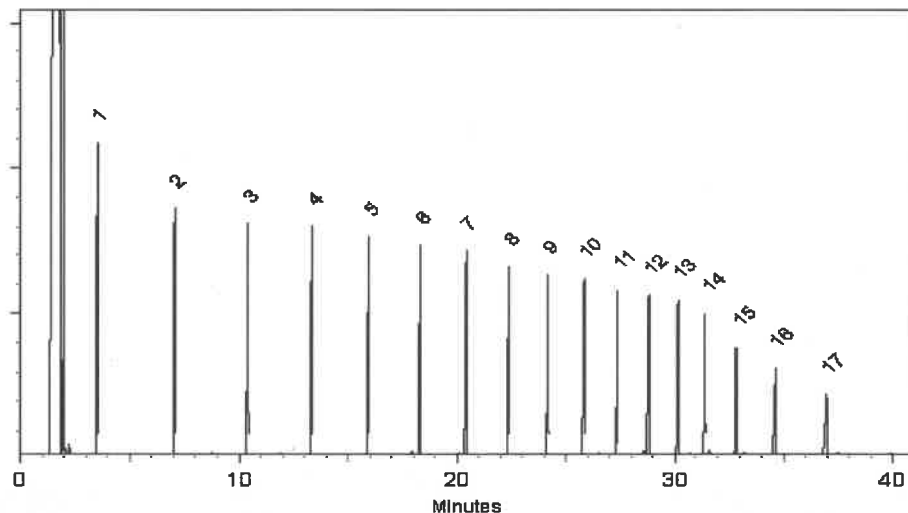


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 29-Nov-2023

Balance Serial # B442140311


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Dec-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266 **Lot No.:** A0204859

Description : Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2030 **Storage:** 25°C nominal

Handling: Sonicate prior to use. **Ship:** Ambient

P13103 } Y.P.
↓
P13112 } 01/12/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Octane (C8)	111-65-9	SHBP9758	99%	504.4 µg/mL	+/- 13.0305
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	503.6 µg/mL	+/- 13.0098
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	503.6 µg/mL	+/- 13.0098
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	504.0 µg/mL	+/- 13.0201
5	n-Hexadecane (C16)	544-76-3	SHBP8192	99%	504.0 µg/mL	+/- 13.0201
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	504.1 µg/mL	+/- 13.0230
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	504.0 µg/mL	+/- 13.0204
8	n-Docosane (C22)	629-97-0	MKCQ3882	99%	503.6 µg/mL	+/- 13.0098
9	n-Tetracosane (C24)	646-31-1	MKCQ8345	99%	504.0 µg/mL	+/- 13.0201
10	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	504.0 µg/mL	+/- 13.0201
11	n-Octacosane (C28)	630-02-4	BCCG0084	99%	504.0 µg/mL	+/- 13.0201
12	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	504.0 µg/mL	+/- 13.0204
13	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	504.0 µg/mL	+/- 13.0201
14	n-Tetratriacontane (C34)	14167-59-0	OML4N	99%	504.4 µg/mL	+/- 13.0305
15	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	504.0 µg/mL	+/- 13.0201
16	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	503.8 µg/mL	+/- 13.0152
17	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	503.6 µg/mL	+/- 13.0098

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

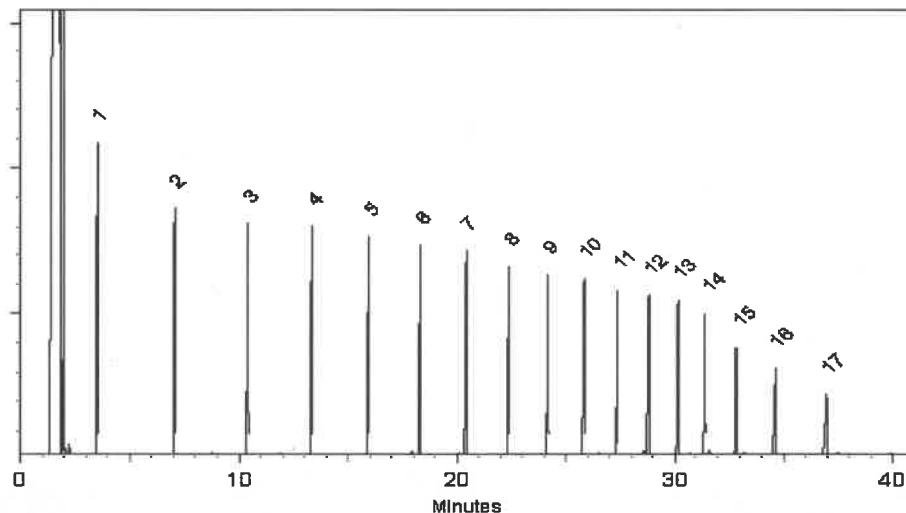


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 29-Nov-2023

Balance Serial # B442140311


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Dec-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

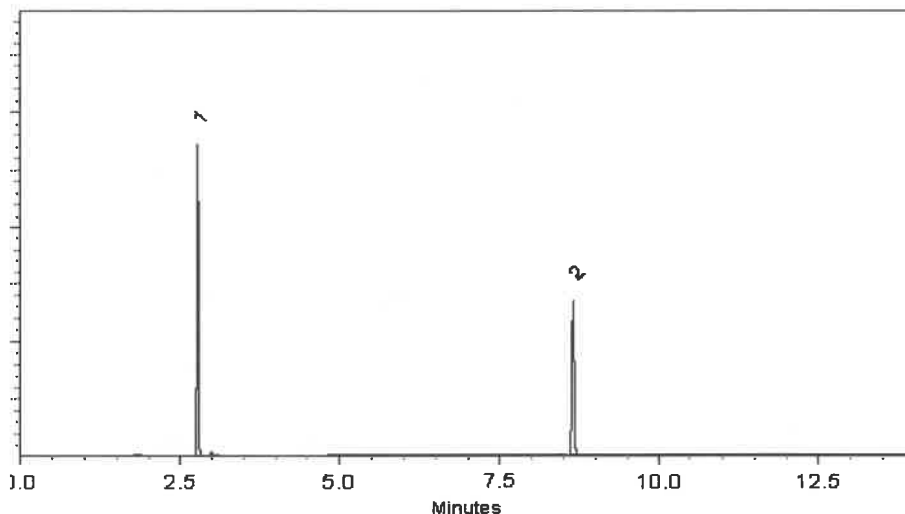


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

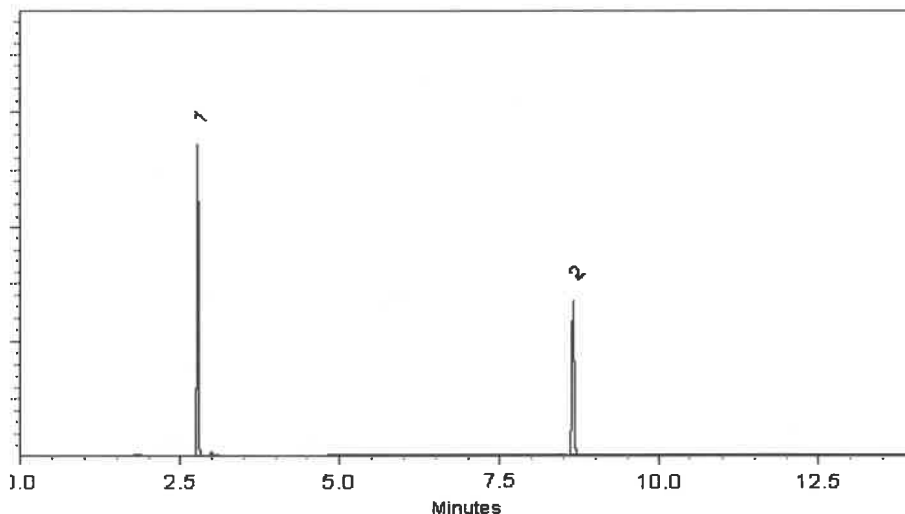


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905



Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



Agilent

Trusted Answers

ISO 17034

Reference Material Certificate

Product Information Sheet

Product Name: Aroclor 1221 Standard
Product Number: PP-292-1
Storage Conditions: Store at Room Temperature (15° to 30°C).

Lot Number: 0006783205
Lot Issue Date: 20-Feb-2024
Expiration Date: 31-Mar-2032

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1221	100.3 ±	0.5 µg/mL	011104-28-2	NT01017

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13342
AJ
05106124
P13343

Page: 1 of 2

CSD-QA-015.2

ISO 17025

Cert No. AT-1937


250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.2

ISO 17025
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



SHIPPING DOCUMENTS

CHEMTECH

CHAIN OF CUSTODY RECORD

284 Sheffield Street, Mountainside, NJ 07092
(908) 789-8900 • Fax (908) 789-8922
www.chemtech.net

CHEMTECH PROJECT NO. PS026
QUOTE NO.
COC Number 2042079

CLIENT INFORMATION

REPORT TO BE SENT TO:

COMPANY: Tully Construction Co. Inc

ADDRESS: 104th St & 164th Drive

CITY: Queens STATE: NY ZIP:

ATTENTION: Dean Devoe

PHONE:

FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME:

PROJECT NO.: LOCATION:

PROJECT MANAGER:

e-mail:

PHONE:

FAX:

CLIENT BILLING INFORMATION

BILL TO: PO#:

ADDRESS:

CITY STATE: ZIP:

ATTENTION: PHONE:

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) DAYS*

HARDCOPY (DATA PACKAGE): DAYS*

EDD: DAYS*

*TO BE APPROVED BY CHEMTECH

STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS DAYS

DATA DELIVERABLE INFORMATION

- ☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☐ Level 2 (Results + QC) ☐ NJ Reduced ☐ US EPA CLP
☐ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
+ Raw Data ☐ Other
☐ EDD FORMAT

1 Vol's 2 Svor & PCB 3 TEL 4 Corrosivity 5 Ignitability 6 Reactivity 7 Reactive Cyn 8 Mercaptan Sulfide 9 TPH

PRESERVATIVES

COMMENTS

CHEMTECH SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									COMMENTS
			COMP	GRAB	DATE	TIME		E/F	E	E	E	E	E	E	E	E	
1.	SOIL-1-HAM	SOL	X		11-27-24	1042	7		X	X	X	X	X	X	X	X	
2.	SOIL-1-HAM			X		1045	4	X									0.0 ppm
3.	SOIL-1-HAM-TPH2		X			1050	1									X	
4.	SOIL-2-HAM		X			1110	7		X	X	X	X	X	X	X	X	
5.	SOIL-2-HAM			X		1112	4	X									0.0 ppm
6.	SOIL-2-HAM-TPH2		X			1115	1									X	
7.																	
8.																	
9.																	
10.																	


SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER: 1. <i>gm</i>	DATE/TIME: 1130 11-27-24	RECEIVED BY: 1. <i>[Signature]</i>	Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP _____ °C Comments: Collected 8:1 Composite Sample + (2) 5:1 Composite Sample for sampling protocol
RELINQUISHED BY SAMPLER: 2. <i>[Signature]</i>	DATE/TIME:	RECEIVED BY: 2.	
RELINQUISHED BY SAMPLER: 3. <i>gm</i>	DATE/TIME: 1400 11-27-24	RECEIVED BY: 3.	PID Calibration 11-27-24

Page 1 of 1

CLIENT: ☐ Hand Delivered ☐ Other _____
CHEMTECH: ☐ Picked Up ☒ Field Sampling

Shipment Complete
☐ YES ☐ NO

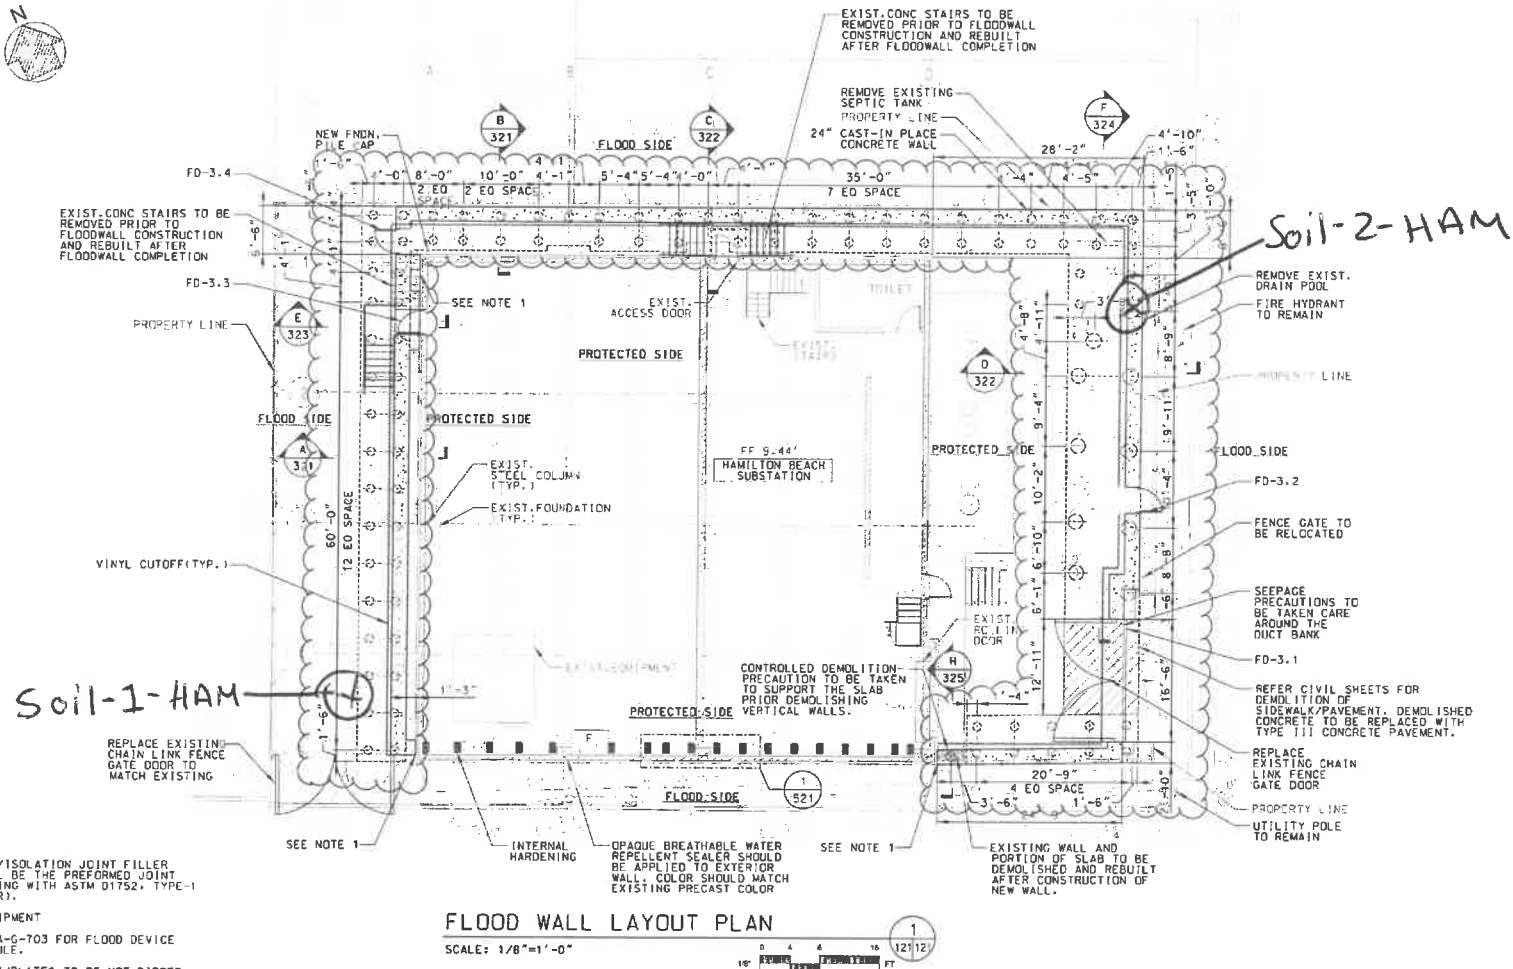

NOTES:

1. THE EXPANSION/ISOLATION JOINT FILLER MATERIAL SHALL BE THE PREFORMED JOINT FILLER COMPLYING WITH ASTM D1752, TYPE-1 (SPONGE RUBBER).
2. F - FIXED EQUIPMENT
3. REFER P36343-6-C-703 FOR FLOOD DEVICE OPENING SCHEDULE.
4. ALL HSS/ANGLES/PLATES TO BE HOT DIPPED GALVANIZED SECTIONS.

FLOOD WALL LAYOUT PLAN

SCALE: 1/8"=1'-0"



IT IS A VIOLATION OF THE PROFESSIONAL LICENSE LAW FOR ANY PERSON TO ALTER THIS DRAWING IN ANY WAY, UNLESS ACTING UNDER THE DIRECTION OF A LICENSED PROFESSIONAL ENGINEER, REGISTERED ARCHITECT, THE ALTERING ENGINEER OR ARCHITECT. THE DRAWING NUMBER, SCALE, DATE, TITLE, PROJECT NAME, AND A SIGNATURE OF THE ENGINEER OR ARCHITECT SHALL BE PLACED IN THE BOTTOM RIGHT CORNER OF THE DRAWING.

CONTRACT P-36343
FLOOD MITIGATION AT TWENTY SIX (26) SUBSTATIONS
IN THE BOROUGH OF BROOKLYN, MANHATTAN AND QUEENS
**HAMILTON BEACH
SUBSTATION FLOOD
WALL PLAN**



DRAWN BY	R. NUTHAN	<i>Nathan</i>	DATE	04/15/2024
DESIGNED BY	KUDAY	<i>Kuday</i>	DRAWING	STRUCTURAL
CHECKED BY	DINAKAR KN	<i>Dinakar</i>	PROJECT NO.	P36343-HAM-CS-121
APPROVED BY	C. JEDRICH, PE	<i>Jedrich</i>	REVISION	

REVISION	DESCRIPTION	DATE	APPROVED

REVISIONS

SDSIGN&FILEEXPANDEDSSPECS

PRINT AS OF SDATES&OFSPLOTTINGS

USERSNAME



Environmental Laboratory

www.chemtech.net | EMAIL: PM@chemtech.net

Project Name: _____

Chemtech Order ID: _____

Service Order #: _____

Sampler Name: Jeremy N
Client Project Coordinator & Phone: _____

Work Order #: _____

Dean D

Labor WBS #: _____

Page #: 1 of 1

Facility/Site: Hamilton Beach Sub

Date: 11-27-24

Site Address: 104th Street &

Arrive Time: 1030

104th Drive, Queens NY

Depart Time: 1130

Waste Stream (circle one): drum / roll-off / soil pile / in-situ / linear construction / frac-tank

Sample Matrices (circle all that apply): Water / Solid / NAPL / Concrete / Wipe

Collection Depths: _____

Dimensions/CY: _____

Temp (range): 2-3 °C

PID Readings (range): 0-0

PPM

Odor: y

N

Color: y

(N)

Sample Description: wet sand, rocks.

Field Observations: very wet sand, (2) unique locations

Grid/Area Composite Map:

QA Control # A3041134

See

Affirmed

MAP

Sampler Signature: JN

Supervisor Review/Date: _____

Client Signature: _____

Date/Time Arrived at Lab: _____



284 Sheffield Street, Mountainside NJ 07092 (908)-789-8900 Fax : 908 789 8922

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

LOGIN REPORT/SAMPLE TRANSFER

Order ID : P5026 TULL02

Order Date : 11/27/2024 11:24:00 AM

Project Mgr :

Client Name : Tully Construction Co., Inc.

Project Name : Hamilton

Report Type : Level 1

Client Contact : Dean Devoe

Receive DateTime : 11/27/2024 2:00:00 PM

EDD Type : Excel NY 375

Invoice Name : Tully Construction Co., Inc.

Purchase Order :

Hard Copy Date :

Invoice Contact : Dean Devoe

Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
P5026-04	SOIL-1-HAM-GRAB	Solid	11/27/2024	10:45					
					VOC-TCLVOA-10		8260D	5 Bus. Days	
P5026-08	SOIL-1-HAM-GRAB	Solid	11/27/2024	11:12					
					VOC-TCLVOA-10		8260D	5 Bus. Days	

Relinquished By :

Date / Time :

DM
11-27-24 1435

Received By :

Date / Time :

Sam
11/27/24 14:35 RJL
A22

Storage Area : VOA Refridgerator Room