


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120324\
Data File : BF140701.D
Acq On : 03 Dec 2024 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

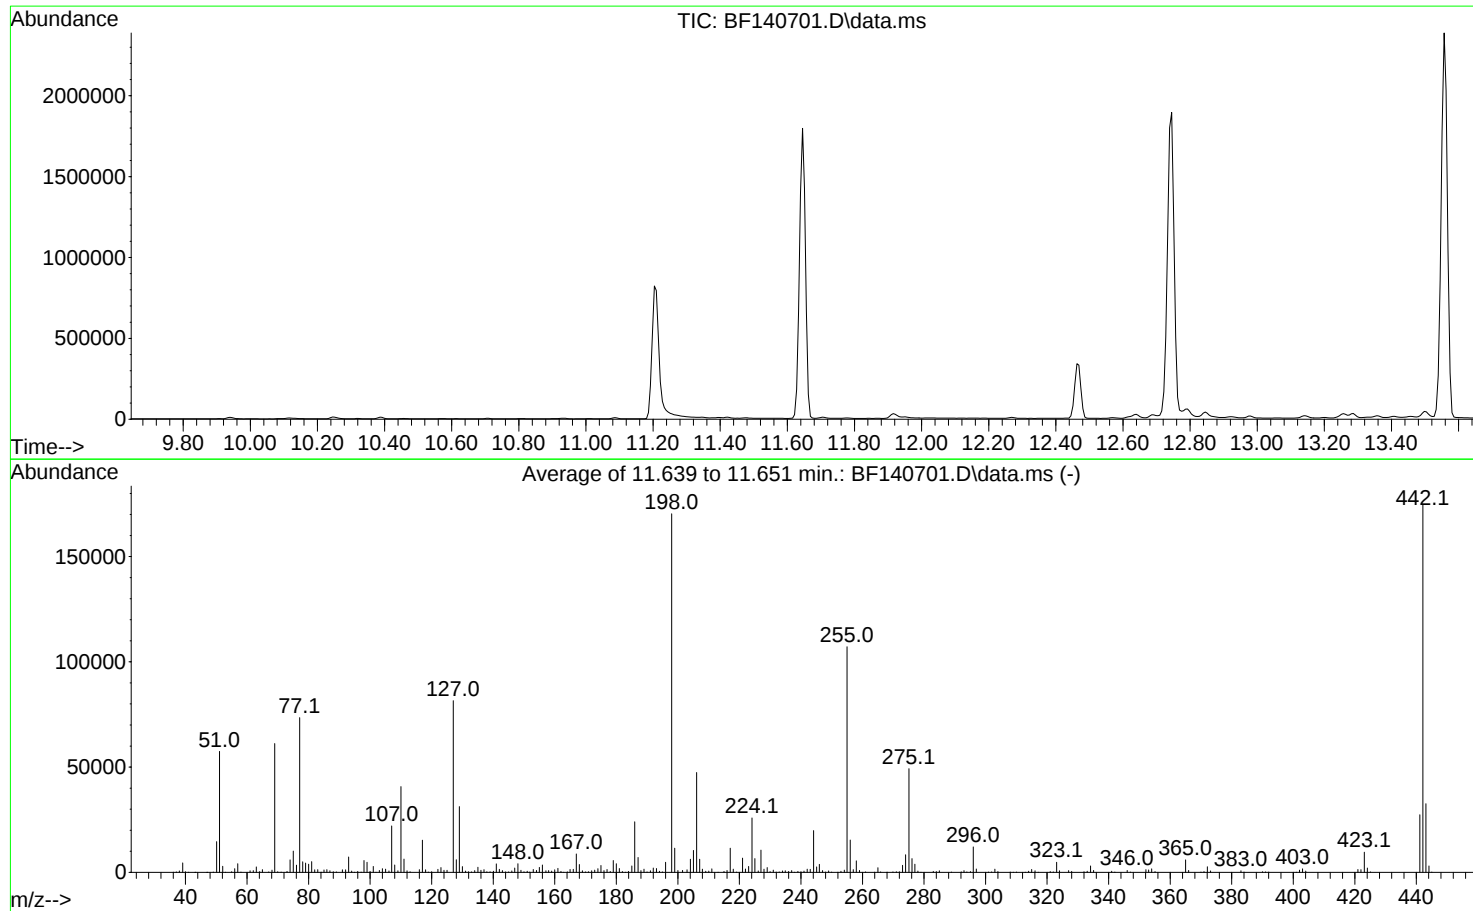

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	57429	PASS
68	69	0.00	2	1.8	1107	PASS
69	198	0.00	100	35.9	61161	PASS
70	69	0.00	2	0.6	346	PASS
127	198	10	80	47.9	81539	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	170304	PASS
199	198	5	9	6.8	11503	PASS
275	198	10	60	28.9	49245	PASS
365	198	1	100	3.5	5967	PASS
441	198	0.01	100	16.1	27336	PASS
442	442	50	100	100.0	174739	PASS
443	442	15	24	18.7	32595	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/3/2024	BNA_F	<u>BF140701.D</u>
Compound Name	Response	Retention Time
DDT	617260	13.557
DDD	16771	13.257
DDE	2986	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19757	637017	3.10

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120324\
Data File : BF140701.D
Acq On : 03 Dec 2024 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 03 12:35:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

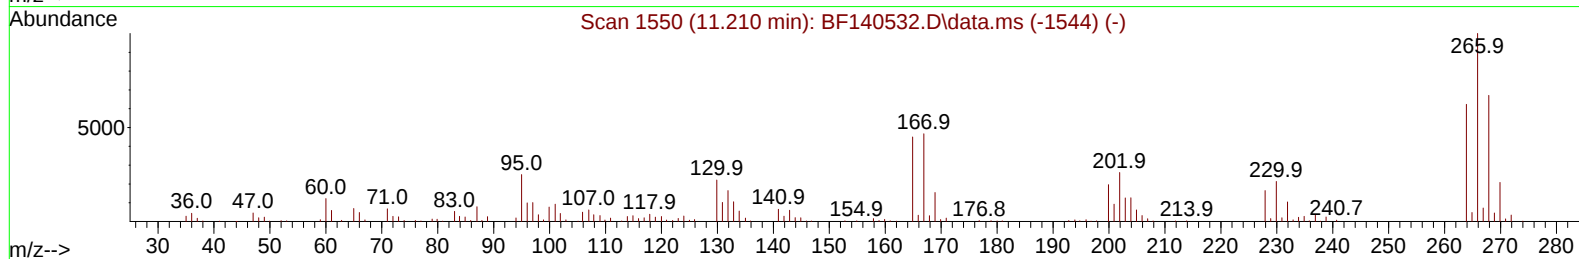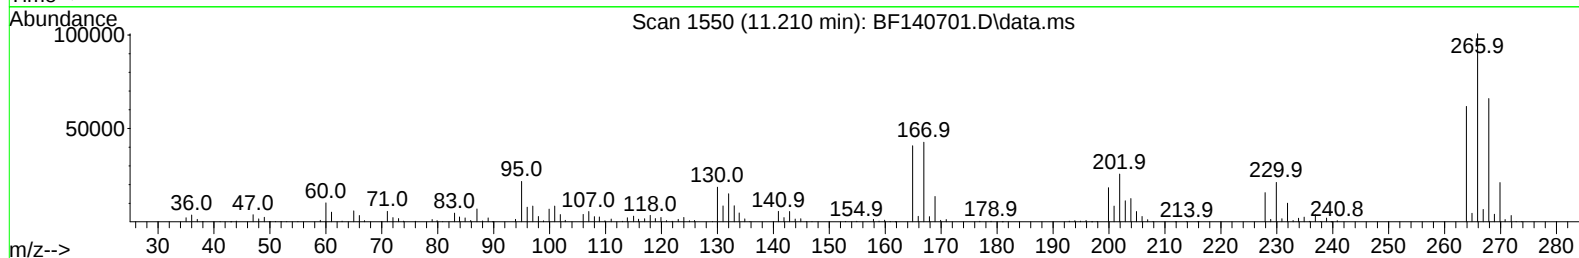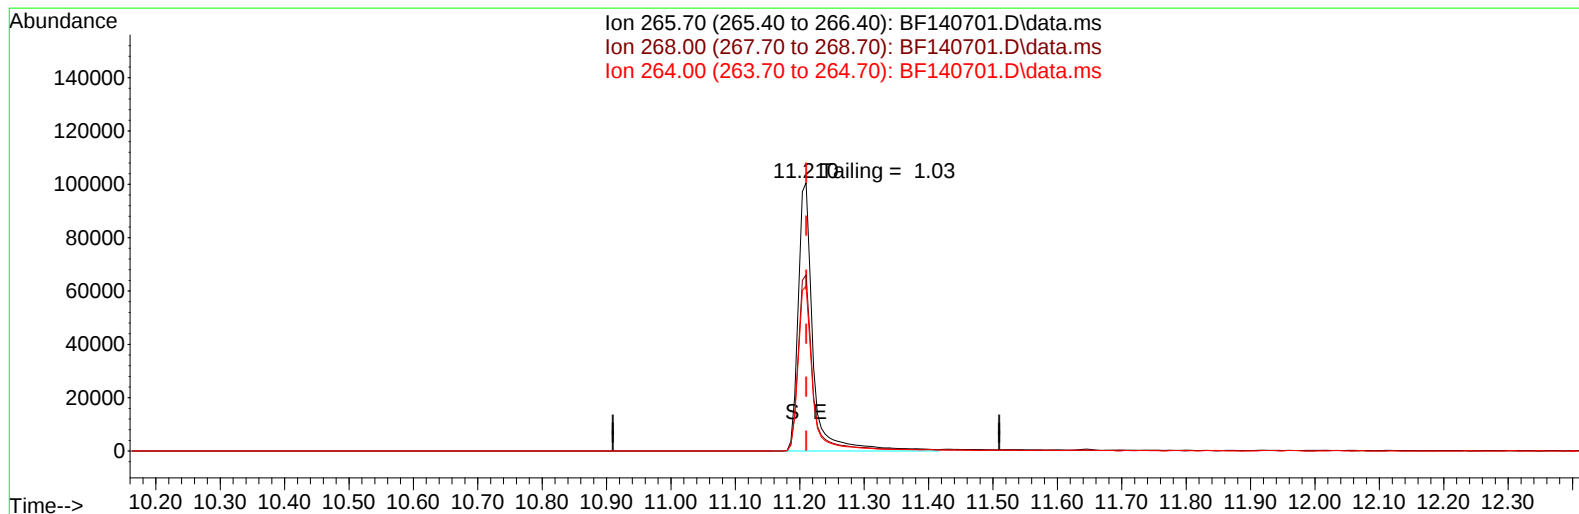

TIC: BF140701.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 13968.96 ng




response 162096

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	65.61
264.00	62.30	61.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120324\
Data File : BF140701.D
Acq On : 03 Dec 2024 10:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 03 12:35:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

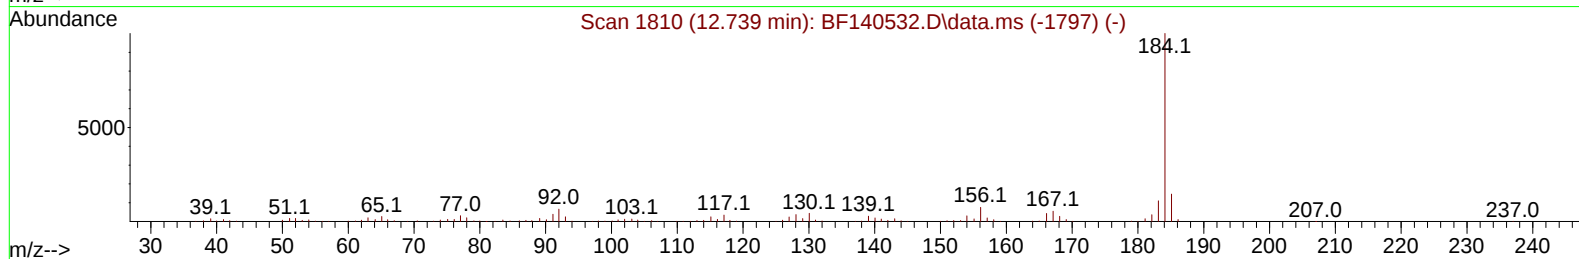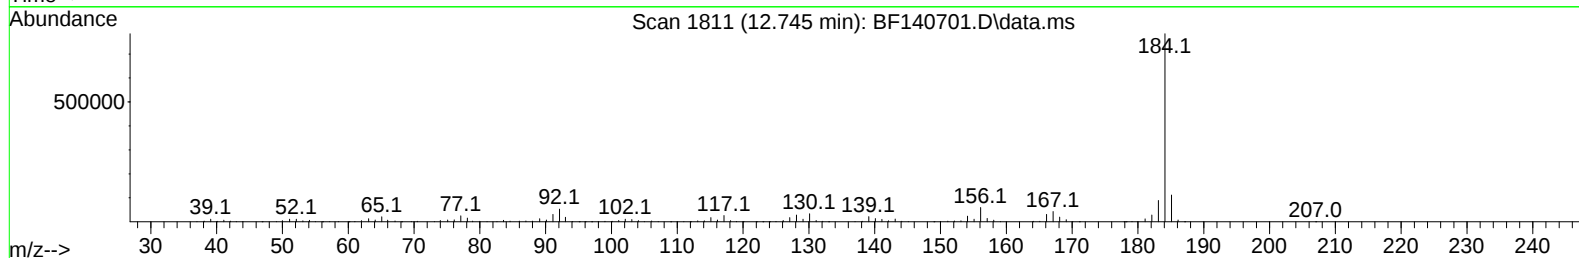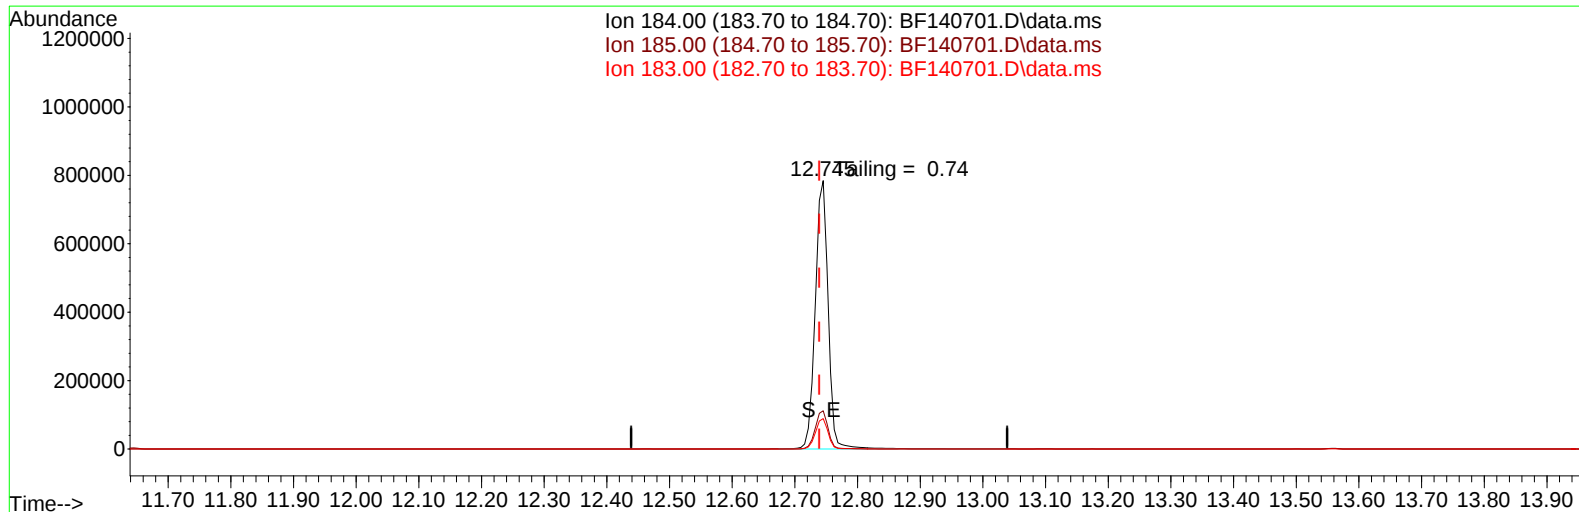

TIC: BF140701.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 19954.27 ng

response 1120287

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.27
183.00	11.00	11.36
0.00	0.00	0.00