


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120624\
Data File : BF140759.D
Acq On : 06 Dec 2024 11:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

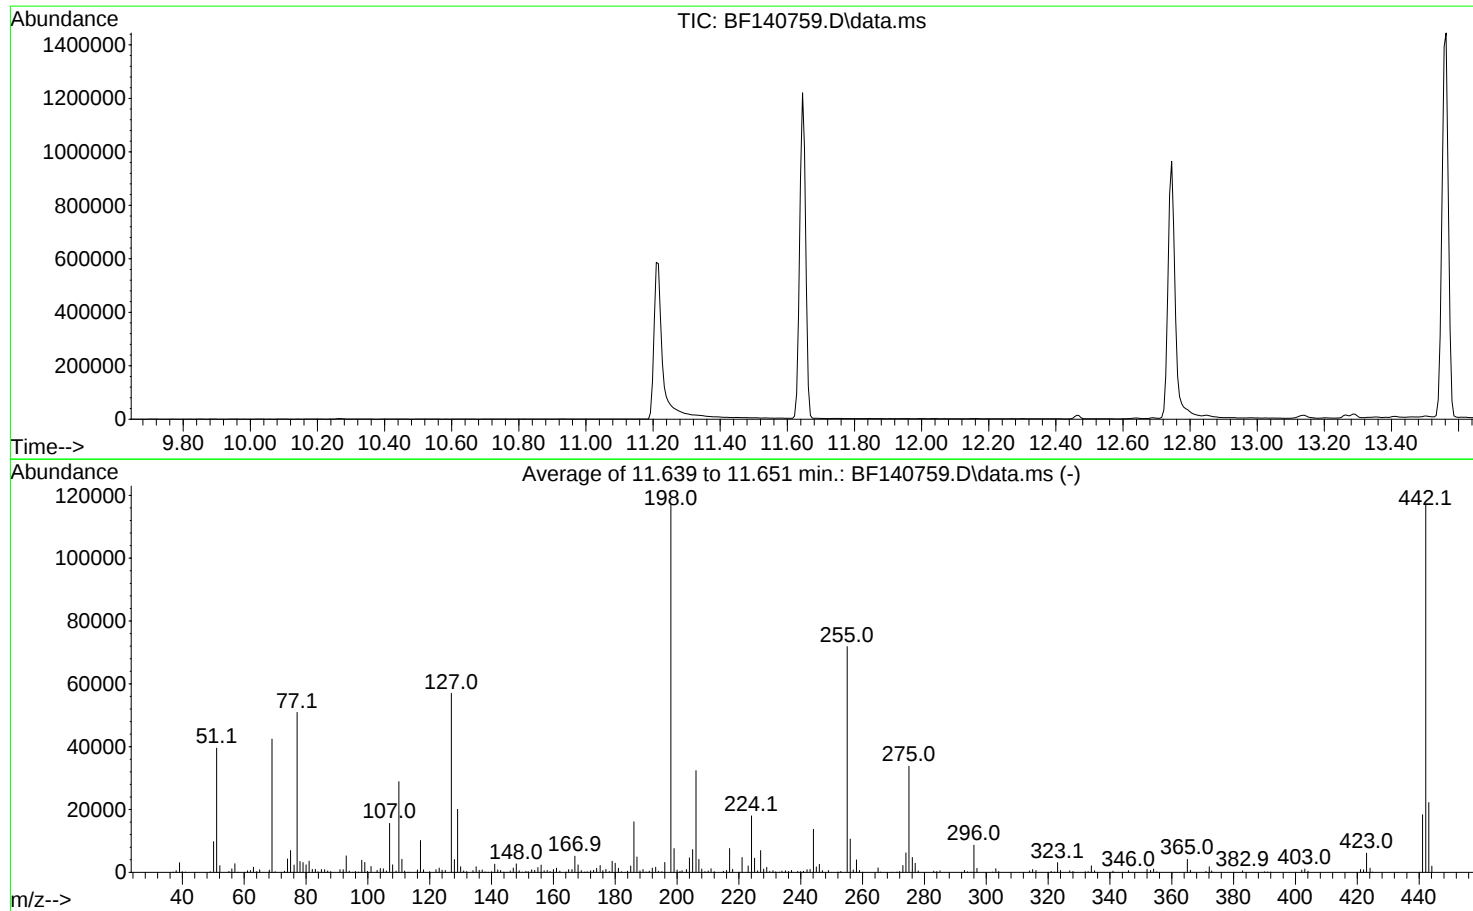

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	39536	PASS
68	69	0.00	2	1.7	736	PASS
69	198	0.00	100	36.2	42400	PASS
70	69	0.00	2	0.5	199	PASS
127	198	10	80	48.7	56981	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	117088	PASS
199	198	5	9	6.5	7592	PASS
275	198	10	60	28.8	33768	PASS
365	198	1	100	3.5	4147	PASS
441	198	0.01	100	15.7	18356	PASS
442	442	50	100	100.0	116827	PASS
443	442	15	24	19.0	22187	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/6/2024	BNA_F	<u>BF140759.D</u>
Compound Name	Response	Retention Time
DDT	385885	13.563
DDD	10302	13.286
DDE	523	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10825	396710	2.73

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120624\
Data File : BF140759.D
Acq On : 06 Dec 2024 11:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 06 11:51:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

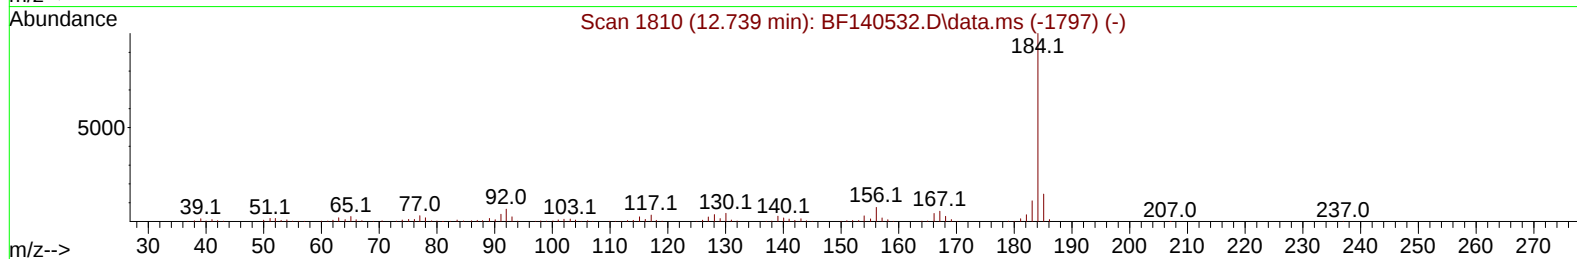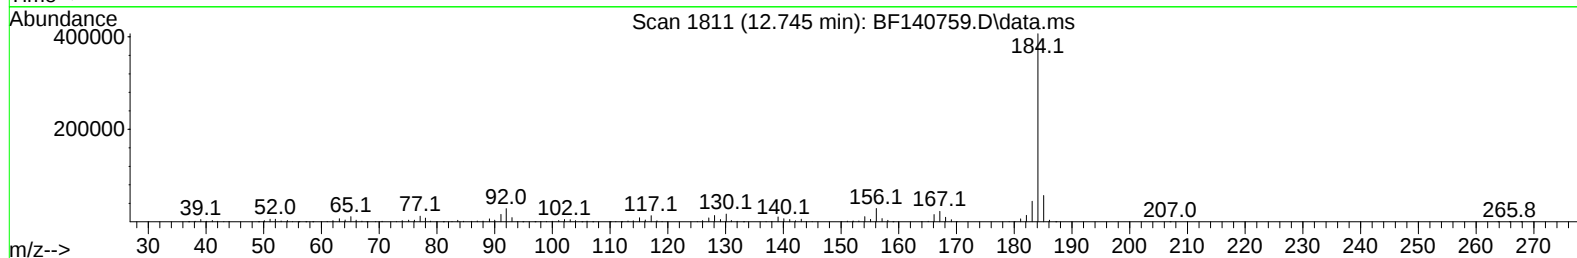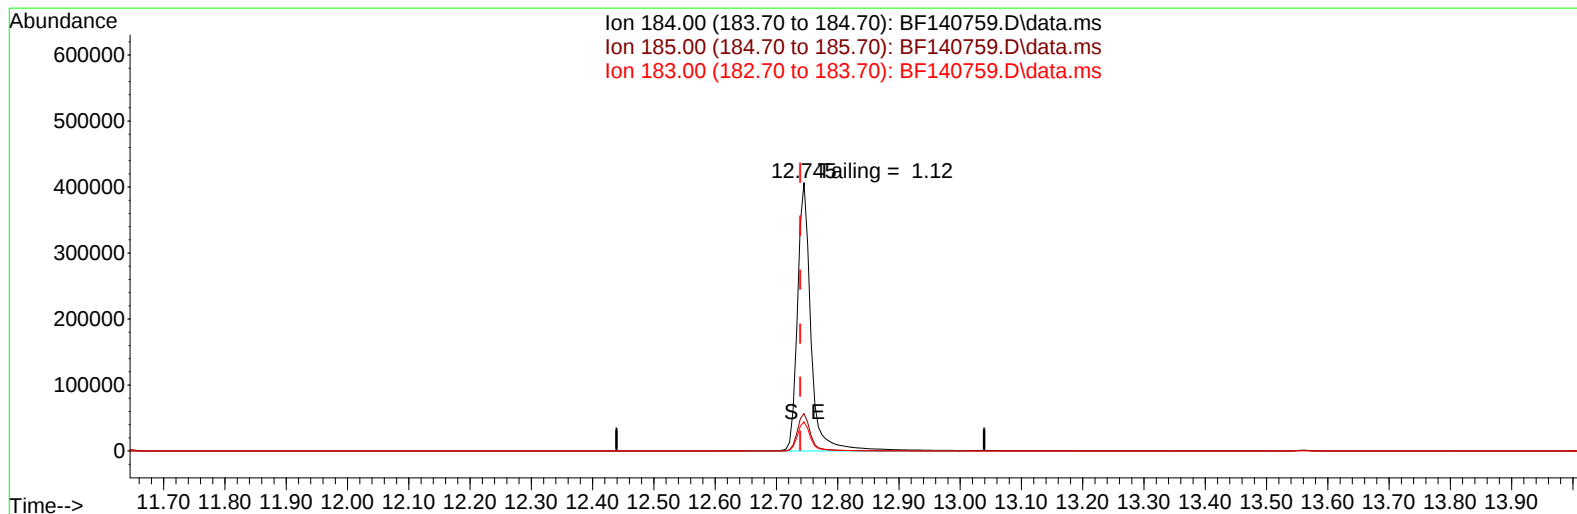

TIC: BF140759.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 121878.40 ng

response 623664

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.97
183.00	11.00	10.91
0.00	0.00	0.00