

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112724\
 Data File : PD086946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2024 11:15
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 13:49:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112724.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 13:46:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.884	40763452	247.1E6	20.384	21.591
28)	SA Decachlor...	9.088	8.088	67435812	299.6E6	21.200	21.501
Target Compounds							
9)	A Endosulfan I	6.084	5.256	33253236	160.7E6	9.909	11.319
10)	B gamma-Chl...	5.955	5.135	35074611	179.2E6	9.928	11.517
12)	B 4,4'-DDE	6.205	5.385	64098695	324.3E6	19.700	21.510
13)	MA Dieldrin	6.357	5.522	69568570	326.7E6	19.257	20.981
19)	B Endosulfa...	7.158	6.492	55616433	299.3E6	19.112	22.125
20)	A Methoxychlor	7.503	6.766	155.5E6	637.5E6	97.214	88.874
21)	B Endrin ke...	7.640	7.002	64894282	316.5E6	19.997	21.002



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112724\
Data File : PD086946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2024 11:15
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 13:49:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112724.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 13:46:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

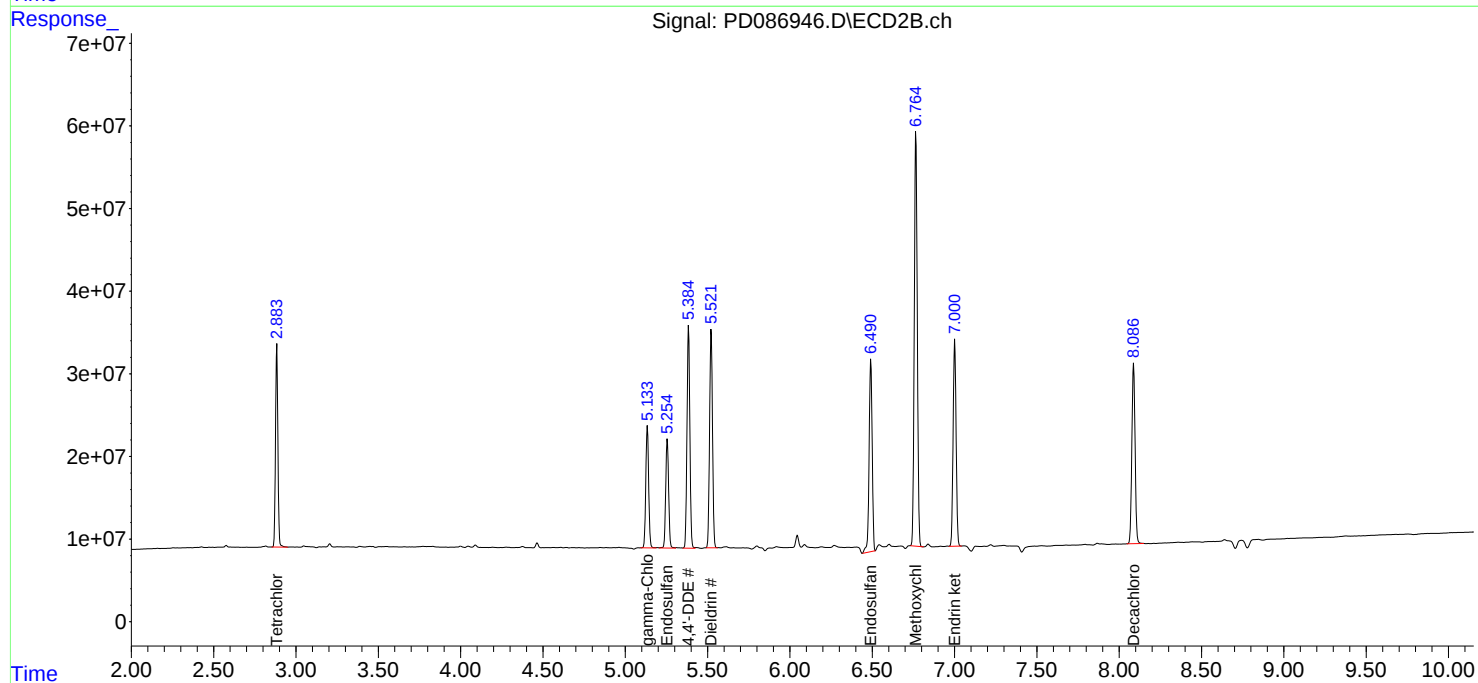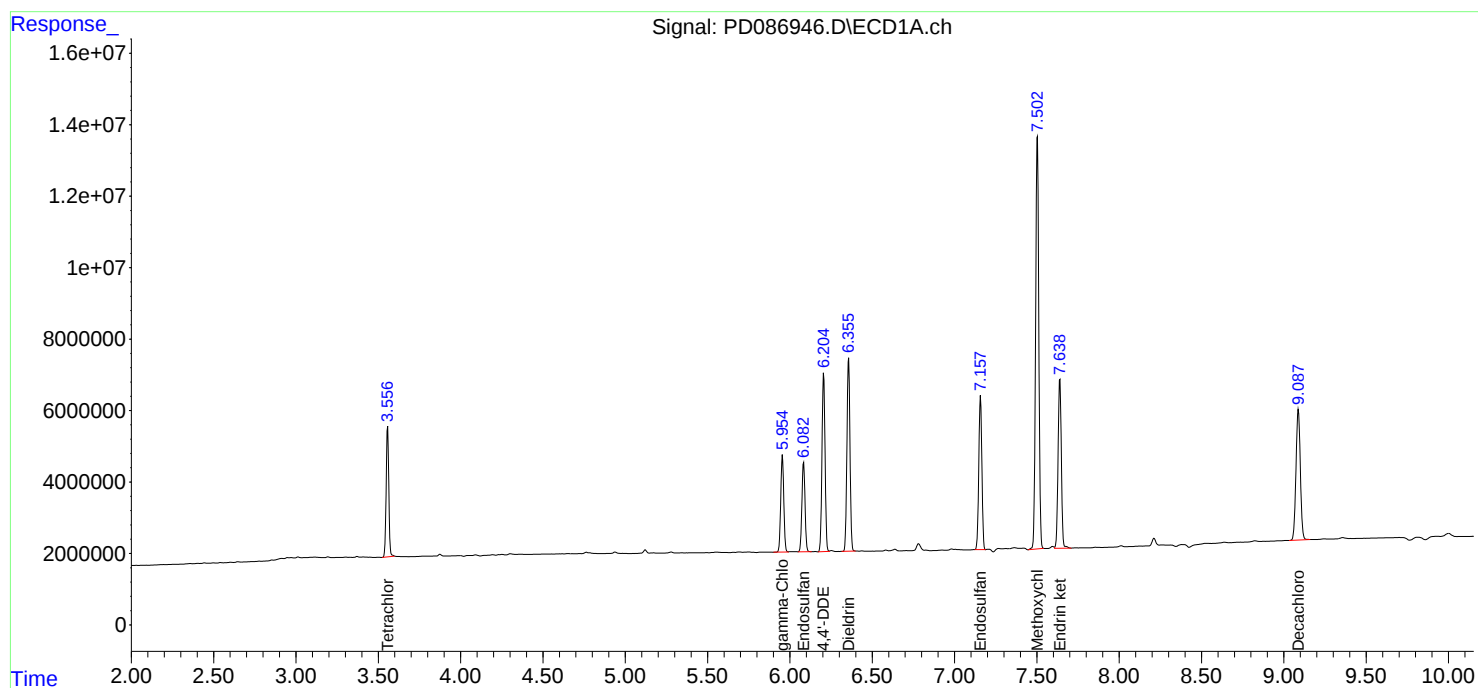


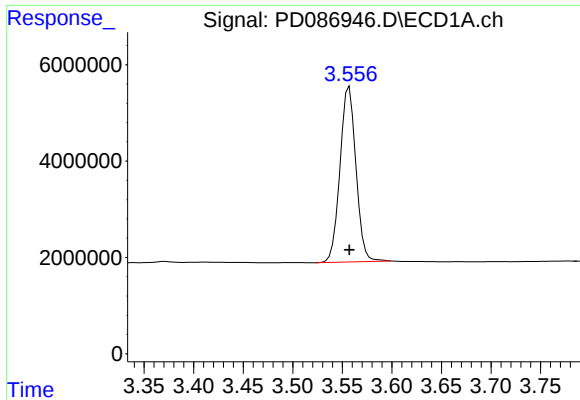

#1 Tetrachloro-m-xylene


R.T.: 3.557 min
Delta R.T.: 0.000 min
Response: 40763452
Conc: 20.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

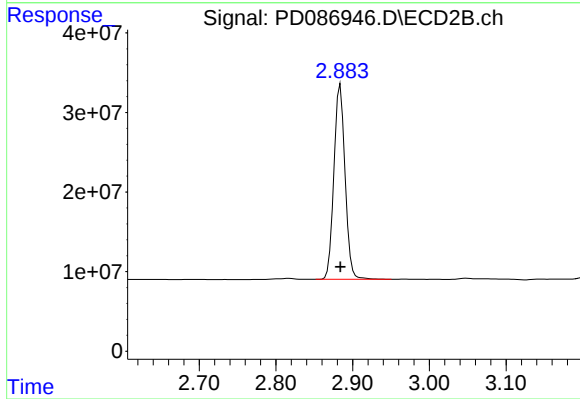


#1 Tetrachloro-m-xylene

R.T.: 2.884 min
Delta R.T.: 0.000 min
Response: 247138182
Conc: 21.59 ng/ml

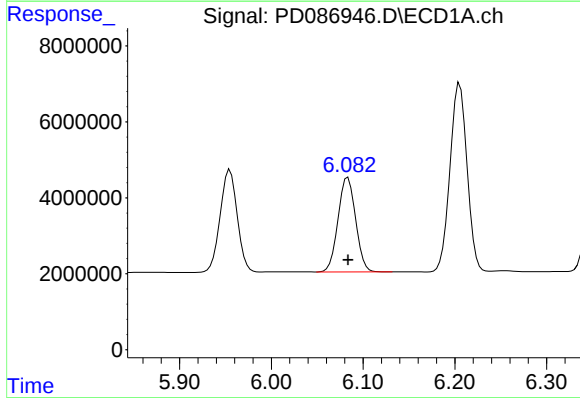


#9 Endosulfan I

R.T.: 6.084 min
Delta R.T.: 0.000 min
Response: 33253236
Conc: 9.91 ng/ml

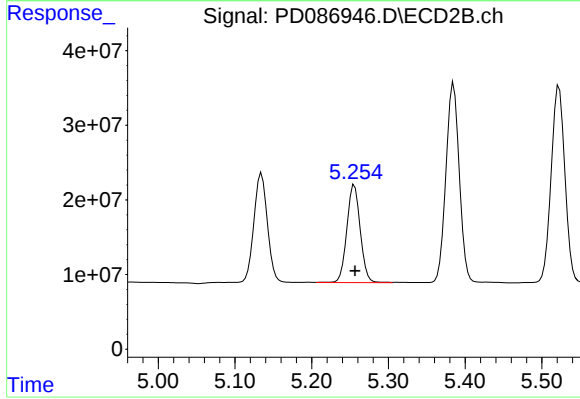

#9 Endosulfan I


R.T.: 5.256 min
Delta R.T.: 0.000 min
Response: 160691906
Conc: 11.32 ng/ml

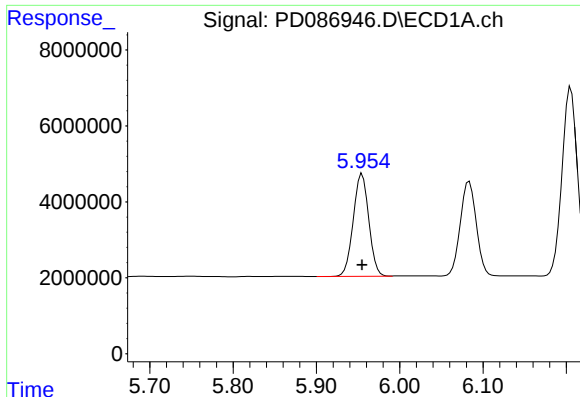

#10 gamma-Chlordane


R.T.: 5.955 min
Delta R.T.: 0.000 min
Response: 35074611
Conc: 9.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

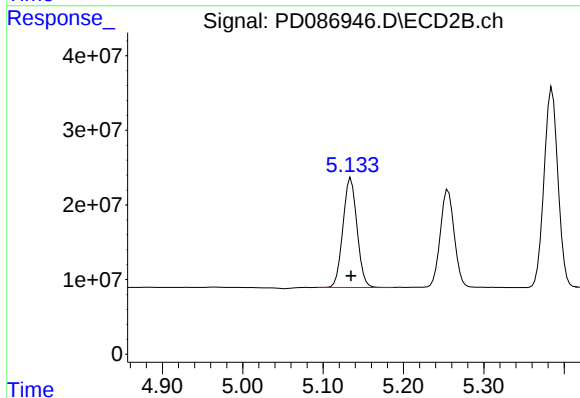


#10 gamma-Chlordane

R.T.: 5.135 min
Delta R.T.: 0.000 min
Response: 179153290
Conc: 11.52 ng/ml

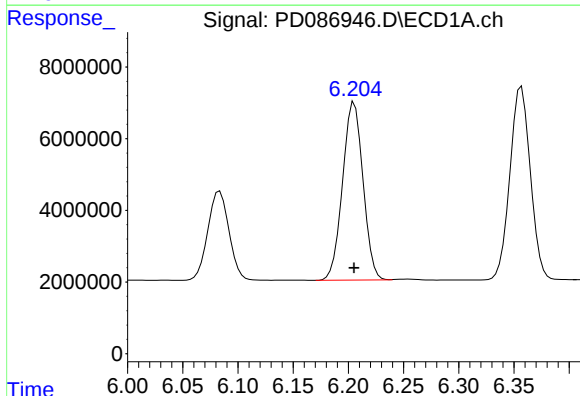


#12 4,4'-DDE

R.T.: 6.205 min
Delta R.T.: 0.000 min
Response: 64098695
Conc: 19.70 ng/ml

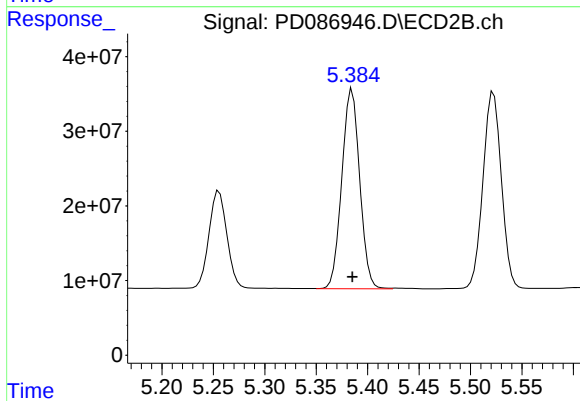

#12 4,4'-DDE


R.T.: 5.385 min
Delta R.T.: 0.000 min
Response: 324258463
Conc: 21.51 ng/ml

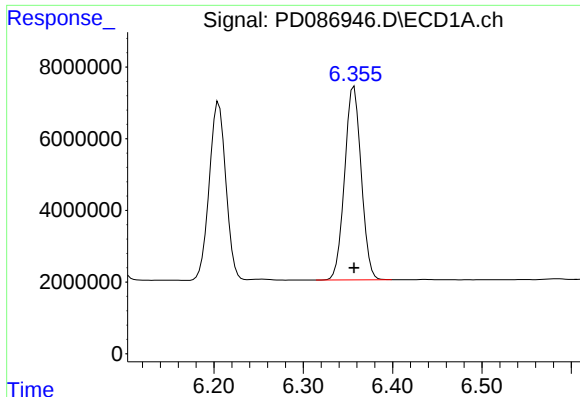

#13 Dieldrin


R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 69568570
Conc: 19.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

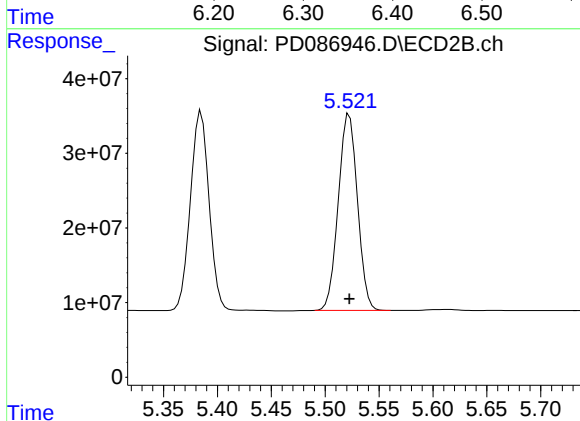


#13 Dieldrin

R.T.: 5.522 min
Delta R.T.: 0.000 min
Response: 326707069
Conc: 20.98 ng/ml

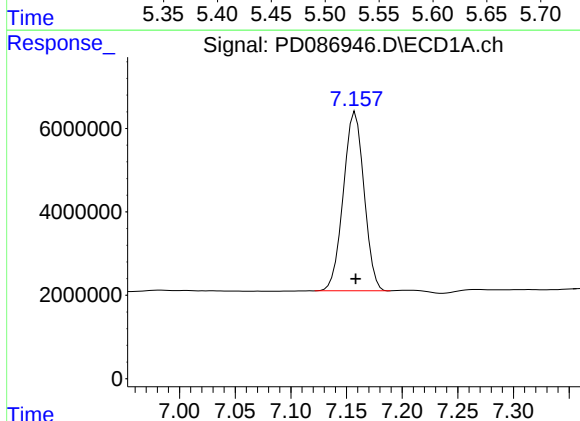


#19 Endosulfan Sulfate

R.T.: 7.158 min
Delta R.T.: 0.000 min
Response: 55616433
Conc: 19.11 ng/ml

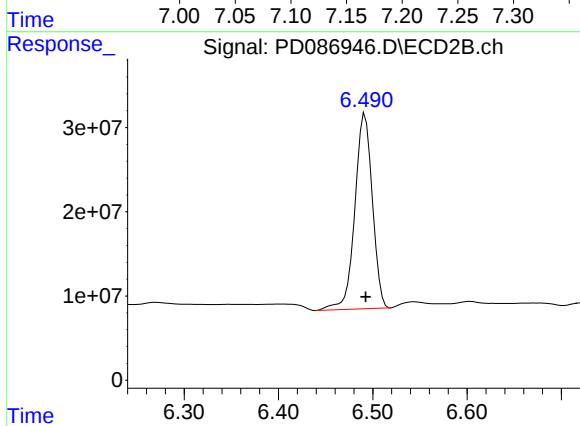

#19 Endosulfan Sulfate


R.T.: 6.492 min
Delta R.T.: 0.000 min
Response: 299343796
Conc: 22.12 ng/ml

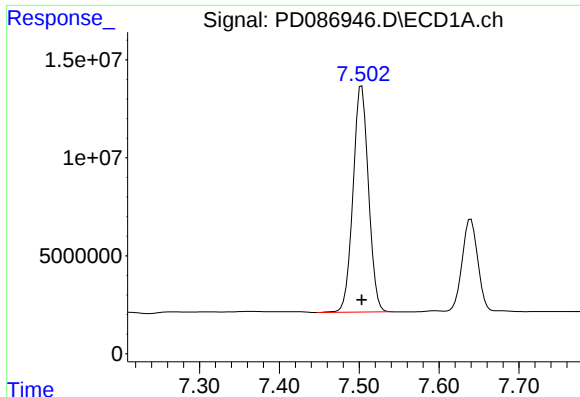

#20 Methoxychlor


R.T.: 7.503 min
Delta R.T.: 0.000 min
Response: 155472121
Conc: 97.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

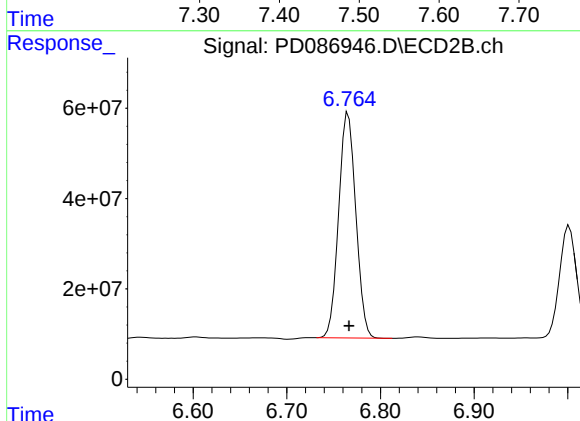


#20 Methoxychlor

R.T.: 6.766 min
Delta R.T.: 0.000 min
Response: 637512350
Conc: 88.87 ng/ml

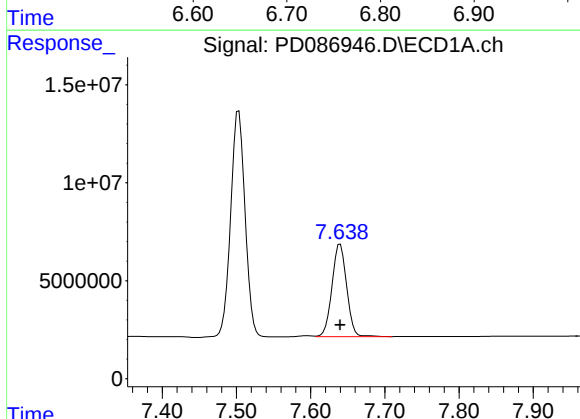


#21 Endrin ketone

R.T.: 7.640 min
Delta R.T.: 0.000 min
Response: 64894282
Conc: 20.00 ng/ml

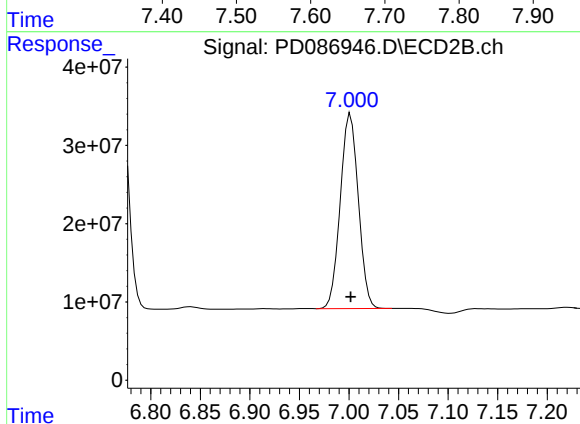

#21 Endrin ketone

R.T.: 7.002 min
Delta R.T.: 0.000 min
Response: 316538342
Conc: 21.00 ng/ml

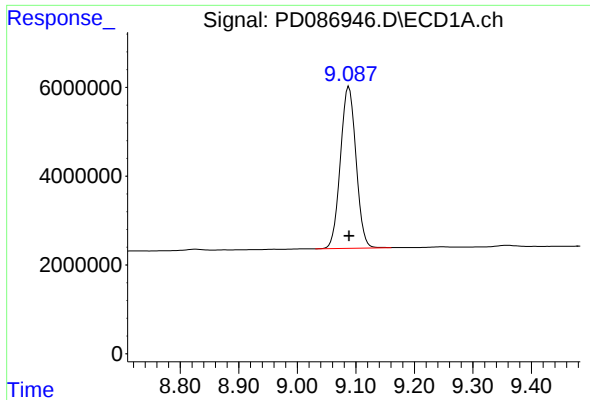

#28 Decachlorobiphenyl


R.T.: 9.088 min

Delta R.T.: 0.000 min

Response: 67435812

Conc: 21.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

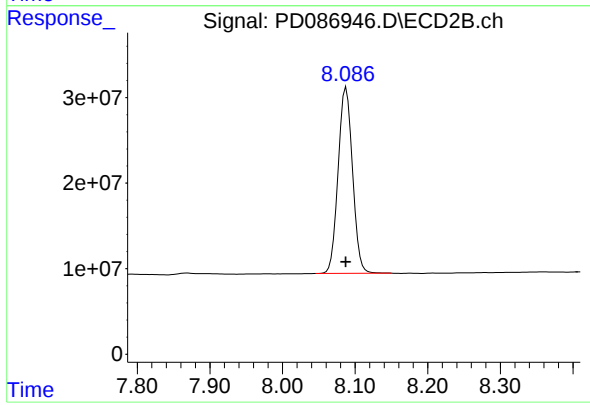

#28 Decachlorobiphenyl

R.T.: 8.088 min

Delta R.T.: 0.000 min

Response: 299575626

Conc: 21.50 ng/ml