

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120624\
 Data File : PP068874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 23:10
 Operator : YP\AJ
 Sample : P5123-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
ClientSampleId :
 1939-1915-BIDS-2A-2B-2C-BUILDING-CONCRETE

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2024
 Supervised By :Ankita Jodhani 12/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 00:14:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 11:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.758	4.048	25364506	21905653	26.132	22.623
2) SA Decachlor...	10.675	9.200	24561725	24190859	19.626	21.386m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120624\
Data File : PP068874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 23:10
Operator : YP\AJ
Sample : P5123-02
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
1939-1915-BIDS-2A-2B-2C-BUILDING-CONCRETE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2024
Supervised By :Ankita Jodhani 12/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 00:14:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

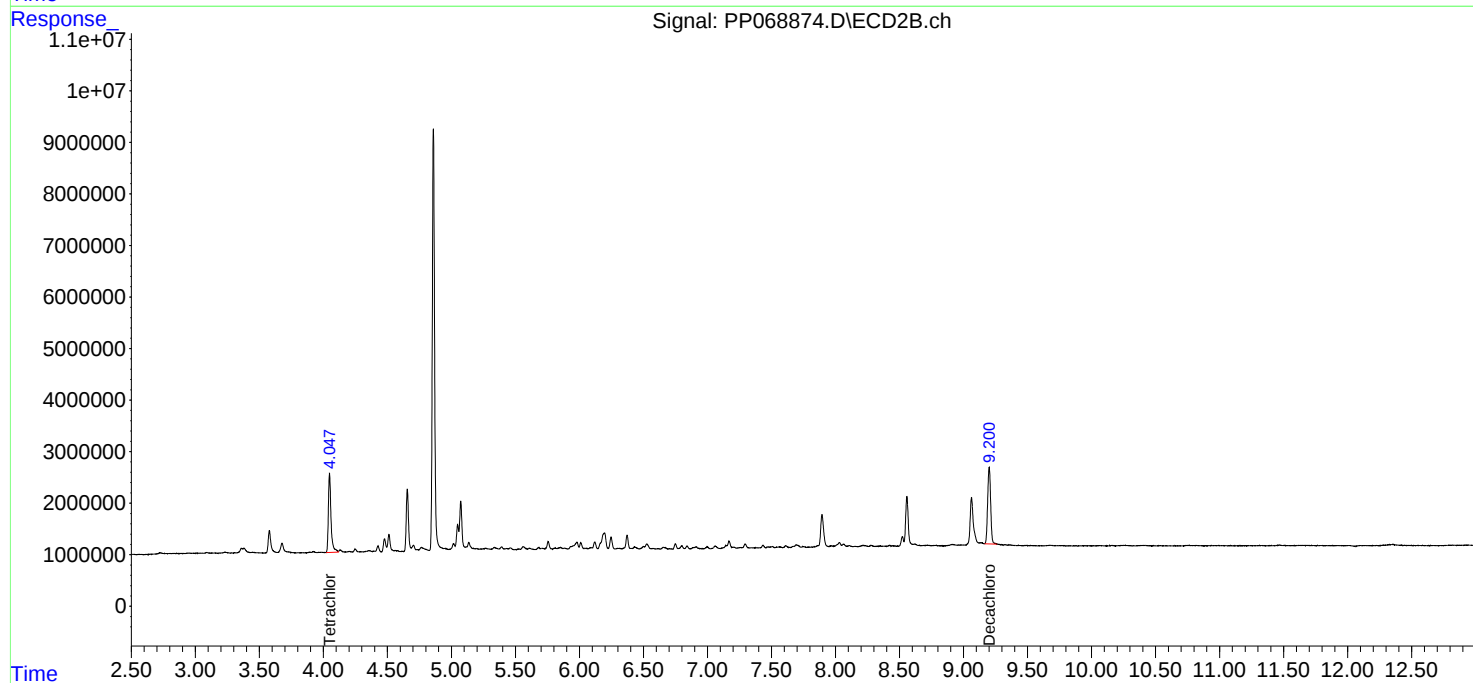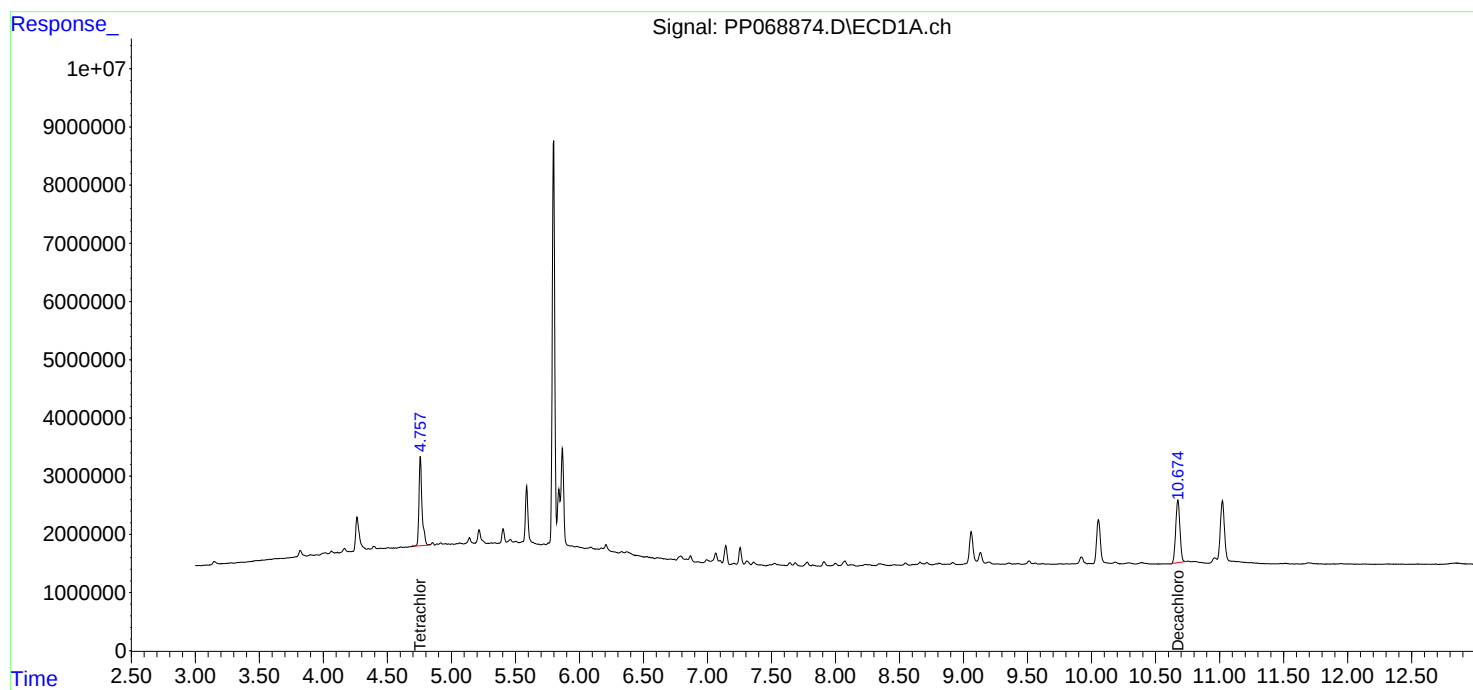

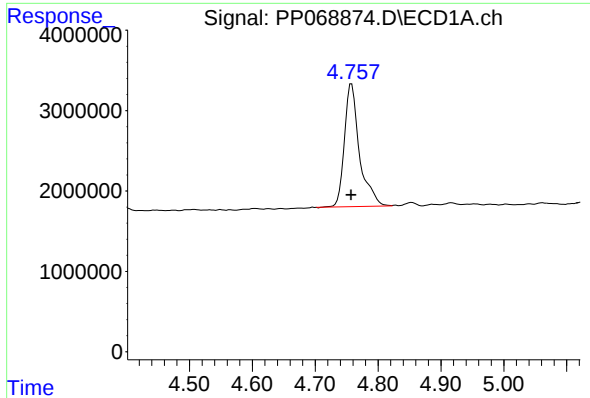

#1 Tetrachloro-m-xylene

R.T.: 4.758 min
Delta R.T.: 0.000 min
Response: 25364506
Conc: 26.13 ng/ml

Instrument :

ECD_P


ClientSampleId :

1939-1915-BIDS-2A-2B-2C-BUILDING-CONCRETE

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 12/09/2024
Supervised By :Ankita Jodhani 12/09/2024

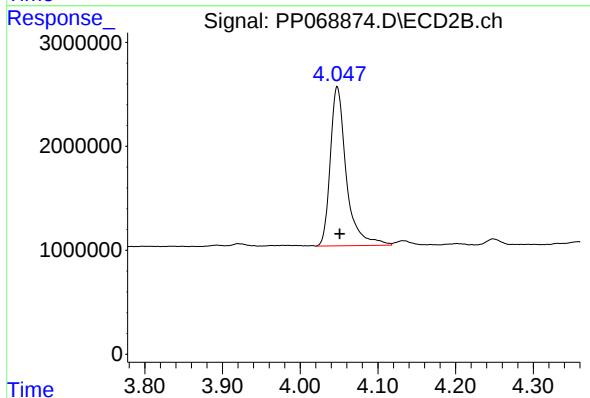


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: -0.003 min
Response: 21905653
Conc: 22.62 ng/ml

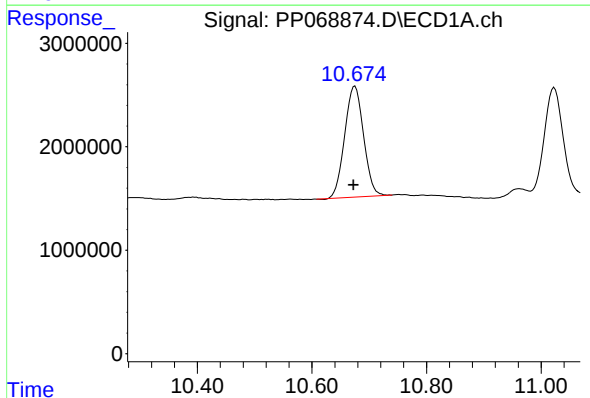

#2 Decachlorobiphenyl

R.T.: 10.675 min
Delta R.T.: 0.003 min
Response: 24561725
Conc: 19.63 ng/ml

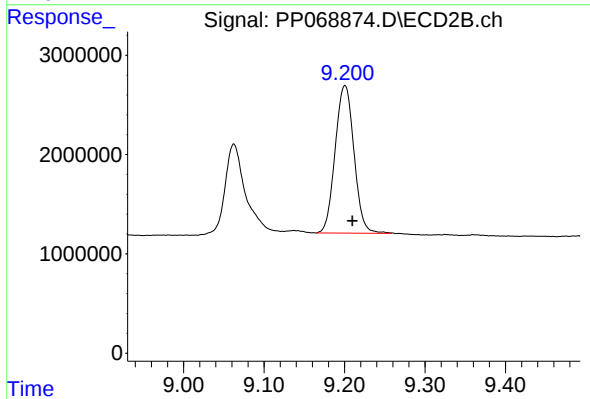

#2 Decachlorobiphenyl

R.T.: 9.200 min
Delta R.T.: -0.010 min
Response: 24190859
Conc: 21.39 ng/ml m