
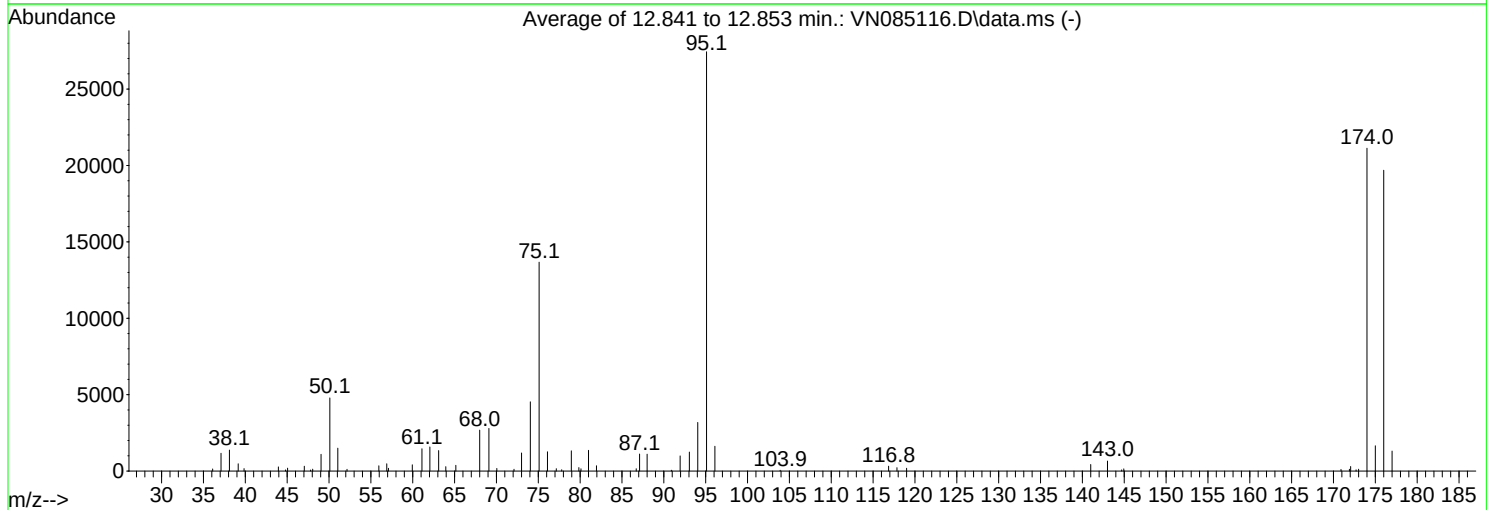


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN120624\
Data File : VN085116.D
Acq On : 06 Dec 2024 08:14
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N120624W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Dec 06 22:50:42 2024

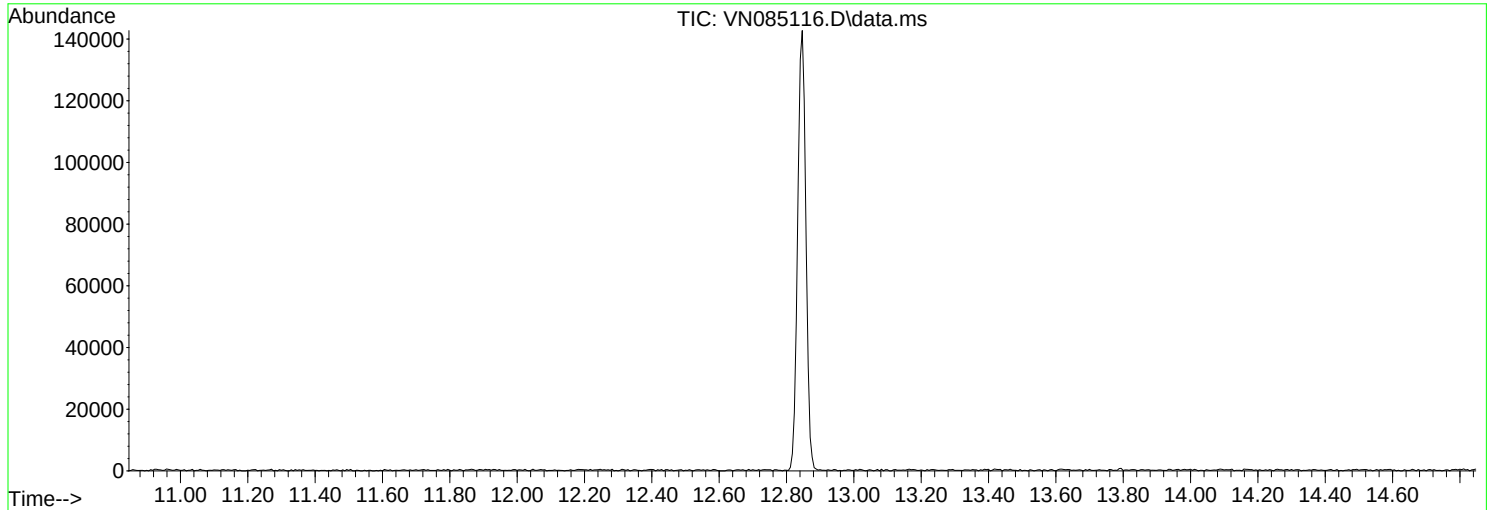

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	4787	PASS
75	95	30	60	49.8	13671	PASS
95	95	100	100	100.0	27445	PASS
96	95	5	9	5.9	1624	PASS
173	174	0.00	2	0.6	123	PASS
174	95	50	100	77.0	21131	PASS
175	174	5	9	7.8	1656	PASS
176	174	95	101	93.2	19688	FAIL*
177	176	5	9	6.7	1311	PASS