


LB133852

245.1

INSTRUMENT ID: CV1

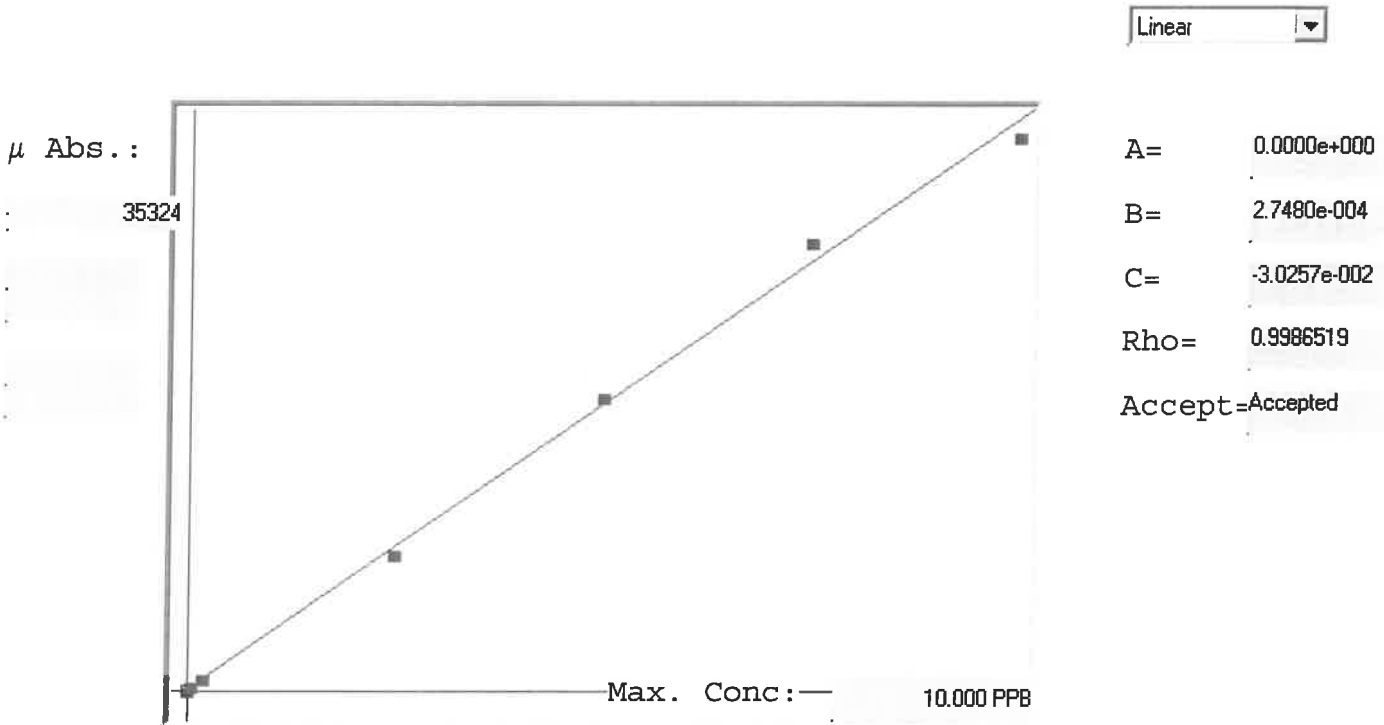

| Std ID | Conc.  | Calc.  | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 | 0/0/1) |
|--------|--------|--------|--------|-------|------------|-------|-------|-------|-------|-------|--------|
| 0.0    | 0.000  | -0.020 | -0.020 | 36    | 0.000      | 36    |       |       |       |       | 1      |
| 0.05   | 0.050  | 0.051  | 0.001  | 297   | 0.0 %      | 297   | 0     |       |       |       | 2      |
| 0.2    | 0.200  | 0.183  | -0.017 | 777   | 0.0 %      | 777   |       |       |       |       | 9      |
| 2.5    | 2.500  | 2.383  | -0.117 | 8781  | 0.0 %      | 8781  |       |       |       |       | 1      |
| 5.0    | 5.000  | 5.121  | 0.121  | 18746 | 0.0 %      | 18746 |       |       |       |       | 5      |
| 7.5    | 7.500  | 7.855  | 0.355  | 28696 | 0.0 %      | 28696 |       |       |       |       | 2      |
| 10.0   | 10.000 | 9.677  | -0.323 | 35324 | 0.0 %      | 35324 |       |       |       |       | 5      |

# LB133852 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 10 Dec 2024 09:29:03

| Sample ID       | Extended ID               | µ Abs | Conc    | Std Conc | Method | Units | Date                 | Type | Type |
|-----------------|---------------------------|-------|---------|----------|--------|-------|----------------------|------|------|
| 0.0 - 1         | 30                        | 38    | -       | 0.000    | 245.1  | PPB   | 10 Dec 2024 09:37:35 | S    | Std  |
| 0.05 - 1        | 50.05                     | 297   | -       | 0.050    | 245.1  | PPB   | 10 Dec 2024 09:42:31 | S    | Std  |
| 0.2 - 1         | 50.2                      | 777   | -       | 0.200    | 245.1  | PPB   | 10 Dec 2024 09:44:48 | S    | Std  |
| 2.5 - 1         | 52.5                      | 8781  | -       | 2.500    | 245.1  | PPB   | 10 Dec 2024 09:47:04 | S    | Std  |
| 5.0 - 1         | 55                        | 18746 | -       | 5.000    | 245.1  | PPB   | 10 Dec 2024 09:49:20 | S    | Std  |
| 7.5 - 1         | 57.5                      | 28696 | -       | 7.500    | 245.1  | PPB   | 10 Dec 2024 09:51:37 | S    | Std  |
| 10.0 - 1        | 510                       | 35324 | -       | 10.000   | 245.1  | PPB   | 10 Dec 2024 09:59:28 | S    | Std  |
| ICV14 - 1       | ICV14                     | 14778 | 4.0307  | -245.1   |        | PPB   | 10 Dec 2024 10:09:31 | U    | SMPL |
| ICB14 - 1       | ICB14                     | -6    | -0.0319 | -245.1   |        | PPB   | 10 Dec 2024 10:17:09 | U    | SMPL |
| CCV10 - 1       | CCV10                     | 19970 | 5.4574  | -245.1   |        | PPB   | 10 Dec 2024 10:29:43 | U    | SMPL |
| CCB10 - 1       | CCB10                     | 48    | -0.0171 | -245.1   |        | PPB   | 10 Dec 2024 10:34:42 | U    | SMPL |
| CRA - 1         | CRA                       | 248   | 0.0379  | -245.1   |        | PPB   | 10 Dec 2024 10:39:32 | U    | SMPL |
| HighStd - 1     | HighStd                   | 31722 | 8.6868  | -245.1   |        | PPB   | 10 Dec 2024 10:49:15 | U    | SMPL |
| ChkStd - 1      | ChkStd                    | 23934 | 6.5467  | -245.1   |        | PPB   | 10 Dec 2024 10:51:31 | U    | SMPL |
| PB165519BL - 1  | PBW                       | -208  | -0.0874 | -245.1   |        | PPB   | 10 Dec 2024 10:53:49 | U    | SMPL |
| PB165519BS - 1  | LCWS                      | 14515 | 3.9584  | -245.1   |        | PPB   | 10 Dec 2024 11:02:20 | U    | SMPL |
| P4368-10 - 1    | LOD-MDL-WATER-04-QT4-2024 | 233   | 0.0338  | -245.1   |        | PPB   | 10 Dec 2024 11:12:18 | U    | SMPL |
| P4368-11 - 1    | LOQ-WATER-05-QT4-2024     | 925   | 0.2239  | -245.1   |        | PPB   | 10 Dec 2024 11:14:34 | U    | SMPL |
| P5051-07 - 1    | 14B-(1-4)-COMP            | 4142  | 1.1079  | -245.1   |        | PPB   | 10 Dec 2024 11:16:51 | U    | SMPL |
| P5068-07 - 1    | 14B-(1-4)-COMP            | 3264  | 0.8667  | -245.1   |        | PPB   | 10 Dec 2024 11:19:08 | U    | SMPL |
| P5192-02 - 1    | EFF-WASTE WATER           | 98    | -0.0033 | -245.1   |        | PPB   | 10 Dec 2024 11:21:26 | U    | SMPL |
| CCV11 - 1       | CCV11                     | 17194 | 4.6946  | -245.1   |        | PPB   | 10 Dec 2024 11:26:17 | U    | SMPL |
| CCB11 - 1       | CCB11                     | 6     | -0.0286 | -245.1   |        | PPB   | 10 Dec 2024 11:31:06 | U    | SMPL |
| P5192-02DUP - 1 | EFF-WASTE WATERDUP        | 73    | -0.0102 | -245.1   |        | PPB   | 10 Dec 2024 11:33:20 | U    | SMPL |
| P5192-02MS - 1  | EFF-WASTE WATERMS         | 13290 | 3.6218  | -245.1   |        | PPB   | 10 Dec 2024 11:35:35 | U    | SMPL |
| P5192-02MSD - 1 | EFF-WASTE WATERMSD        | 14418 | 3.9318  | -245.1   |        | PPB   | 10 Dec 2024 11:37:51 | U    | SMPL |
| P5192-02LX5 - 1 |                           | -187  | -0.0816 | -245.1   |        | PPB   | 10 Dec 2024 11:40:09 | U    | SMPL |
| P5192-02A - 1   |                           | 13463 | 3.6693  | -245.1   |        | PPB   | 10 Dec 2024 11:42:27 | U    | SMPL |
| CCV12 - 1       | CCV12                     | 19587 | 5.3522  | -245.1   |        | PPB   | 10 Dec 2024 11:44:43 | U    | SMPL |
| CCB12 - 1       | CCB12                     | 2     | -0.0297 | -245.1   |        | PPB   | 10 Dec 2024 11:49:38 | U    | SMPL |