

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121024\
 Data File : P0108451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2024 17:43
 Operator : YP/AJ
 Sample : P5217-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MIXED-DEMO

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 00:34:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.709	3.707	108.4E6	56212172	12.464	11.089
2) SA Decachlor...	8.784	8.732	60711459	38575311	8.312	9.955

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121024\
Data File : PO108451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2024 17:43
Operator : YP/AJ
Sample : P5217-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MIXED-DEMO

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 00:34:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

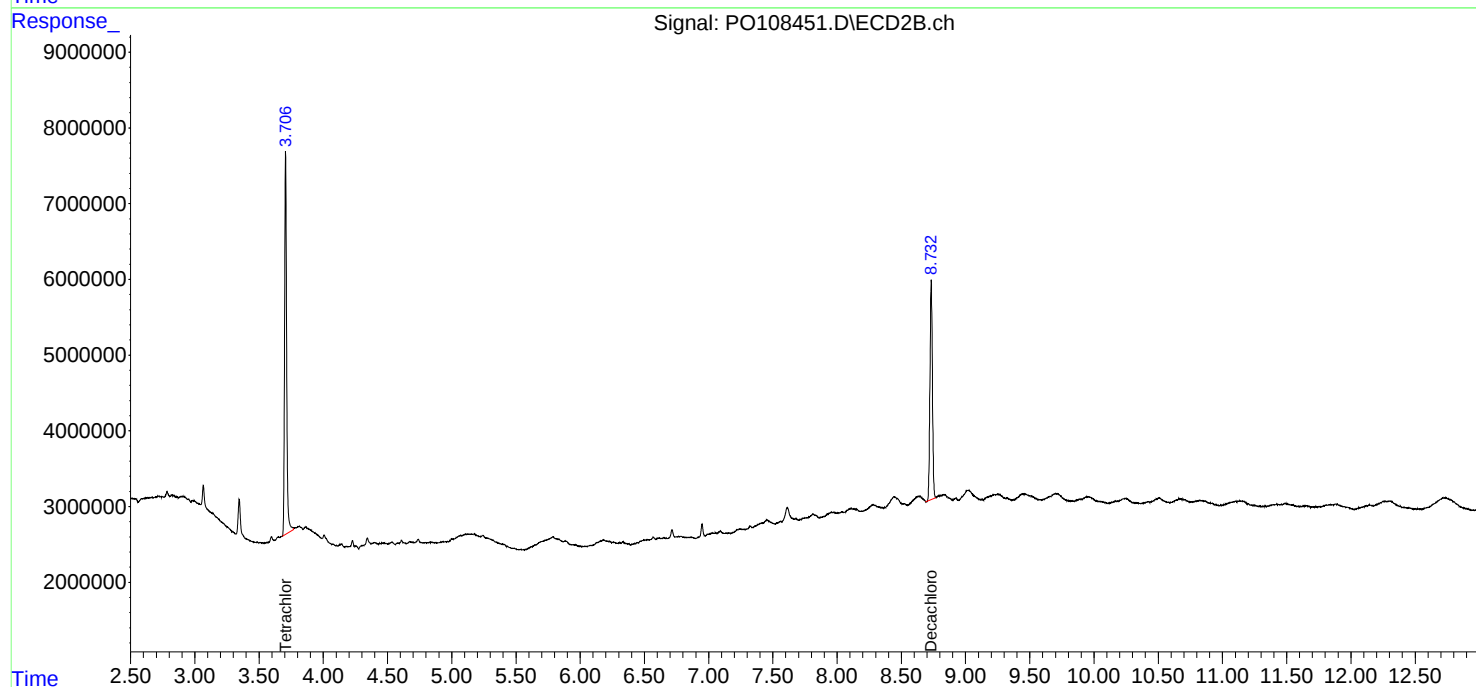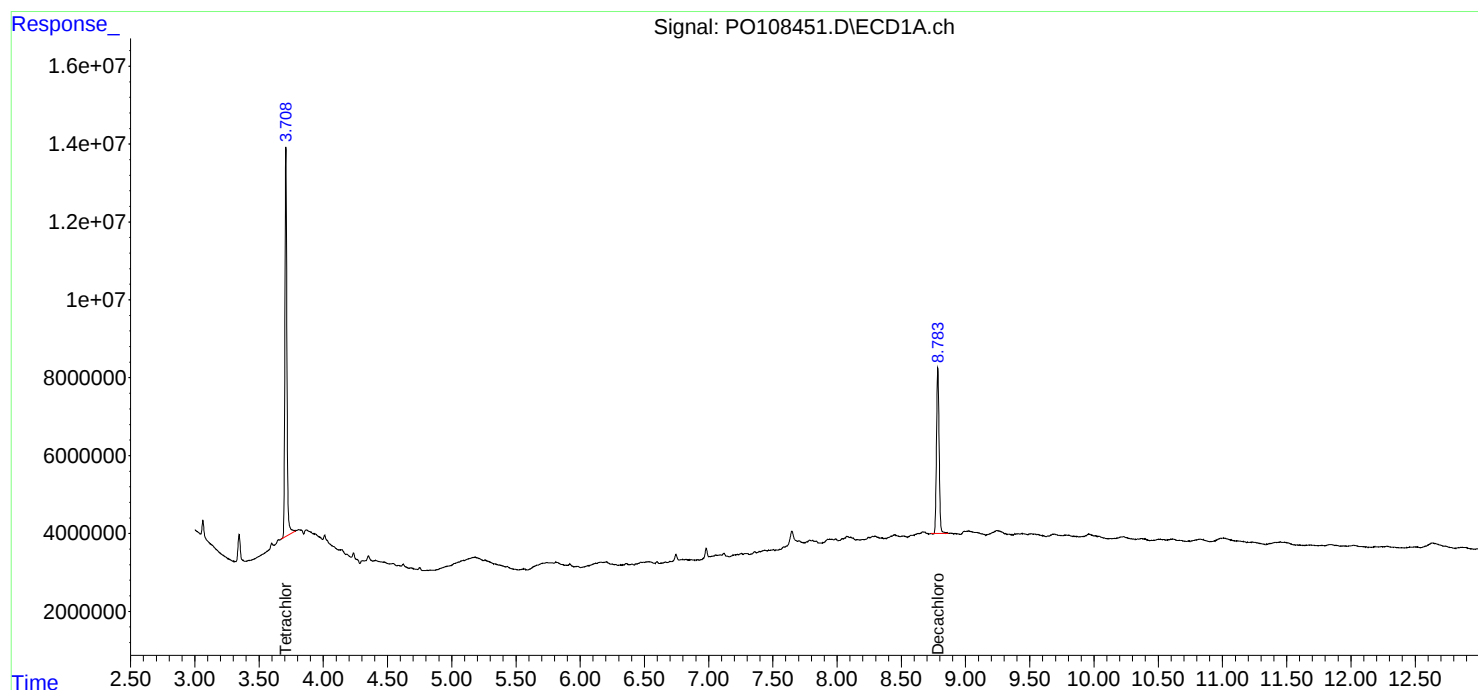


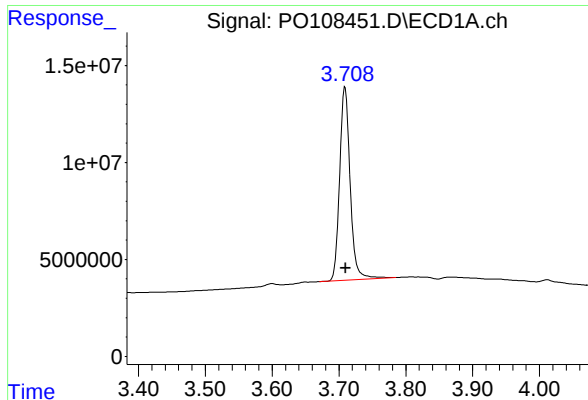

#1 Tetrachloro-m-xylene


R.T.: 3.709 min
Delta R.T.: 0.000 min
Response: 108441038
Conc: 12.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
MIXED-DEMO

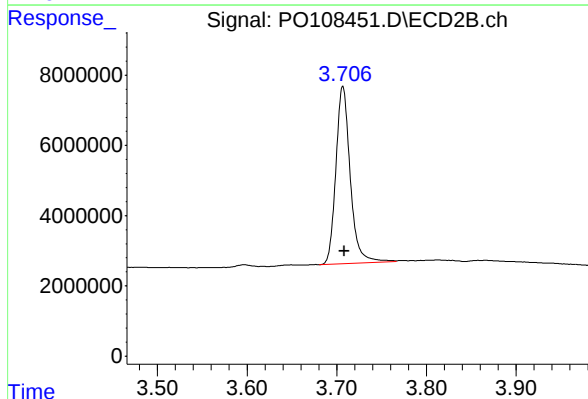


#1 Tetrachloro-m-xylene

R.T.: 3.707 min
Delta R.T.: -0.002 min
Response: 56212172
Conc: 11.09 ng/ml

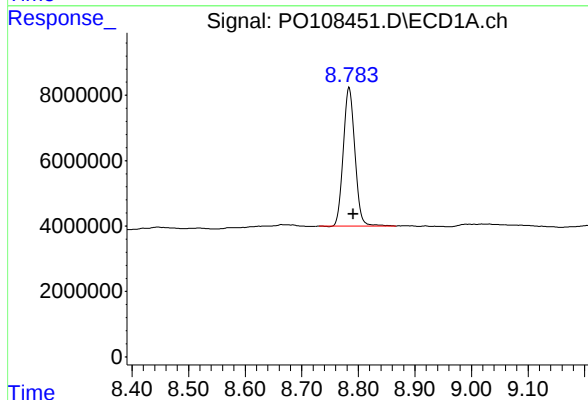

#2 Decachlorobiphenyl

R.T.: 8.784 min
Delta R.T.: -0.007 min
Response: 60711459
Conc: 8.31 ng/ml

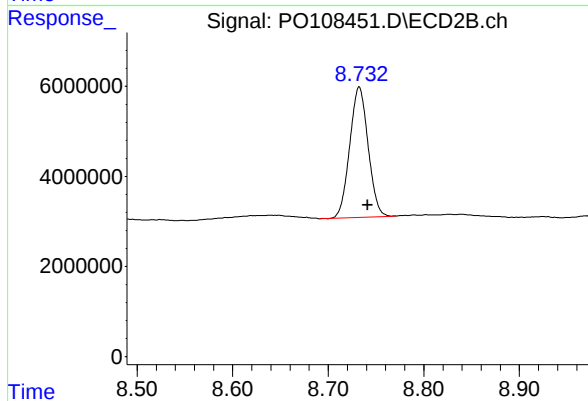

#2 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.009 min
Response: 38575311
Conc: 9.96 ng/ml