

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121224\
 Data File : P0108523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2024 09:56
 Operator : YP/AJ
 Sample : P5225-03DL 30X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 3A-3B-3C-ABDL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/13/2024
 Supervised By :Ankita Jodhani 12/13/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 06:41:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

26)	L6	AR-1254-1	5.616	5.596	670.2E6	404.2E6	1304.896	1492.271
27)	L6	AR-1254-2	5.764	5.743	504.3E6	301.3E6	1107.323	1255.315
28)	L6	AR-1254-3	6.171	6.147	694.0E6	395.6E6	963.719m	1053.397m
29)	L6	AR-1254-4	6.401	6.375	185.2E6	103.0E6	422.076	473.390
30)	L6	AR-1254-5	6.822	6.793	209.4E6	117.3E6	329.666	363.392

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121224\
Data File : PO108523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2024 09:56
Operator : YP/AJ
Sample : P5225-03DL 30X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
3A-3B-3C-ABDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/13/2024
Supervised By :Ankita Jodhani 12/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 06:41:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

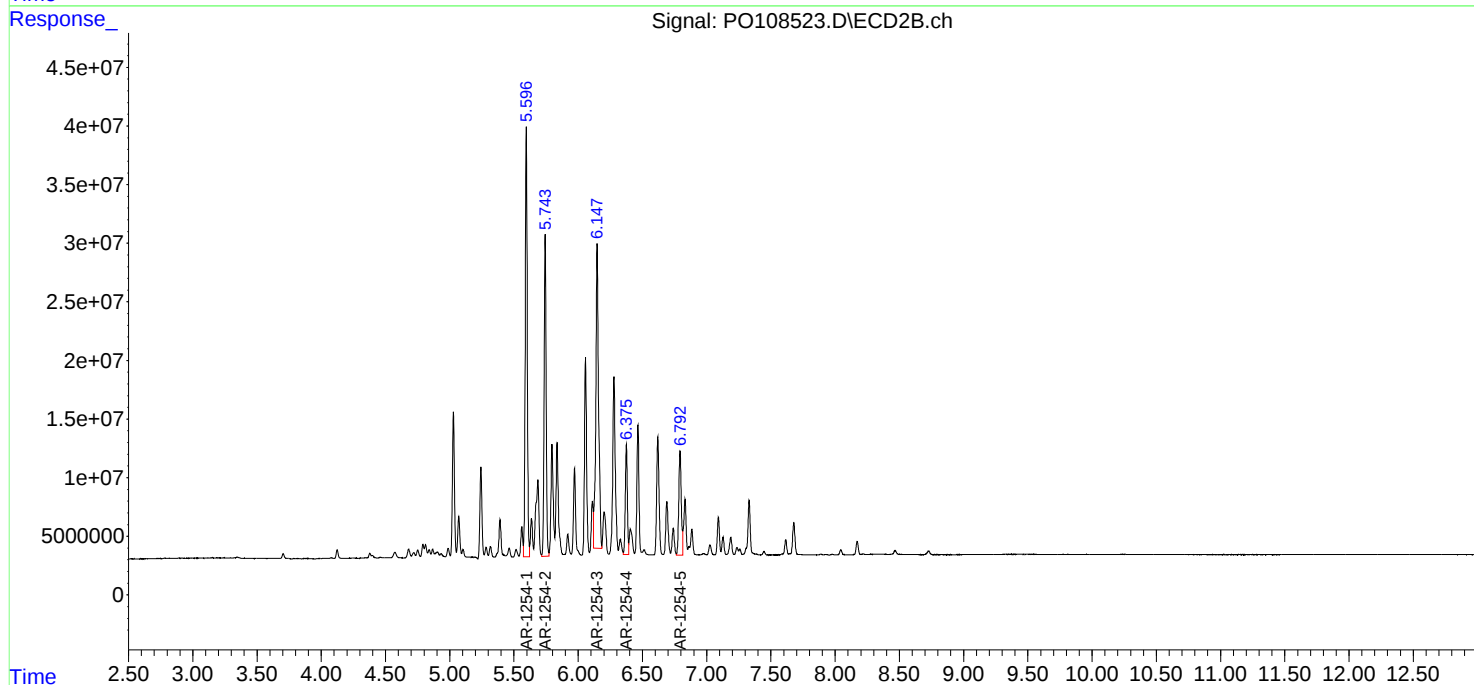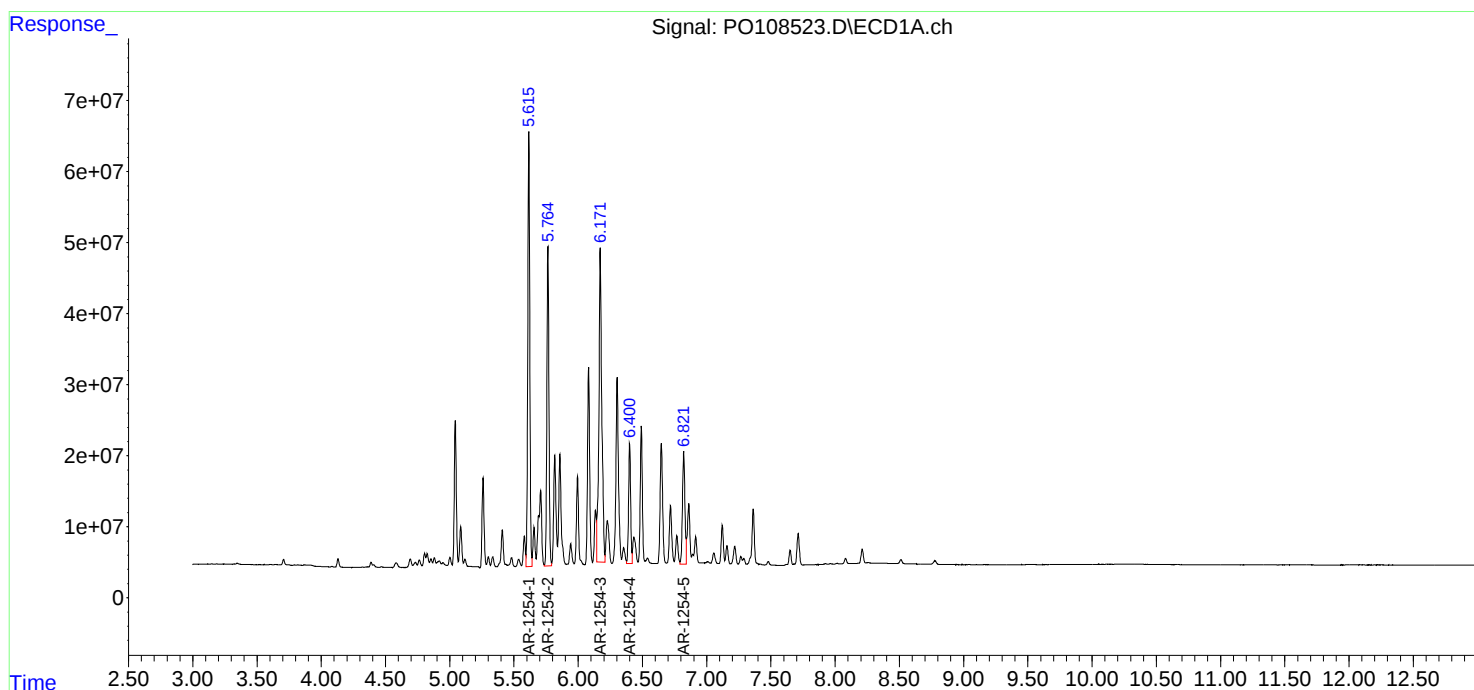

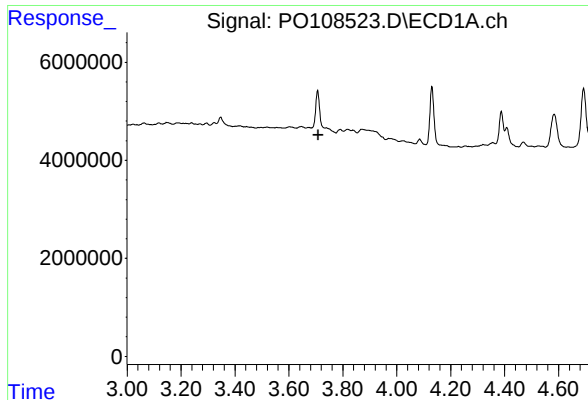


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
3A-3B-3C-ABDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/13/2024
Supervised By :Ankita Jodhani 12/13/2024

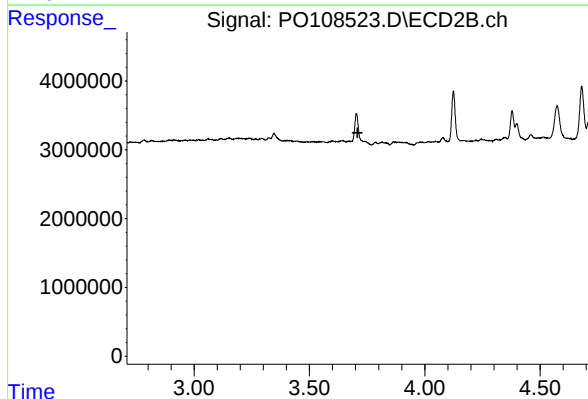


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.708 min
Response: 0
Conc: N.D.

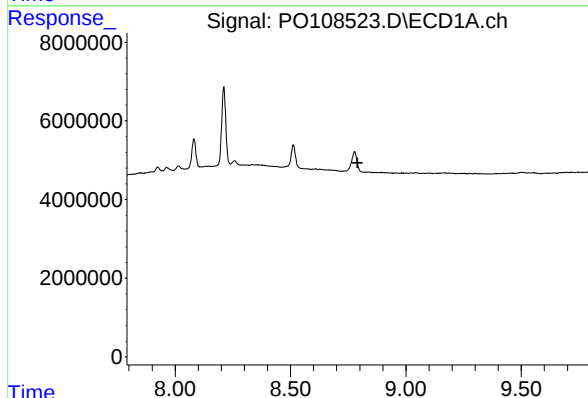


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

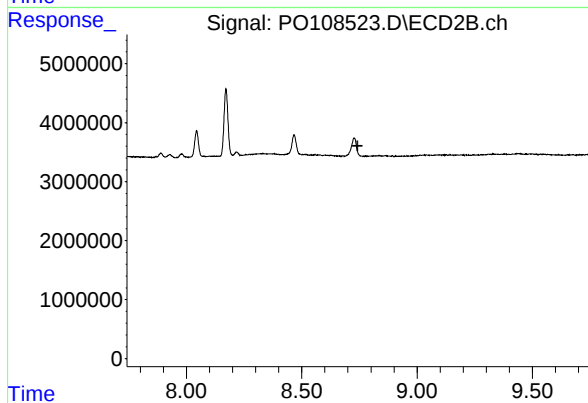

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.741 min
Response: 0
Conc: N.D.

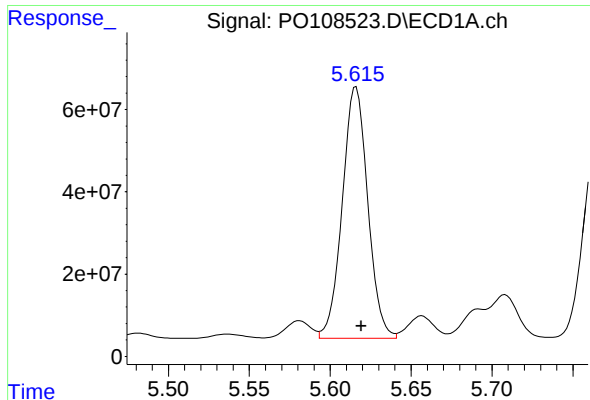


#26 AR-1254-1

R.T.: 5.616 min
Delta R.T.: -0.003 min
Response: 670247397
Conc: 1304.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
3A-3B-3C-ABDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/13/2024
Supervised By :Ankita Jodhani 12/13/2024

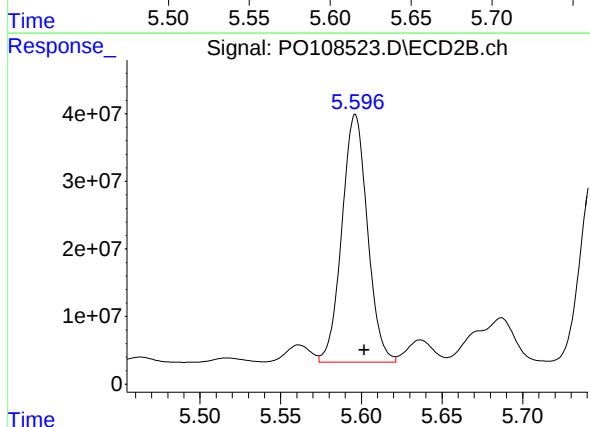


#26 AR-1254-1

R.T.: 5.596 min
Delta R.T.: -0.006 min
Response: 404154831
Conc: 1492.27 ng/ml

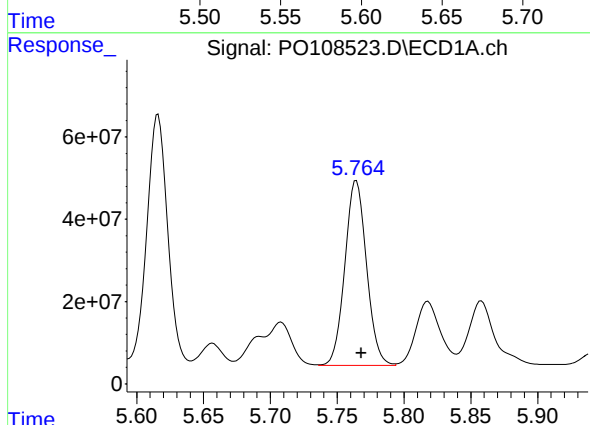


#27 AR-1254-2

R.T.: 5.764 min
Delta R.T.: -0.004 min
Response: 504339109
Conc: 1107.32 ng/ml

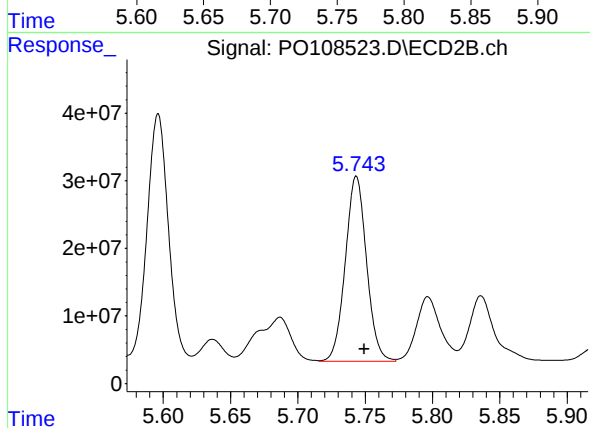

#27 AR-1254-2

R.T.: 5.743 min
Delta R.T.: -0.006 min
Response: 301301252
Conc: 1255.32 ng/ml

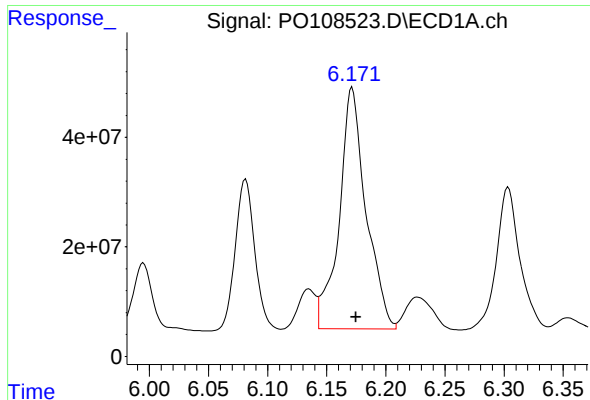


#28 AR-1254-3

R.T.: 6.171 min
Delta R.T.: -0.004 min
Response: 694001332
Conc: 963.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
3A-3B-3C-ABDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/13/2024
Supervised By :Ankita Jodhani 12/13/2024

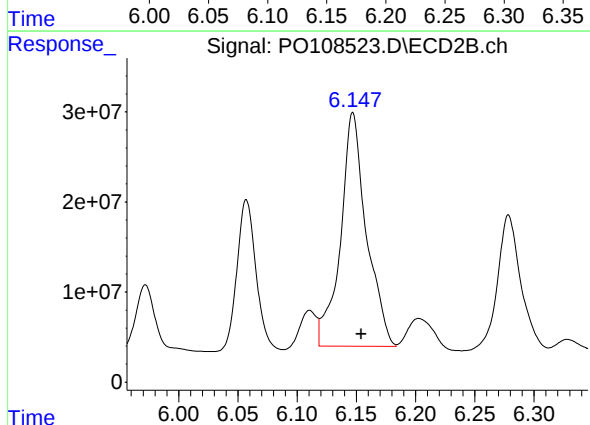


#28 AR-1254-3

R.T.: 6.147 min
Delta R.T.: -0.008 min
Response: 395562453
Conc: 1053.40 ng/ml

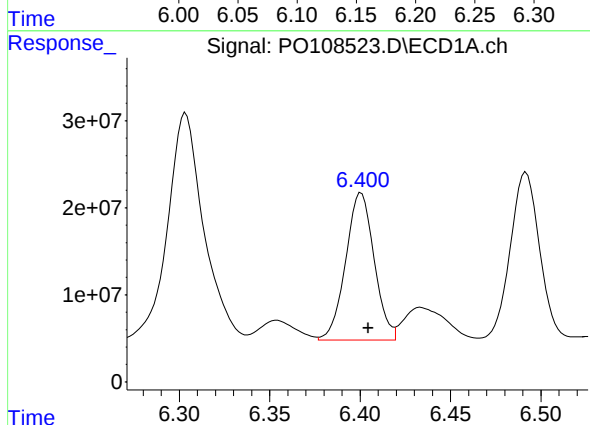


#29 AR-1254-4

R.T.: 6.401 min
Delta R.T.: -0.004 min
Response: 185212276
Conc: 422.08 ng/ml

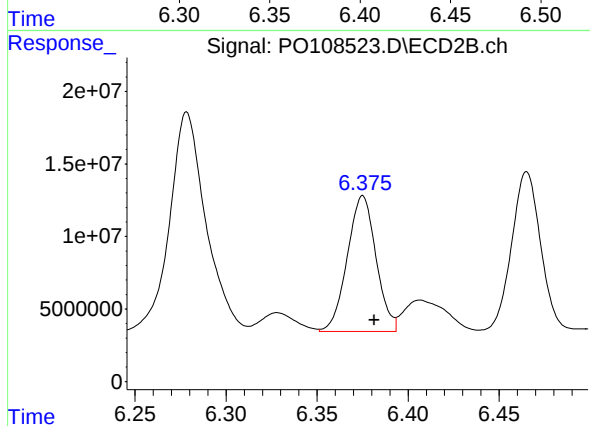

#29 AR-1254-4

R.T.: 6.375 min
Delta R.T.: -0.006 min
Response: 103046272
Conc: 473.39 ng/ml

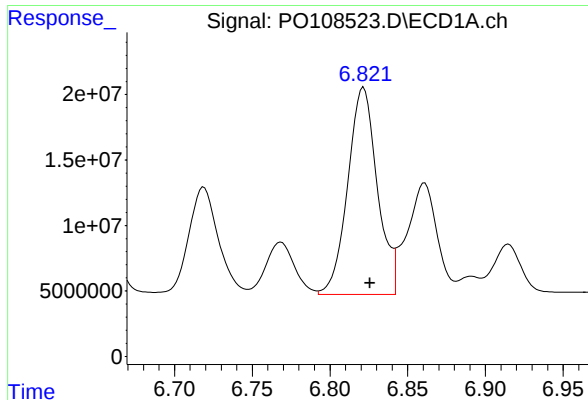


#30 AR-1254-5

R.T.: 6.822 min
Delta R.T.: -0.004 min
Response: 209378030
Conc: 329.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
3A-3B-3C-ABDL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/13/2024
Supervised By :Ankita Jodhani 12/13/2024

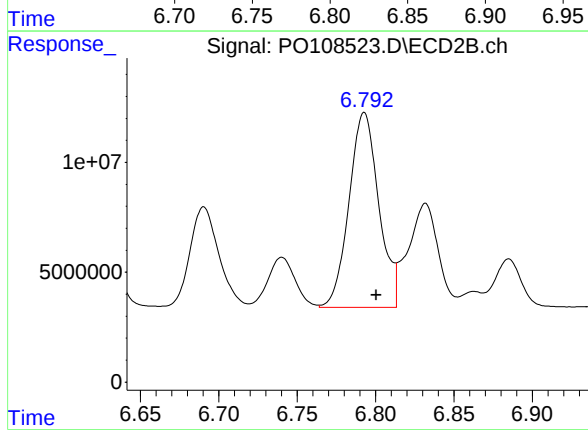

#30 AR-1254-5

R.T.: 6.793 min
Delta R.T.: -0.008 min
Response: 117288408
Conc: 363.39 ng/ml