


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121924\
Data File : BN035711.D
Acq On : 19 Dec 2024 18:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 19 23:06:19 2024

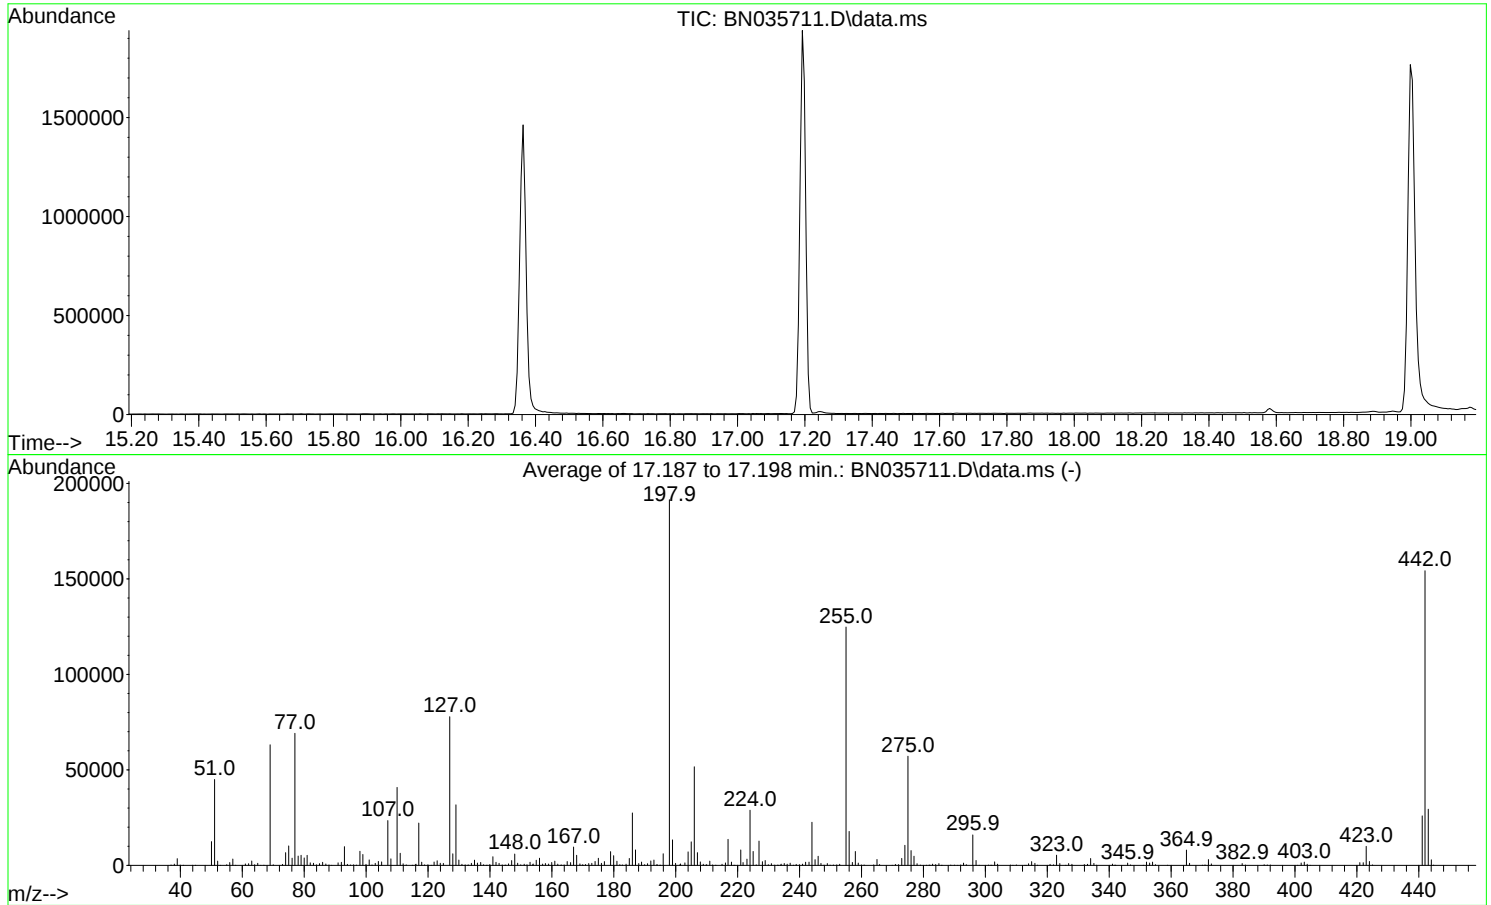




AutoFind: Scans 2431, 2432, 2433; Background Corrected with Scan 2425

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.5	44968	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.0	63147	PASS
70	69	0.00	2	0.5	327	PASS
127	198	10	80	40.6	77835	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	191488	PASS
199	198	5	9	7.0	13338	PASS
275	198	10	60	29.9	57160	PASS
365	198	1	100	4.2	8014	PASS
441	198	0.01	100	13.5	25920	PASS
442	442	50	100	100.0	154288	PASS
443	442	15	24	19.1	29413	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121924\
Data File : BN035711.D
Acq On : 19 Dec 2024 18:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 20 01:29:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 01:29:08 2024
Response via : Initial Calibration

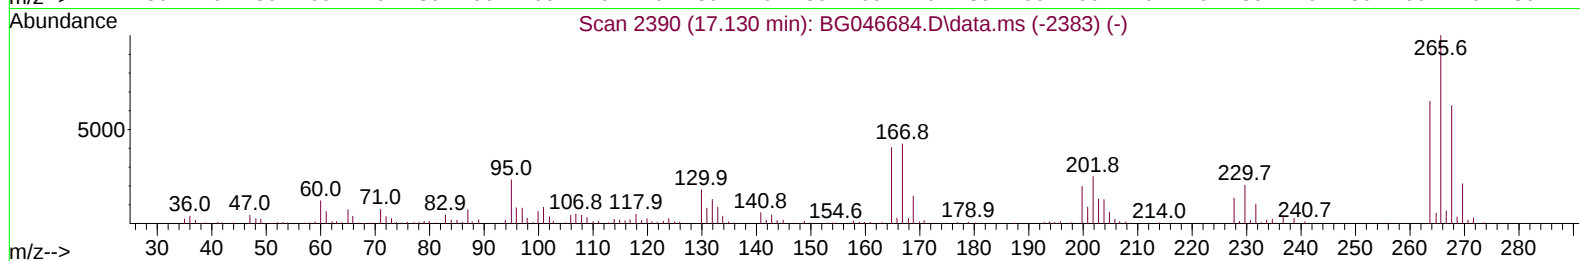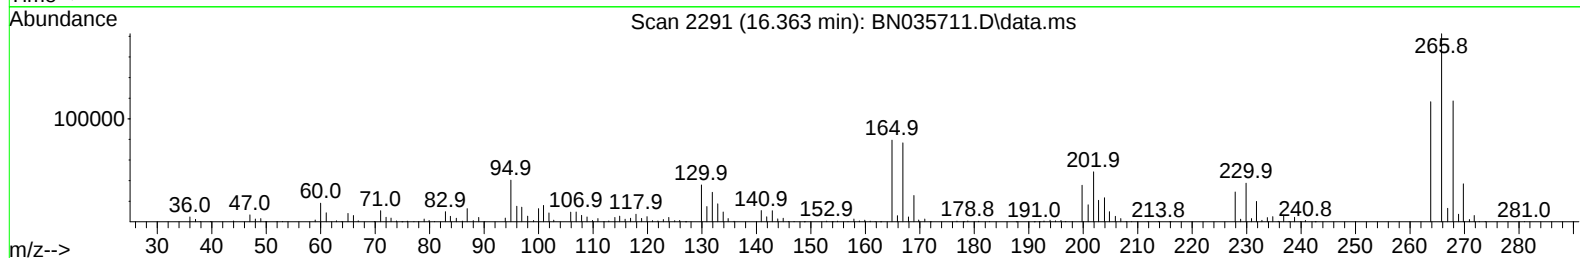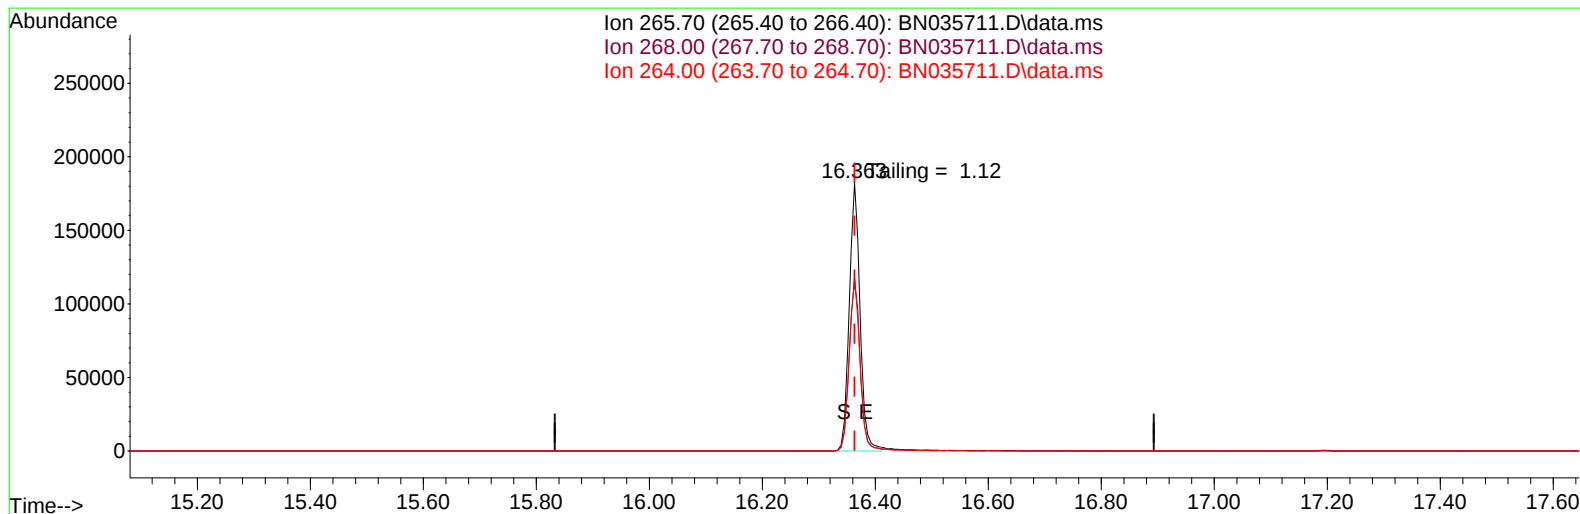

TIC: BN035711.D\data.ms

(70) Pentachlorophenol (C)

16.363min (0.000) 25694.23 ng




response 246608

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.25
264.00	61.60	63.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121924\
Data File : BN035711.D
Acq On : 19 Dec 2024 18:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 20 01:29:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 01:29:08 2024
Response via : Initial Calibration

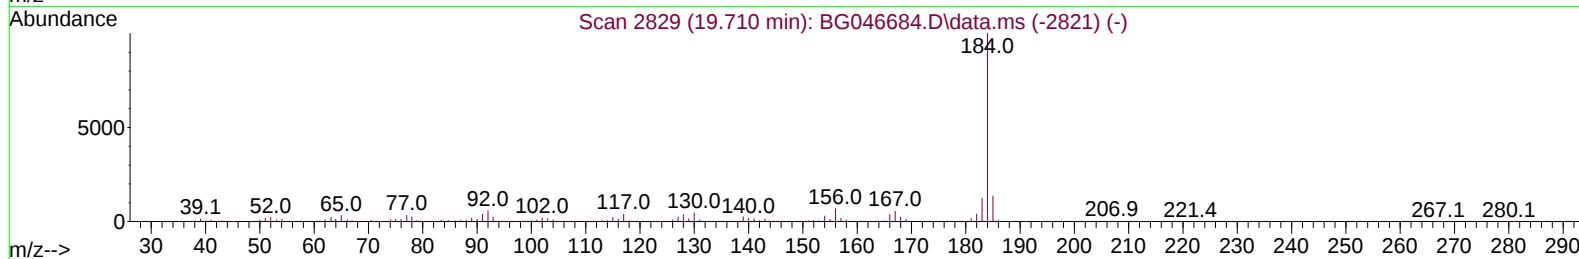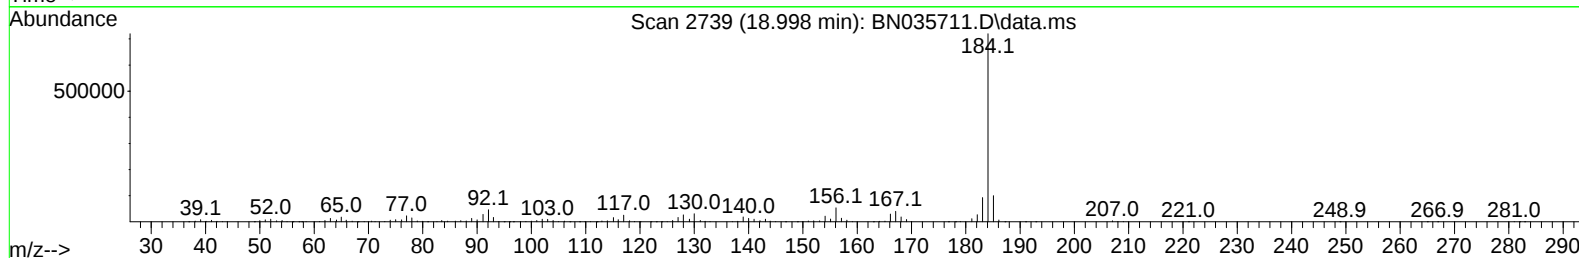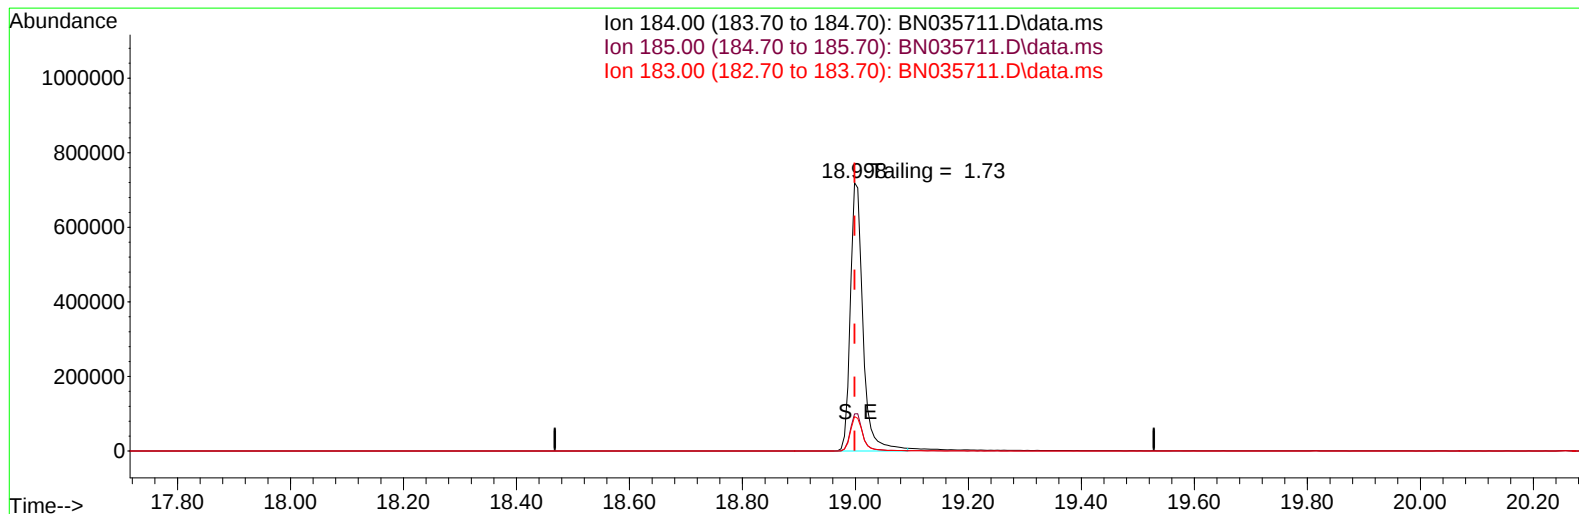

TIC: BN035711.D\data.ms

(77) Benzidine

18.998min (0.000) 0.00 ng

response 1146216

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.87
183.00	13.20	12.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/19/2024	BNA_N	<u>BN035711.D</u>
Compound Name	Response	Retention Time
DDT	267822	20.257
DDD	246838	19.816
DDE	1376	19.298
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
248214	516036	48.10

Instrument :
BNA_N
ClientSampleId :
DFTPP