

Clear table


Instrument ID: IC-2									
Analyst :				IZ		Method:		300.0 / 9056A	
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	Initial wt/ Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-111824	Final
STD2	0.402	0.571	0.601	1.961	0.489	1.025	3.062	IC1-111824	10 NF/IZ
STD3	0.794	1.185	1.175	3.939	0.997	1.928	6.062	IC1-111824	10 NF/IZ
STD4	1.023	1.554	1.535	5.128	1.284	2.665	7.843	IC1-111824	10 NF/IZ
STD5	1.997	3.009	2.993	9.997	2.488	4.960	14.679	IC1-111824	10 NF/IZ
STD6	3.936	5.952	5.978	19.928	4.964	9.645	28.993	IC1-111824	10 NF/IZ
STD7	5.049	7.529	7.517	25.045	6.279	12.776	37.863	IC1-111824	10 NF/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1									
STD2	0.5000	-4.8333	0.1667	-1.9500	-2.2000	2.5000	2.0667		
STD3	-0.7500	-1.2500	-2.0833	-1.5250	-0.3000	-3.6000	1.0333		
STD4	2.3000	3.6000	2.3333	2.5600	2.7200	6.6000	4.5733		
STD5	-0.1500	0.3000	-0.2333	-0.0300	-0.4800	-0.8000	-2.1400		
STD6	-1.6000	-0.8000	-0.3667	-0.3600	-0.7200	-3.5500	-3.3567		
STD7	0.9800	0.3867	0.2267	0.1800	0.4640	2.2080	2.3324		

Initial
wt/
Final

Analyst

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

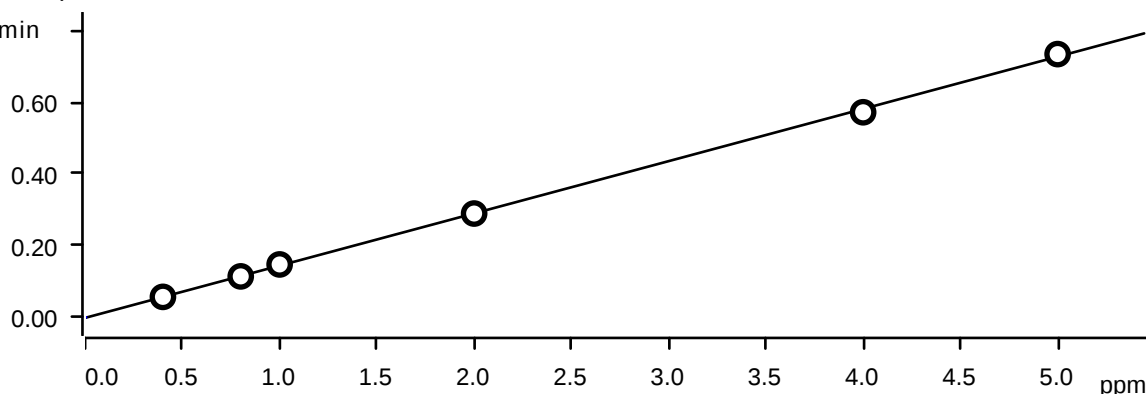

Function: $A = -1.48773E-3 + 0.0145652 \times Q$


Relative standard deviation: 1.923523 %

Correlation coefficient: 0.999800

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.114	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.147	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.289	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.572	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.734	STD7	2024-11-18 13:33:24 UTC-5	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

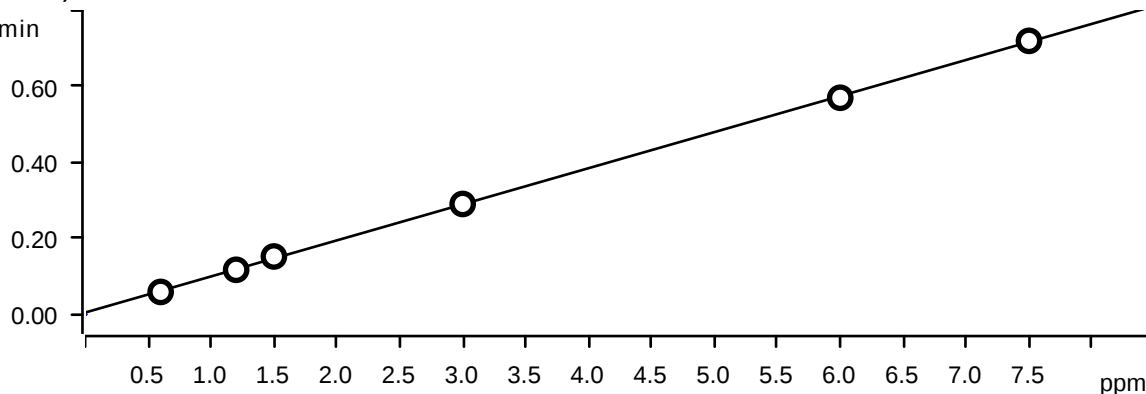


Function: $A = 4.85841E-3 + 9.50243E-3 \times Q$

Relative standard deviation 1.265280 %

Correlation coefficient 0.999910

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.059	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.153	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.291	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.570	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.720	STD7	2024-11-18 13:33:24 UTC-5	used

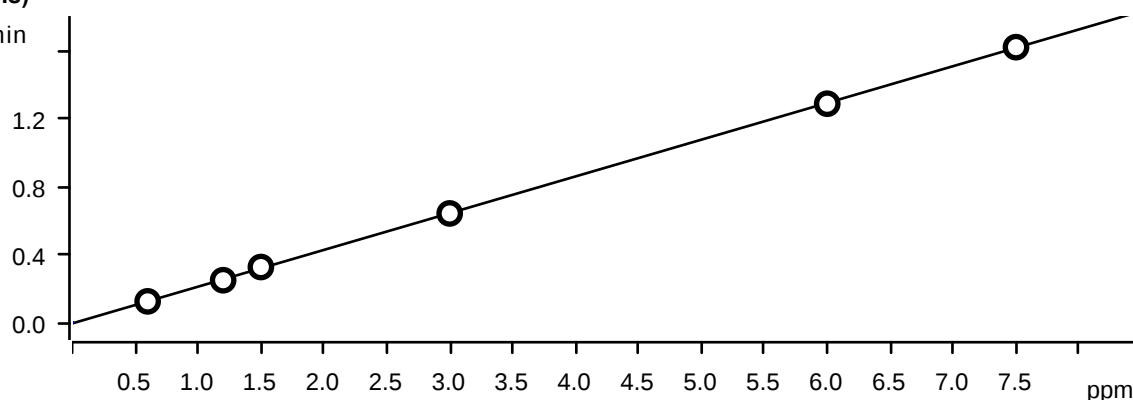Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -5.27414E-3 + 0.0216316 \times Q$


Relative standard deviation 0.783603 %

Correlation coefficient 0.999967

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.125	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.249	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.327	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.642	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.288	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.621	STD7	2024-11-18 13:33:24 UTC-5	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

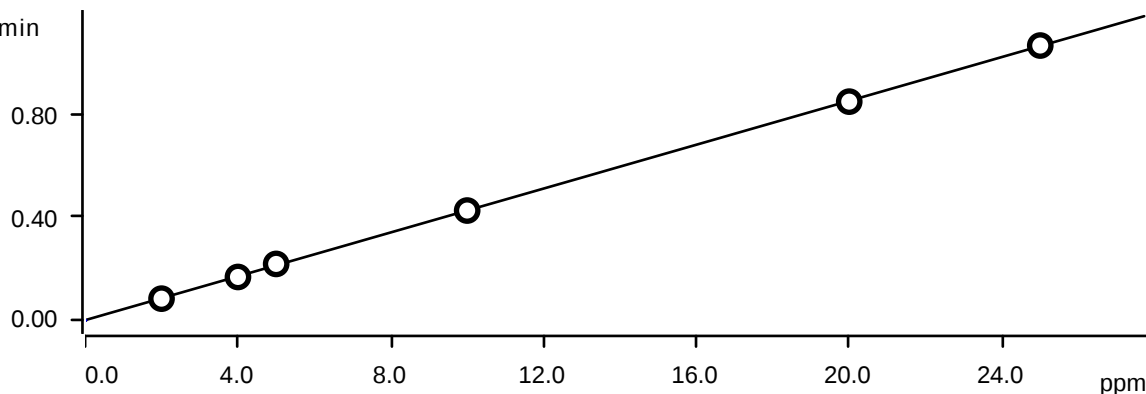

Function: $A = 7.64331E-4 + 4.24604E-3 \times Q$


Relative standard deviation 0.771268 %

Correlation coefficient 0.999967

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	2.000	10.0	1.0	1.0	0.084	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.168	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.219	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.425	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.847	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.064	STD7	2024-11-18 13:33:24 UTC-5	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

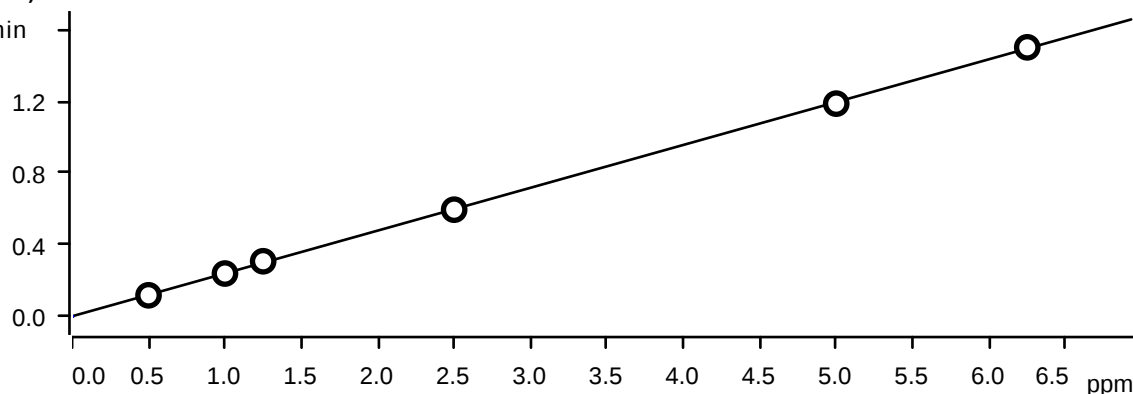


Function: $A = 1.14484E-3 + 0.0238833 \times Q$

Relative standard deviation 1.085494 %

Correlation coefficient 0.999936

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	0.500	10.0	1.0	1.0	0.118	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	1.000	10.0	1.0	1.0	0.239	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.308	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.595	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.187	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.501	STD7	2024-11-18 13:33:24 UTC-5	used

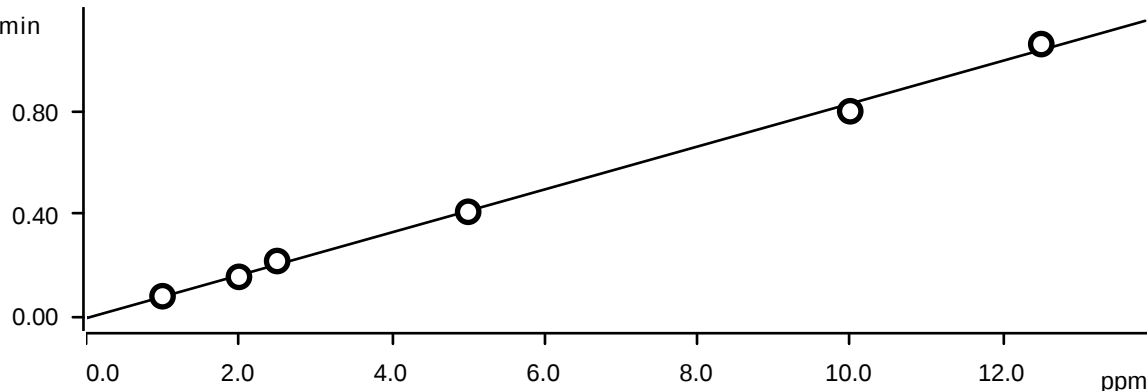
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -2.33576E-3 + 8.30878E-3 \times Q$

Relative standard deviation 4.444706 %

Correlation coefficient 0.998936

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	1.000	10.0	1.0	1.0	0.083	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.158	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.219	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.410	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.799	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.059	STD7	2024-11-18 13:33:24 UTC-5	used

Sulfate (Anions)

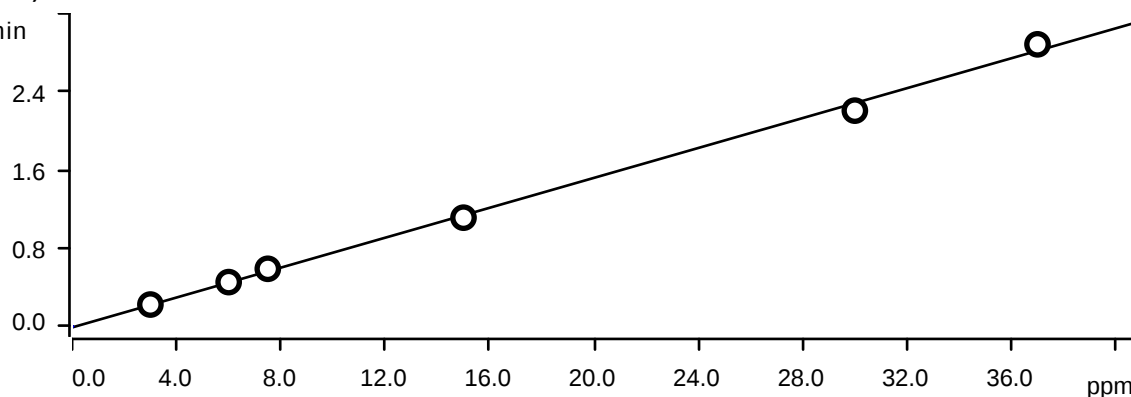 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -9.71222E-3 + 7.64397E-3 \times Q$

Relative standard deviation 4.327283 %

Correlation coefficient 0.998986

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2024-11-18 11:24:52 UTC-5	used
Standard 2	1	3.000	10.0	1.0	1.0	0.224	STD2	2024-11-18 11:46:16 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.454	STD3	2024-11-18 12:07:40 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.590	STD4	2024-11-18 12:29:05 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.112	STD5	2024-11-18 12:50:30 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.206	STD6	2024-11-18 13:11:57 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.884	STD7	2024-11-18 13:33:24 UTC-5	used


Sample data

Ident STD1
Sample type Standard 1
Determination start 2024-11-18 11:24:52 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

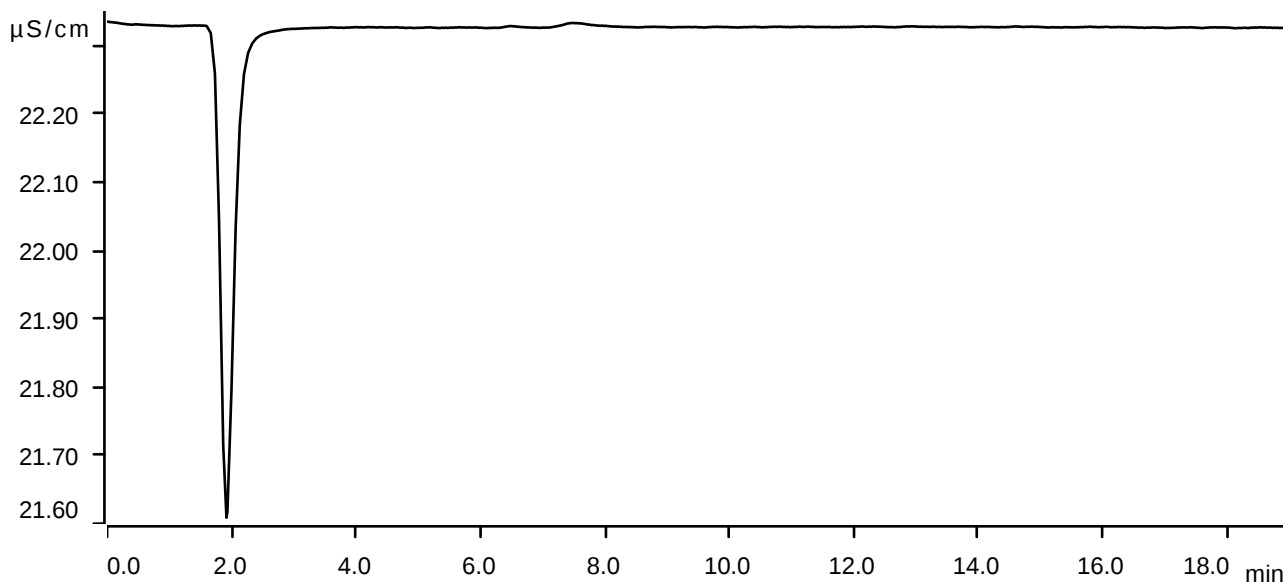


Sample data

Ident STD2
Sample type Standard 2
Determination start 2024-11-18 11:46:16 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

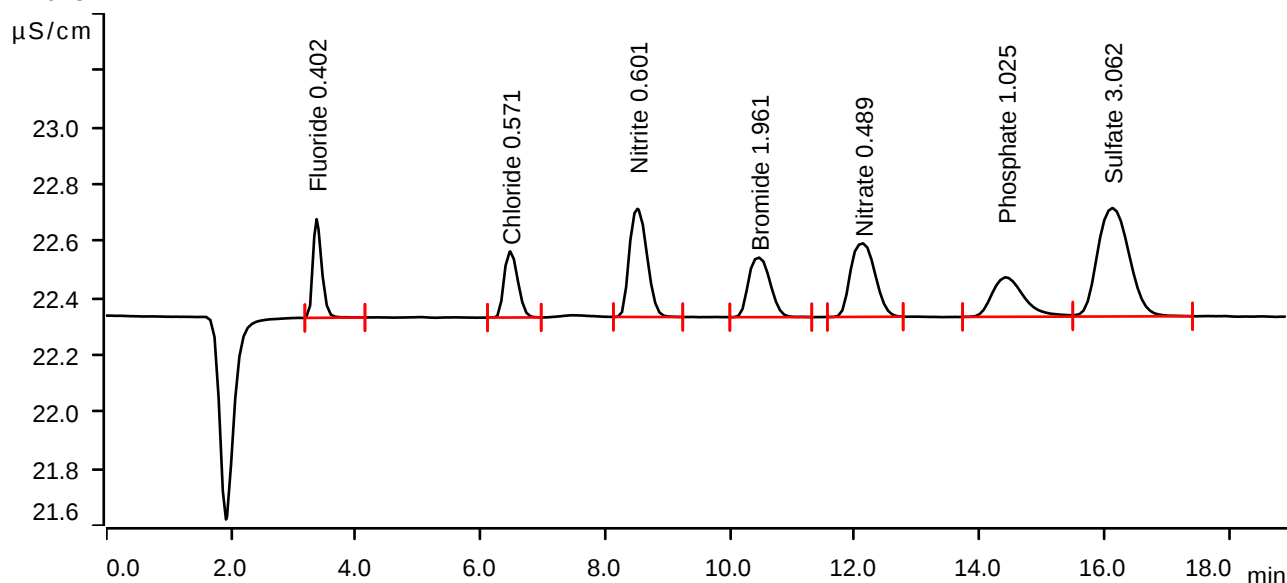

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.372	0.0570	0.347	0.402	Fluoride
2	6.477	0.0592	0.232	0.571	Chloride
3	8.515	0.1247	0.380	0.601	Nitrite
4	10.463	0.0840	0.209	1.961	Bromide
5	12.127	0.1179	0.258	0.489	Nitrate
6	14.418	0.0829	0.139	1.025	Phosphate
7	16.130	0.2243	0.381	3.062	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2024-11-18 12:07:40 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

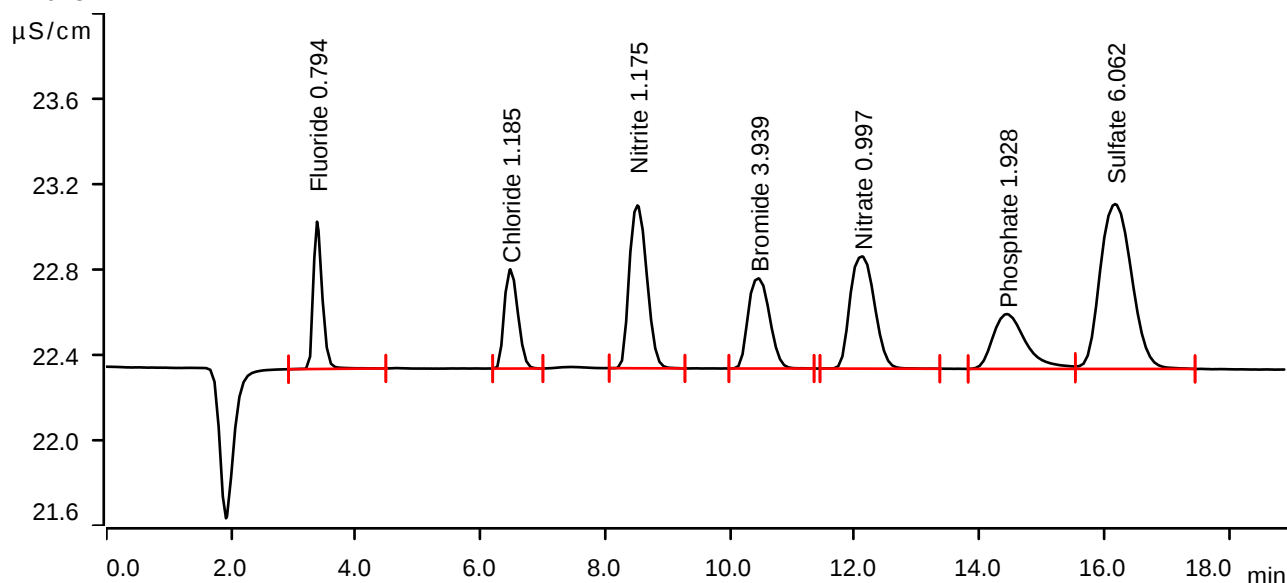

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.1141	0.690	0.794	Fluoride
2	6.478	0.1175	0.465	1.185	Chloride
3	8.515	0.2490	0.763	1.175	Nitrite
4	10.453	0.1680	0.422	3.939	Bromide
5	12.117	0.2394	0.526	0.997	Nitrate
6	14.440	0.1579	0.257	1.928	Phosphate
7	16.173	0.4537	0.772	6.062	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2024-11-18 12:29:05 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

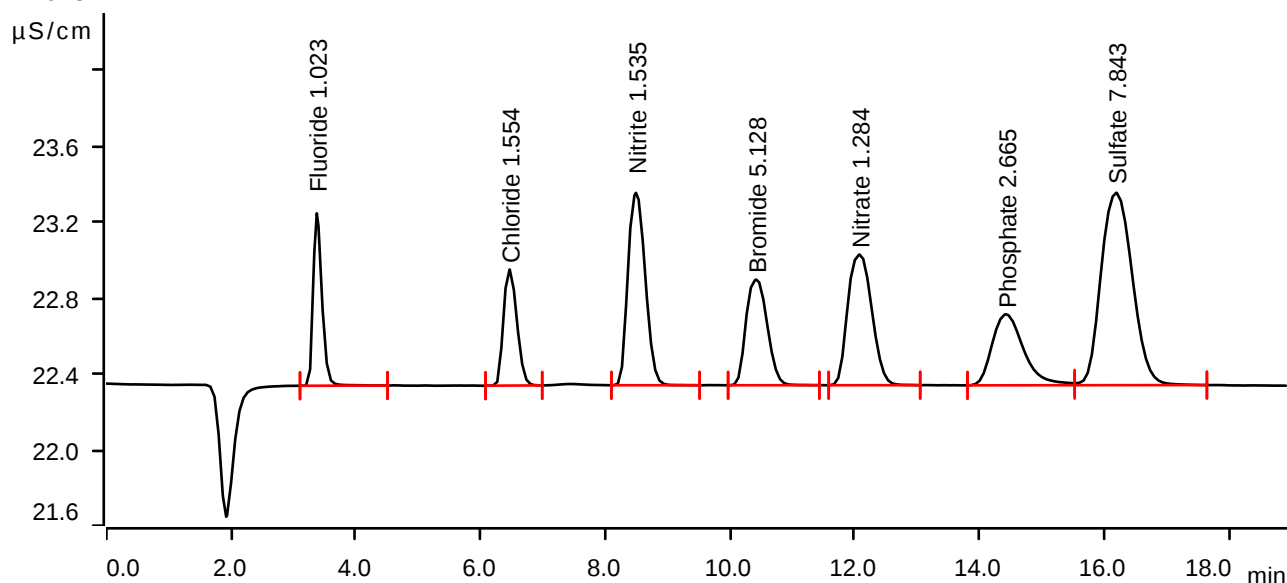

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.375	0.1475	0.909	1.023	Fluoride
2	6.465	0.1525	0.612	1.554	Chloride
3	8.493	0.3268	1.014	1.535	Nitrite
4	10.420	0.2185	0.557	5.128	Bromide
5	12.077	0.3078	0.689	1.284	Nitrate
6	14.427	0.2191	0.375	2.665	Phosphate
7	16.192	0.5898	1.014	7.843	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2024-11-18 12:50:30 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

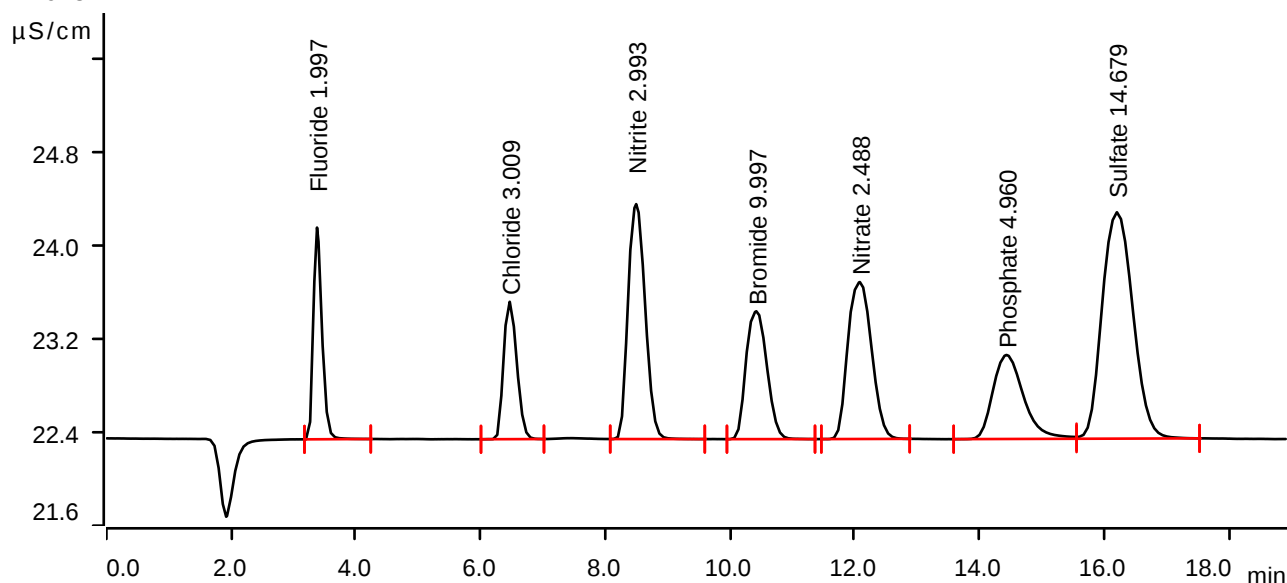

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.2894	1.819	1.997	Fluoride
2	6.467	0.2908	1.180	3.009	Chloride
3	8.495	0.6422	2.018	2.993	Nitrite
4	10.422	0.4253	1.098	9.997	Bromide
5	12.082	0.5953	1.348	2.488	Nitrate
6	14.432	0.4098	0.722	4.960	Phosphate
7	16.203	1.1123	1.944	14.679	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2024-11-18 13:11:57 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

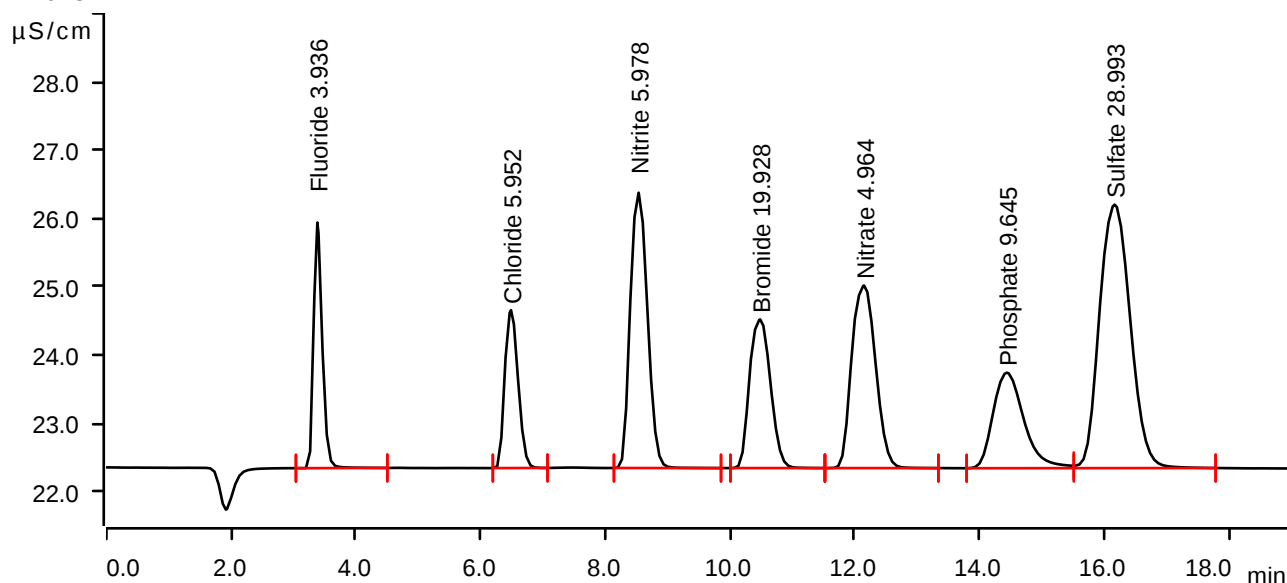

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.383	0.5717	3.596	3.936	Fluoride
2	6.488	0.5704	2.311	5.952	Chloride
3	8.533	1.2879	4.031	5.978	Nitrite
4	10.483	0.8469	2.176	19.928	Bromide
5	12.148	1.1866	2.673	4.964	Nitrate
6	14.438	0.7991	1.399	9.645	Phosphate
7	16.165	2.2065	3.859	28.993	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2024-11-18 13:33:24 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

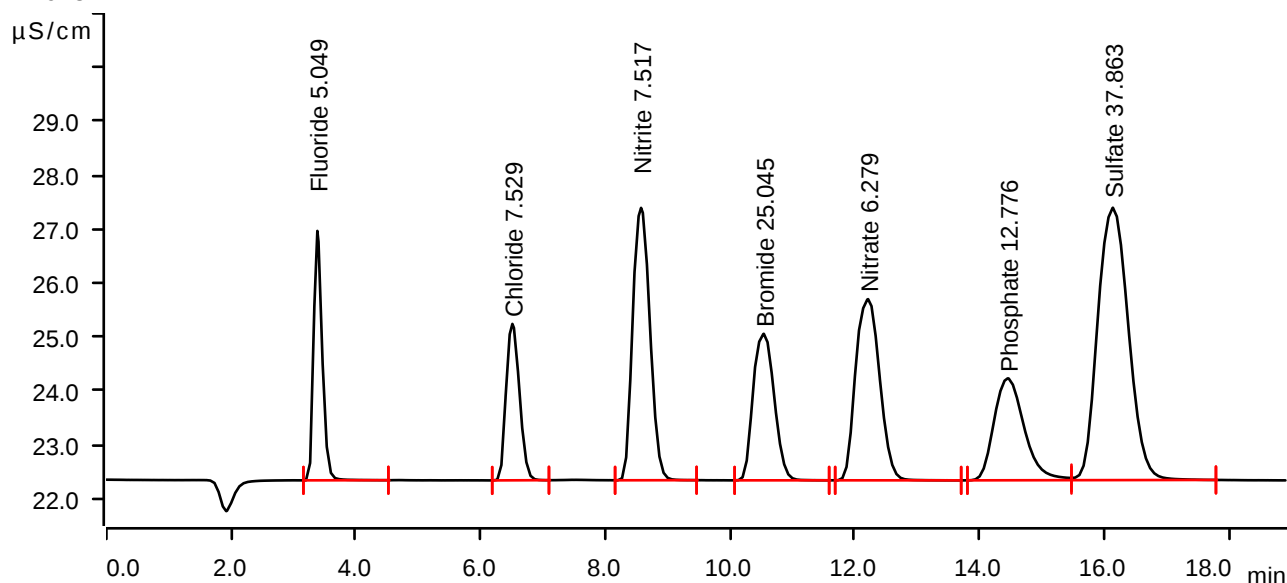

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.383	0.7339	4.626	5.049	Fluoride
2	6.510	0.7203	2.901	7.529	Chloride
3	8.573	1.6208	5.052	7.517	Nitrite
4	10.542	1.0642	2.717	25.045	Bromide
5	12.213	1.5007	3.361	6.279	Nitrate
6	14.452	1.0592	1.891	12.776	Phosphate
7	16.138	2.8845	5.052	37.863	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2024-11-18 13:54:44 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

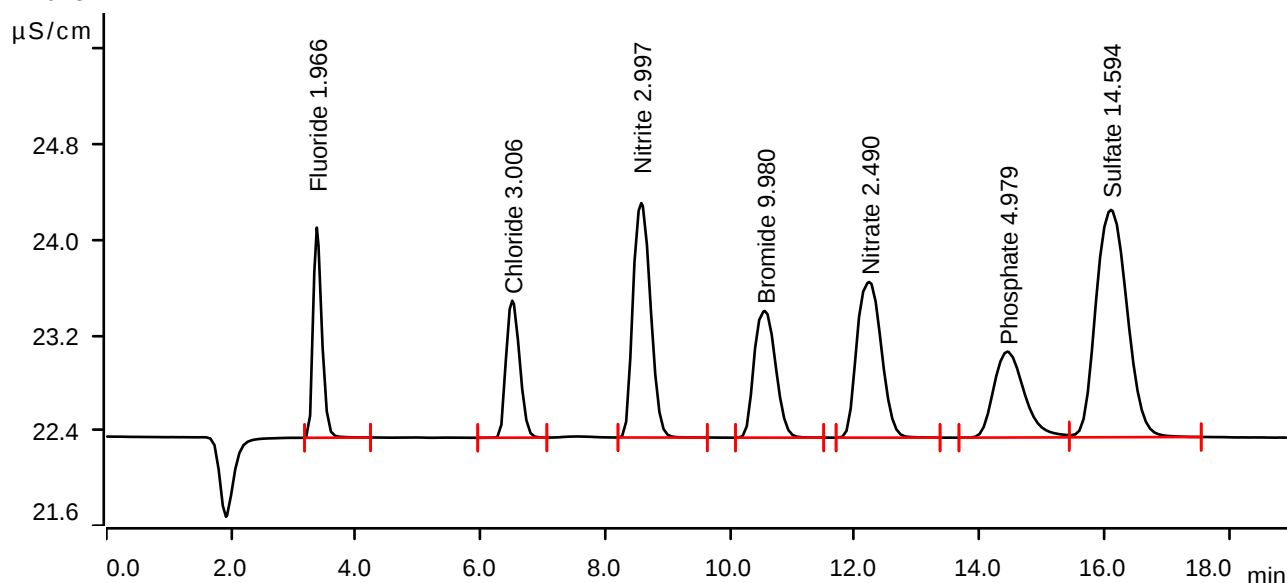


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.375	0.2848	1.764	1.966	Fluoride
2	6.508	0.2905	1.150	3.006	Chloride
3	8.577	0.6430	1.968	2.997	Nitrite
4	10.557	0.4245	1.063	9.980	Bromide
5	12.230	0.5959	1.307	2.490	Nitrate
6	14.447	0.4114	0.721	4.979	Phosphate
7	16.107	1.1058	1.909	14.594	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2024-11-18 14:16:12 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

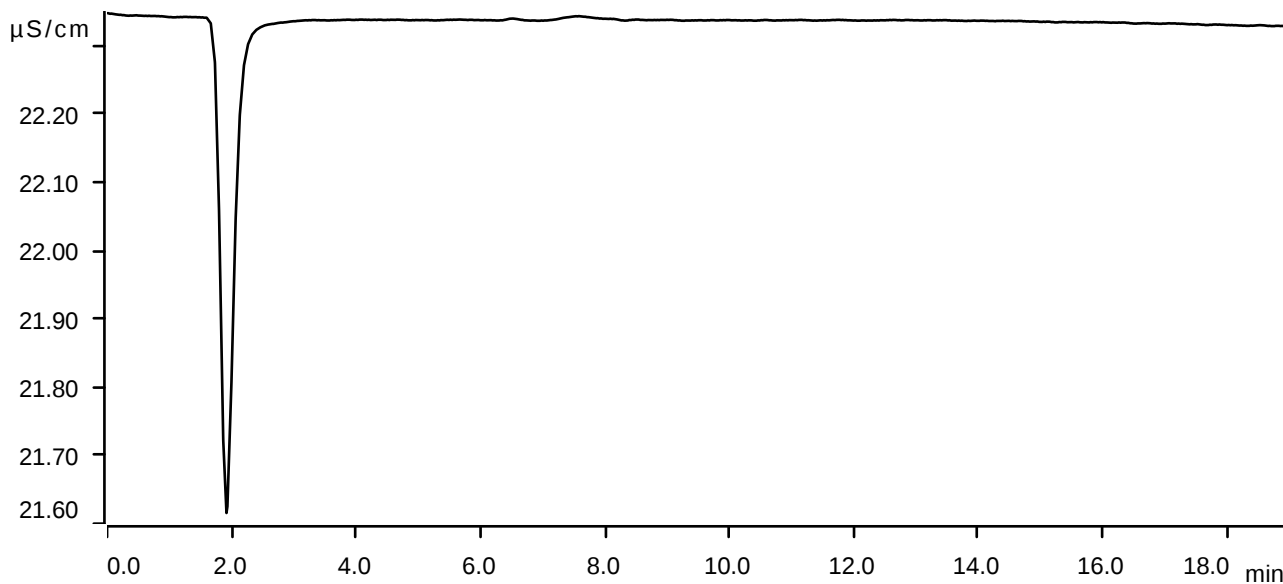Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-12-13 11:09:32 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

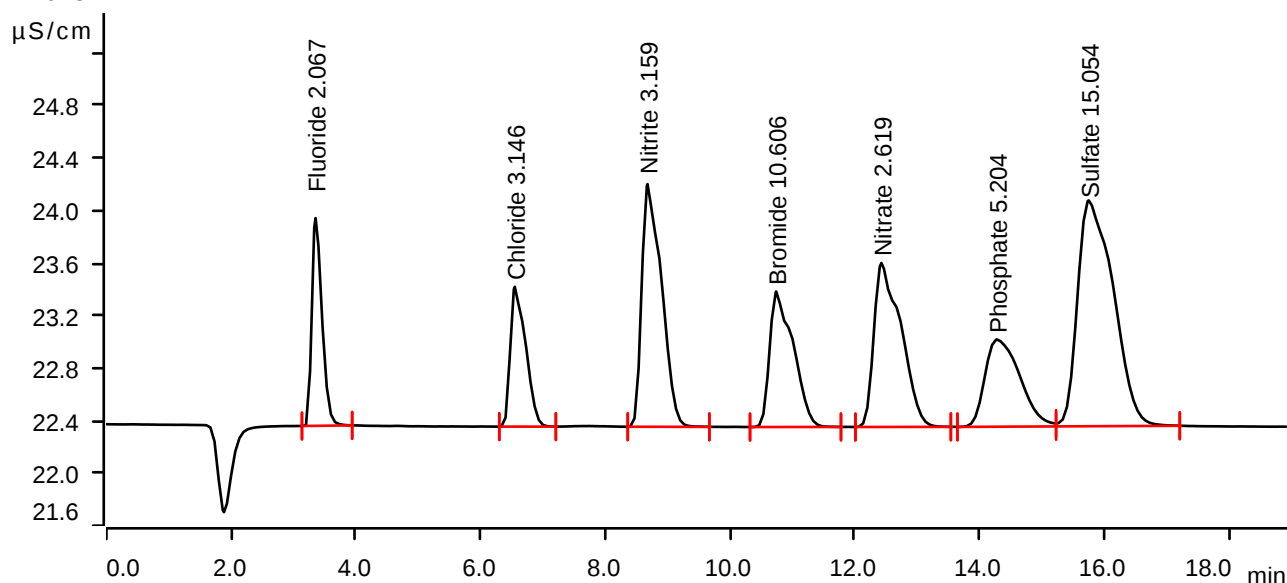


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.2995	1.582	2.067	Fluoride
2	6.548	0.3038	1.065	3.146	Chloride
3	8.677	0.6780	1.848	3.159	Nitrite
4	10.740	0.4511	1.032	10.606	Bromide
5	12.427	0.6265	1.249	2.619	Nitrate
6	14.278	0.4301	0.664	5.204	Phosphate
7	15.750	1.1410	1.719	15.054	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-12-13 11:31:02 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

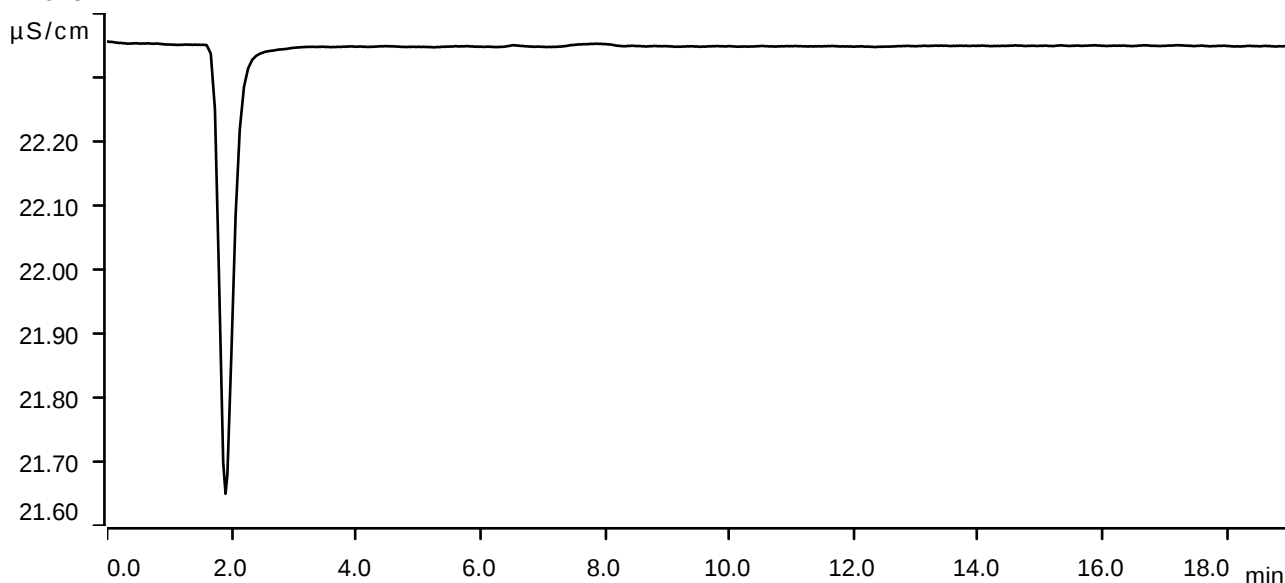Anions


Sample data

Ident LB133942BLW
Sample type Sample
Determination start 2024-12-13 11:52:32 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

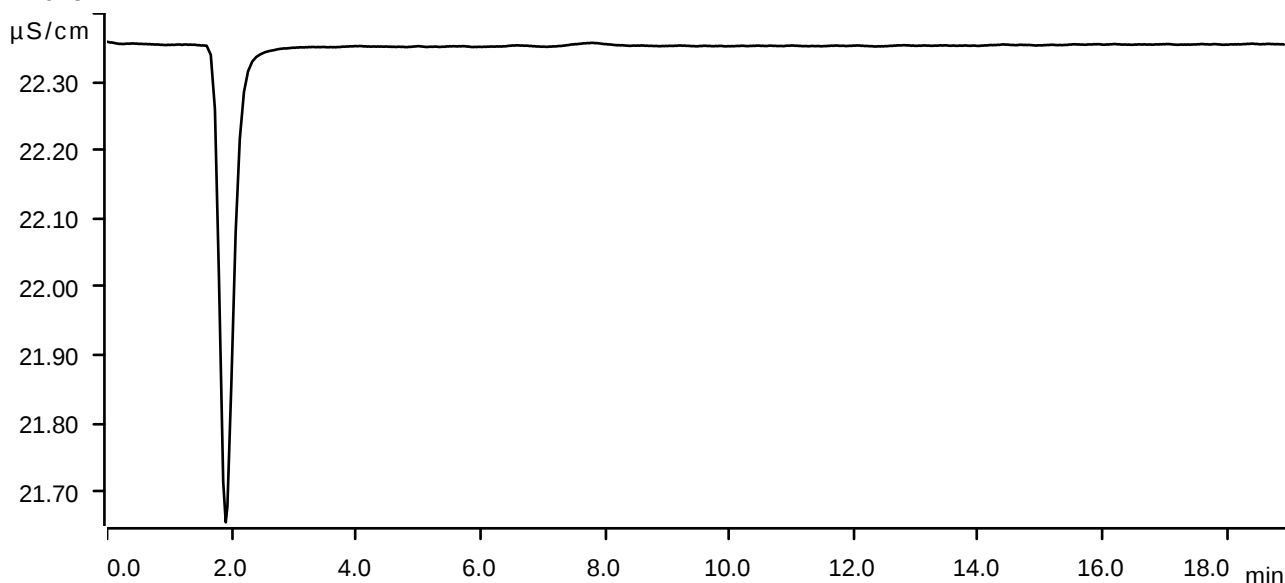


Sample data

Ident LB133942BSW
Sample type Check standard 1
Determination start 2024-12-13 12:14:04 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

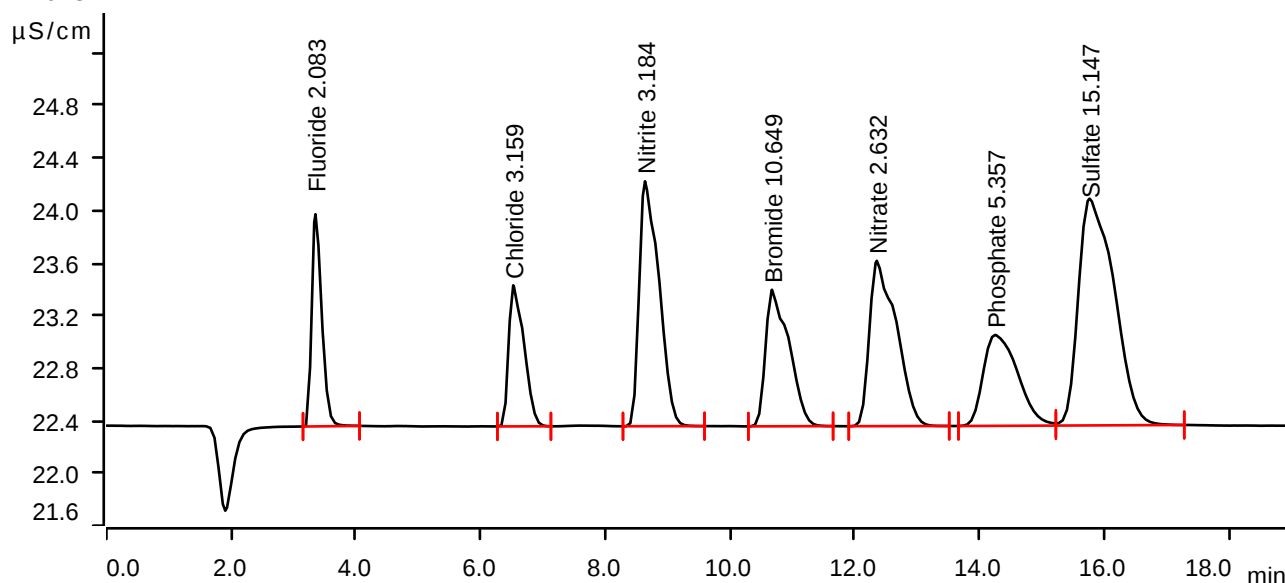

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.3020	1.615	2.083	Fluoride
2	6.523	0.3050	1.074	3.159	Chloride
3	8.637	0.6836	1.865	3.184	Nitrite
4	10.673	0.4529	1.040	10.649	Bromide
5	12.353	0.6298	1.259	2.632	Nitrate
6	14.250	0.4427	0.692	5.357	Phosphate
7	15.763	1.1481	1.727	15.147	Sulfate


Sample data

Ident P5270-01
Sample type Sample
Determination start 2024-12-13 13:02:49 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

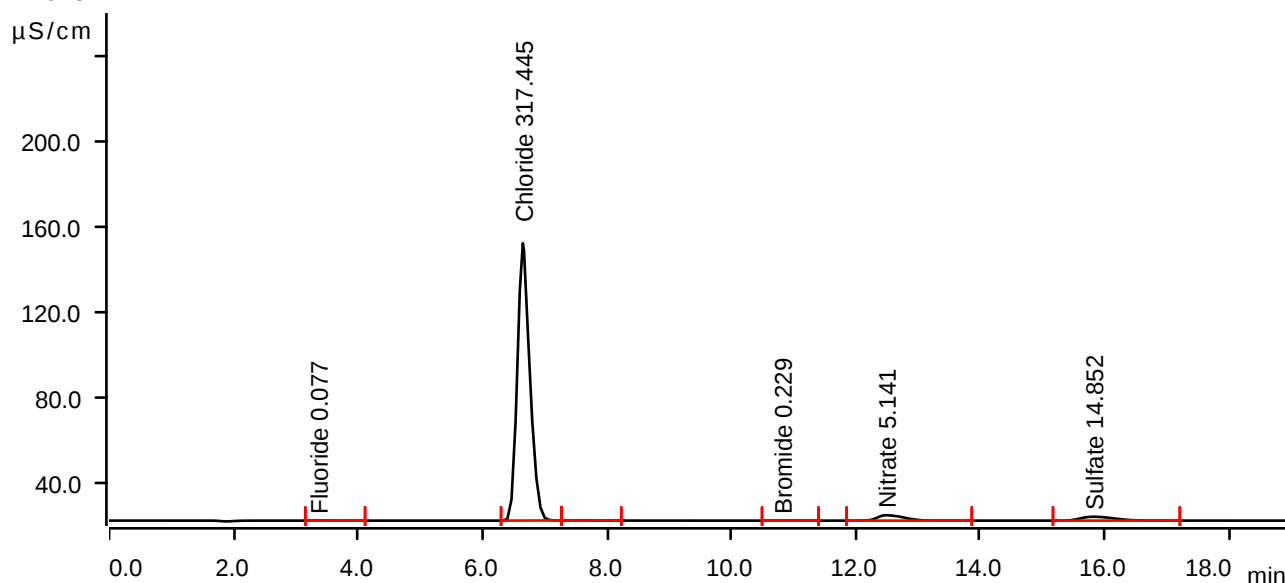

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.0097	0.046	0.077	Fluoride
2	6.650	30.1699	129.945	317.445	Chloride
3	7.520	0.0211	0.045	invalid	
4	10.813	0.0105	0.025	0.229	Bromide
5	12.485	1.2291	2.544	5.141	Nitrate
6	15.812	1.1256	1.813	14.852	Sulfate


Sample data

Ident P5270-03
Sample type Sample
Determination start 2024-12-13 13:24:27 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

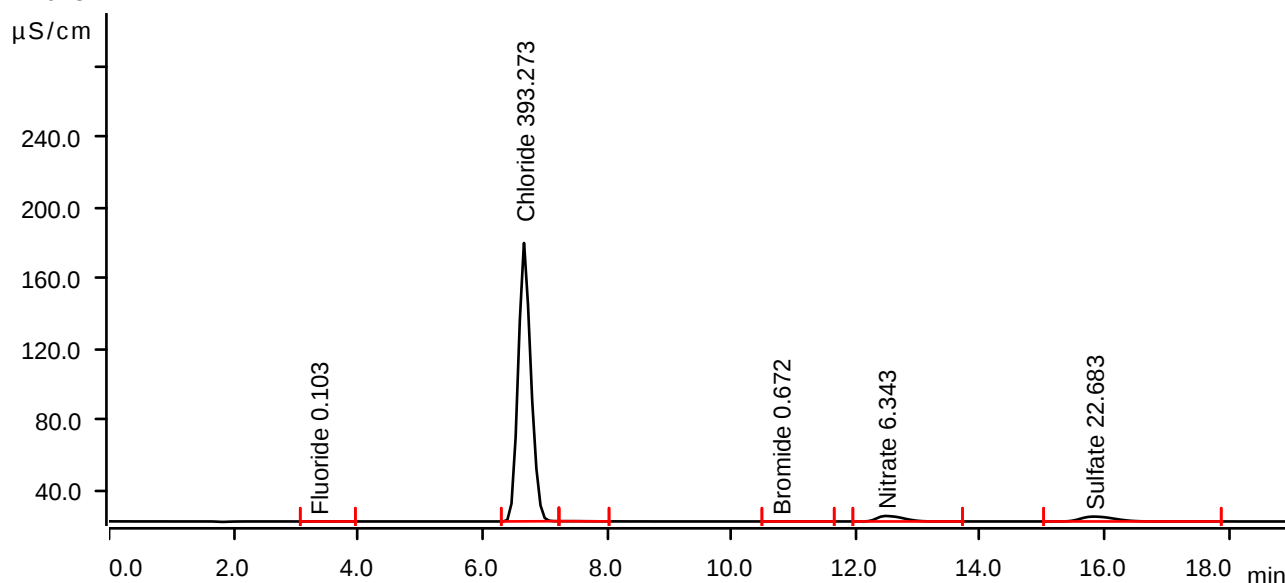

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.360	0.0136	0.068	0.103	Fluoride
2	6.670	37.3754	157.603	393.273	Chloride
3	7.415	0.0187	0.043	invalid	
4	10.788	0.0293	0.069	0.672	Bromide
5	12.480	1.5160	3.109	6.343	Nitrate
6	15.823	1.7241	2.749	22.683	Sulfate


Sample data

Ident P5270-04
Sample type Sample
Determination start 2024-12-13 13:46:01 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

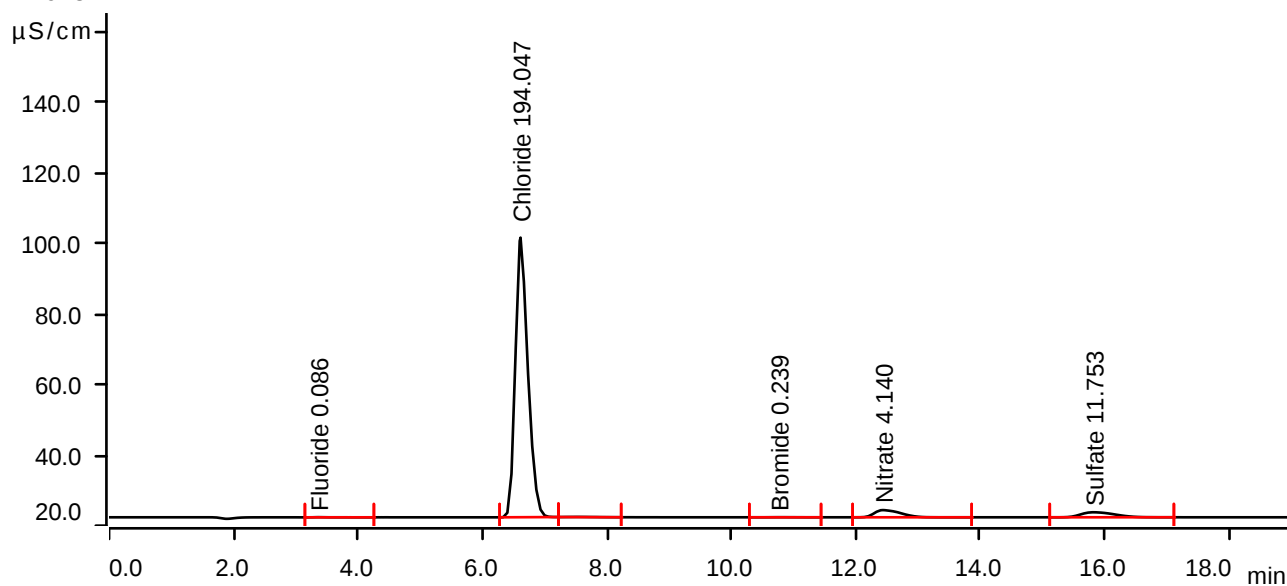

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.363	0.0111	0.047	0.086	Fluoride
2	6.613	18.4440	79.148	194.047	Chloride
3	7.513	0.0255	0.052	invalid	
4	10.760	0.0109	0.026	0.239	Bromide
5	12.435	0.9899	2.041	4.140	Nitrate
6	15.818	0.8887	1.421	11.753	Sulfate


Sample data

Ident P5270-05
Sample type Sample
Determination start 2024-12-13 14:07:35 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

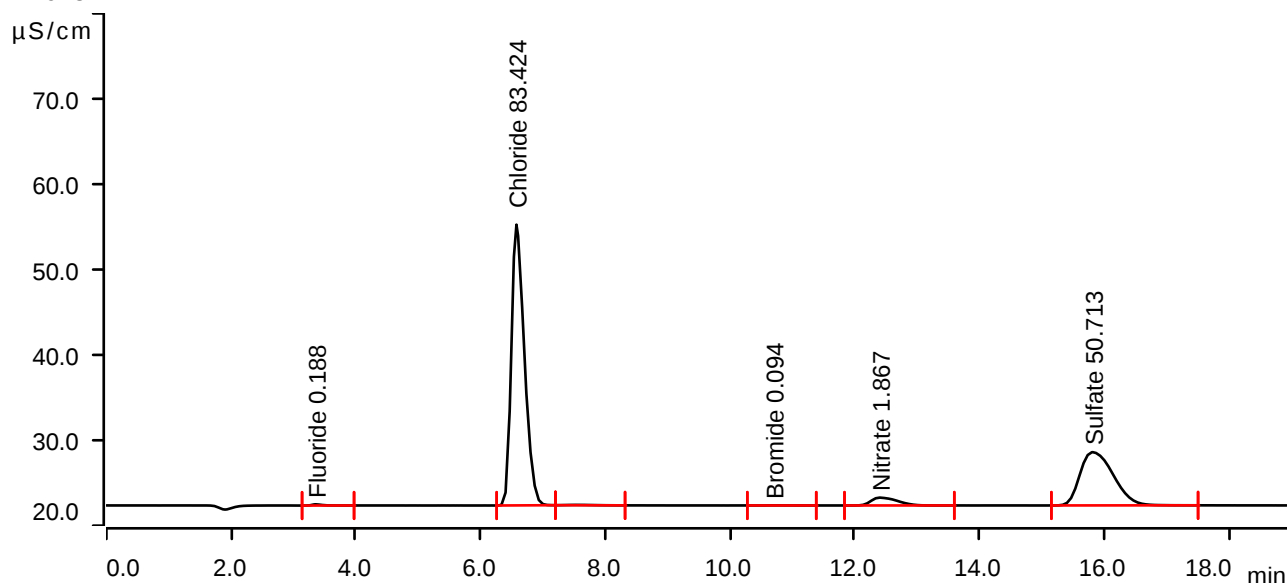

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.0259	0.140	0.188	Fluoride
2	6.575	7.9322	32.887	83.424	Chloride
3	7.535	0.0213	0.042	invalid	
4	10.698	0.0048	0.011	0.094	Bromide
5	12.400	0.4469	0.922	1.867	Nitrate
6	15.815	3.8668	6.237	50.713	Sulfate


Sample data

Ident P5270-09
Sample type Sample
Determination start 2024-12-13 14:29:10 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

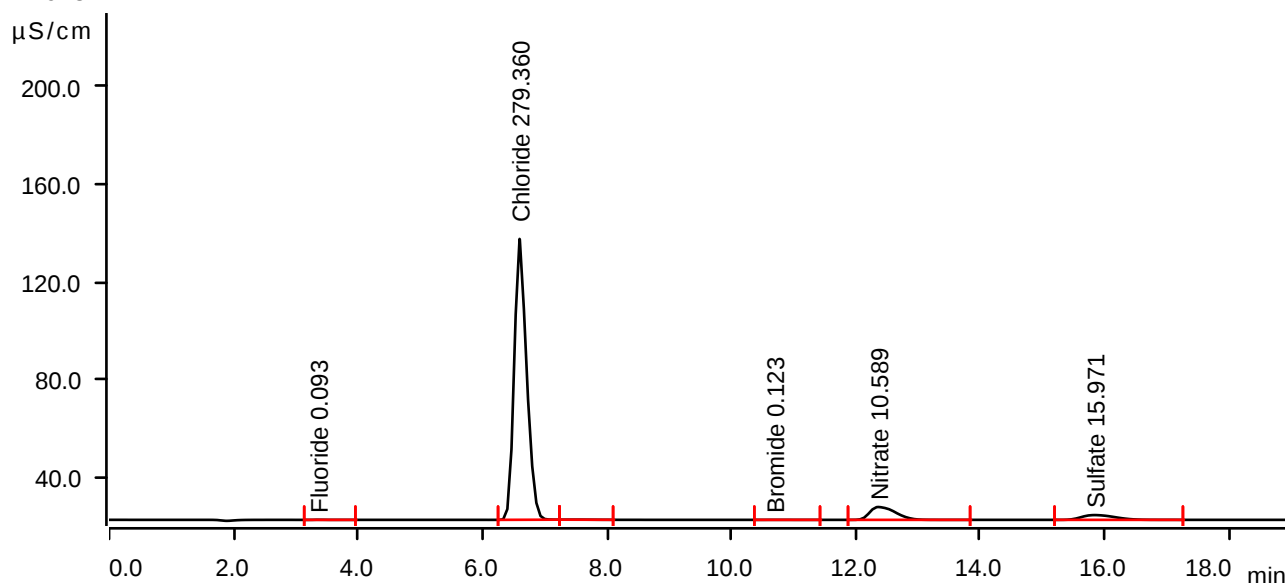

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.0121	0.057	0.093	Fluoride
2	6.597	26.5508	115.162	279.360	Chloride
3	7.472	0.0130	0.030	invalid	
4	10.688	0.0060	0.014	0.123	Bromide
5	12.362	2.5302	5.276	10.589	Nitrate
6	15.833	1.2111	1.956	15.971	Sulfate


Sample data

Ident P5270-09MS
Sample type Sample
Determination start 2024-12-13 14:50:44 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

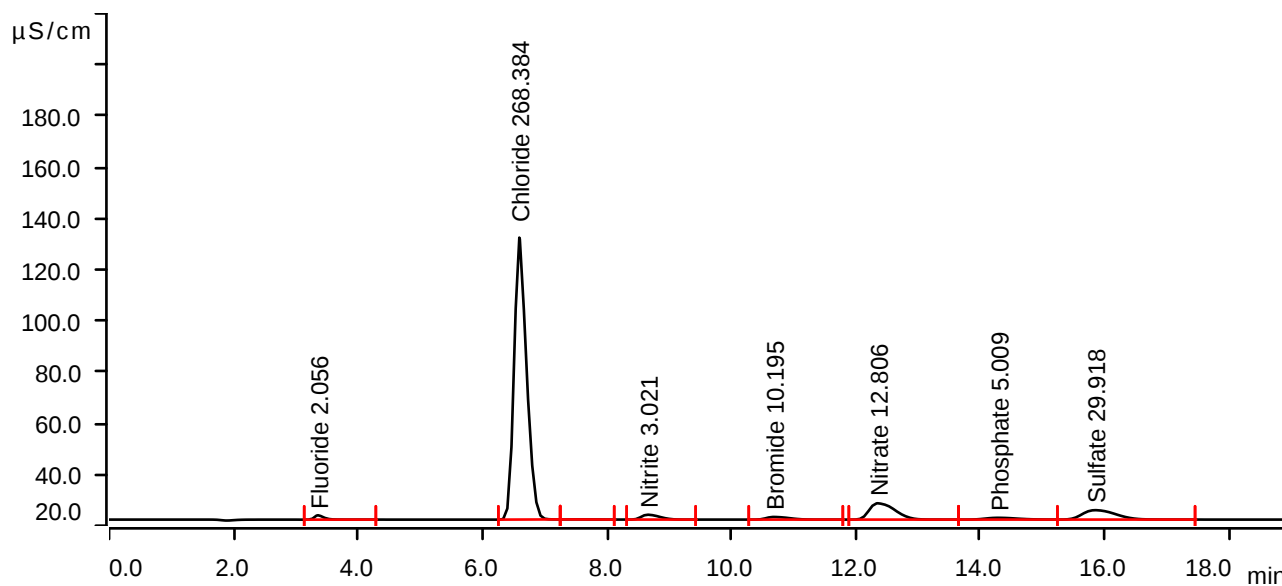

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.358	0.2980	1.709	2.056	Fluoride
2	6.593	25.5079	110.089	268.384	Chloride
3	7.480	0.0116	0.027	invalid	
4	8.660	0.6482	1.893	3.021	Nitrite
5	10.682	0.4336	1.037	10.195	Bromide
6	12.353	3.0596	6.375	12.806	Nitrate
7	14.293	0.4138	0.697	5.009	Phosphate
8	15.848	2.2772	3.671	29.918	Sulfate


Sample data

Ident P5270-09MSD
Sample type Sample
Determination start 2024-12-13 15:12:18 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

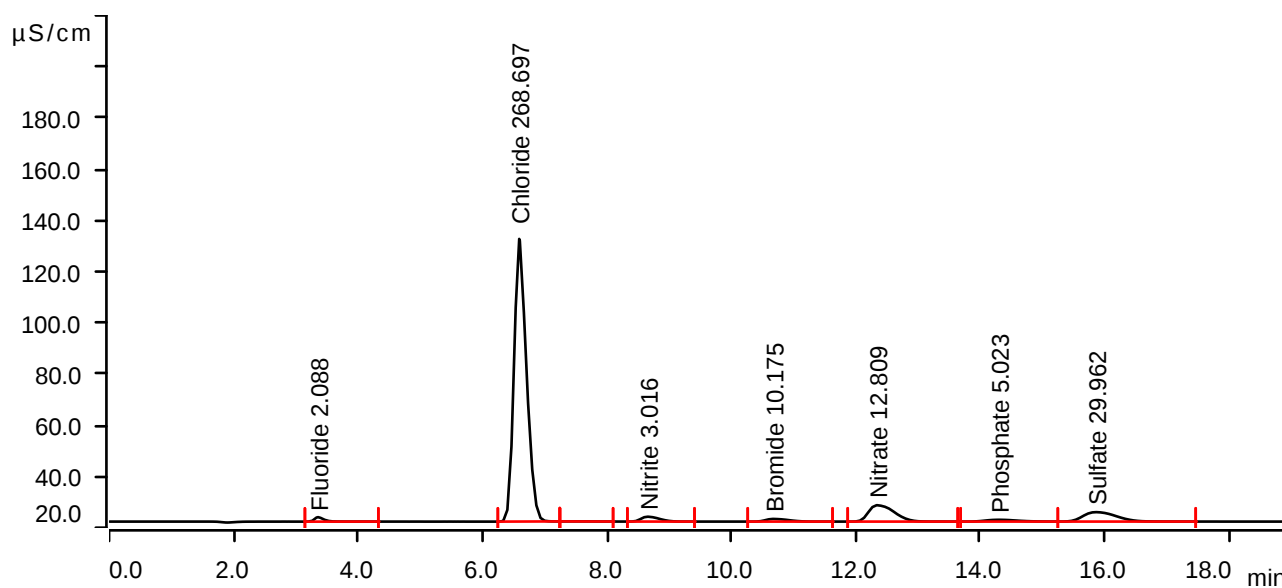

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.360	0.3026	1.743	2.088	Fluoride
2	6.592	25.5376	110.349	268.697	Chloride
3	7.465	0.0119	0.026	invalid	
4	8.657	0.6471	1.899	3.016	Nitrite
5	10.675	0.4328	1.039	10.175	Bromide
6	12.343	3.0604	6.393	12.809	Nitrate
7	14.300	0.4151	0.702	5.023	Phosphate
8	15.862	2.2806	3.682	29.962	Sulfate


Sample data

Ident P5270-05DLX5
Sample type Sample
Determination start 2024-12-13 15:33:51 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

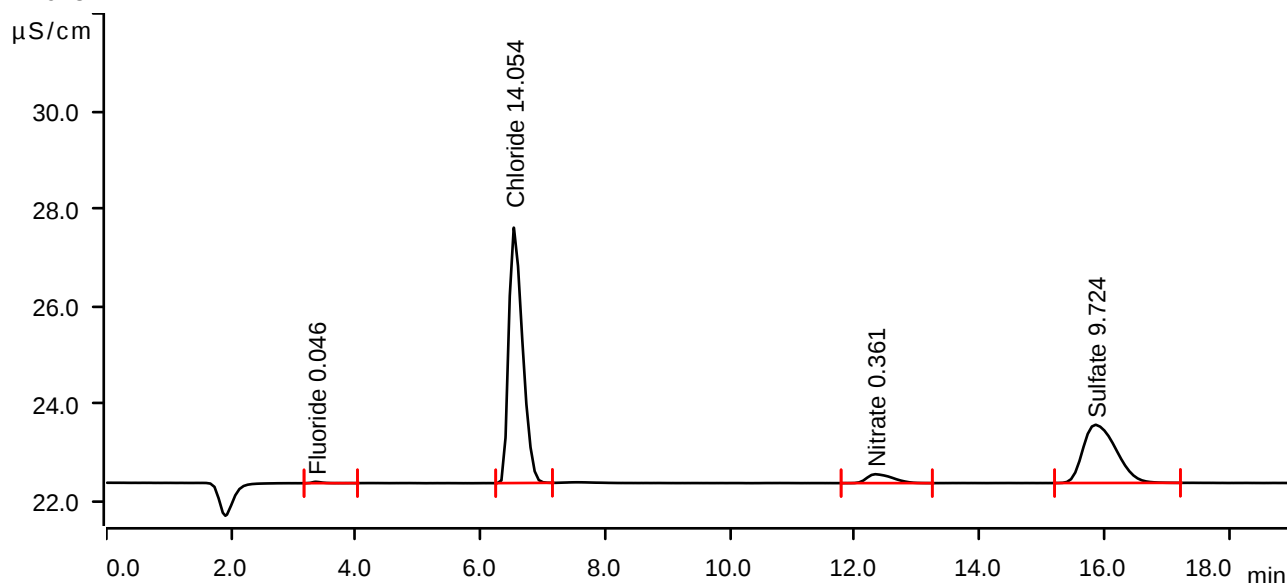

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.0052	0.028	0.046	Fluoride
2	6.532	1.3404	5.236	14.054	Chloride
3	12.327	0.0873	0.183	0.361	Nitrate
4	15.858	0.7336	1.192	9.724	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-12-13 15:55:23 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

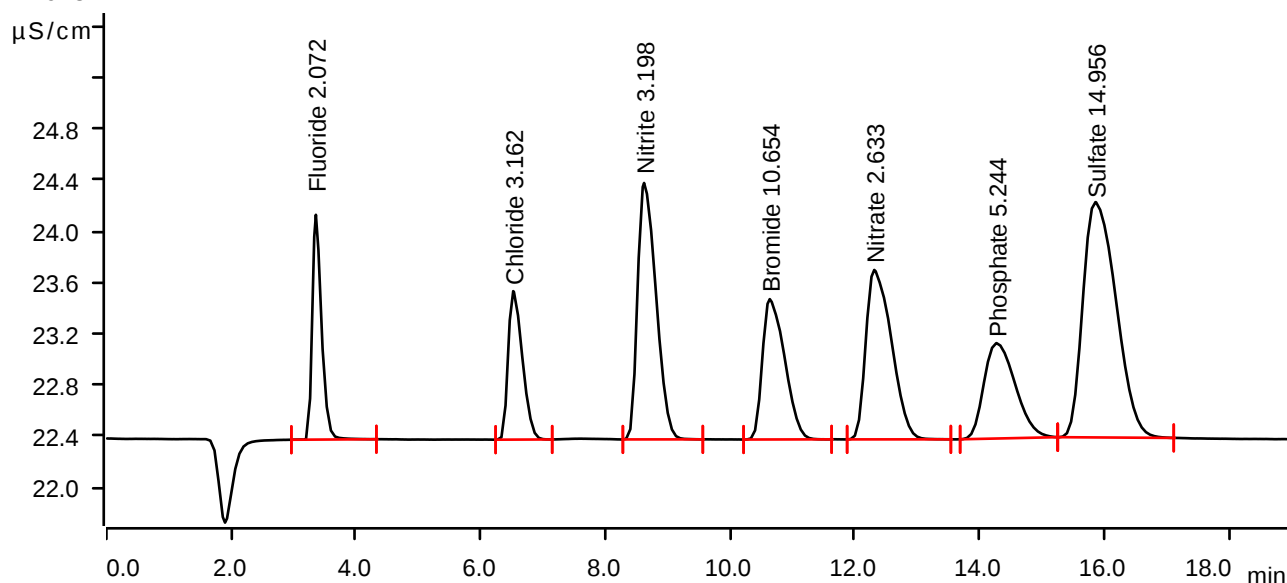

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.360	0.3003	1.756	2.072	Fluoride
2	6.523	0.3054	1.159	3.162	Chloride
3	8.622	0.6865	2.003	3.198	Nitrite
4	10.637	0.4531	1.096	10.654	Bromide
5	12.312	0.6301	1.323	2.633	Nitrate
6	14.273	0.4333	0.745	5.244	Phosphate
7	15.858	1.1335	1.838	14.956	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-12-13 16:16:53 UTC-5
Method IC1-111824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions