
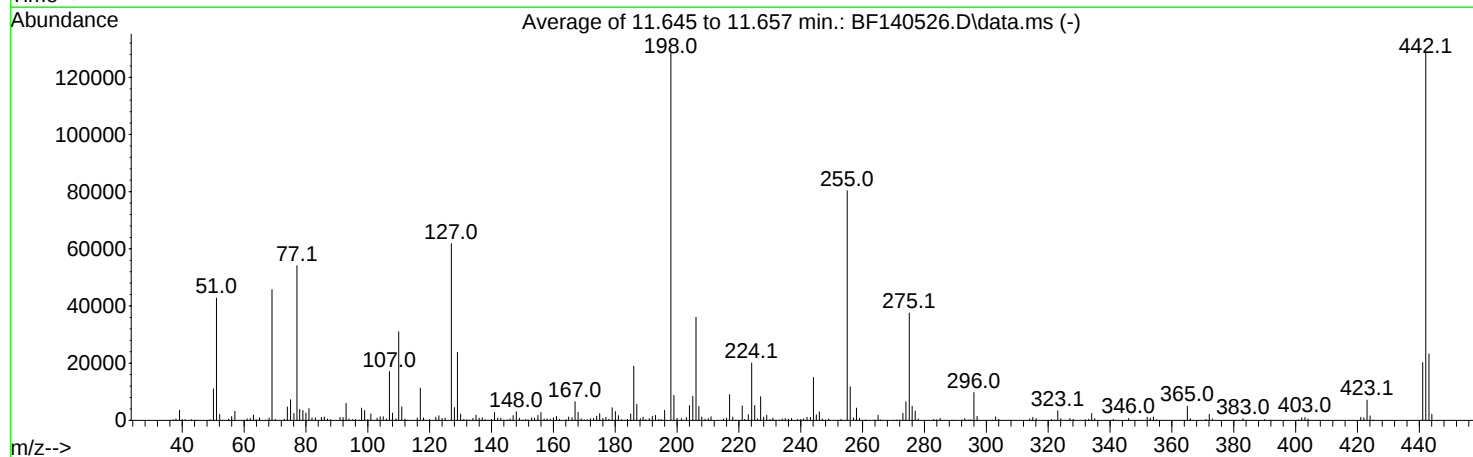


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112124\  
Data File : BF140526.D  
Acq On : 21 Nov 2024 10:17  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112124.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Nov 21 15:23:48 2024

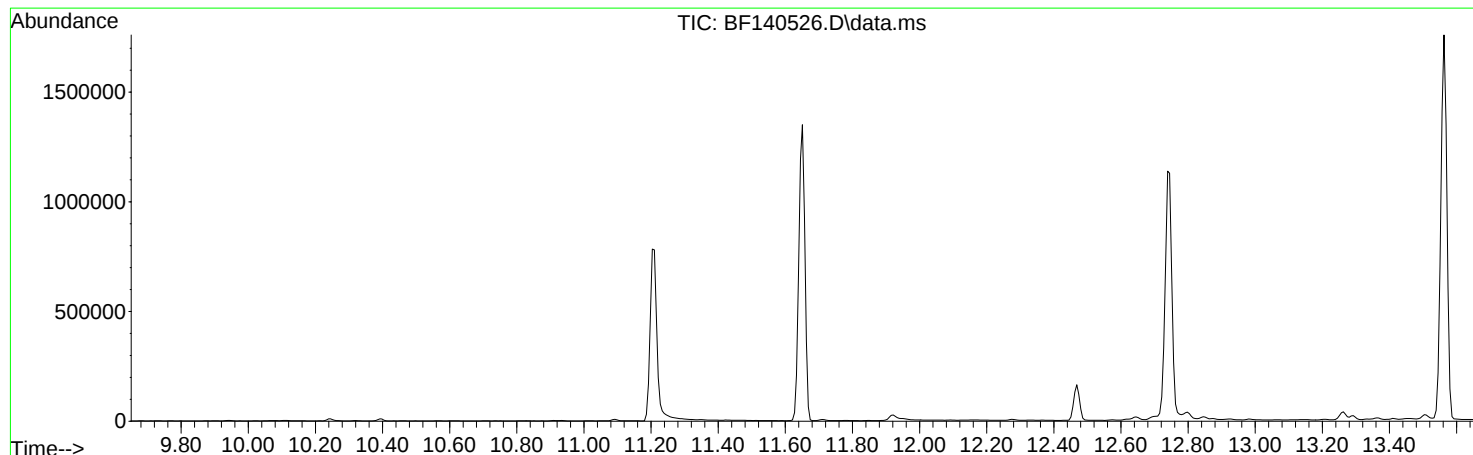

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 33.3         | 42792      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 810        | PASS                |
| 69             | 198             | 0.00            | 100             | 35.5         | 45731      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.7          | 327        | PASS                |
| 127            | 198             | 10              | 80              | 48.0         | 61811      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 128688     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 8723       | PASS                |
| 275            | 198             | 10              | 60              | 29.2         | 37552      | PASS                |
| 365            | 198             | 1               | 100             | 3.8          | 4944       | PASS                |
| 441            | 198             | 0.01            | 100             | 15.7         | 20189      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 128421     | PASS                |
| 443            | 442             | 15              | 24              | 18.1         | 23261      | PASS                |

### DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/21/2024    | BNA_F            | <u>BF140526.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 424151           | 13.562             |
| DDD           | 14557            | 13.262             |
| DDE           | 1132             | 12.921             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 15689         | 439840           | 3.57               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF-2024\BN-NOV-24\BF112124\  
Data File : BF140526.D  
Acq On : 21 Nov 2024 10:17  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Nov 21 23:23:25 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112124.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 21 15:23:48 2024  
Response via : Initial Calibration

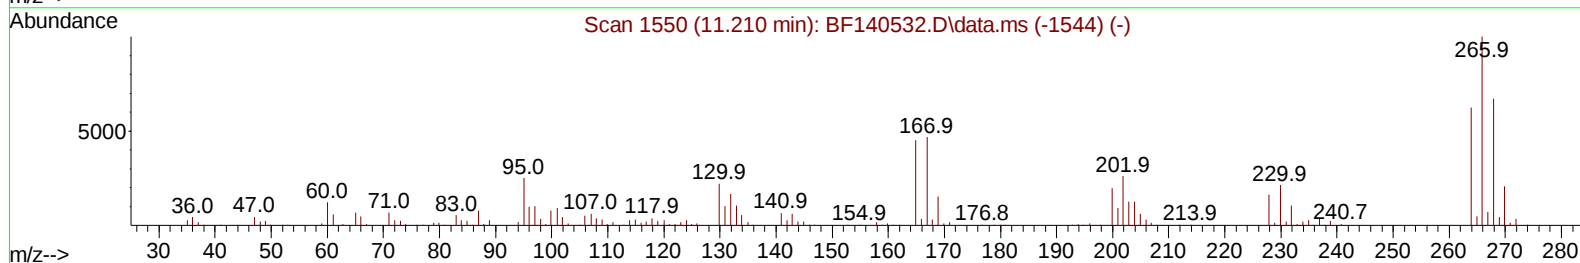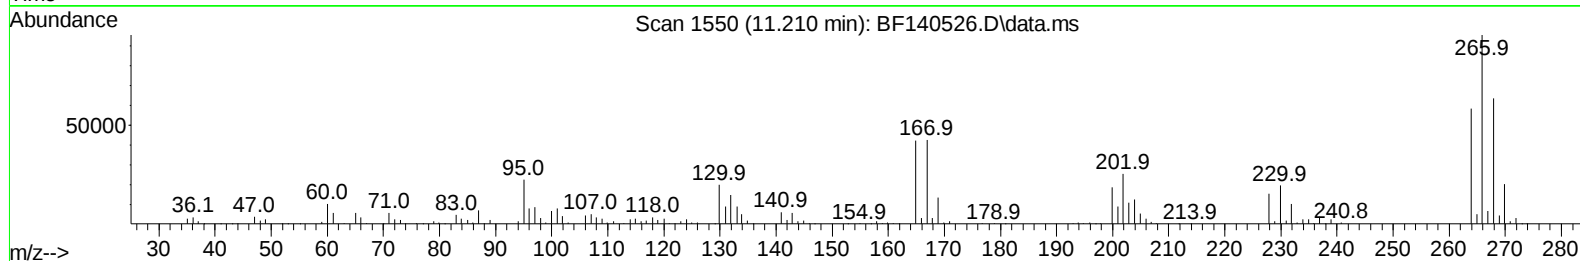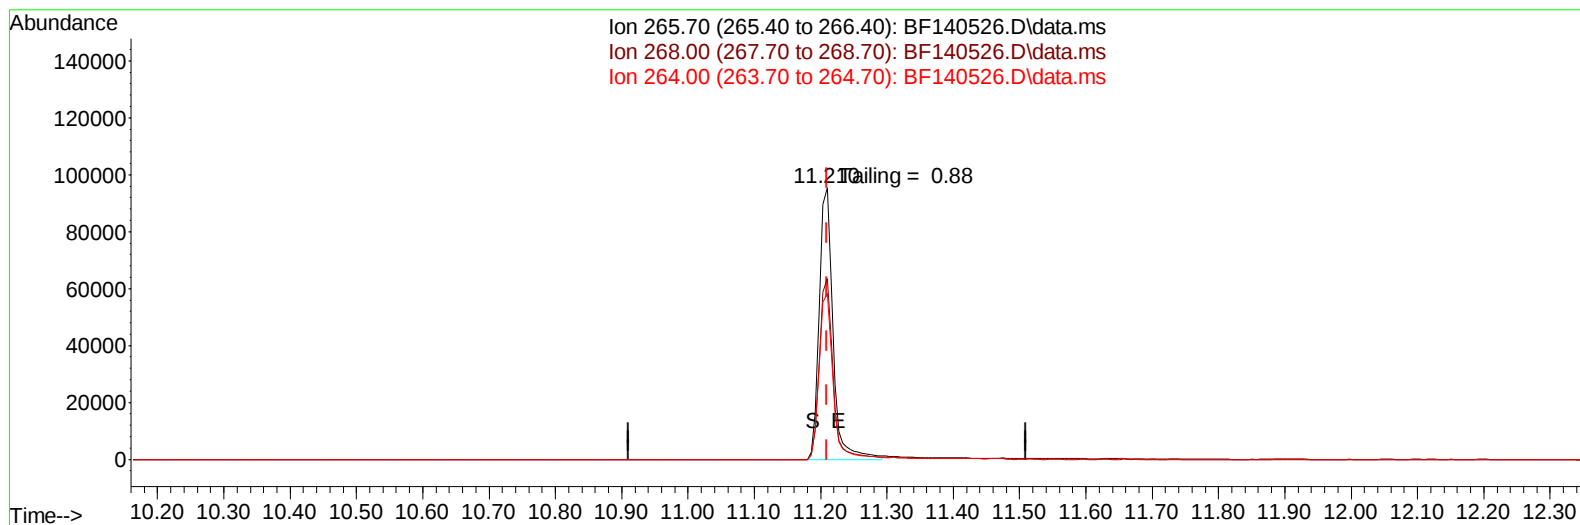

TIC: BF140526.D\data.ms

**(70) Pentachlorophenol (C)**

**11.210min (-0.000) 34448.94 ng**




**response 138311**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 67.10  | 66.58  |
| 264.00 | 62.30  | 61.22  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF112124\  
Data File : BF140526.D  
Acq On : 21 Nov 2024 10:17  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Nov 21 15:24:39 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF112124.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 21 15:23:48 2024  
Response via : Initial Calibration

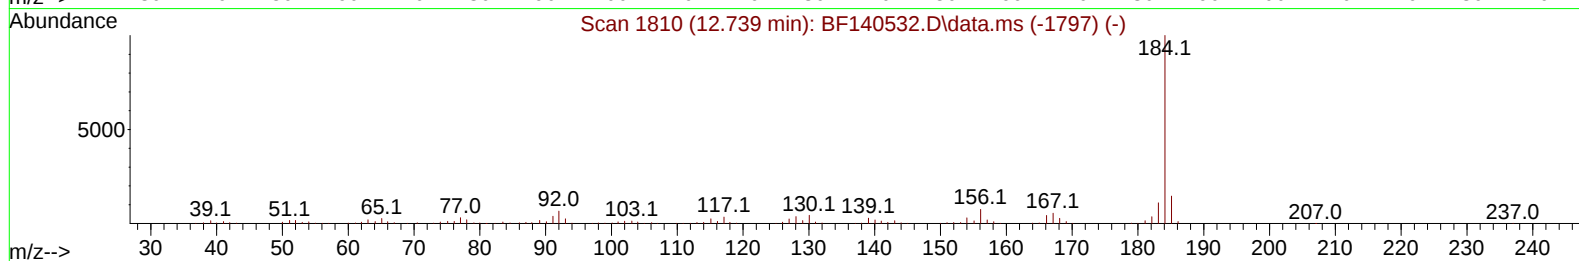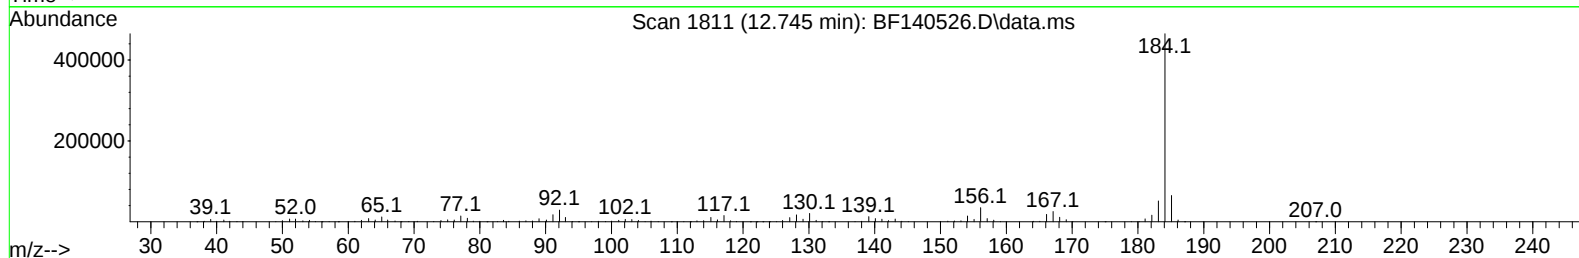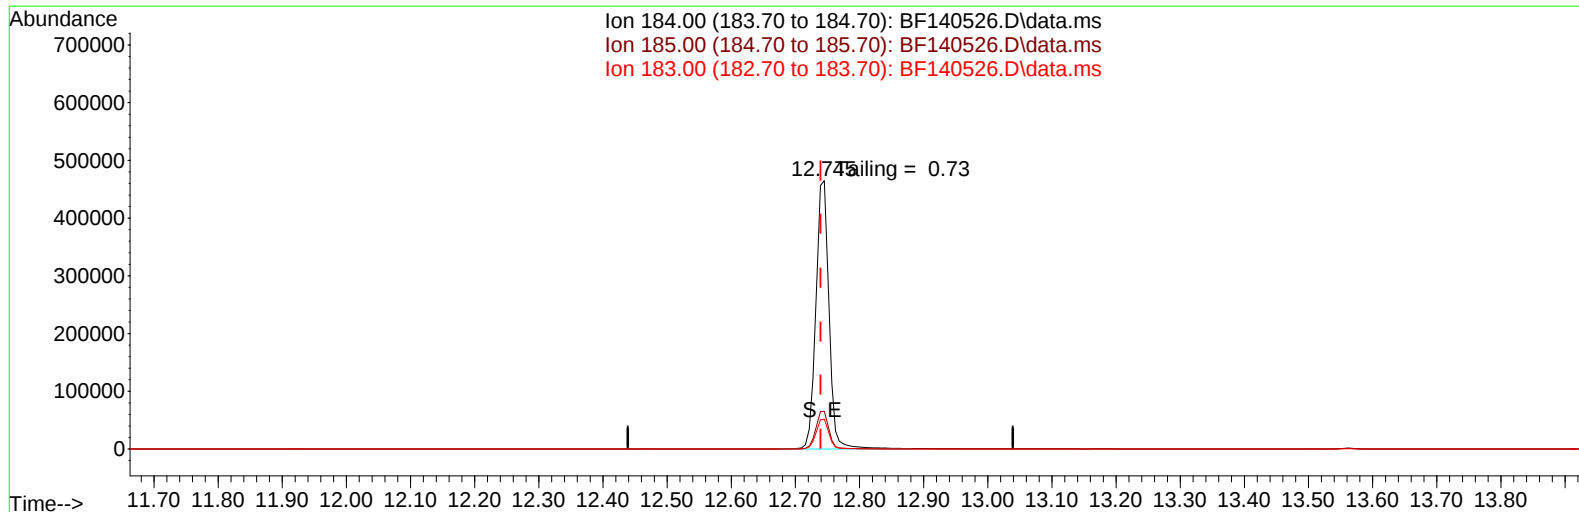

TIC: BF140526.D\data.ms

**(77) Benzidine**

12.745min (+ 0.006) 32779.12 ng

response 668077

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.60  | 14.02  |
| 183.00 | 11.00  | 11.11  |
| 0.00   | 0.00   | 0.00   |