


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121324\
Data File : BF140837.D
Acq On : 13 Dec 2024 11:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

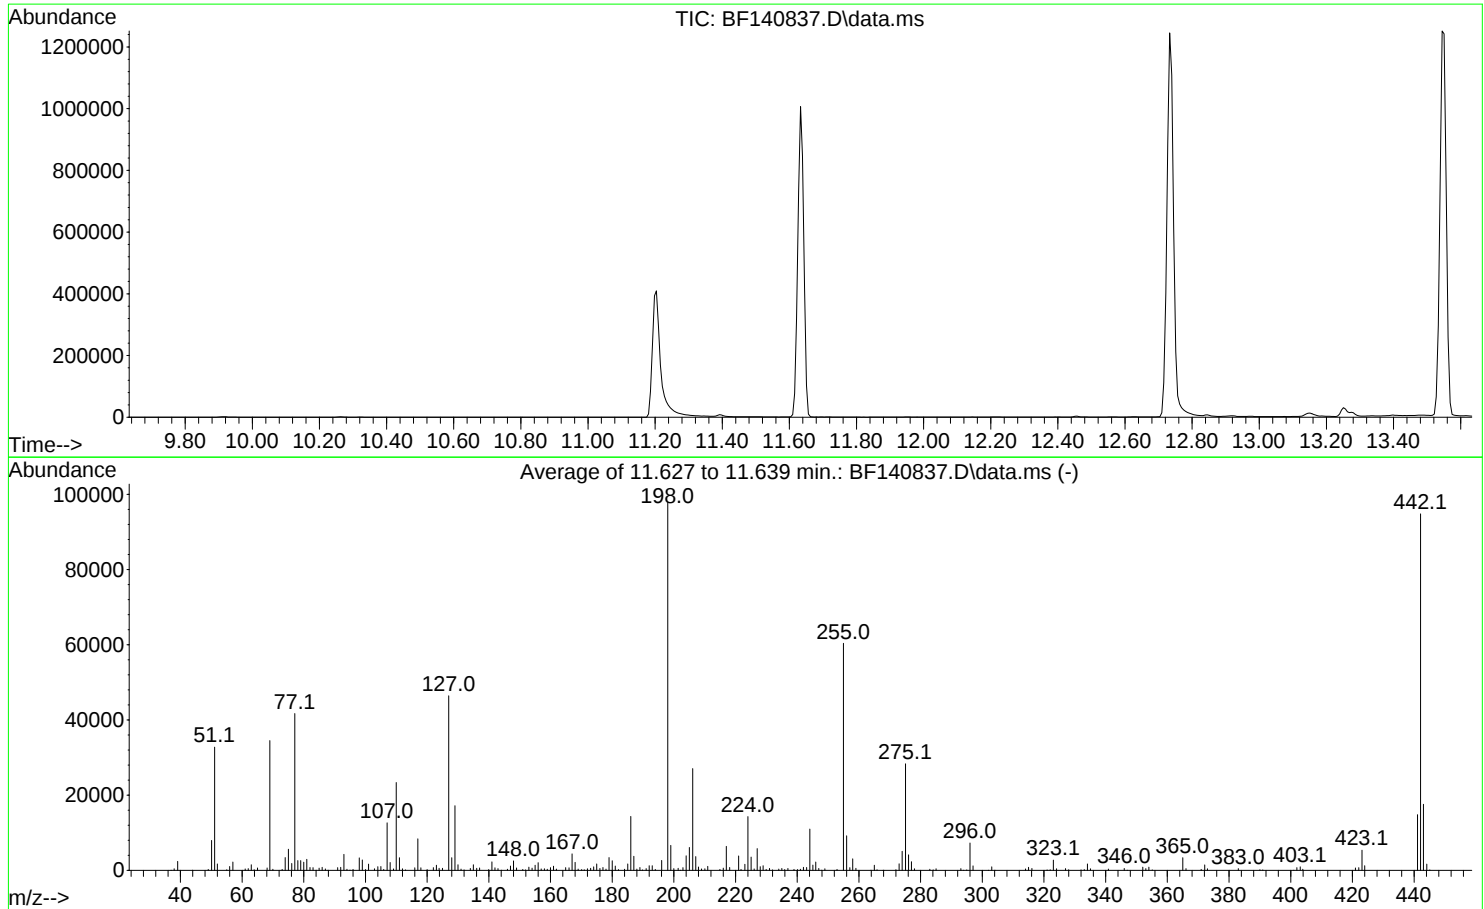

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	32749	PASS
68	69	0.00	2	1.9	640	PASS
69	198	0.00	100	35.3	34501	PASS
70	69	0.00	2	0.8	285	PASS
127	198	10	80	47.4	46419	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97829	PASS
199	198	5	9	6.8	6649	PASS
275	198	10	60	29.0	28363	PASS
365	198	1	100	3.4	3375	PASS
441	198	0.01	100	15.1	14794	PASS
442	442	50	100	100.0	94824	PASS
443	442	15	24	18.5	17582	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/13/2024	BNA_F	<u>BF140837.D</u>
Compound Name	Response	Retention Time
DDT	337813	13.551
DDD	12498	13.251
DDE	1383	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13881	351694	3.95

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121324\
Data File : BF140837.D
Acq On : 13 Dec 2024 11:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 13 16:12:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

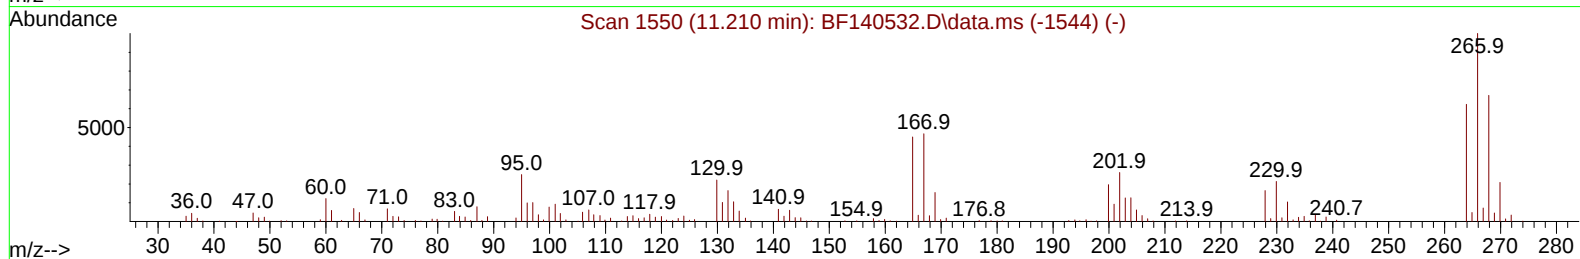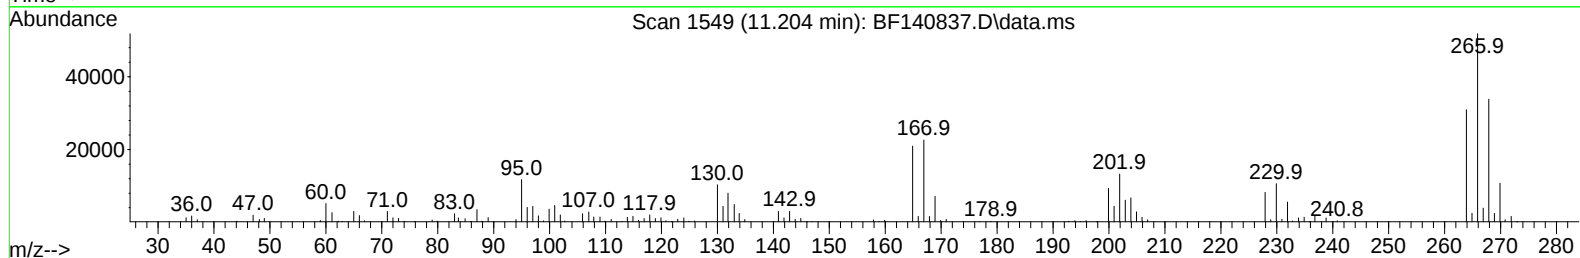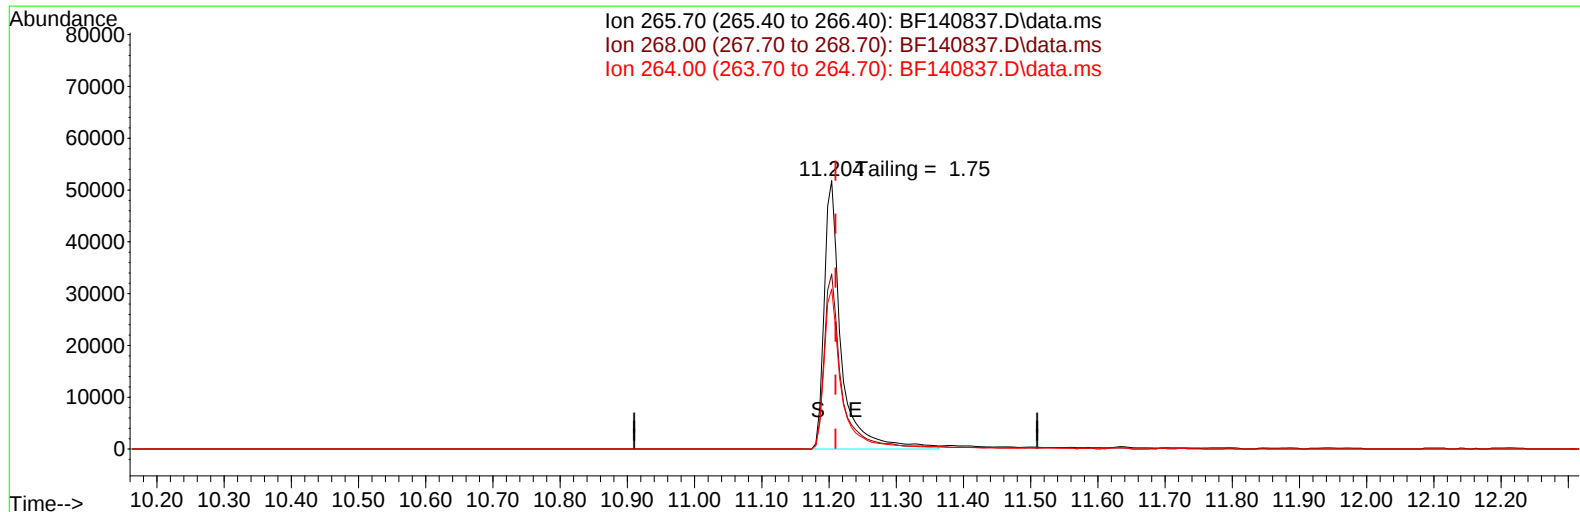

TIC: BF140837.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 3831.04 ng m




response 91786

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	65.26
264.00	62.30	59.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121324\
Data File : BF140837.D
Acq On : 13 Dec 2024 11:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 13 16:12:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

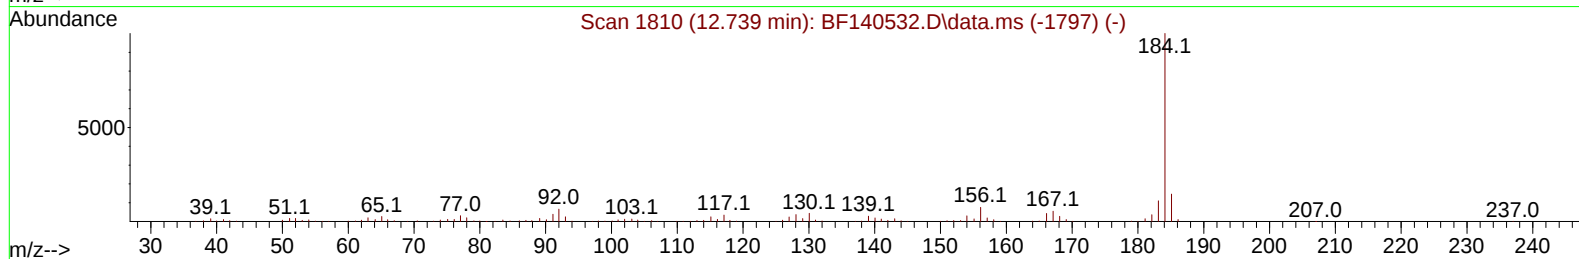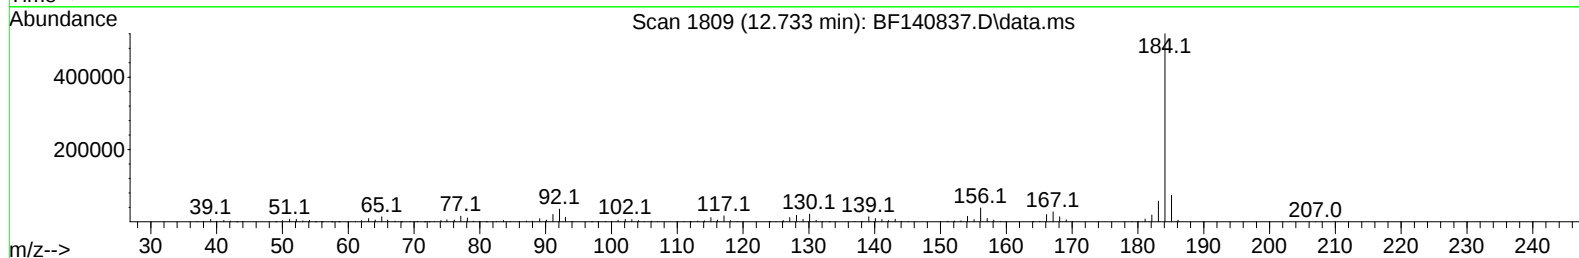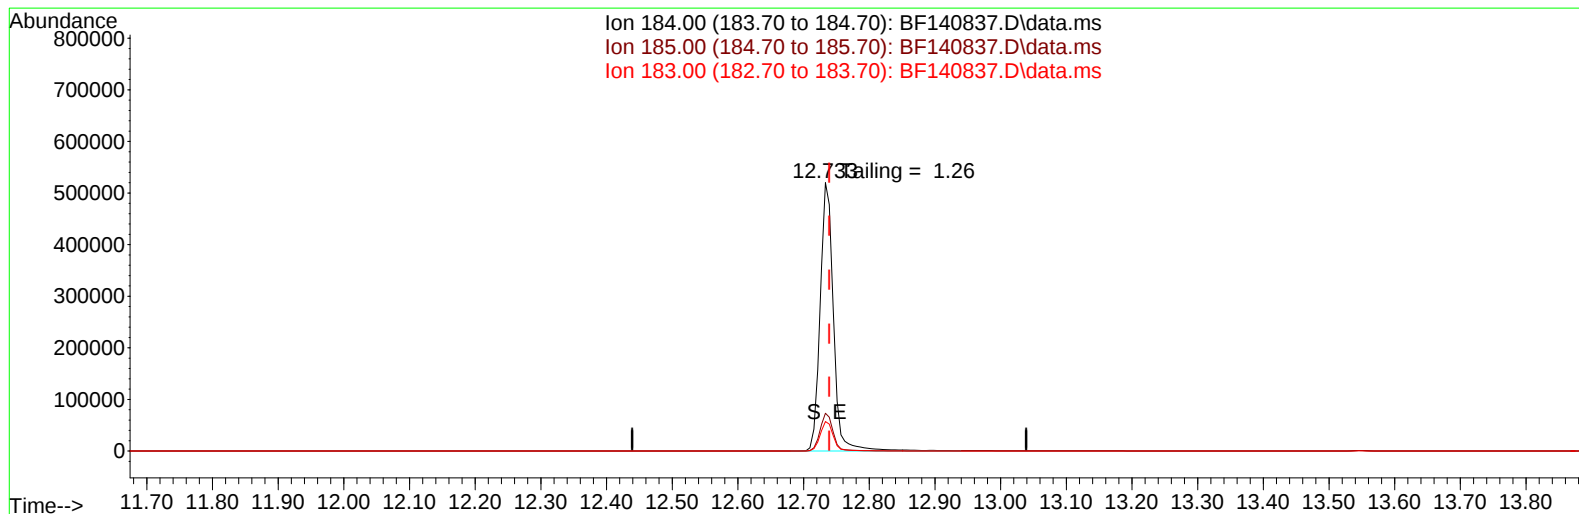

TIC: BF140837.D\data.ms

(77) Benzidine

12.733min (-0.006) 4659.58 ng

response 731021

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.09
183.00	11.00	11.00
0.00	0.00	0.00