


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121724\
Data File : BF140871.D
Acq On : 17 Dec 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 16 16:59:50 2024

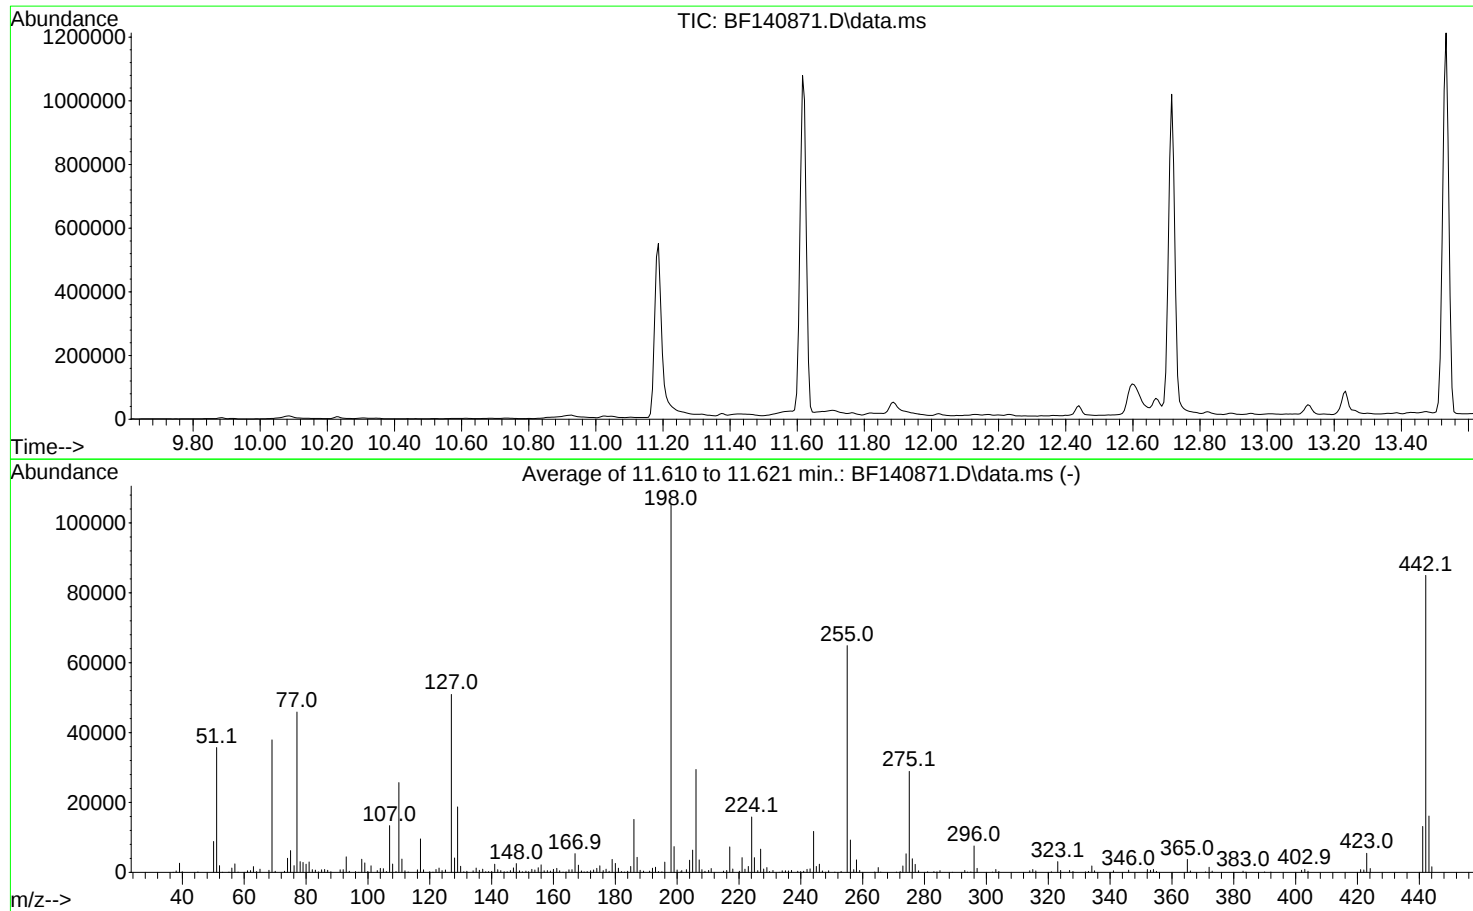

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	35723	PASS
68	69	0.00	2	1.6	613	PASS
69	198	0.00	100	36.0	37923	PASS
70	69	0.00	2	0.8	308	PASS
127	198	10	80	48.4	50941	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	105283	PASS
199	198	5	9	7.0	7376	PASS
275	198	10	60	27.5	28917	PASS
365	198	1	100	3.5	3701	PASS
441	198	0.01	100	12.5	13159	PASS
442	442	50	100	100.0	84981	PASS
443	442	15	24	19.0	16139	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/17/2024	BNA_F	<u>BF140871.D</u>
Compound Name	Response	Retention Time
DDT	301277	13.533
DDD	21919	13.233
DDE	1352	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23271	324548	7.17

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121724\
Data File : BF140871.D
Acq On : 17 Dec 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 17 10:34:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

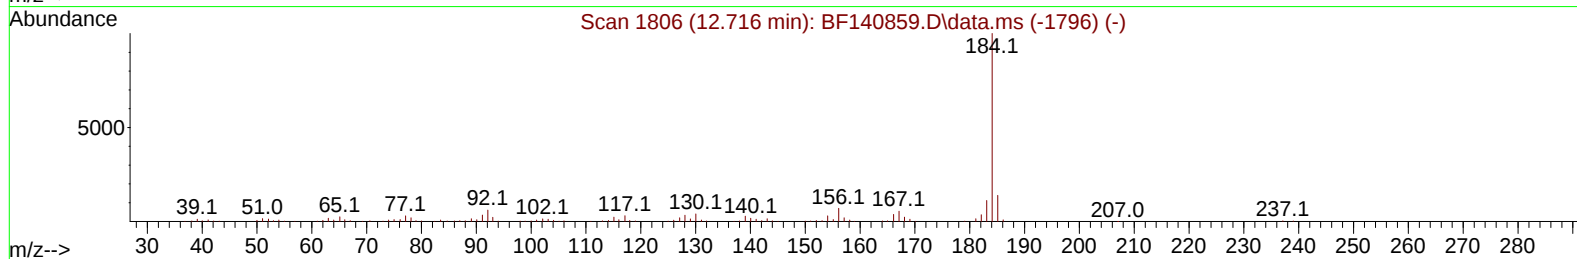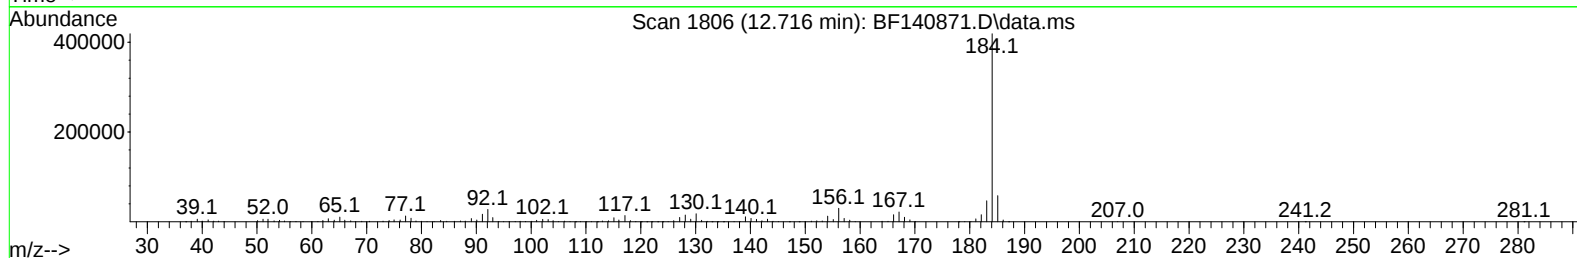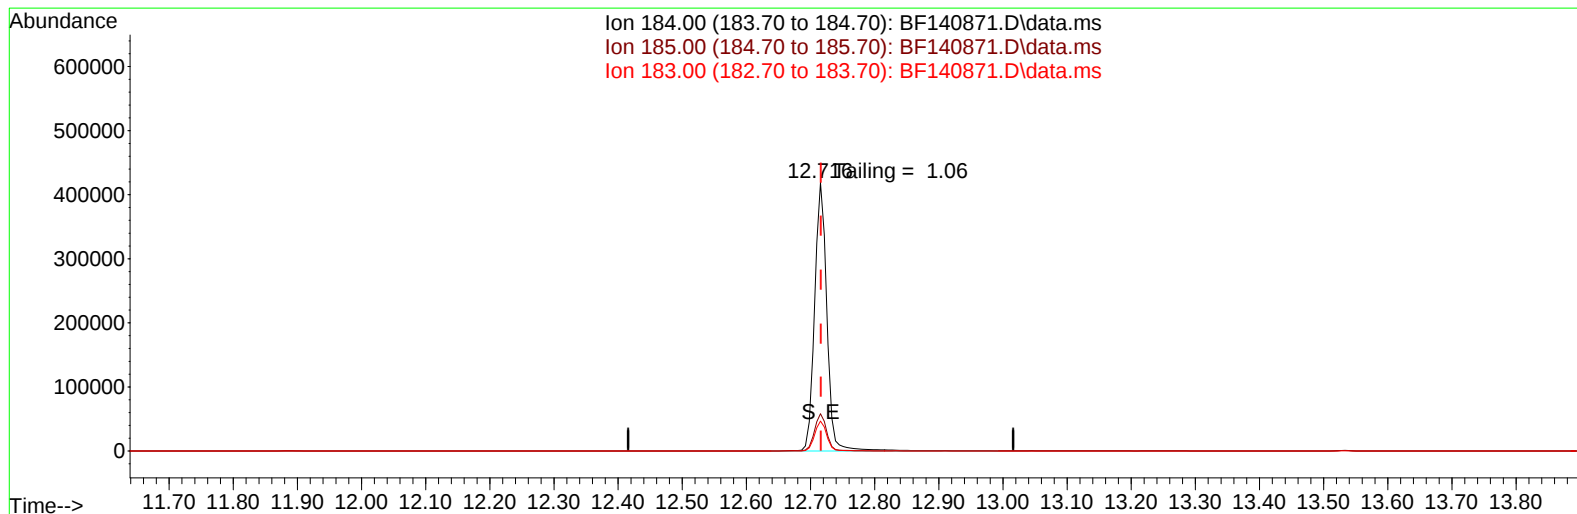

TIC: BF140871.D\data.ms

(77) Benzidine

12.716min (-0.000) 4637.75 ng

response 561870

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.89
183.00	11.20	11.16
0.00	0.00	0.00