

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121924\
Data File : FE051706.D
Signal(s) : FID1B.ch
Acq On : 19 Dec 2024 11:00
Operator : YP\AJ
Sample : P5279-01 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
ROCKAWAY-PARK

Integration File: Sample.e
Quant Time: Dec 20 02:44:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE121824.M
Quant Title :
QLast Update : Thu Dec 19 02:46:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.074	388024	3.148 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE121924\
Data File : FE051706.D
Signal(s) : FID1B.ch
Acq On : 19 Dec 2024 11:00
Operator : YP\AJ
Sample : P5279-01 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
ROCKAWAY-PARK

Integration File: Sample.e
Quant Time: Dec 20 02:44:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE121824.M
Quant Title :
QLast Update : Thu Dec 19 02:46:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

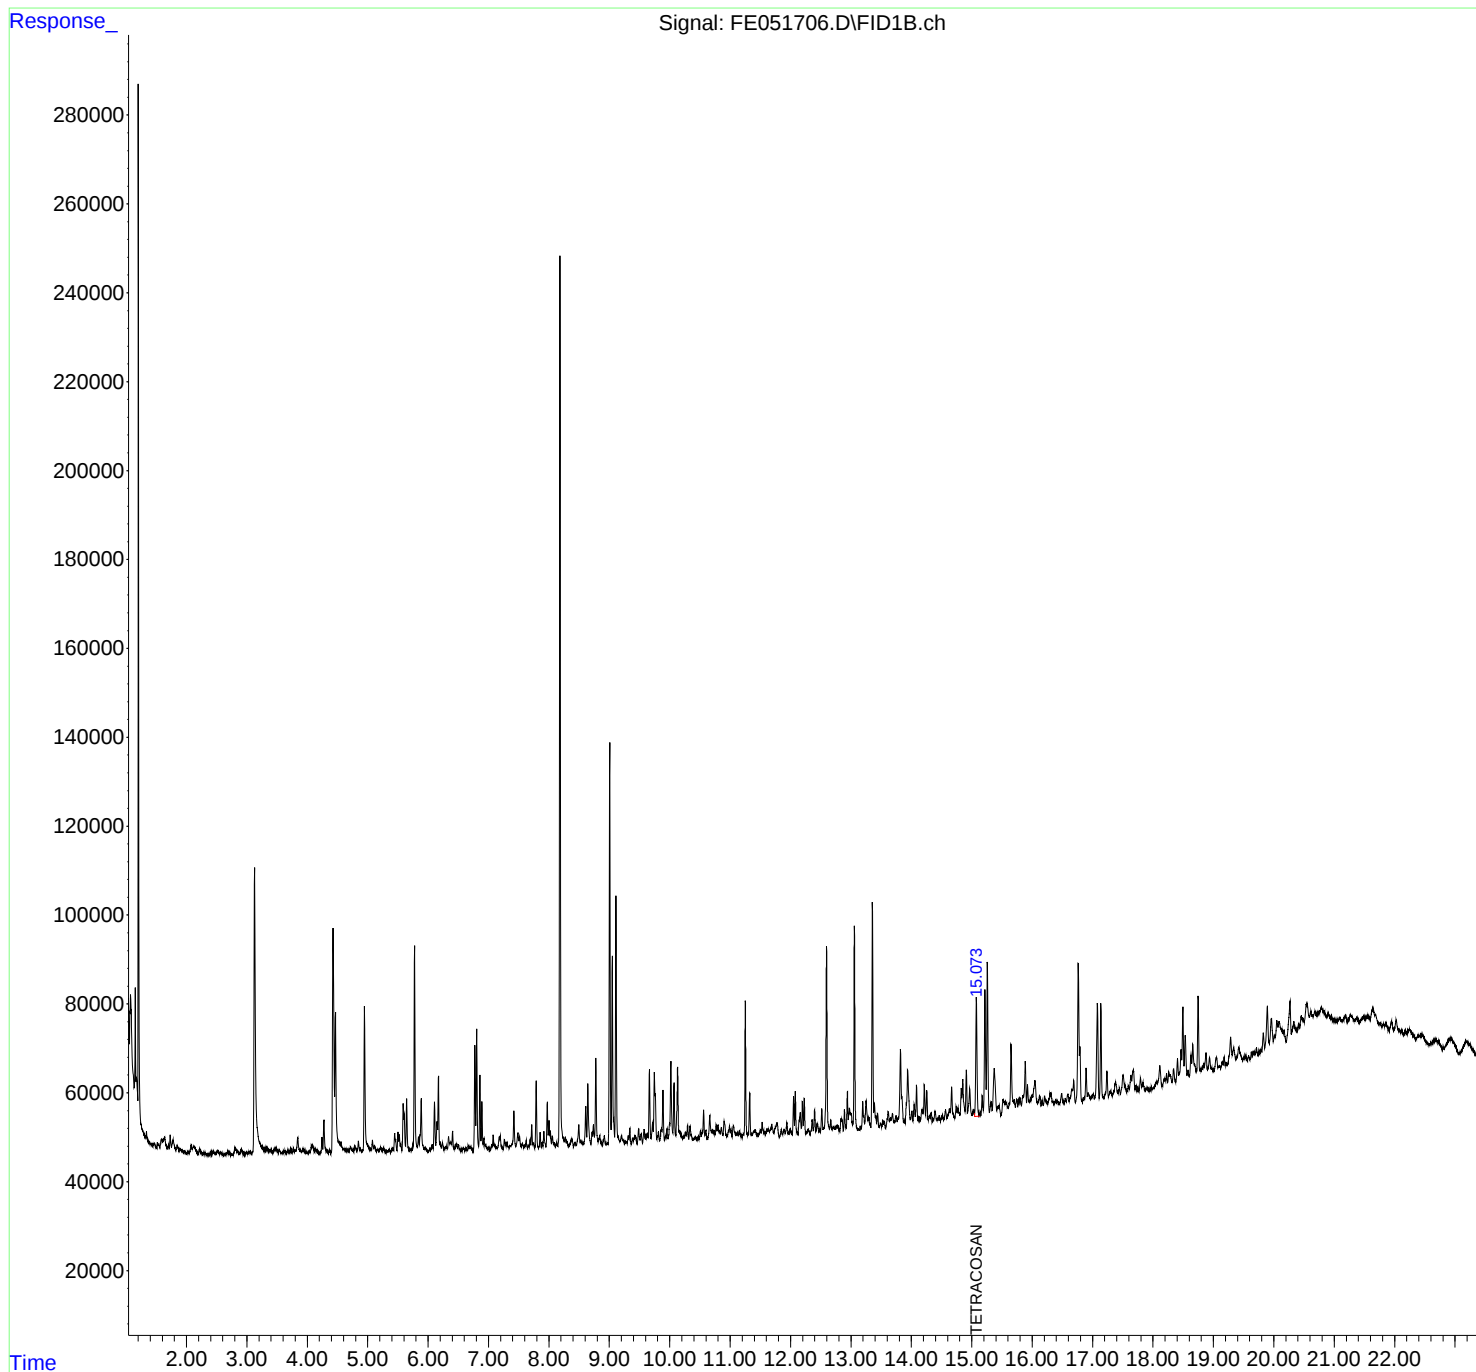

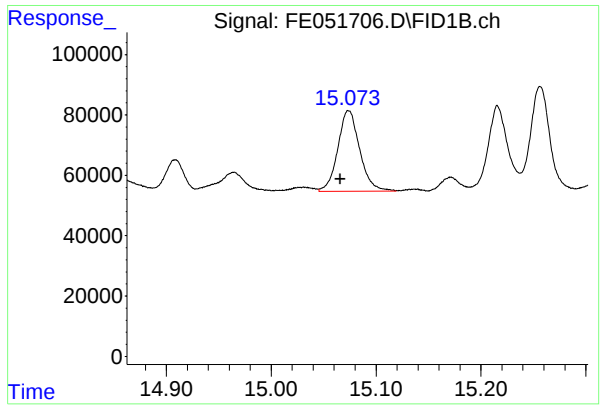

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.074 min
Delta R.T.: 0.008 min
Response: 388024
Conc: 3.15 ug/ml

Instrument :
FID_E
ClientSampleId :
ROCKAWAY-PARK