
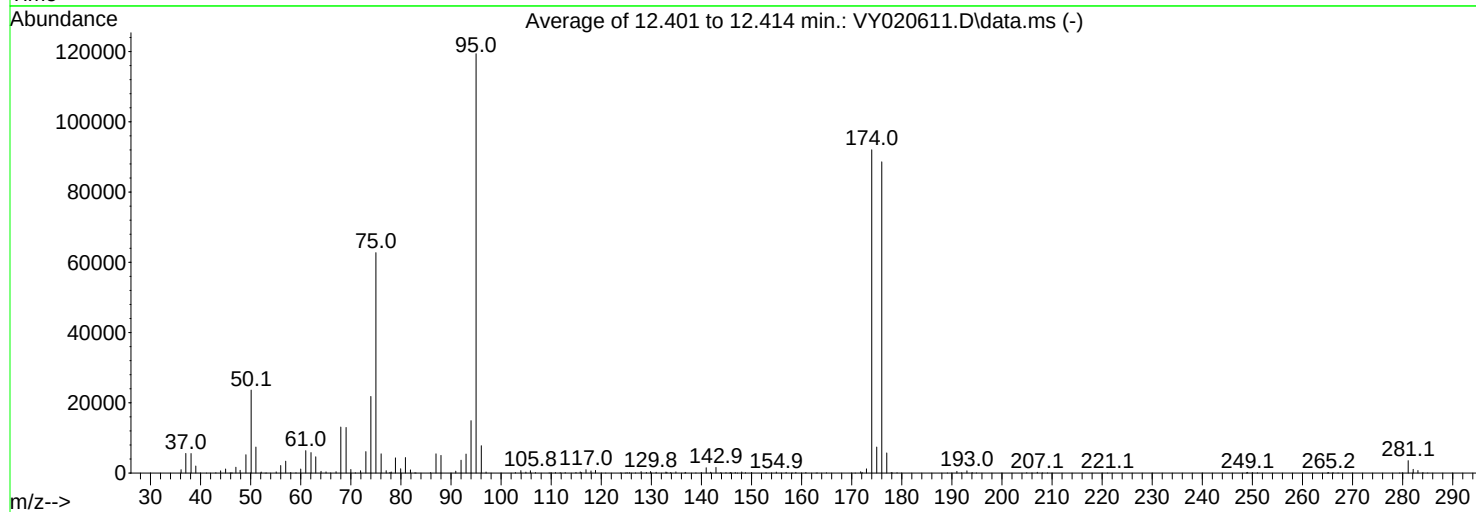


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY121724\
Data File : VY020611.D
Acq On : 17 Dec 2024 09:00
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y121724S.M
Title : SW846 8260
Last Update : Wed Dec 18 05:27:13 2024

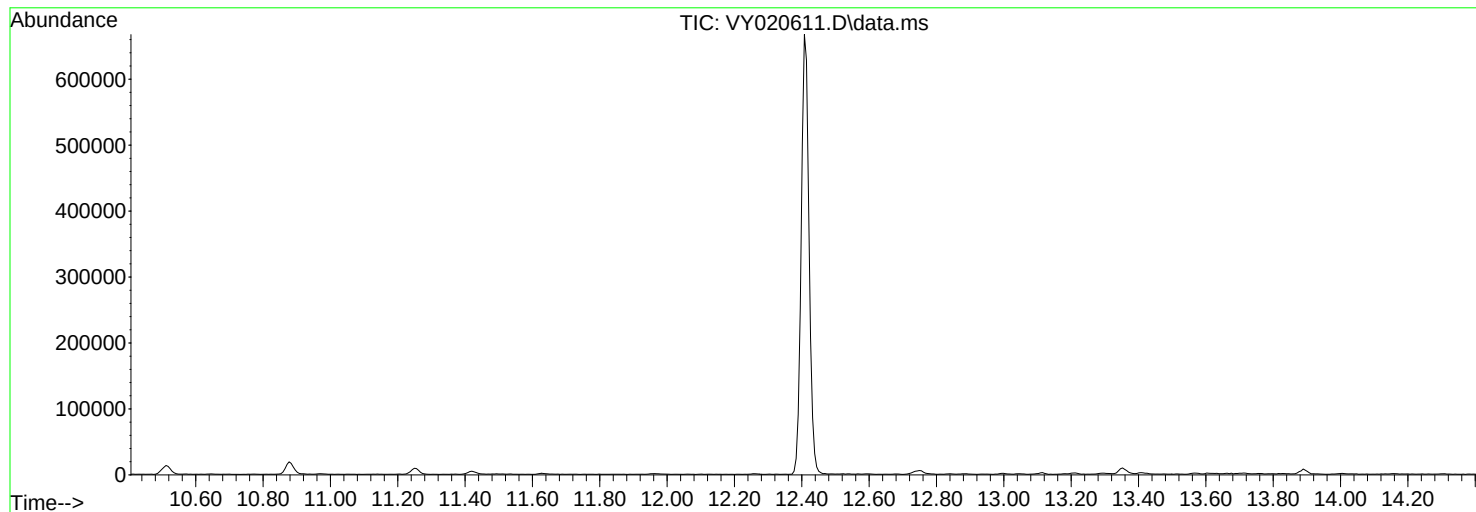

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	23624	PASS
75	95	30	60	52.6	62757	PASS
95	95	100	100	100.0	119384	PASS
96	95	5	9	6.5	7799	PASS
173	174	0.00	2	1.3	1208	PASS
174	95	50	100	77.1	92040	PASS
175	174	5	9	8.0	7407	PASS
176	174	95	101	96.3	88608	PASS
177	176	5	9	6.5	5728	PASS