


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121924\
Data File : BN035730.D
Acq On : 20 Dec 2024 07:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 19 23:06:19 2024



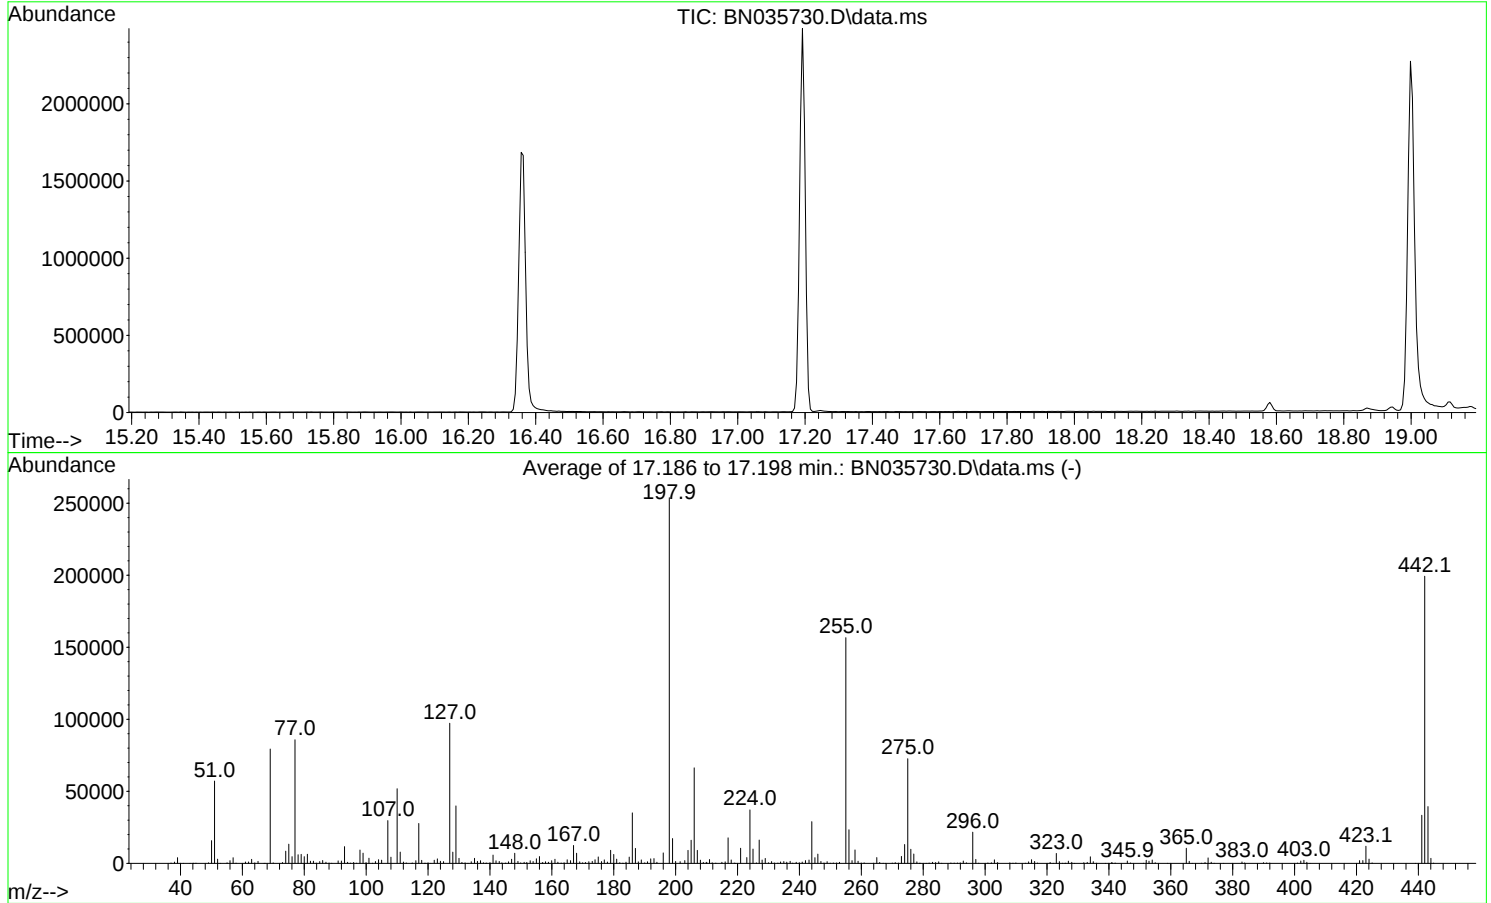


AutoFind: Scans 2431, 2432, 2433; Background Corrected with Scan 2424

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.5	57147	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.3	79373	PASS
70	69	0.00	2	0.5	393	PASS
127	198	10	80	38.3	97248	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	253824	PASS
199	198	5	9	6.8	17235	PASS
275	198	10	60	28.6	72629	PASS
365	198	1	100	4.1	10491	PASS
441	198	0.01	100	13.2	33387	PASS
442	442	50	100	100.0	199296	PASS
443	442	15	24	19.8	39411	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 20 08:05:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 08:05:13 2024
Response via : Initial Calibration

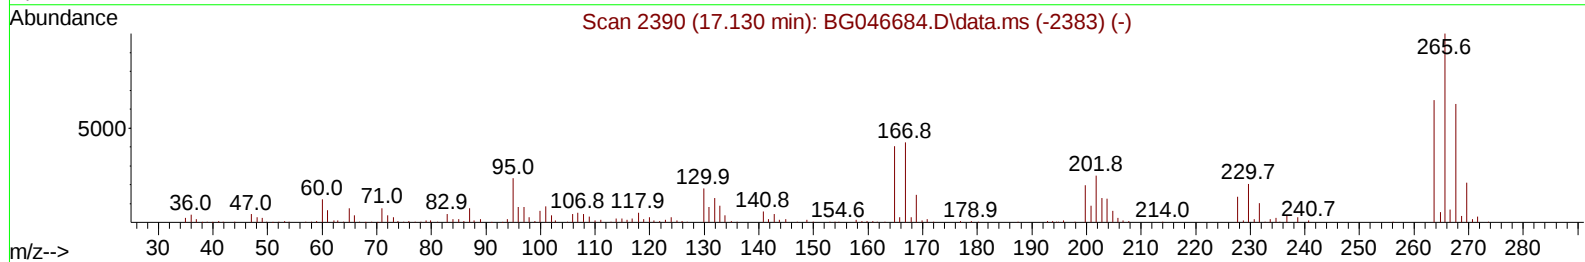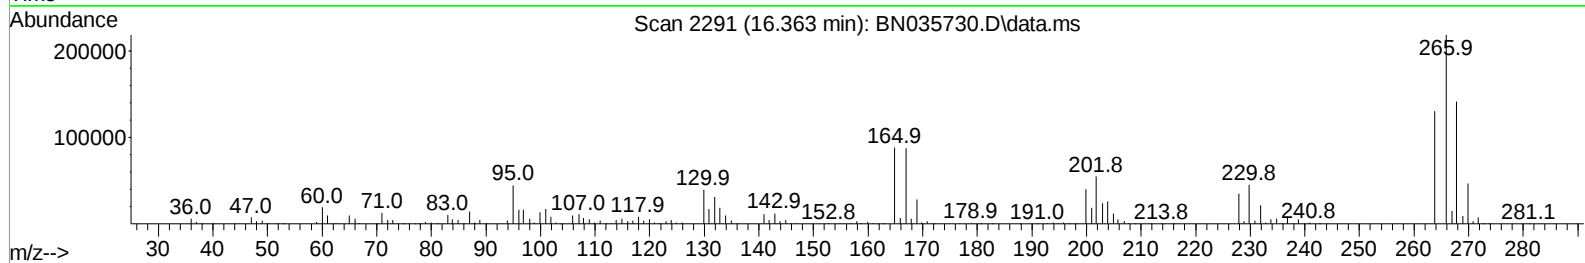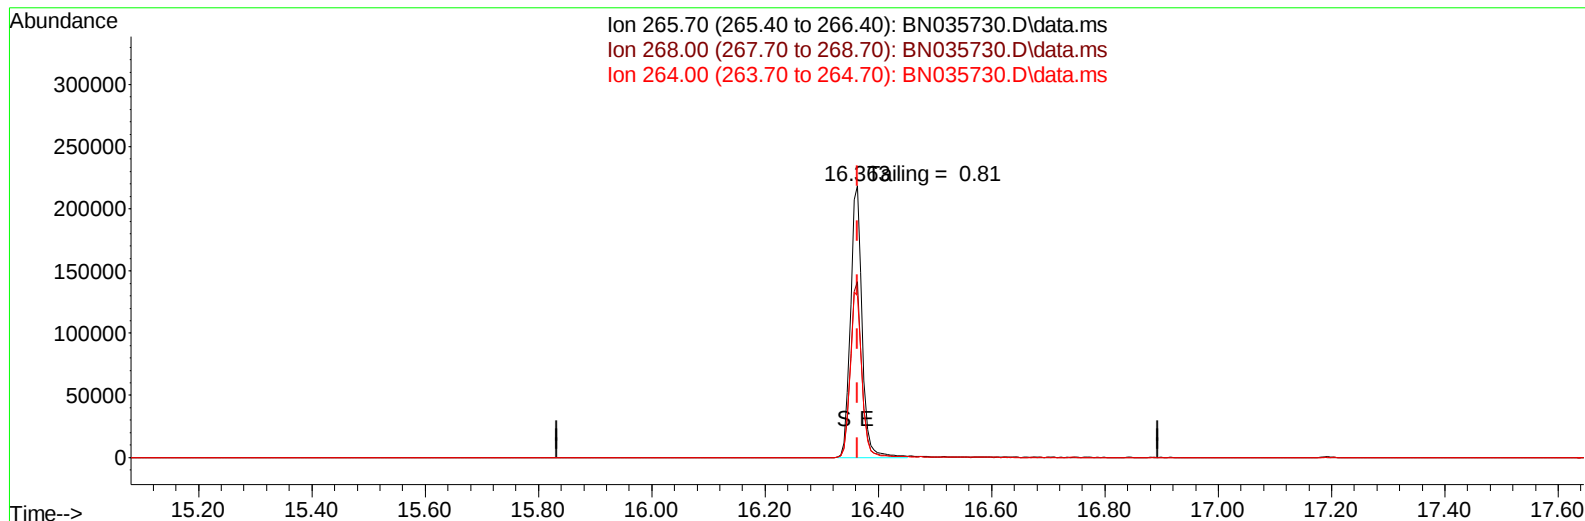

TIC: BN035730.D\data.ms

16.363min (0.000) 28931.39 ng




response **314005**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.75
264.00	61.60	59.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121924\
Data File : BN035730.D
Acq On : 20 Dec 2024 07:25
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 20 08:05:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 08:05:13 2024
Response via : Initial Calibration

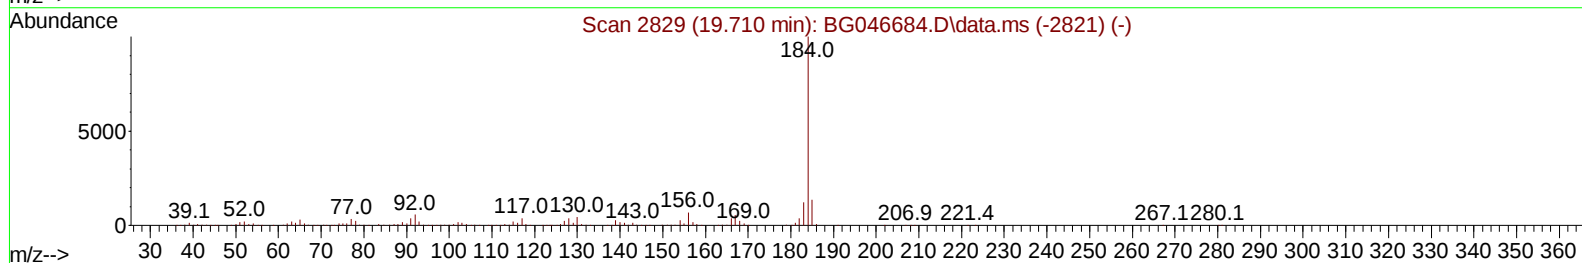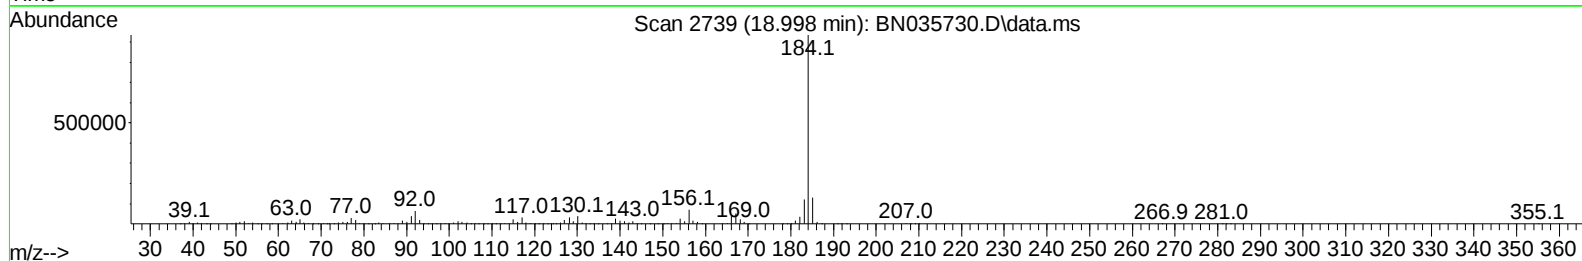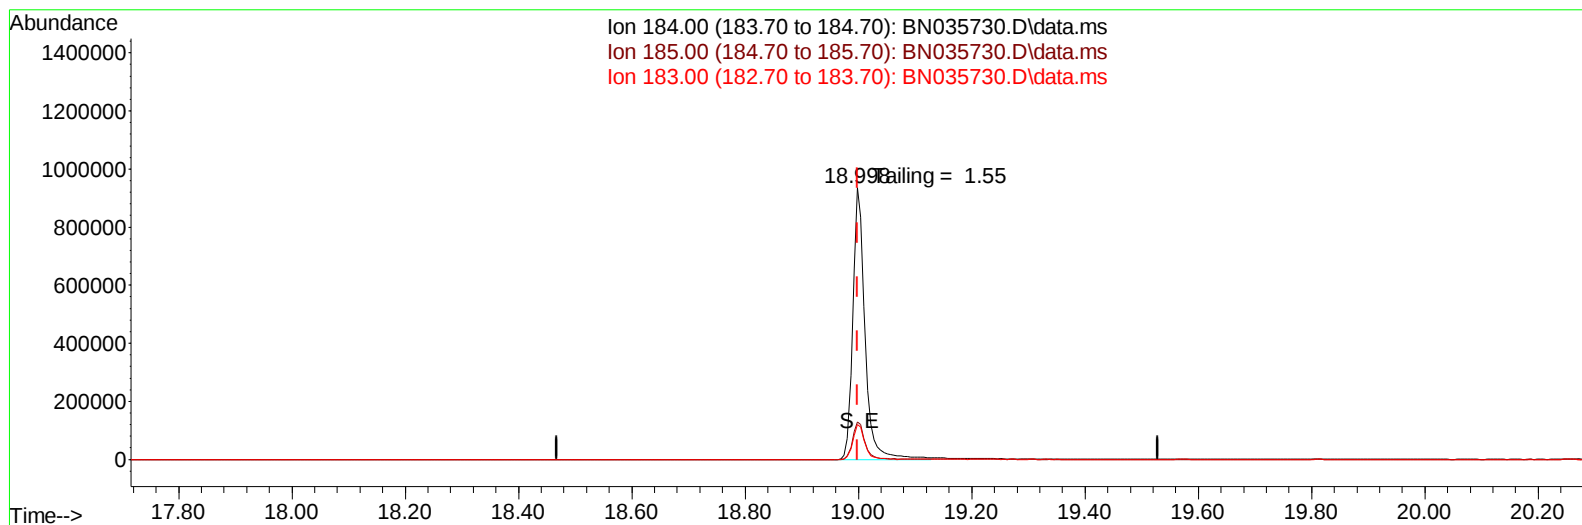

TIC: BN035730.D\data.ms

(77) Benzidine

18.998min (0.000) 0.00 ng

response 1433915

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.90
183.00	13.20	12.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/19/2024	BNA_N	<u>BN035730.D</u>
Compound Name	Response	Retention Time
DDT	433840	20.257
DDD	250906	19.81
DDE	2152	19.292
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
253058	686898	36.84

Instrument :
BNA_N
ClientSampleId :
DFTPP