
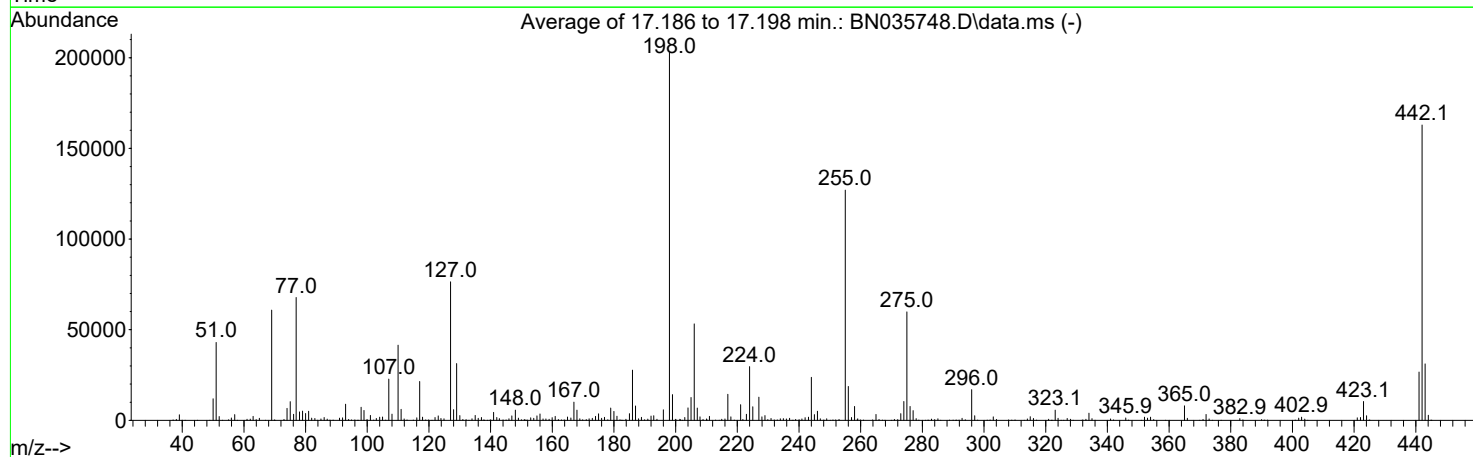


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121924\
Data File : BN035748.D
Acq On : 20 Dec 2024 18:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 19 23:06:19 2024

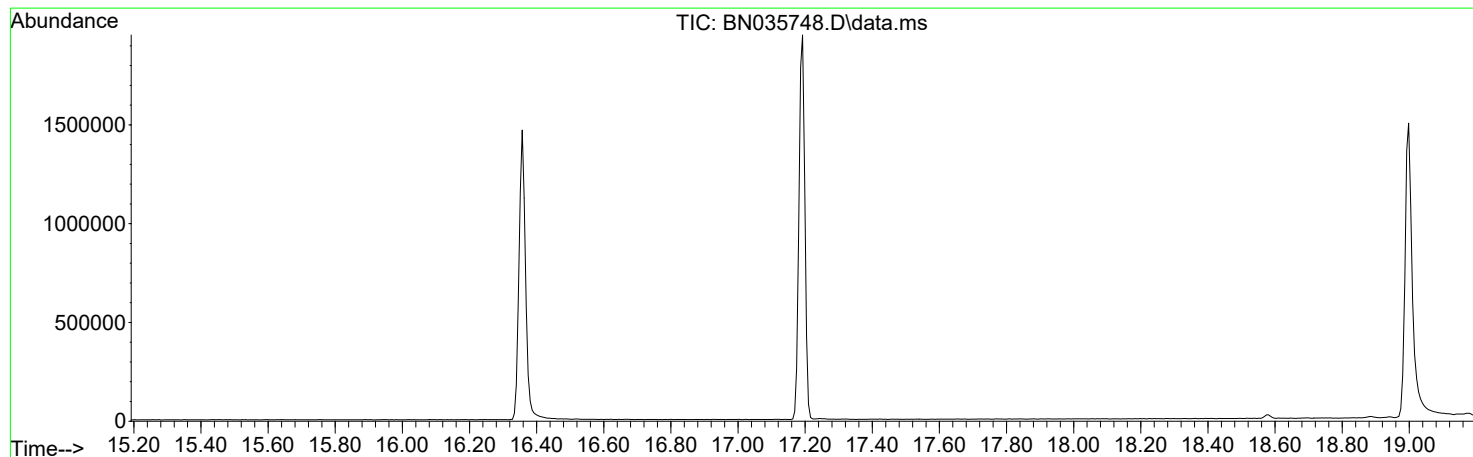

AutoFind: Scans 2431, 2432, 2433; Background Corrected with Scan 2424

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	21.2	43029	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.0	60827	PASS
70	69	0.00	2	0.5	295	PASS
127	198	10	80	37.7	76443	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	202901	PASS
199	198	5	9	7.0	14189	PASS
275	198	10	60	29.5	59856	PASS
365	198	1	100	4.0	8044	PASS
441	198	0.01	100	13.1	26624	PASS
442	442	50	100	100.0	162944	PASS
443	442	15	24	19.1	31128	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/19/2024	BNA_N	<u>BN035748.D</u>
Compound Name	Response	Retention Time
DDT	418200	20.257
DDD	184217	19.816
DDE	2622	19.292
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
186839	605039	30.88

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121924\
Data File : BN035748.D
Acq On : 20 Dec 2024 18:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 21 02:12:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 21 02:12:53 2024
Response via : Initial Calibration

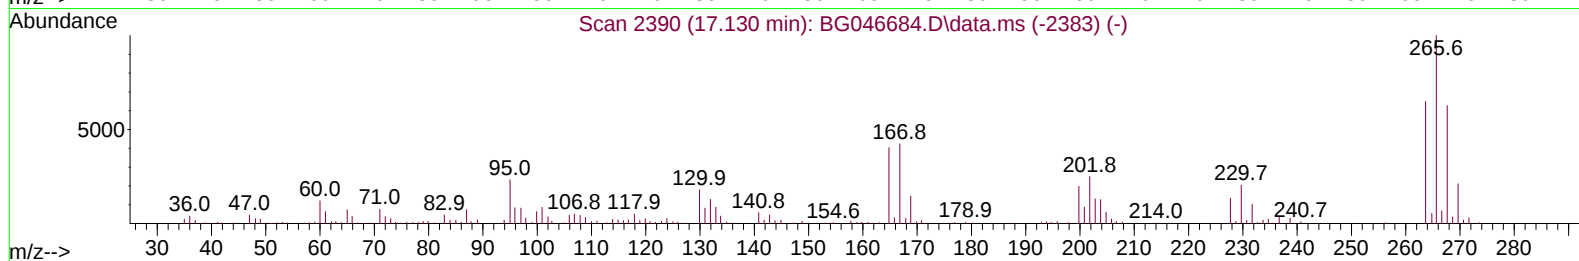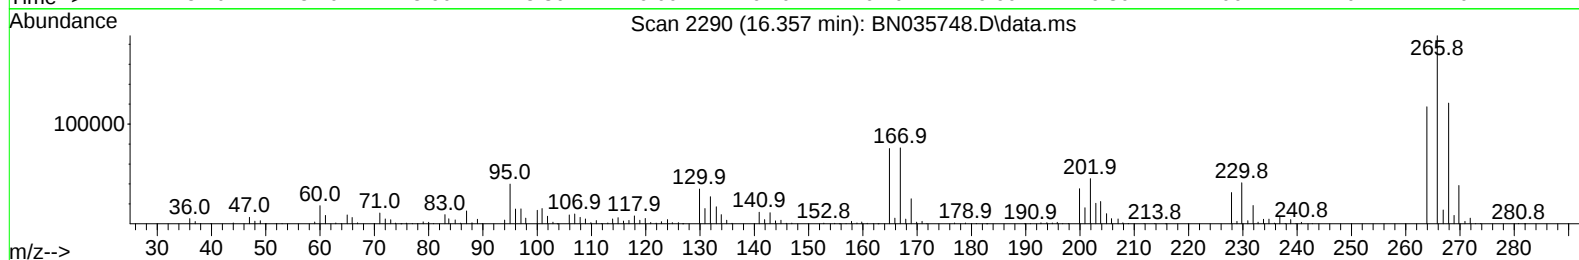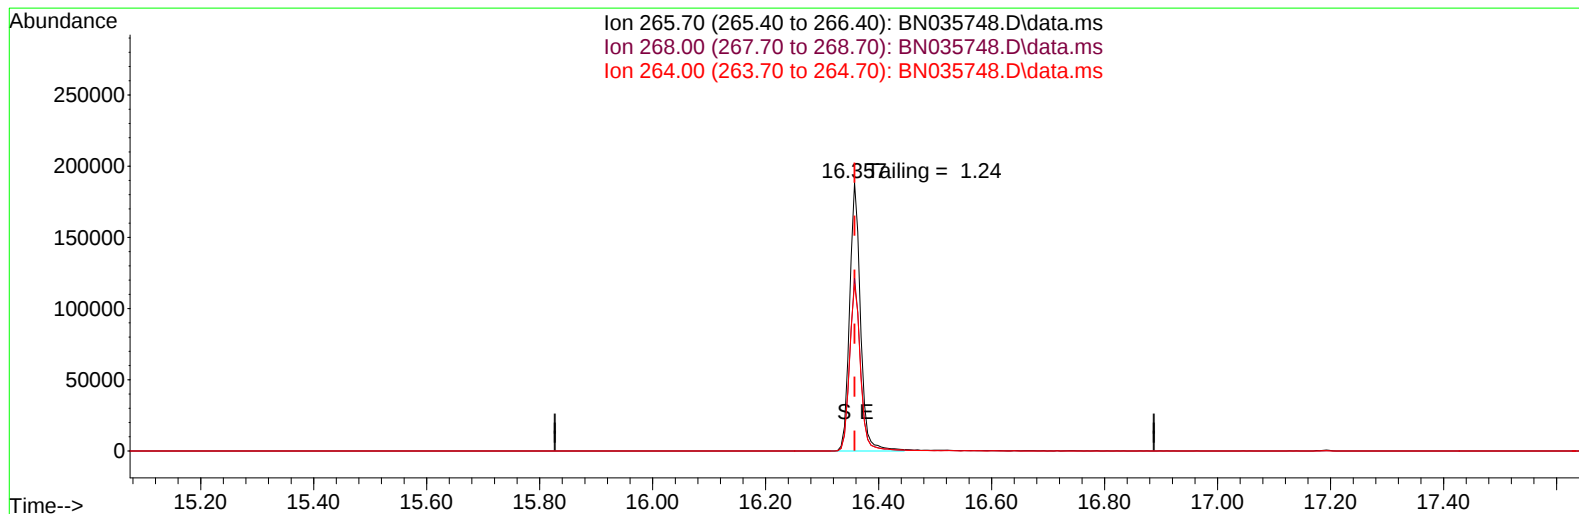

TIC: BN035748.D\data.ms

(70) Pentachlorophenol (C)

16.357min (0.000) 26492.80 ng

response 255312

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.24
264.00	61.60	62.22
0.00	0.00	0.00

