
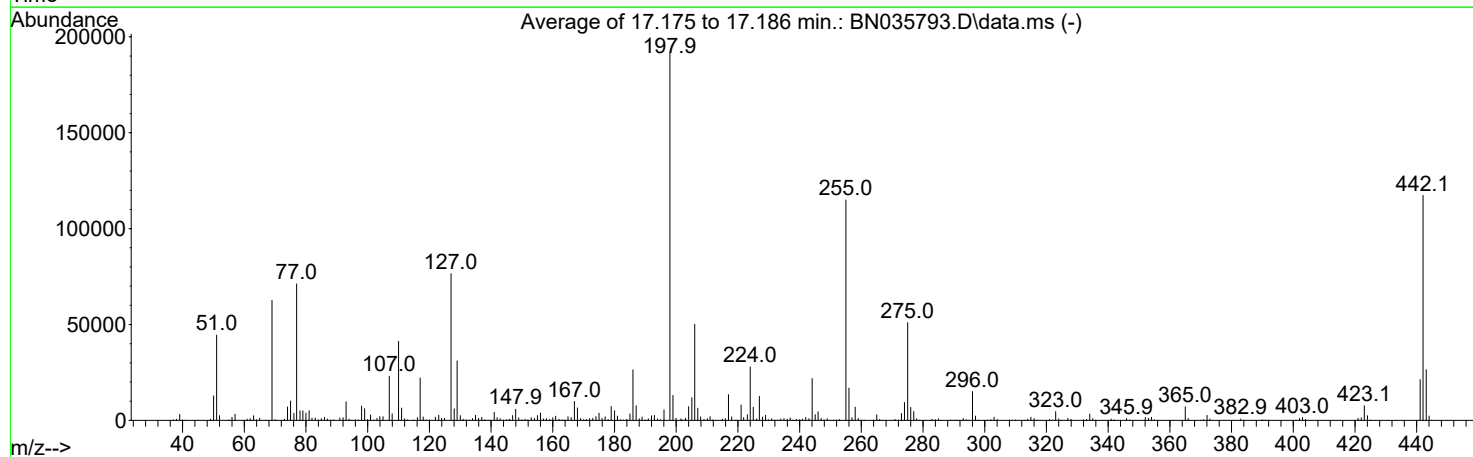


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035793.D
Acq On : 23 Dec 2024 20:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 19 23:06:19 2024

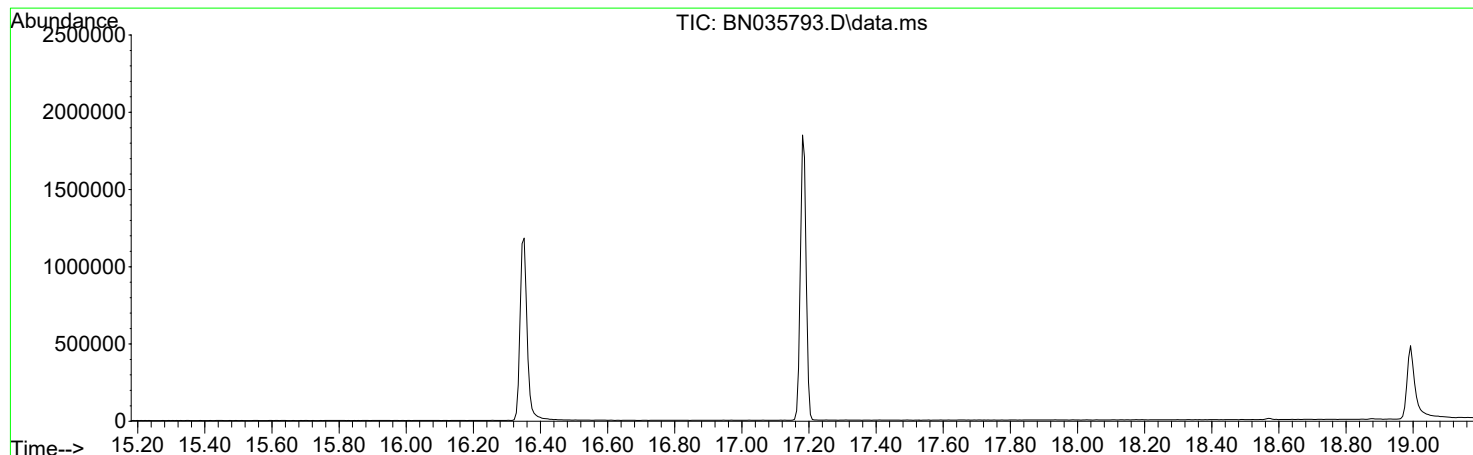

AutoFind: Scans 2429, 2430, 2431; Background Corrected with Scan 2423

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	23.2	44520	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.6	62576	PASS
70	69	0.00	2	0.6	362	PASS
127	198	10	80	39.9	76520	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	191851	PASS
199	198	5	9	6.8	13033	PASS
275	198	10	60	26.6	50979	PASS
365	198	1	100	3.7	7105	PASS
441	198	0.01	100	11.1	21259	PASS
442	442	50	100	100.0	117307	PASS
443	442	15	24	22.6	26498	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/23/2024	BNA_N	<u>BN035793.D</u>
Compound Name	Response	Retention Time
DDT	527491	20.245
DDD	59938	19.804
DDE	3046	19.286
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
62984	590475	10.67

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
 Data File : BN035793.D
 Acq On : 23 Dec 2024 20:26
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 24 06:28:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 24 06:28:04 2024
 Response via : Initial Calibration

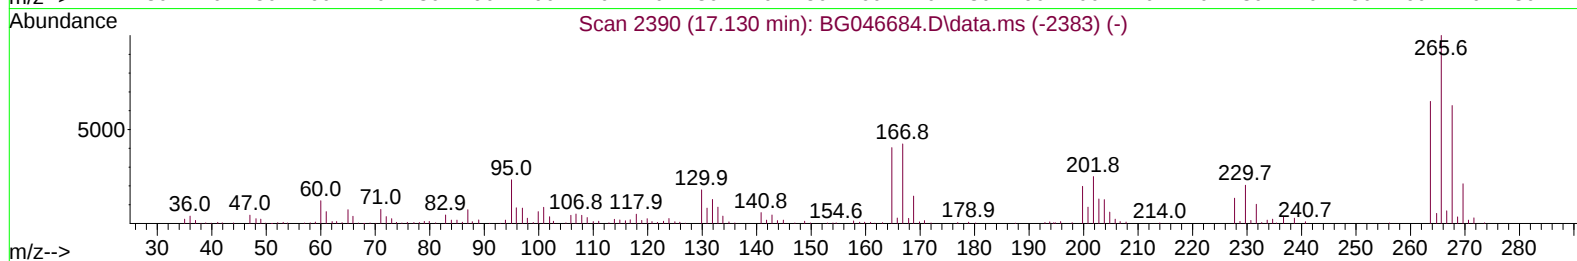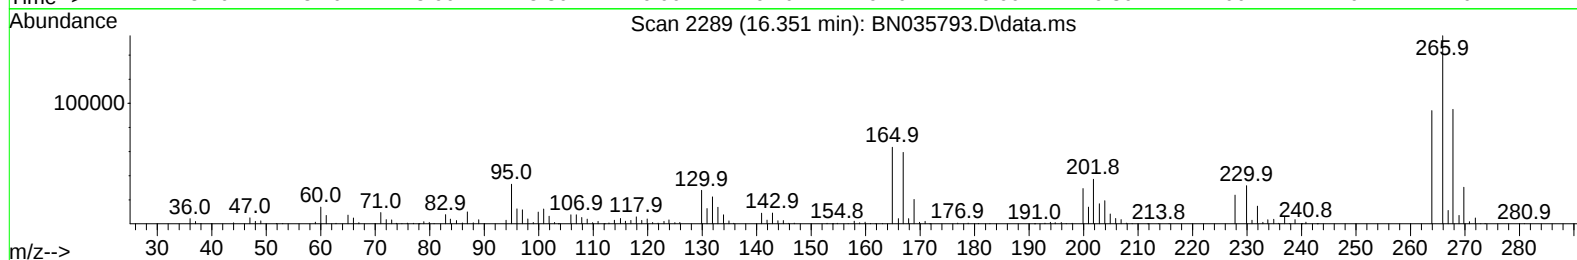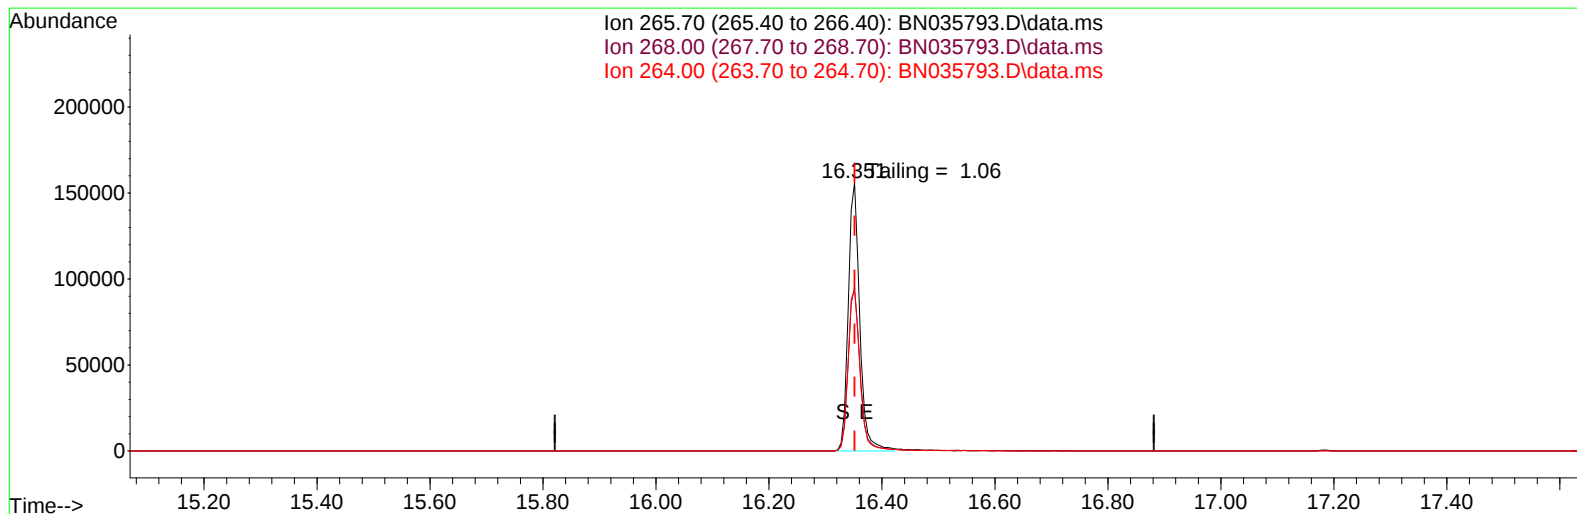

TIC: BN035793.D\data.ms

(70) Pentachlorophenol (C)

16.351min (0.000) 22129.06 ng




response 222810

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.87
264.00	61.60	60.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035793.D
Acq On : 23 Dec 2024 20:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 24 06:28:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 24 06:28:04 2024
Response via : Initial Calibration

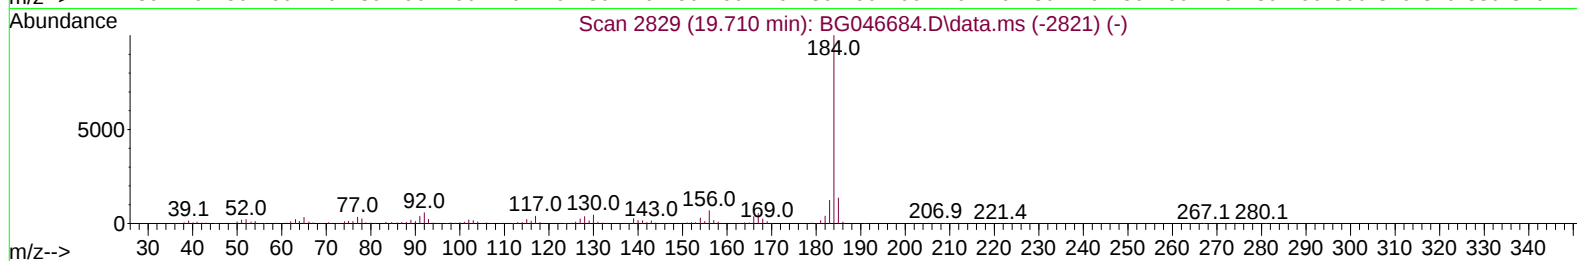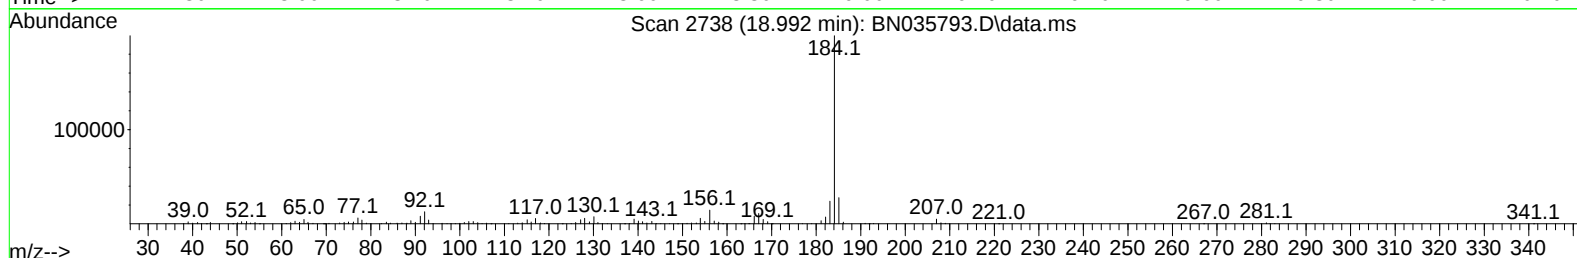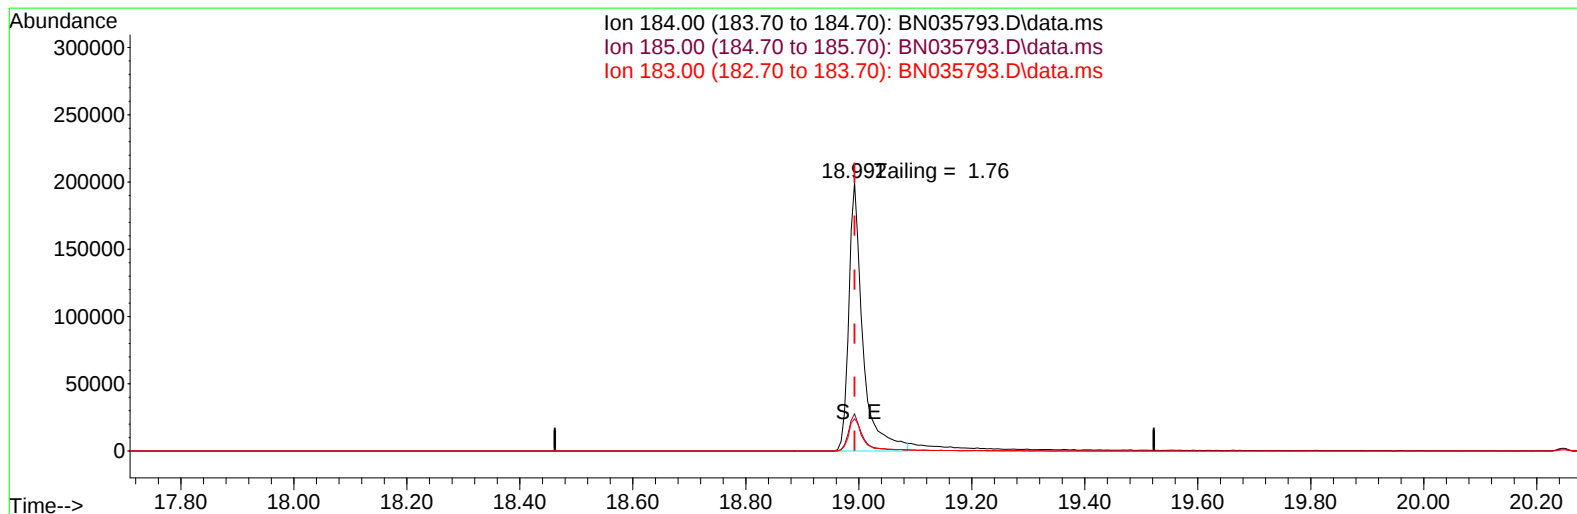

TIC: BN035793.D\data.ms

(77) Benzidine

18.992min (0.000) 0.00 ng

response 368634

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.92
183.00	13.20	12.06
0.00	0.00	0.00