


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122624\
Data File : BN035844.D
Acq On : 26 Dec 2024 09:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 19 23:06:19 2024

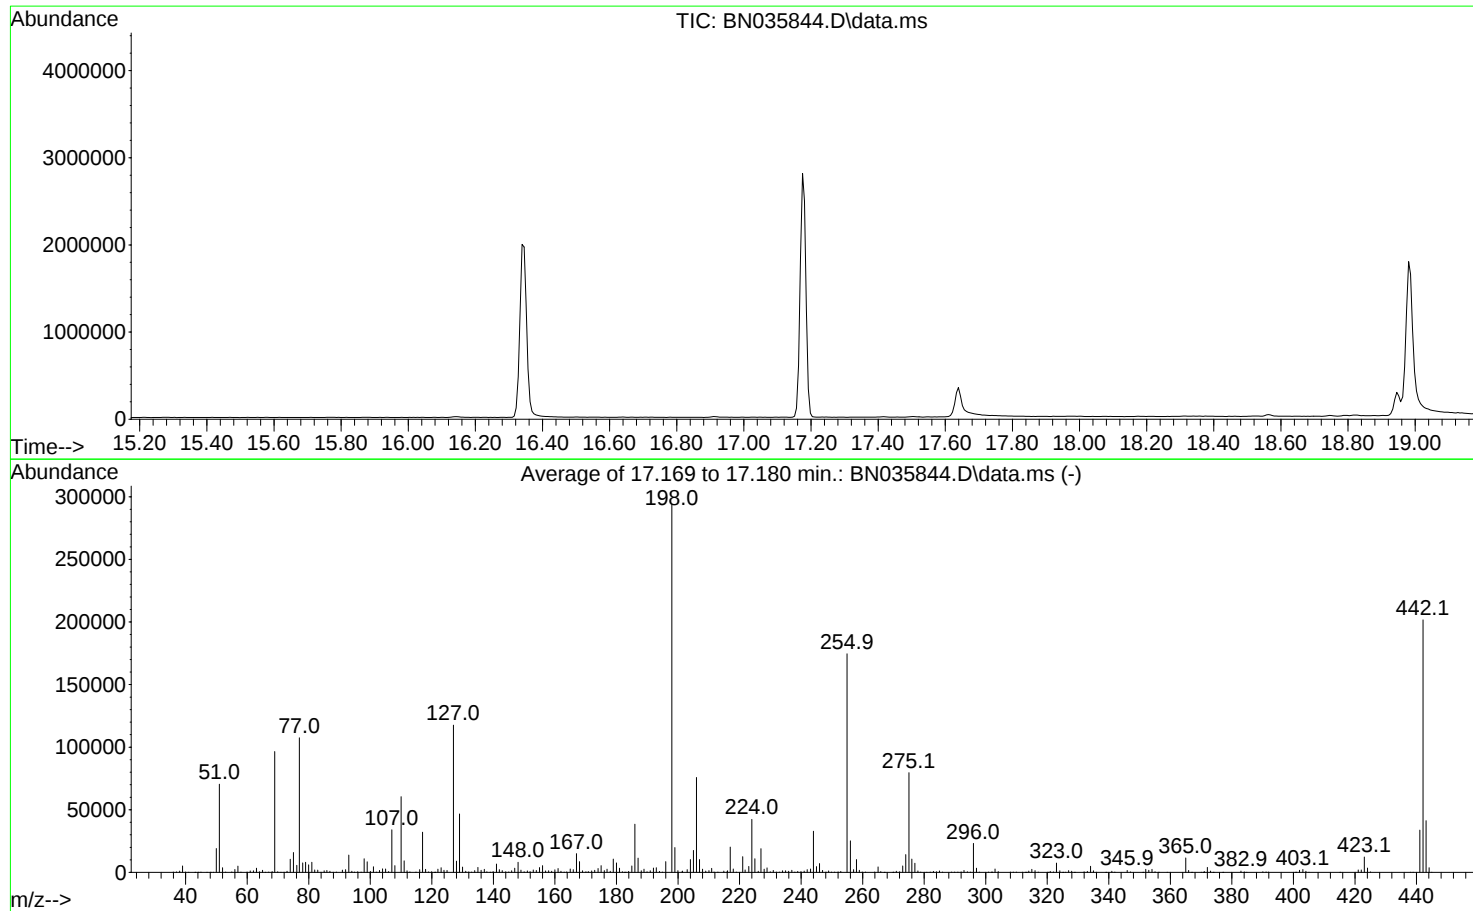

AutoFind: Scans 2428, 2429, 2430; Background Corrected with Scan 2422

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	24.0	70451	PASS
68	69	0.00	2	0.6	610	PASS
69	198	0.00	100	32.9	96557	PASS
70	69	0.00	2	0.5	480	PASS
127	198	10	80	40.0	117549	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	293824	PASS
199	198	5	9	6.7	19833	PASS
275	198	10	60	27.1	79648	PASS
365	198	1	100	3.9	11517	PASS
441	198	0.01	100	11.5	33733	PASS
442	442	50	100	100.0	201656	PASS
443	442	15	24	20.5	41285	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/26/2024	BNA_N	<u>BN035844.D</u>
Compound Name	Response	Retention Time
DDT	999259	20.239
DDD	18711	19.798
DDE	516	19.28
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19227	1018486	1.89

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122624\
Data File : BN035844.D
Acq On : 26 Dec 2024 09:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 26 18:22:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

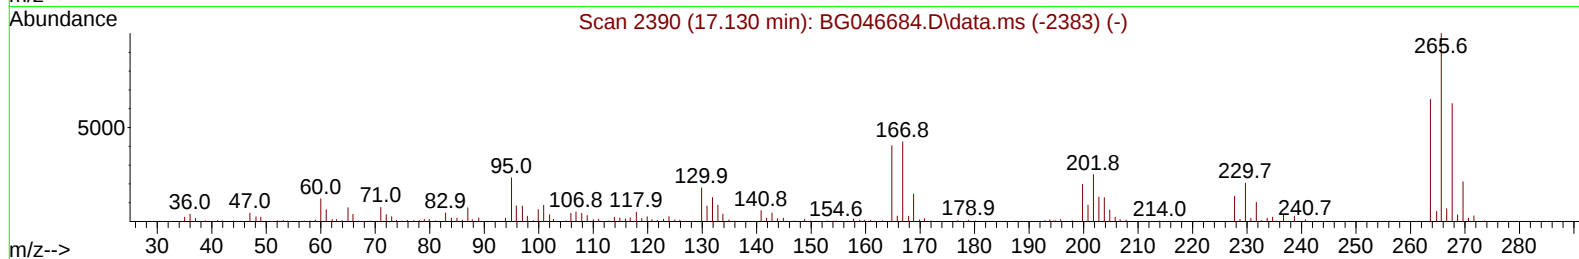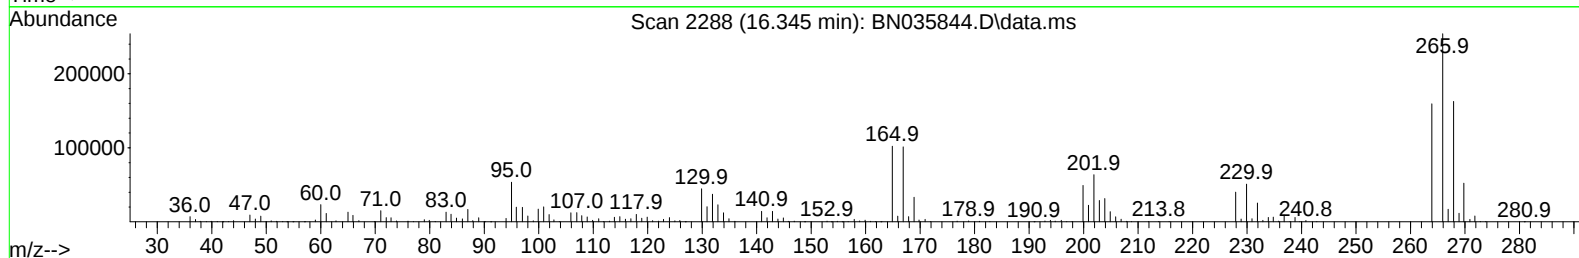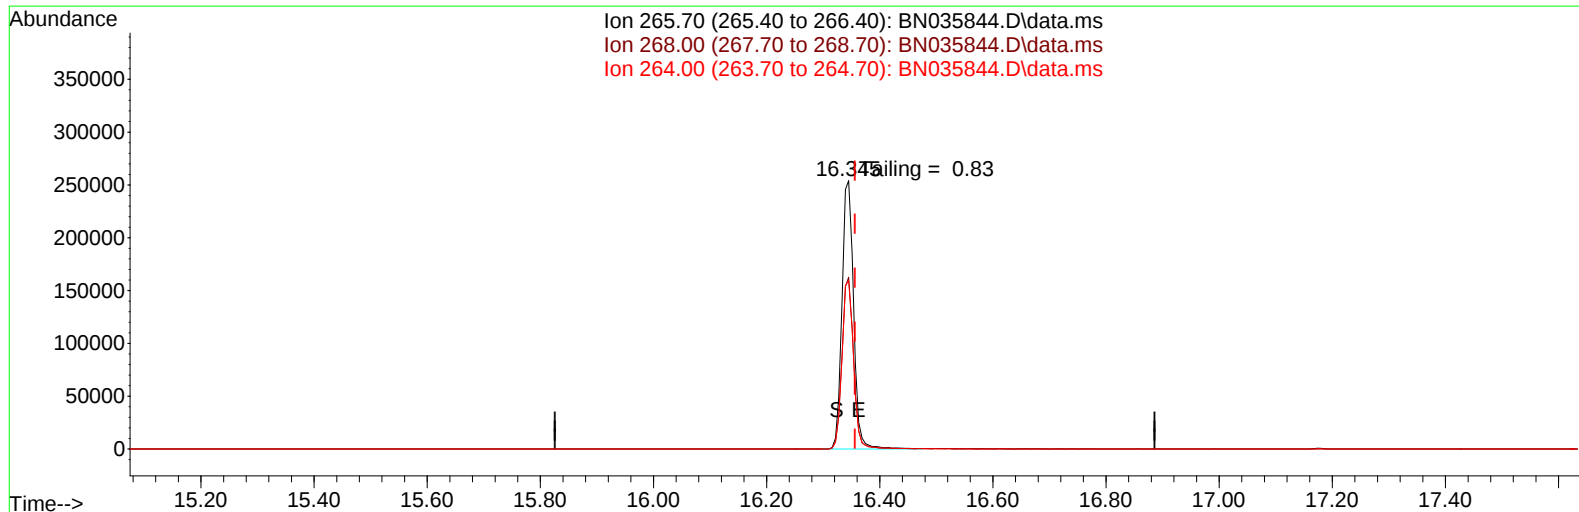

TIC: BN035844.D\data.ms

(70) Pentachlorophenol (C)

16.345min (-0.011) 24950.02 ng




response 363016

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.03
264.00	61.60	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122624\
Data File : BN035844.D
Acq On : 26 Dec 2024 09:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 26 18:24:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

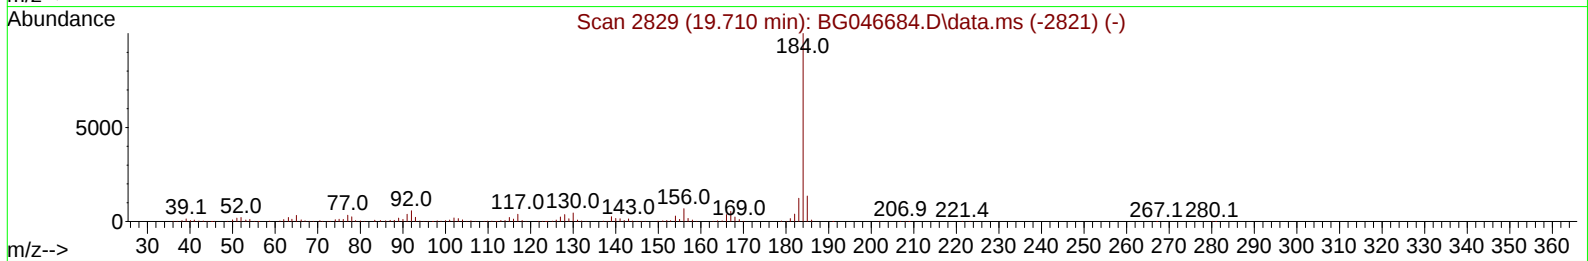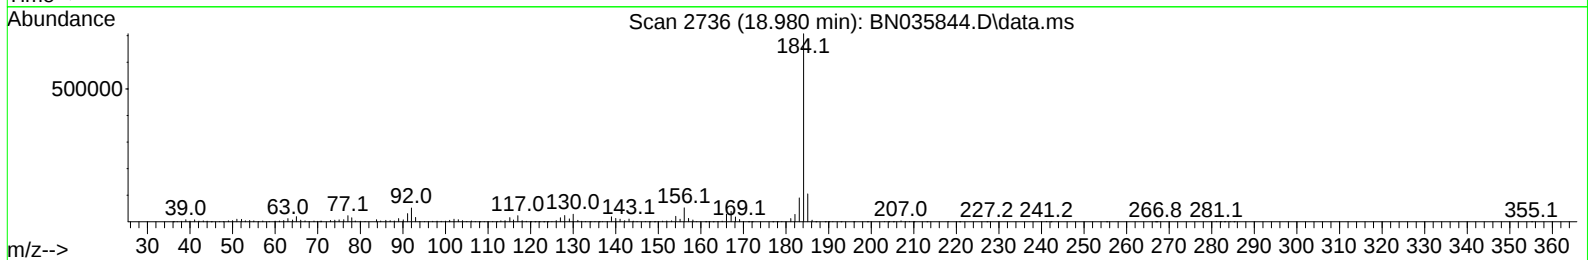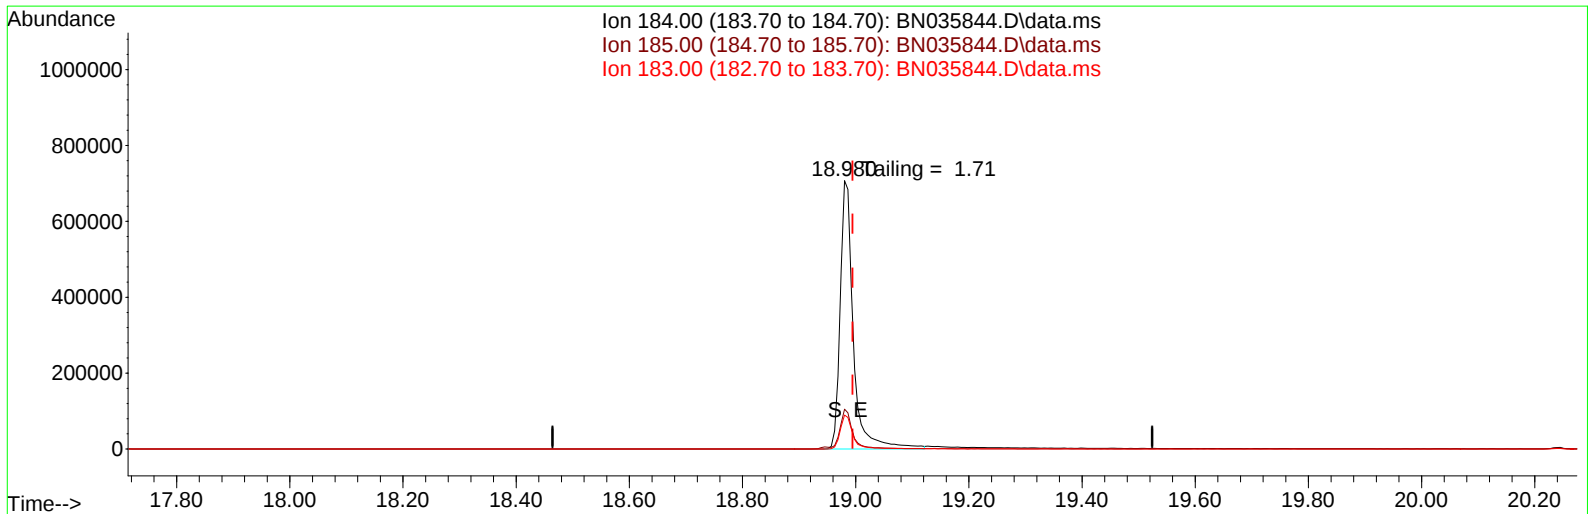

TIC: BN035844.D\data.ms

(77) Benzidine

18.980min (-0.014) 0.00 ng

response 1183784

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.84
183.00	13.20	12.69
0.00	0.00	0.00