

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
 Data File : BN035350.D
 Acq On : 27 Nov 2024 15:34
 Operator : RC/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Quant Time: Nov 27 22:52:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 27 22:48:24 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.308	152	2237	0.400	ng	0.00
7) Naphthalene-d8	10.052	136	5753	0.400	ng	0.00
13) Acenaphthene-d10	13.967	164	4077	0.400	ng	0.00
19) Phenanthrene-d10	16.736	188	10855	0.400	ng	0.00
29) Chrysene-d12	20.974	240	11269	0.400	ng	0.00
35) Perylene-d12	23.067	264	13004	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	4.968	112	573	0.101	ng	0.00
5) Phenol-d6	6.513	99	686	0.096	ng	0.00
8) Nitrobenzene-d5	8.450	82	492	0.098	ng	0.01
11) 2-Methylnaphthalene-d10	11.661	152	850	0.083	ng	0.00
14) 2,4,6-Tribromophenol	15.475	330	278	0.095	ng	0.00
15) 2-Fluorobiphenyl	12.574	172	1518	0.092	ng	0.00
27) Fluoranthene-d10	18.785	212	3265	0.098	ng	0.00
31) Terphenyl-d14	19.412	244	2344	0.099	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.003	88	227	0.112	ng	# 87
3) n-Nitrosodimethylamine	3.299	42	187	0.099	ng	# 90
6) bis(2-Chloroethyl)ether	6.759	93	579	0.108	ng	98
9) Naphthalene	10.105	128	1527	0.102	ng	# 91
10) Hexachlorobutadiene	10.404	225	352	0.080	ng	# 97
12) 2-Methylnaphthalene	11.737	142	1042	0.094	ng	96
16) Acenaphthylene	13.679	152	1675	0.096	ng	100
17) Acenaphthene	14.031	154	1143	0.100	ng	99
18) Fluorene	15.026	166	1620	0.096	ng	98
20) 4,6-Dinitro-2-methylph...	15.133	198	103	0.046	ng	# 29
21) 4-Bromophenyl-phenylether	15.941	248	612	0.088	ng	# 94
22) Hexachlorobenzene	16.041	284	720	0.100	ng	97
23) Atrazine	16.227	200	421	0.068	ng	# 86
24) Pentachlorophenol	16.401	266	381	0.114	ng	90
25) Phenanthrene	16.773	178	2963	0.104	ng	99
26) Anthracene	16.860	178	2617	0.100	ng	98
28) Fluoranthene	18.817	202	4173	0.106	ng	99
30) Pyrene	19.184	202	4461	0.119	ng	100
32) Benzo(a)anthracene	20.956	228	4031	0.103	ng	99
33) Chrysene	21.010	228	4123	0.106	ng	97
34) Bis(2-ethylhexyl)phtha...	20.929	149	1999	0.097	ng	99
36) Indeno(1,2,3-cd)pyrene	25.105	276	4586	0.088	ng	97
37) Benzo(b)fluoranthene	22.456	252	4243	0.097	ng	# 82
38) Benzo(k)fluoranthene	22.494	252	4378	0.100	ng	# 80
39) Benzo(a)pyrene	22.977	252	3913	0.102	ng	# 69
40) Dibenzo(a,h)anthracene	25.126	278	3588	0.087	ng	# 86
41) Benzo(g,h,i)perylene	25.725	276	3863	0.088	ng	# 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
Data File : BN035350.D
Acq On : 27 Nov 2024 15:34
Operator : RC/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Quant Time: Nov 27 22:52:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 27 22:48:24 2024
Response via : Initial Calibration








#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.308 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN035350.D
 Acq: 27 Nov 2024 15:34

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1







Tgt Ion:152 Resp: 2237
 Ion Ratio Lower Upper
 152 100
 150 153.6 124.0 186.0
 115 62.8 49.6 74.4



#2
 1,4-Dioxane
 Concen: 0.112 ng
 RT: 3.003 min Scan# 17
 Delta R.T. 0.000 min
 Lab File: BN035350.D
 Acq: 27 Nov 2024 15:34

Tgt Ion: 88 Resp: 227
 Ion Ratio Lower Upper
 88 100
 43 41.4 17.2 25.8#
 58 54.6 44.5 66.7









#3
n-Nitrosodimethylamine
Concen: 0.099 ng
RT: 3.299 min Scan# 51
Delta R.T. 0.007 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion: 42 Resp: 187
Ion Ratio Lower Upper
42 100
74 146.5 124.9 187.3
44 51.9 2.2 3.4#



#4
2-Fluorophenol
Concen: 0.101 ng
RT: 4.968 min Scan# 289
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34

Tgt Ion: 112 Resp: 573
Ion Ratio Lower Upper
112 100
64 52.0 39.8 59.8
63 28.8 21.0 31.6









#5
Phenol-d6
Concen: 0.096 ng
RT: 6.513 min Scan# 503
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion: 99 Resp: 686
Ion Ratio Lower Upper
99 100
42 13.7 11.4 17.2
71 38.9 29.3 43.9



#6
bis(2-Chloroethyl)ether
Concen: 0.108 ng
RT: 6.759 min Scan# 537
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34

Tgt Ion: 93 Resp: 579
Ion Ratio Lower Upper
93 100
63 61.7 50.4 75.6
95 31.3 25.7 38.5





#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.052 min Scan# 915

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1

Tgt Ion:136 Resp: 5753





Ion Ratio Lower Upper

136 100

137 12.6 10.2 15.2

54 7.7 6.1 9.1

68 7.8 6.4 9.6



#8

Nitrobenzene-d5

Concen: 0.098 ng

RT: 8.450 min Scan# 765

Delta R.T. 0.011 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34




Tgt Ion: 82 Resp: 492


Ion Ratio Lower Upper

82 100

128 64.5 33.4 50.0#

54 52.5 36.7 55.1





#9

Naphthalene

Concen: 0.102 ng

RT: 10.105 min Scan# 91

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:128 Resp: 1527

Ion Ratio Lower Upper

128 100

129 16.2 9.8 14.6#

127 17.2 11.4 17.2#



#10

Hexachlorobutadiene

Concen: 0.080 ng

RT: 10.404 min Scan# 948

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34




Tgt Ion:225 Resp: 352


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 66.2 51.3 76.9









#11
2-Methylnaphthalene-d10
Concen: 0.083 ng
RT: 11.661 min Scan# 1082
Delta R.T. 0.005 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:152 Resp: 850
Ion Ratio Lower Upper
152 100
151 21.1 16.6 25.0



#12
2-Methylnaphthalene
Concen: 0.094 ng
RT: 11.737 min Scan# 1097
Delta R.T. 0.005 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34

Tgt Ion:142 Resp: 1042
Ion Ratio Lower Upper
142 100
141 91.0 72.2 108.4
115 46.5 31.4 47.0





#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 13.967 min Scan# 14

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:164 Resp: 4077

Ion Ratio Lower Upper

164 100

162 103.9 82.2 123.2

160 50.4 40.1 60.1



#14

2,4,6-Tribromophenol

Concen: 0.095 ng

RT: 15.475 min Scan# 1578

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34




Tgt Ion:330 Resp: 278


Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0

141 29.1 26.6 40.0





#15

2-Fluorobiphenyl

Concen: 0.092 ng

RT: 12.574 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:172 Resp: 1518

Ion Ratio Lower Upper

172 100

171 39.7 29.0 43.4

170 27.7 19.8 29.8



#16

Acenaphthylene

Concen: 0.096 ng

RT: 13.679 min Scan# 1410

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34




Tgt Ion:152 Resp: 1675


Ion Ratio Lower Upper

152 100

151 20.4 16.2 24.2

153 13.1 10.4 15.6









#17
Acenaphthene
Concen: 0.100 ng
RT: 14.031 min Scan# 1443
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:154 Resp: 1143
Ion Ratio Lower Upper
154 100
153 115.0 92.6 139.0
152 60.9 49.0 73.6



#18
Fluorene
Concen: 0.096 ng
RT: 15.026 min Scan# 1536
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34

Tgt Ion:166 Resp: 1620
Ion Ratio Lower Upper
166 100
165 97.7 79.7 119.5
167 13.1 10.8 16.2





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.736 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:188 Resp: 10855

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 6.4 4.6 6.8



#20

4,6-Dinitro-2-methylphenol

Concen: 0.046 ng

RT: 15.133 min Scan# 1546

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34




Tgt Ion:198 Resp: 103


Ion Ratio Lower Upper

198 100

51 119.8 46.5 69.7#

105 100.0 45.3 67.9#









#21
4-Bromophenyl-phenylether
Concen: 0.088 ng
RT: 15.941 min Scan# 1616
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:248 Resp: 612
Ion Ratio Lower Upper
248 100
250 102.5 80.6 120.8
141 48.6 31.5 47.3#



#22
Hexachlorobenzene
Concen: 0.100 ng
RT: 16.041 min Scan# 1624
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34

Tgt Ion:284 Resp: 720
Ion Ratio Lower Upper
284 100
142 35.4 26.7 40.1
249 32.2 24.6 36.8





#23

Atrazine

Concen: 0.068 ng

RT: 16.227 min Scan# 1639

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:200 Resp: 421

Ion Ratio Lower Upper

200 100

173 39.9 24.1 36.1#

215 54.2 36.9 55.3



#24

Pentachlorophenol

Concen: 0.114 ng

RT: 16.401 min Scan# 1653

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34




Tgt Ion:266 Resp: 381


Ion Ratio Lower Upper

266 100

264 58.3 42.3 63.5

268 63.3 43.3 64.9





#25

Phenanthrene

Concen: 0.104 ng

RT: 16.773 min Scan# 1683

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:178 Resp: 2963

Ion Ratio Lower Upper

178 100

176 18.8 15.4 23.2

179 15.6 12.3 18.5



#26

Anthracene

Concen: 0.100 ng

RT: 16.860 min Scan# 1690

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34




Tgt Ion:178 Resp: 2617


Ion Ratio Lower Upper

178 100

176 18.8 15.0 22.6

179 14.3 12.6 18.8









#27
Fluoranthene-d10
Concen: 0.098 ng
RT: 18.785 min Scan# 1882
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:212 Resp: 3265
Ion Ratio Lower Upper
212 100
106 12.8 9.2 13.8
104 7.6 5.3 7.9



#28
Fluoranthene
Concen: 0.106 ng
RT: 18.817 min Scan# 1889
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34

Tgt Ion:202 Resp: 4173
Ion Ratio Lower Upper
202 100
101 10.2 7.4 11.0
203 17.3 13.7 20.5









#29
Chrysene-d12
Concen: 0.400 ng
RT: 20.974 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:240 Resp: 11269
Ion Ratio Lower Upper
240 100
120 10.1 7.9 11.9
236 28.8 22.9 34.3



#30
Pyrene
Concen: 0.119 ng
RT: 19.184 min Scan# 1968
Delta R.T. 0.005 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34

Tgt Ion:202 Resp: 4461
Ion Ratio Lower Upper
202 100
200 21.1 17.0 25.4
203 18.0 14.3 21.5





#31

Terphenyl-d14

Concen: 0.099 ng

RT: 19.412 min Scan# 2017

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:244 Resp: 2344

Ion Ratio Lower Upper

244 100

212 11.4 8.1 12.1

122 16.3 10.3 15.5#



#32

Benzo(a)anthracene

Concen: 0.103 ng

RT: 20.956 min Scan# 2251

Delta R.T. 0.000 min

Lab File: BN035350.D

Acq: 27 Nov 2024 15:34




Tgt Ion:228 Resp: 4031


Ion Ratio Lower Upper

228 100

226 28.5 22.5 33.7

229 20.4 15.8 23.8









#33
Chrysene
Concen: 0.106 ng
RT: 21.010 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:228 Resp: 4123
Ion Ratio Lower Upper
228 100
226 32.3 24.6 37.0
229 21.5 15.9 23.9



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.097 ng
RT: 20.929 min Scan# 2248
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34

Tgt Ion:149 Resp: 1999
Ion Ratio Lower Upper
149 100
167 27.5 22.2 33.4
279 3.6 2.7 4.1









#35
Perylene-d12
Concen: 0.400 ng
RT: 23.067 min Scan# 2
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:264 Resp: 13004




Ion	Ratio	Lower	Upper
264	100		
260	27.0	21.4	32.2
265	48.7	40.2	60.4




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.088 ng
RT: 25.105 min Scan# 3336
Delta R.T. -0.003 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34

Tgt Ion:276 Resp: 4586

Ion	Ratio	Lower	Upper
276	100		
138	26.2	19.4	29.0
277	25.6	19.8	29.6









#37
Benzo(b)fluoranthene
Concen: 0.097 ng
RT: 22.456 min Scan# 2430
Delta R.T. 0.003 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:252 Resp: 4243
Ion Ratio Lower Upper
252 100
253 32.1 19.6 29.4#
125 21.0 9.6 14.4#



#38
Benzo(k)fluoranthene
Concen: 0.100 ng
RT: 22.494 min Scan# 2443
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34


Tgt Ion:252 Resp: 4378
Ion Ratio Lower Upper
252 100
253 32.2 19.5 29.3#
125 23.7 10.2 15.4#








#39
Benzo(a)pyrene
Concen: 0.102 ng
RT: 22.977 min Scan# 2608
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1







Tgt Ion:252 Resp: 3913
Ion Ratio Lower Upper
252 100
253 36.1 20.2 30.4#
125 33.1 10.9 16.3#



#40
Dibenzo(a,h)anthracene
Concen: 0.087 ng
RT: 25.126 min Scan# 3343
Delta R.T. 0.000 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34


Tgt Ion:278 Resp: 3588
Ion Ratio Lower Upper
278 100
139 23.6 14.2 21.4#
279 32.6 20.5 30.7#



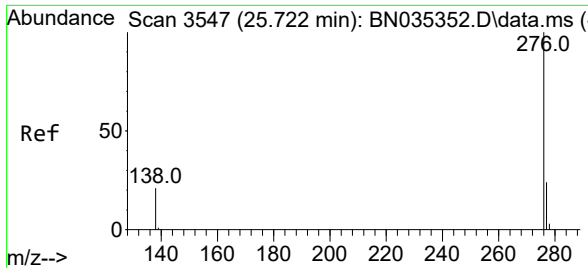

#41
Benzo(g,h,i)perylene
Concen: 0.088 ng
RT: 25.725 min Scan# 31
Delta R.T. 0.003 min
Lab File: BN035350.D
Acq: 27 Nov 2024 15:34

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1



Tgt Ion:276 Resp: 3863
Ion Ratio Lower Upper
276 100
277 26.9 19.9 29.9
138 26.8 17.8 26.8#

