
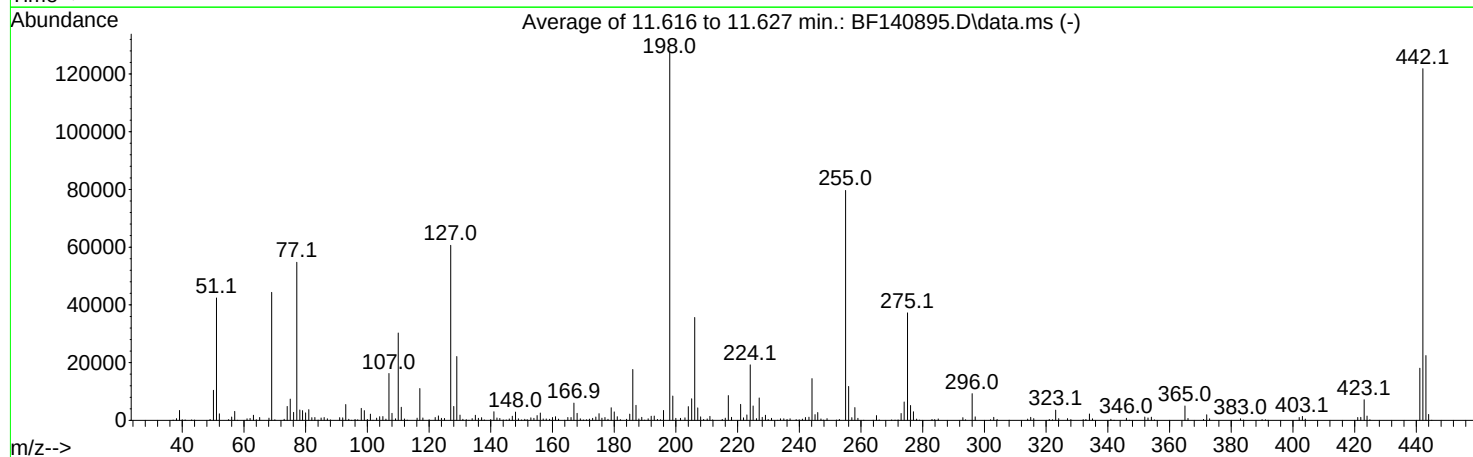


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121824\
Data File : BF140895.D
Acq On : 18 Dec 2024 09:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 16 16:59:50 2024

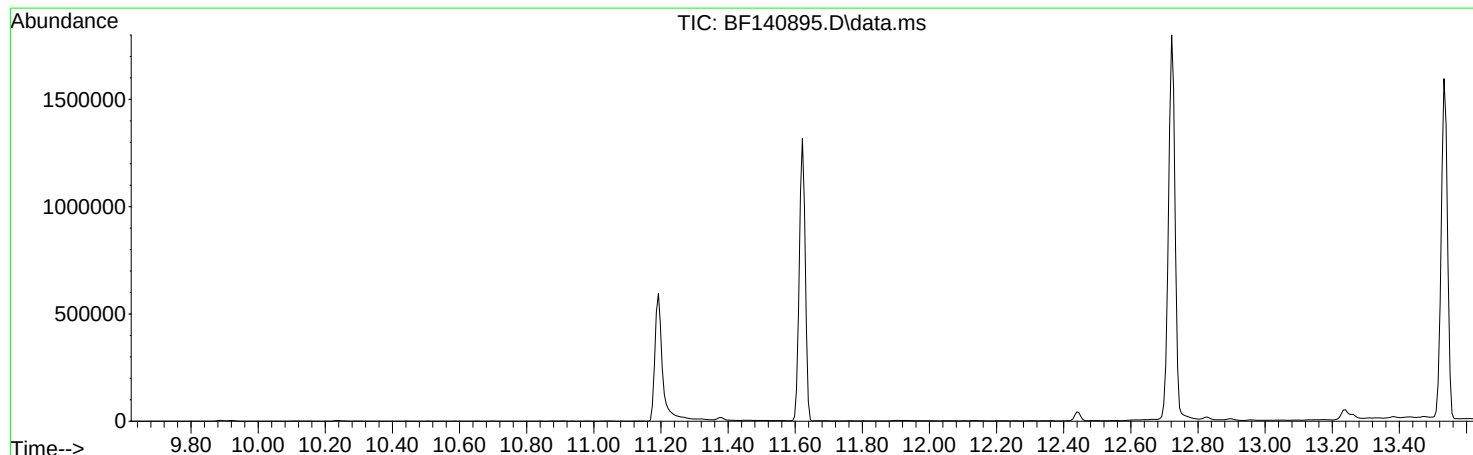

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	42411	PASS
68	69	0.00	2	1.7	771	PASS
69	198	0.00	100	34.8	44341	PASS
70	69	0.00	2	0.5	230	PASS
127	198	10	80	47.6	60667	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	127443	PASS
199	198	5	9	6.6	8447	PASS
275	198	10	60	29.2	37243	PASS
365	198	1	100	3.9	4975	PASS
441	198	0.01	100	14.2	18050	PASS
442	442	50	100	100.0	121843	PASS
443	442	15	24	18.4	22475	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/18/2024	BNA_F	<u>BF140895.D</u>
Compound Name	Response	Retention Time
DDT	415662	13.533
DDD	22730	13.239
DDE	2369	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25099	440761	5.69

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121824\
Data File : BF140895.D
Acq On : 18 Dec 2024 09:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 18 11:45:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

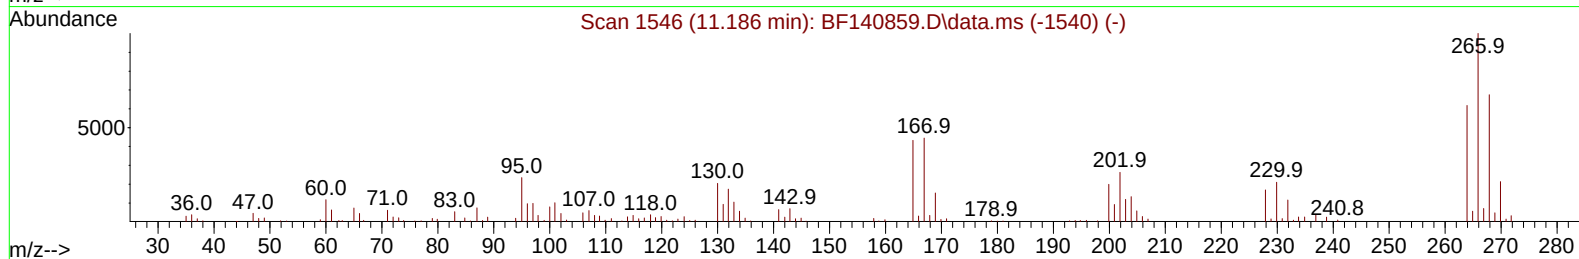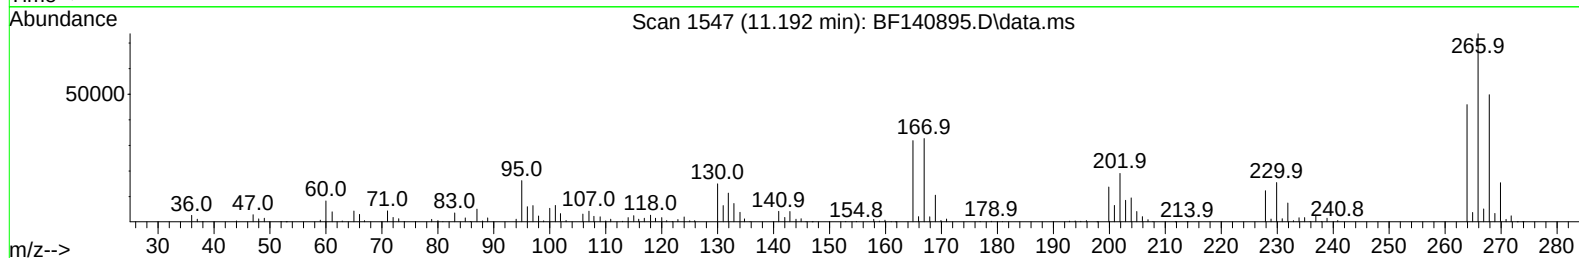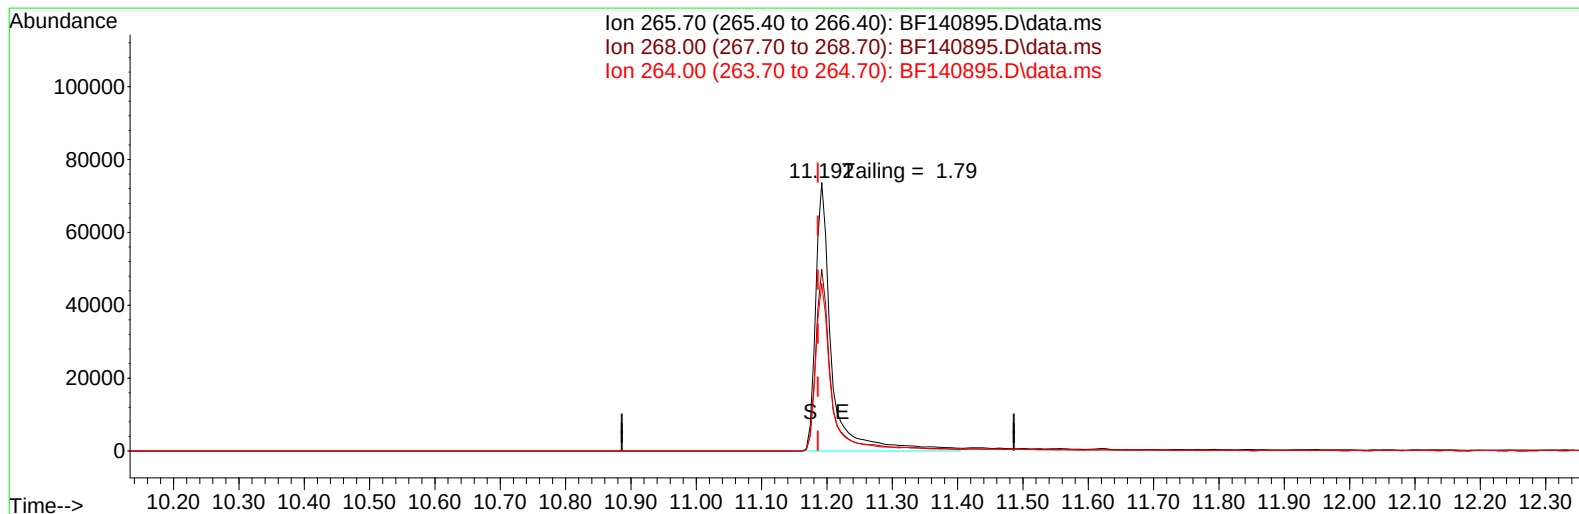

TIC: BF140895.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.006) 3663.45 ng m




response 126345

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	67.63
264.00	61.80	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121824\
Data File : BF140895.D
Acq On : 18 Dec 2024 09:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 18 11:45:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

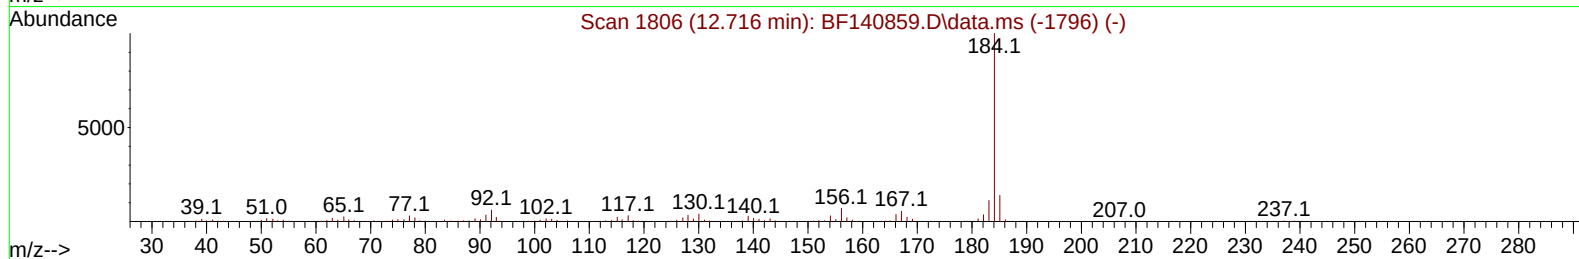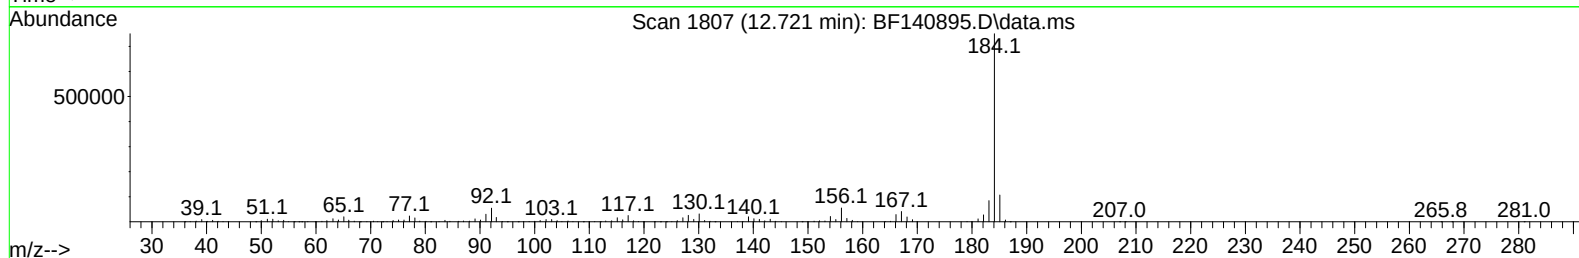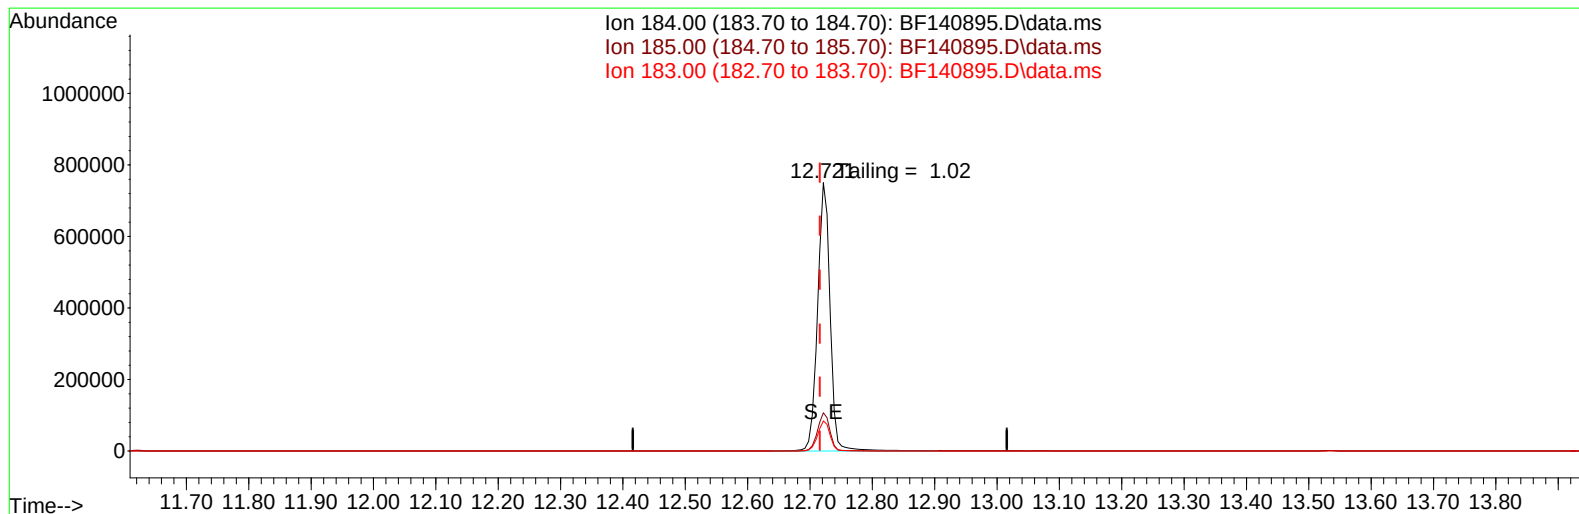

TIC: BF140895.D\data.ms

(77) Benzidine

12.721min (+ 0.005) 6539.55 ng

response 1054410

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.27
183.00	11.20	11.25
0.00	0.00	0.00