
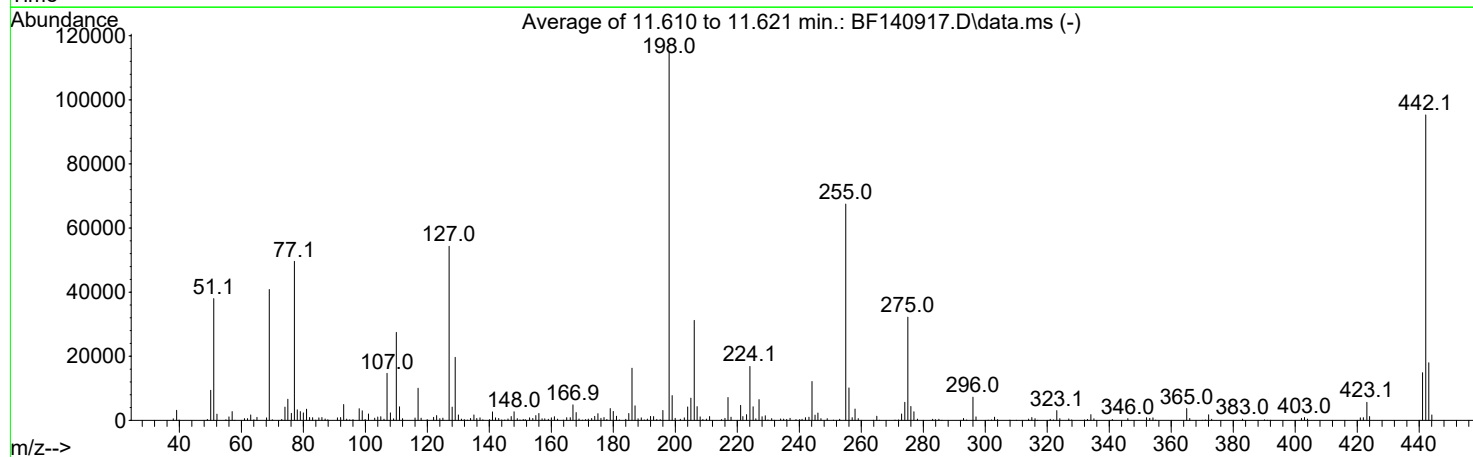


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121924\
Data File : BF140917.D
Acq On : 19 Dec 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 16 16:59:50 2024

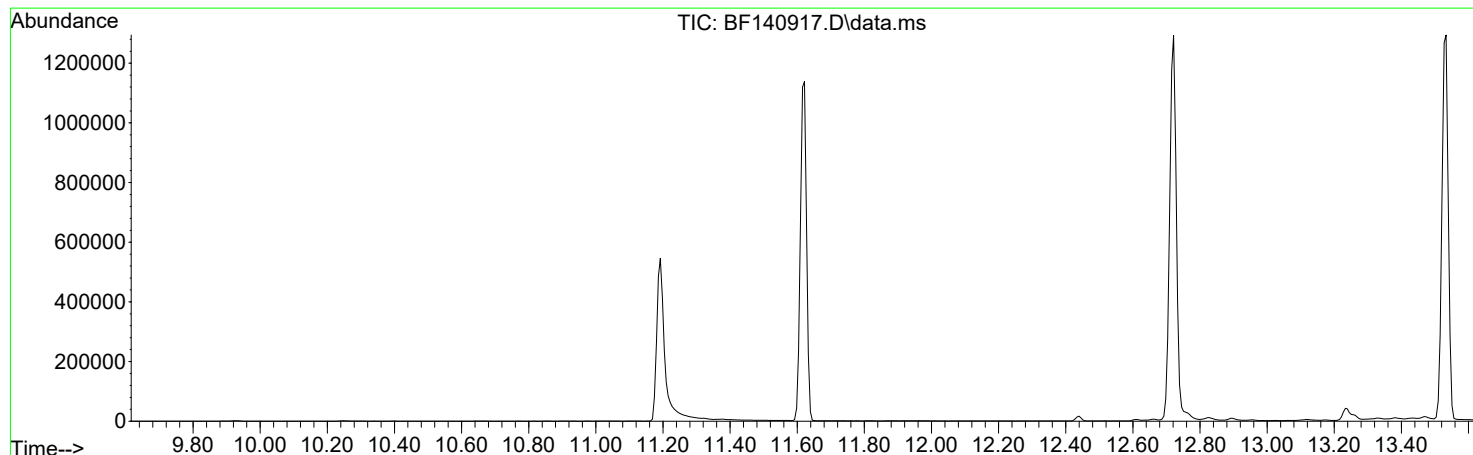

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	33.1	37984	PASS
68	69	0.00	2	2.0	803	PASS
69	198	0.00	100	35.6	40840	PASS
70	69	0.00	2	0.5	215	PASS
127	198	10	80	47.3	54309	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	114771	PASS
199	198	5	9	6.8	7753	PASS
275	198	10	60	28.1	32213	PASS
365	198	1	100	3.2	3709	PASS
441	198	0.01	100	13.0	14889	PASS
442	442	50	100	100.0	95291	PASS
443	442	15	24	18.9	17985	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/19/2024	BNA_F	<u>BF1408917.D</u>
Compound Name	Response	Retention Time
DDT	347372	13.533
DDD	20697	13.239
DDE	3231	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23928	371300	6.44

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121924\
Data File : BF140917.D
Acq On : 19 Dec 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 19 12:07:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

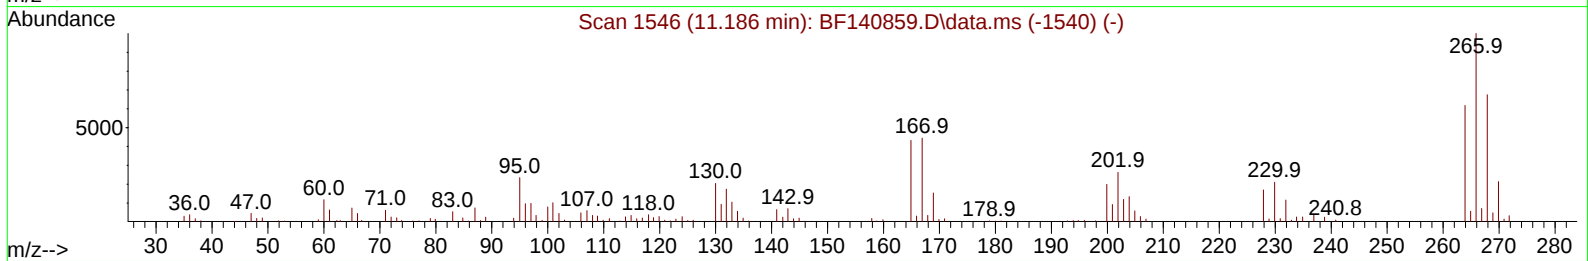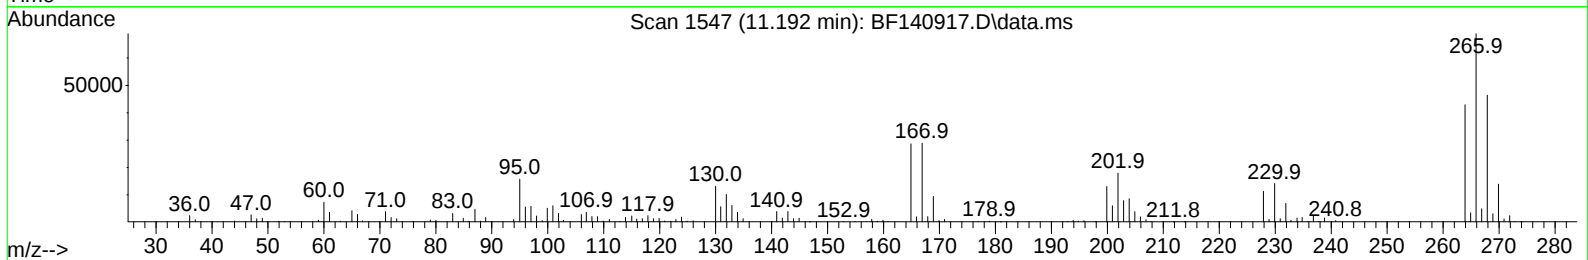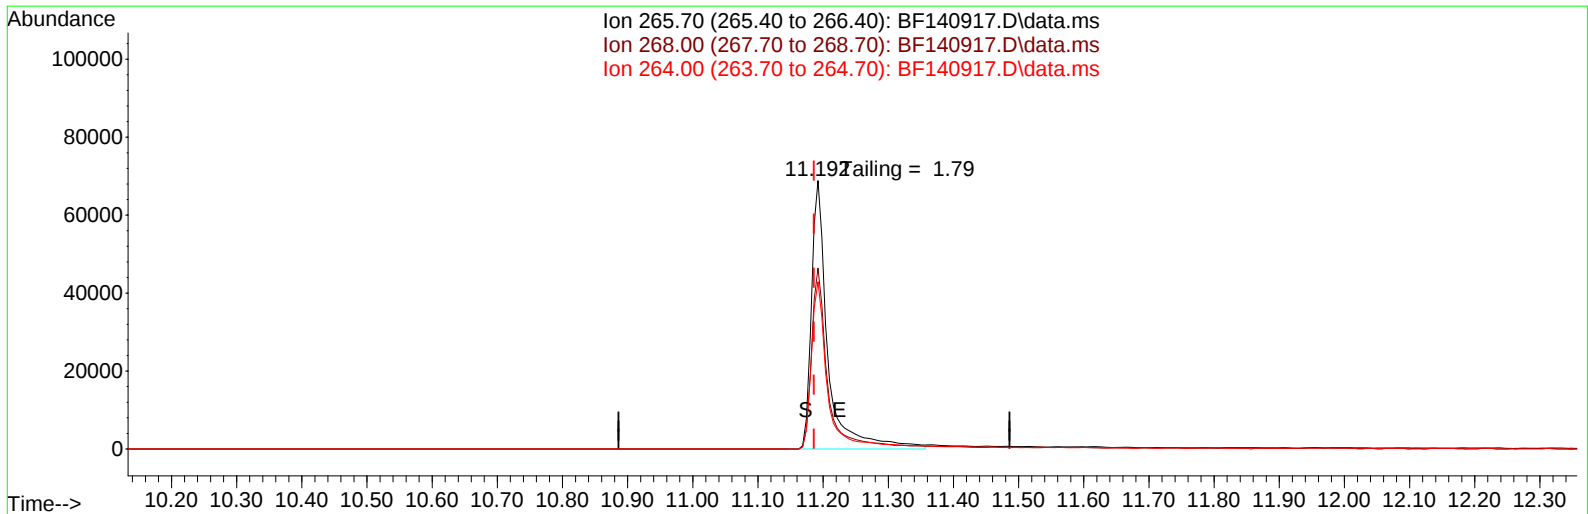

TIC: BF140917.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.006) 16315.61 ng




response 121966

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	67.35
264.00	61.80	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121924\
Data File : BF140917.D
Acq On : 19 Dec 2024 10:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 19 12:07:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

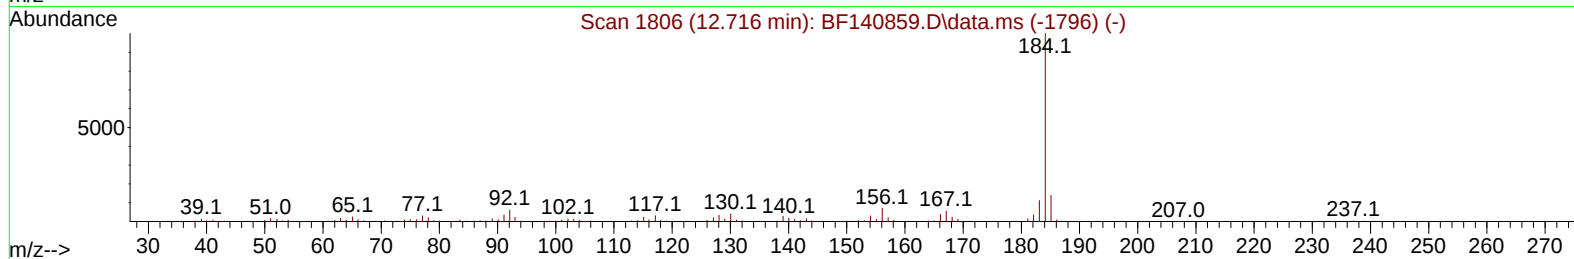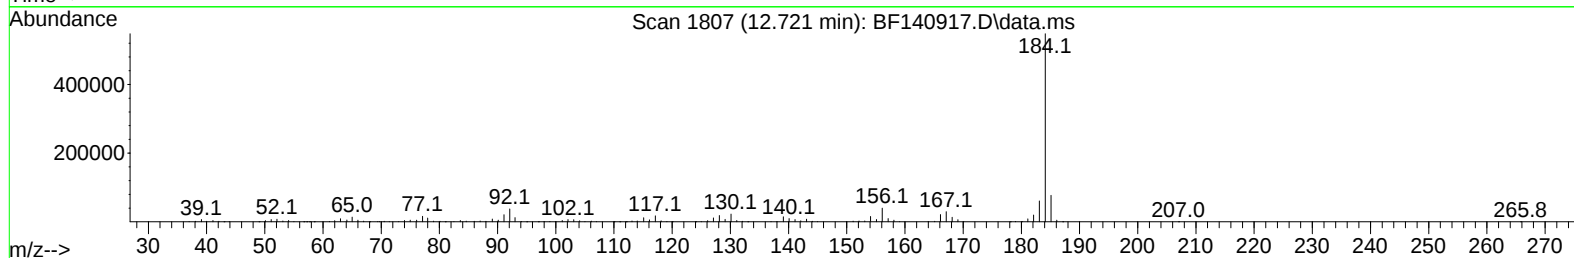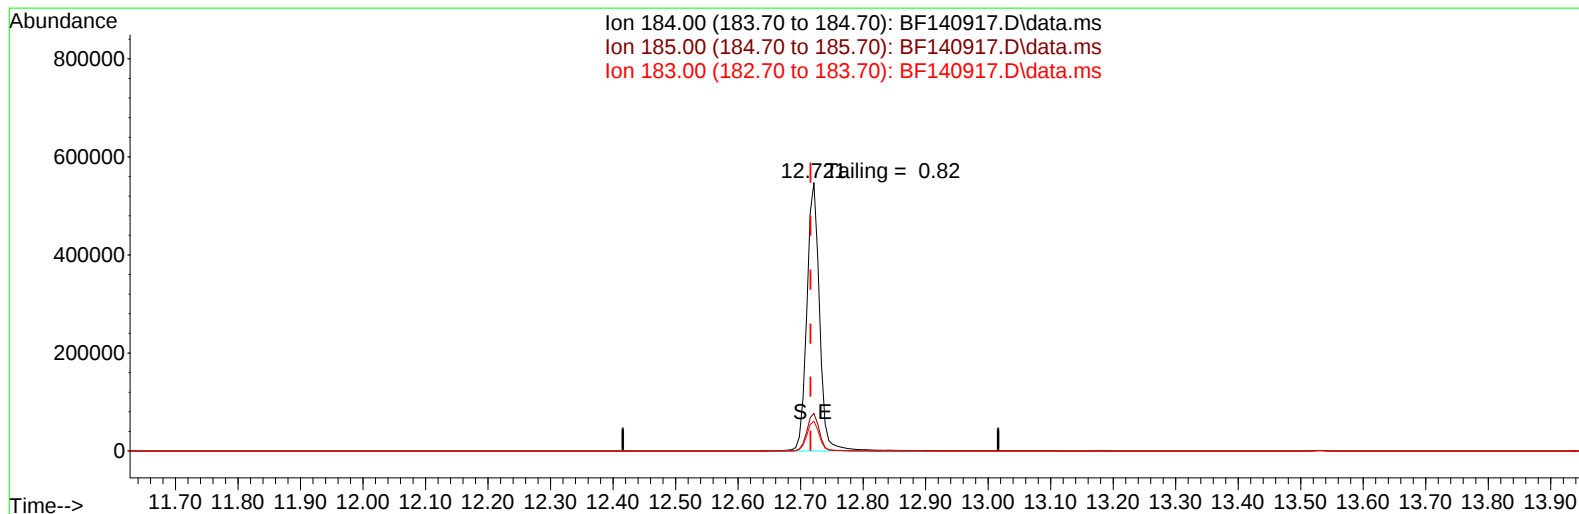

TIC: BF140917.D\data.ms

(77) Benzidine

12.721min (+ 0.005) 26320.69 ng

response 778933

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.04
183.00	11.20	11.10
0.00	0.00	0.00