
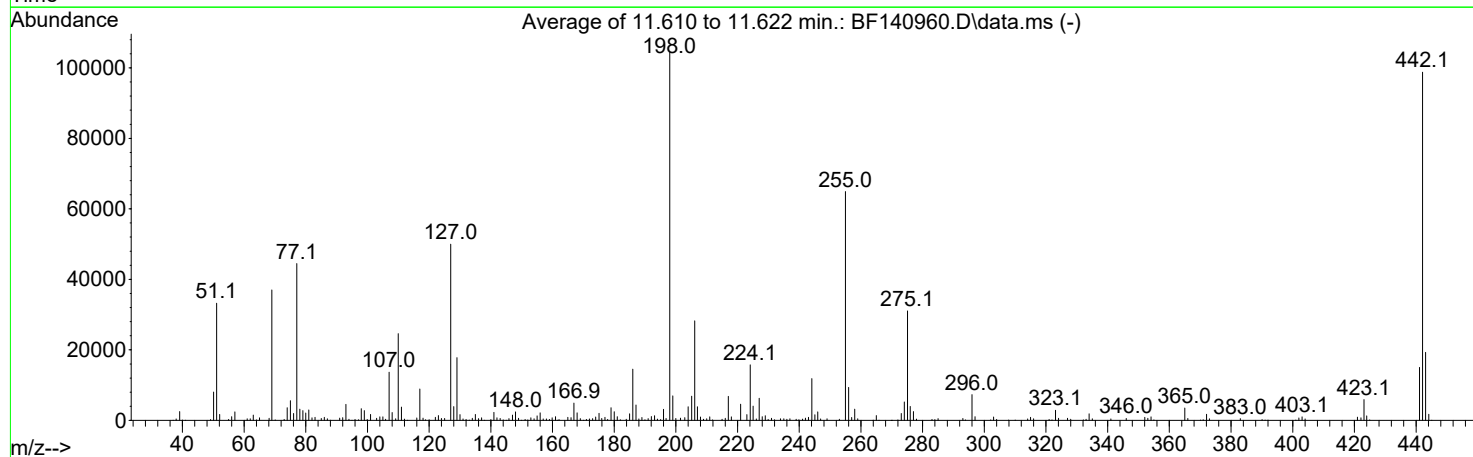


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122324\
Data File : BF140960.D
Acq On : 23 Dec 2024 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 16 16:59:50 2024

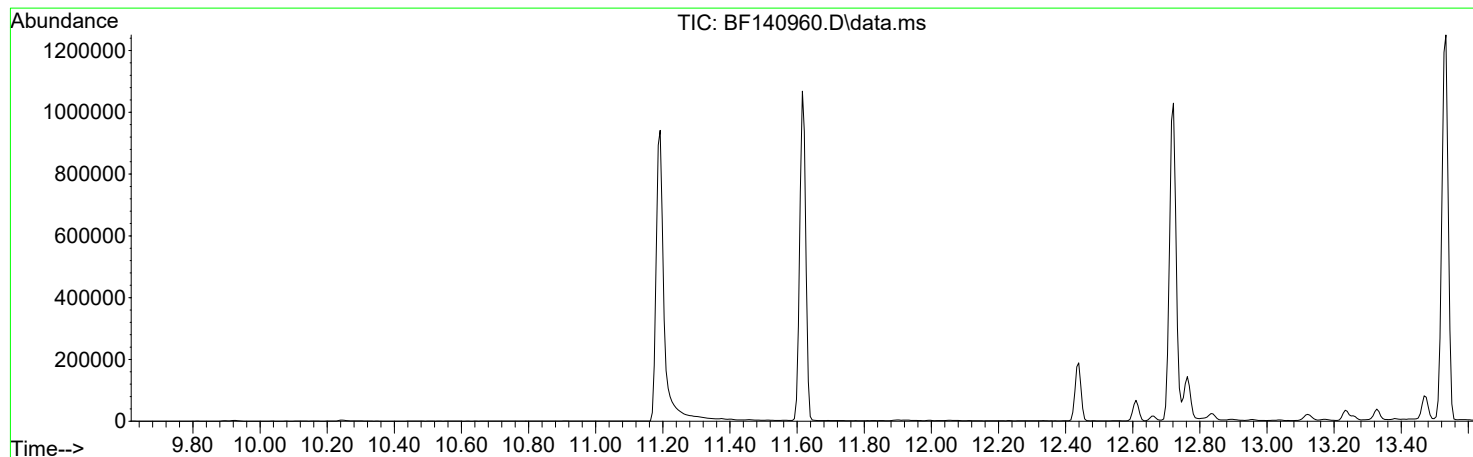

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	33216	PASS
68	69	0.00	2	1.6	610	PASS
69	198	0.00	100	35.4	36976	PASS
70	69	0.00	2	0.4	131	PASS
127	198	10	80	47.9	49984	PASS
197	198	0.00	2	0.5	552	PASS
198	198	100	100	100.0	104365	PASS
199	198	5	9	6.6	6939	PASS
275	198	10	60	29.8	31069	PASS
365	198	1	100	3.3	3490	PASS
441	198	0.01	100	14.4	15051	PASS
442	442	50	100	100.0	98797	PASS
443	442	15	24	19.5	19272	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/23/2024	BNA_F	<u>BF140960.D</u>
Compound Name	Response	Retention Time
DDT	336428	13.533
DDD	15941	13.233
DDE	2131	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18072	354500	5.10

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122324\
Data File : BF140960.D
Acq On : 23 Dec 2024 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 23 11:30:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 16:59:50 2024
Response via : Initial Calibration

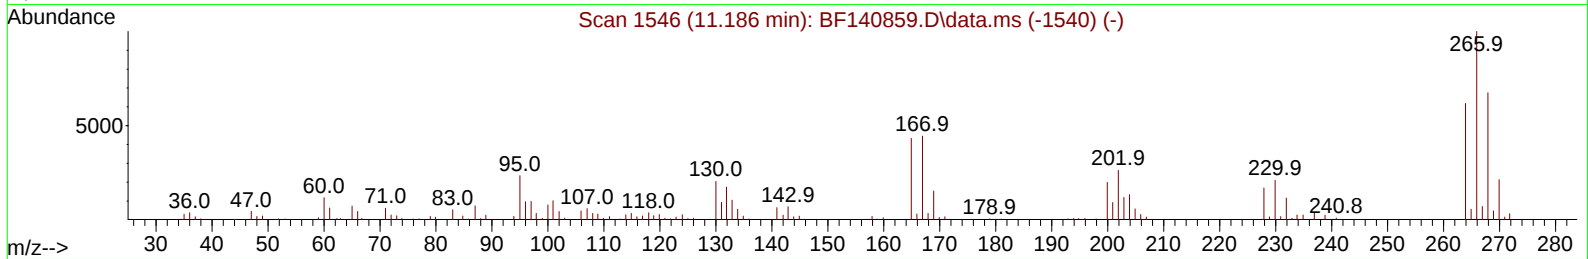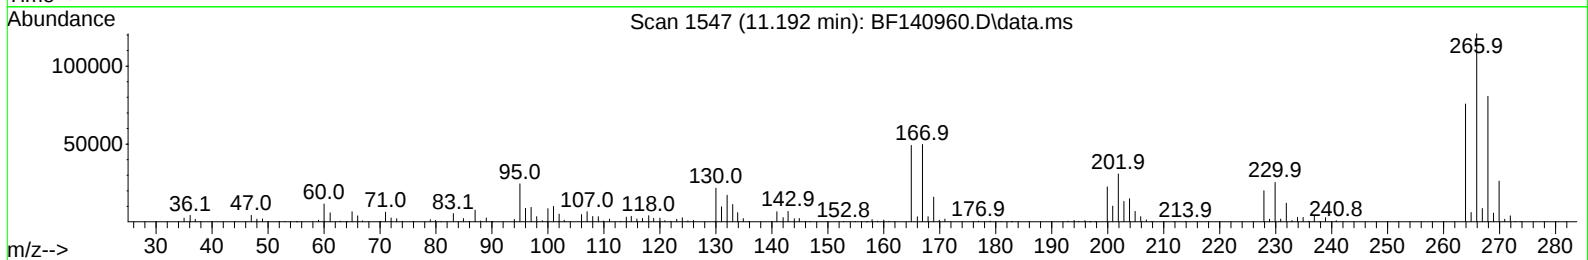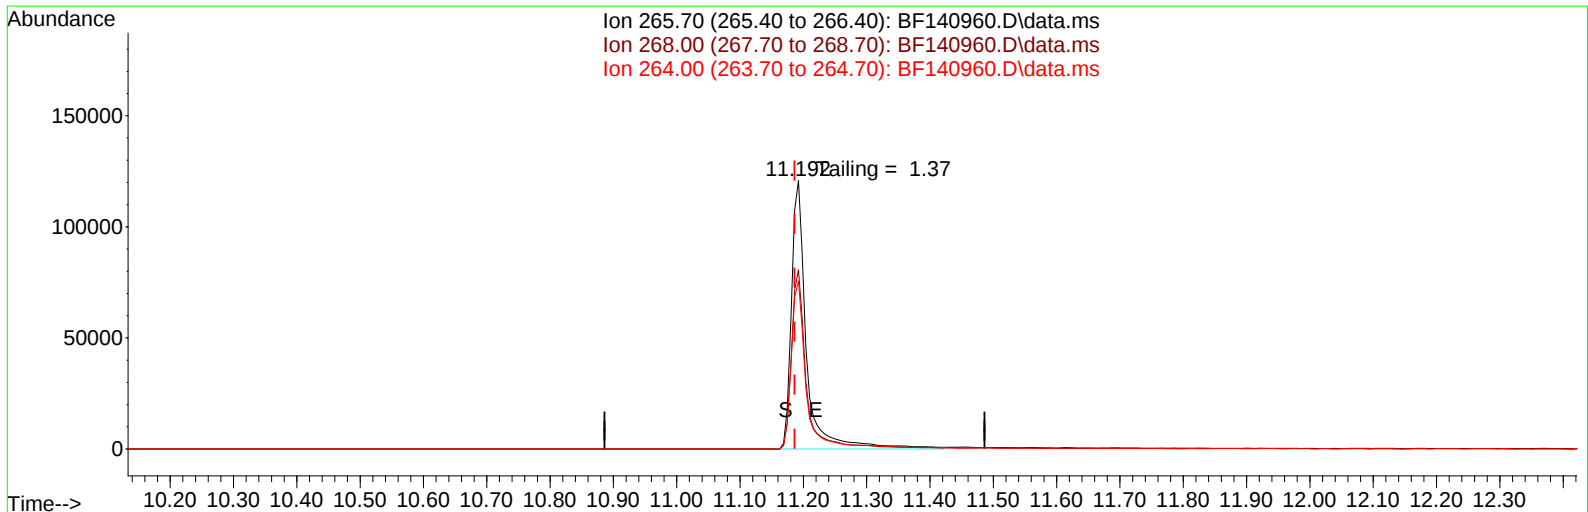

TIC: BF140960.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.006) 23080.12 ng




response 202074

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	66.80
264.00	61.80	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122324\
 Data File : BF140960.D
 Acq On : 23 Dec 2024 09:05
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 23 11:30:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 16 16:59:50 2024
 Response via : Initial Calibration

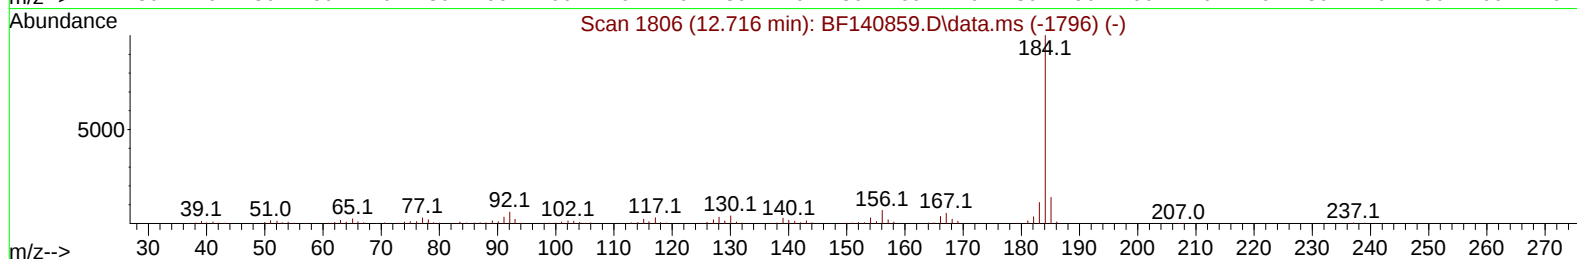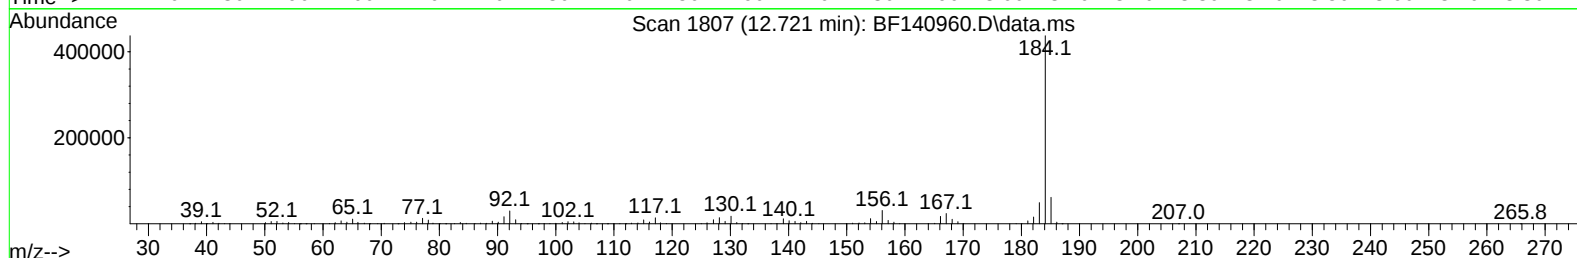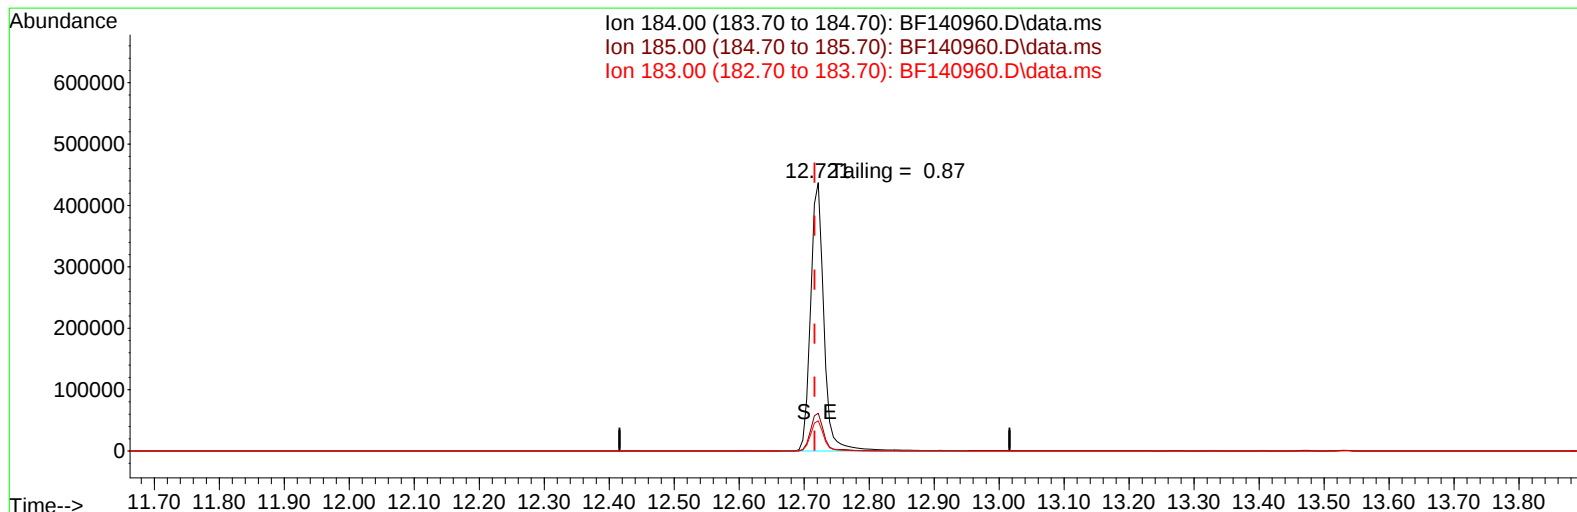

TIC: BF140960.D\data.ms

(77) Benzidine

12.721min (+ 0.005) 19990.23 ng

response 627493

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.08
183.00	11.20	11.28
0.00	0.00	0.00