


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121624\
Data File : BF140854.D
Acq On : 16 Dec 2024 11:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 16 16:59:50 2024

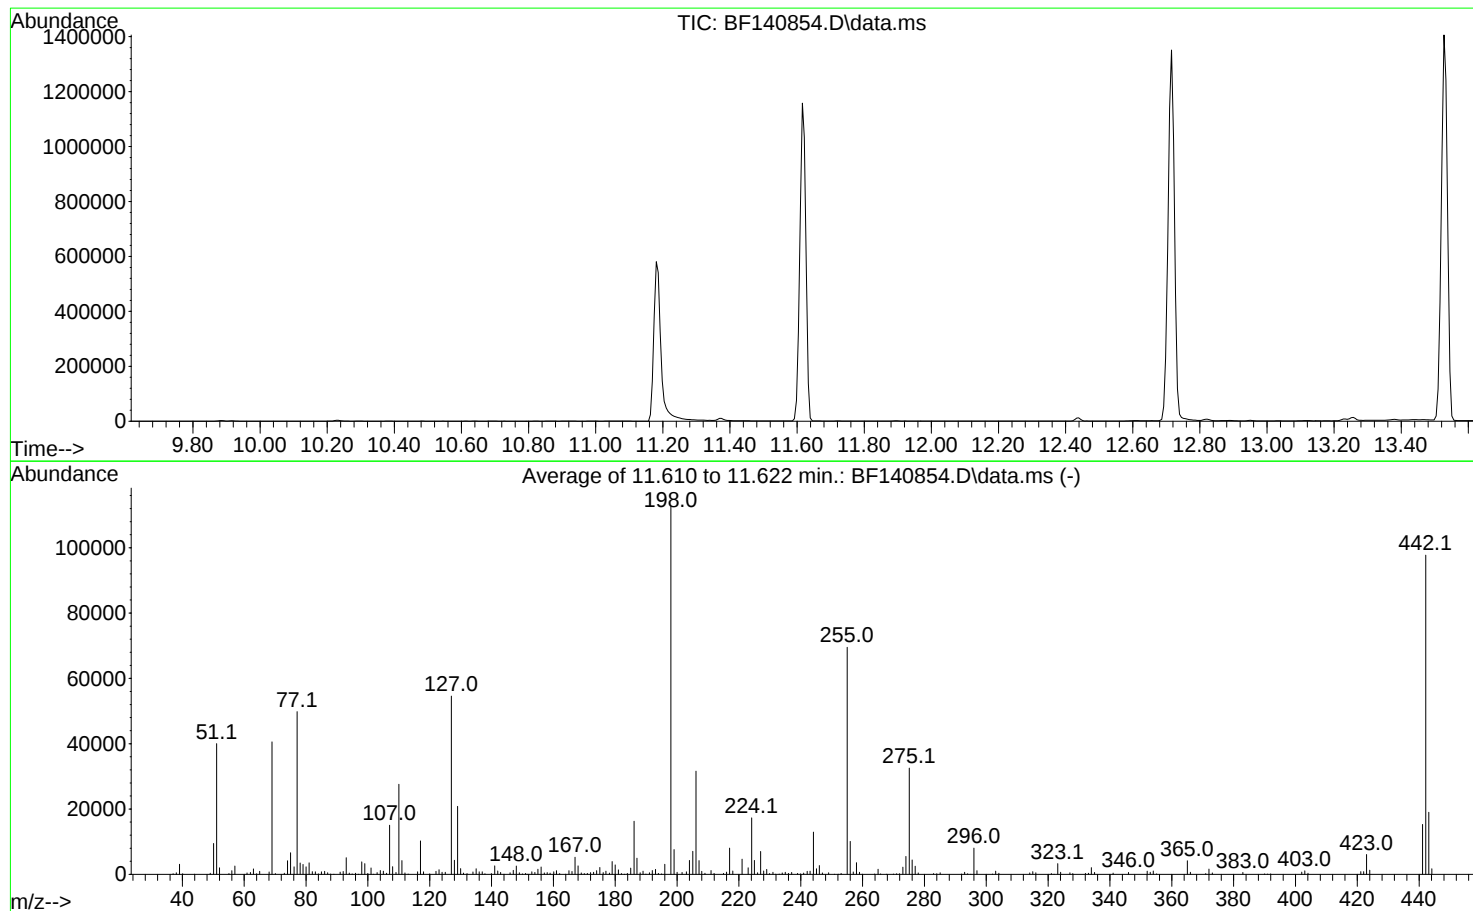

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	35.6	40051	PASS
68	69	0.00	2	1.9	751	PASS
69	198	0.00	100	36.0	40557	PASS
70	69	0.00	2	0.6	252	PASS
127	198	10	80	48.5	54581	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	112637	PASS
199	198	5	9	6.7	7601	PASS
275	198	10	60	28.9	32549	PASS
365	198	1	100	3.7	4169	PASS
441	198	0.01	100	13.6	15301	PASS
442	442	50	100	100.0	97731	PASS
443	442	15	24	19.4	18998	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/16/2024	BNA_F	<u>BF140854.D</u>
Compound Name	Response	Retention Time
DDT	360303	13.527
DDD	6357	13.257
DDE	1383	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7740	368043	2.10

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121624\
Data File : BF140854.D
Acq On : 16 Dec 2024 11:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 16 12:02:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

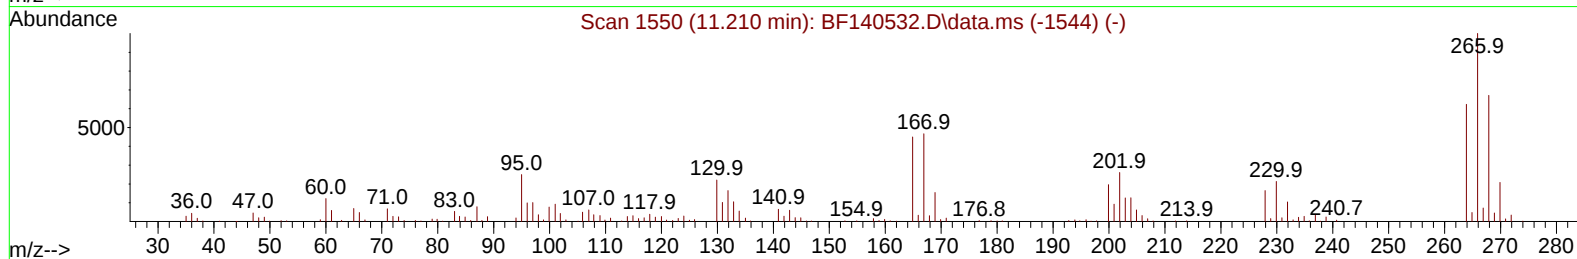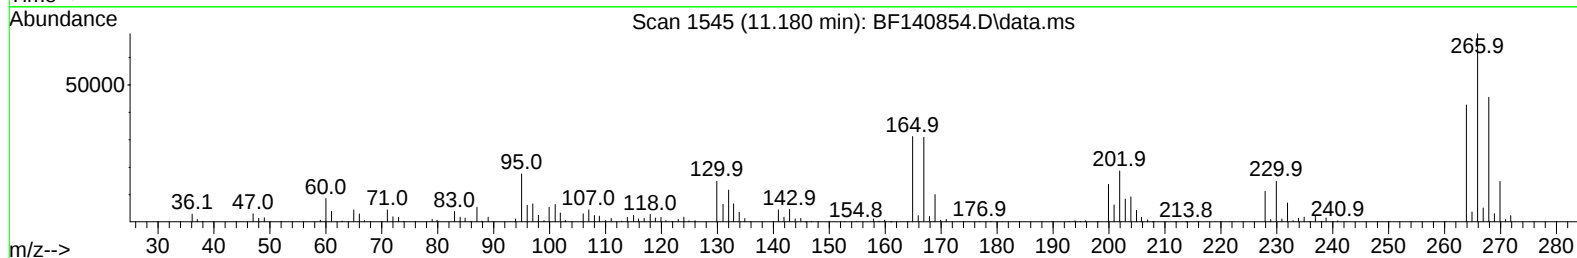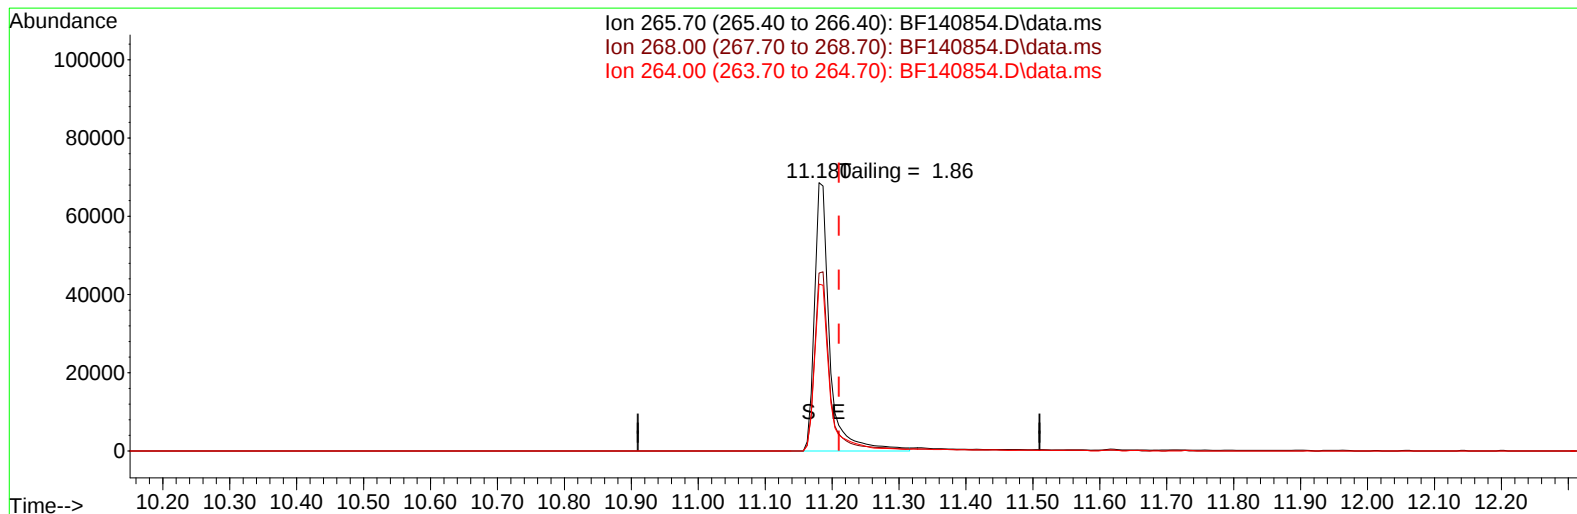

TIC: BF140854.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.030) 3894.75 ng m




response 108541

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	66.31
264.00	62.30	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121624\
Data File : BF140854.D
Acq On : 16 Dec 2024 11:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 16 12:02:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

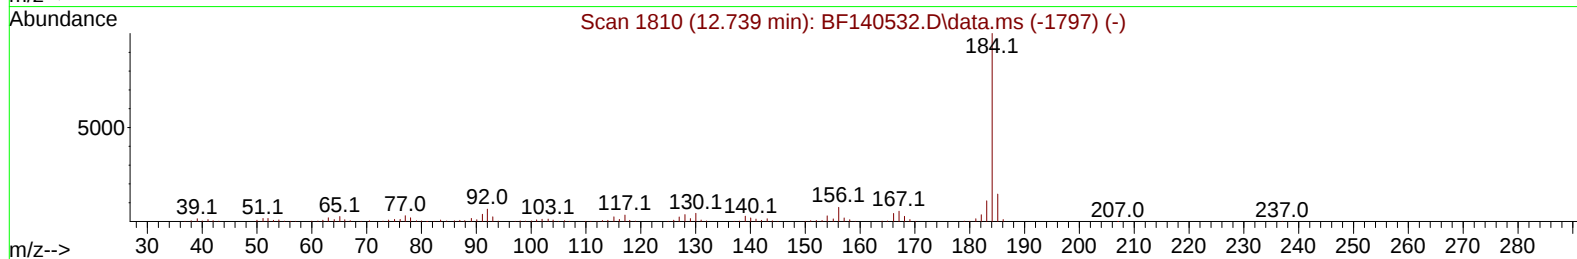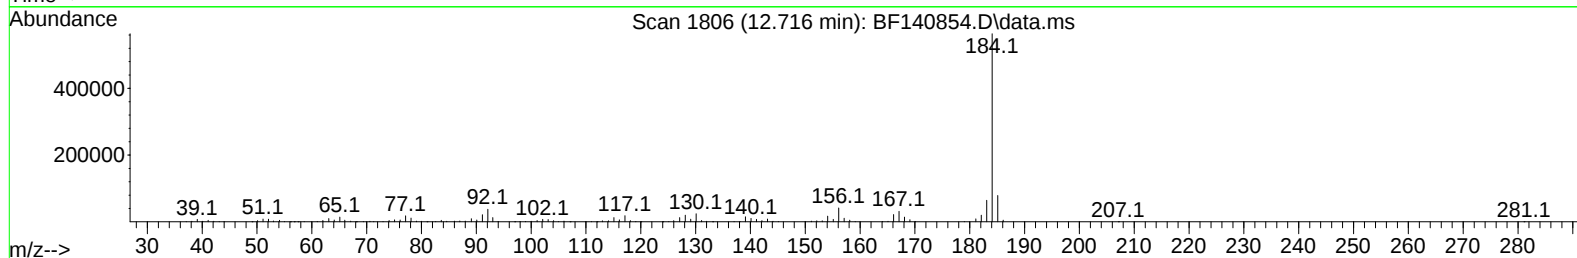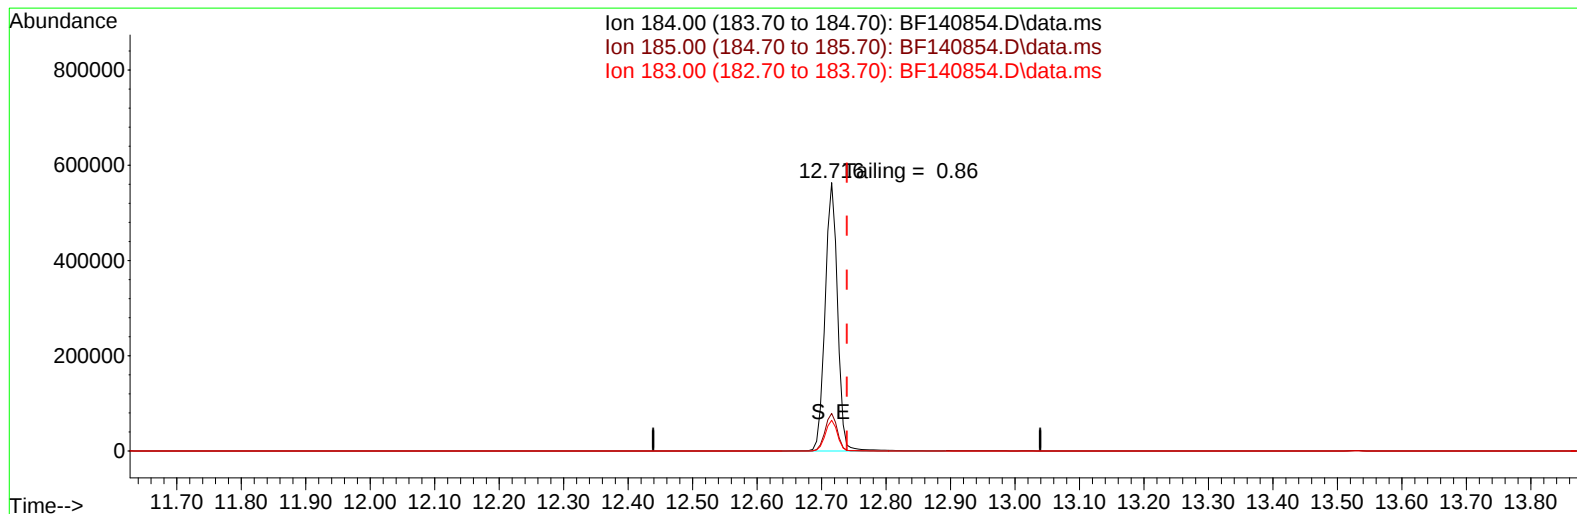

TIC: BF140854.D\data.ms

(77) Benzidine

12.716min (-0.023) 4792.75 ng

response 759160

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.01
183.00	11.00	11.44
0.00	0.00	0.00