
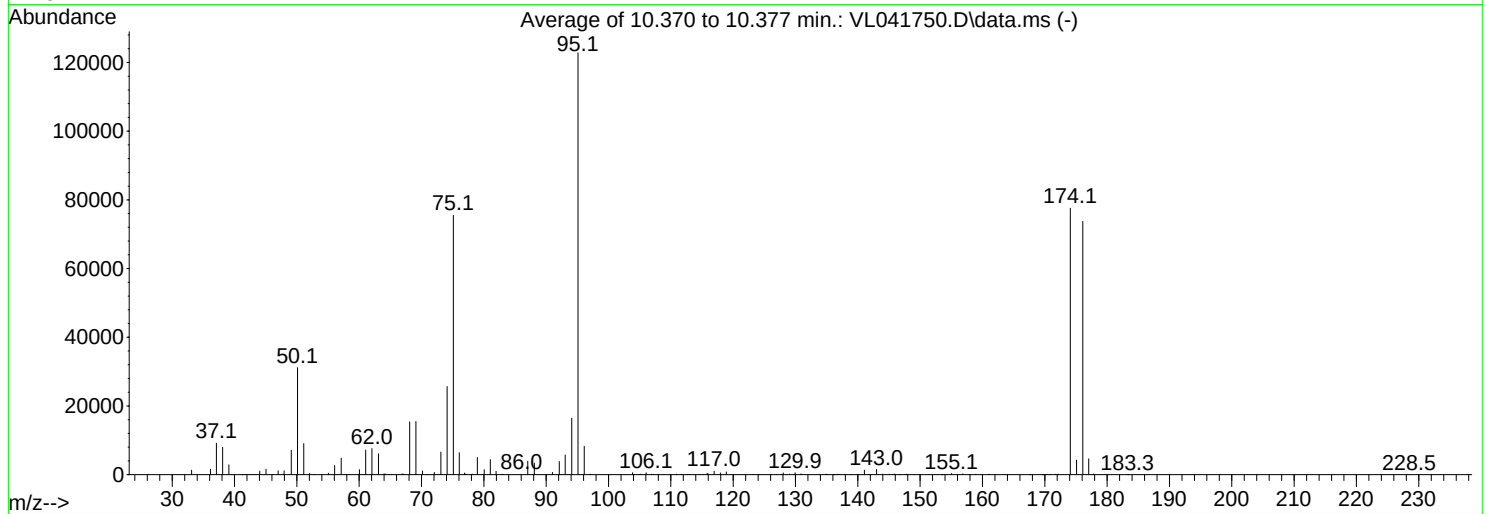


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121624\
Data File : VL041750.D
Acq On : 16 Dec 2024 12:02
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Title : AIR ANALYSIS BY METHOD T0-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Dec 19 07:32:09 2024

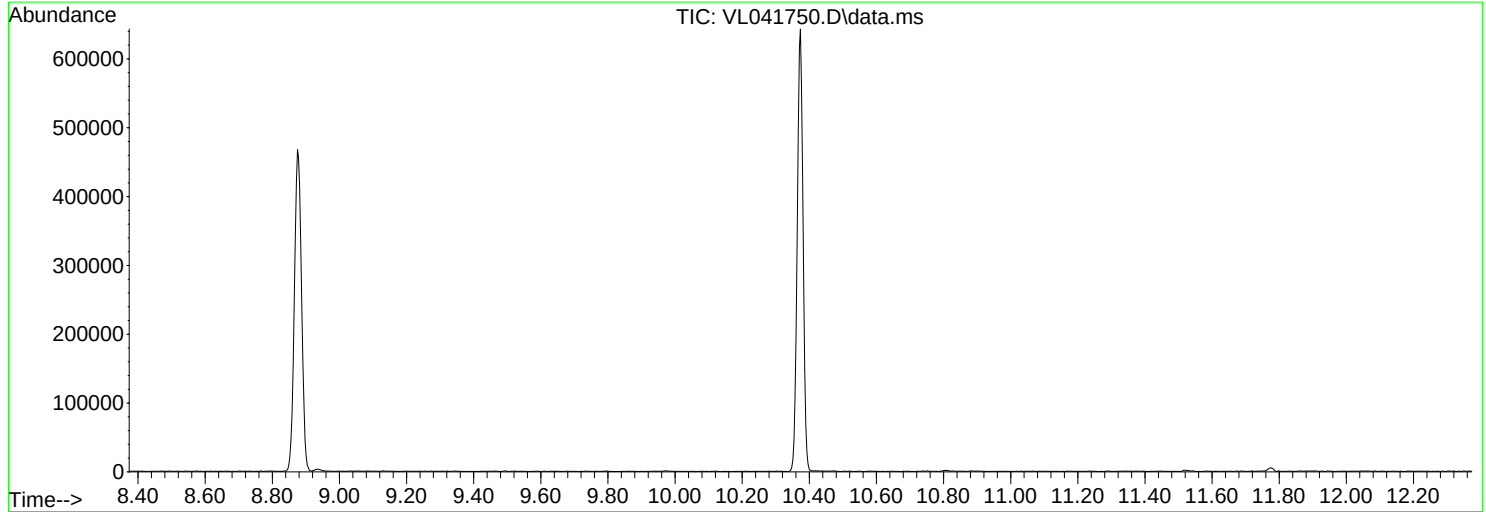

AutoFind: Scans 3177, 3178, 3179; Background Corrected with Scan 3162

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	8	40	25.4	31157	PASS
75	95	30	66	61.5	75504	PASS
95	95	100	100	100.0	122797	PASS
96	95	5	9	6.7	8239	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	63.2	77565	PASS
175	174	4	9	5.5	4234	PASS
176	174	93	101	95.0	73717	PASS
177	176	5	9	6.3	4630	PASS

Average of 10.370 to 10.377 min.: VL041750.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1322	44.05	1016	56.05	2649	65.20	61
36.15	1587	45.05	1575	57.10	4784	66.90	24
37.10	9134	46.15	66	57.90	94	67.10	12
38.10	7991	47.00	1132	58.30	32	68.10	1535
39.10	2839	47.95	1114	60.05	1454	69.10	15463
40.00	41	49.10	7069	61.05	7192	70.15	1071
41.20	26	50.10	31157	62.05	7600	70.90	28
41.70	49	51.10	9016	63.10	6081	72.05	651
42.35	60	52.05	392	64.00	224	73.10	6573
42.95	115	52.80	56	64.20	202	74.10	25661
43.40	59	55.05	422	64.80	43	75.10	75504

Average of 10.370 to 10.377 min.: VL041750.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	6364	87.05	3899	103.85	544	113.00	66
76.90	489	88.10	3363	104.10	151	114.70	31
77.10	175	91.00	654	104.90	42	115.15	90
78.10	122	92.10	3845	105.10	151	115.80	221
78.95	4994	93.05	5724	106.05	566	115.95	358
80.05	1429	94.10	16382	106.95	120	116.95	974
81.05	4383	95.10	122797	107.20	40	117.95	511
81.95	969	96.10	8239	109.95	51	118.90	777
82.90	123	97.00	110	110.95	130	123.10	50
83.10	33	97.15	142	111.70	88	124.00	17
86.05	99	102.70	65	112.65	61	126.90	78

Average of 10.370 to 10.377 min.: VL041750.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
127.70	134	138.95	48	147.70	72	158.95	148
128.05	509	140.00	35	147.85	142	161.05	144
129.05	205	141.05	1317	149.15	97	167.60	18
129.95	553	141.80	73	149.90	118	169.60	17
130.90	245	142.00	67	151.40	43	169.90	39
134.90	170	143.00	1489	152.70	31	170.30	41
135.10	61	144.00	186	153.50	25	170.50	88
136.10	17	145.00	136	154.15	44	170.95	118
136.50	51	145.60	39	155.05	332	171.75	129
136.80	153	145.90	181	156.85	228	172.00	95
137.00	50	146.80	77	158.00	44	172.20	138

Average of 10.370 to 10.377 min.: VL041750.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.10	77565						
175.10	4234						
176.10	73717						
177.05	4630						
177.85	181						
183.30	17						
228.50	47						

Instrument :

MSVOA_L

ClientSampleId :

BFB