
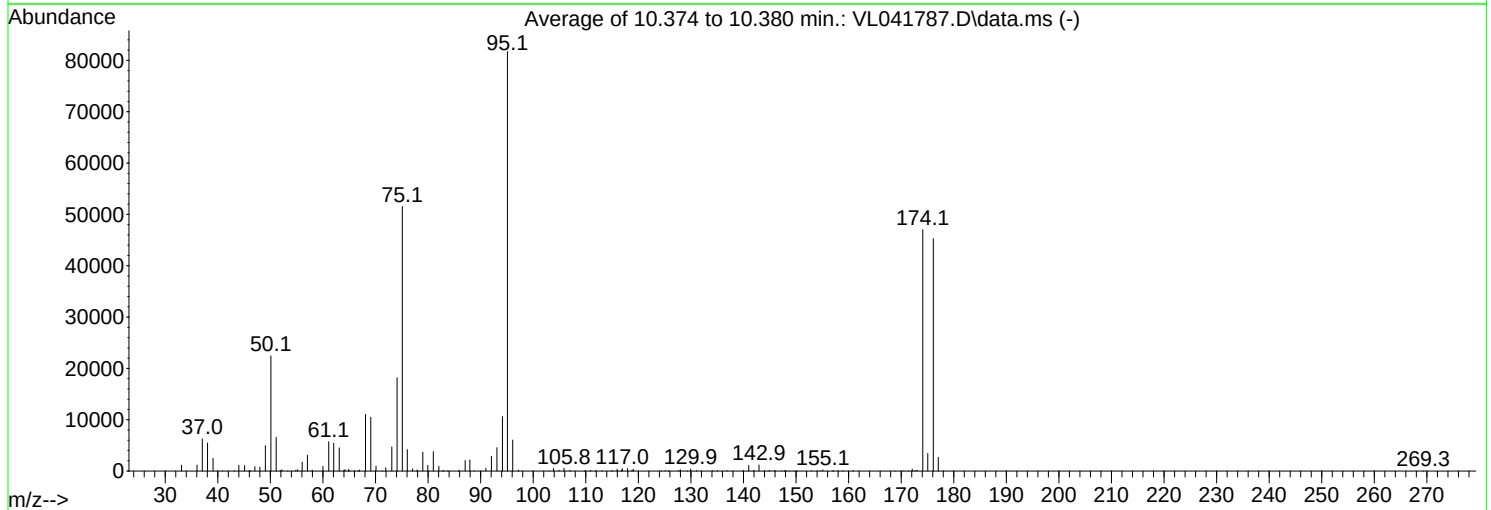


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL121824\
Data File : VL041787.D
Acq On : 18 Dec 2024 08:06
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL121624AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Dec 19 07:32:09 2024

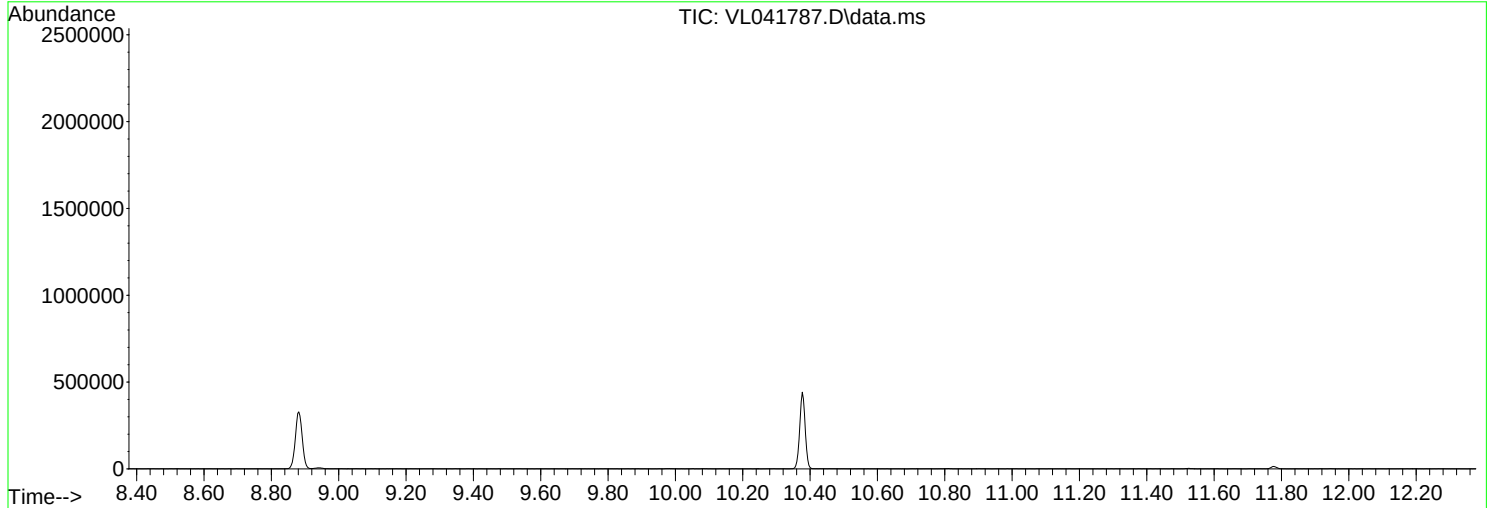

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3165

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	27.5	22445	PASS
75	95	30	66	63.1	51533	PASS
95	95	100	100	100.0	81685	PASS
96	95	5	9	7.4	6040	PASS
173	174	0.00	2	0.4	189	PASS
174	95	50	120	57.6	47024	PASS
175	174	4	9	7.3	3435	PASS
176	174	93	101	96.3	45299	PASS
177	176	5	9	5.9	2683	PASS

Average of 10.374 to 10.380 min.: VL041787.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1141	47.05	858	57.05	3102	66.70	47
36.05	1180	48.00	764	57.95	178	66.95	200
37.05	6288	49.05	4965	60.00	923	68.10	11038
38.05	5467	50.10	22445	61.10	5714	69.10	10482
39.10	2494	51.10	6553	62.05	5427	70.10	981
40.90	31	51.90	123	63.10	4527	71.30	41
43.15	73	52.20	256	64.00	189	71.95	649
44.00	1141	53.30	30	64.20	301	73.10	4685
45.10	1066	54.85	179	64.85	304	74.10	18195
45.95	73	55.20	262	65.10	104	75.10	51533
46.20	47	56.05	1736	65.95	70	76.05	4174

Instrument :

MSVOA_L

ClientSampleId :

BFB

Average of 10.374 to 10.380 min.: VL041787.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.05	436	87.95	2170	104.90	187	116.95	484
77.90	224	88.80	41	105.85	548	117.95	466
79.00	3700	91.00	562	107.00	137	118.80	212
79.95	1115	92.05	2894	109.75	61	119.05	329
81.00	3787	93.10	4562	110.90	154	124.40	18
82.05	950	94.15	10629	111.85	82	125.10	79
82.70	32	95.10	81685	113.10	84	125.75	80
83.00	122	96.10	6040	114.80	31	127.70	141
83.75	45	97.20	186	115.10	55	128.00	257
85.80	123	103.00	19	115.95	361	129.30	28
87.05	2079	103.85	509	116.80	188	129.95	400

Average of 10.374 to 10.380 min.: VL041787.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
131.05	108	147.30	17	157.15	89	175.05	3435
134.10	38	147.85	124	158.05	61	176.10	45299
135.00	142	148.10	54	158.90	87	177.05	2683
136.85	125	148.70	21	160.85	126	178.10	67
139.90	91	149.60	20	168.80	17	269.30	24
141.00	1101	150.15	64	170.50	21		
141.95	144	152.90	26	171.40	50		
142.95	1185	154.00	17	172.10	387		
143.95	74	154.60	41	172.60	118		
144.90	164	155.10	249	173.00	189		
146.00	151	156.90	28	174.10	47024		