


7471B

LB133991

INSTRUMENT ID: CV1

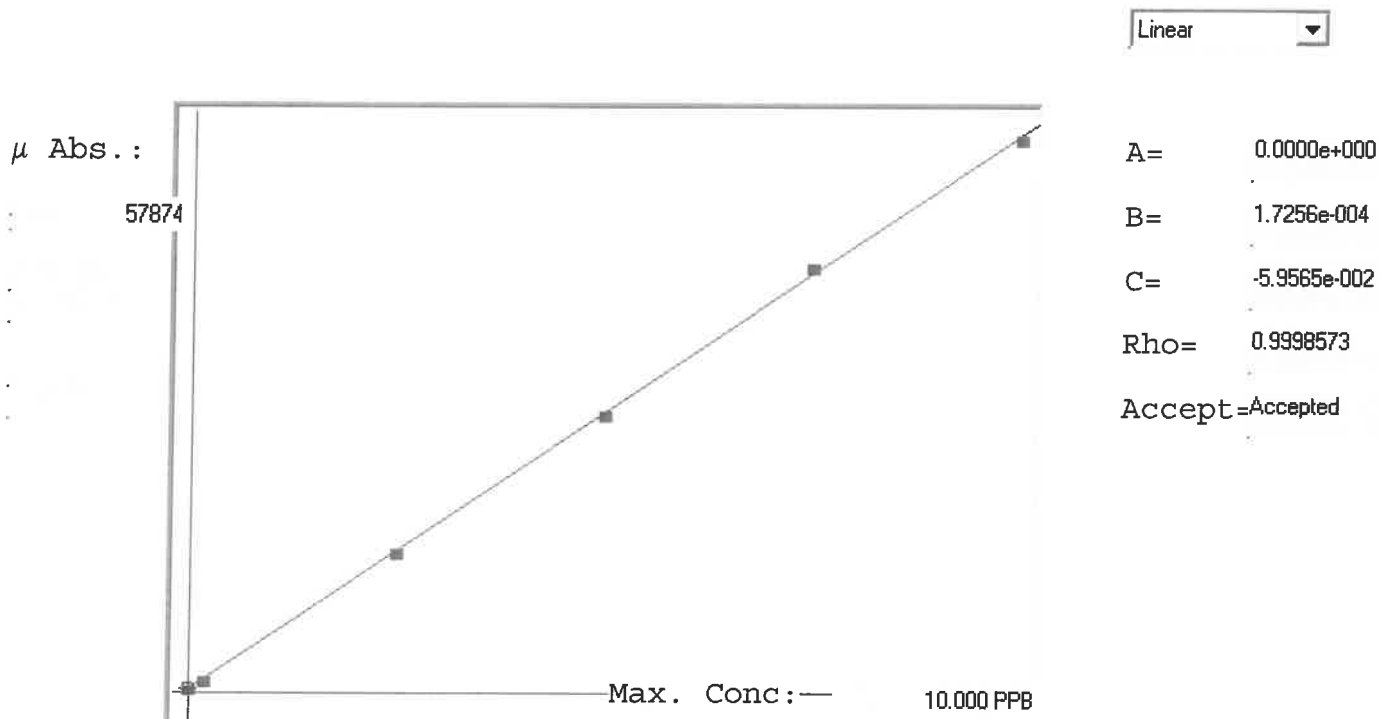

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	g/a))
0.0	0.000	0.030	0.030	520	0.000	520					-
0.2	0.200	0.162	-0.038	1283	0.0 %	1283					19
2.5	2.500	2.496	-0.004	14811	0.0 %	14811					0
5.0	5.000	4.965	-0.035	29118	0.0 %	29118					1
7.5	7.500	7.620	0.120	44504	0.0 %	44504					2
10.0	10.000	9.927	-0.073	57874	0.0 %	57874					1

LB133991 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 18 Dec 2024 13:15:54

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	80	520	-	0.0000	7471B	PPB	18 Dec 2024 13:19:48	S	Std
0.2 - 1	1283	1283	-	0.2000	7471B	PPB	18 Dec 2024 13:22:05	S	Std
2.5 - 1	14811	14811	-	2.5000	7471B	PPB	18 Dec 2024 13:24:22	S	Std
5.0 - 1	29118	29118	-	5.0000	7471B	PPB	18 Dec 2024 13:26:39	S	Std
7.5 - 1	44504	44504	-	7.5000	7471B	PPB	18 Dec 2024 13:28:57	S	Std
10.0 - 1	57874	57874	-	10.0000	7471B	PPB	18 Dec 2024 13:31:16	S	Std
ICV24 - 1	ICV24	23822	4.0511	-7471B	PPB	PPB	18 Dec 2024 13:36:51	U	SMPL
ICB24 - 1	ICB24	287	-0.0100	-7471B	PPB	PPB	18 Dec 2024 13:39:06	U	SMPL
CCV42 - 1	CCV42	26606	4.5315	-7471B	PPB	PPB	18 Dec 2024 13:41:24	U	SMPL
CCB42 - 1	CCB42	535	0.0328	-7471B	PPB	PPB	18 Dec 2024 13:43:38	U	SMPL
CRA - 1	CRA	1289	0.1629	-7471B	PPB	PPB	18 Dec 2024 13:45:58	U	SMPL
HighStd - 1	HighStd	58947	10.1121	-7471B	PPB	PPB	18 Dec 2024 13:48:13	U	SMPL
ChkStd - 1	ChkStd	40999	7.0151	-7471B	PPB	PPB	18 Dec 2024 13:50:28	U	SMPL
PB165728BL - 1	PBS	89	-0.0442	-7471B	PPB	PPB	18 Dec 2024 13:52:49	U	SMPL
PB165728BS - 1	LCSS	20330	3.4485	-7471B	PPB	PPB	18 Dec 2024 13:55:08	U	SMPL
P5299-01 - 1	SB-01	10161	1.6938	-7471B	PPB	PPB	18 Dec 2024 13:57:25	U	SMPL
P5299-02 - 1	SB-02	6996	1.1476	-7471B	PPB	PPB	18 Dec 2024 13:59:43	U	SMPL
P5299-03 - 1	SB-01	7020	1.1518	-7471B	PPB	PPB	18 Dec 2024 14:02:03	U	SMPL
P5299-04 - 1	SB-02	1808	0.2524	-7471B	PPB	PPB	18 Dec 2024 14:04:22	U	SMPL
P5301-01 - 1	HR-01-121624	23554	4.0048	-7471B	PPB	PPB	18 Dec 2024 14:06:39	U	SMPL
CCV43 - 1	CCV43	27689	4.7184	-7471B	PPB	PPB	18 Dec 2024 14:08:55	U	SMPL
CCB43 - 1	CCB43	137	-0.0359	-7471B	PPB	PPB	18 Dec 2024 14:11:13	U	SMPL
P5301-03 - 1	HR-04-121624	3057	0.4679	-7471B	PPB	PPB	18 Dec 2024 14:13:31	U	SMPL
P5301-03DUP - 1	HR-04-121624DUP	2668	0.4008	-7471B	PPB	PPB	18 Dec 2024 14:25:15	U	SMPL
P5301-03MS - 1	HR-04-121624MS	20839	3.5363	-7471B	PPB	PPB	18 Dec 2024 14:27:30	U	SMPL
P5301-03MSD - 1	HR-04-121624MSD	20533	3.4835	-7471B	PPB	PPB	18 Dec 2024 14:29:46	U	SMPL
P5306-01 - 1	OU4-VSL-07-121224	969	0.1076	-7471B	PPB	PPB	18 Dec 2024 14:32:05	U	SMPL
P5306-03 - 1	OU4-VSL-08-121224	377	0.0055	-7471B	PPB	PPB	18 Dec 2024 14:34:24	U	SMPL
P5306-05 - 1	OU4-VSL-09-121224	540	0.0336	-7471B	PPB	PPB	18 Dec 2024 14:36:41	U	SMPL
P5306-07 - 1	OU4-VSL-10-121224	489	0.0248	-7471B	PPB	PPB	18 Dec 2024 14:38:58	U	SMPL
P5306-09 - 1	OU4-VSL-11-121224	480	0.0233	-7471B	PPB	PPB	18 Dec 2024 14:41:14	U	SMPL
P5306-11 - 1	OU4-VSL-12-121224	460	0.0198	-7471B	PPB	PPB	18 Dec 2024 14:43:30	U	SMPL
CCV44 - 1	CCV44	26503	4.5137	-7471B	PPB	PPB	18 Dec 2024 14:45:45	U	SMPL
CCB44 - 1	CCB44	125	-0.0380	-7471B	PPB	PPB	18 Dec 2024 14:48:01	U	SMPL
P5306-13 - 1	OU4-VSL-13-121224	1044	0.1206	-7471B	PPB	PPB	18 Dec 2024 14:50:19	U	SMPL
P5306-15 - 1	OU4-VSL-14-121224	433	0.0152	-7471B	PPB	PPB	18 Dec 2024 14:52:35	U	SMPL
P5312-01 - 1	SOIL-VNJ-222	1155	0.1397	-7471B	PPB	PPB	18 Dec 2024 14:54:50	U	SMPL
P5312-03 - 1	CONCRETE-VNJ-222	536	0.0329	-7471B	PPB	PPB	18 Dec 2024 14:57:06	U	SMPL
P5301-03LX5 - 1		664	0.0550	-7471B	PPB	PPB	18 Dec 2024 15:03:03	U	SMPL
CCV45 - 1	CCV45	22572	3.8354	-7471B	PPB	PPB	18 Dec 2024 15:05:19	U	SMPL
CCB45 - 1	CCB45	28352	4.8328	-7471B	PPB	PPB	18 Dec 2024 15:07:36	U	SMPL
		197	-0.0256	-7471B	PPB	PPB	18 Dec 2024 15:09:56	U	SMPL