


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122624\
Data File : BF140969.D
Acq On : 26 Dec 2024 15:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 27 00:31:16 2024

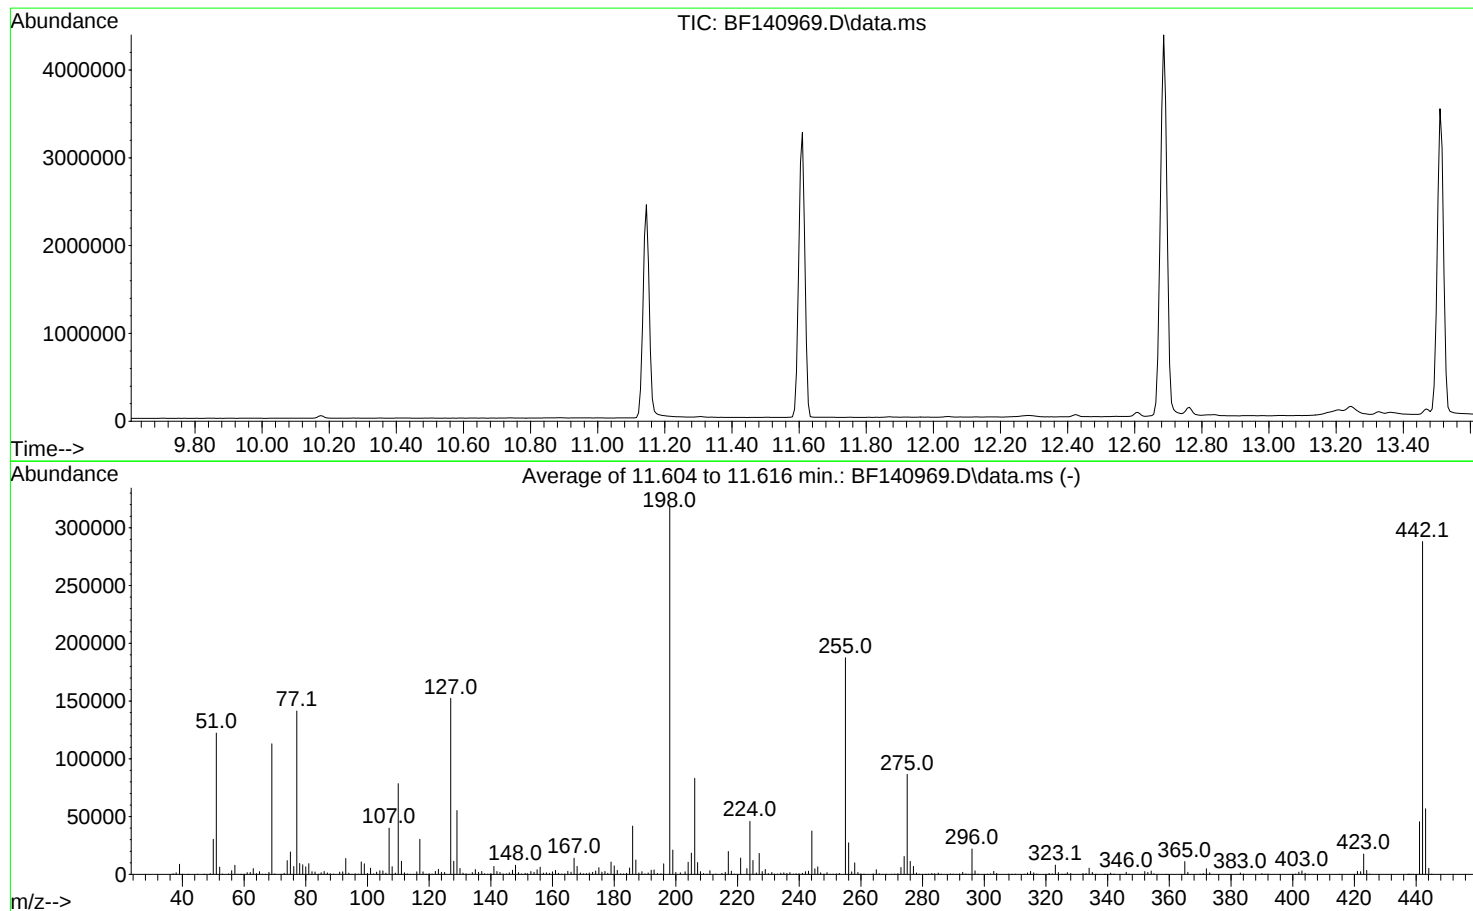




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1610

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	38.4	122253	PASS
68	69	0.00	2	1.7	1874	PASS
69	198	0.00	100	35.5	113056	PASS
70	69	0.00	2	0.4	479	PASS
127	198	10	80	47.8	152328	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	318400	PASS
199	198	5	9	6.6	21108	PASS
275	198	10	60	27.2	86501	PASS
365	198	1	100	3.5	11162	PASS
441	198	0.01	100	14.3	45621	PASS
442	442	50	100	100.0	288064	PASS
443	442	15	24	19.7	56736	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122624\
Data File : BF140969.D
Acq On : 26 Dec 2024 15:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 27 00:41:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

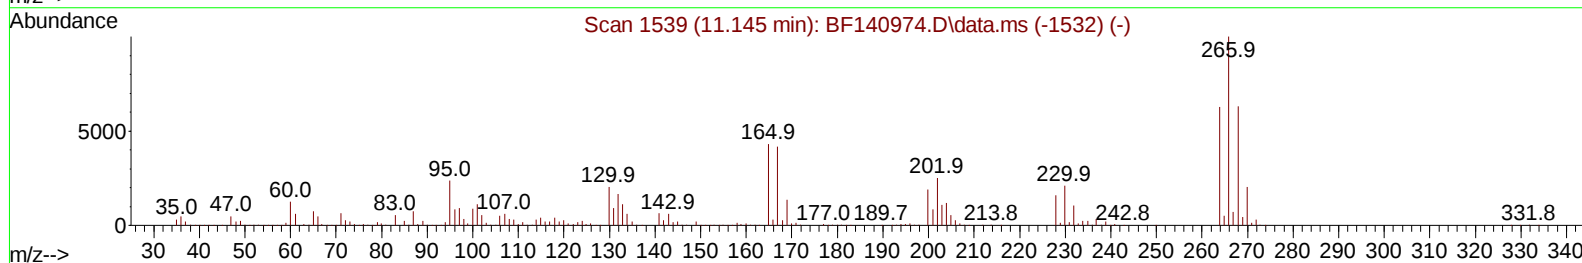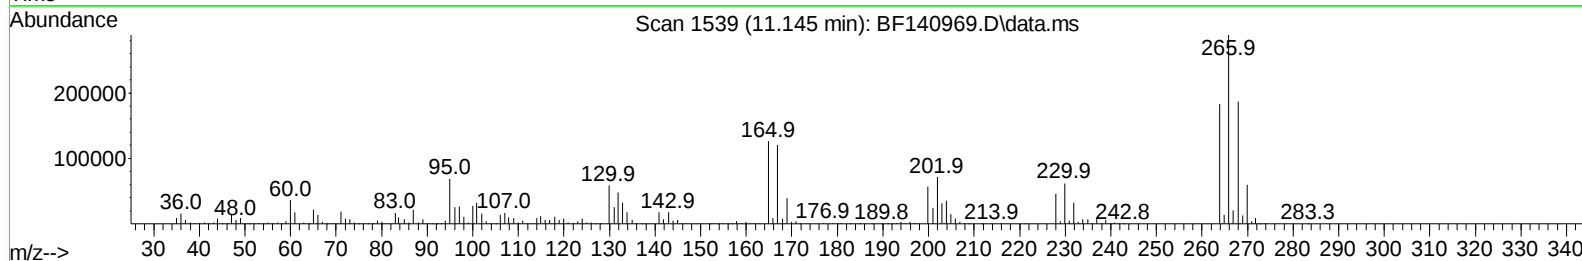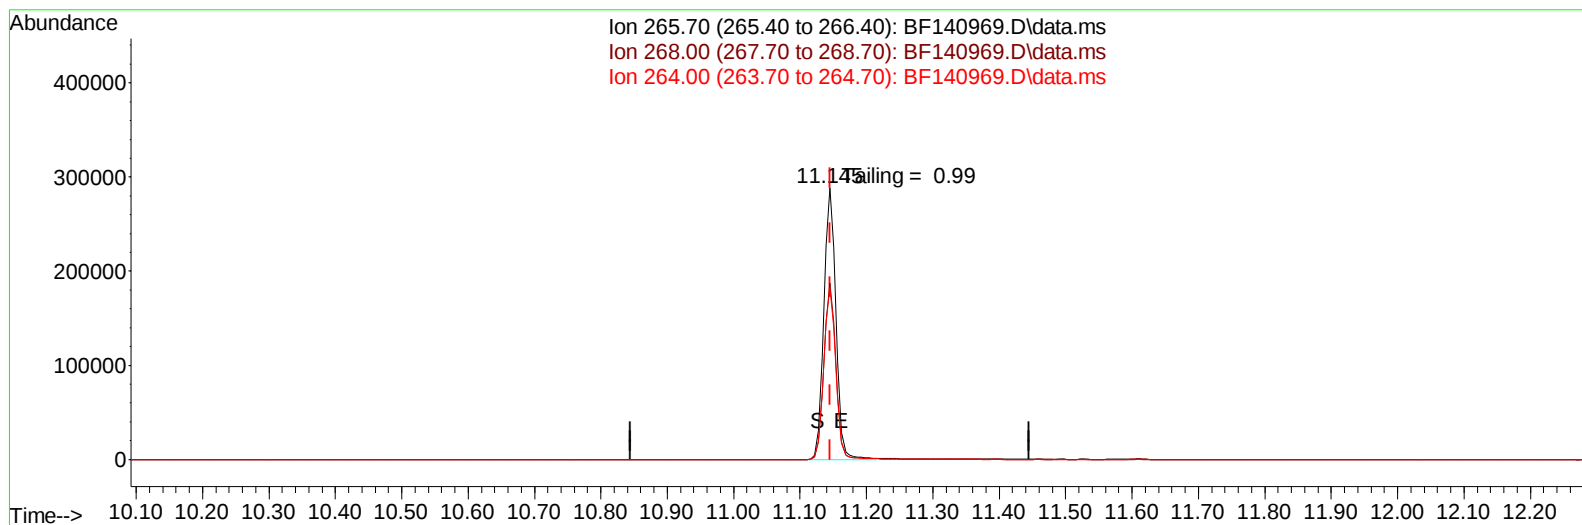

TIC: BF140969.D\data.ms

(70) Pentachlorophenol (C)

11.145min (+ 0.000) 171712.33 ng




response 370836

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.90
264.00	62.80	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122624\
Data File : BF140969.D
Acq On : 26 Dec 2024 15:57
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 27 00:41:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

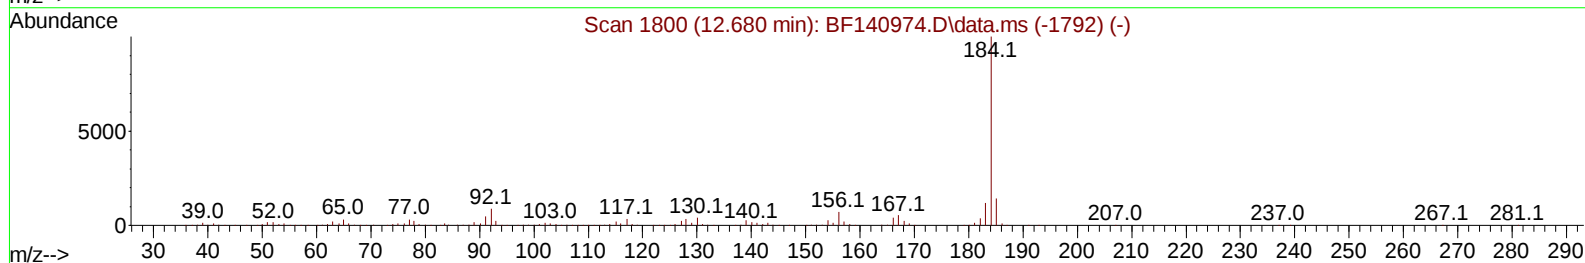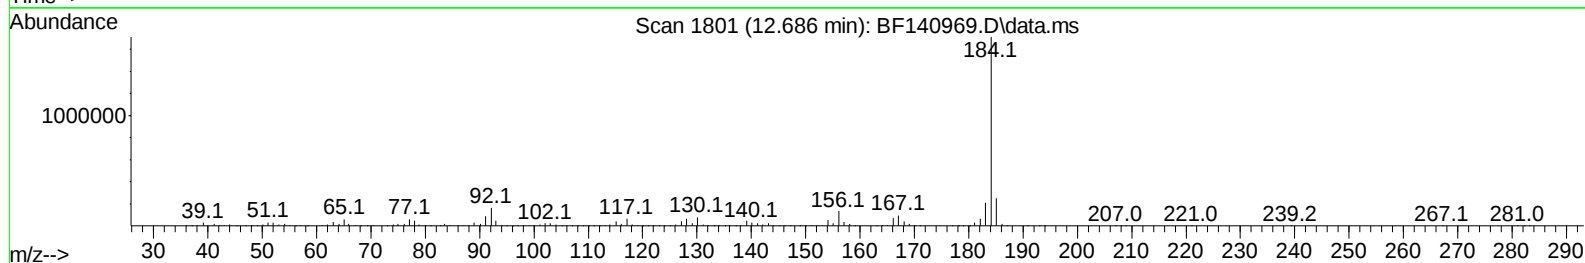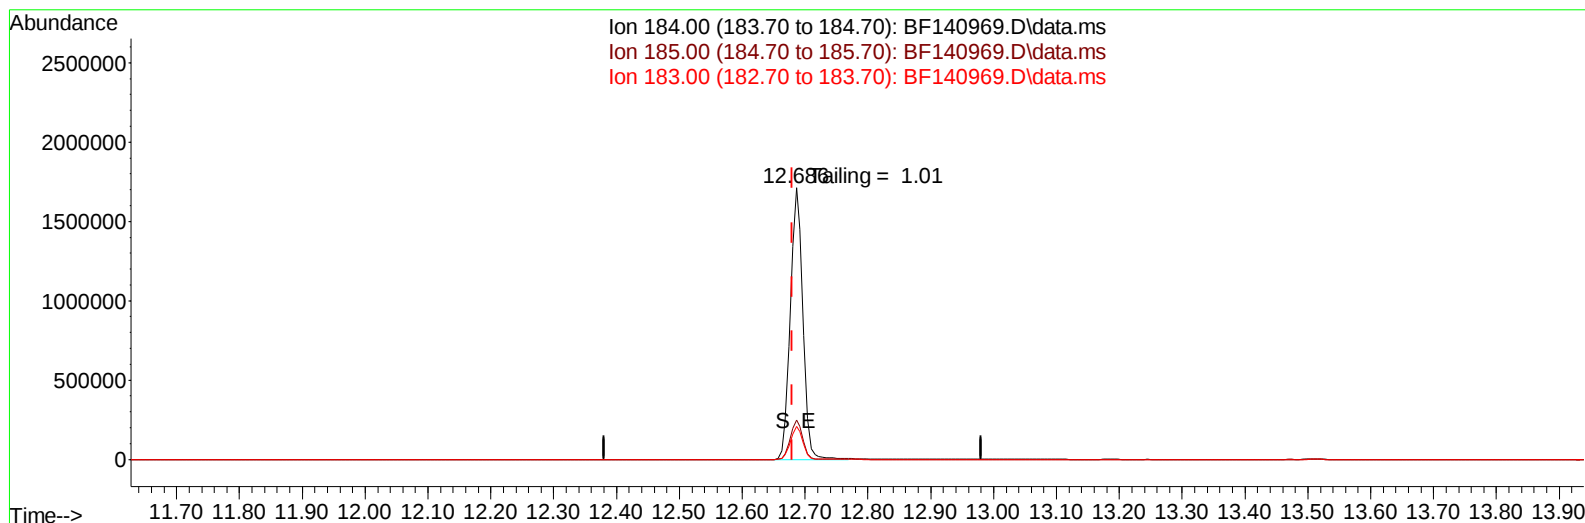

TIC: BF140969.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 253030.63 ng

response 2406398

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.44
183.00	11.70	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/26/2024	BNA_F	<u>BF140969.D</u>
Compound Name	Response	Retention Time
DDT	737647	13.51
DDD	7676	13.239
DDE	0	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7676	745323	1.03

Instrument :
BNA_F
ClientSampleId :
DFTPP