

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121924\
 Data File : PL093436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Dec 2024 15:47
 Operator : AR\AJ
 Sample : P5306-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU4-VSL-10-121224

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/20/2024
 Supervised By : Ankita Jodhani 12/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 19 21:51:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 15:18:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.775	56444065	62562836	21.718m	21.693
28) SA Decachlor...	9.057	7.912	44384342	68709325	25.530	24.054

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL121924\
Data File : PL093436.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Dec 2024 15:47
Operator : AR\AJ
Sample : P5306-07
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OU4-VSL-10-121224


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/20/2024
Supervised By : Ankita Jodhani 12/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 19 21:51:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 15:18:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

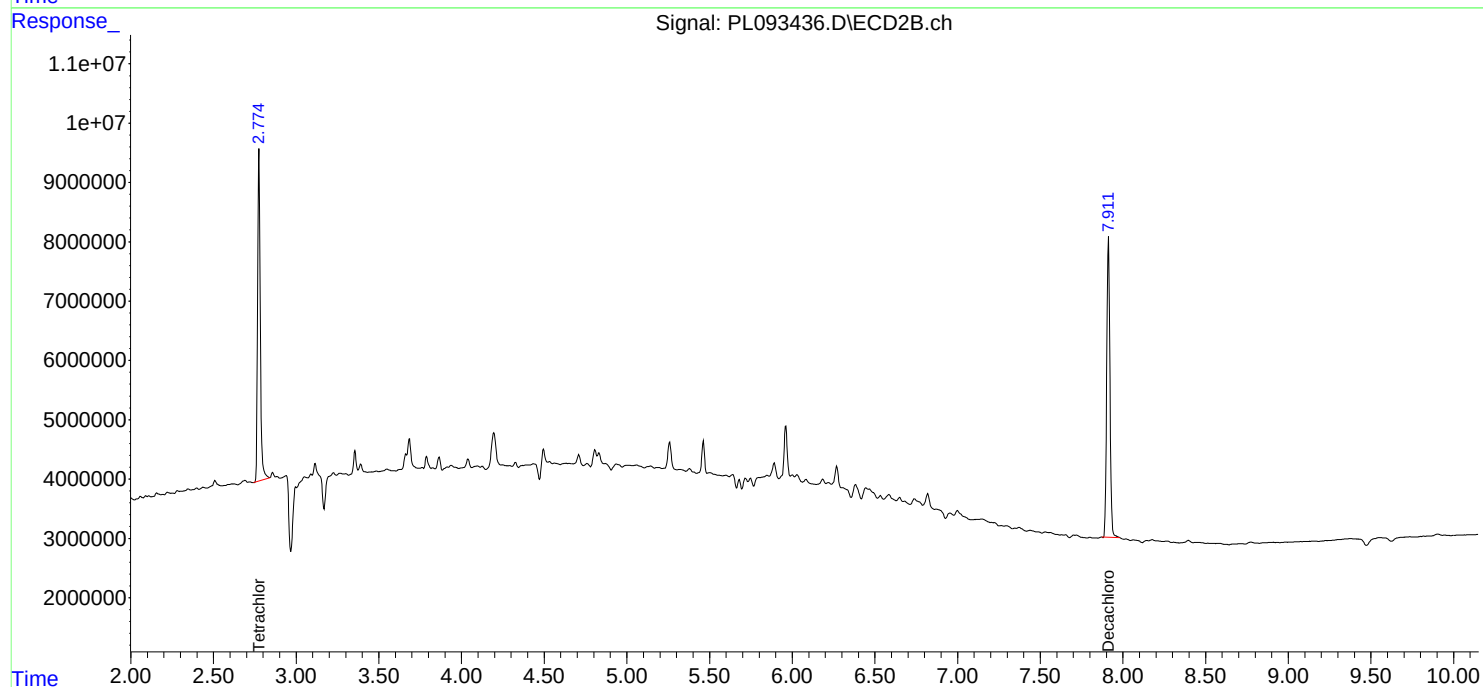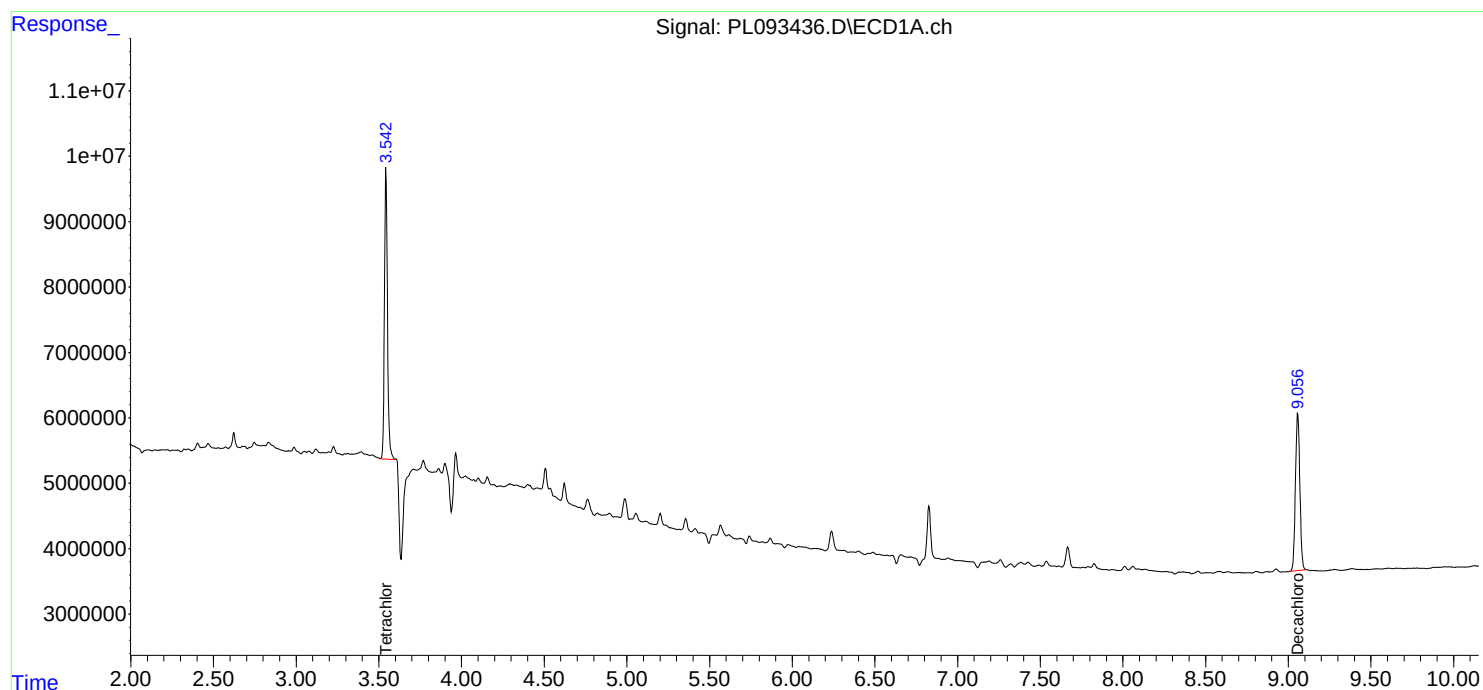

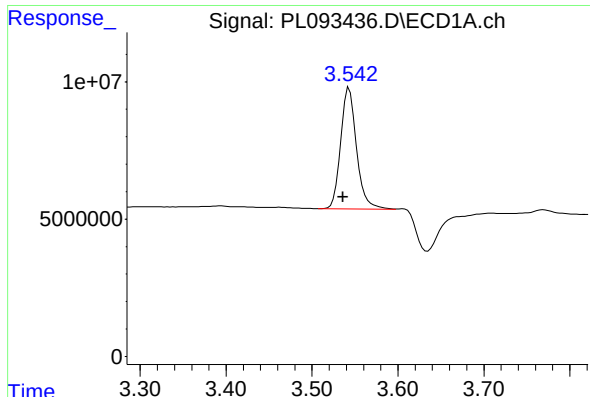


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: 0.006 min
Response: 56444065
Conc: 21.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU4-VSL-10-121224


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/20/2024
Supervised By :Ankita Jodhani 12/20/2024

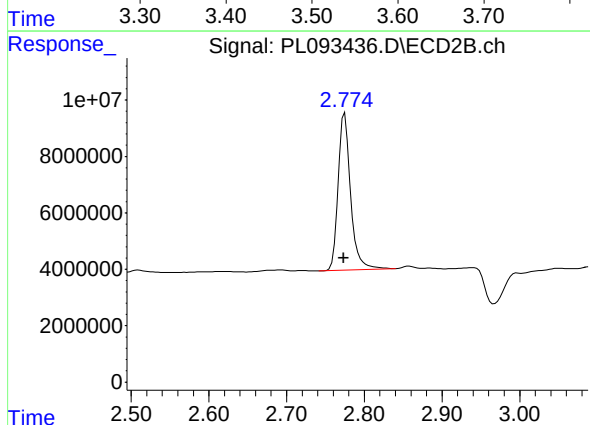


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.001 min
Response: 62562836
Conc: 21.69 ng/ml

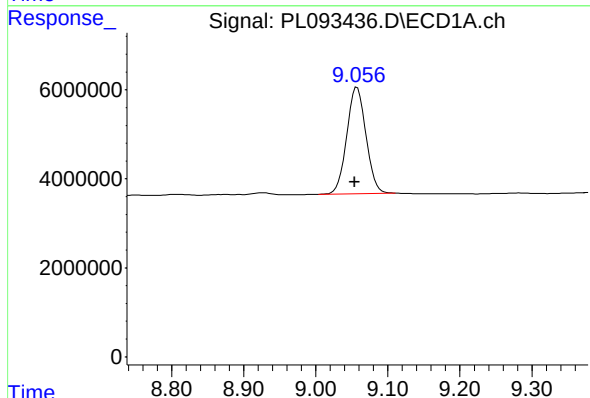

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: 0.003 min
Response: 44384342
Conc: 25.53 ng/ml

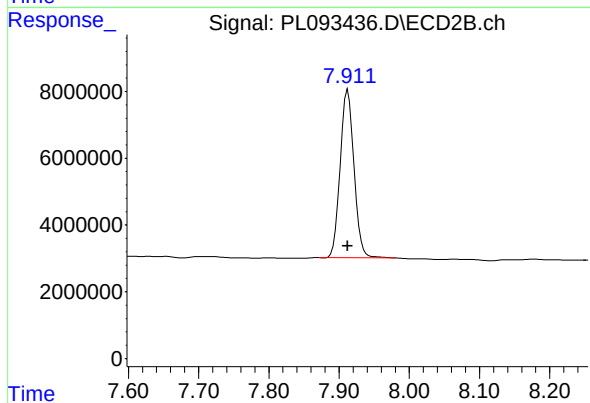

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 68709325
Conc: 24.05 ng/ml