

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122624\
 Data File : BN035846.D
 Acq On : 26 Dec 2024 10:35
 Operator : RC/JU
 Sample : PB165724BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB165724BL

Quant Time: Dec 27 00:40:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 23:06:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.257	152	4513	0.400	ng	-0.01
7) Naphthalene-d8	9.999	136	10649	0.400	ng	-0.02
13) Acenaphthene-d10	13.924	164	6575	0.400	ng	-0.01
19) Phenanthrene-d10	16.698	188	14052	0.400	ng	# 0.00
29) Chrysene-d12	20.947	240	10269	0.400	ng	# 0.00
35) Perylene-d12	23.029	264	9894	0.400	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	4.924	112	3643	0.323	ng	-0.01
5) Phenol-d6	6.470	99	3773	0.278	ng	-0.02
8) Nitrobenzene-d5	8.397	82	3146	0.484	ng	-0.01
11) 2-Methylnaphthalene-d10	11.610	152	6172	0.370	ng	-0.01
14) 2,4,6-Tribromophenol	15.443	330	975	0.209	ng	-0.01
15) 2-Fluorobiphenyl	12.533	172	9551	0.384	ng	-0.01
27) Fluoranthene-d10	18.747	212	15078	0.379	ng	-0.01
31) Terphenyl-d14	19.375	244	10893	0.538	ng	-0.01
Target Compounds						
34) Bis(2-ethylhexyl)phtha...	20.893	149	381	0.027	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122624\
Data File : BN035846.D
Acq On : 26 Dec 2024 10:35
Operator : RC/JU
Sample : PB165724BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB165724BL


Quant Time: Dec 27 00:40:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 19 23:06:19 2024
Response via : Initial Calibration

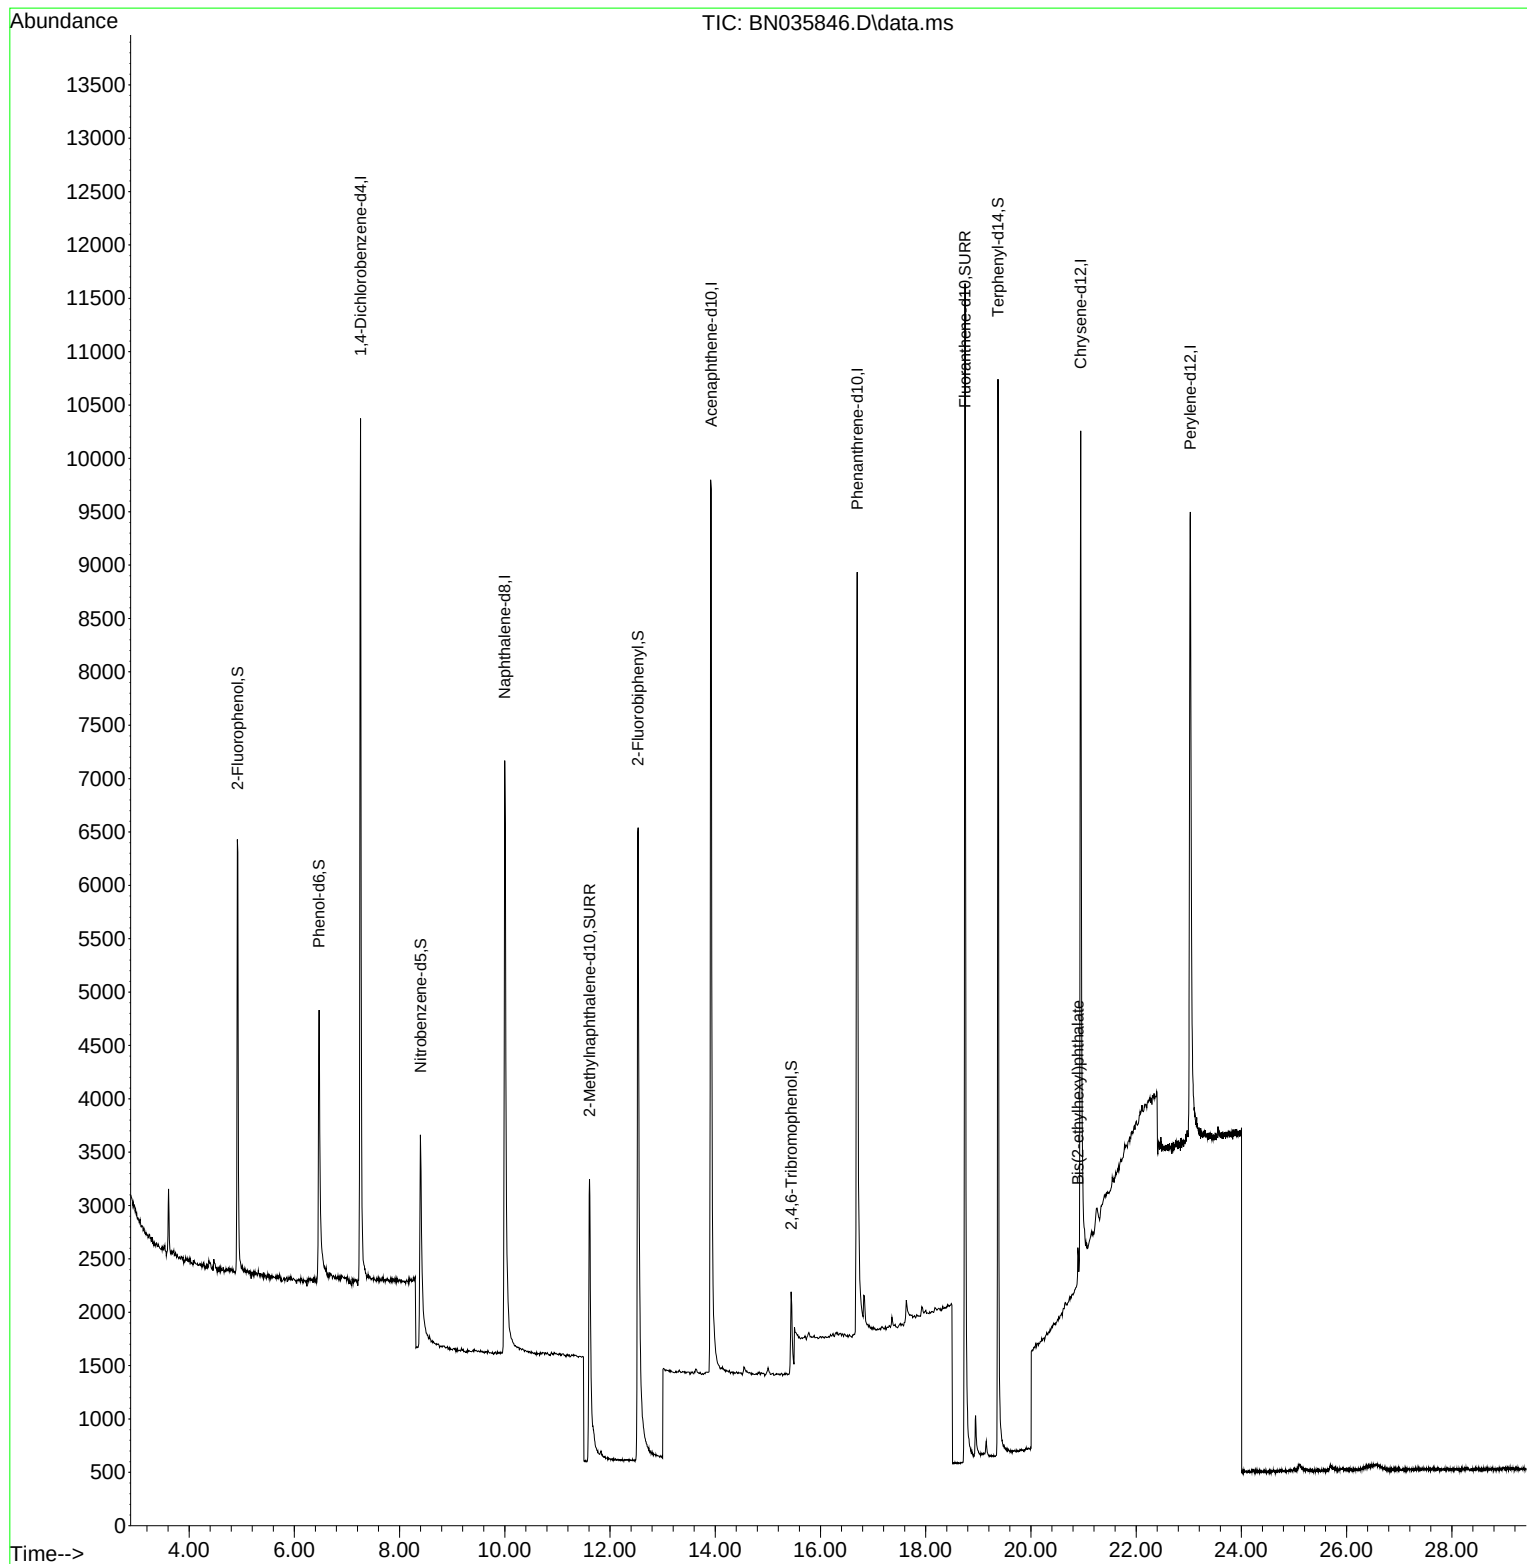

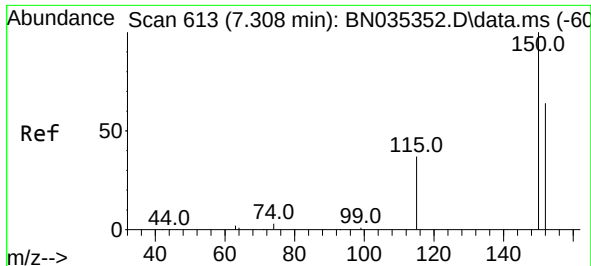




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.257 min Scan# 606
 Delta R.T. -0.015 min
 Lab File: BN035846.D
 Acq: 26 Dec 2024 10:35

Instrument :
 BNA_N
 ClientSampleId :
 PB165724BL

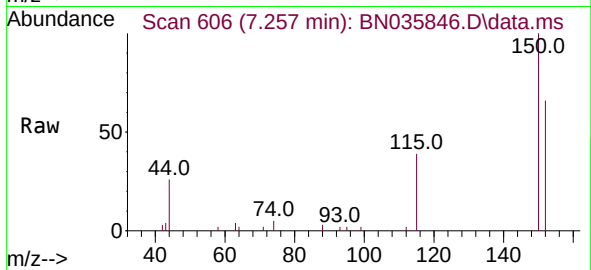

Tgt Ion:152 Resp: 4513




Ion	Ratio	Lower	Upper
152	100		
150	152.2	124.0	186.0
115	58.6	49.6	74.4

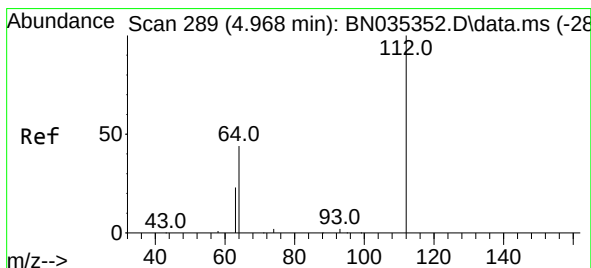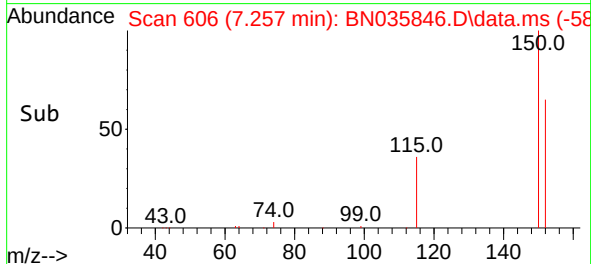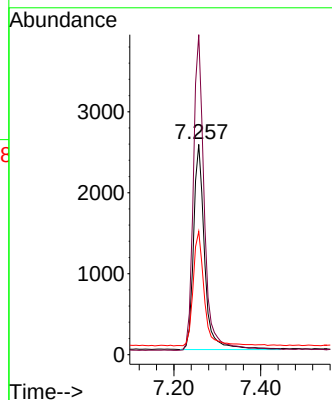


#4
 2-Fluorophenol
 Concen: 0.323 ng
 RT: 4.924 min Scan# 283
 Delta R.T. -0.015 min
 Lab File: BN035846.D
 Acq: 26 Dec 2024 10:35

Tgt Ion:112 Resp: 3643

Ion	Ratio	Lower	Upper
112	100		
64	52.8	39.8	59.8
63	27.4	21.0	31.6


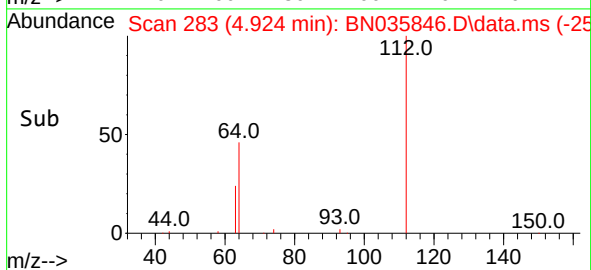
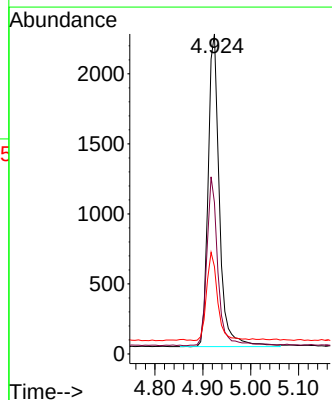
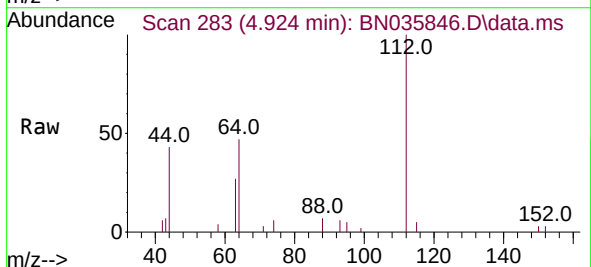


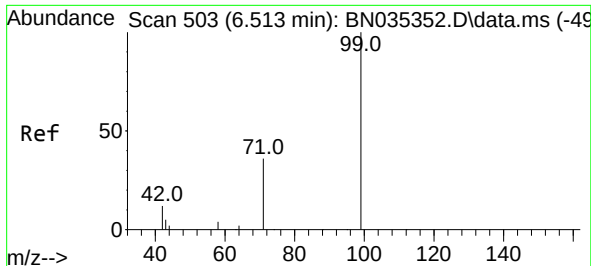

#5
Phenol-d6
Concen: 0.278 ng
RT: 6.470 min Scan# 497
Delta R.T. -0.022 min
Lab File: BN035846.D
Acq: 26 Dec 2024 10:35




Instrument :
BNA_N
ClientSampleId :
PB165724BL


Tgt Ion:	99	Resp:	3773
Ion	Ratio	Lower	Upper
99	100		
42	12.5	11.4	17.2
71	37.4	29.3	43.9

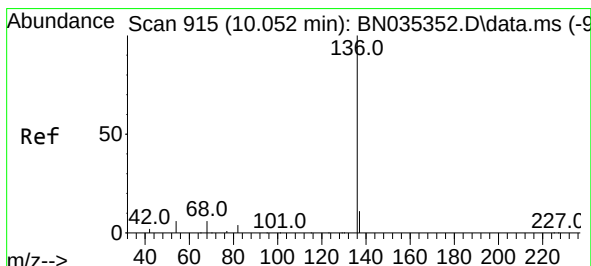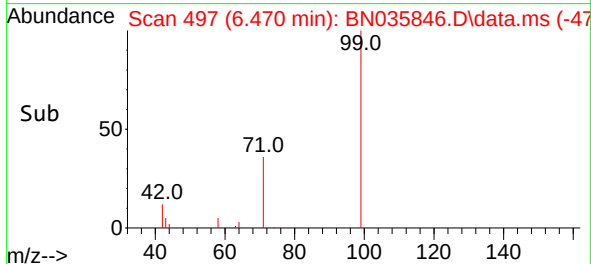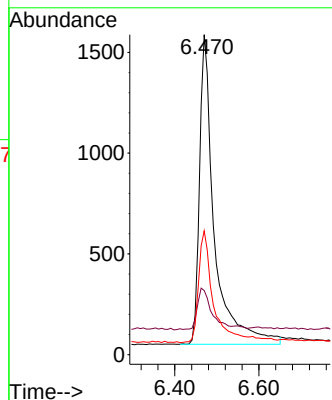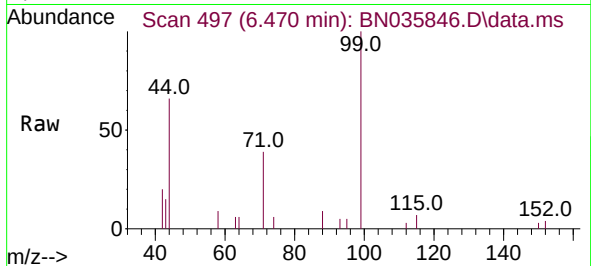

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 9.999 min Scan# 910
Delta R.T. -0.022 min
Lab File: BN035846.D
Acq: 26 Dec 2024 10:35

Tgt Ion:	136	Resp:	10649
Ion	Ratio	Lower	Upper
136	100		
137	12.1	10.2	15.2
54	7.7	6.1	9.1
68	8.0	6.4	9.6


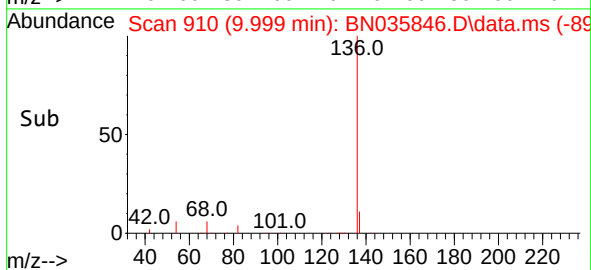
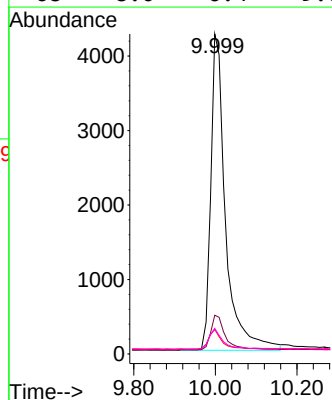
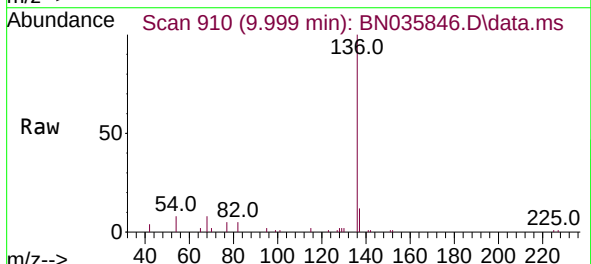


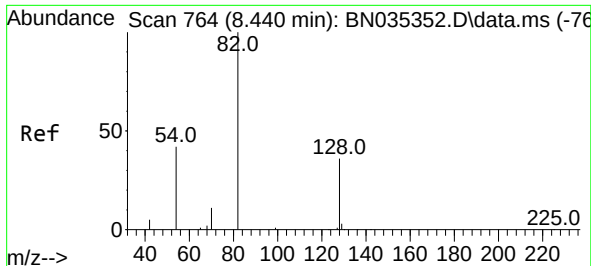

#8
Nitrobenzene-d5
Concen: 0.484 ng
RT: 8.397 min Scan# 70
Delta R.T. -0.011 min
Lab File: BN035846.D
Acq: 26 Dec 2024 10:35




Instrument :
BNA_N
ClientSampleId :
PB165724BL


Tgt Ion: 82 Resp: 3146
Ion Ratio Lower Upper
82 100
128 43.9 33.4 50.0
54 43.1 36.7 55.1

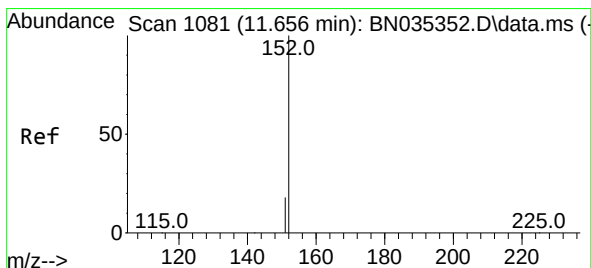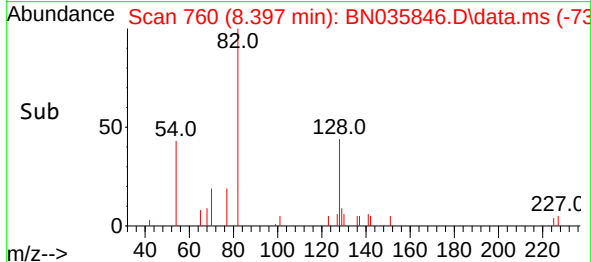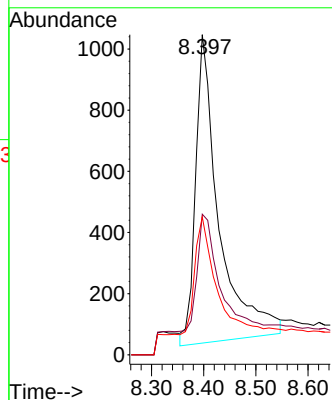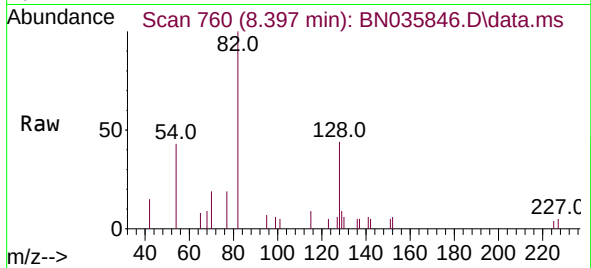

#11
2-Methylnaphthalene-d10
Concen: 0.370 ng
RT: 11.610 min Scan# 1072
Delta R.T. -0.010 min
Lab File: BN035846.D
Acq: 26 Dec 2024 10:35

Tgt Ion: 152 Resp: 6172
Ion Ratio Lower Upper
152 100
151 21.4 16.6 25.0

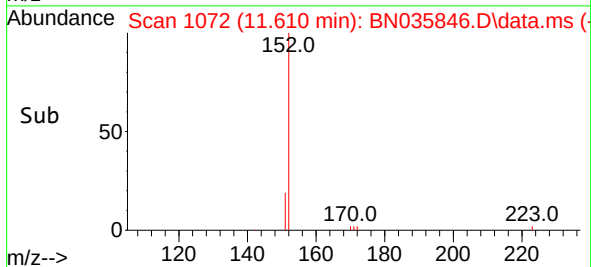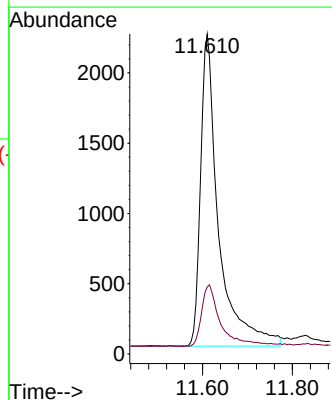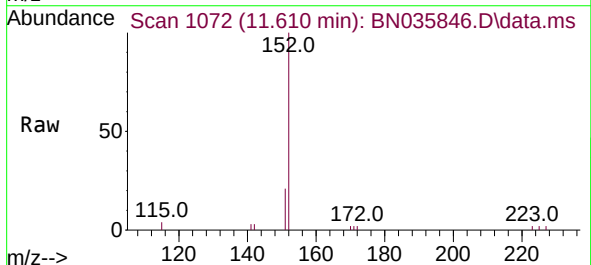

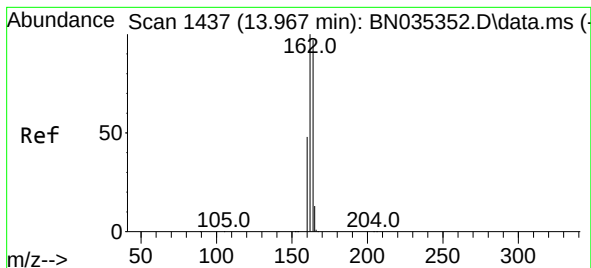

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 13.924 min Scan# 14

Delta R.T. -0.011 min

Lab File: BN035846.D

Acq: 26 Dec 2024 10:35

Instrument :

BNA_N

ClientSampleId :

PB165724BL





Tgt Ion:164 Resp: 6575

Ion Ratio Lower Upper

164 100

162 101.8 82.2 123.2

160 50.1 40.1 60.1

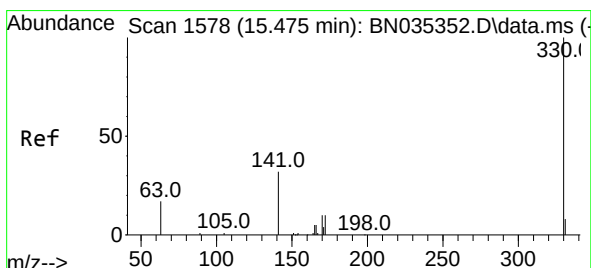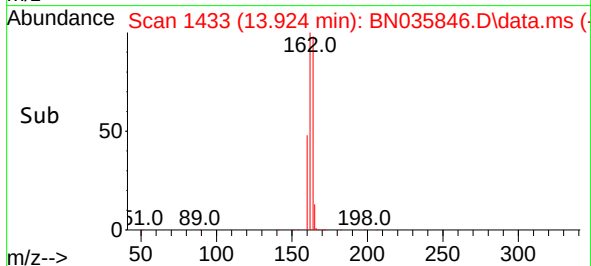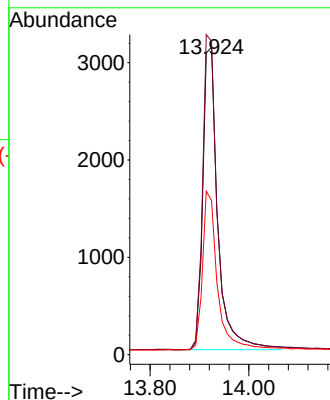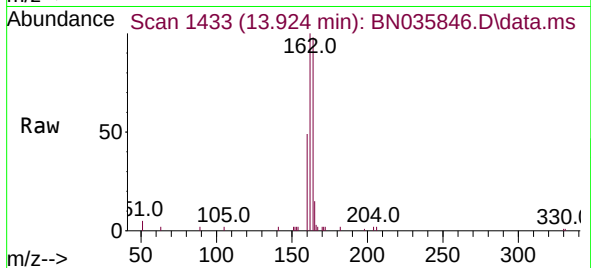

#14

2,4,6-Tribromophenol

Concen: 0.209 ng

RT: 15.443 min Scan# 1575

Delta R.T. -0.011 min

Lab File: BN035846.D

Acq: 26 Dec 2024 10:35




Tgt Ion:330 Resp: 975


Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0

141 32.3 26.6 40.0


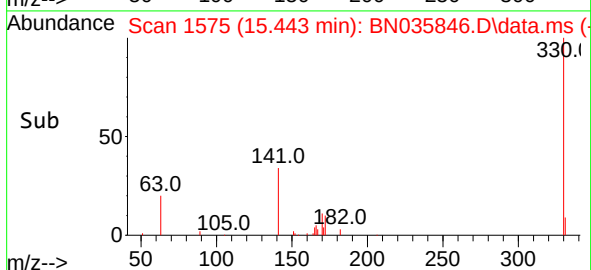
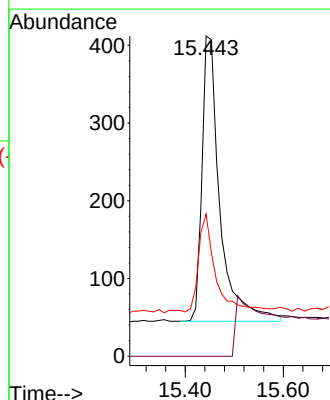
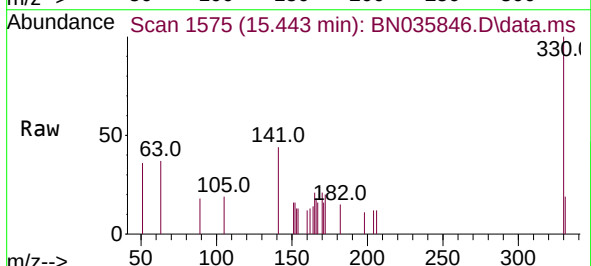


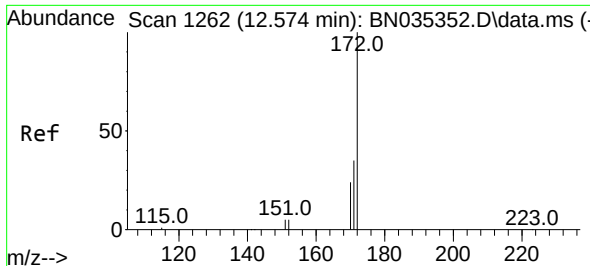

#15
2-Fluorobiphenyl
Concen: 0.384 ng
RT: 12.533 min Scan# 11
Delta R.T. -0.010 min
Lab File: BN035846.D
Acq: 26 Dec 2024 10:35




Instrument :
BNA_N
ClientSampleId :
PB165724BL


Tgt Ion:172	Resp:	9551
Ion Ratio	Lower	Upper
172	100	
171	35.7	29.0 43.4
170	24.0	19.8 29.8

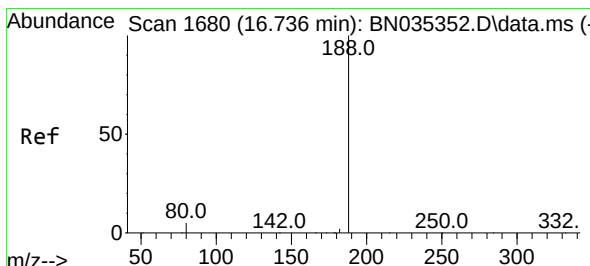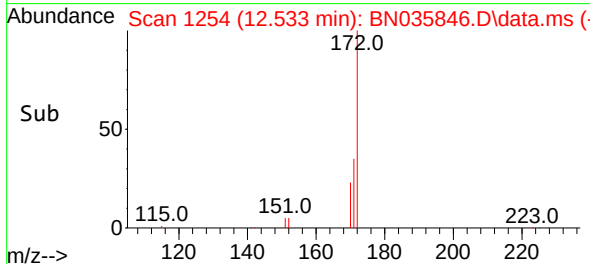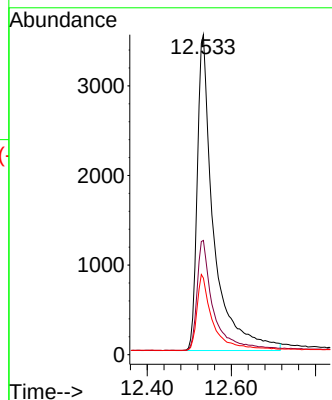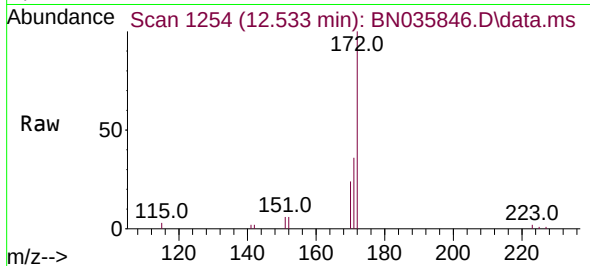

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.698 min Scan# 1677
Delta R.T. -0.000 min
Lab File: BN035846.D
Acq: 26 Dec 2024 10:35

Tgt Ion:188	Resp:	14052
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0 0.0
80	8.5	4.6 6.8


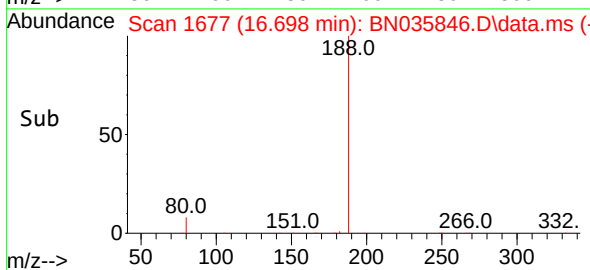
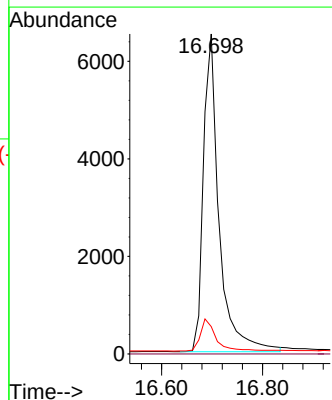
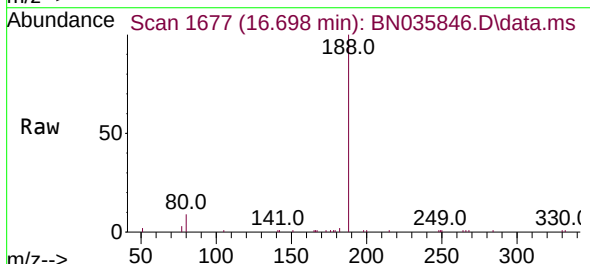


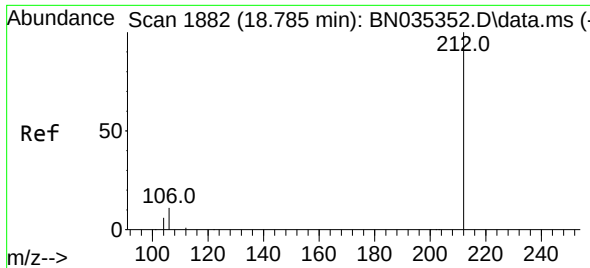

#27
Fluoranthene-d10
Concen: 0.379 ng
RT: 18.747 min Scan# 11
Delta R.T. -0.014 min
Lab File: BN035846.D
Acq: 26 Dec 2024 10:35




Instrument :
BNA_N
ClientSampleId :
PB165724BL


Tgt Ion:212 Resp: 15078
Ion Ratio Lower Upper
212 100
106 12.7 9.2 13.8
104 7.2 5.3 7.9

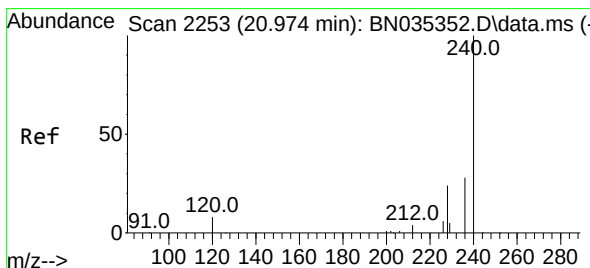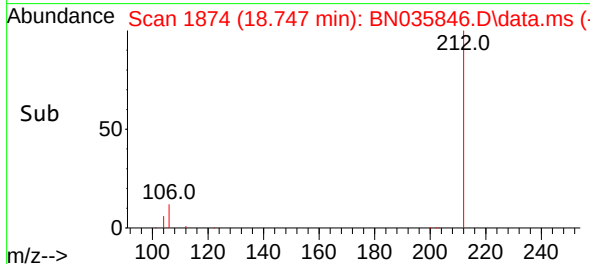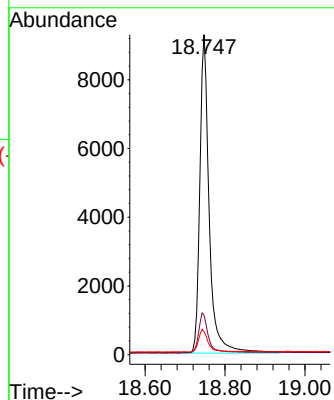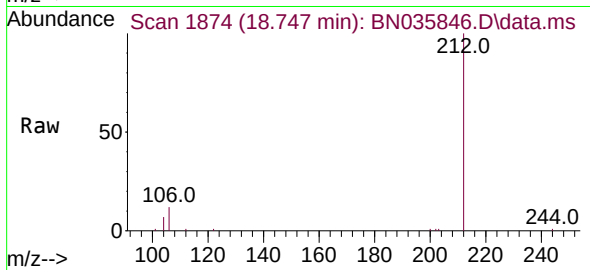

#29
Chrysene-d12
Concen: 0.400 ng
RT: 20.947 min Scan# 2250
Delta R.T. -0.009 min
Lab File: BN035846.D
Acq: 26 Dec 2024 10:35

Tgt Ion:240 Resp: 10269
Ion Ratio Lower Upper
240 100
120 12.5 7.9 11.9#
236 28.9 22.9 34.3


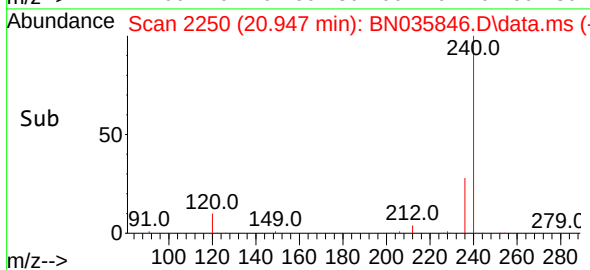
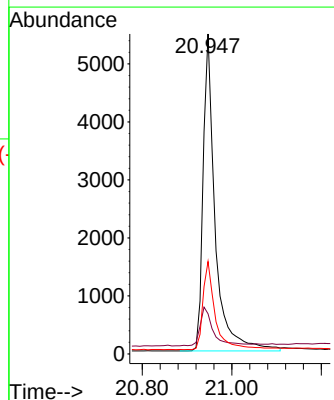
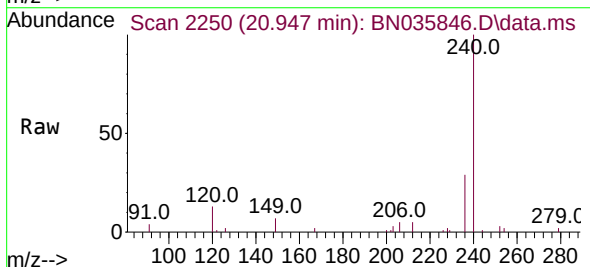


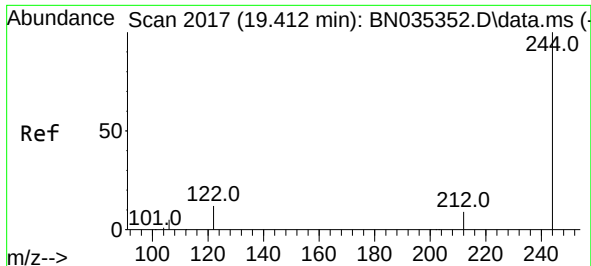

#31
 Terphenyl-d14
 Concen: 0.538 ng
 RT: 19.375 min Scan# 2017
 Delta R.T. -0.014 min
 Lab File: BN035846.D
 Acq: 26 Dec 2024 10:35




Instrument :
 BNA_N
 ClientSampleId :
 PB165724BL


Tgt Ion:244 Resp: 10893
 Ion Ratio Lower Upper
 244 100
 212 9.6 8.1 12.1
 122 14.2 10.3 15.5

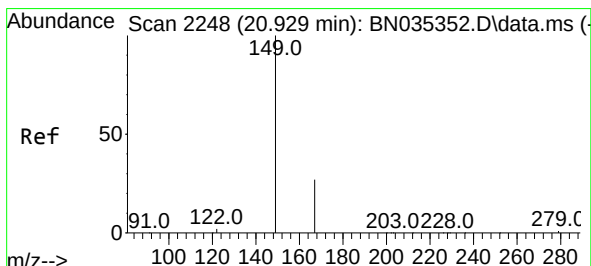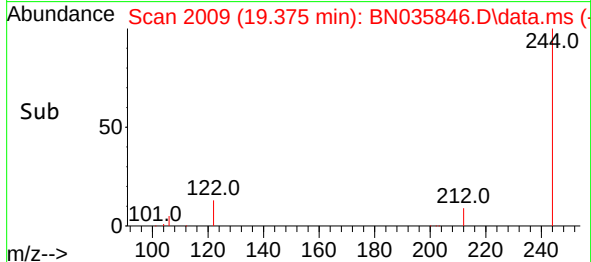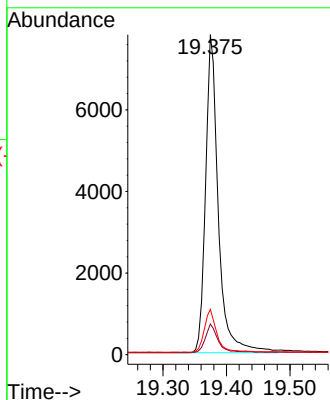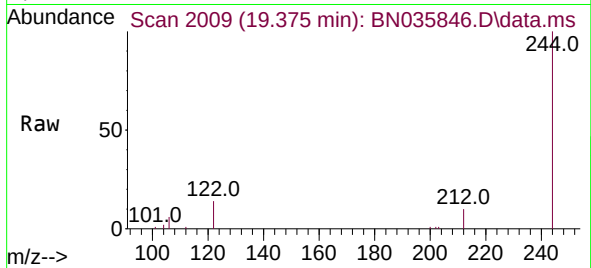

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.027 ng
 RT: 20.893 min Scan# 2244
 Delta R.T. -0.018 min
 Lab File: BN035846.D
 Acq: 26 Dec 2024 10:35


Tgt Ion:149 Resp: 381
 Ion Ratio Lower Upper
 149 100
 167 31.0 22.2 33.4
 279 4.2 2.7 4.1#

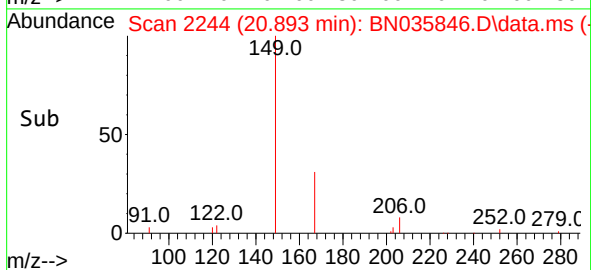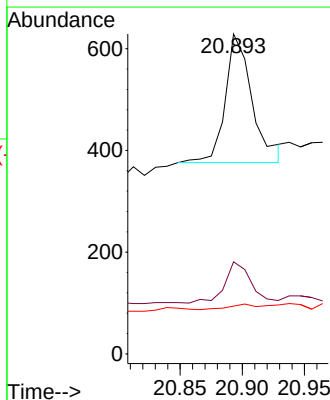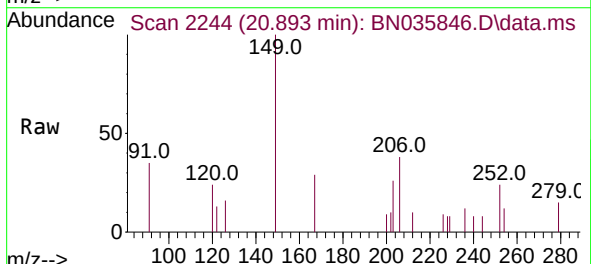

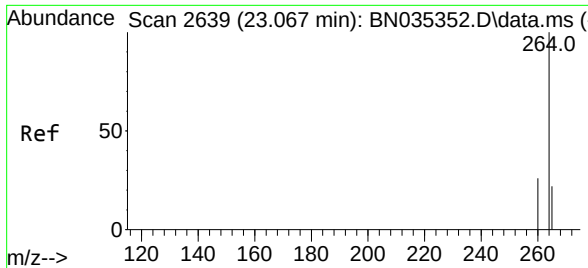

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.029 min Scan# 20
Delta R.T. -0.012 min
Lab File: BN035846.D
Acq: 26 Dec 2024 10:35

Instrument :
BNA_N
ClientSampleId :
PB165724BL

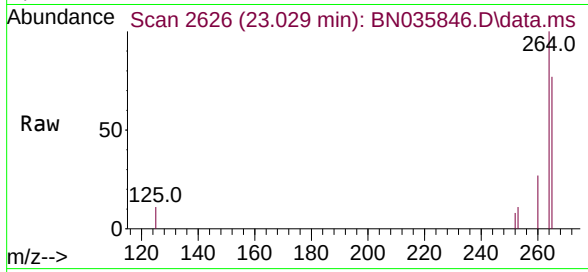

Tgt Ion:264 Resp: 9894

Ion	Ratio	Lower	Upper
264	100		
260	26.8	21.4	32.2
265	77.1	40.2	60.4

