Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121924\
Data File : BN035765.D
Acq On : 21 Dec 2024 05:10
Operator : RC/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

Quant Time: Dec 21 05:39:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 19 23:06:19 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units		Dev(Min)
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.264	152	3545	0.400	ng		0.00
7) Naphthalene-d8	10.009	136	9106	0.400	ng		#-0.01
13) Acenaphthene-d10	13.924	164	5821	0.400	ng		-0.01
19) Phenanthrene-d10	16.698	188	12321	0.400	ng		# 0.00
29) Chrysene-d12	20.947	240	9836	0.400	ng		# 0.00
35) Perylene-d12	23.035	264	10740	0.400	ng		# 0.00
System Monitoring Compounds							
4) 2-Fluorophenol	4.932	112	3403	0.384	ng		0.00
5) Phenol-d6	6.477	99	3879	0.364	ng		-0.01
8) Nitrobenzene-d5	8.408	82	2582m	0.464	ng		0.00
11) 2-Methylnaphthalene-d10	11.616	152	5263	0.369	ng		0.00
14) 2,4,6-Tribromophenol	15.453	330	1253	0.303	ng		0.00
15) 2-Fluorobiphenyl	12.538	172	8084	0.367	ng		0.00
27) Fluoranthene-d10	18.757	212	12191	0.349	ng		0.00
31) Terphenyl-d14	19.388	244	8488	0.437	ng		0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	2.982	88	1555	0.459	ng		96
3) n-Nitrosodimethylamine	3.278	42	1104	0.391	ng	#	93
6) bis(2-Chloroethyl)ether	6.723	93	3165	0.353	ng		98
9) Naphthalene	10.063	128	9097	0.379	ng		100
10) Hexachlorobutadiene	10.351	225	2300	0.415	ng	#	99
12) 2-Methylnaphthalene	11.692	142	6016	0.350	ng		99
16) Acenaphthylene	13.636	152	8764	0.359	ng		99
17) Acenaphthene	13.989	154	6047	0.373	ng		98
18) Fluorene	14.993	166	7942	0.342	ng		100
20) 4,6-Dinitro-2-methylph...	15.132	198	142	0.117	ng	#	1
21) 4-Bromophenyl-phenylether	15.904	248	2531	0.351	ng	#	83
22) Hexachlorobenzene	16.003	284	3667	0.433	ng		97
23) Atrazine	16.202	200	1895	0.369	ng		96
24) Pentachlorophenol	16.376	266	1177	0.320	ng	#	86
25) Phenanthrene	16.735	178	12350	0.365	ng		99
26) Anthracene	16.835	178	10612	0.347	ng		99
28) Fluoranthene	18.789	202	15375	0.337	ng		99
30) Pyrene	19.156	202	15587	0.429	ng		100
32) Benzo(a)anthracene	20.938	228	11659	0.339	ng		100
33) Chrysene	20.991	228	14263	0.402	ng		99
34) Bis(2-ethylhexyl)phtha...	20.902	149	5697	0.419	ng		99
36) Indeno(1,2,3-cd)pyrene	25.064	276	15666	0.373	ng		99
37) Benzo(b)fluoranthene	22.427	252	19003	0.484	ng		98
38) Benzo(k)fluoranthene	22.468	252	15020m	0.388	ng		
39) Benzo(a)pyrene	22.947	252	11742	0.363	ng		94
40) Dibenzo(a,h)anthracene	25.079	278	11661	0.352	ng		97
41) Benzo(g,h,i)perylene	25.675	276	14236	0.411	ng		99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121924\
Data File : BN035765.D
Acq On : 21 Dec 2024 05:10
Operator : RC/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 56 Sample Multiplier: 1

Quant Time: Dec 21 05:39:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 19 23:06:19 2024
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

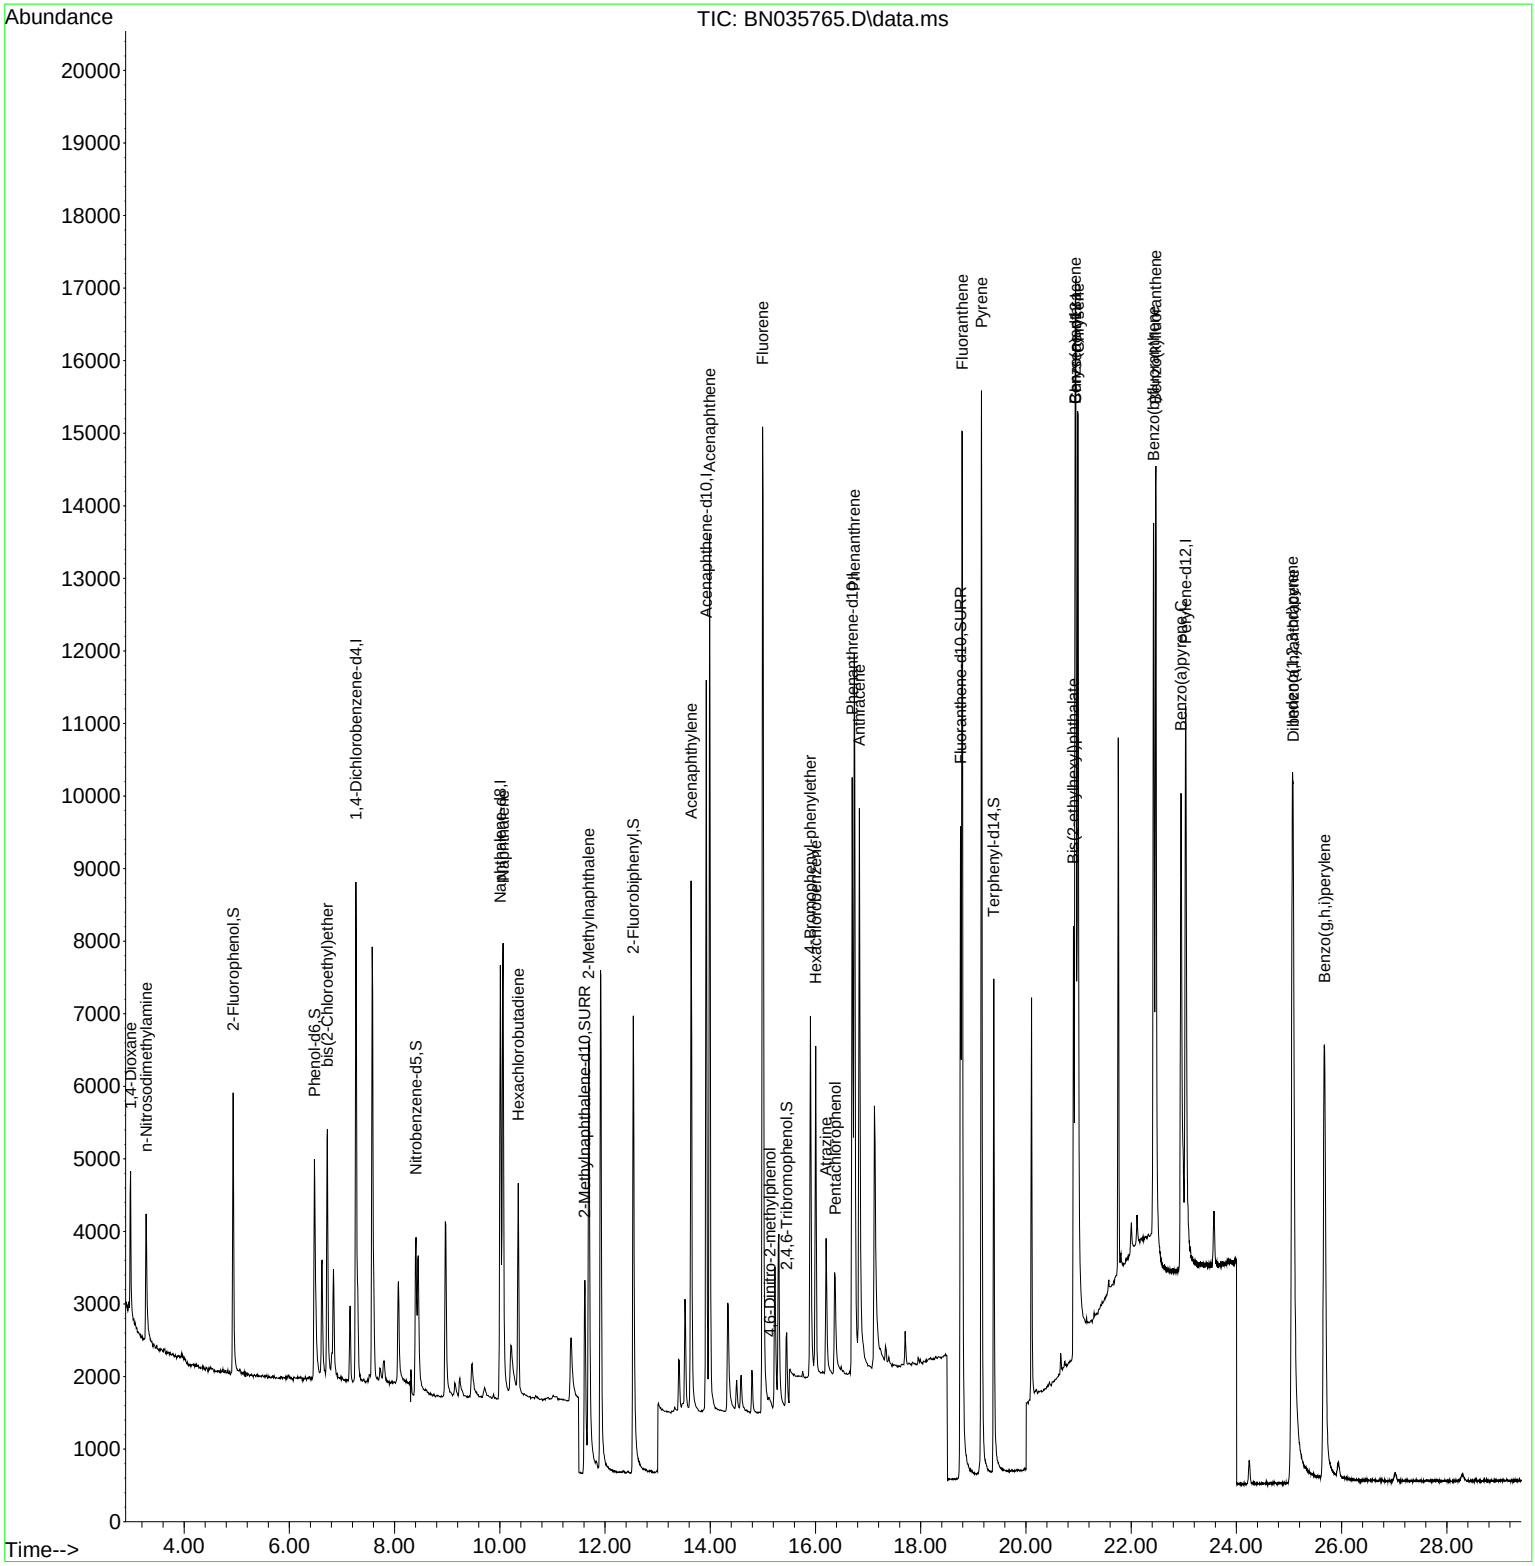

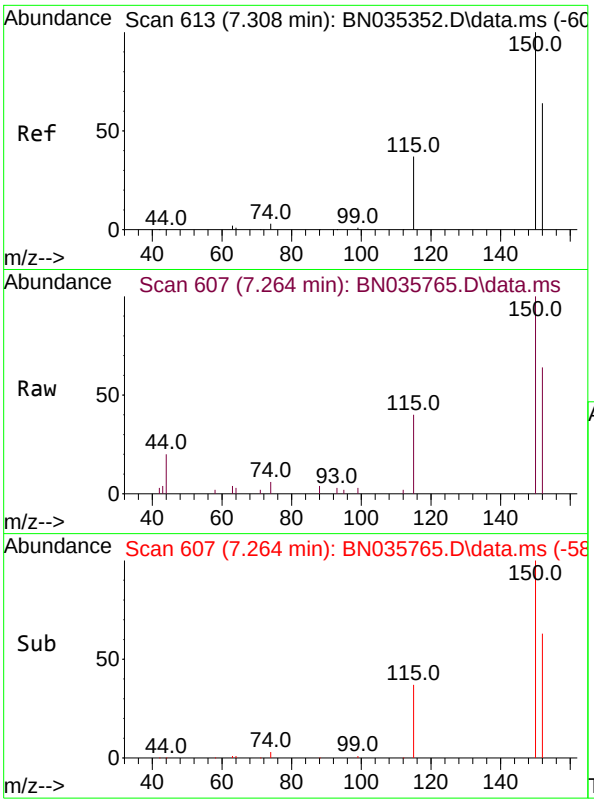

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.264 min Scan# 6(
Delta R.T. -0.008 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:152 Resp: 354

Ion	Ratio	Lower	Upper
152	100		
150	156.6	124.0	186.0
115	63.3	49.6	74.4



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

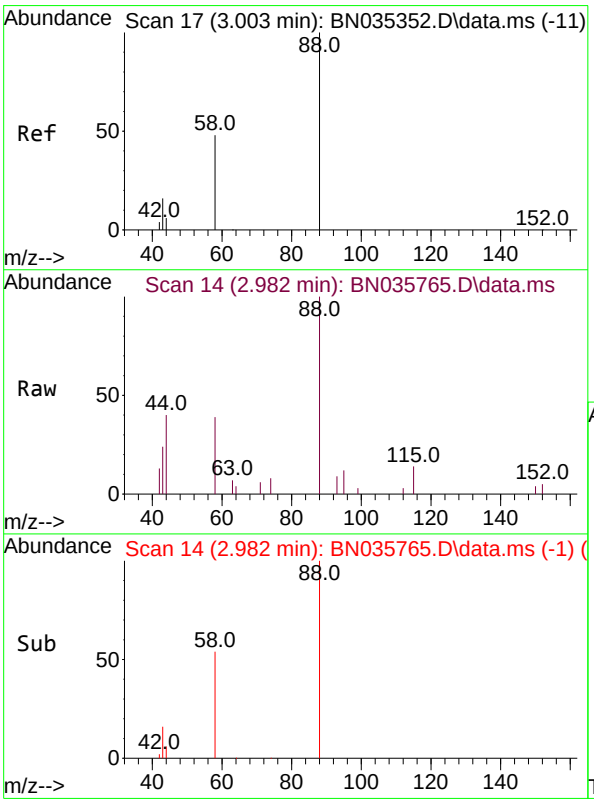

#2
1,4-Dioxane
Concen: 0.459 ng
RT: 2.982 min Scan# 14
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion: 88 Resp: 1555

Ion	Ratio	Lower	Upper
88	100		
43	22.1	17.2	25.8
58	52.2	44.5	66.7



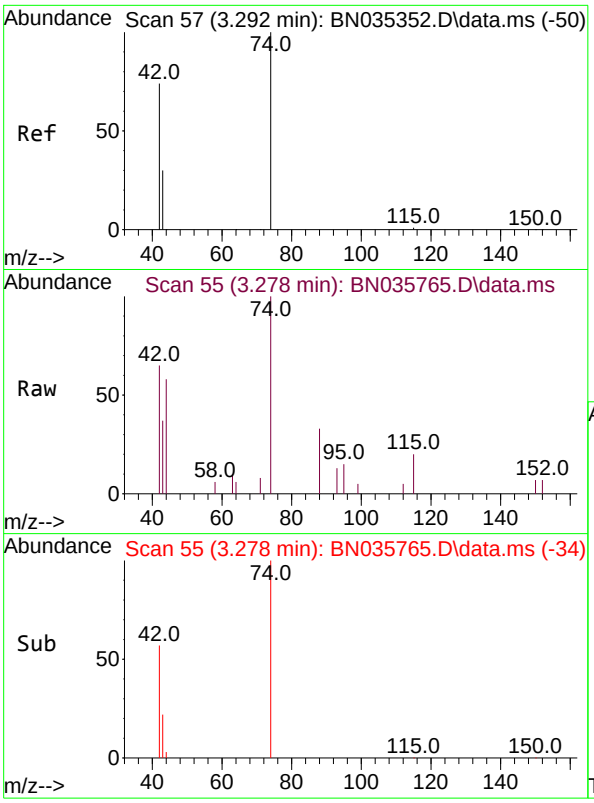

#3
n-Nitrosodimethylamine
Concen: 0.391 ng
RT: 3.278 min Scan# 5
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion: 42 Resp: 110

Ion	Ratio	Lower	Upper
42	100		
74	165.7	124.9	187.3
44	6.3	2.2	3.4

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024



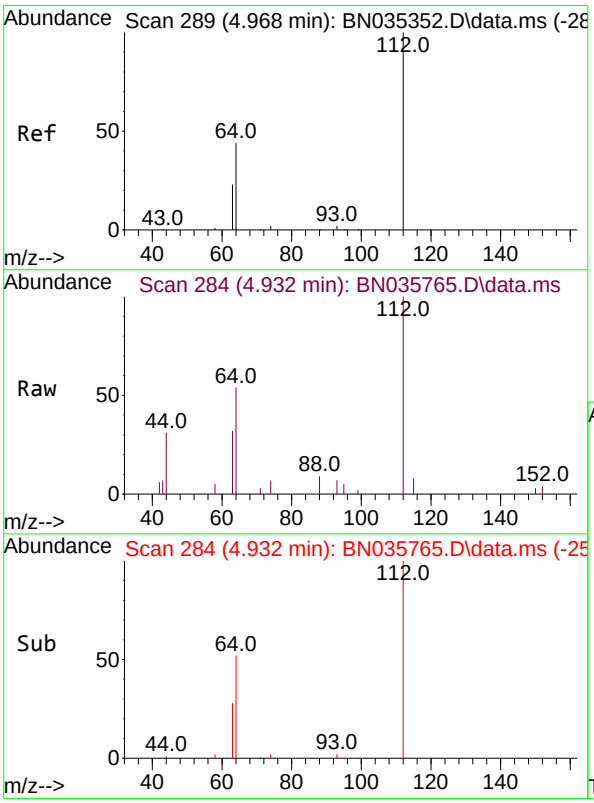

#4
2-Fluorophenol
Concen: 0.384 ng
RT: 4.932 min Scan# 284
Delta R.T. -0.007 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:112 Resp: 3403

Ion	Ratio	Lower	Upper
112	100		
64	51.2	39.8	59.8
63	28.0	21.0	31.6



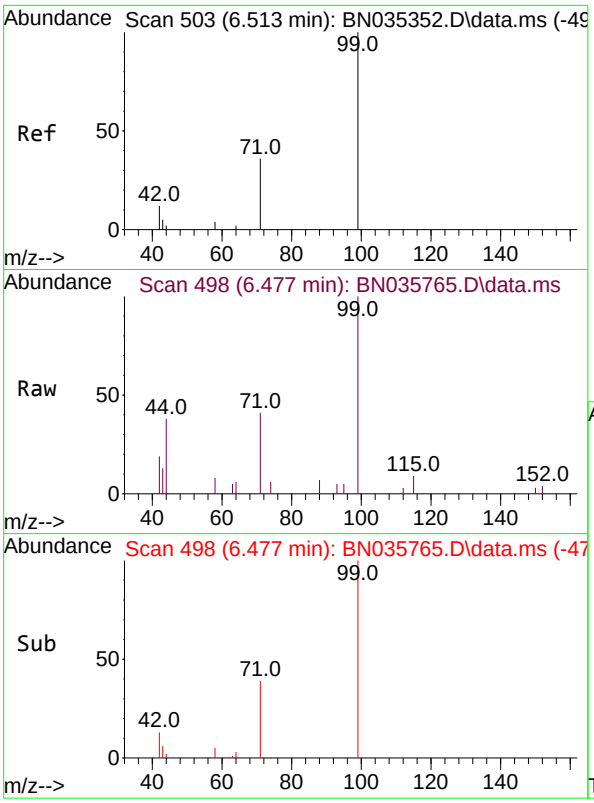

#5
Phenol-d6
Concen: 0.364 ng
RT: 6.477 min Scan# 4
Delta R.T. -0.015 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion: 99 Resp: 387

Ion	Ratio	Lower	Upper
99	100		
42	14.6	11.4	17.2
71	35.9	29.3	43.9



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

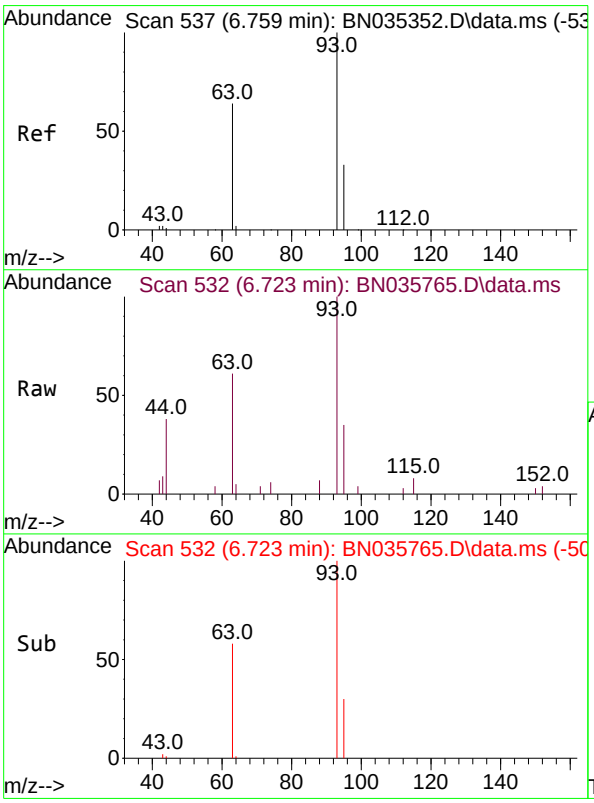

#6
bis(2-Chloroethyl)ether
Concen: 0.353 ng
RT: 6.723 min Scan# 532
Delta R.T. -0.007 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion: 93 Resp: 3165

Ion	Ratio	Lower	Upper
93	100		
63	61.5	50.4	75.6
95	30.6	25.7	38.5



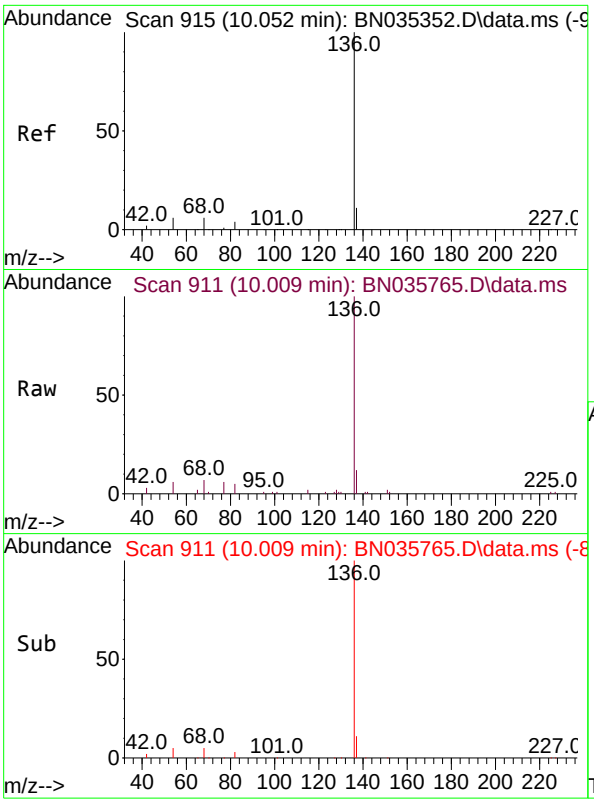

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.009 min Scan# 9
Delta R.T. -0.011 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:136 Resp: 910

Ion	Ratio	Lower	Upper
136	100		
137	11.8	10.2	15.2
54	5.8	6.1	9.1
68	6.6	6.4	9.6



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

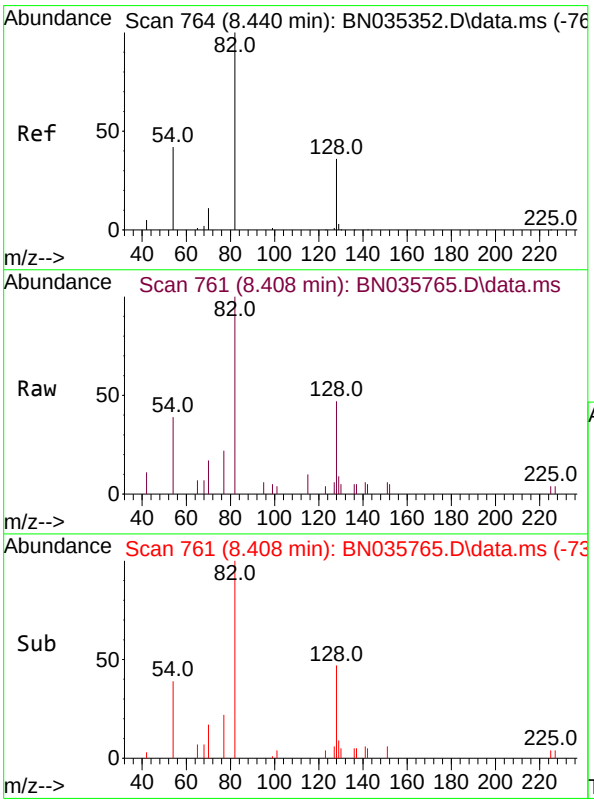

#8
Nitrobenzene-d5
Concen: 0.464 ng m
RT: 8.408 min Scan# 761
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion: 82 Resp: 2582

Ion	Ratio	Lower	Upper
82	100		
128	46.7	33.4	50.0
54	39.0	36.7	55.1



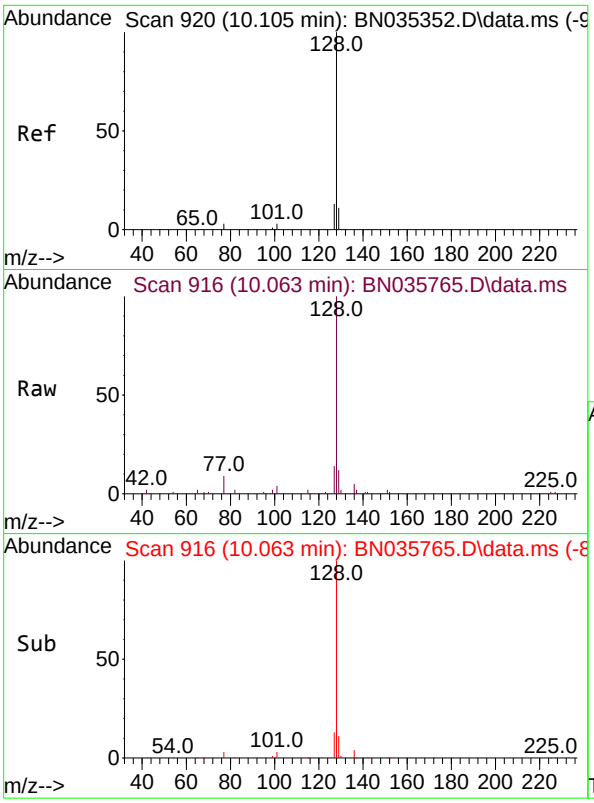

#9
Naphthalene
Concen: 0.379 ng
RT: 10.063 min Scan# 9
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:128 Resp: 909

Ion	Ratio	Lower	Upper
128	100		
129	12.2	9.8	14.6
127	14.3	11.4	17.2



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

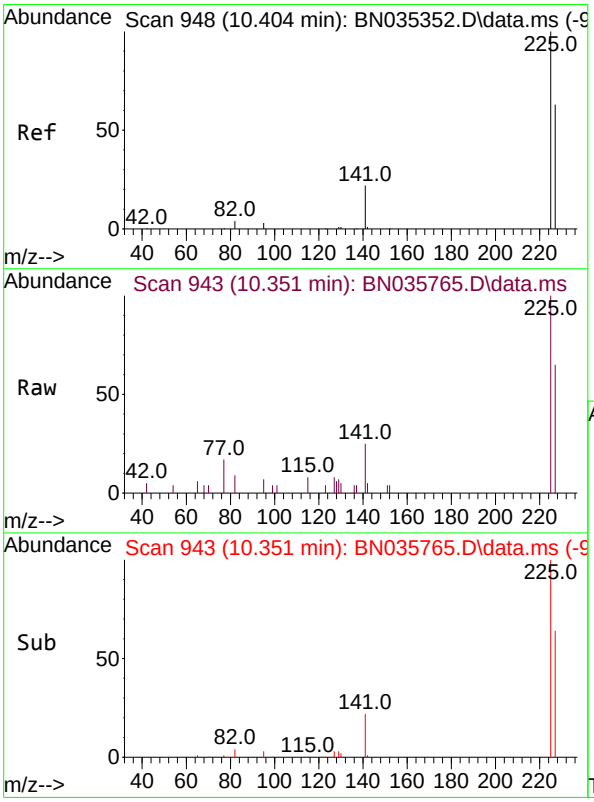

#10
Hexachlorobutadiene
Concen: 0.415 ng
RT: 10.351 min Scan# 943
Delta R.T. -0.011 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:225 Resp: 2300

Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	65.0	51.3	76.9



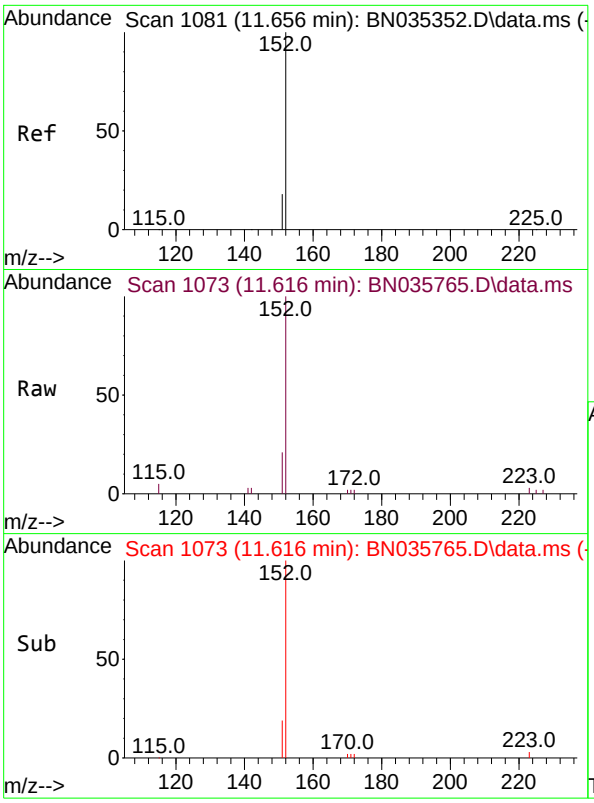

#11
2-Methylnaphthalene-d10
Concen: 0.369 ng
RT: 11.616 min Scan# 1
Delta R.T. -0.005 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:152 Resp: 526

Ion	Ratio	Lower	Upper
152	100		
151	19.7	16.6	25.0

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024



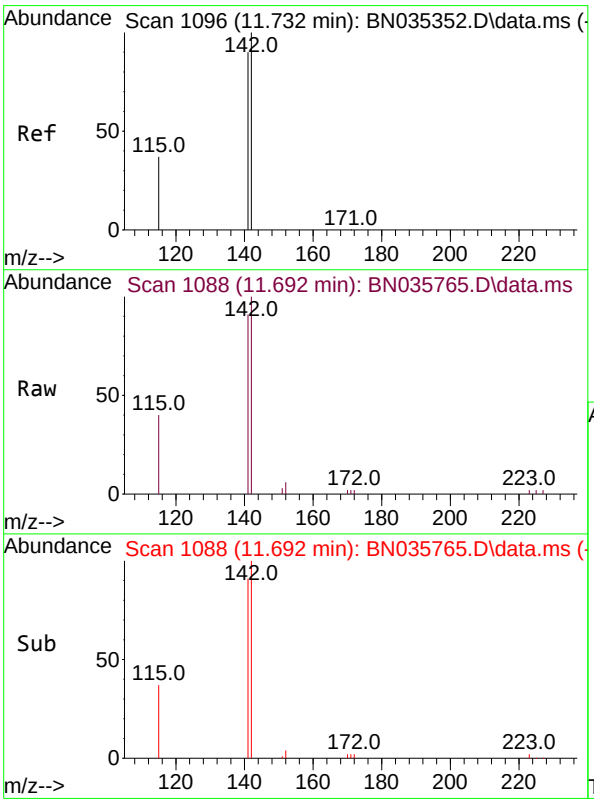

#12
2-Methylnaphthalene
Concen: 0.350 ng
RT: 11.692 min Scan# 1088
Delta R.T. -0.005 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:142 Resp: 6016

Ion	Ratio	Lower	Upper
142	100		
141	90.5	72.2	108.4
115	39.9	31.4	47.0



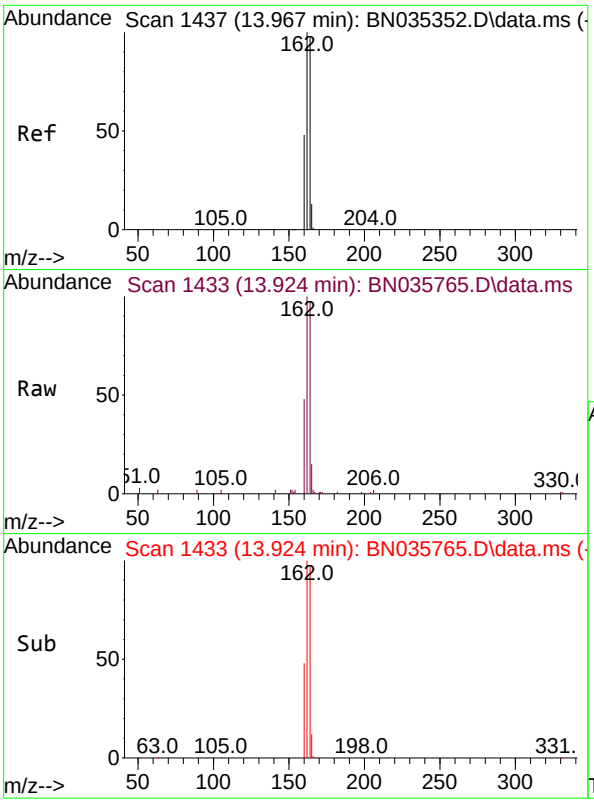

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 13.924 min Scan# 14
Delta R.T. -0.011 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:164 Resp: 582

Ion	Ratio	Lower	Upper
164	100		
162	103.2	82.2	123.2
160	49.6	40.1	60.1



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

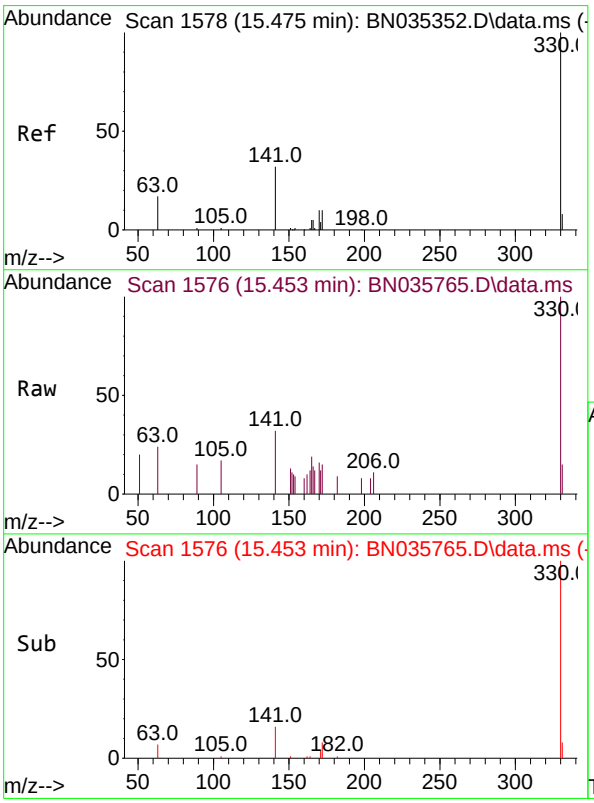

#14
2,4,6-Tribromophenol
Concen: 0.303 ng
RT: 15.453 min Scan# 1576
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:330 Resp: 1253

Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	29.6	26.6	40.0



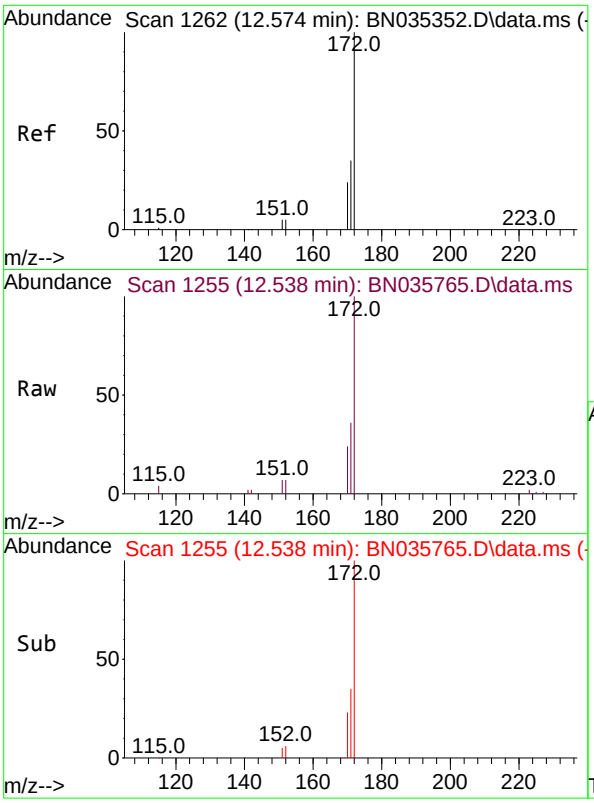

#15
2-Fluorobiphenyl
Concen: 0.367 ng
RT: 12.538 min Scan# 1
Delta R.T. -0.005 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:172 Resp: 808

Ion	Ratio	Lower	Upper
172	100		
171	36.1	29.0	43.4
170	24.5	19.8	29.8



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

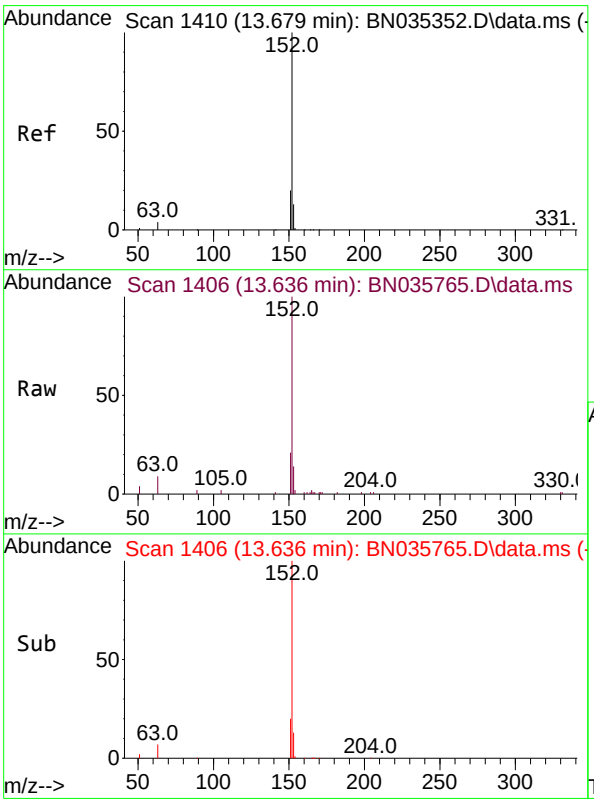

#16
Acenaphthylene
Concen: 0.359 ng
RT: 13.636 min Scan# 1406
Delta R.T. -0.011 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:152 Resp: 8764

Ion	Ratio	Lower	Upper
152	100		
151	19.7	16.2	24.2
153	13.0	10.4	15.6



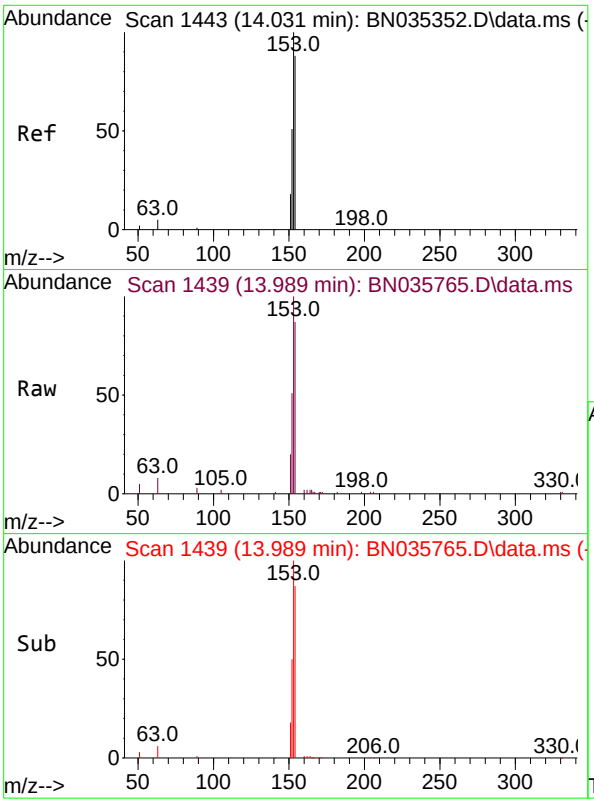

#17
Acenaphthene
Concen: 0.373 ng
RT: 13.989 min Scan# 14
Delta R.T. -0.011 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:154 Resp: 604

Ion	Ratio	Lower	Upper
154	100		
153	114.7	92.6	139.0
152	58.8	49.0	73.6



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

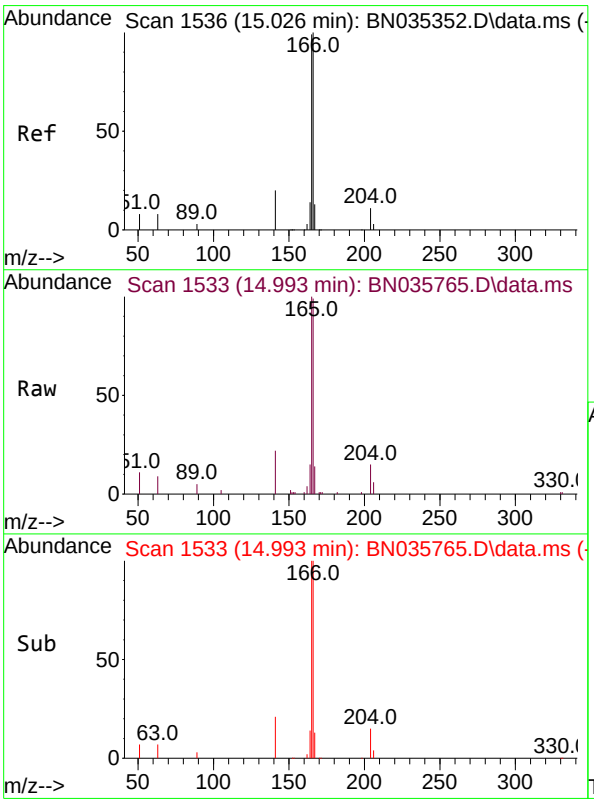

#18
Fluorene
Concen: 0.342 ng
RT: 14.993 min Scan# 1533
Delta R.T. -0.011 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:166 Resp: 7942

Ion	Ratio	Lower	Upper
166	100		
165	99.1	79.7	119.5
167	13.6	10.8	16.2



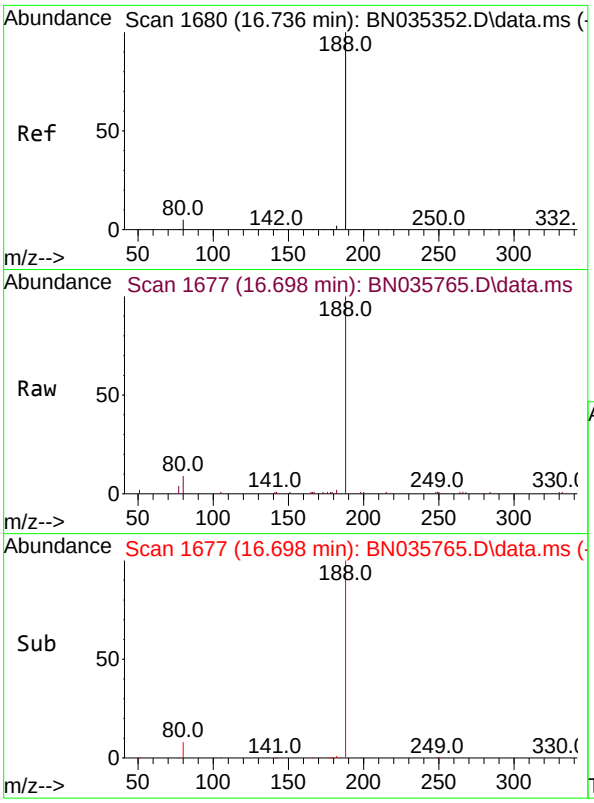

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.698 min Scan# 1(
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:188 Resp: 1232

Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	8.9	4.6	6.8#



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

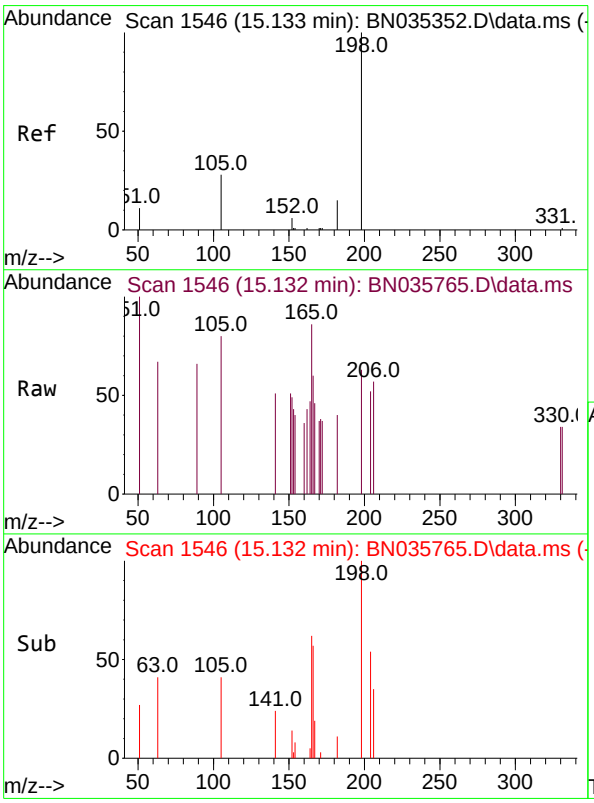

#20
4,6-Dinitro-2-methylphenol
Concen: 0.117 ng
RT: 15.132 min Scan# 1546
Delta R.T. 0.011 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:198 Resp: 142

Ion	Ratio	Lower	Upper
198	100		
51	157.6	46.5	69.7#
105	125.9	45.3	67.9#



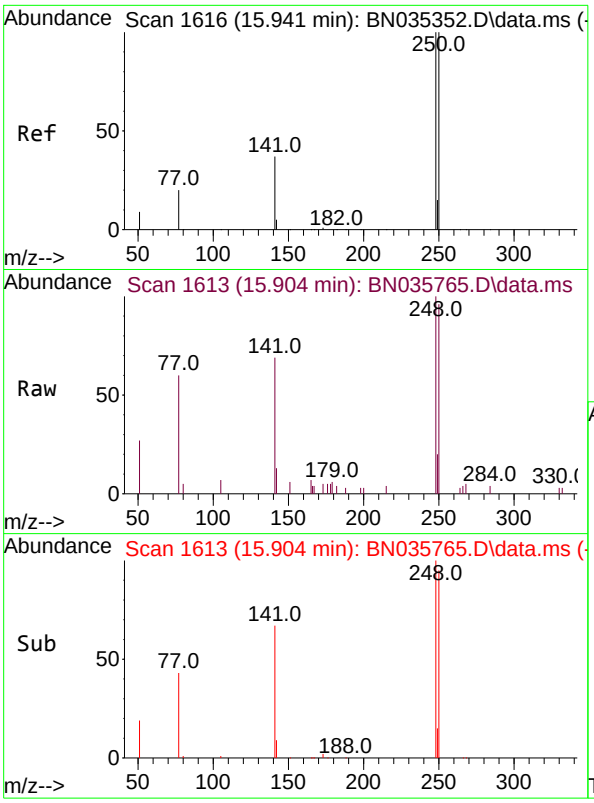

#21
4-Bromophenyl-phenylether
Concen: 0.351 ng
RT: 15.904 min Scan# 1(
Delta R.T. -0.013 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:248 Resp: 253

Ion	Ratio	Lower	Upper
248	100		
250	96.2	80.6	120.8
141	69.2	31.5	47.3#

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024



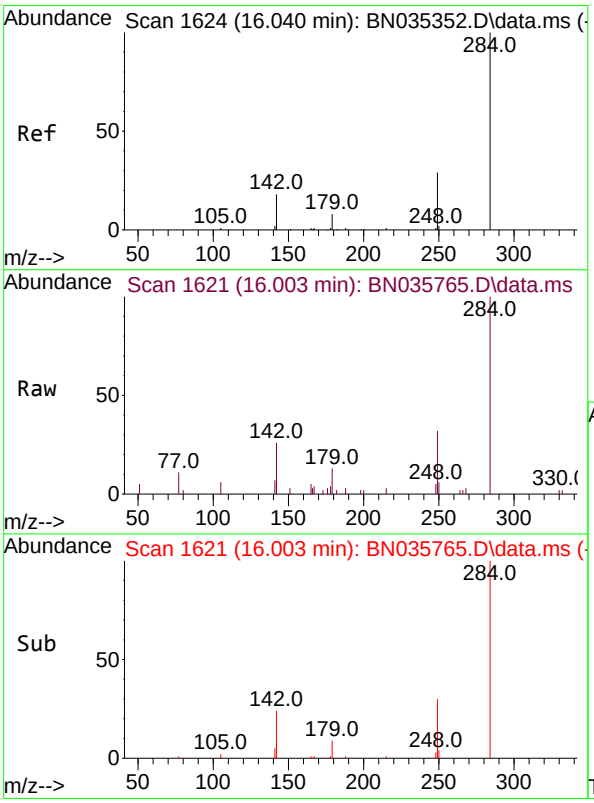

#22
Hexachlorobenzene
Concen: 0.433 ng
RT: 16.003 min Scan# 1621
Delta R.T. -0.013 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:284 Resp: 3667

Ion	Ratio	Lower	Upper
284	100		
142	30.7	26.7	40.1
249	29.9	24.6	36.8



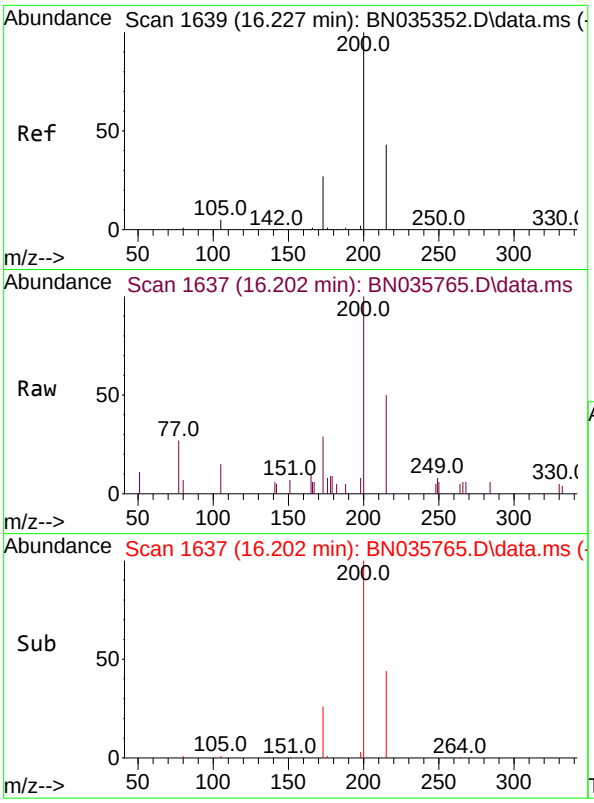

#23
Atrazine
Concen: 0.369 ng
RT: 16.202 min Scan# 1(
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:200 Resp: 189

Ion	Ratio	Lower	Upper
200	100		
173	29.4	24.1	36.1
215	49.7	36.9	55.3



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

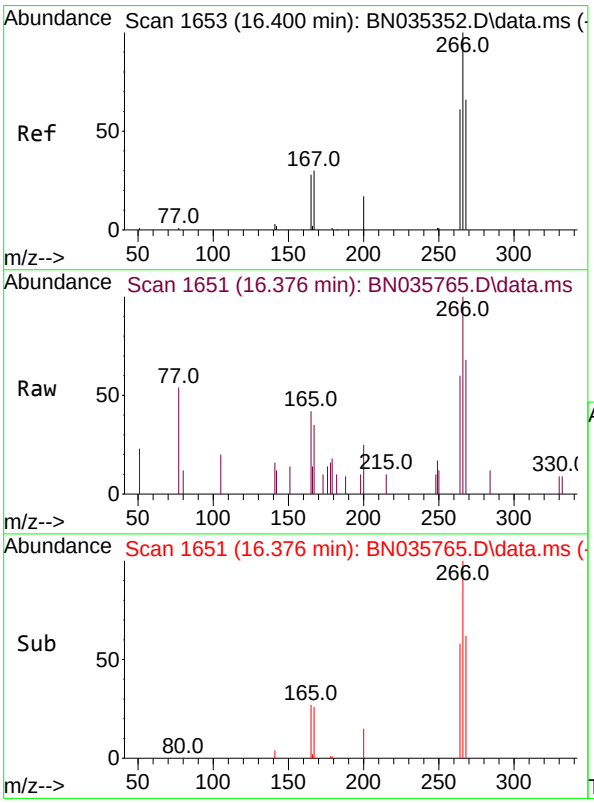

#24
Pentachlorophenol
Concen: 0.320 ng
RT: 16.376 min Scan# 1651
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:266 Resp: 1177

Ion	Ratio	Lower	Upper
266	100		
264	59.3	42.3	63.5
268	67.2	43.3	64.9#



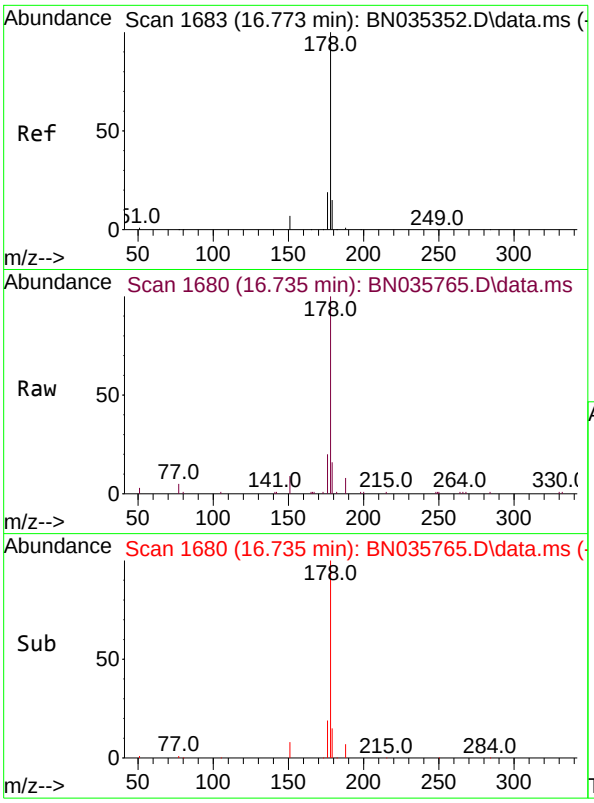

#25
Phenanthrene
Concen: 0.365 ng
RT: 16.735 min Scan# 1(
Delta R.T. -0.013 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:178 Resp: 1235(

Ion	Ratio	Lower	Upper
178	100		
176	18.8	15.4	23.2
179	15.4	12.3	18.5



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

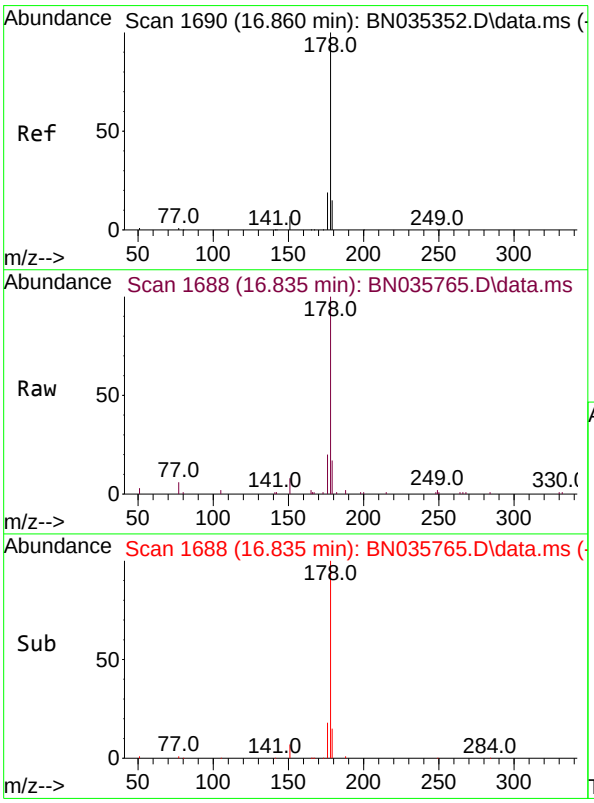

#26
Anthracene
Concen: 0.347 ng
RT: 16.835 min Scan# 1688
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:178 Resp: 10612

Ion	Ratio	Lower	Upper
178	100		
176	18.5	15.0	22.6
179	15.2	12.6	18.8



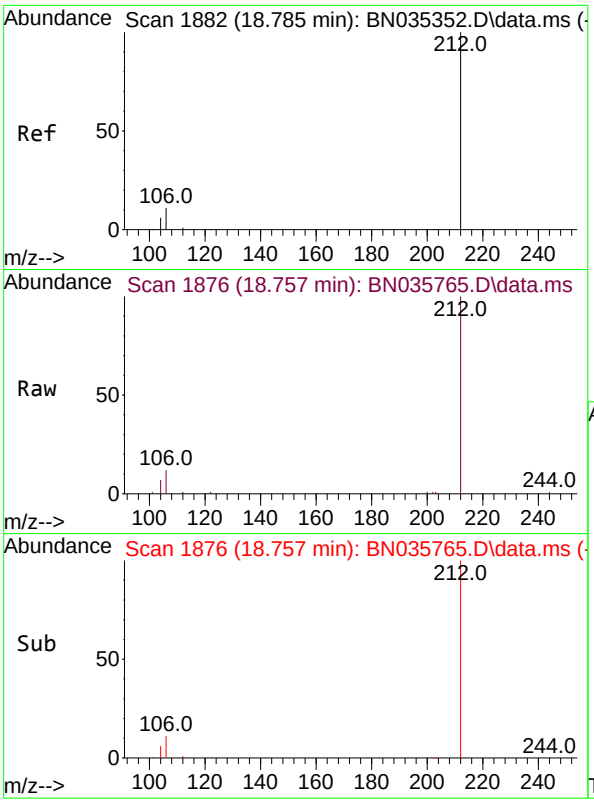

#27
Fluoranthene-d10
Concen: 0.349 ng
RT: 18.757 min Scan# 1
Delta R.T. -0.005 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:212 Resp: 1219

Ion	Ratio	Lower	Upper
212	100		
106	11.4	9.2	13.8
104	6.5	5.3	7.9



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

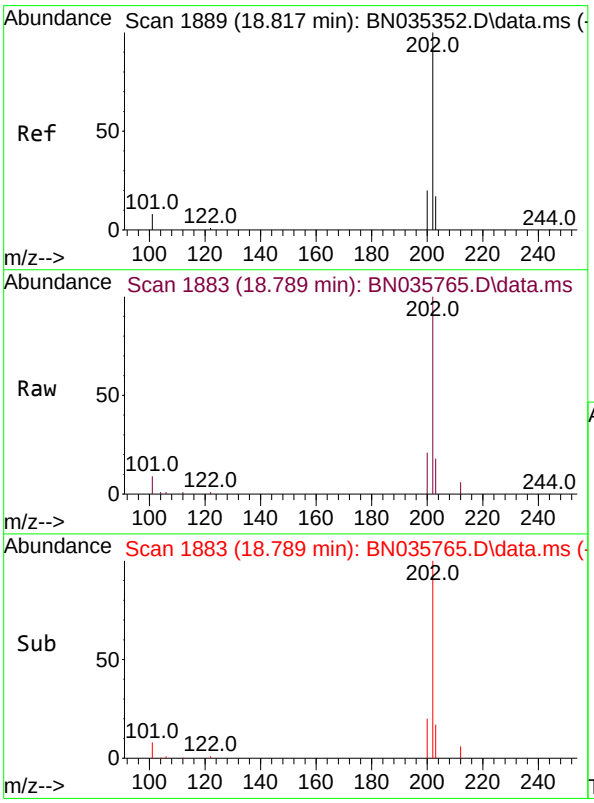

#28
Fluoranthene
Concen: 0.337 ng
RT: 18.789 min Scan# 1883
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:202 Resp: 15375

Ion	Ratio	Lower	Upper
202	100		
101	9.2	7.4	11.0
203	16.8	13.7	20.5



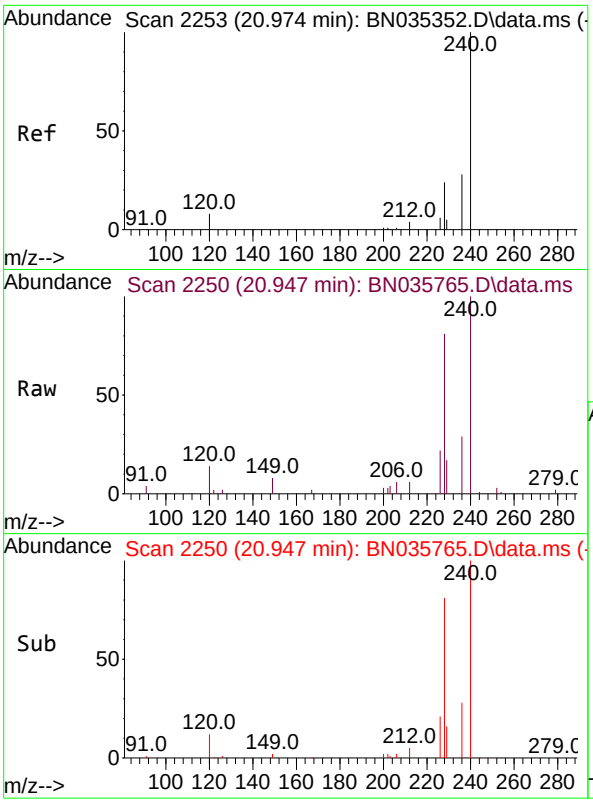

#29
Chrysene-d12
Concen: 0.400 ng
RT: 20.947 min Scan# 2
Delta R.T. -0.009 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:240 Resp: 983

Ion	Ratio	Lower	Upper
240	100		
120	14.2	7.9	11.9
236	29.4	22.9	34.3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024



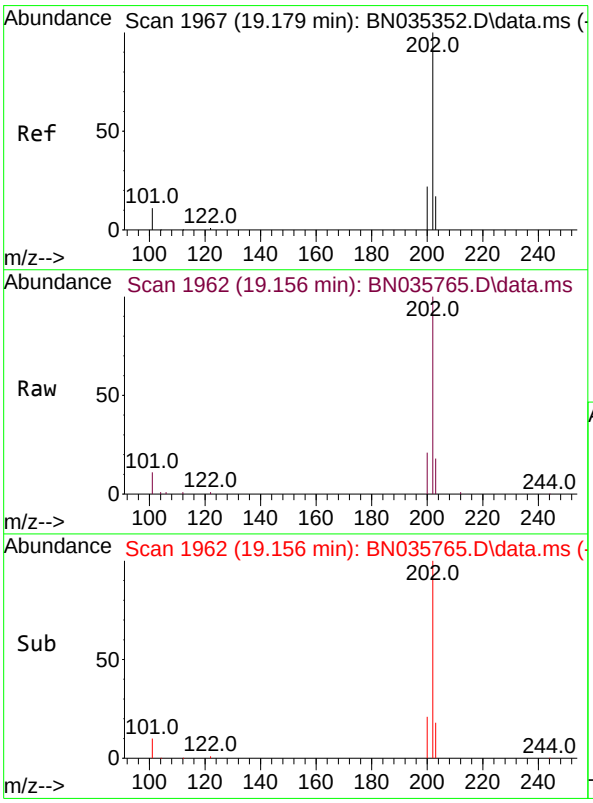

#30
Pyrene
Concen: 0.429 ng
RT: 19.156 min Scan# 1962
Delta R.T. -0.005 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:202 Resp: 15587

Ion	Ratio	Lower	Upper
202	100		
200	21.1	17.0	25.4
203	18.0	14.3	21.5



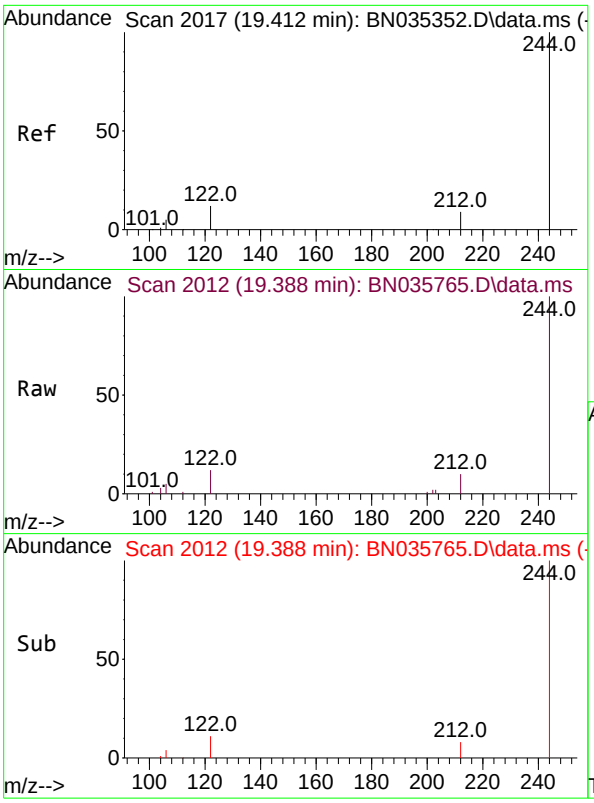

#31
Terphenyl-d14
Concen: 0.437 ng
RT: 19.388 min Scan# 2
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:244 Resp: 848

Ion	Ratio	Lower	Upper
244	100		
212	9.6	8.1	12.1
122	12.1	10.3	15.5



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

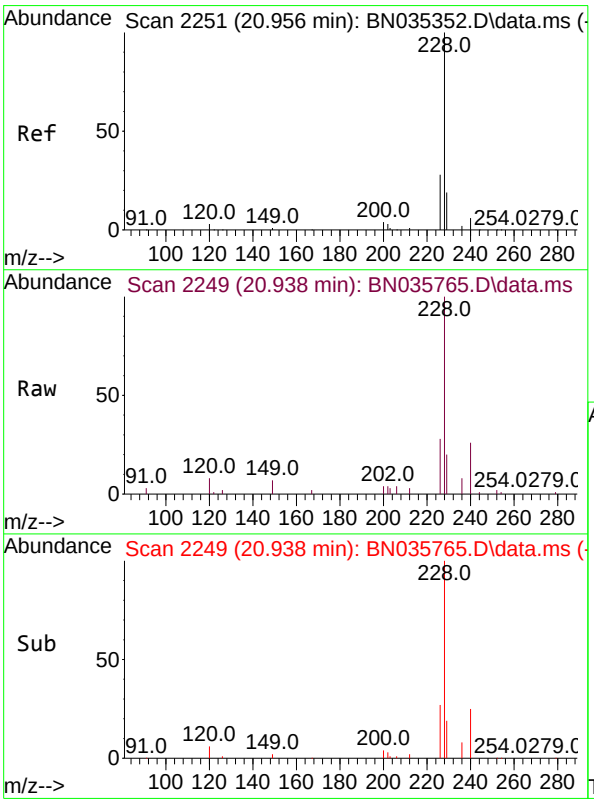

#32
Benzo(a)anthracene
Concen: 0.339 ng
RT: 20.938 min Scan# 2249
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:228 Resp: 11659

Ion	Ratio	Lower	Upper
228	100		
226	27.9	22.5	33.7
229	19.8	15.8	23.8



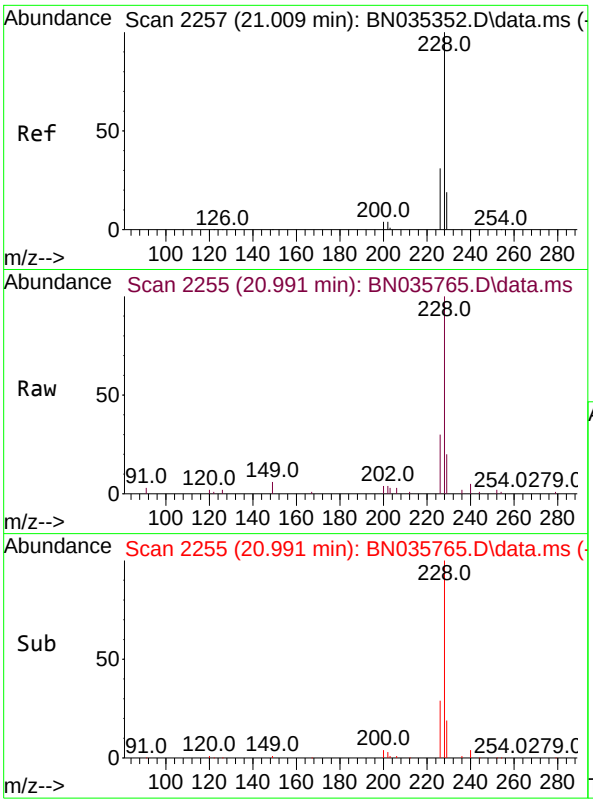

#33
Chrysene
Concen: 0.402 ng
RT: 20.991 min Scan# 2
Delta R.T. -0.000 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:228 Resp: 1426

Ion	Ratio	Lower	Upper
228	100		
226	29.6	24.6	37.0
229	20.0	15.9	23.9



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

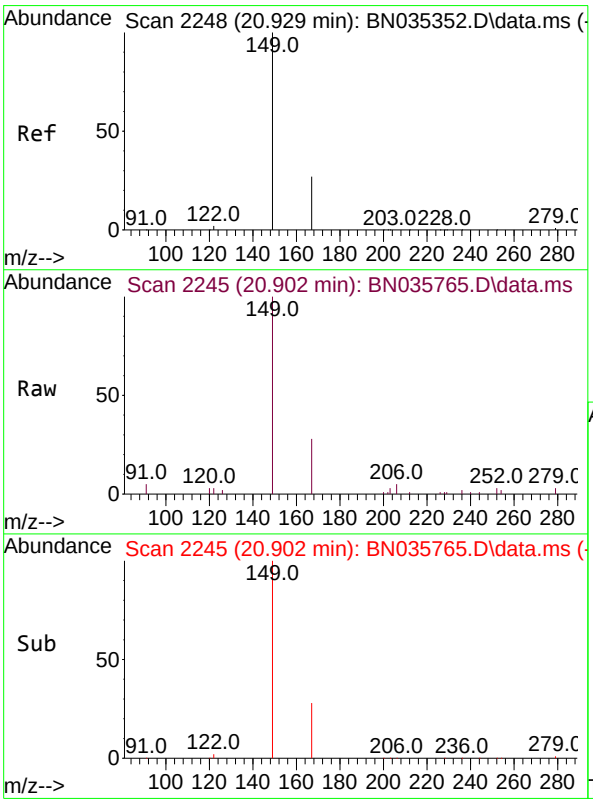

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.419 ng
RT: 20.902 min Scan# 2245
Delta R.T. -0.009 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:149 Resp: 5697

Ion	Ratio	Lower	Upper
149	100		
167	28.5	22.2	33.4
279	3.9	2.7	4.1



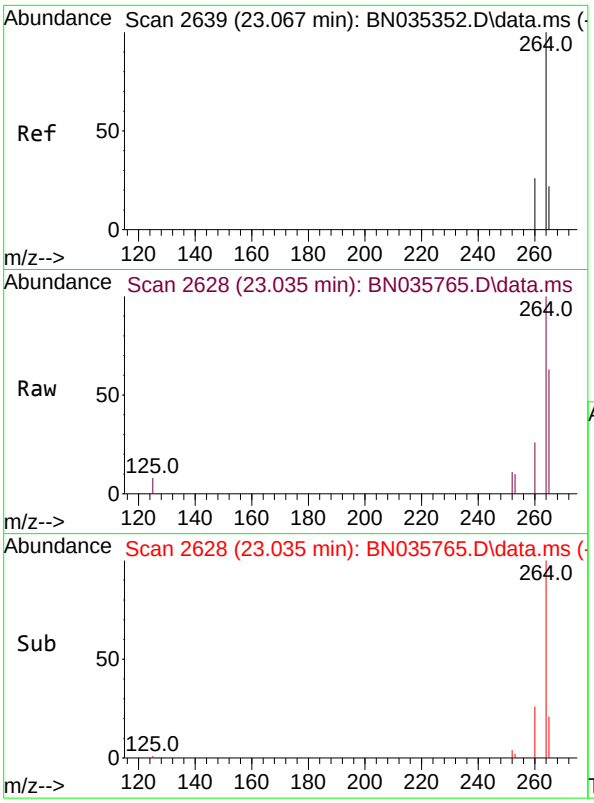

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.035 min Scan# 2
Delta R.T. -0.006 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:264 Resp: 1074

Ion	Ratio	Lower	Upper
264	100		
260	26.2	21.4	32.2
265	63.0	40.2	60.4



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

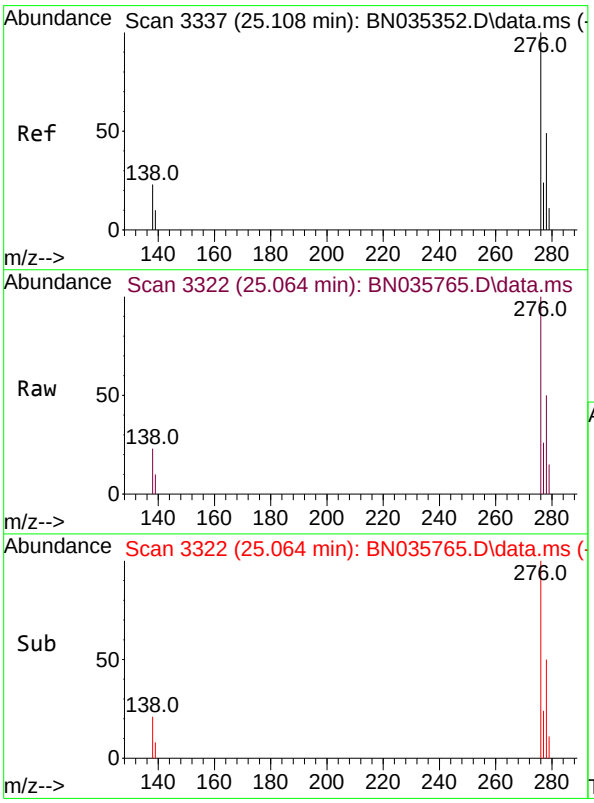

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.373 ng
RT: 25.064 min Scan# 3322
Delta R.T. -0.003 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:276 Resp: 15666

Ion	Ratio	Lower	Upper
276	100		
138	22.9	19.4	29.0
277	24.7	19.8	29.6



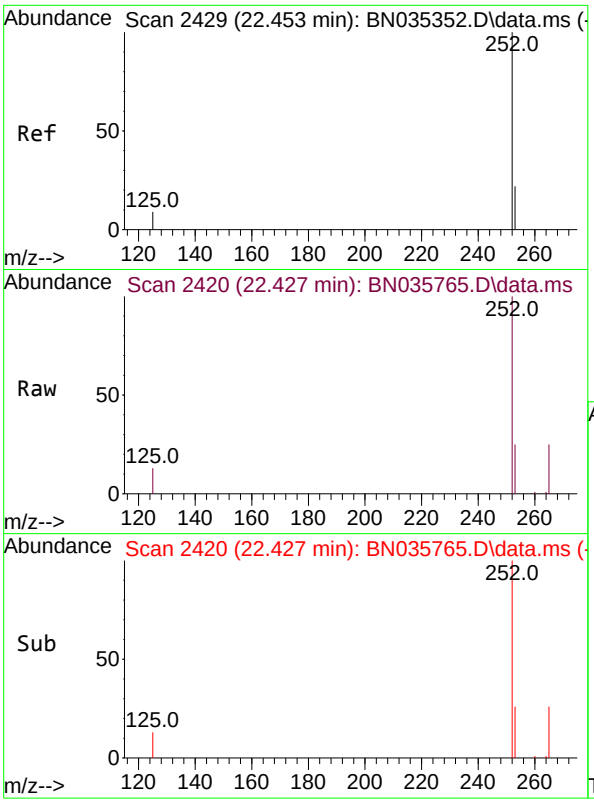

#37
Benzo(b)fluoranthene
Concen: 0.484 ng
RT: 22.427 min Scan# 24
Delta R.T. -0.003 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:252 Resp: 1900

Ion	Ratio	Lower	Upper
252	100		
253	25.5	19.6	29.4
125	12.7	9.6	14.4

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024



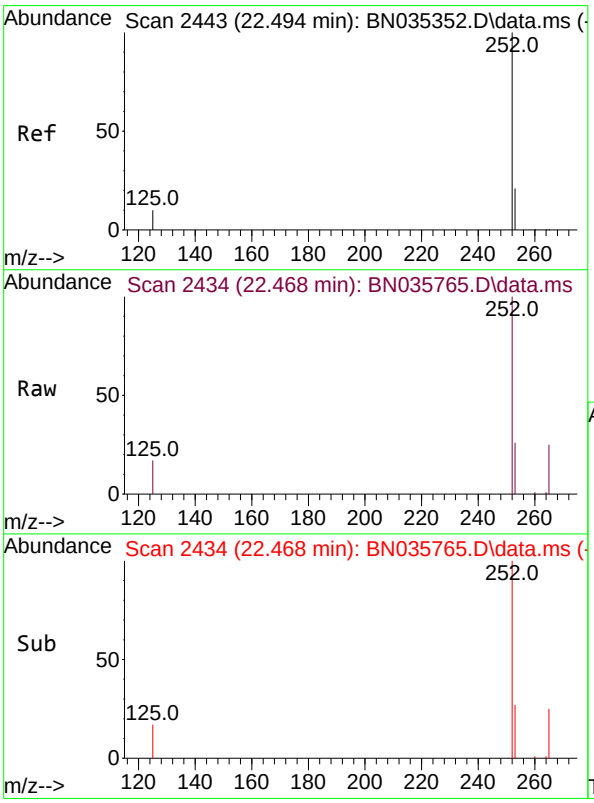

#38
Benzo(k)fluoranthene
Concen: 0.388 ng m
RT: 22.468 min Scan# 2434
Delta R.T. -0.003 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:252 Resp: 15020

Ion	Ratio	Lower	Upper
252	100		
253	26.3	19.5	29.3
125	16.6	10.2	15.4#



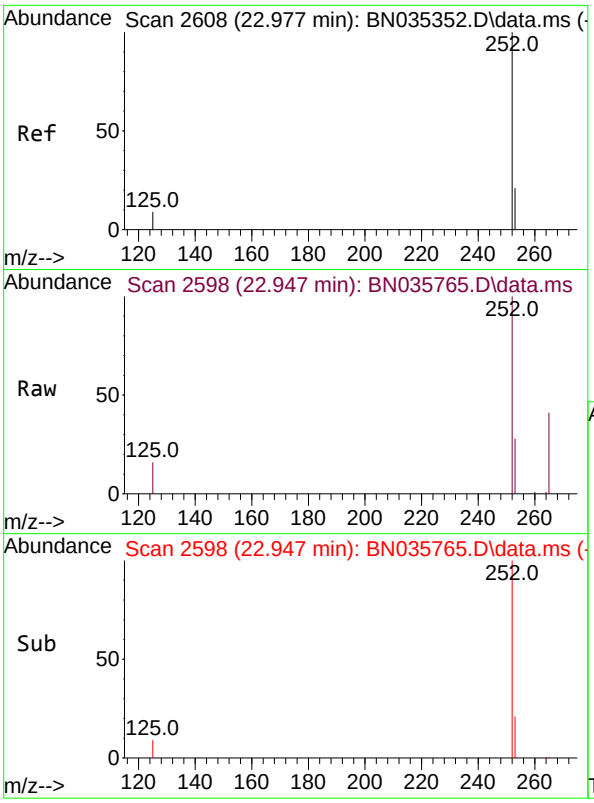

#39
Benzo(a)pyrene
Concen: 0.363 ng
RT: 22.947 min Scan# 2
Delta R.T. -0.003 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:252 Resp: 1174

Ion	Ratio	Lower	Upper
252	100		
253	27.9	20.2	30.4
125	16.1	10.9	16.3



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024

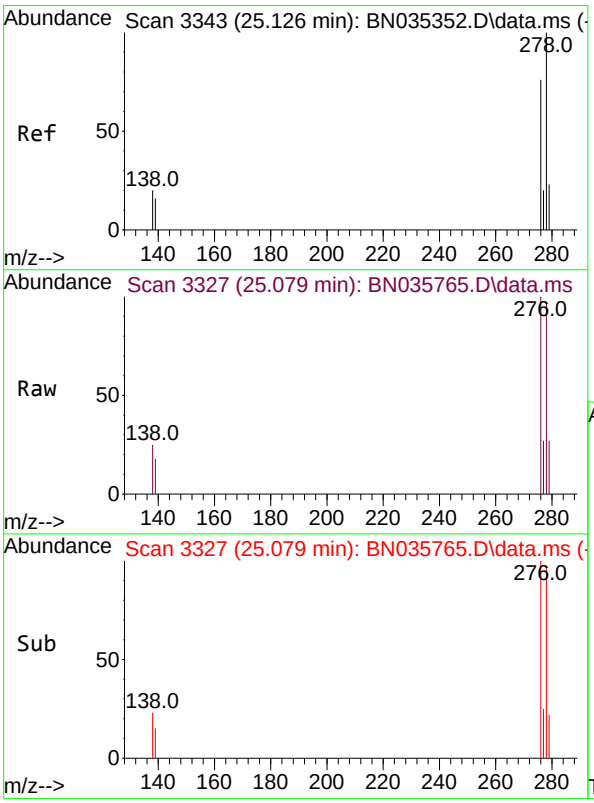

#40
Dibenzo(a,h)anthracene
Concen: 0.352 ng
RT: 25.079 min Scan# 3327
Delta R.T. -0.003 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:278 Resp: 11661

Ion	Ratio	Lower	Upper
278	100		
139	18.3	14.2	21.4
279	27.7	20.5	30.7



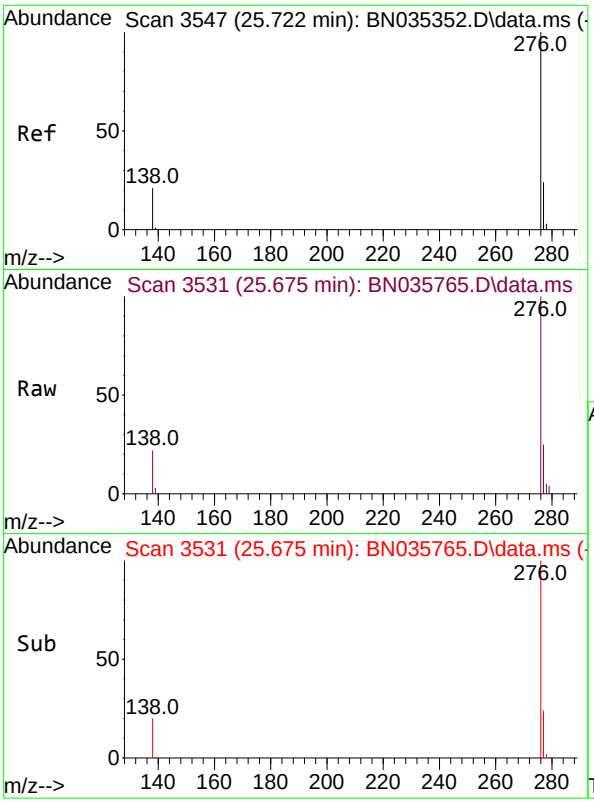

#41
Benzo(g,h,i)perylene
Concen: 0.411 ng
RT: 25.675 min Scan# 3
Delta R.T. -0.003 min
Lab File: BN035765.D
Acq: 21 Dec 2024 05:10

Tgt Ion:276 Resp: 1423

Ion	Ratio	Lower	Upper
276	100		
277	25.2	19.9	29.9
138	21.5	17.8	26.8



Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/23/2024
Supervised By :mohammad ahmed 12/24/2024