

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
 Data File : BN035781.D
 Acq On : 23 Dec 2024 13:19
 Operator : RC/JU
 Sample : P5317-17
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DUP-06-20241217

Quant Time: Dec 23 13:56:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 23:06:19 2024
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/24/2024
 Supervised By :mohammad ahmed 12/26/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.264	152	3246	0.400	ng	0.00
7) Naphthalene-d8	10.009	136	8200	0.400	ng	-0.01
13) Acenaphthene-d10	13.924	164	4641	0.400	ng	-0.01
19) Phenanthrene-d10	16.698	188	9144	0.400	ng	# 0.00
29) Chrysene-d12	20.947	240	7343	0.400	ng	# 0.00
35) Perylene-d12	23.029	264	7454	0.400	ng	#-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	4.932	112	1082	0.133	ng	0.00
5) Phenol-d6	6.484	99	575	0.059	ng	0.00
8) Nitrobenzene-d5	8.408	82	2186m	0.436	ng	0.00
11) 2-Methylnaphthalene-d10	11.610	152	5355	0.417	ng	-0.01
14) 2,4,6-Tribromophenol	15.453	330	733	0.222	ng	0.00
15) 2-Fluorobiphenyl	12.533	172	7800	0.445	ng	-0.01
27) Fluoranthene-d10	18.752	212	12266	0.473	ng	0.00
31) Terphenyl-d14	19.379	244	9828	0.678	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	2.982	88	1543	0.497	ng	99
34) Bis(2-ethylhexyl)phtha...	20.902	149	780	0.077	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122324\
Data File : BN035781.D
Acq On : 23 Dec 2024 13:19
Operator : RC/JU
Sample : P5317-17
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DUP-06-20241217

Quant Time: Dec 23 13:56:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 19 23:06:19 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

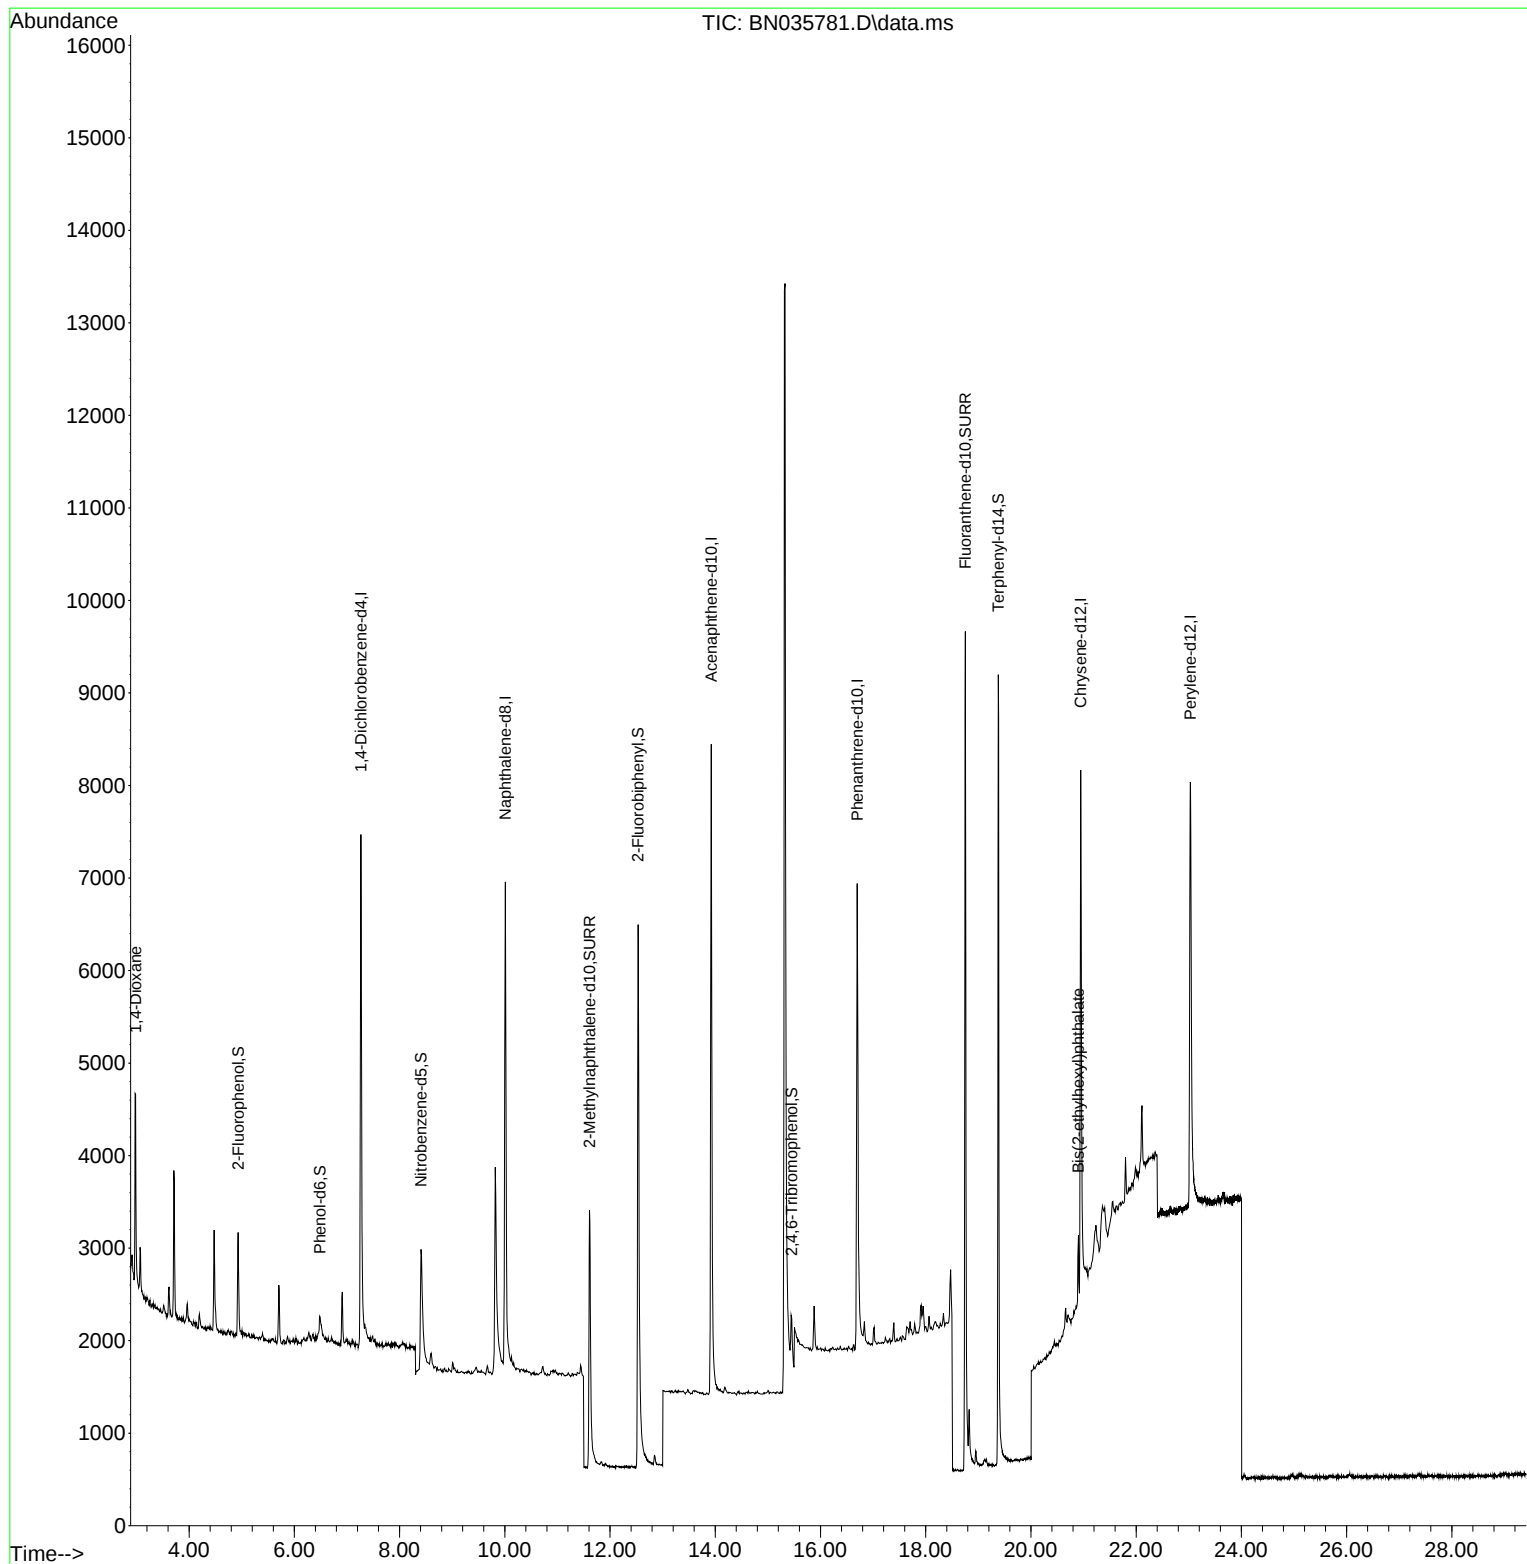



#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.264 min Scan# 607
Delta R.T. -0.008 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19




Instrument :
BNA_N
ClientSampleId :
DUP-06-20241217

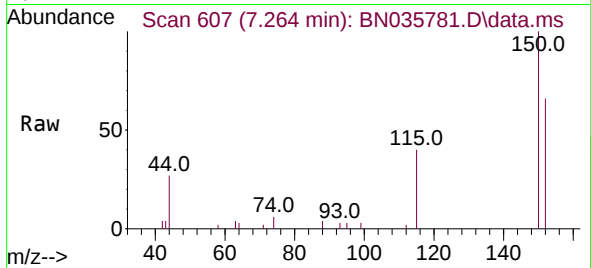

Tgt Ion: 152 Resp: 3240
Ion Ratio Lower Upper
152 100
150 151.7 124.0 186.0
115 60.6 49.6 74.4




Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

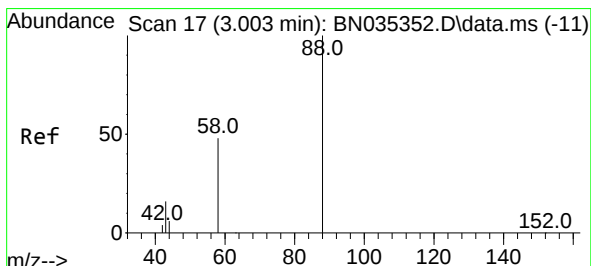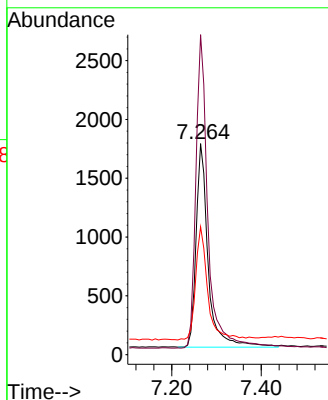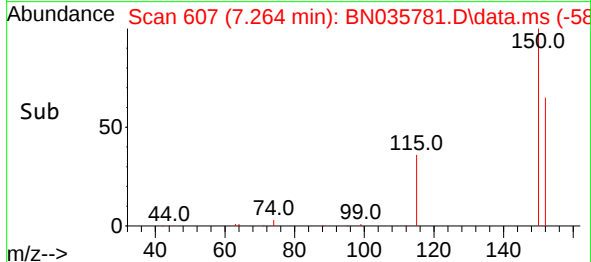

#2
1,4-Dioxane
Concen: 0.497 ng
RT: 2.982 min Scan# 14
Delta R.T. -0.000 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19

Tgt Ion: 88 Resp: 1543
Ion Ratio Lower Upper
88 100
43 22.4 17.2 25.8
58 55.3 44.5 66.7

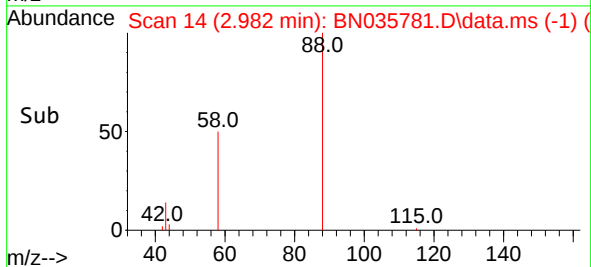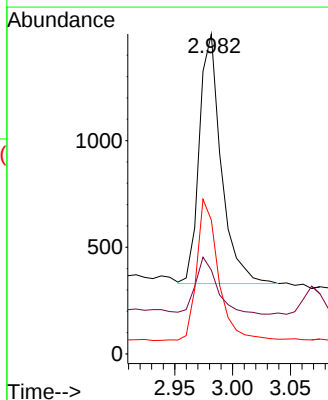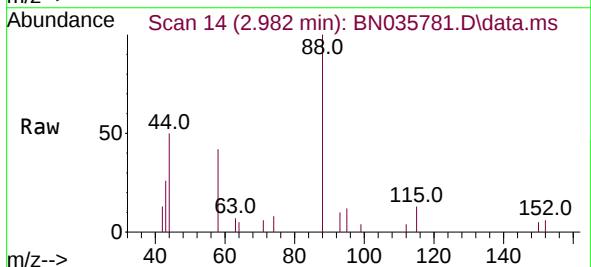



#4
2-Fluorophenol
Concen: 0.133 ng
RT: 4.932 min Scan# 21
Delta R.T. -0.007 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19

Instrument :

BNA_N





ClientSampleId :

DUP-06-20241217

Tgt Ion:112 Resp: 108
Ion Ratio Lower Upper
112 100
64 54.9 39.8 59.8
63 24.0 21.0 31.6




Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

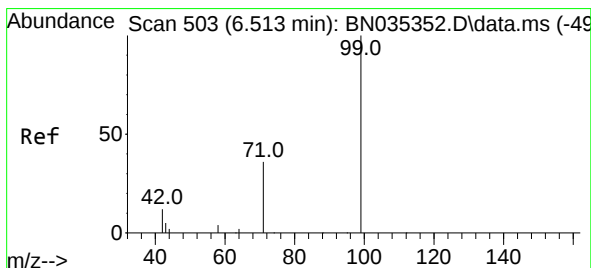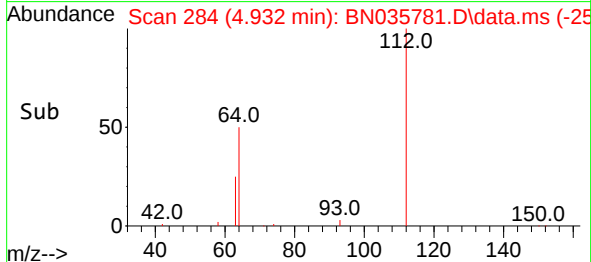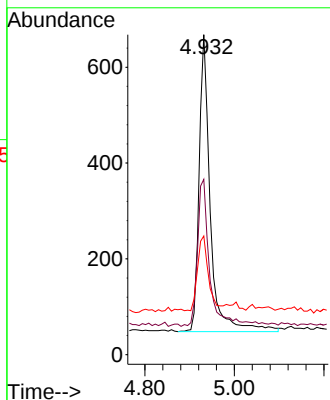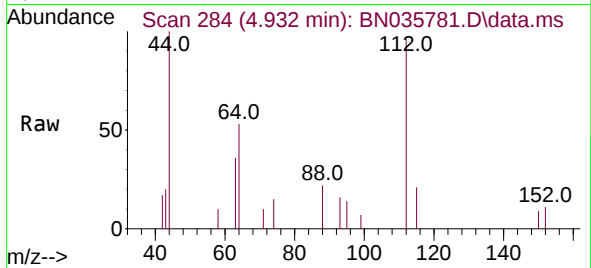

#5
Phenol-d6
Concen: 0.059 ng
RT: 6.484 min Scan# 499
Delta R.T. -0.007 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19

Tgt Ion: 99 Resp: 575
Ion Ratio Lower Upper
99 100
42 12.2 11.4 17.2
71 40.5 29.3 43.9

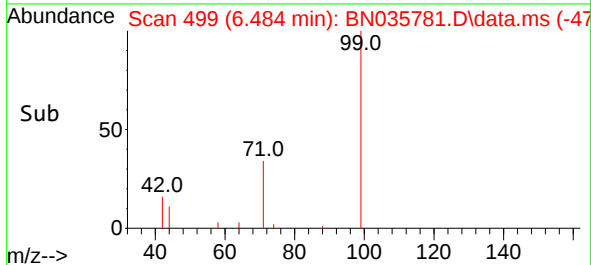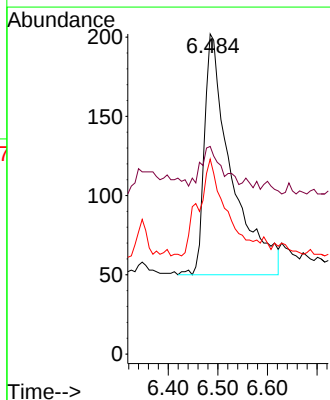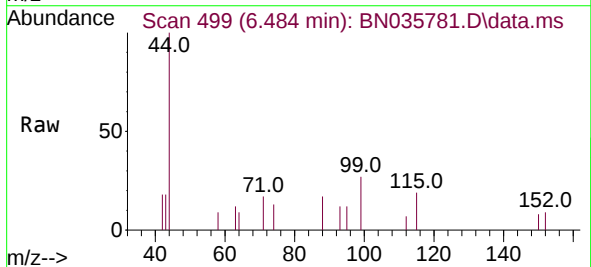







#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.009 min Scan# 915
Delta R.T. -0.011 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19

Instrument :
BNA_N
ClientSampleId :
DUP-06-20241217

Tgt Ion:	136	Resp:	8200
Ion	Ratio	Lower	Upper
136	100		
137	12.2	10.2	15.2
54	6.4	6.1	9.1
68	7.0	6.4	9.6




Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

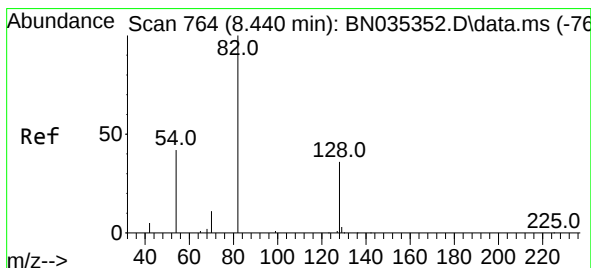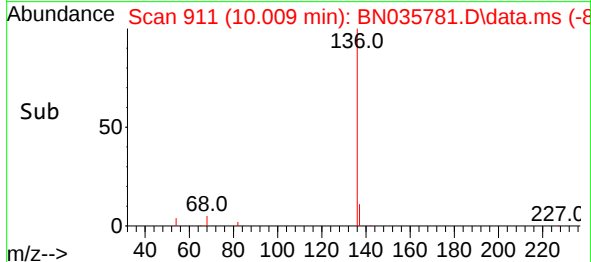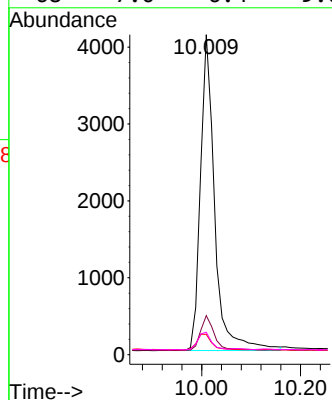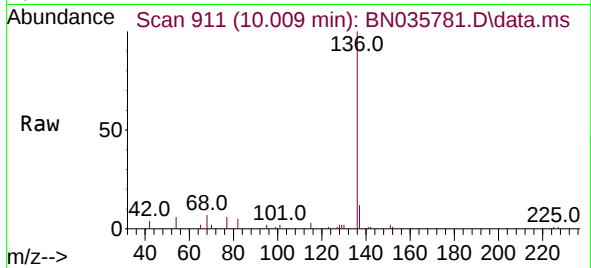

#8
Nitrobenzene-d5
Concen: 0.436 ng m
RT: 8.408 min Scan# 761
Delta R.T. -0.000 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19


Tgt Ion:	82	Resp:	2186
Ion	Ratio	Lower	Upper
82	100		
128	42.5	33.4	50.0
54	43.6	36.7	55.1

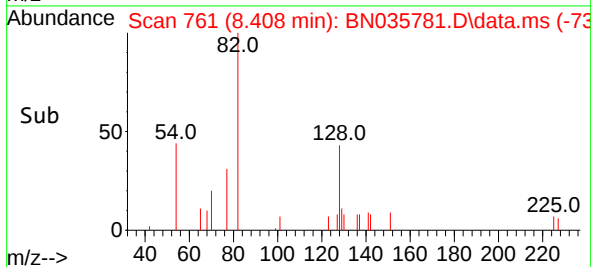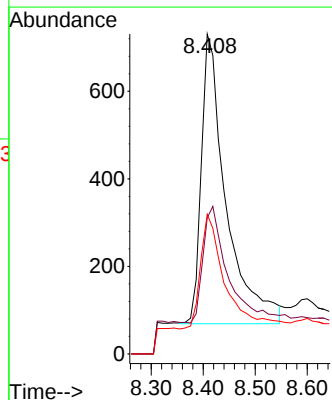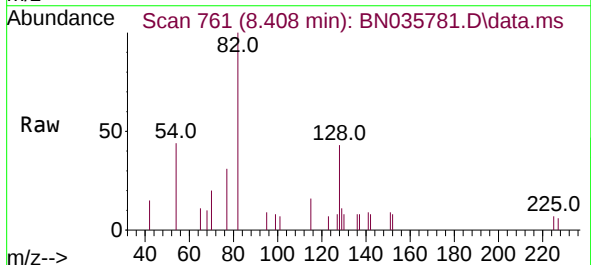



#11
2-Methylnaphthalene-d10
Concen: 0.417 ng
RT: 11.610 min Scan# 1081
Delta R.T. -0.010 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19




Instrument :
BNA_N
ClientSampleId :
DUP-06-20241217

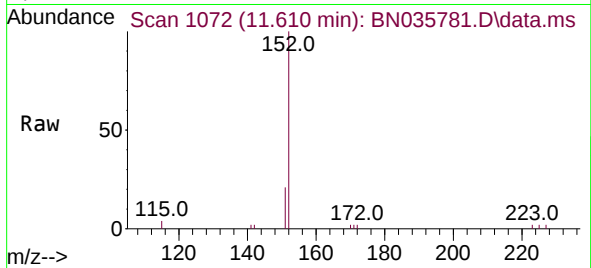


Tgt Ion:152 Resp: 5358
Ion Ratio Lower Upper
152 100
151 20.9 16.6 25.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

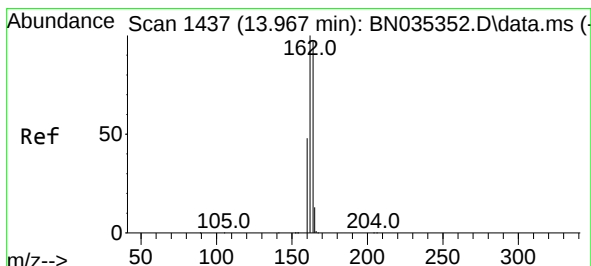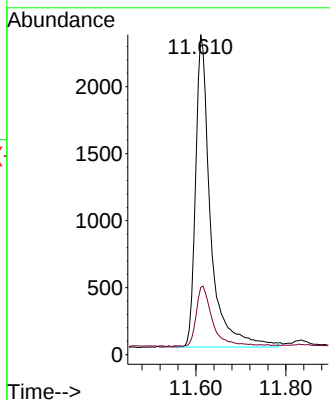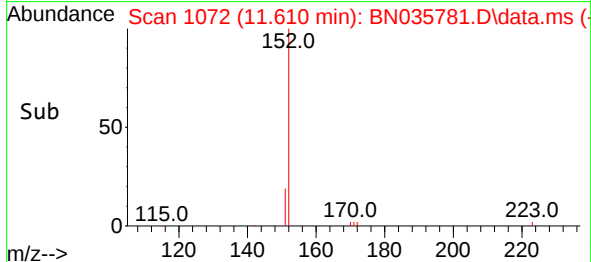


#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 13.924 min Scan# 1433
Delta R.T. -0.011 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19

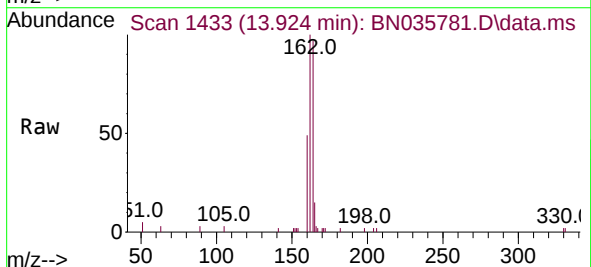


Tgt Ion:164 Resp: 4641
Ion Ratio Lower Upper
164 100
162 103.0 82.2 123.2
160 50.1 40.1 60.1

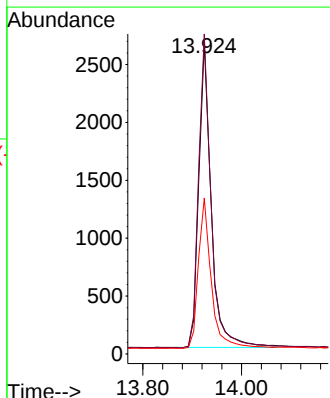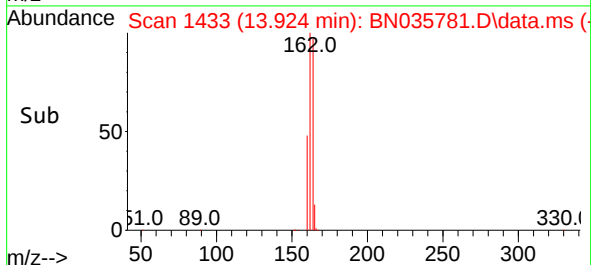

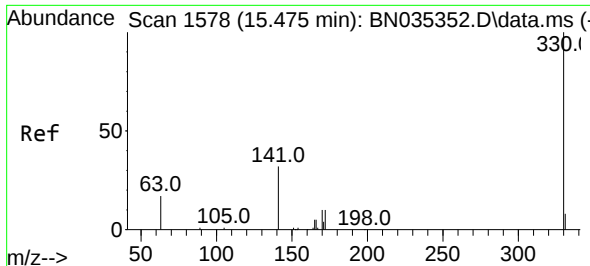

#14
2,4,6-Tribromophenol
Concen: 0.222 ng
RT: 15.453 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19




Instrument :
BNA_N
ClientSampleId :
DUP-06-20241217

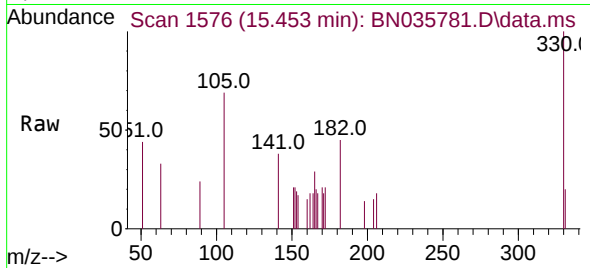

Tgt Ion:330 Resp: 73
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.2 26.6 40.0




Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

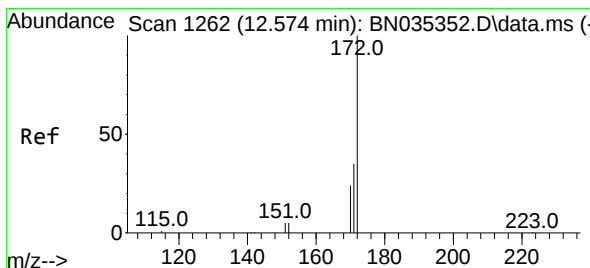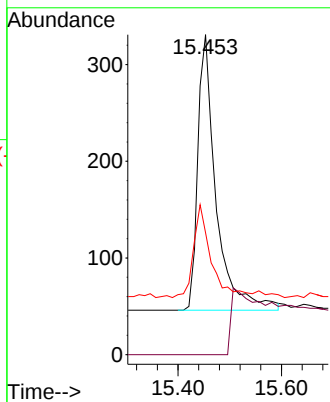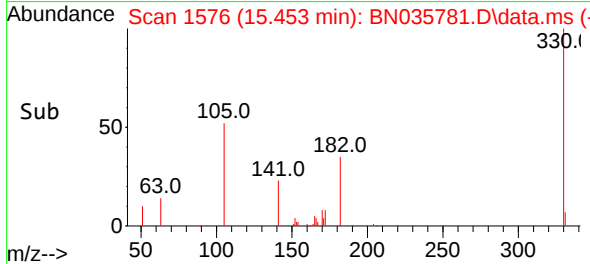

#15
2-Fluorobiphenyl
Concen: 0.445 ng
RT: 12.533 min Scan# 1254
Delta R.T. -0.010 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19


Tgt Ion:172 Resp: 7800
Ion Ratio Lower Upper
172 100
171 36.0 29.0 43.4
170 24.1 19.8 29.8

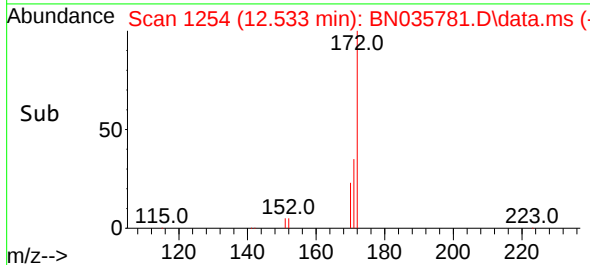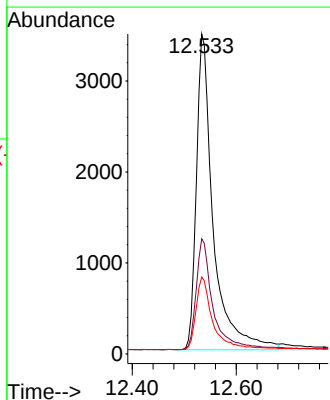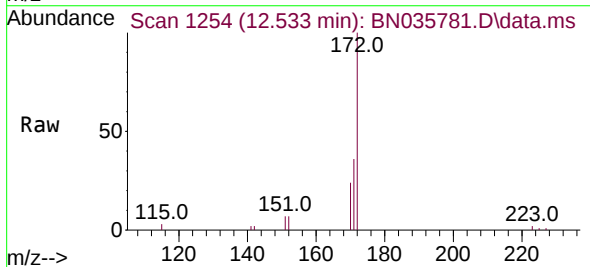



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.698 min Scan# 10
Delta R.T. -0.000 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19




Instrument :
BNA_N
ClientSampleId :
DUP-06-20241217

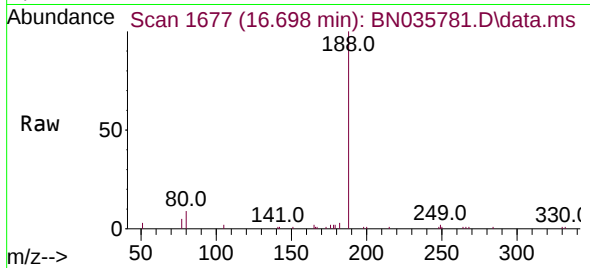

Tgt Ion:188 Resp: 9144
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.4 4.6 6.8




Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

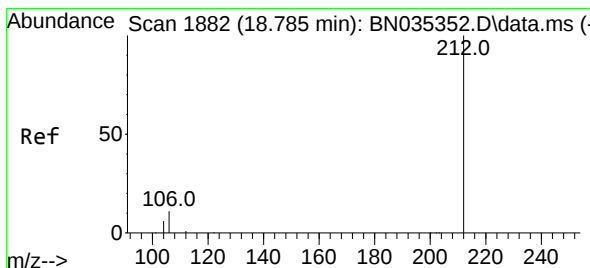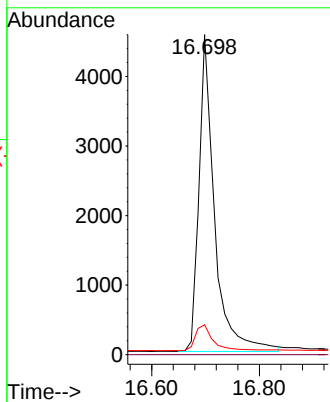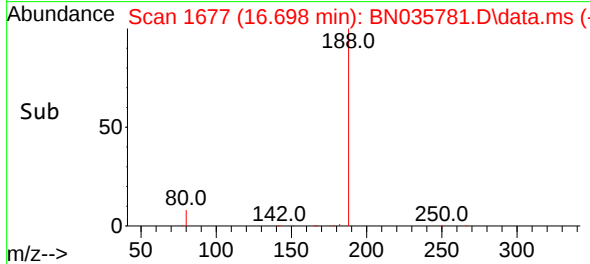

#27
Fluoranthene-d10
Concen: 0.473 ng
RT: 18.752 min Scan# 1875
Delta R.T. -0.009 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19


Tgt Ion:212 Resp: 12266
Ion Ratio Lower Upper
212 100
106 11.4 9.2 13.8
104 6.5 5.3 7.9

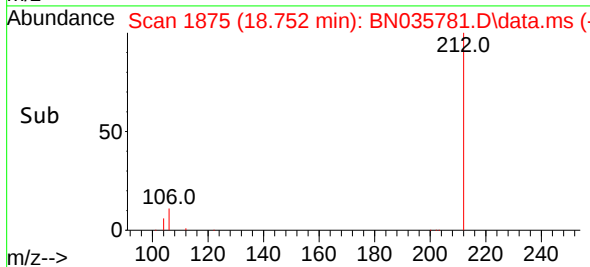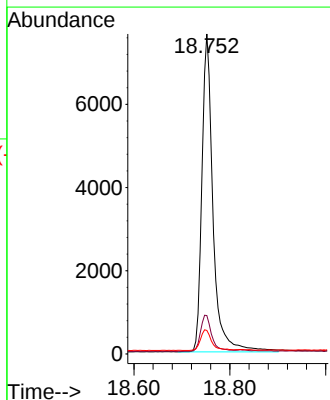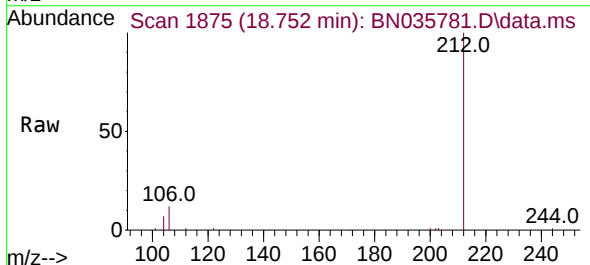



#29
Chrysene-d12
Concen: 0.400 ng
RT: 20.947 min Scan# 21
Delta R.T. -0.009 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19




Instrument :
BNA_N
ClientSampleId :
DUP-06-20241217

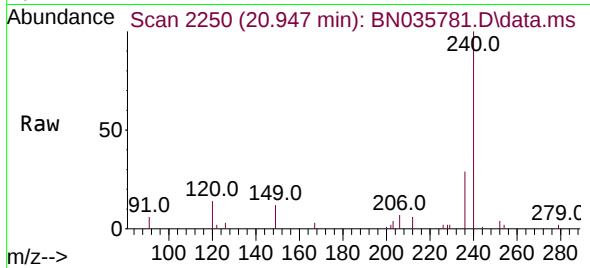

Tgt Ion:240 Resp: 734
Ion Ratio Lower Upper
240 100
120 14.5 7.9 11.9
236 29.3 22.9 34.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

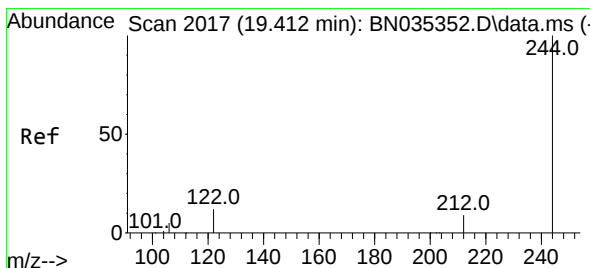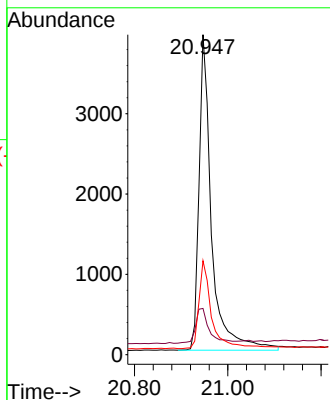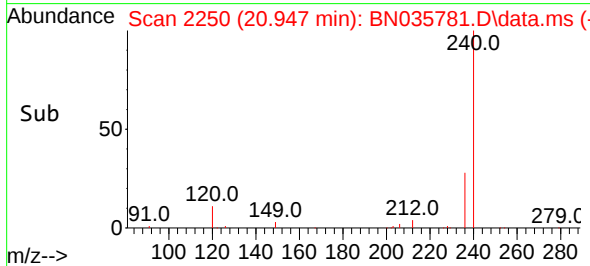

#31
Terphenyl-d14
Concen: 0.678 ng
RT: 19.379 min Scan# 2010
Delta R.T. -0.009 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19


Tgt Ion:244 Resp: 9828
Ion Ratio Lower Upper
244 100
212 9.5 8.1 12.1
122 13.3 10.3 15.5

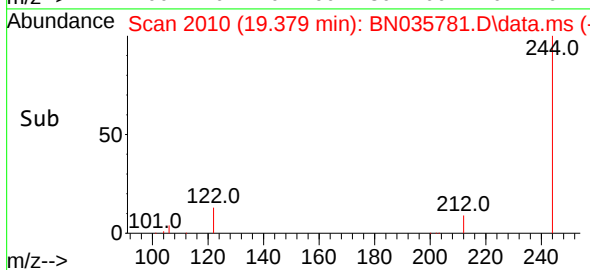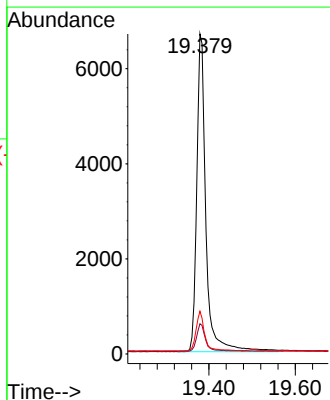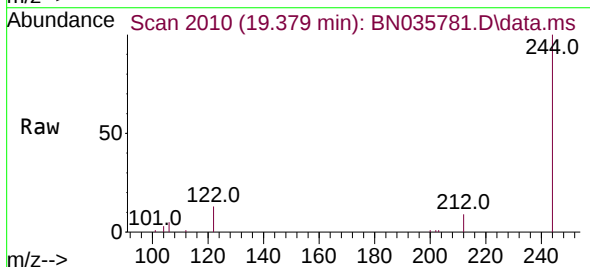

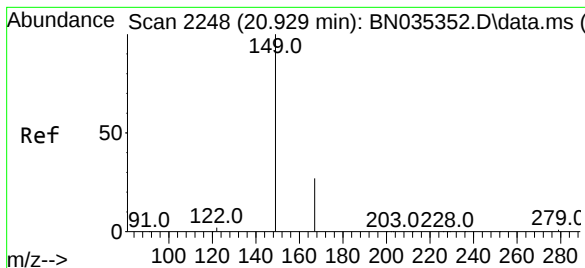

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.077 ng
RT: 20.902 min Scan# 21
Delta R.T. -0.009 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19




Instrument :
BNA_N
ClientSampleId :
DUP-06-20241217

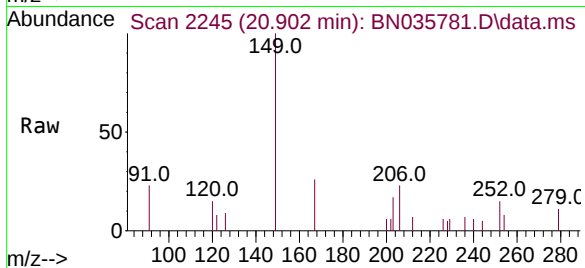

Tgt Ion:149 Resp: 780
Ion Ratio Lower Upper
149 100
167 27.9 22.2 33.4
279 3.7 2.7 4.1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

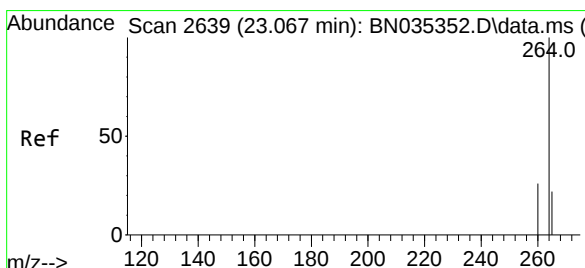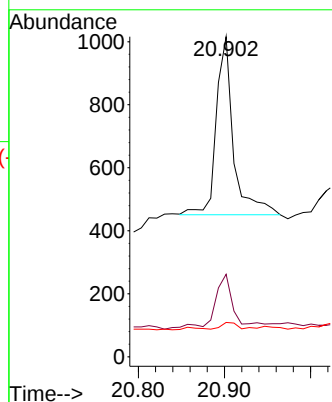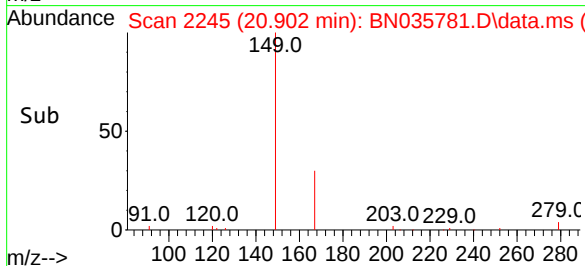

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.029 min Scan# 2626
Delta R.T. -0.012 min
Lab File: BN035781.D
Acq: 23 Dec 2024 13:19

Tgt Ion:264 Resp: 7454
Ion Ratio Lower Upper
264 100
260 27.4 21.4 32.2
265 88.9 40.2 60.4#

