

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122324\
Data File : VX044486.D
Acq On : 23 Dec 2024 17:31
Operator : JC/MD
Sample : P5317-22 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20241217

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Title : SW846 8260

Signal : TIC: VX044486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.636	68	90	91	rBV2	21802	108790	13.00%	2.309%
2	2.941	297	304	316	rVB	11554	26171	3.13%	0.556%
3	5.379	694	704	719	rBV	99837	294873	35.23%	6.259%
4	5.544	721	731	749	rVB	151628	440376	52.61%	9.348%
5	5.946	785	797	810	rBV	115826	304337	36.36%	6.460%
6	6.757	920	930	951	rBV	238385	588971	70.37%	12.502%
7	7.117	982	989	1002	rBV	124308	281031	33.58%	5.965%
8	8.647	1233	1240	1253	rBV	527682	837007	100.00%	17.767%
9	10.049	1465	1470	1483	rBV	469926	671020	80.17%	14.243%
10	11.079	1634	1639	1650	rBV	411128	533219	63.71%	11.318%
11	12.018	1788	1793	1807	rBV	494807	625316	74.71%	13.273%




Sum of corrected areas: 4711111

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122324\
Data File : VX044486.D
Acq On : 23 Dec 2024 17:31
Operator : JC/MD
Sample : P5317-22 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20241217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

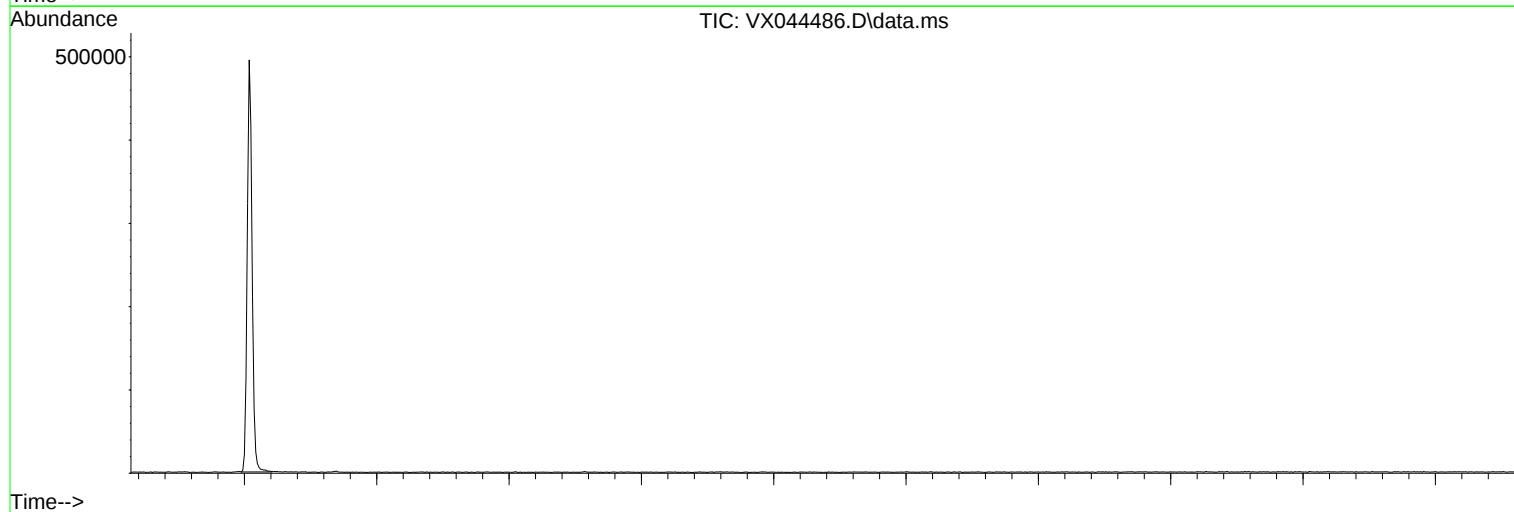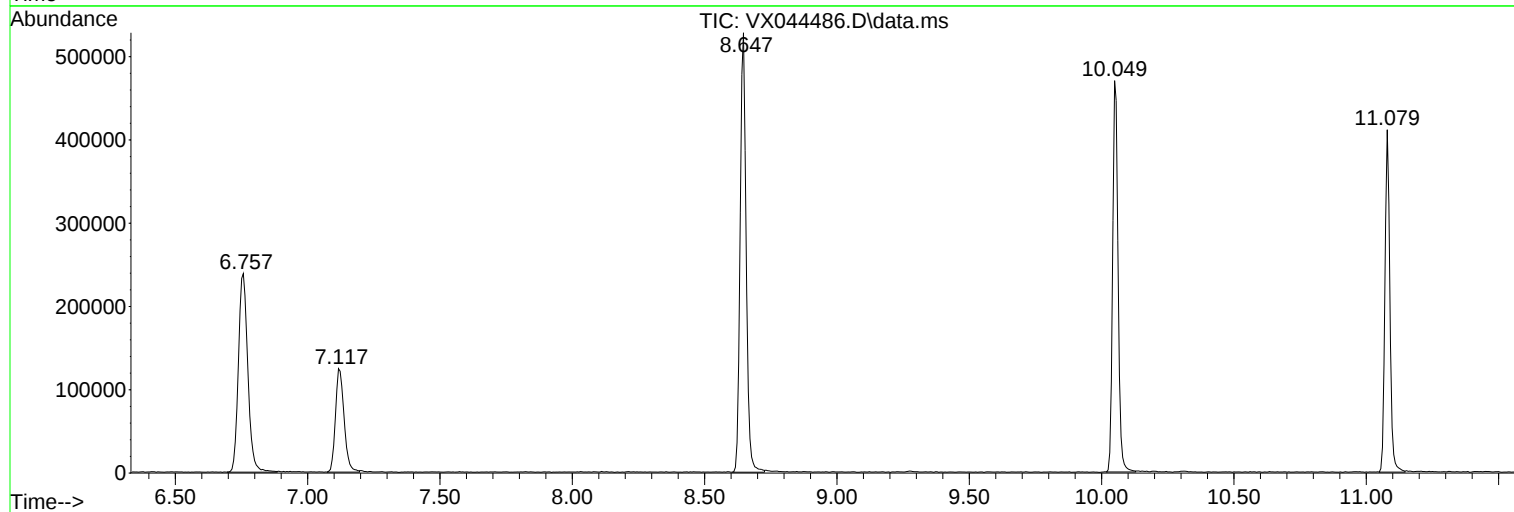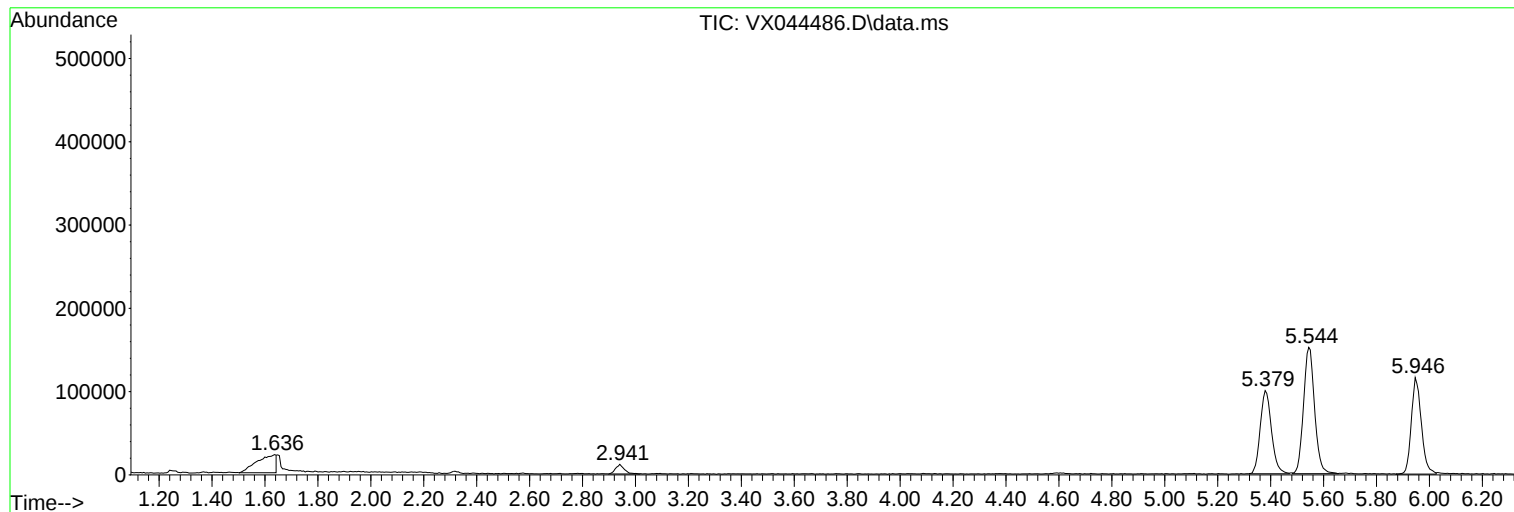

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122324\
Data File : VX044486.D
Acq On : 23 Dec 2024 17:31
Operator : JC/MD
Sample : P5317-22 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20241217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.636 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
1.636	12.35 ug/l	108790	Pentafluorobenzene	5.544	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Dimethylamine	45	C2H7N	000124-40-3	10
2	sec-Butylamine	73	C4H11N	013952-84-6	9
3	(R)-(-)-2-Amino-1-propanol	75	C3H9NO	035320-23-1	9
4	2-Amino-4-dimethylaminomethylene...	164	C8H12N4	1000191-40-0	9
5	1-Propanol, 2-amino-, (+/-)-	75	C3H9NO	006168-72-5	9

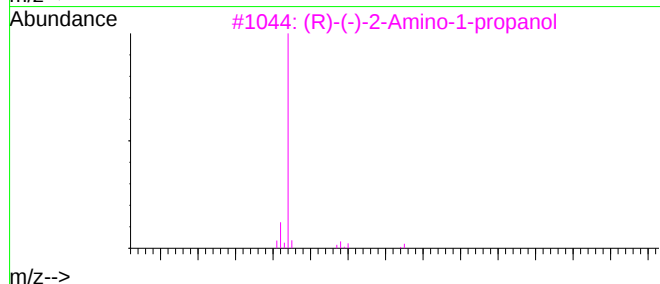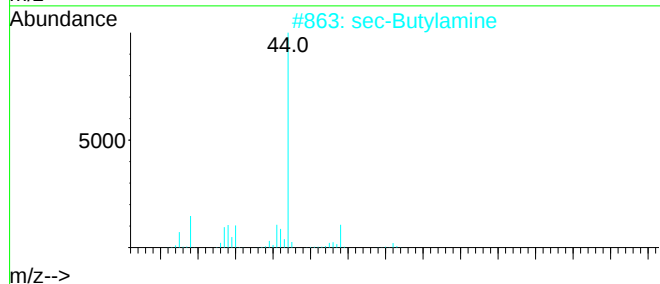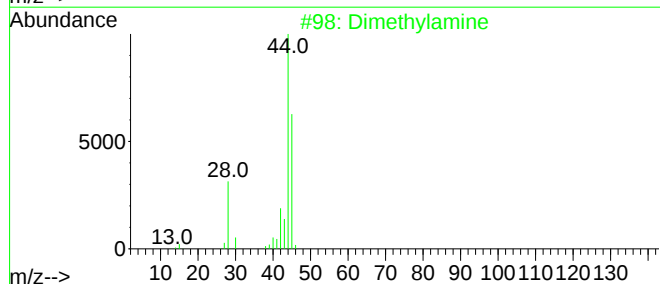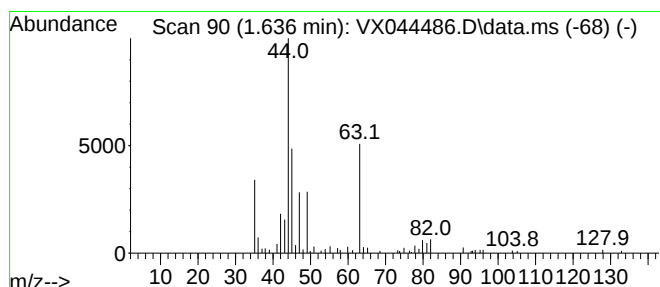

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122324\
Data File : VX044486.D
Acq On : 23 Dec 2024 17:31
Operator : JC/MD
Sample : P5317-22 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D7-20241217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.636	1.636	12.4	ug/l	108790	1	5.544	440376	50.0