

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122324\
 Data File : VX044487.D
 Acq On : 23 Dec 2024 17:54
 Operator : JC/MD
 Sample : P5317-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP-04-20241216

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
 Title : SW846 8260

Signal : TIC: VX044487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	68	84	86	rBV3	17824	68628	8.47%	1.596%
2	2.319	195	202	208	rBV4	9133	18071	2.23%	0.420%
3	5.379	694	704	721	rBV	97578	286538	35.36%	6.663%
4	5.544	721	731	745	rVV2	145733	421815	52.06%	9.809%
5	5.946	788	797	812	rBV	106140	294114	36.30%	6.839%
6	6.757	919	930	946	rBV	236224	577493	71.27%	13.429%
7	7.123	979	990	999	rBV3	37743	87342	10.78%	2.031%
8	8.647	1233	1240	1256	rBV	497603	810319	100.00%	18.843%
9	10.049	1465	1470	1480	rBV	460866	662168	81.72%	15.398%
10	11.079	1634	1639	1653	rBV	378704	501867	61.93%	11.670%
11	12.018	1788	1793	1807	rBV	457493	572041	70.59%	13.302%




Sum of corrected areas: 4300396

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122324\
Data File : VX044487.D
Acq On : 23 Dec 2024 17:54
Operator : JC/MD
Sample : P5317-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-04-20241216

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

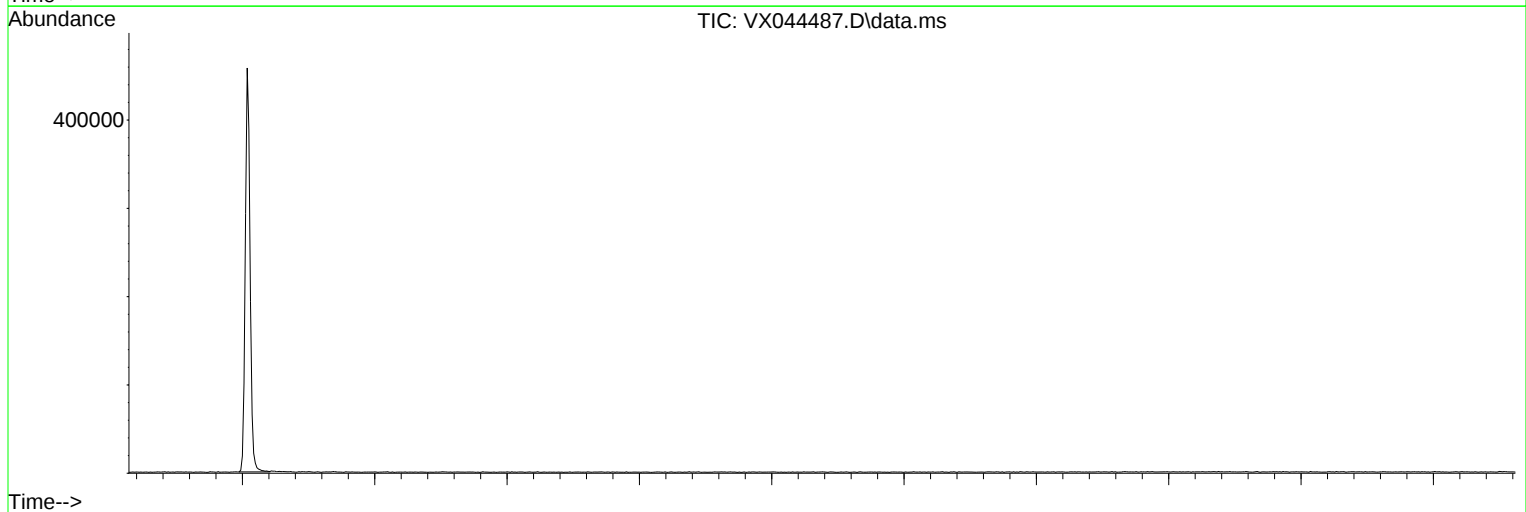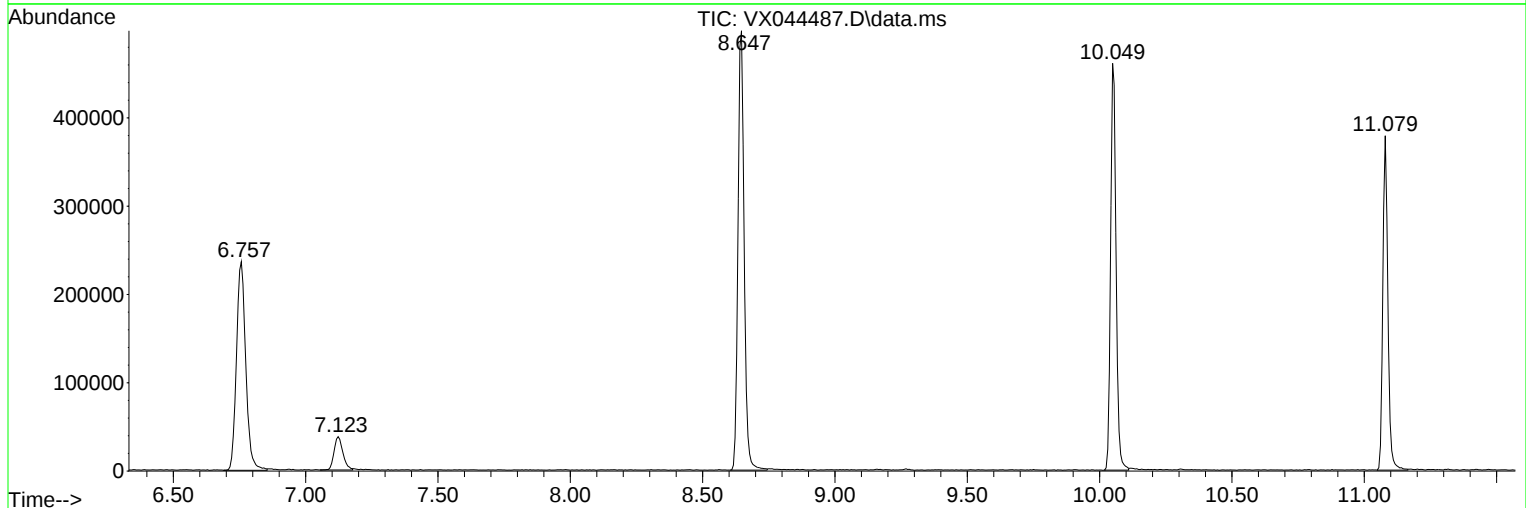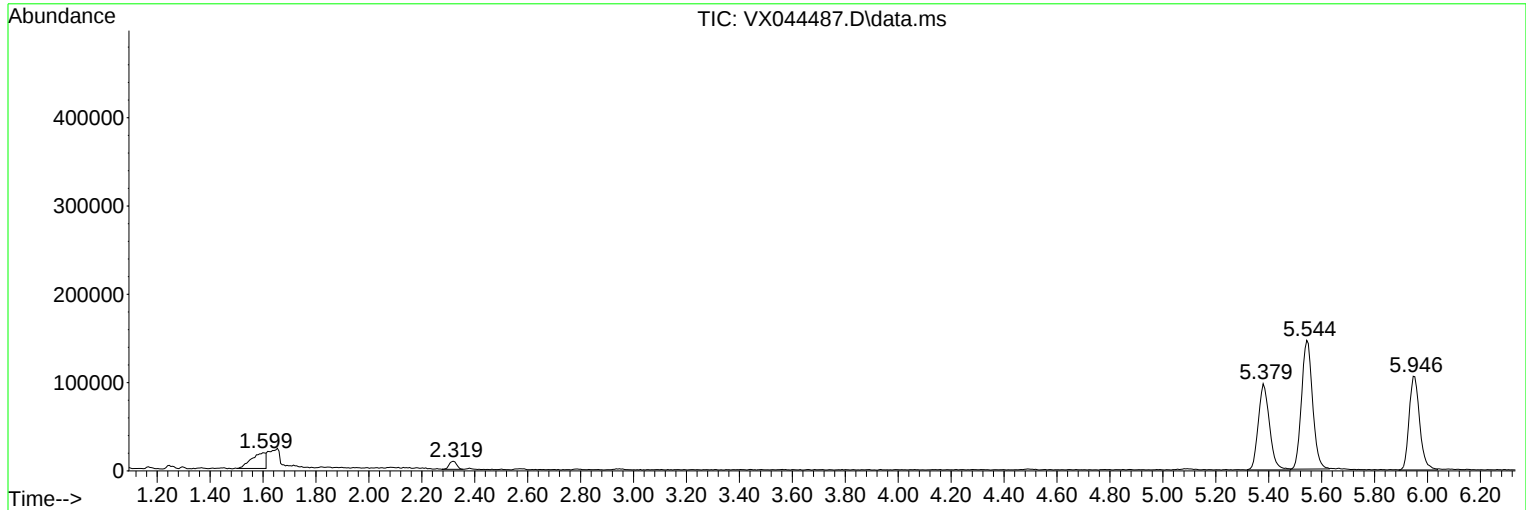

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122324\
Data File : VX044487.D
Acq On : 23 Dec 2024 17:54
Operator : JC/MD
Sample : P5317-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-04-20241216

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX122324\
Data File : VX044487.D
Acq On : 23 Dec 2024 17:54
Operator : JC/MD
Sample : P5317-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-04-20241216

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------