

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0122024\
 Data File : P0108718.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Dec 2024 17:56
 Operator : YP/AJ
 Sample : P5361-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-01-20241219-9.0-9.5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 21 01:23:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.704	3.702	165.6E6	100.9E6	19.038	19.910
2) SA Decachlor...	8.772	8.724	106.4E6	63764622	14.570	16.456

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122024\
Data File : PO108718.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Dec 2024 17:56
Operator : YP/AJ
Sample : P5361-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-01-20241219-9.0-9.5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 21 01:23:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

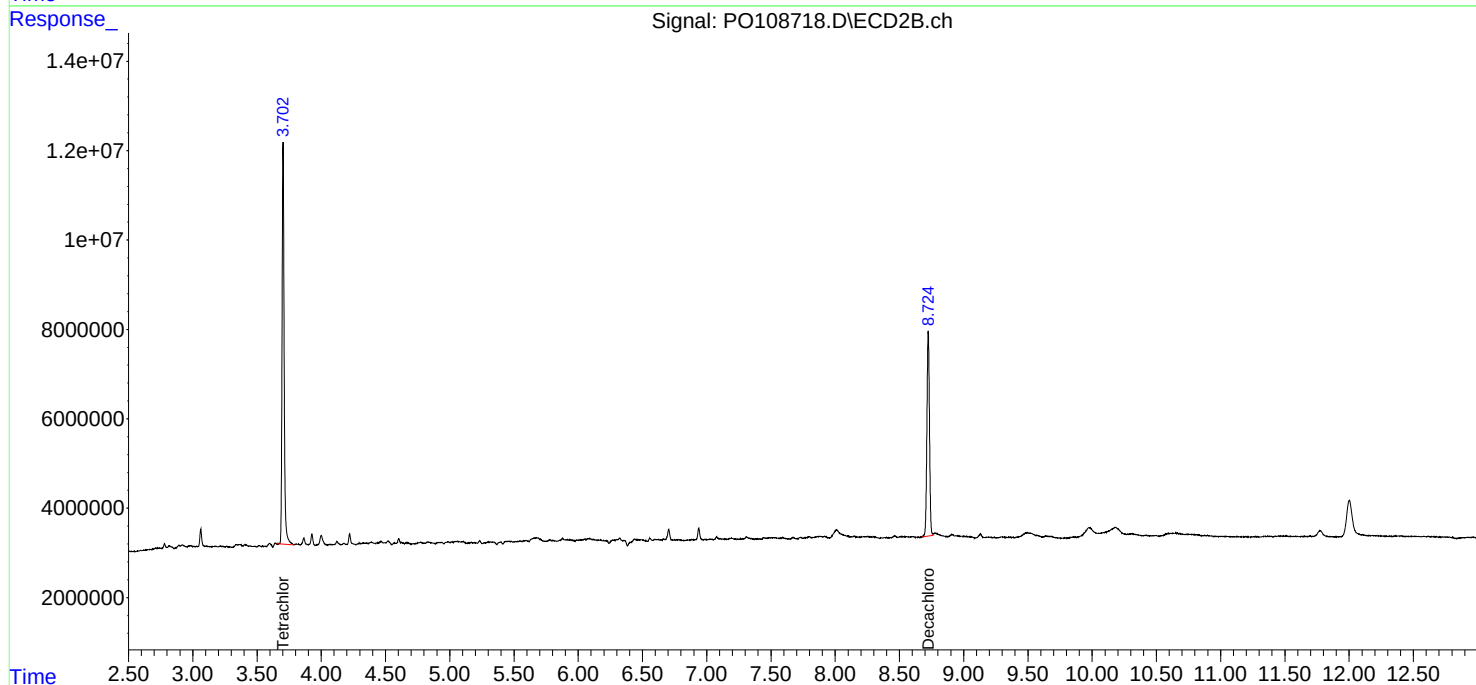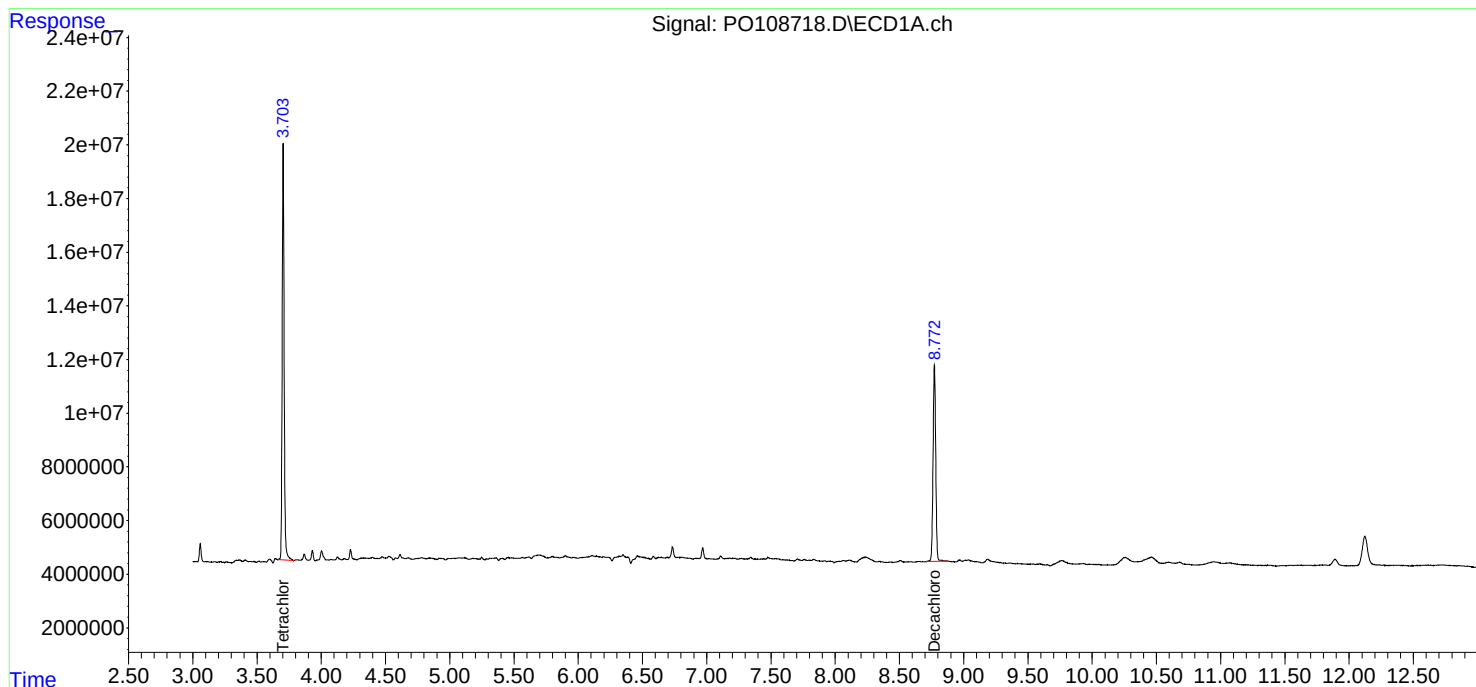


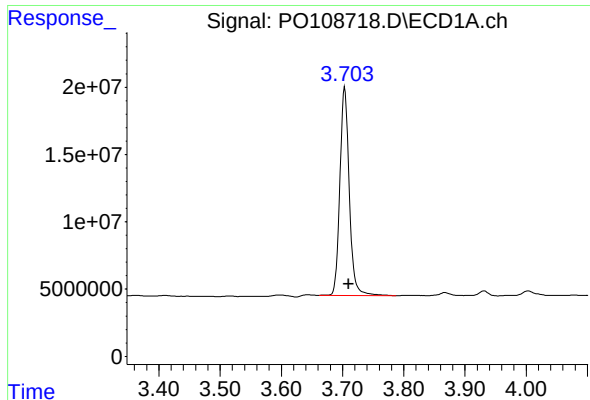

#1 Tetrachloro-m-xylene


R.T.: 3.704 min
Delta R.T.: -0.006 min
Response: 165631817
Conc: 19.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01-20241219-9.0-9.5

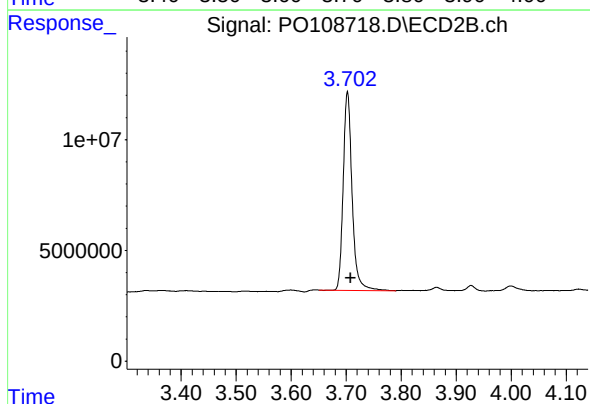


#1 Tetrachloro-m-xylene

R.T.: 3.702 min
Delta R.T.: -0.006 min
Response: 100933136
Conc: 19.91 ng/ml

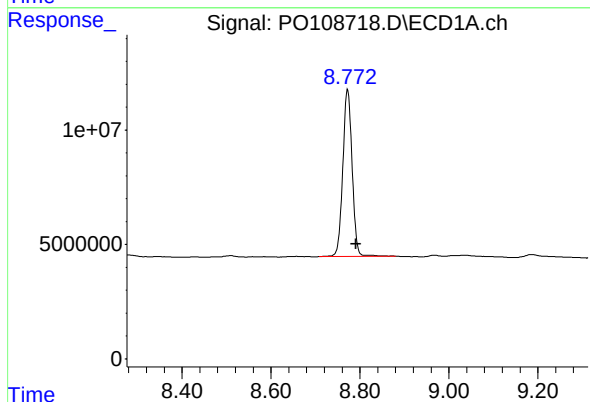

#2 Decachlorobiphenyl

R.T.: 8.772 min
Delta R.T.: -0.019 min
Response: 106419620
Conc: 14.57 ng/ml

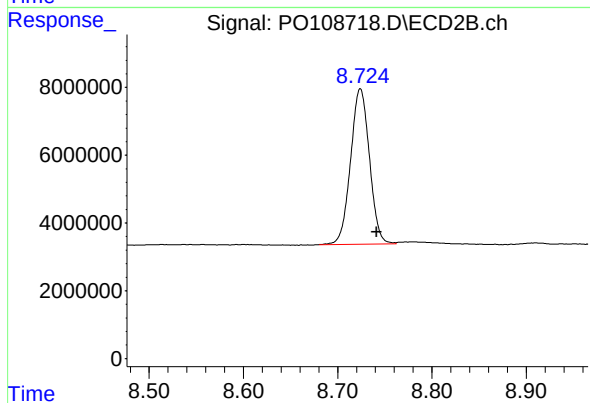

#2 Decachlorobiphenyl

R.T.: 8.724 min
Delta R.T.: -0.017 min
Response: 63764622
Conc: 16.46 ng/ml