

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122724\
 Data File : PL093546.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Dec 2024 16:33
 Operator : AR\AJ
 Sample : PB165895BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB165895BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 12/30/2024
 Supervised By : Ankita Jodhani 12/30/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 28 00:59:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:29:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.538	2.774	47558557	54679617	19.210m	18.783
2) SA Decachlor...	9.053	7.911	40689175	62794962	22.006	21.030

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL122724\
Data File : PL093546.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Dec 2024 16:33
Operator : AR\AJ
Sample : PB165895BL
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB165895BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/30/2024
Supervised By : Ankita Jodhani 12/30/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 28 00:59:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:29:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

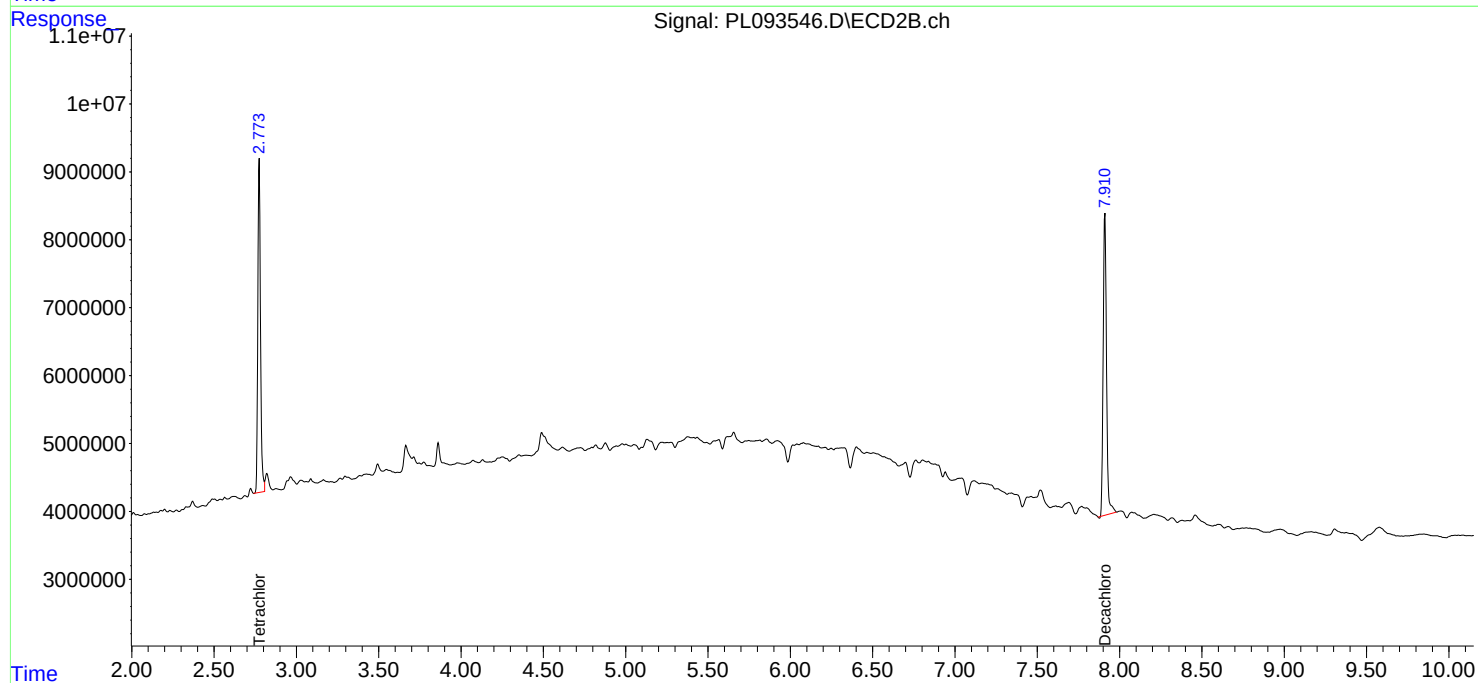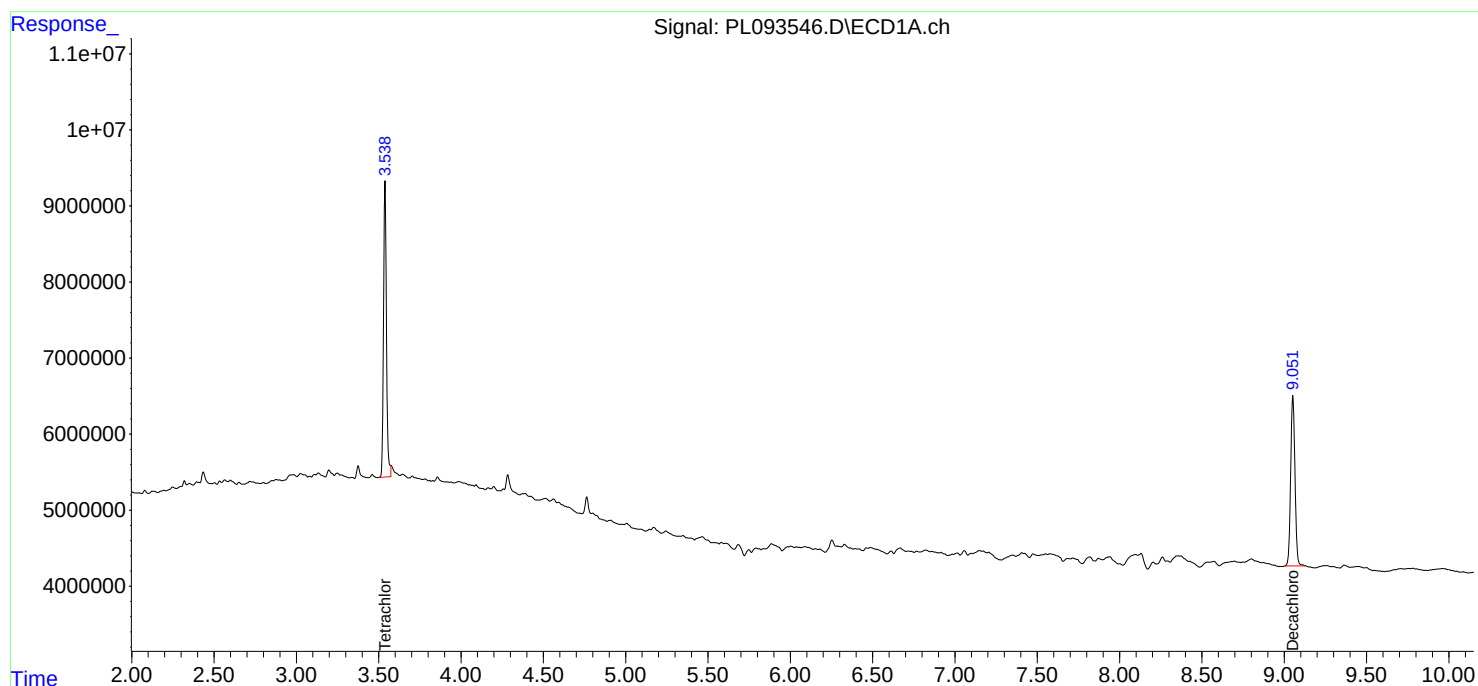

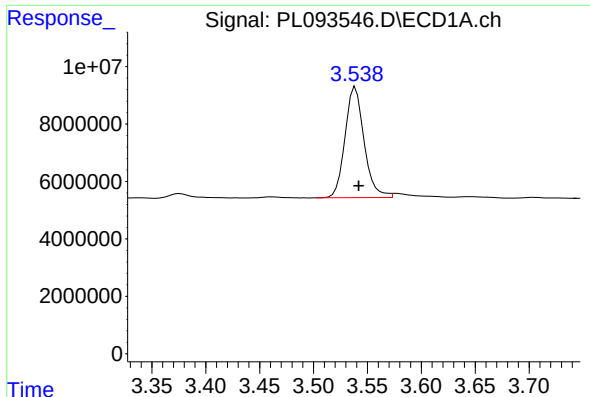


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: -0.004 min
Response: 47558557
Conc: 19.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB165895BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/30/2024
Supervised By :Ankita Jodhani 12/30/2024

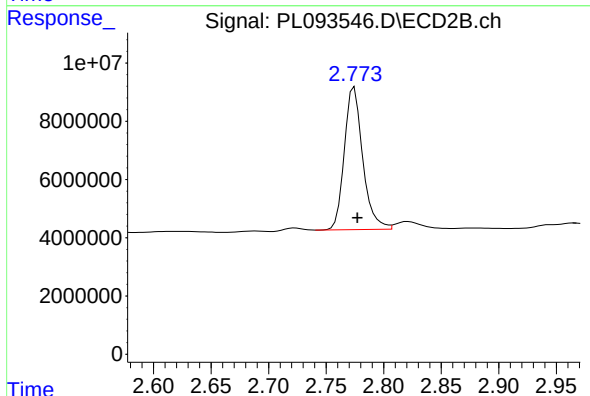


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: -0.003 min
Response: 54679617
Conc: 18.78 ng/ml

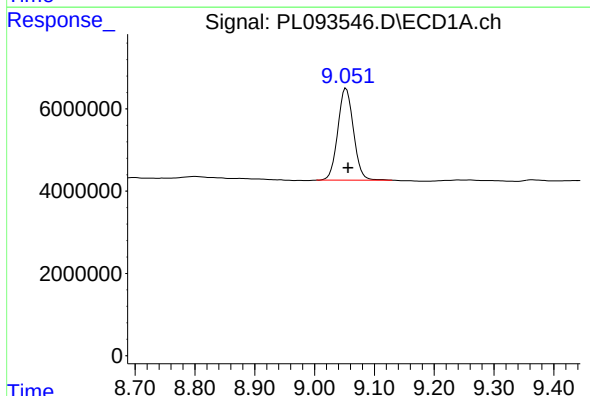

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.003 min
Response: 40689175
Conc: 22.01 ng/ml

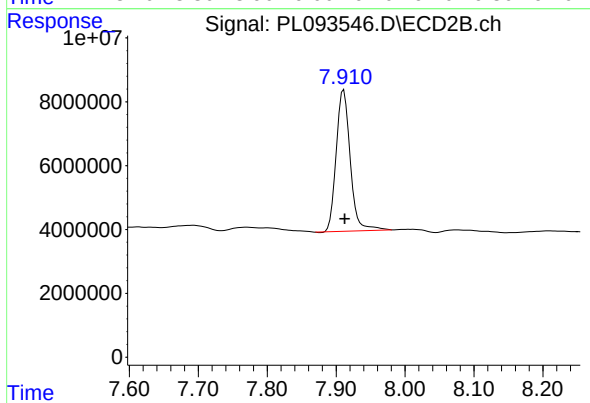

#28 Decachlorobiphenyl

R.T.: 7.911 min
Delta R.T.: -0.001 min
Response: 62794962
Conc: 21.03 ng/ml