
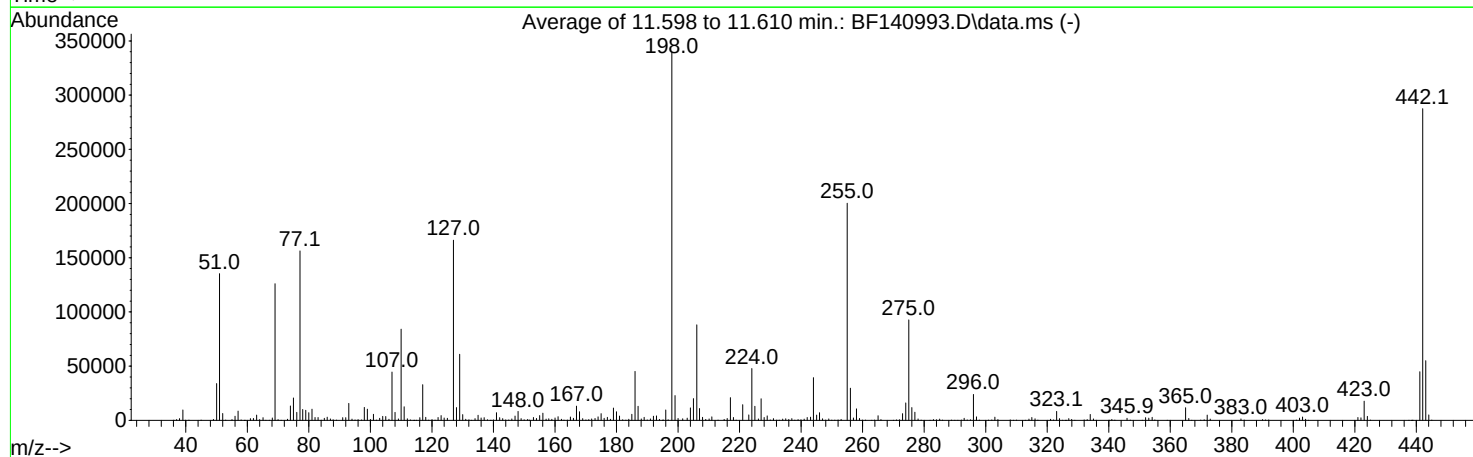


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122724\
Data File : BF140993.D
Acq On : 27 Dec 2024 13:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 27 00:31:16 2024

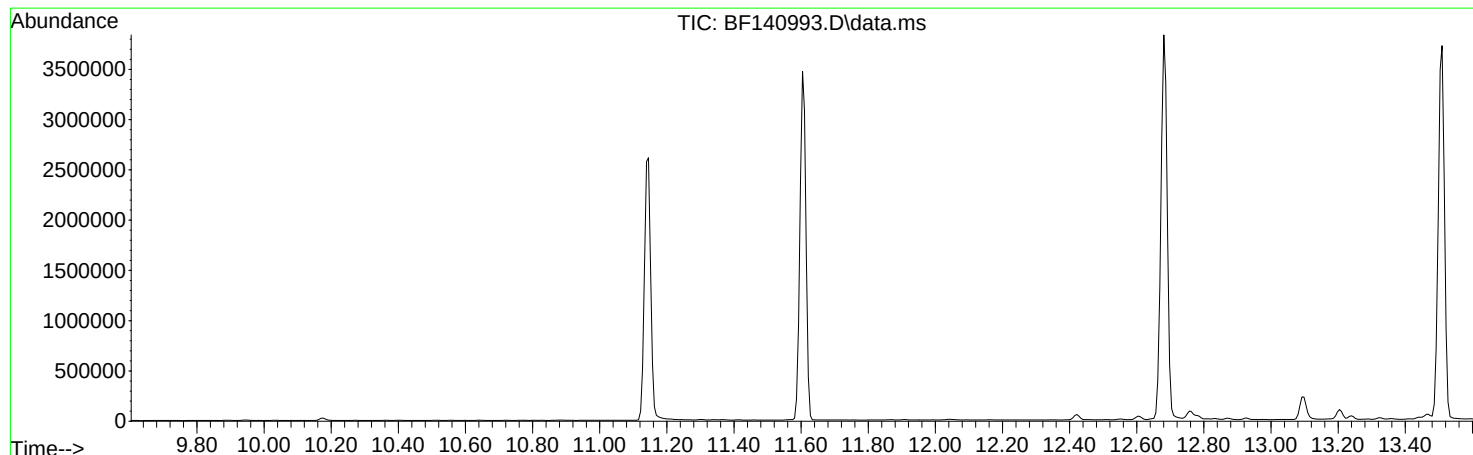

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	135298	PASS
68	69	0.00	2	1.8	2267	PASS
69	198	0.00	100	37.1	126038	PASS
70	69	0.00	2	0.6	718	PASS
127	198	10	80	49.0	166187	PASS
197	198	0.00	2	0.2	570	PASS
198	198	100	100	100.0	339328	PASS
199	198	5	9	6.7	22835	PASS
275	198	10	60	27.3	92720	PASS
365	198	1	100	3.5	11707	PASS
441	198	0.01	100	13.2	44816	PASS
442	442	50	100	100.0	287488	PASS
443	442	15	24	19.1	55021	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/27/2024	BNA_F	<u>BF140993.D</u>
Compound Name	Response	Retention Time
DDT	916292	13.51
DDD	30550	13.204
DDE	2523	12.869
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33073	949365	3.48

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122724\
Data File : BF140993.D
Acq On : 27 Dec 2024 13:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 27 14:11:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

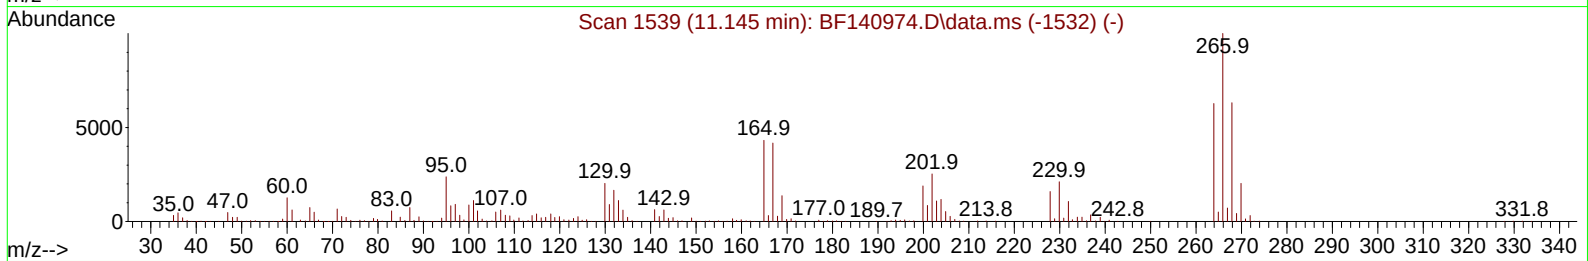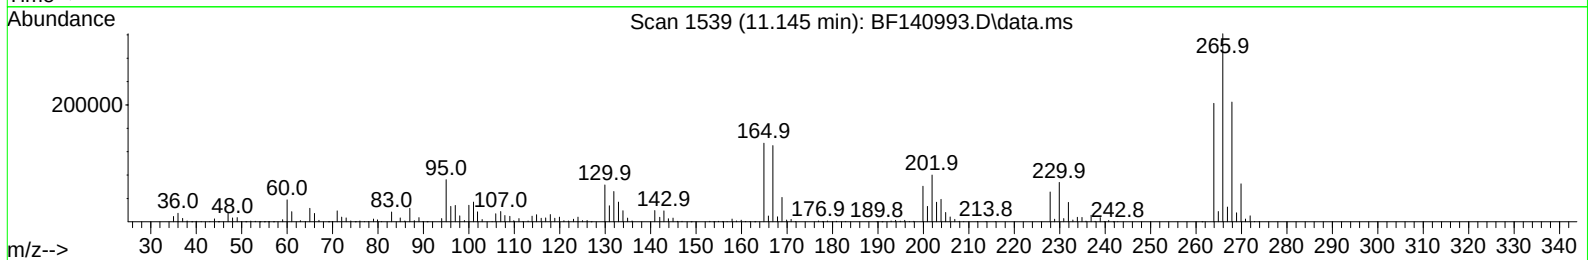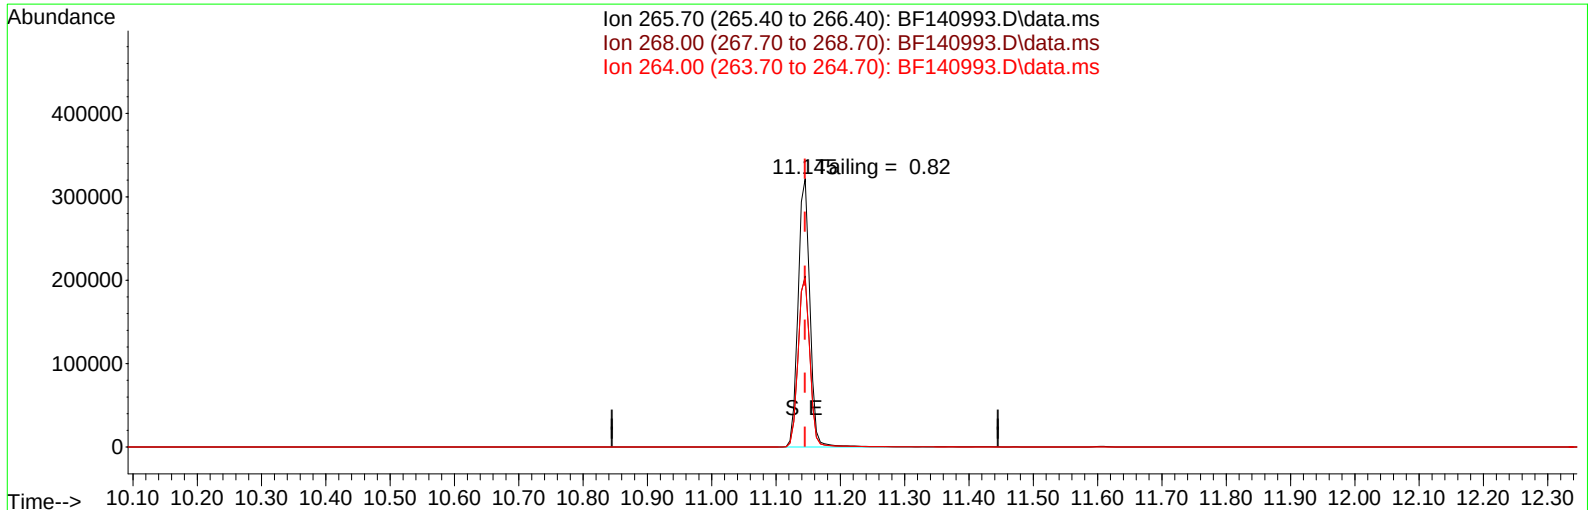

TIC: BF140993.D\data.ms

(70) Pentachlorophenol (C)

11.145min (+ 0.000) 33852.29 ng

response 415287

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.69
264.00	62.80	63.03
0.00	0.00	0.00

