
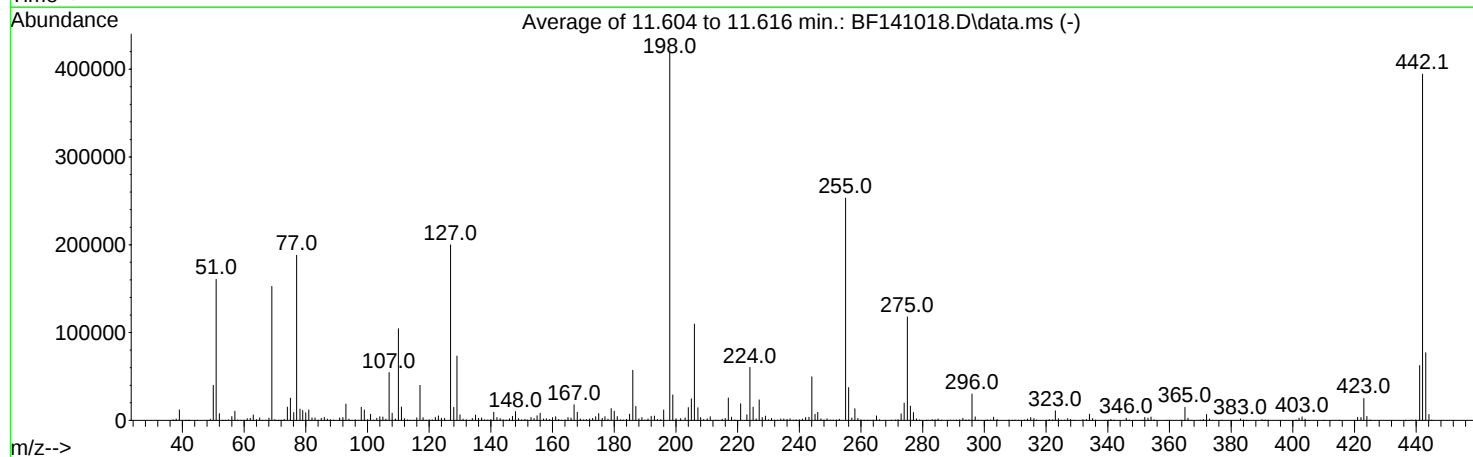


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141018.D
Acq On : 30 Dec 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 27 00:31:16 2024

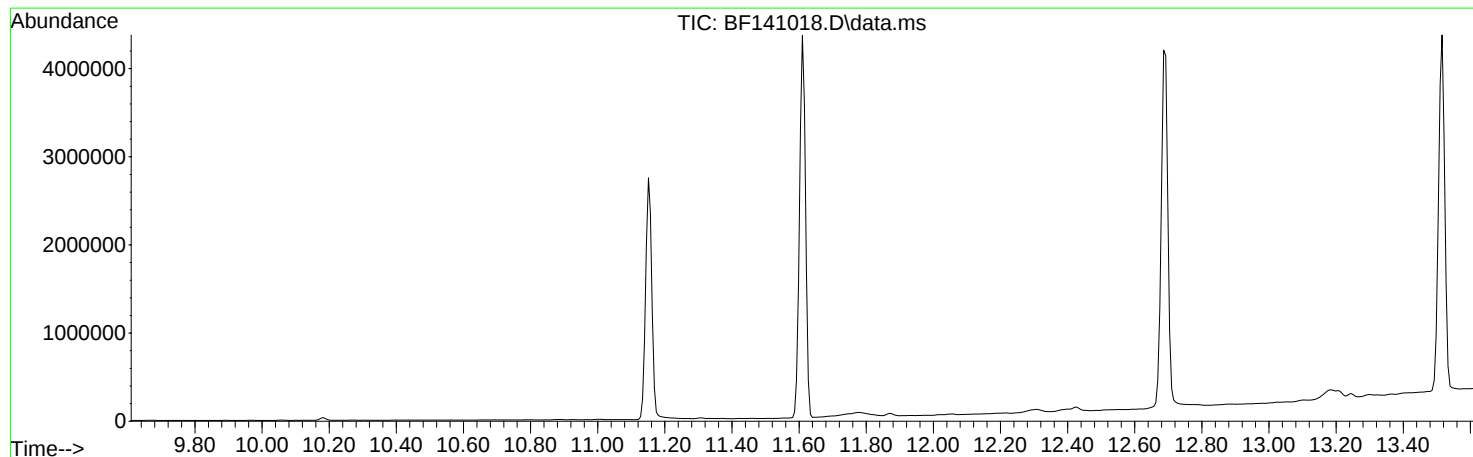

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	160811	PASS
68	69	0.00	2	1.7	2616	PASS
69	198	0.00	100	36.4	152490	PASS
70	69	0.00	2	0.6	903	PASS
127	198	10	80	47.7	199893	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	418987	PASS
199	198	5	9	6.9	28909	PASS
275	198	10	60	28.2	118011	PASS
365	198	1	100	3.6	14923	PASS
441	198	0.01	100	14.9	62432	PASS
442	442	50	100	100.0	394133	PASS
443	442	15	24	19.6	77104	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/30/2024	BNA_F	<u>BF141018.D</u>
Compound Name	Response	Retention Time
DDT	927446	13.516
DDD	23538	13.21
DDE	2456	12.875
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25994	953440	2.73

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141018.D
Acq On : 30 Dec 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 30 10:08:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

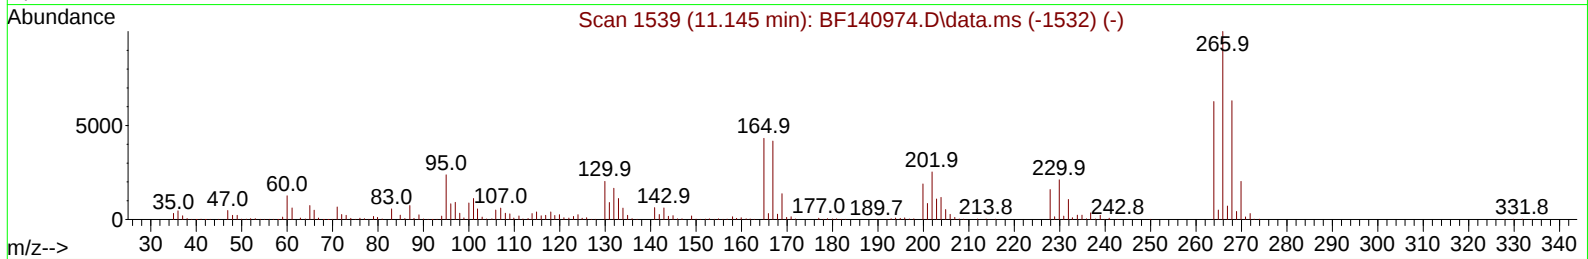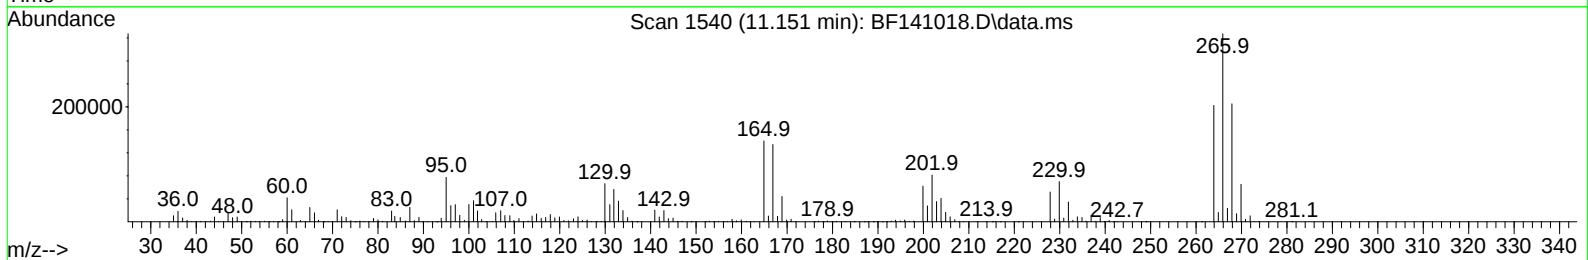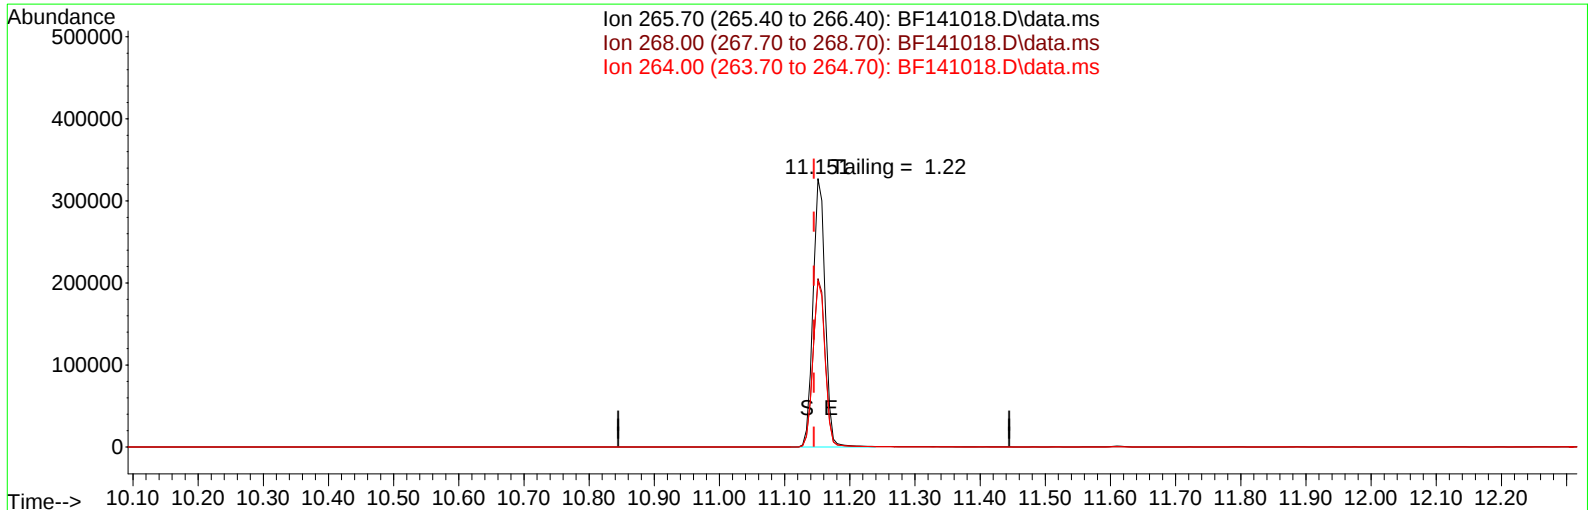

TIC: BF141018.D\data.ms

(70) Pentachlorophenol (C)

11.151min (+ 0.006) 118641.00 ng




response 426155

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.72
264.00	62.80	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141018.D
Acq On : 30 Dec 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 30 10:08:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

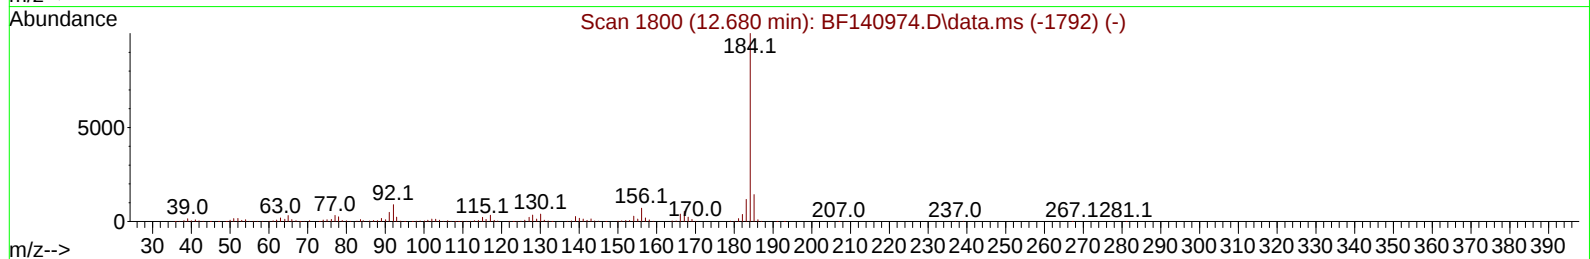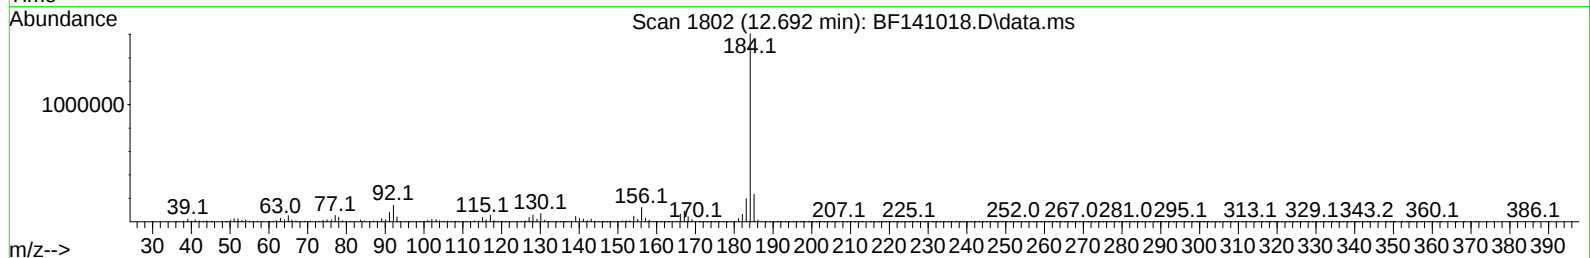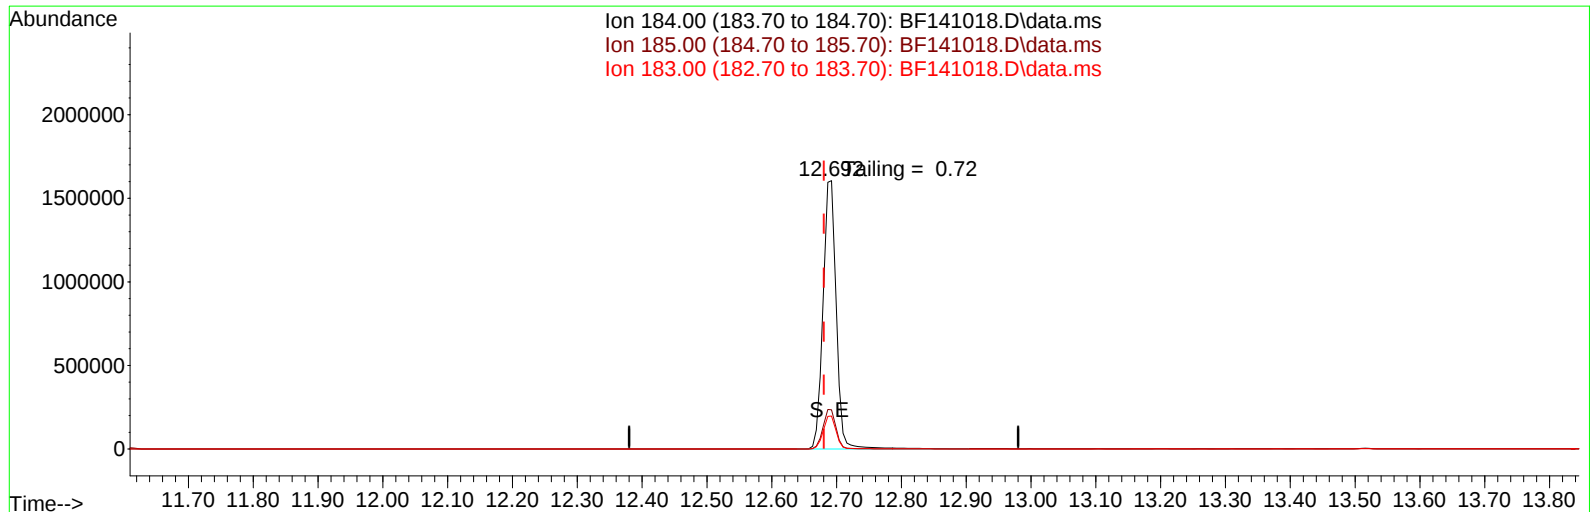

TIC: BF141018.D\data.ms

(77) Benzidine

12.692min (+ 0.012) 182948.18 ng

response 2285059

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.65
183.00	11.70	12.30
0.00	0.00	0.00