


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141030.D
Acq On : 30 Dec 2024 14:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 27 00:31:16 2024

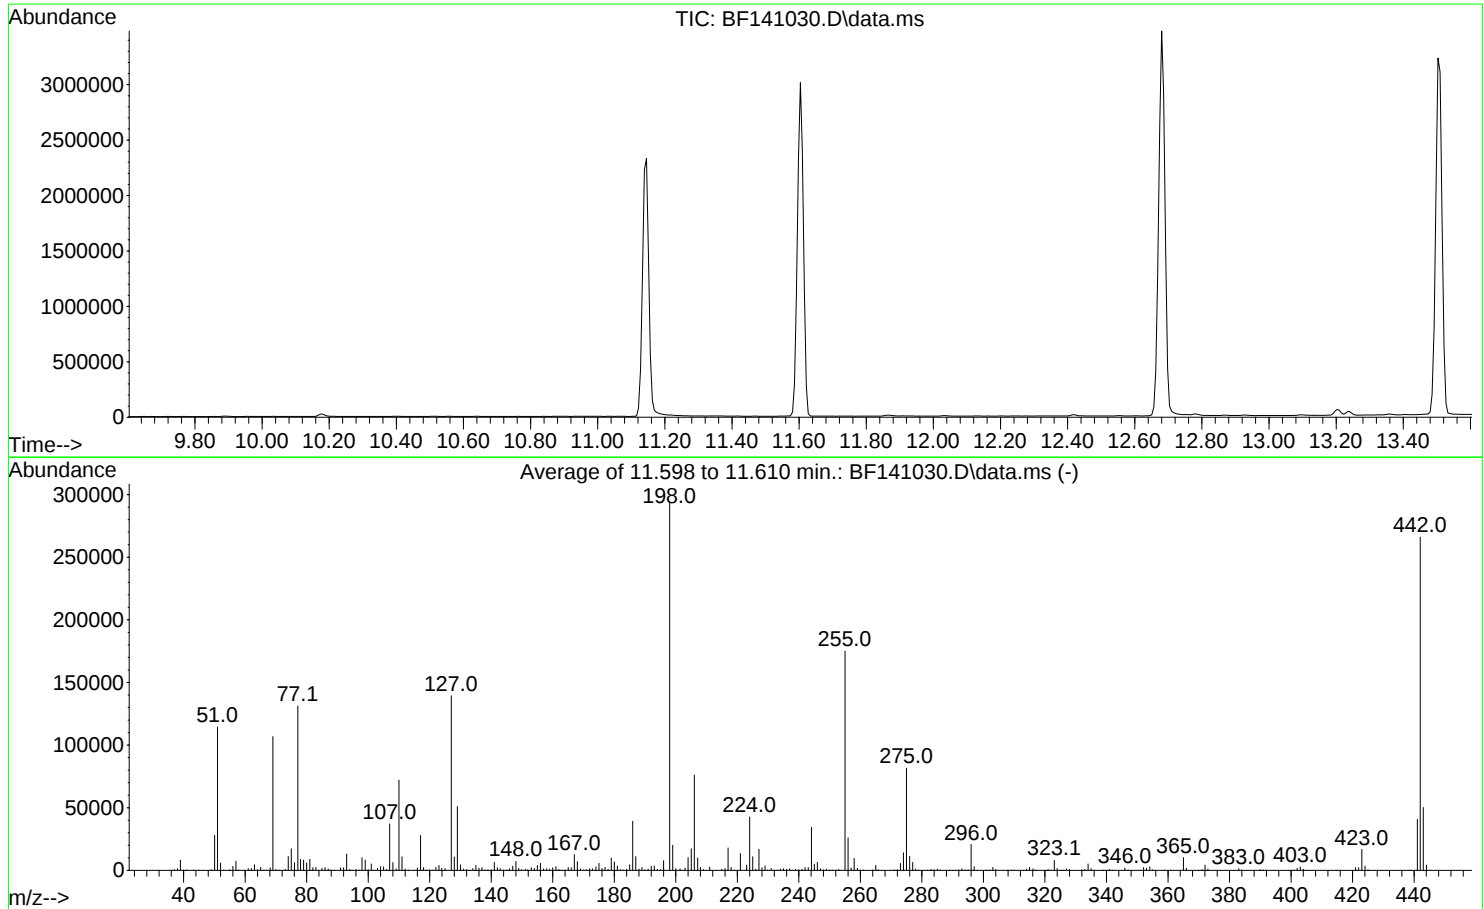

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	114464	PASS
68	69	0.00	2	1.9	1987	PASS
69	198	0.00	100	36.4	106829	PASS
70	69	0.00	2	0.6	594	PASS
127	198	10	80	47.5	139389	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	293696	PASS
199	198	5	9	6.8	20080	PASS
275	198	10	60	27.8	81659	PASS
365	198	1	100	3.5	10285	PASS
441	198	0.01	100	13.9	40797	PASS
442	442	50	100	100.0	265920	PASS
443	442	15	24	18.9	50208	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/30/2024	BNA_F	<u>BF141030.D</u>
Compound Name	Response	Retention Time
DDT	828346	13.51
DDD	20589	13.204
DDE	1143	12.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21732	850078	2.56

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141030.D
Acq On : 30 Dec 2024 14:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 30 15:22:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

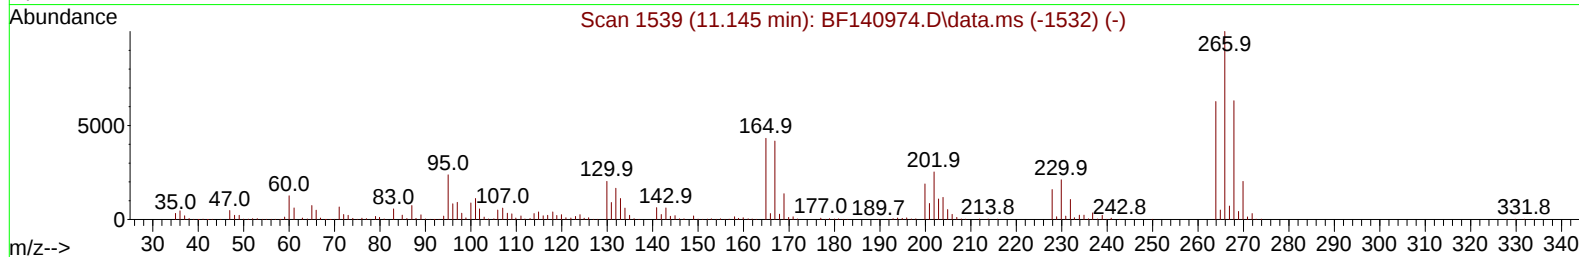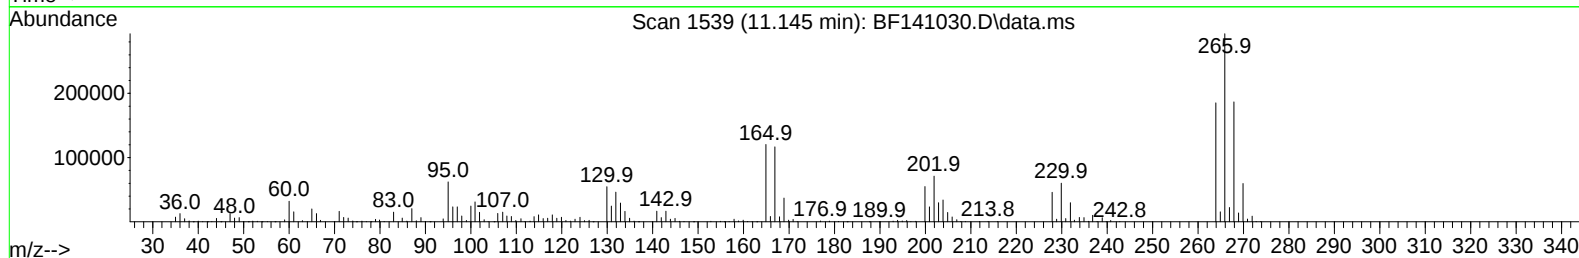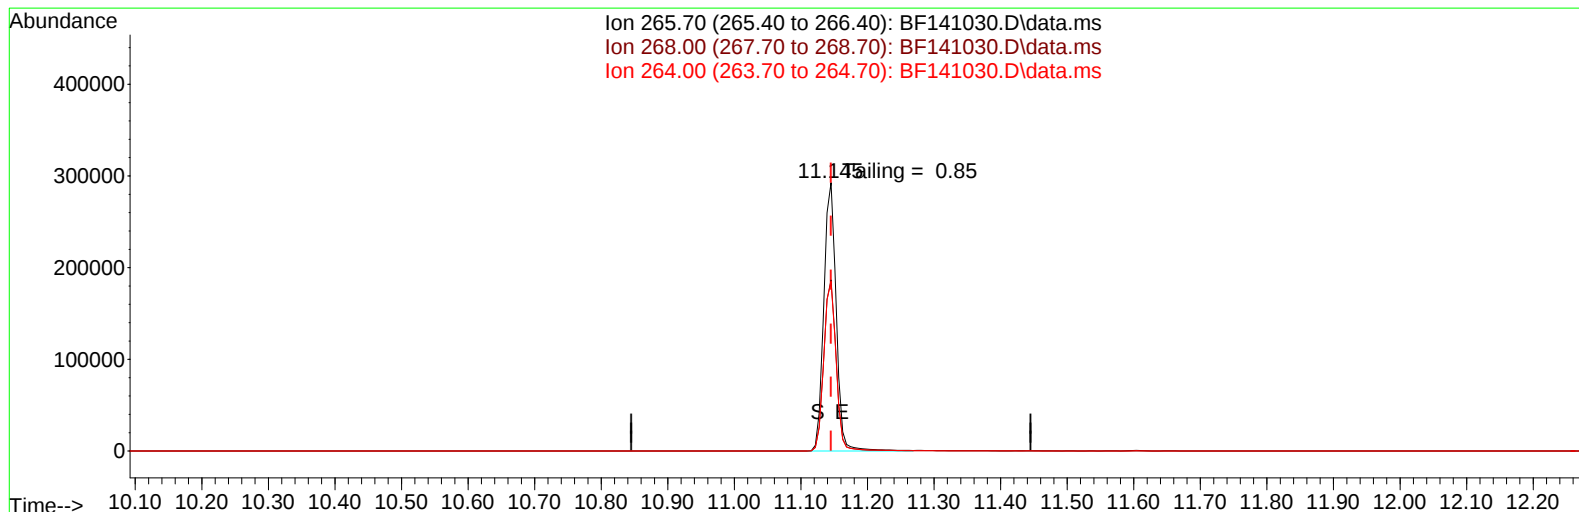

TIC: BF141030.D\data.ms

(70) Pentachlorophenol (C)

11.145min (+ 0.000) 50298.96 ng




response 379636

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.75
264.00	62.80	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF123024\
Data File : BF141030.D
Acq On : 30 Dec 2024 14:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 30 15:22:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

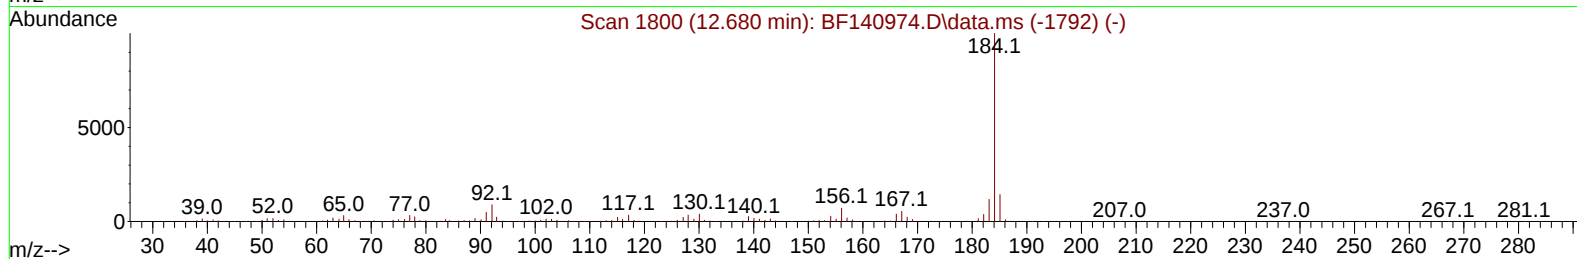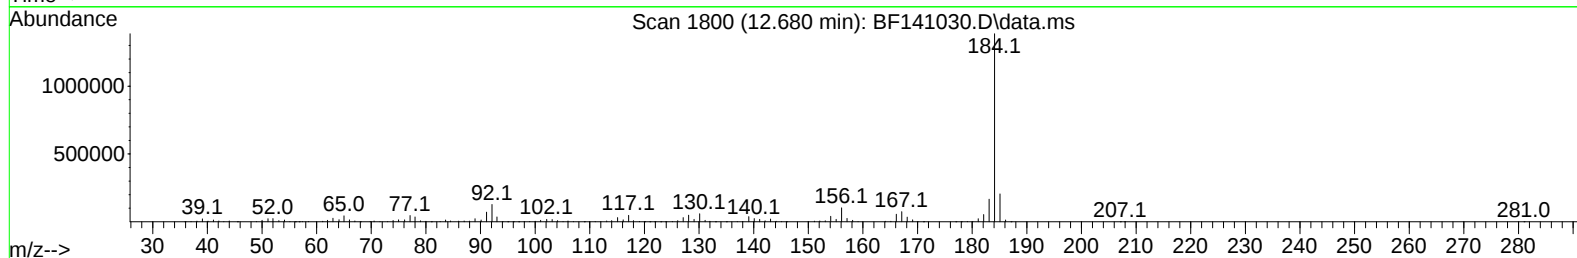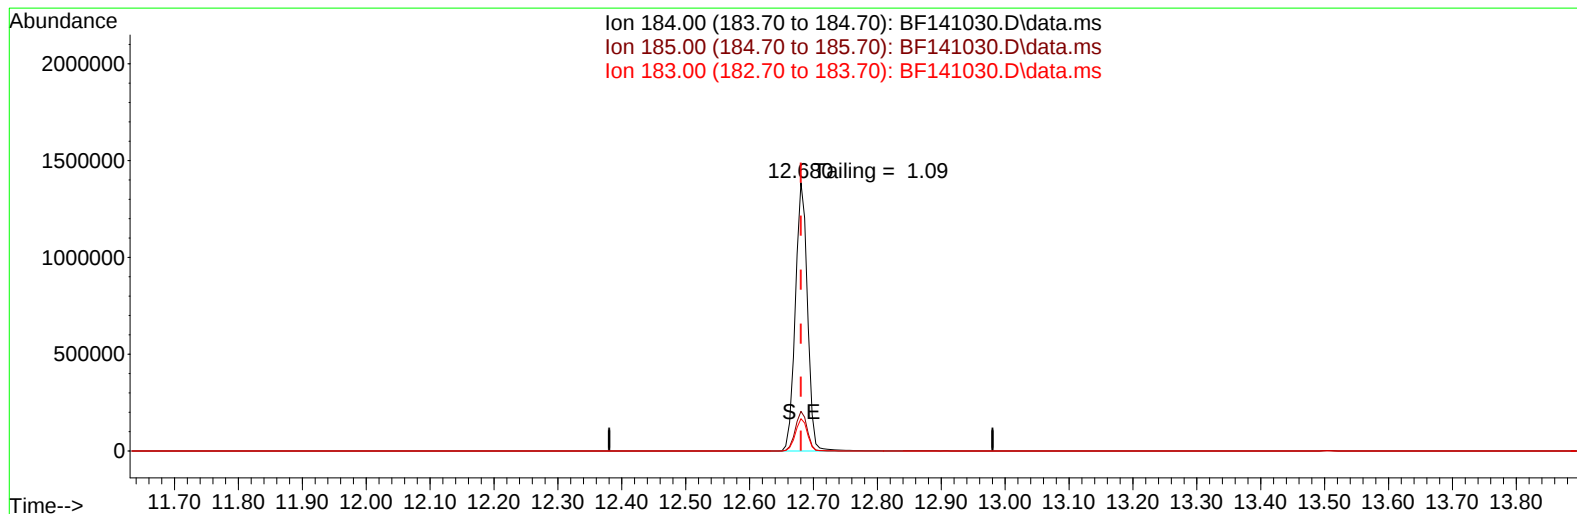

TIC: BF141030.D\data.ms

(77) Benzidine

12.680min (-0.000) 126224.53 ng

response 1846000

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.80
183.00	11.70	12.03
0.00	0.00	0.00