


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF123124\  
Data File : BF141046.D  
Acq On : 31 Dec 2024 09:24  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122624.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Dec 27 00:31:16 2024

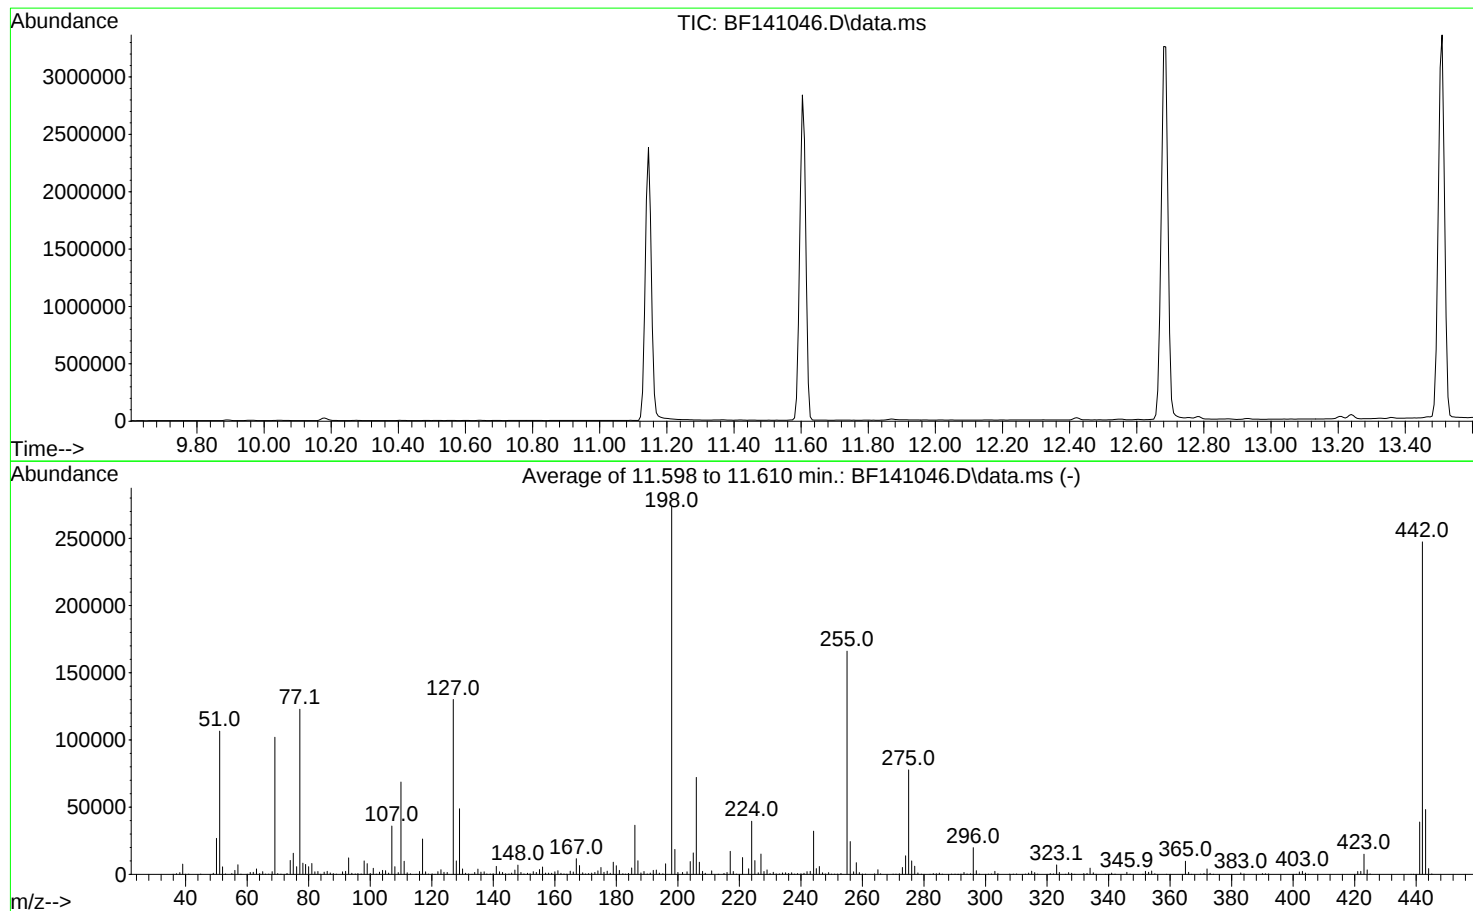

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 38.9         | 106613     | PASS                |
| 68             | 69              | 0.00            | 2               | 2.0          | 2008       | PASS                |
| 69             | 198             | 0.00            | 100             | 37.3         | 102035     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 571        | PASS                |
| 127            | 198             | 10              | 80              | 47.5         | 130099     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 273728     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 18630      | PASS                |
| 275            | 198             | 10              | 60              | 28.4         | 77821      | PASS                |
| 365            | 198             | 1               | 100             | 3.6          | 9770       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.2         | 38936      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 247424     | PASS                |
| 443            | 442             | 15              | 24              | 19.5         | 48189      | PASS                |

### DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 12/31/2024    | BNA_F            | <u>BF141046.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 862159           | 13.51              |
| DDD           | 13357            | 13.239             |
| DDE           | 935              | 12.874             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 14292         | 876451           | 1.63               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF123124\  
Data File : BF141046.D  
Acq On : 31 Dec 2024 09:24  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Dec 31 10:36:33 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 27 00:31:16 2024  
Response via : Initial Calibration

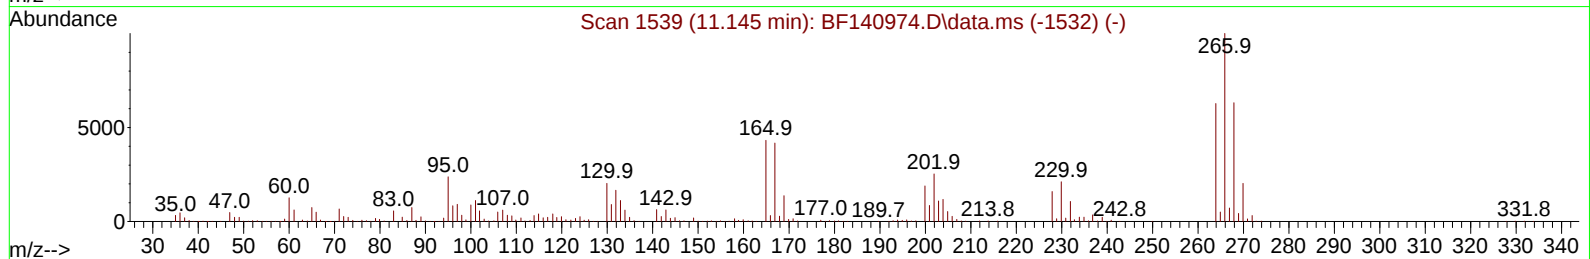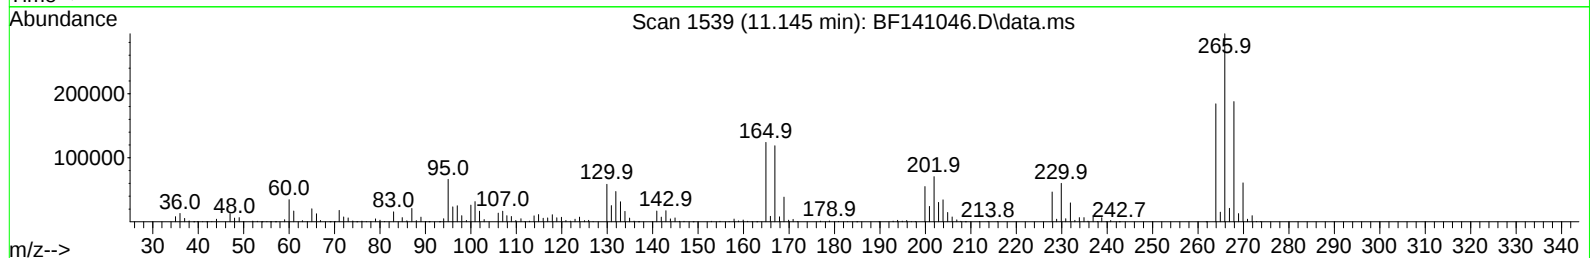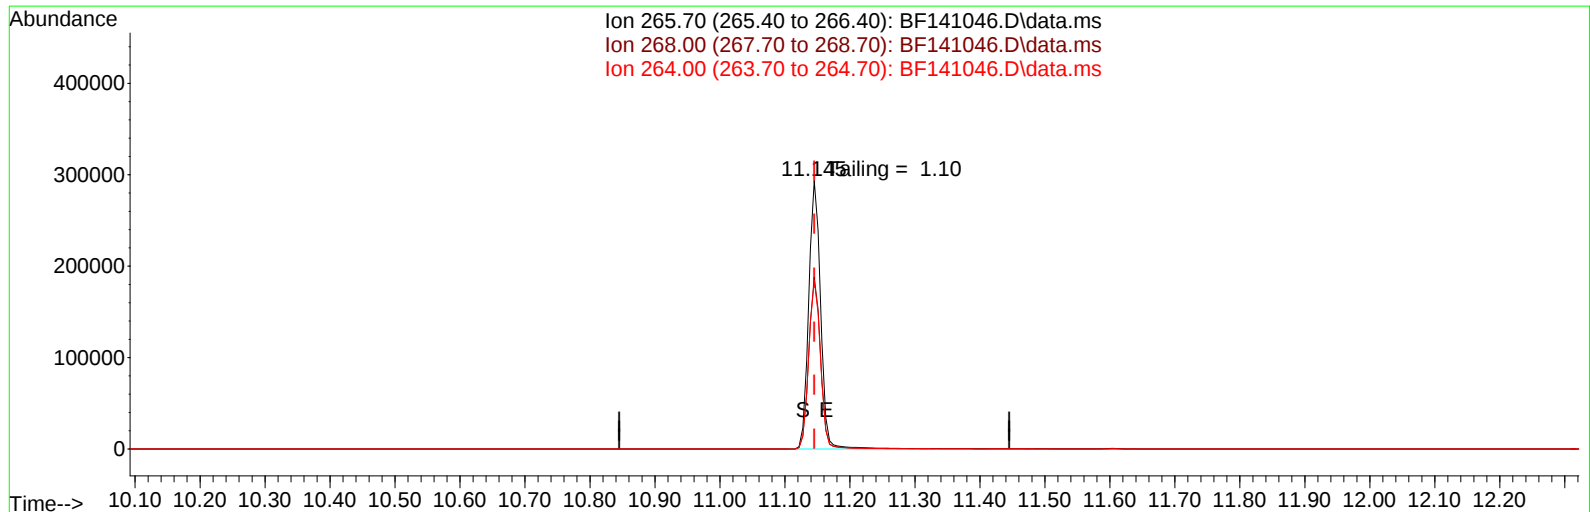

TIC: BF141046.D\data.ms

**(70) Pentachlorophenol (C)**

**11.145min (+ 0.000) 35586.54 ng**




**response 377139**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.10  | 63.90  |
| 264.00 | 62.80  | 62.76  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF123124\  
Data File : BF141046.D  
Acq On : 31 Dec 2024 09:24  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Dec 31 10:36:33 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF122624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 27 00:31:16 2024  
Response via : Initial Calibration

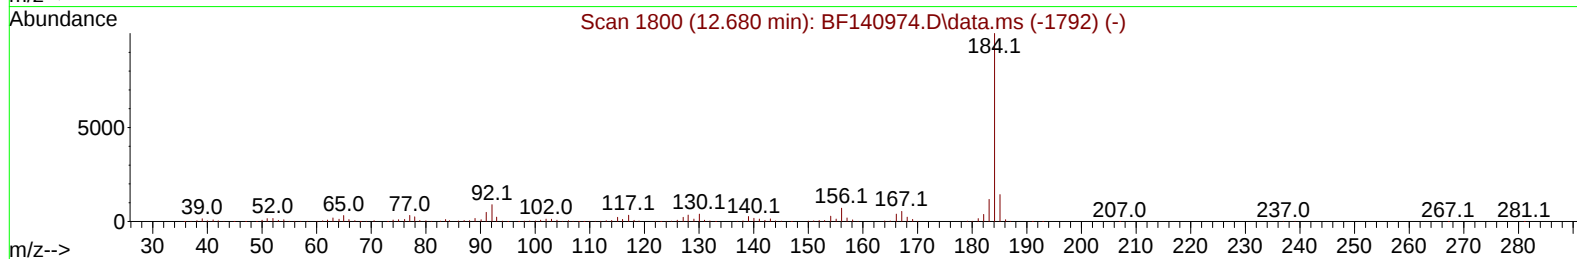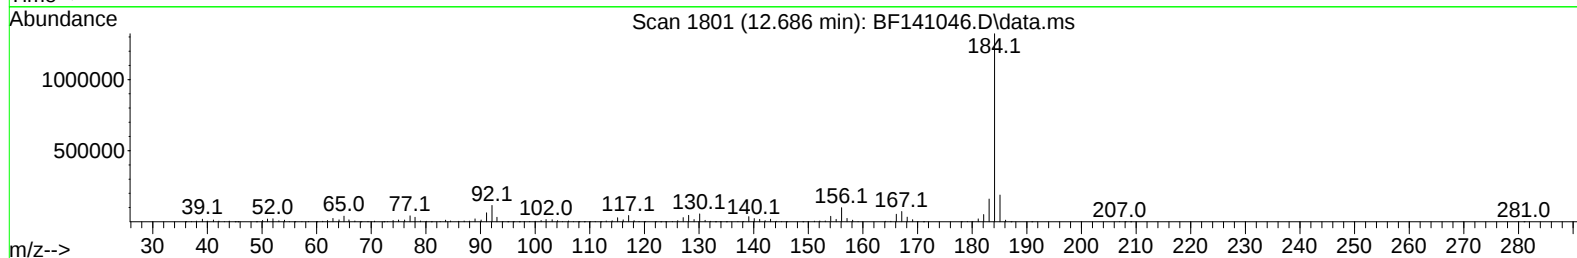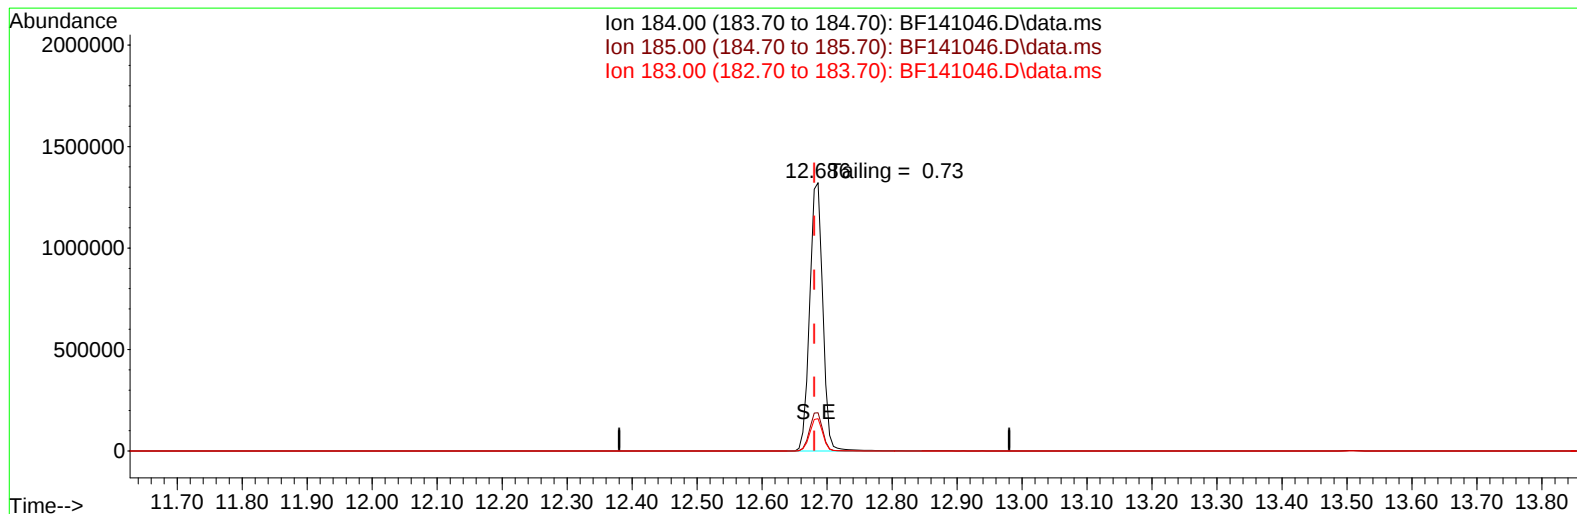

TIC: BF141046.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 81977.79 ng

response 1855528

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.30  | 14.27  |
| 183.00 | 11.70  | 12.07  |
| 0.00   | 0.00   | 0.00   |