
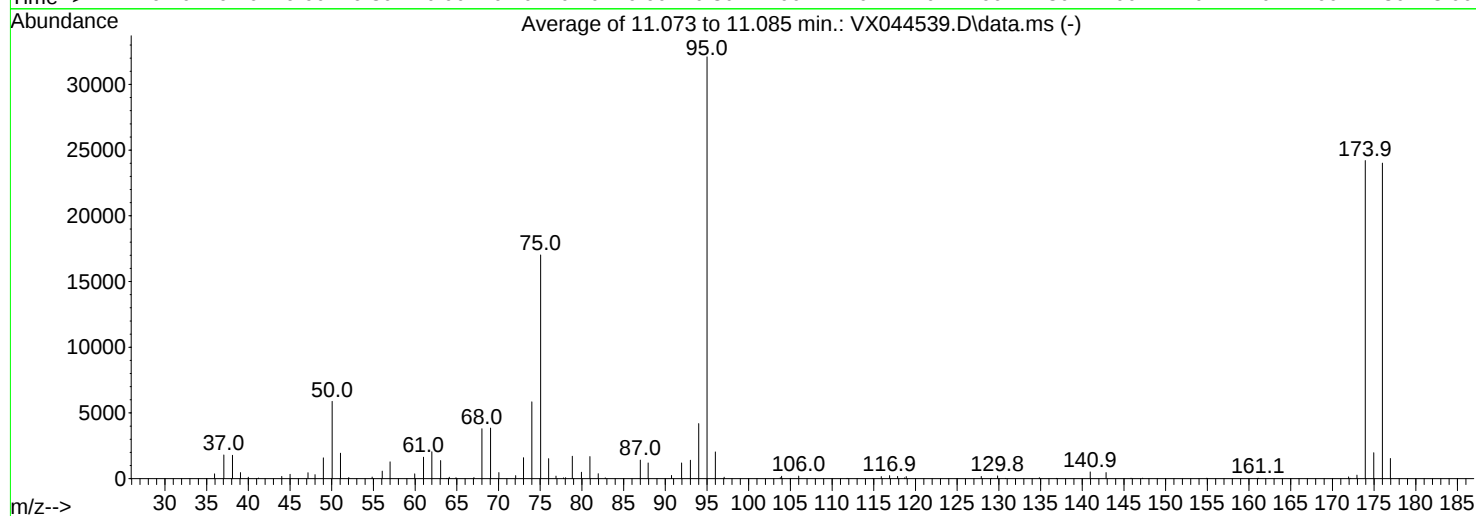


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX123124\
Data File : VX044539.D
Acq On : 30 Dec 2024 12:39
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Title : SW846 8260
Last Update : Thu Dec 28 04:28:14 2024

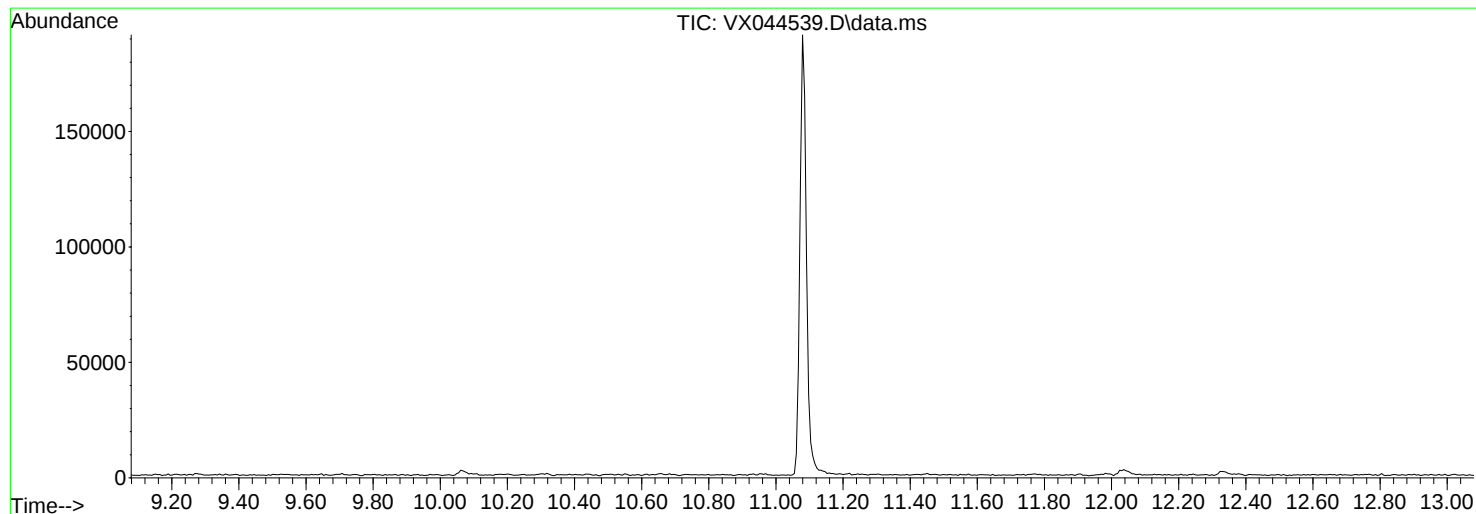

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	5876	PASS
75	95	30	60	53.0	17024	PASS
95	95	100	100	100.0	32099	PASS
96	95	5	9	6.3	2033	PASS
173	174	0.00	2	1.1	271	PASS
174	95	50	100	75.4	24205	PASS
175	174	5	9	8.2	1978	PASS
176	174	95	101	99.2	24012	PASS
177	176	5	9	6.4	1533	PASS