


Instrument I		IC-1	Analyst: NF		Method: J0.0 / 9056A		Method name		date time	initial wt/Final Vc	Analyst
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	initial wt/Final Vc	Analyst
STD1	0	0	0	0	0	0	0	IC1-121824	12/18/2024 10:39	10	NF/IZ
STD2	0.319	0.475	0.485	1.586	0.405	0.794	2.525	IC1-121824	12/18/2024 11:00	10	NF/IZ
STD3	0.867	1.29	1.286	4.307	1.073	2.153	6.454	IC1-121824	12/18/2024 11:22	10	NF/IZ
STD4	1.065	1.59	1.587	5.29	1.327	2.68	7.947	IC1-121824	12/18/2024 11:43	10	NF/IZ
STD5	1.968	2.98	2.975	9.935	2.472	4.928	14.761	IC1-121824	12/18/2024 12:04	10	NF/IZ
STD6	3.929	5.897	5.891	19.654	4.906	9.805	29.16	IC1-121824	12/18/2024 12:26	10	NF/IZ
STD7	5.052	7.568	7.575	25.229	6.317	12.641	37.652	IC1-121824	12/18/2024 12:47	10	NF/IZ
ICV	2.021	3.088	3.087	10.28	2.565	5.117	15.271	IC1-121824	12/18/2024 13:09	10	NF/IZ
ICB	0	0	0	0	0	0	0	IC1-121824	12/18/2024 13:30	10	NF/IZ
CCV	2.082	3.132	3.1	10.411	2.596	4.919	15.65	IC1-121824	12/26/2024 9:53	10	NF/IZ
CCB	0	0	0	0	0	0	0	IC1-121824	12/26/2024 10:14	10	NF/IZ
LB134081BLS	0	0	0	0	0	0	0	IC1-121824	12/26/2024 10:36	5.00g/100ML	NF/IZ
LB134081BSS	2.078	3.122	3.113	10.431	2.599	5.125	15.617	IC1-121824	12/26/2024 10:57	5.00g/100ML	NF/IZ
P5382-01	0.281	0.293	0	0	0.182	0	1.688	IC1-121824	12/26/2024 11:19	5.02g/100ML	NF/IZ
P5382-01MS	2.152	3.358	3.184	10.667	2.663	4.618	16.373	IC1-121824	12/26/2024 11:40	5.03g/100ML	NF/IZ
P5382-01MSD	2.168	3.389	3.181	10.625	2.669	4.458	16.37	IC1-121824	12/26/2024 12:02	5.03g/100ML	NF/IZ
P5382-02	0.355	0.401	0	0	0.177	0	1.466	IC1-121824	12/26/2024 12:24	5.01g/100ML	NF/IZ
P5382-03	0.286	0.3	0	0	0	0	1.383	IC1-121824	12/26/2024 12:45	5.02g/100ML	NF/IZ
CCV	2.065	3.141	3.111	10.43	2.6	5.262	15.514	IC1-121824	12/26/2024 13:07	10	NF/IZ
CCB	0	0	0	0	0	0	0	IC1-121824	12/26/2024 13:28	10	NF/IZ

Fluoride (Anions)

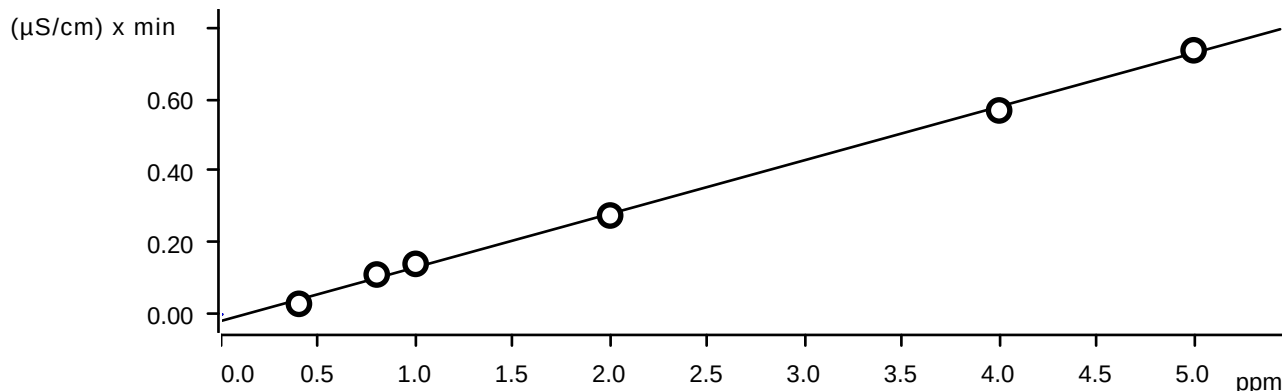


Function: $A = -0.0183596 + 0.0149351 \times Q$

Relative standard deviation 3.731557 %

Correlation coefficient 0.999324

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	0.400	10.0	1.0	1.0	0.029	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.141	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.276	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.568	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.736	STD7	2024-12-18 12:47:45 UTC-5	used

Chloride (Anions)

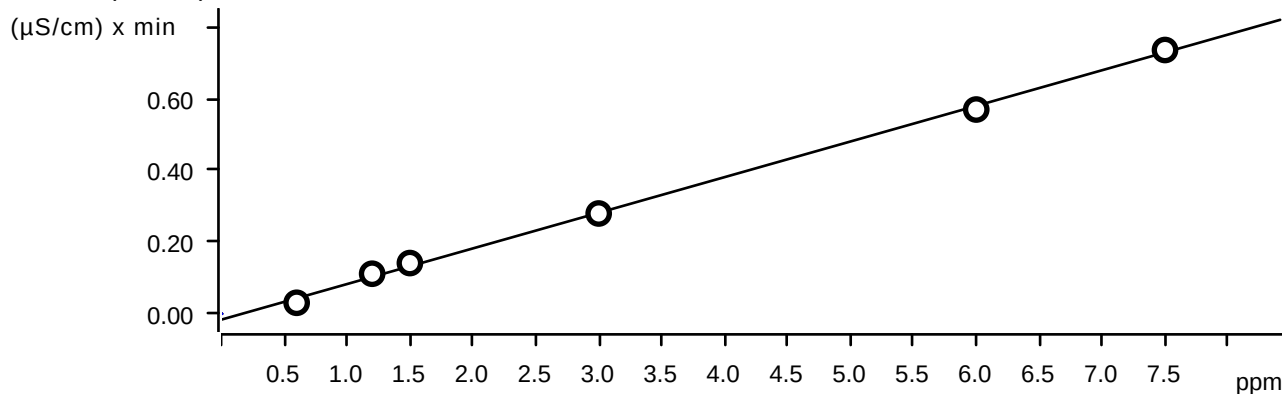


Function: $A = -0.0165562 + 9.93613E-3 \times Q$

Relative standard deviation 3.466087 %

Correlation coefficient 0.999410

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	0.600	10.0	1.0	1.0	0.031	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.112	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.141	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.280	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.569	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.735	STD7	2024-12-18 12:47:45 UTC-5	used

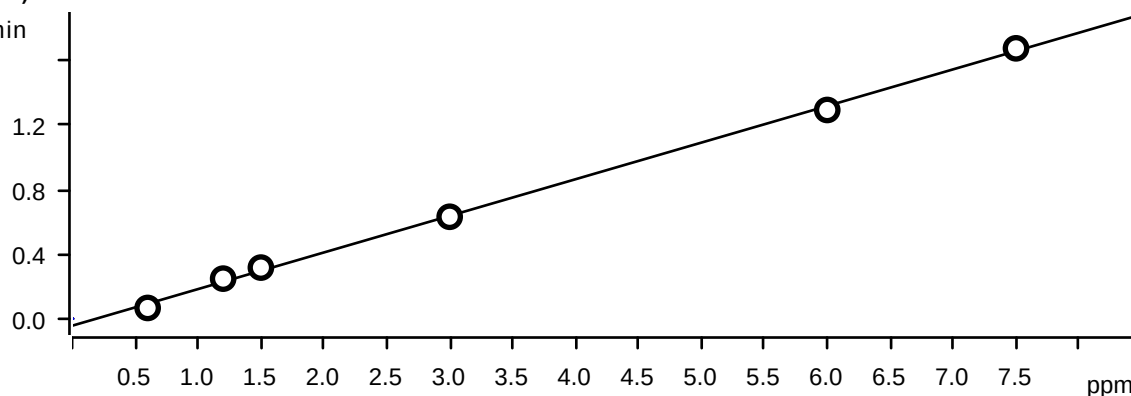Nitrite (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0434679 + 0.0226901 \times Q$


Relative standard deviation 3.455351 %

Correlation coefficient 0.999423

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	0.600	10.0	1.0	1.0	0.067	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.248	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.317	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.632	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.293	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.675	STD7	2024-12-18 12:47:45 UTC-5	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) x min

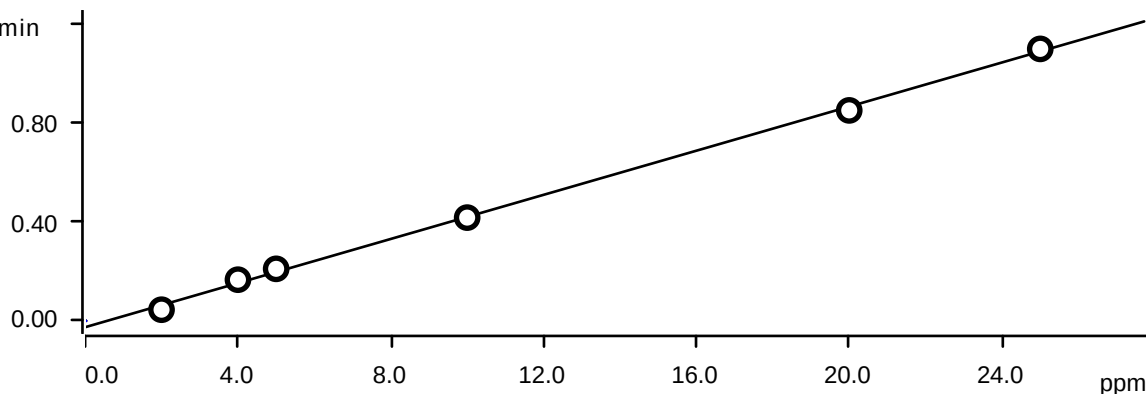

Function: $A = -0.0255661 + 4.44233E-3 \times Q$


Relative standard deviation: 3.478545 %

Correlation coefficient: 0.999408

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	2.000	10.0	1.0	1.0	0.045	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.166	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.209	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.416	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.848	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.095	STD7	2024-12-18 12:47:45 UTC-5	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) x min

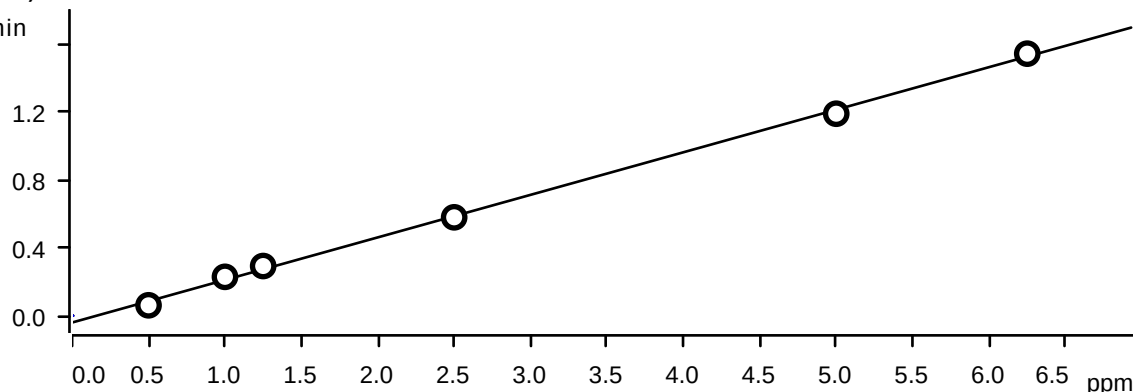


Function: $A = -0.0400484 + 0.0250507 \times Q$

Relative standard deviation: 3.586984 %

Correlation coefficient: 0.999378

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	0.500	10.0	1.0	1.0	0.061	STD2	2024-12-18 11:00:37 UTC-5	used

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 3	1	1.000	10.0	1.0	1.0	0.229	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.292	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.579	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.189	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.542	STD7	2024-12-18 12:47:45 UTC-5	used

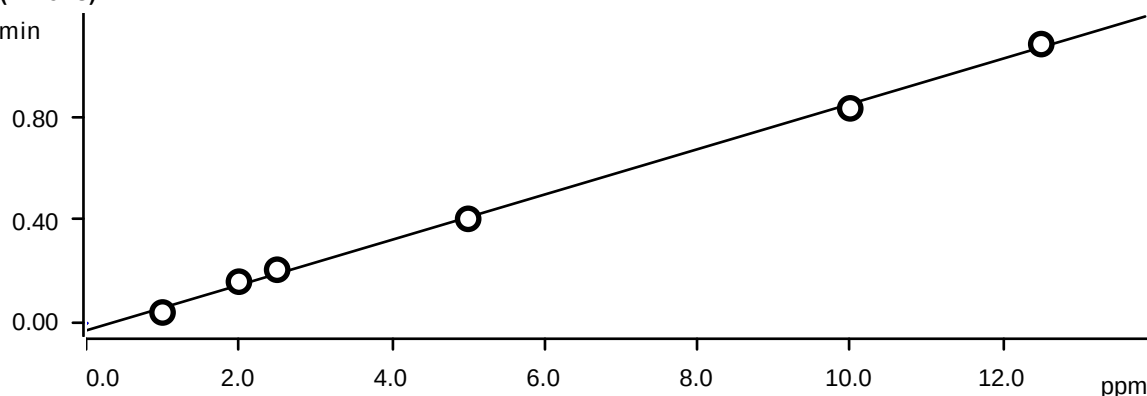
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0282076 + 8.77175E-3 \times Q$

Relative standard deviation 3.880200 %

Correlation coefficient 0.999273

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	1.000	10.0	1.0	1.0	0.041	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.161	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.207	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.404	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.832	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.081	STD7	2024-12-18 12:47:45 UTC-5	used

Sulfate (Anions)

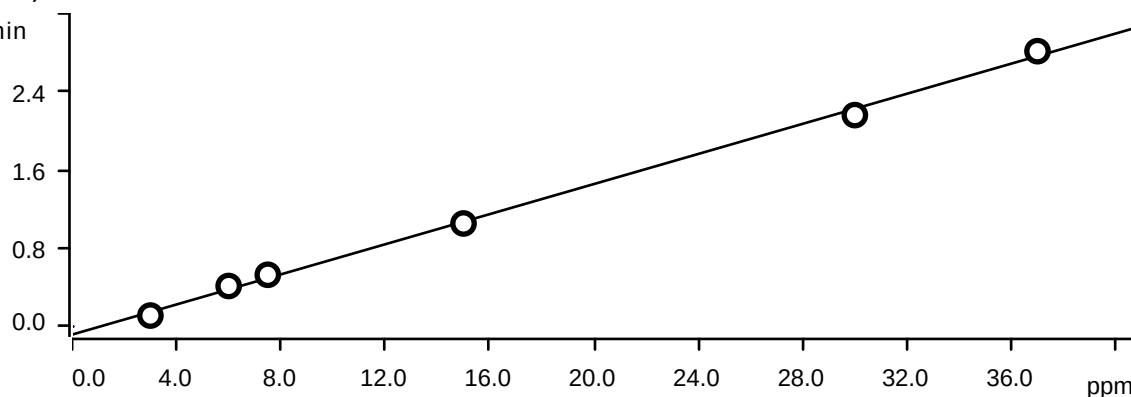 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0827937 + 7.69466E-3 \times Q$

Relative standard deviation 4.394299 %

Correlation coefficient 0.999072

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 2	1	3.000	10.0	1.0	1.0	0.112	STD2	2024-12-18 11:00:37 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.414	STD3	2024-12-18 11:22:01 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.529	STD4	2024-12-18 11:43:26 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.053	STD5	2024-12-18 12:04:52 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.161	STD6	2024-12-18 12:26:18 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.814	STD7	2024-12-18 12:47:45 UTC-5	used


Sample data

Ident STD1
Sample type Standard 1
Determination start 2024-12-18 10:39:14 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

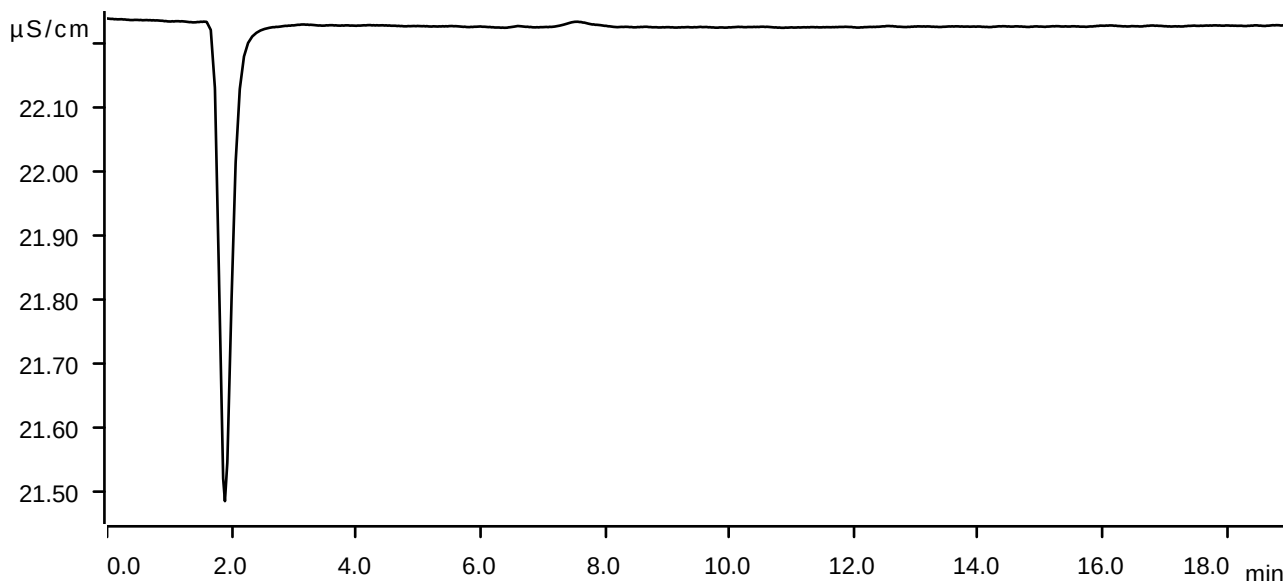


Sample data

Ident STD2
Sample type Standard 2
Determination start 2024-12-18 11:00:37 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

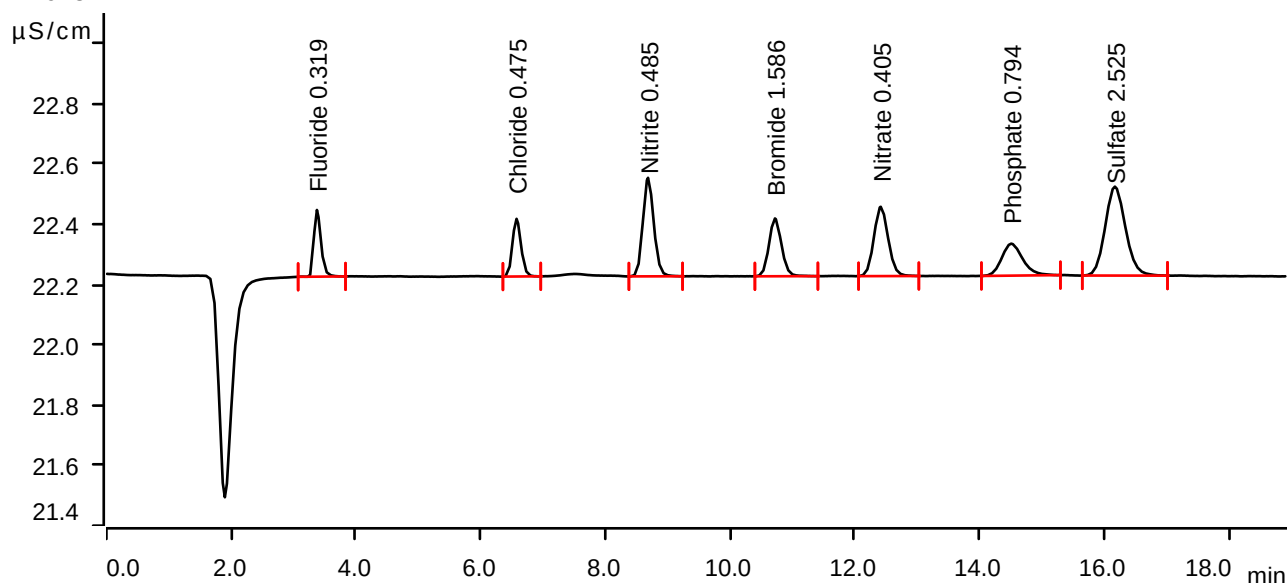

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.377	0.0293	0.221	0.319	Fluoride
2	6.577	0.0307	0.191	0.475	Chloride
3	8.685	0.0666	0.327	0.485	Nitrite
4	10.720	0.0449	0.192	1.586	Bromide
5	12.415	0.0613	0.230	0.405	Nitrate
6	14.510	0.0414	0.106	0.794	Phosphate
7	16.170	0.1115	0.295	2.525	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2024-12-18 11:22:01 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.09 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

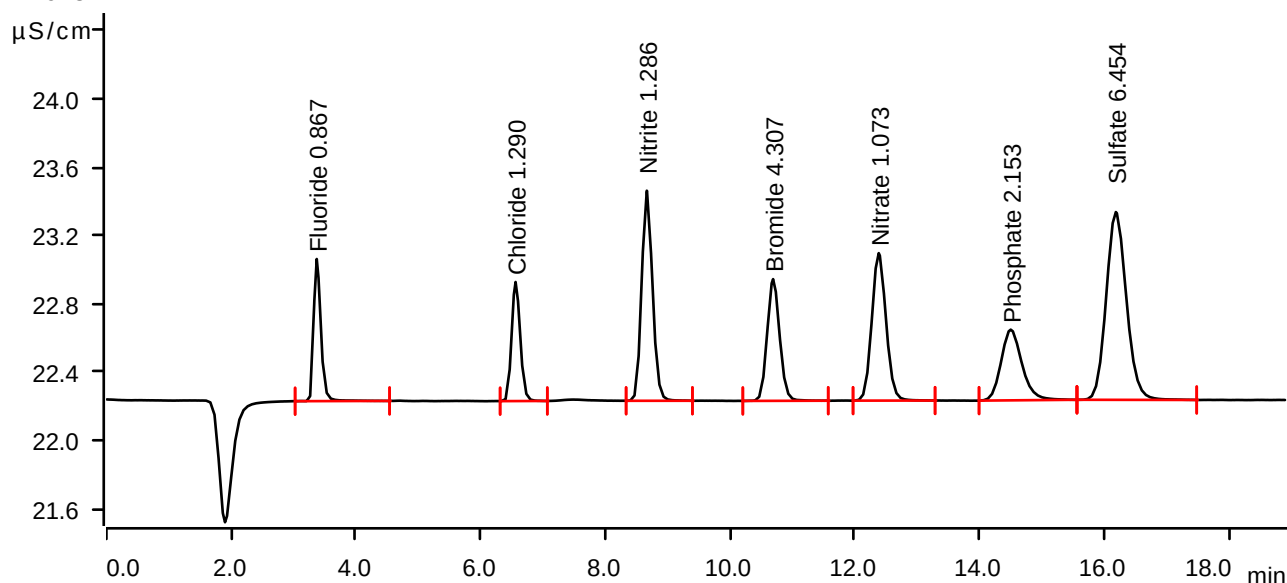

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.373	0.1111	0.832	0.867	Fluoride
2	6.562	0.1116	0.697	1.290	Chloride
3	8.665	0.2483	1.230	1.286	Nitrite
4	10.690	0.1658	0.713	4.307	Bromide
5	12.383	0.2288	0.864	1.073	Nitrate
6	14.500	0.1606	0.414	2.153	Phosphate
7	16.185	0.4138	1.100	6.454	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2024-12-18 11:43:26 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.87 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

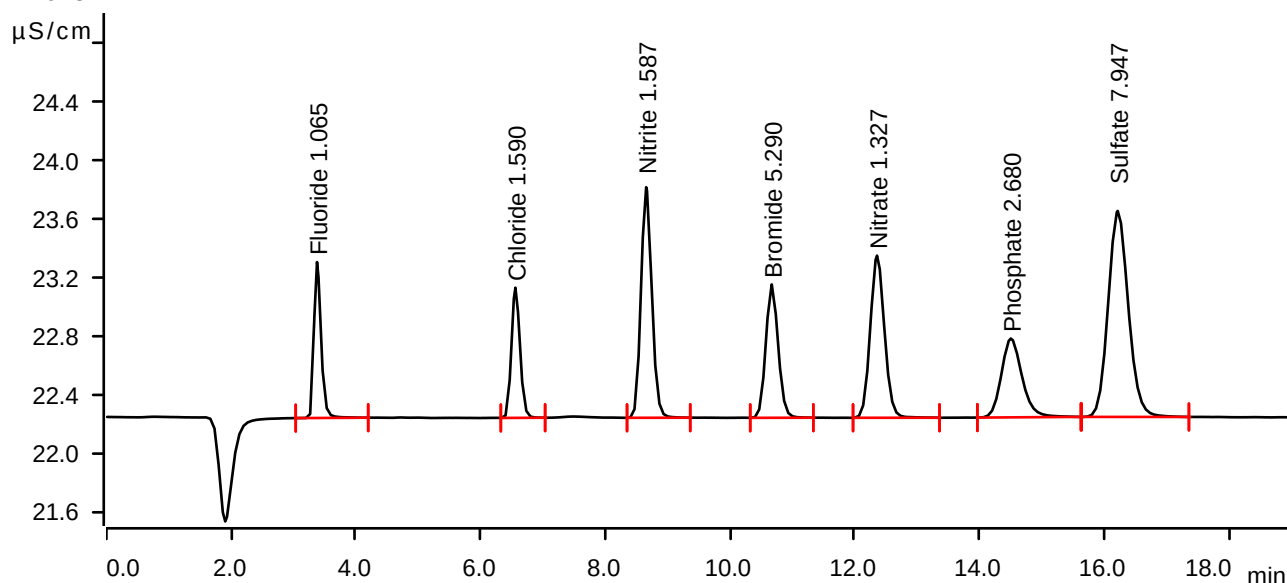

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.1407	1.065	1.065	Fluoride
2	6.558	0.1414	0.890	1.590	Chloride
3	8.655	0.3167	1.575	1.587	Nitrite
4	10.668	0.2094	0.911	5.290	Bromide
5	12.357	0.2924	1.108	1.327	Nitrate
6	14.502	0.2069	0.539	2.680	Phosphate
7	16.215	0.5287	1.408	7.947	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2024-12-18 12:04:52 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.04 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

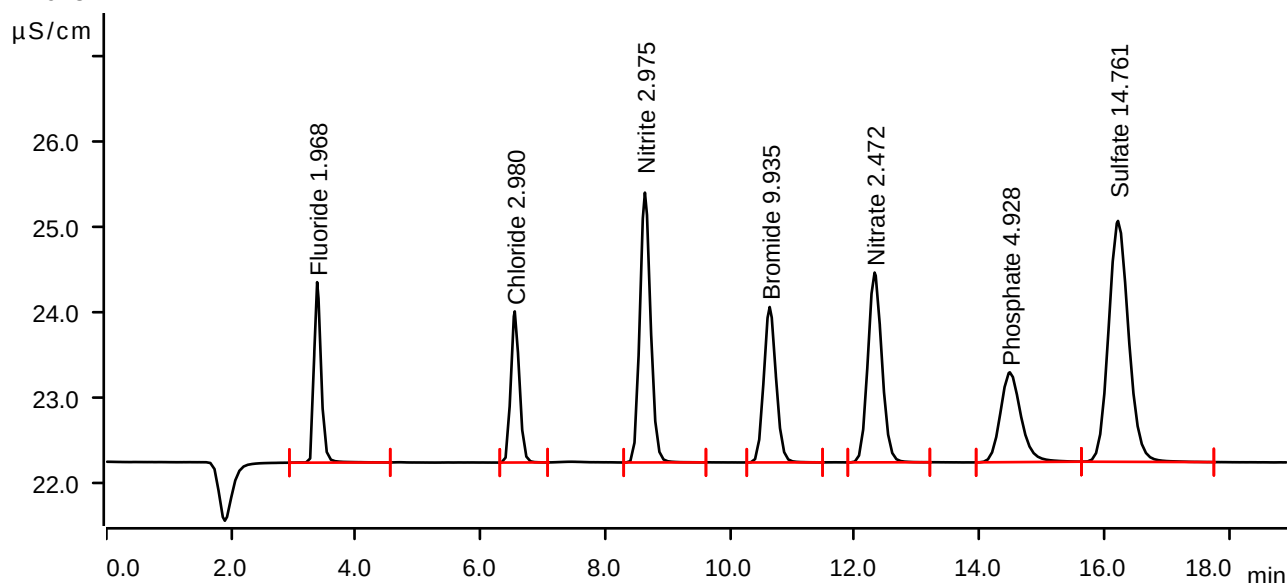

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.380	0.2755	2.114	1.968	Fluoride
2	6.548	0.2796	1.770	2.980	Chloride
3	8.635	0.6316	3.161	2.975	Nitrite
4	10.635	0.4158	1.820	9.935	Bromide
5	12.317	0.5791	2.223	2.472	Nitrate
6	14.485	0.4040	1.052	4.928	Phosphate
7	16.220	1.0530	2.822	14.761	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2024-12-18 12:26:18 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.98 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

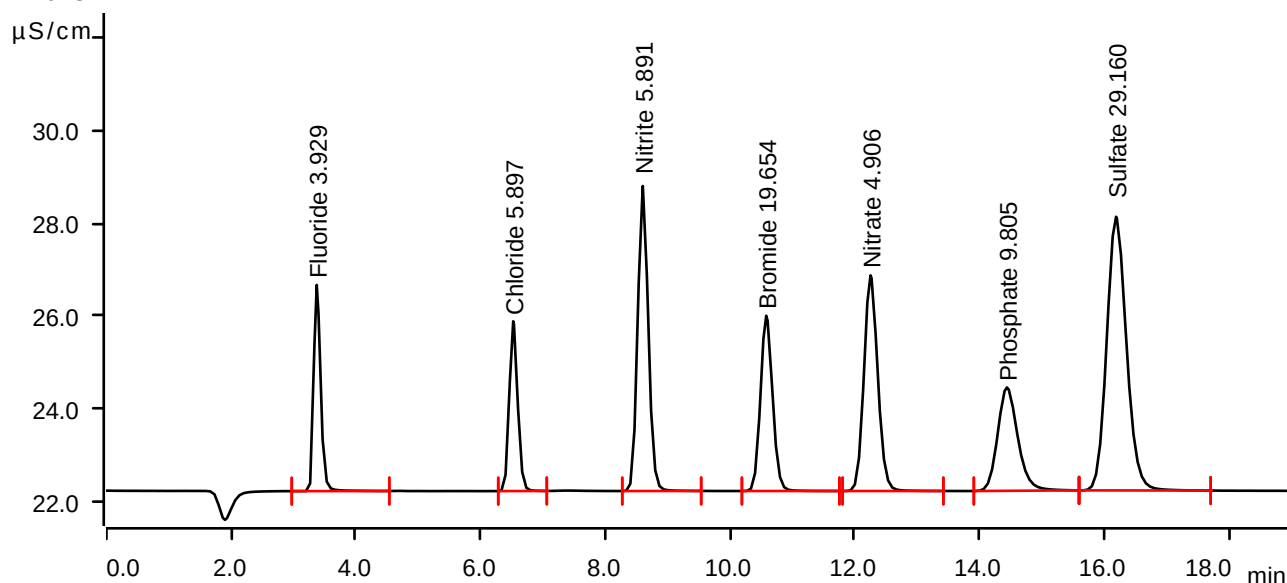

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.373	0.5685	4.427	3.929	Fluoride
2	6.523	0.5694	3.646	5.897	Chloride
3	8.602	1.2933	6.549	5.891	Nitrite
4	10.580	0.8475	3.765	19.654	Bromide
5	12.252	1.1889	4.631	4.906	Nitrate
6	14.438	0.8318	2.220	9.805	Phosphate
7	16.188	2.1610	5.877	29.160	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2024-12-18 12:47:45 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.75 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

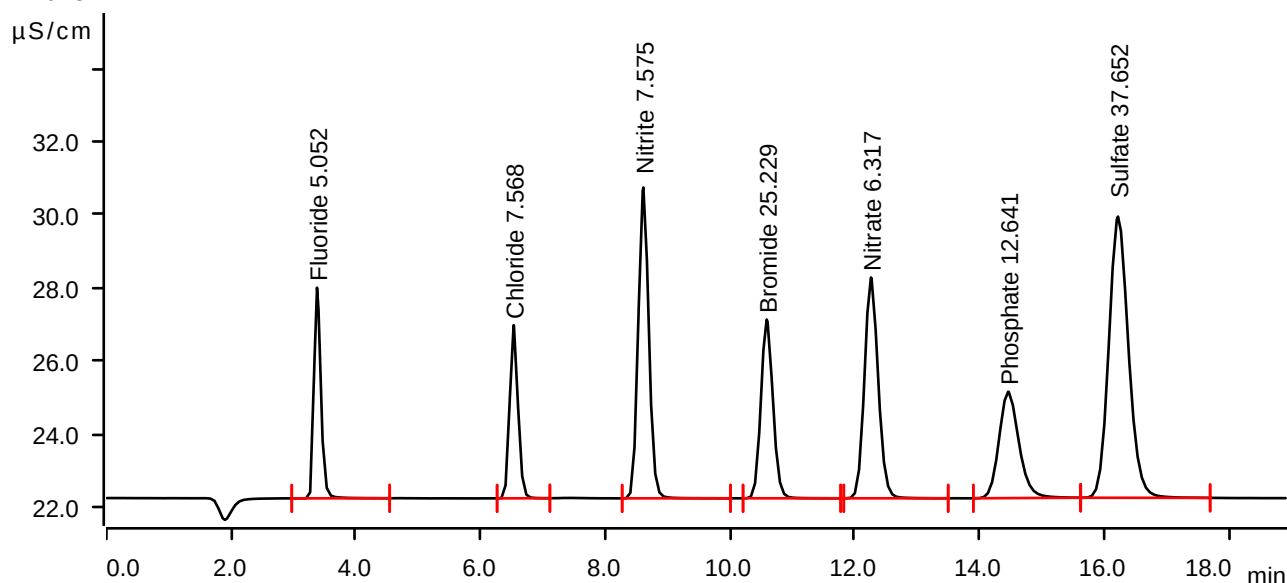

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.7362	5.758	5.052	Fluoride
2	6.530	0.7354	4.734	7.568	Chloride
3	8.610	1.6752	8.496	7.575	Nitrite
4	10.587	1.0952	4.888	25.229	Bromide
5	12.258	1.5424	6.037	6.317	Nitrate
6	14.458	1.0806	2.908	12.641	Phosphate
7	16.220	2.8144	7.686	37.652	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2024-12-18 13:09:13 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.87 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

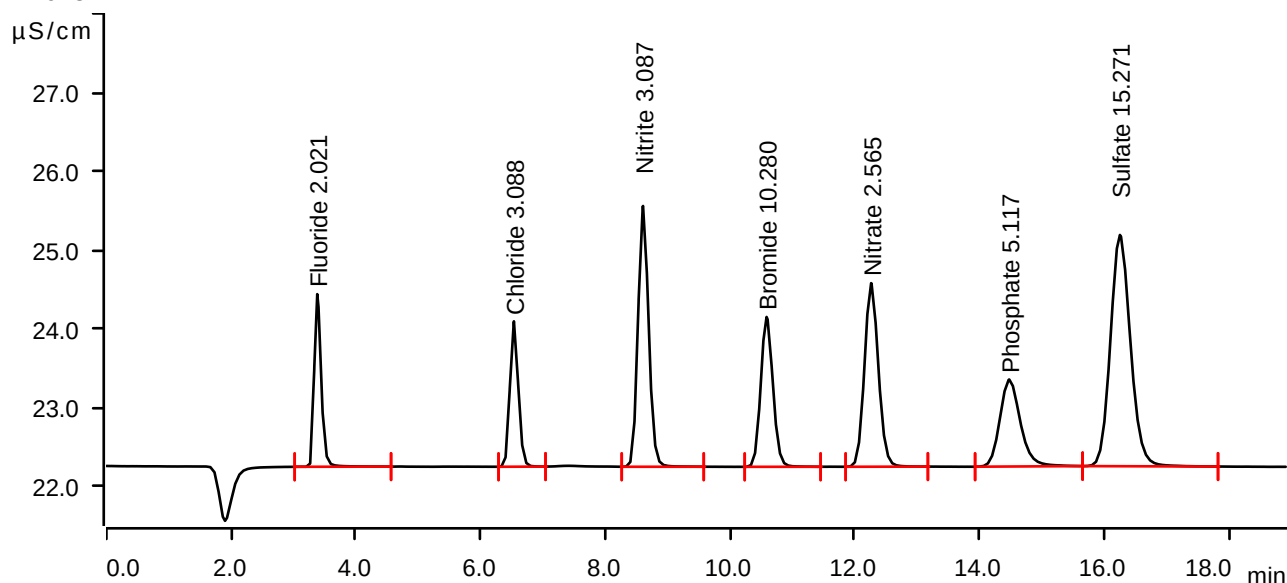

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.382	0.2835	2.190	2.021	Fluoride
2	6.533	0.2903	1.845	3.088	Chloride
3	8.605	0.6571	3.309	3.087	Nitrite
4	10.585	0.4311	1.902	10.280	Bromide
5	12.262	0.6024	2.329	2.565	Nitrate
6	14.477	0.4207	1.104	5.117	Phosphate
7	16.250	1.0923	2.934	15.271	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2024-12-18 13:30:41 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.64 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

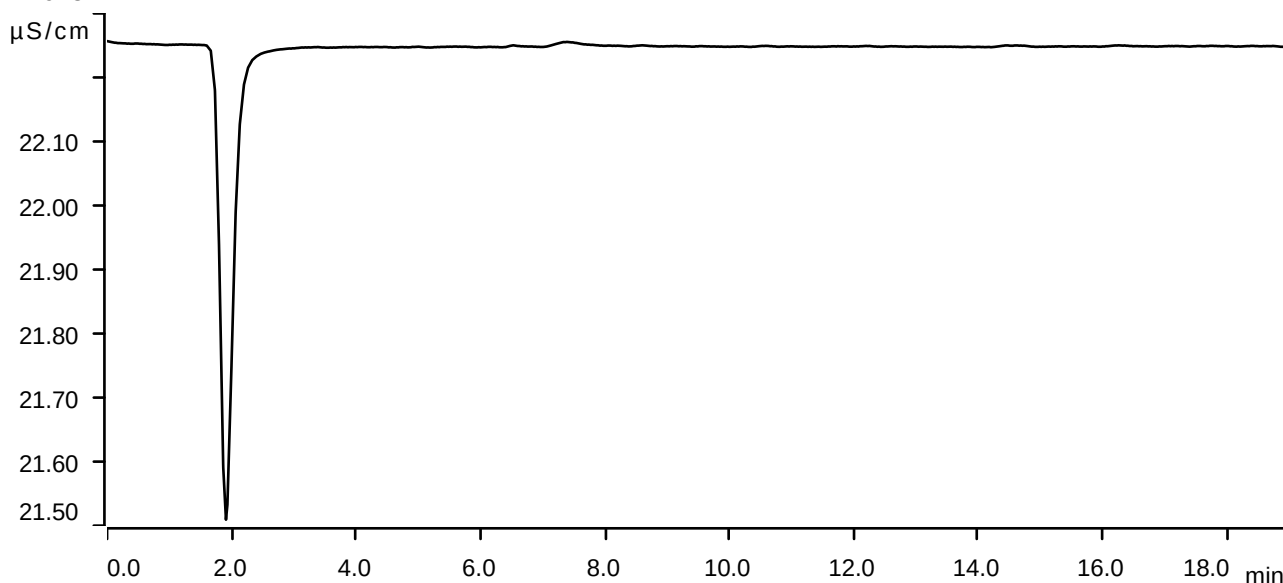


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-12-26 09:53:19 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

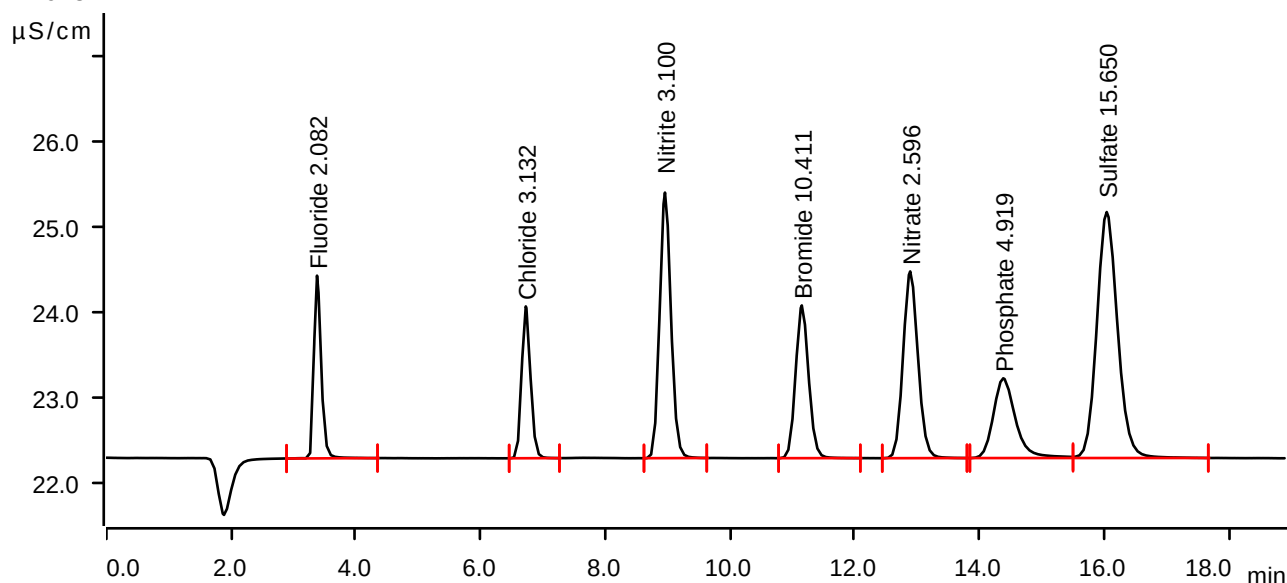

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.2877	2.140	2.082	Fluoride
2	6.725	0.2936	1.778	3.132	Chloride
3	8.957	0.6564	3.111	3.100	Nitrite
4	11.150	0.4335	1.789	10.411	Bromide
5	12.888	0.6057	2.187	2.596	Nitrate
6	14.380	0.3854	0.934	4.919	Phosphate
7	16.038	1.1096	2.881	15.650	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2024-12-26 10:14:49 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

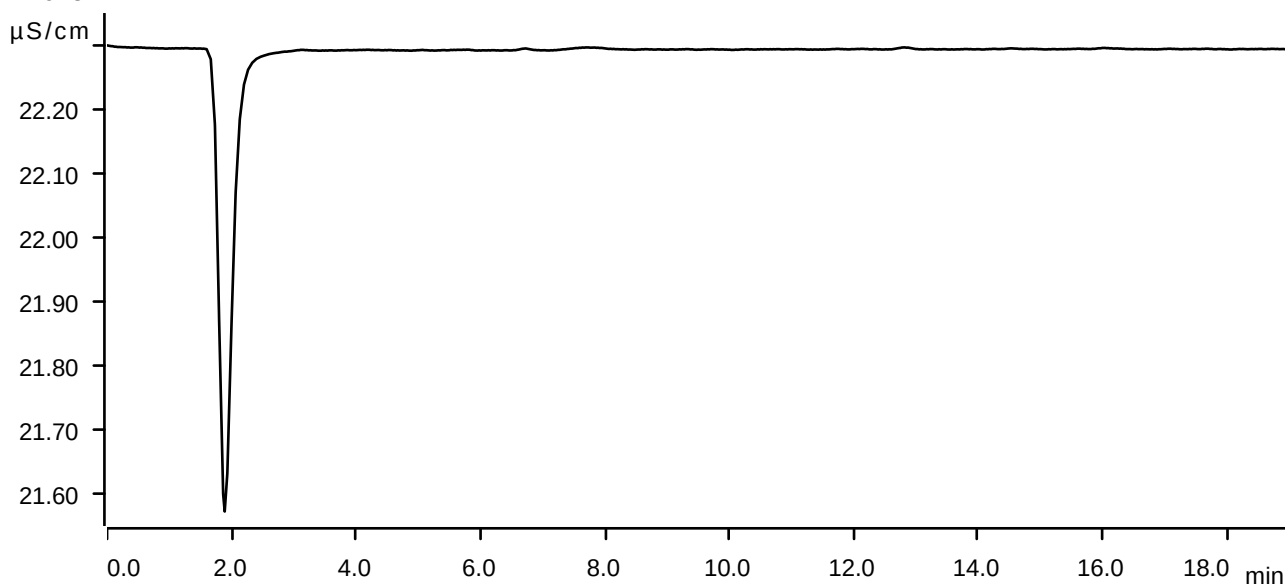


Sample data

Ident LB134081BLS
Sample type Sample
Determination start 2024-12-26 10:36:20 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

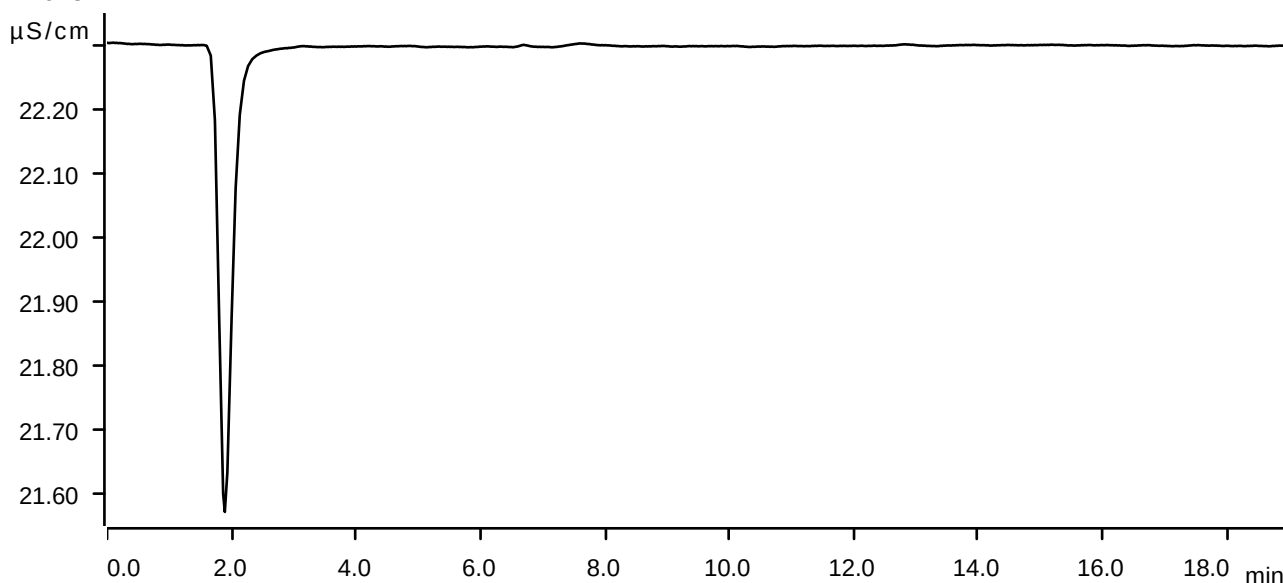


Sample data

Ident LB134081BSS
Sample type Check standard 1
Determination start 2024-12-26 10:57:52 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

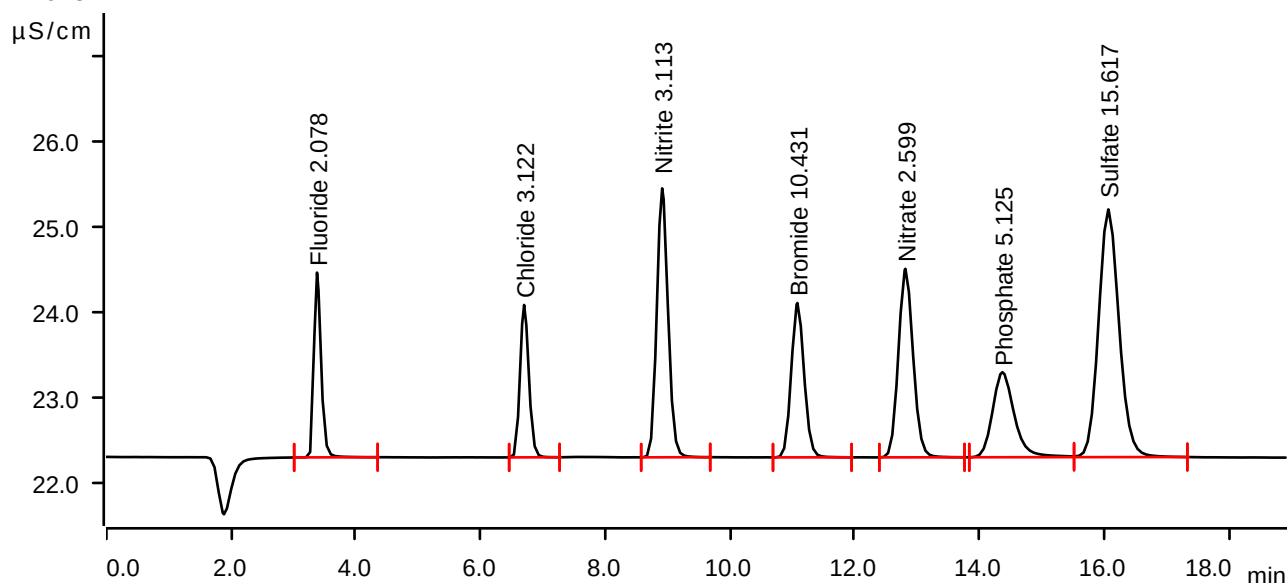

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.378	0.2871	2.164	2.078	Fluoride
2	6.698	0.2926	1.785	3.122	Chloride
3	8.912	0.6593	3.150	3.113	Nitrite
4	11.080	0.4344	1.808	10.431	Bromide
5	12.812	0.6063	2.209	2.599	Nitrate
6	14.367	0.4034	0.996	5.125	Phosphate
7	16.063	1.1071	2.901	15.617	Sulfate


Sample data

Ident P5382-01
Sample type Sample
Determination start 2024-12-26 11:19:25 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

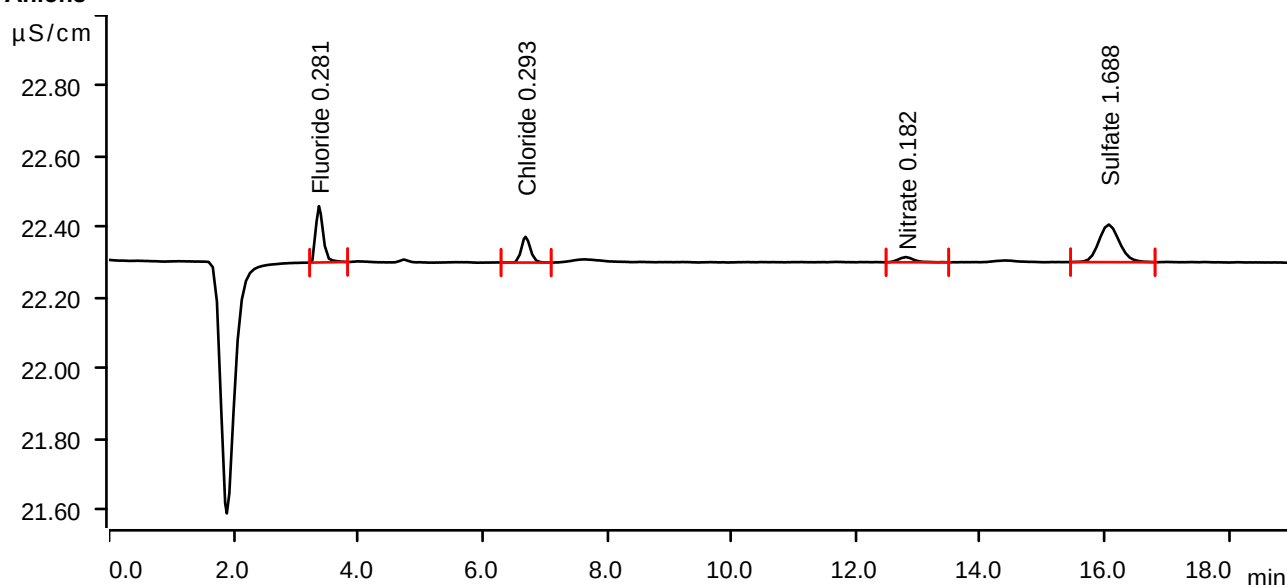

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.373	0.0218	0.160	0.281	Fluoride
2	6.693	0.0123	0.073	0.293	Chloride
3	12.807	0.0042	0.015	0.182	Nitrate
4	16.065	0.0409	0.106	1.688	Sulfate


Sample data

Ident P5382-01MS
Sample type Sample
Determination start 2024-12-26 11:40:59 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

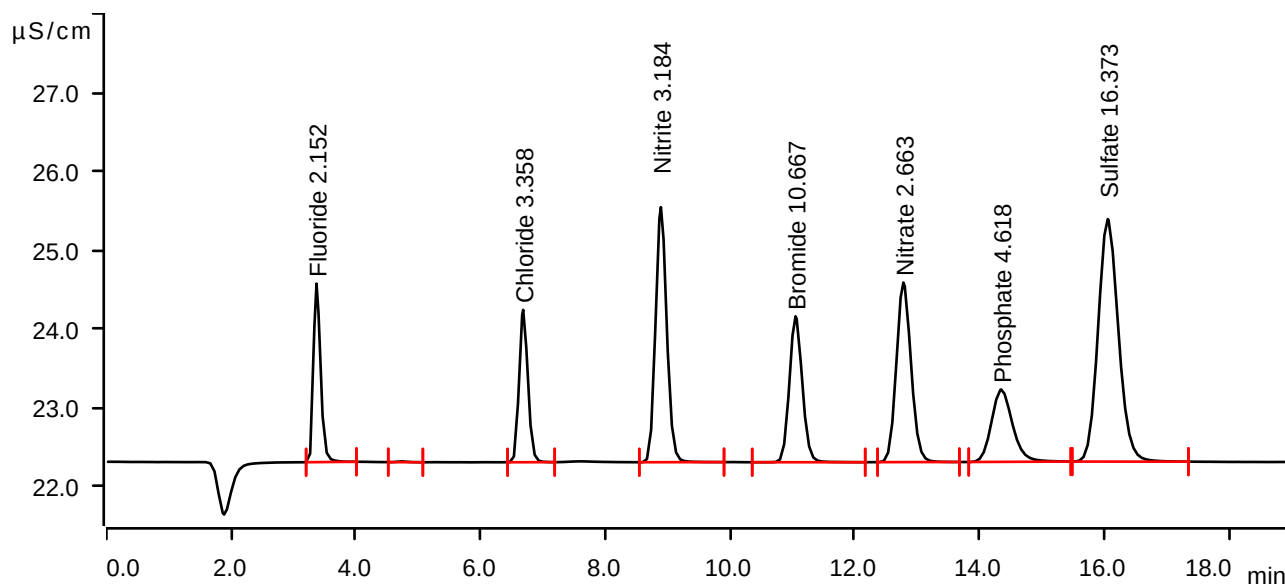

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.370	0.2980	2.265	2.152	Fluoride
2	4.737	0.0020	0.010	invalid	
3	6.683	0.3160	1.934	3.358	Chloride
4	8.892	0.6752	3.237	3.184	Nitrite
5	11.050	0.4448	1.852	10.667	Bromide
6	12.778	0.6224	2.279	2.663	Nitrate
7	14.347	0.3589	0.919	4.618	Phosphate
8	16.055	1.1650	3.077	16.373	Sulfate


Sample data

Ident P5382-01MSD
Sample type Sample
Determination start 2024-12-26 12:02:35 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

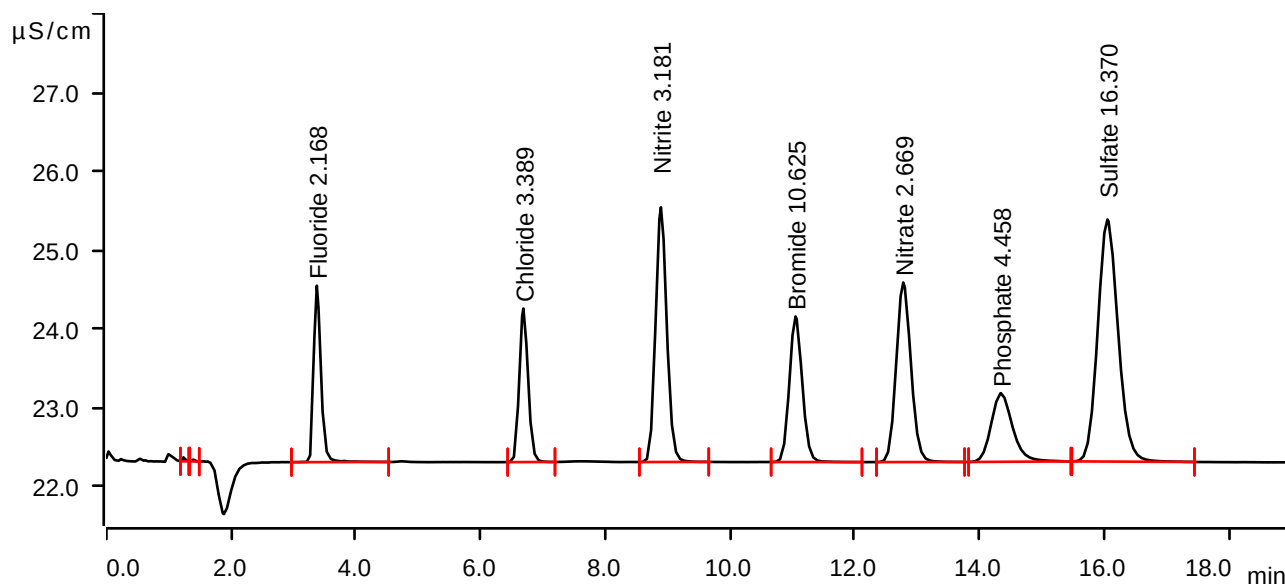

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	1.235	0.0029	0.051	invalid	
2	1.390	0.0013	0.023	invalid	
3	3.375	0.3003	2.239	2.168	Fluoride
4	6.687	0.3191	1.948	3.389	Chloride
5	8.892	0.6746	3.232	3.181	Nitrite
6	11.050	0.4430	1.848	10.625	Bromide
7	12.777	0.6238	2.278	2.669	Nitrate
8	14.343	0.3450	0.870	4.458	Phosphate
9	16.050	1.1648	3.072	16.370	Sulfate


Sample data

Ident P5382-02
Sample type Sample
Determination start 2024-12-26 12:24:10 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

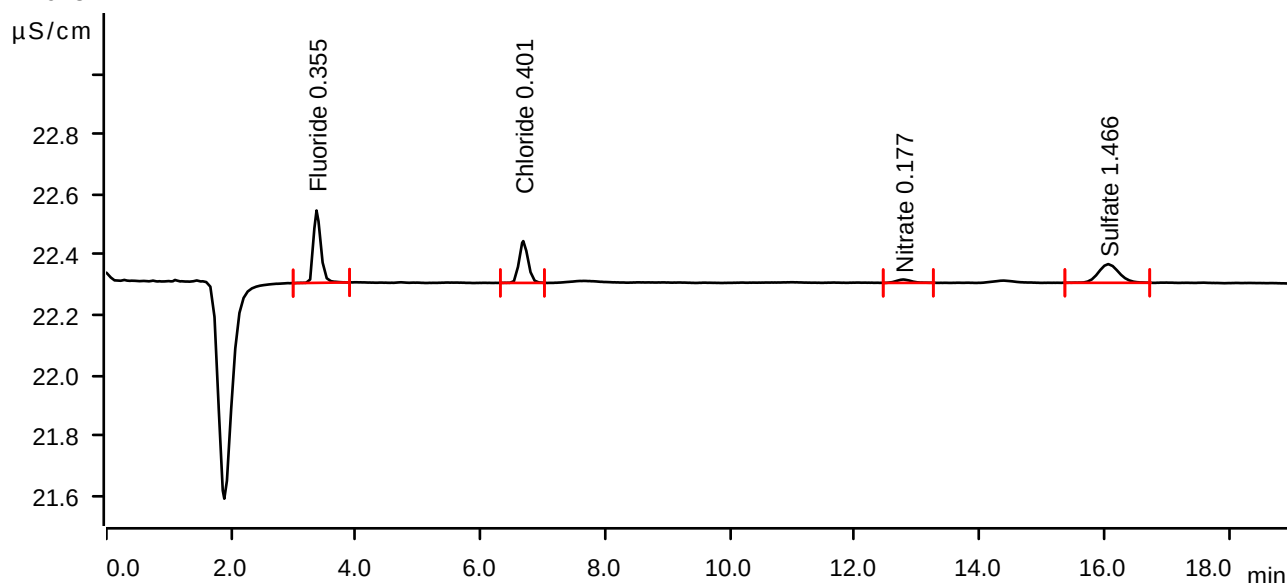

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.372	0.0327	0.240	0.355	Fluoride
2	6.685	0.0230	0.139	0.401	Chloride
3	12.775	0.0031	0.011	0.177	Nitrate
4	16.060	0.0239	0.062	1.466	Sulfate


Sample data

Ident P5382-03
Sample type Sample
Determination start 2024-12-26 12:45:45 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

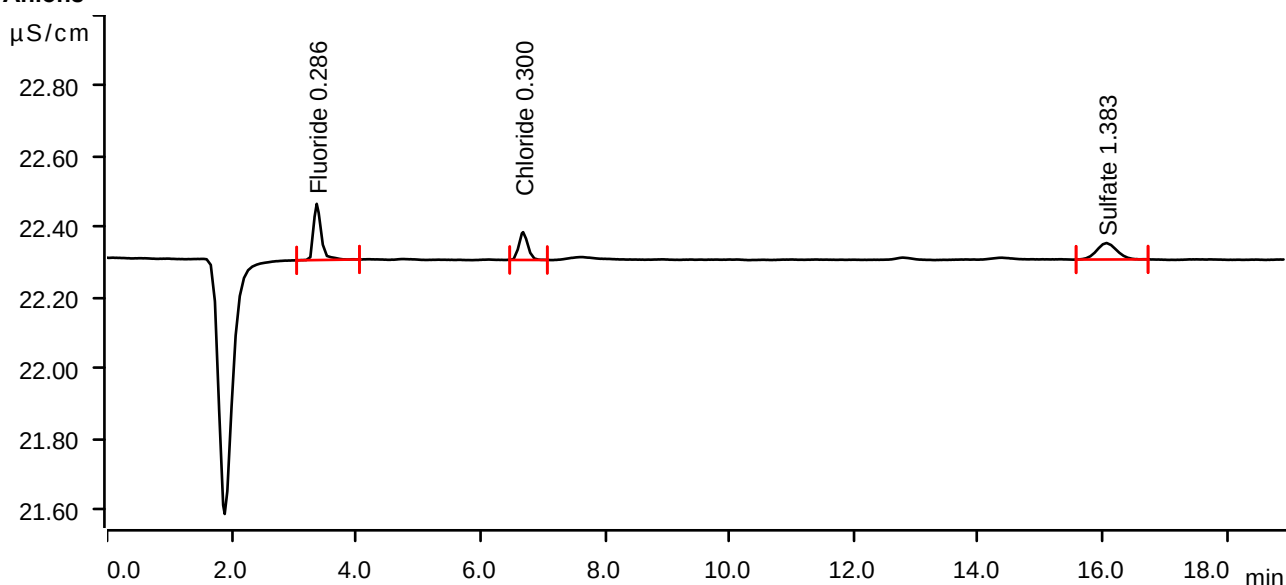

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.370	0.0225	0.159	0.286	Fluoride
2	6.687	0.0130	0.079	0.300	Chloride
3	16.060	0.0175	0.046	1.383	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2024-12-26 13:07:19 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

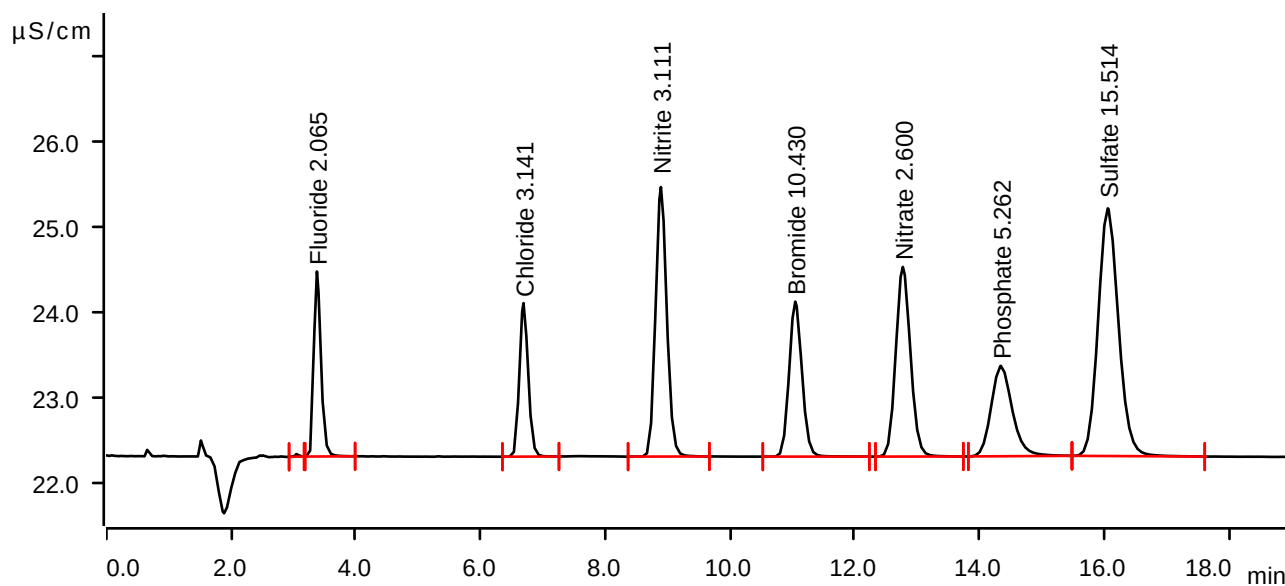

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.048	0.0021	0.031	invalid	
2	3.377	0.2852	2.168	2.065	Fluoride
3	6.688	0.2946	1.798	3.141	Chloride
4	8.892	0.6590	3.157	3.111	Nitrite
5	11.045	0.4344	1.816	10.430	Bromide
6	12.770	0.6066	2.222	2.600	Nitrate
7	14.342	0.4155	1.058	5.262	Phosphate
8	16.055	1.0993	2.901	15.514	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2024-12-26 13:28:50 UTC-5
Method IC1-121824
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 13.23 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions