

Cover Page

Order ID : P5382

Project ID : Comegys School

Client : Kleinfelder

Lab Sample Number

P5382-01
P5382-02
P5382-03
P5382-04
P5382-05
P5382-06
P5382-07
P5382-08
P5382-09
P5382-10
P5382-11
P5382-12
P5382-13
P5382-14
P5382-15

Client Sample Number

COMP-1
COMP-2
COMP-3
SB-1
SB-2
SB-3
SB-4
SB-5
SB-6
SB-7
SB-8
SB-9
SB-10
SB-11
SB-12

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : _____

Date: 12/28/2024

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012



284 Sheffield Street, Mountainside, NJ 07092
Phone: 908 789 8900 Fax: 908 789 8922

CASE NARRATIVE

Kleinfelder

Project Name: Comegys School

Project # N/A

Chemtech Project # P5382

Test Name: PCB Group1

A. Number of Samples and Date of Receipt:

15 Solid samples were received on 12/23/2024.

B. Parameters

According to the Chain of Custody document, the following analyses were requested: Ammonia, Anions Group1, Hexavalent Chromium, Mercury, Metals Group1, Metals ICP-Group1, PCB Group1, PESTICIDE Group1, SVOCMS Group1, Trivalent Chromium and VOCMS Group1. This data package contains results for PCB Group1.

C. Analytical Techniques:

The analyses were performed on instrument GCECD_O. The front column is ZB-MR1 which is 30 meters, 0.32 mm ID, 0.5 um df, Catalogue # 7HM-G016-17. The rear column is ZB-MR2 which is 30 meters, 0.32 mm ID, 0.25 µm; Catalogue # 7HM-G017-11. The analysis of PCB Group1s was based on method 8082A and extraction was done based on method 3541.

D. QA/ QC Samples:

The Holding Times were met for all analysis.

The Surrogate recoveries met the acceptable criteria.

The Retention Times were acceptable for all samples.

The MS recoveries met the requirements for all compounds .

The MSD recoveries met the acceptable requirements .

The RPD met criteria .

The Blank Spike met requirements for all samples .

The Blank analysis did not indicate the presence of lab contamination.

The Initial Calibration met the requirements .

The Continuous Calibration met the requirements .

E. Additional Comments:

The soil samples results are based on a dry weight basis.



284 Sheffield Street, Mountainside, NJ 07092
Phone: 908 789 8900 Fax: 908 789 8922

F. Manual Integration Comments:

Please refer to the Manual integration Report included with the Run Logs for information on the manual integrations performed.

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

Signature_____

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following “ Results Qualifiers” are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. “10 U”. This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as “12 B”.
E	Indicates the analyte ‘s concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a “P”.
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: P5382

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication,airbill, sample management lab chronicle, login page)

✓

Check chain-of-custody for proper relinquish/return of samples

✓

Is the chain of custody signed and complete

✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts

✓

Collect information for each project id from server. Were all requirements followed

✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page

✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody

✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results

✓

Do requested analyses on Chain of Custody agree with the log-in page

✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Custody

✓

Were the samples received within hold time

✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle

✓

ANALYTICAL:

Was method requirement followed?

✓

Was client requirement followed?

✓

Does the case narrative summarize all QC failure?

✓

All runlogs and manual integration are reviewed for requirements

✓

All manual calculations and /or hand notations verified

✓

QA Review Signature: NILESH PRAJAPATI

Date: 12/28/2024

LAB CHRONICLE

OrderID:	P5382	OrderDate:	12/23/2024 11:39:00 AM
Client:	Kleinfelder	Project:	Comegys School
Contact:	Mark Warchol	Location:	N31,VOA Ref. #2 Soil

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
P5382-01	COMP-1	SOIL			12/20/24			12/23/24
			PCB Group1	8082A		12/26/24	12/26/24	
			PESTICIDE Group1	8081B		12/26/24	12/26/24	
P5382-02	COMP-2	SOIL			12/20/24			12/23/24
			PCB Group1	8082A		12/26/24	12/26/24	
			PESTICIDE Group1	8081B		12/26/24	12/26/24	
P5382-03	COMP-3	SOIL			12/20/24			12/23/24
			PCB Group1	8082A		12/26/24	12/26/24	
			PESTICIDE Group1	8081B		12/26/24	12/26/24	



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: P5382

Order ID: P5382

Client: Kleinfelder

Project ID: Comegys School

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------

Client ID :

Total Concentration: 0.000



QC SUMMARY

Surrogate Summary

SDG No.: **P5382**

Client: **Kleinfelder**

Analytical Method: **8082A**

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Rec	Qual	Limits	
								Low	High
I.BLK-PO108361.D	PIBLK-PO108361.D	Tetrachloro-m-xylene	1	20	23.0	115		60	140
		Decachlorobiphenyl	1	20	23.6	118		60	140
		Tetrachloro-m-xylene	2	20	21.6	108		60	140
		Decachlorobiphenyl	2	20	23.6	118		60	140
I.BLK-PO108762.D	PIBLK-PO108762.D	Tetrachloro-m-xylene	1	20	21.8	109		60	140
		Decachlorobiphenyl	1	20	21.3	107		60	140
		Tetrachloro-m-xylene	2	20	20.0	100		60	140
		Decachlorobiphenyl	2	20	22.1	110		60	140
PB165843BL	PB165843BL	Tetrachloro-m-xylene	1	20	22.0	110		32	144
		Decachlorobiphenyl	1	20	22.2	111		32	175
		Tetrachloro-m-xylene	2	20	20.0	100		32	144
		Decachlorobiphenyl	2	20	22.9	115		32	175
PB165843BS	PB165843BS	Tetrachloro-m-xylene	1	20	21.2	106		32	144
		Decachlorobiphenyl	1	20	21.7	108		32	175
		Tetrachloro-m-xylene	2	20	19.2	96		32	144
		Decachlorobiphenyl	2	20	23.2	116		32	175
P5318-01MS	AU-06-122024MS	Tetrachloro-m-xylene	1	20	13.5	67		32	144
		Decachlorobiphenyl	1	20	10.9	55		32	175
		Tetrachloro-m-xylene	2	20	12.4	62		32	144
		Decachlorobiphenyl	2	20	12.1	61		32	175
P5318-01MSD	AU-06-122024MSD	Tetrachloro-m-xylene	1	20	13.9	70		32	144
		Decachlorobiphenyl	1	20	11.8	59		32	175
		Tetrachloro-m-xylene	2	20	13.6	68		32	144
		Decachlorobiphenyl	2	20	13.3	66		32	175
P5382-01	COMP-1	Tetrachloro-m-xylene	1	20	19.2	96		32	144
		Decachlorobiphenyl	1	20	10.9	55		32	175
		Tetrachloro-m-xylene	2	20	18.6	93		32	144
		Decachlorobiphenyl	2	20	12.2	61		32	175
P5382-02	COMP-2	Tetrachloro-m-xylene	1	20	21.4	107		32	144
		Decachlorobiphenyl	1	20	14.9	75		32	175
		Tetrachloro-m-xylene	2	20	20.5	102		32	144
		Decachlorobiphenyl	2	20	16.9	85		32	175
P5382-03	COMP-3	Tetrachloro-m-xylene	1	20	22.7	114		32	144
		Decachlorobiphenyl	1	20	16.4	82		32	175
		Tetrachloro-m-xylene	2	20	21.8	109		32	144
		Decachlorobiphenyl	2	20	18.2	91		32	175
I.BLK-PO108777.D	PIBLK-PO108777.D	Tetrachloro-m-xylene	1	20	20.5	102		60	140
		Decachlorobiphenyl	1	20	18.1	90		60	140
		Tetrachloro-m-xylene	2	20	19.4	97		60	140
		Decachlorobiphenyl	2	20	19.9	100		60	140

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: P5382

Client: Kleinfelder

Analytical Method: 8082A

DataFile : PO108767.D

Lab Sample ID:	Parameter	Spike	Sample		Units	Rec	Rec		RPD		Limits	RPD
			Result	Result			Qual	RPD	Qual	Low	High	
Client Sample ID: P5318-01MS	AU-06-122024MS											
	AR1016	193.2	0	138	ug/kg	71				55	146	
	AR1260	193.2	8.7	124	ug/kg	60				45	144	

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: P5382

Client: Kleinfelder

Analytical Method: 8082A

DataFile : PO108768.D

Lab Sample ID:	Parameter	Spike	Sample Result	Result	Units	Rec	Rec Qual	RPD	RPD Qual	Low	Limits High	RPD
Client Sample ID:	AU-06-122024MSD											
P5318-01MSD	AR1016	193.1	0	134	ug/kg	69		3		55	146	20
	AR1260	193.1	8.7	127	ug/kg	61		2		45	144	20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: P5382

Client: Kleinfelder

Analytical Method: **8082A** **Datafile :** PO108764.D

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD		Limits	
								Qual	Low	High	RPD
PB165843BS	AR1016	166.6	165	ug/kg	99				71	120	
	AR1260	166.6	166	ug/kg	100				65	130	

4C

PESTICIDE METHOD BLANK SUMMARY

EPA SAMPLE NO.

PB165843BL

Lab Name: CHEMTECH

Contract: POWE02

Lab Code: CHEM Case No.: P5382

SAS No.: P5382 SDG NO.: P5382

Lab Sample ID: PB165843BL

Lab File ID: PO108763.D

Matrix: (soil/water) Solid

Extraction: (Type) _____

Sulfur Cleanup: (Y/N) N

Date Extracted: 12/26/2024

Date Analyzed (1): 12/26/2024

Date Analyzed (2): 12/26/2024

Time Analyzed (1): 12:21

Time Analyzed (2): 12:21

Instrument ID (1): ECD_O

Instrument ID (2): ECD_O

GC Column (1): ZB-MR1 ID: 0.32 (mm)

GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
PB165843BS	PB165843BS	PO108764.D	12/26/2024	12/26/2024
AU-06-122024MS	P5318-01MS	PO108767.D	12/26/2024	12/26/2024
AU-06-122024MSD	P5318-01MSD	PO108768.D	12/26/2024	12/26/2024
COMP-1	P5382-01	PO108770.D	12/26/2024	12/26/2024
COMP-2	P5382-02	PO108771.D	12/26/2024	12/26/2024
COMP-3	P5382-03	PO108772.D	12/26/2024	12/26/2024

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	Kleinfelder	Date Collected:	12/20/24
Project:	Comegys School	Date Received:	12/23/24
Client Sample ID:	COMP-1	SDG No.:	P5382
Lab Sample ID:	P5382-01	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	82.8
Sample Wt/Vol:	30.08	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB Group1
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108770.D	1	12/26/24 08:30	12/26/24 14:29	PB165843

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	4.10	U	4.10	20.5	ug/kg
11097-69-1	Aroclor-1254	3.30	U	3.30	20.5	ug/kg
11096-82-5	Aroclor-1260	3.50	U	3.50	20.5	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.2		32 - 144	96%	SPK: 20
2051-24-3	Decachlorobiphenyl	12.2		32 - 175	61%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
 Data File : PO108770.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 14:29
 Operator : YP/AJ
 Sample : P5382-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 20:26:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.703	3.700	167.2E6	94334296	19.222	18.609
2) SA Decachlor...	8.766	8.716	79748377	47433176	10.918	12.241m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
Data File : PO108770.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 14:29
Operator : YP/AJ
Sample : P5382-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

COMP-1

Manual Integrations



APPROVED


Reviewed By :Yogesh Patel 12/27/2024

Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 20:26:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

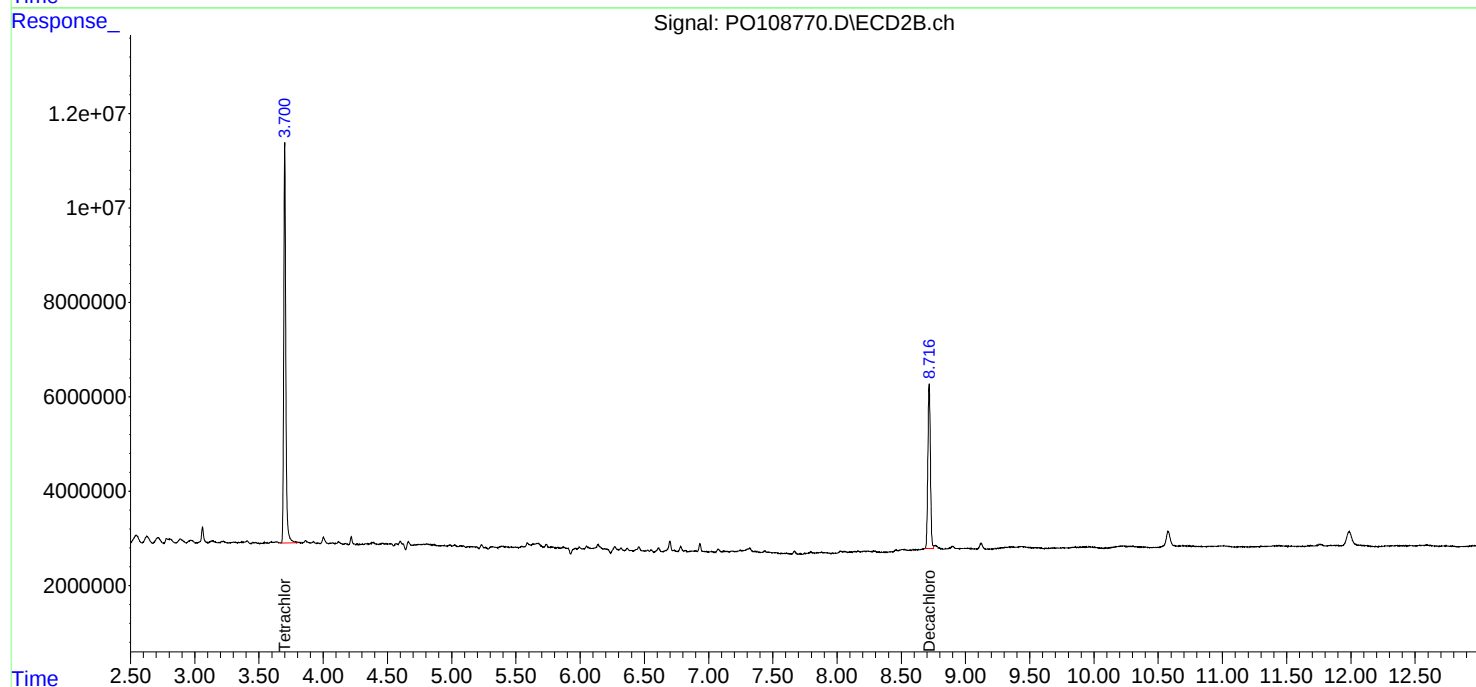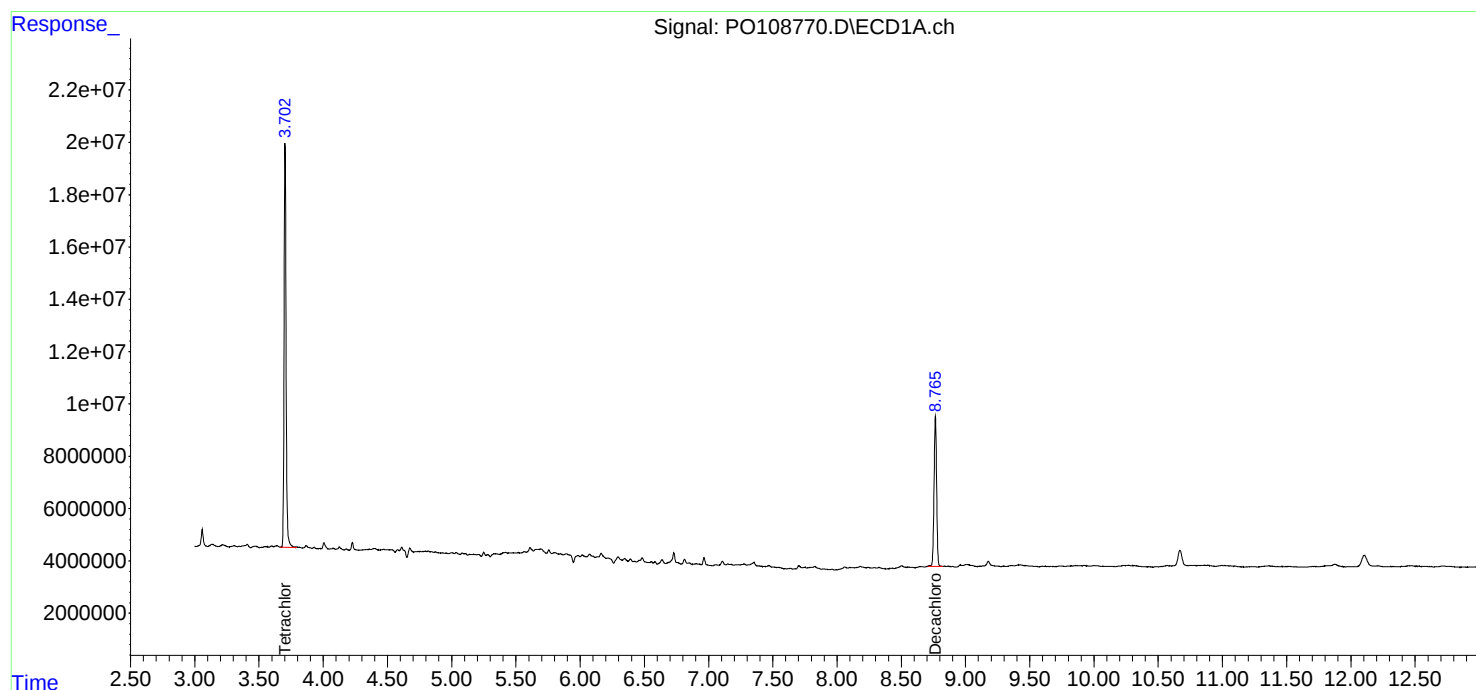

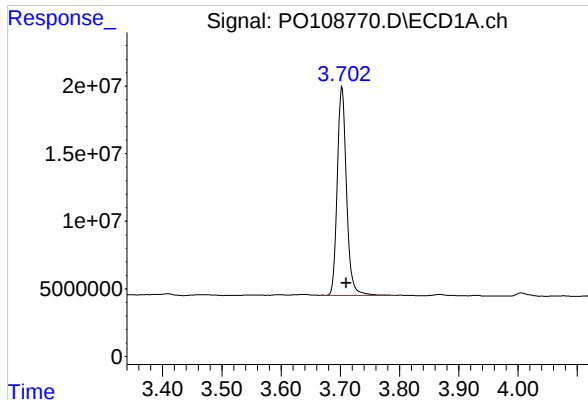


#1 Tetrachloro-m-xylene

R.T.: 3.703 min
Delta R.T.: -0.007 min
Response: 167231871
Conc: 19.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2024
Supervised By :Ankita Jodhani 12/27/2024

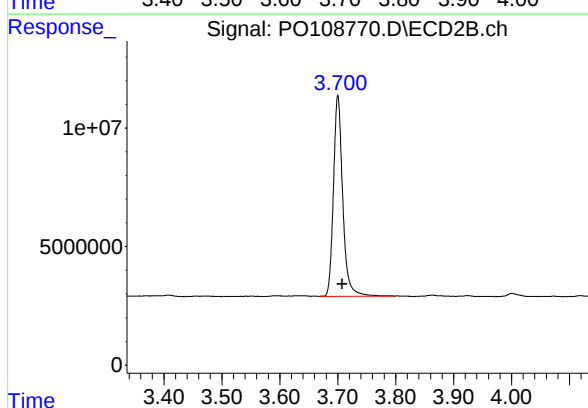


#1 Tetrachloro-m-xylene

R.T.: 3.700 min
Delta R.T.: -0.008 min
Response: 94334296
Conc: 18.61 ng/ml

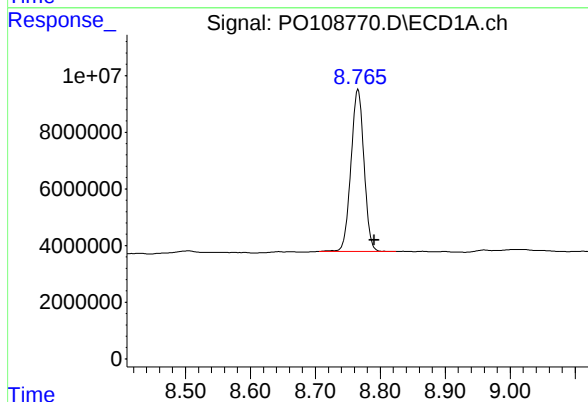

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.025 min
Response: 79748377
Conc: 10.92 ng/ml

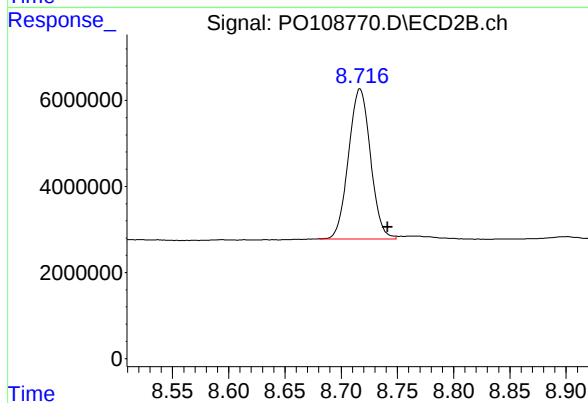

#2 Decachlorobiphenyl

R.T.: 8.716 min
Delta R.T.: -0.025 min
Response: 47433176
Conc: 12.24 ng/ml m

Report of Analysis

Client:	Kleinfelder	Date Collected:	12/20/24
Project:	Comegys School	Date Received:	12/23/24
Client Sample ID:	COMP-2	SDG No.:	P5382
Lab Sample ID:	P5382-02	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	82.5
Sample Wt/Vol:	30.03	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB Group1
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108771.D	1	12/26/24 08:30	12/26/24 14:47	PB165843

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	4.10	U	4.10	20.6	ug/kg
11097-69-1	Aroclor-1254	3.30	U	3.30	20.6	ug/kg
11096-82-5	Aroclor-1260	3.50	U	3.50	20.6	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.4		32 - 144	107%	SPK: 20
2051-24-3	Decachlorobiphenyl	16.9		32 - 175	85%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
 Data File : PO108771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 14:47
 Operator : YP/AJ
 Sample : P5382-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 20:26:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.703	3.700	186.2E6	103.8E6	21.403	20.480
2) SA Decachlor...	8.765	8.716	109.0E6	65681806	14.918	16.951m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
Data File : PO108771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 14:47
Operator : YP/AJ
Sample : P5382-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

COMP-2



Manual Integrations**APPROVED**


Reviewed By :Yogesh Patel 12/27/2024

Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 20:26:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

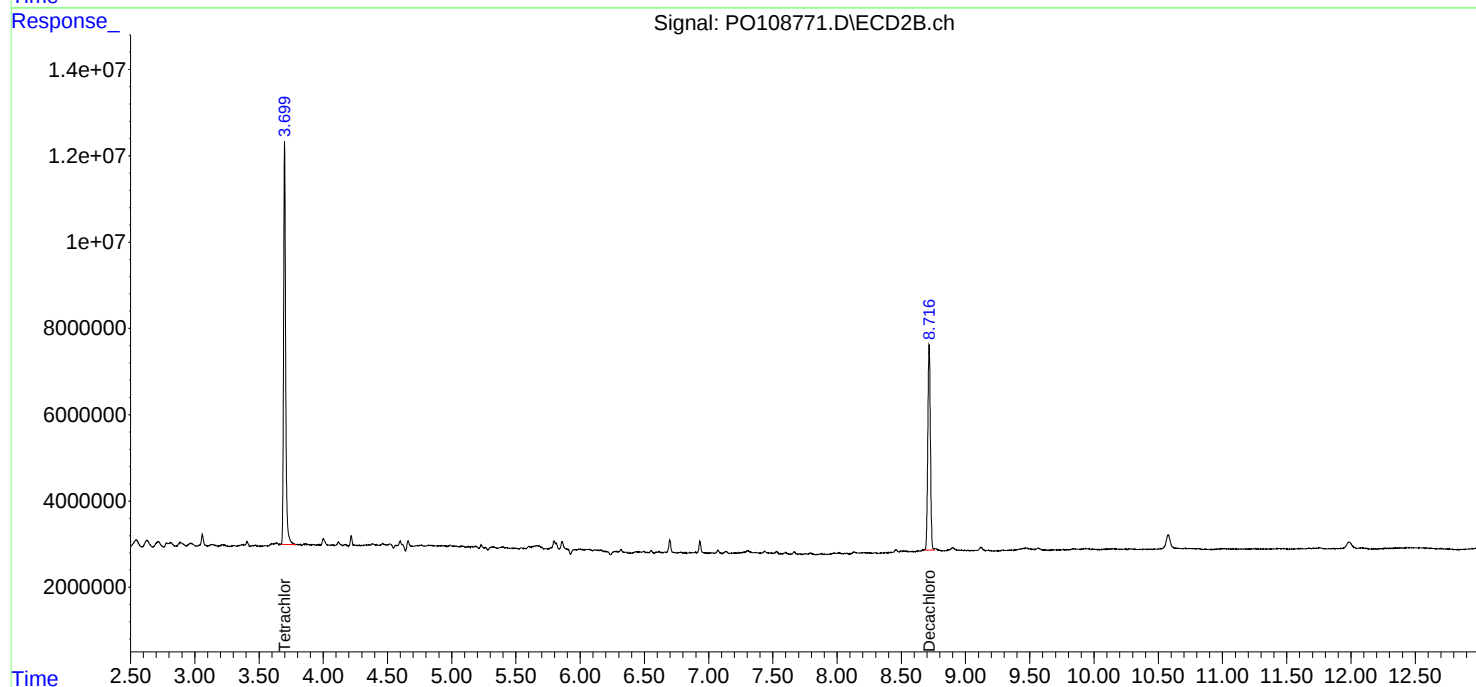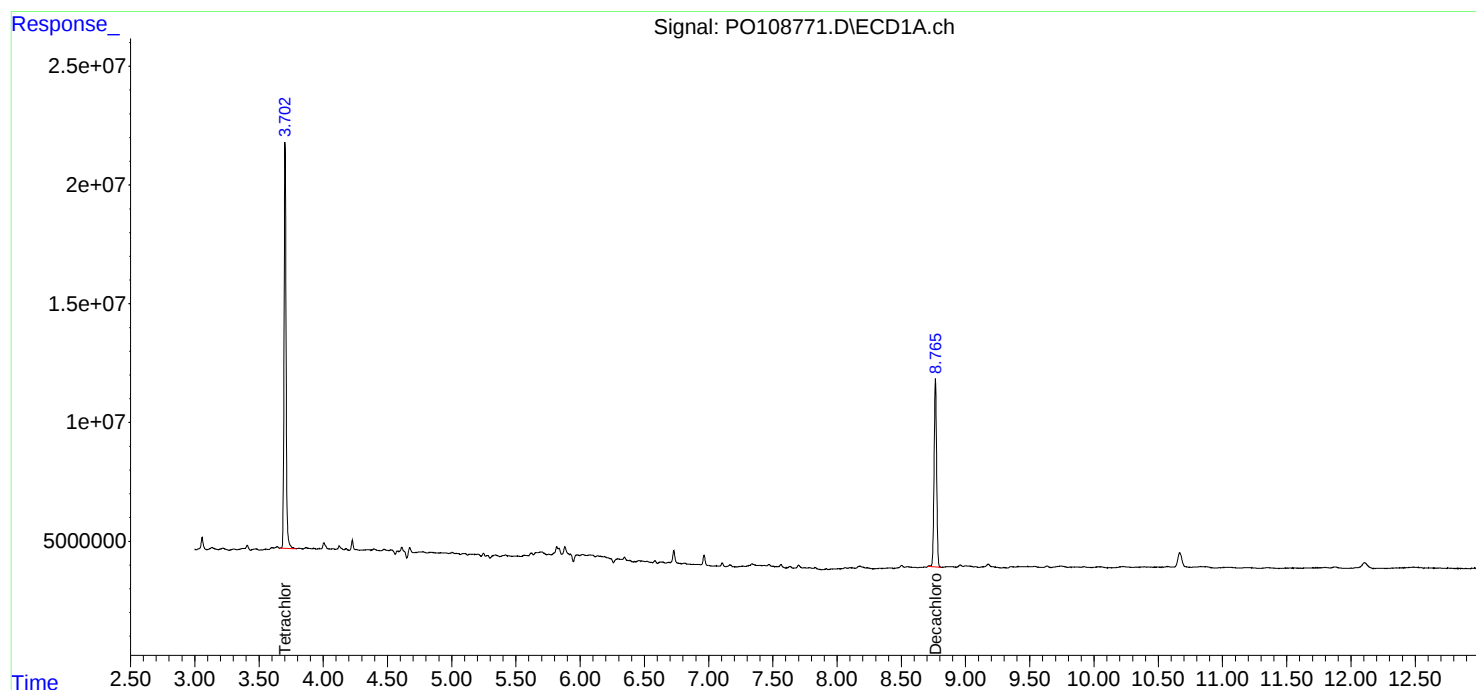

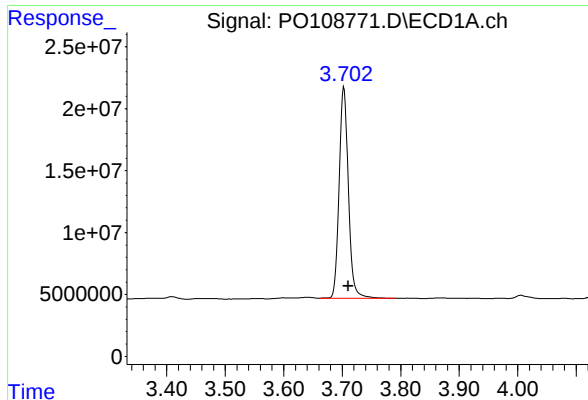


#1 Tetrachloro-m-xylene

R.T.: 3.703 min
Delta R.T.: -0.007 min
Response: 186204922
Conc: 21.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2024
Supervised By :Ankita Jodhani 12/27/2024

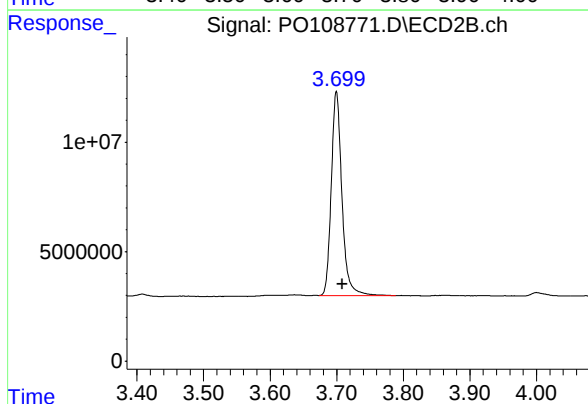


#1 Tetrachloro-m-xylene

R.T.: 3.700 min
Delta R.T.: -0.009 min
Response: 103819591
Conc: 20.48 ng/ml

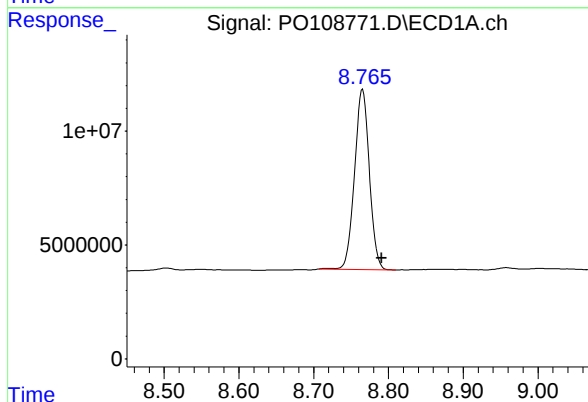

#2 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: -0.026 min
Response: 108965585
Conc: 14.92 ng/ml

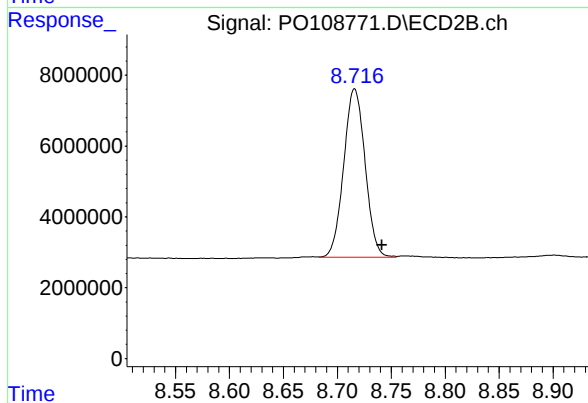

#2 Decachlorobiphenyl

R.T.: 8.716 min
Delta R.T.: -0.026 min
Response: 65681806
Conc: 16.95 ng/ml m

Report of Analysis

Client:	Kleinfelder	Date Collected:	12/20/24
Project:	Comegys School	Date Received:	12/23/24
Client Sample ID:	COMP-3	SDG No.:	P5382
Lab Sample ID:	P5382-03	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	82.8
Sample Wt/Vol:	30.01	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB Group1
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108772.D	1	12/26/24 08:30	12/26/24 15:05	PB165843

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	4.10	U	4.10	20.5	ug/kg
11097-69-1	Aroclor-1254	3.30	U	3.30	20.5	ug/kg
11096-82-5	Aroclor-1260	3.50	U	3.50	20.5	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	22.7		32 - 144	114%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.2		32 - 175	91%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
 Data File : PO108772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 15:05
 Operator : YP/AJ
 Sample : P5382-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 20:27:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.704	3.700	197.5E6	110.5E6	22.699	21.793
2) SA Decachlor...	8.766	8.716	119.7E6	70687977	16.390	18.242m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
Data File : PO108772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 15:05
Operator : YP/AJ
Sample : P5382-03
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2024
Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 20:27:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

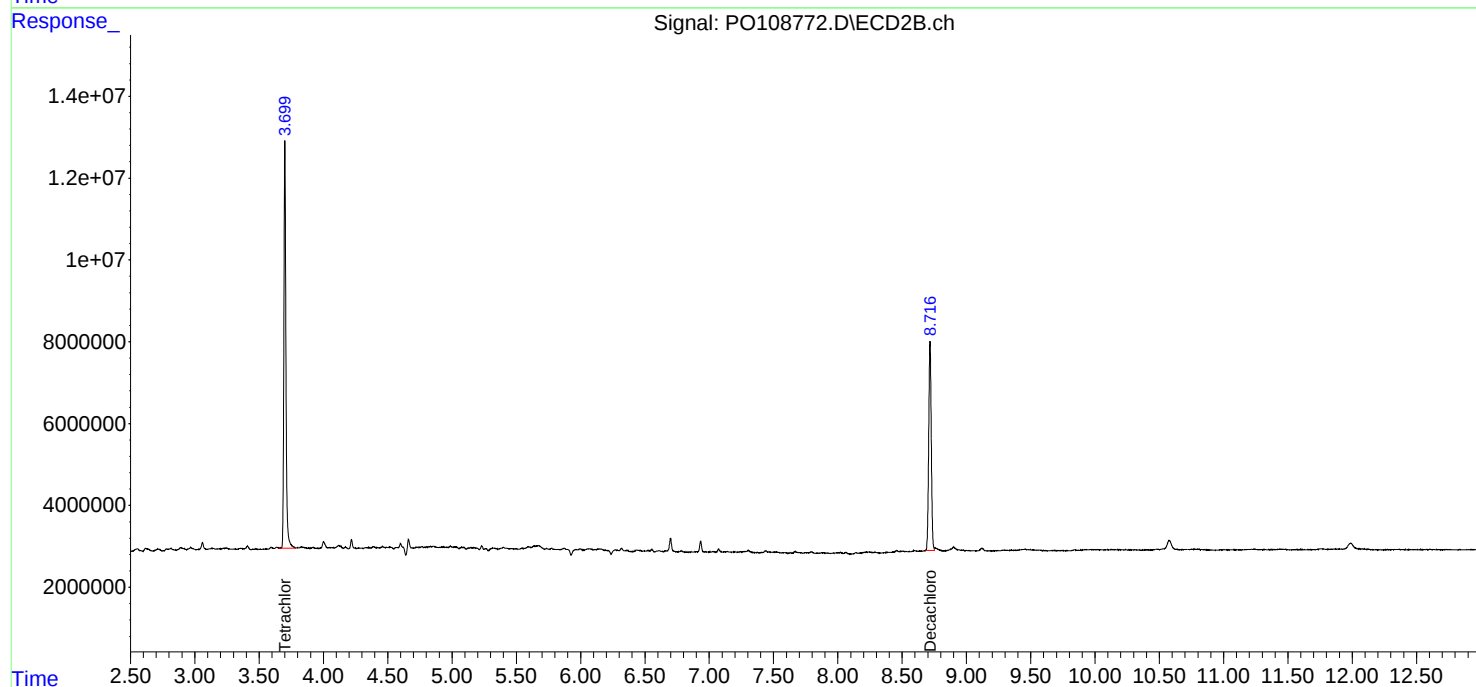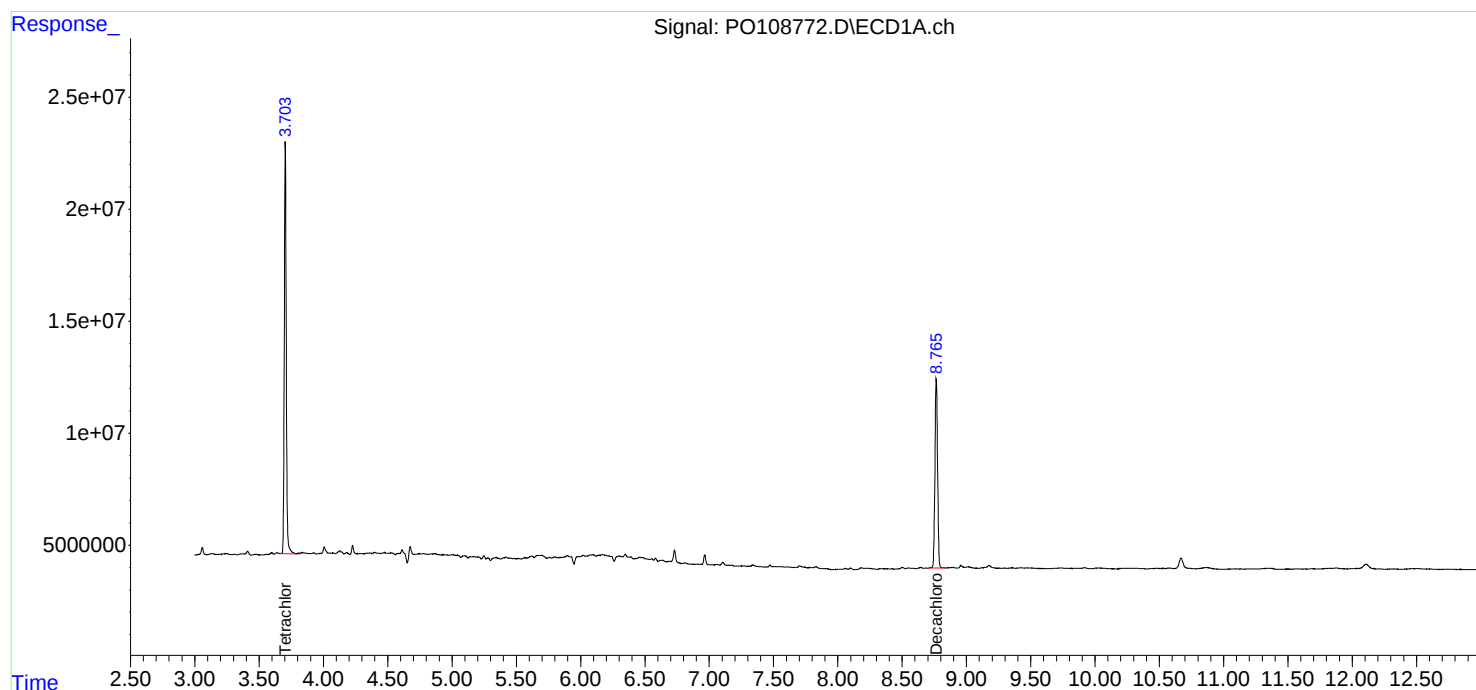

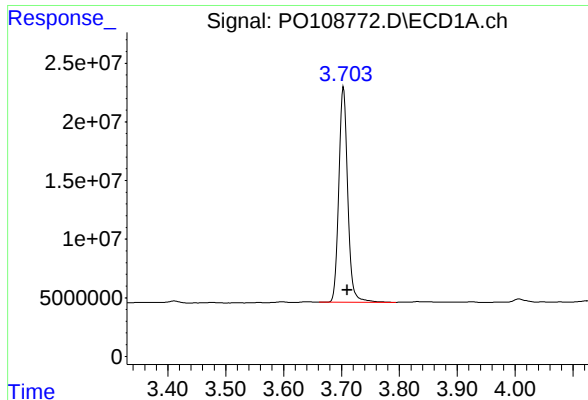


#1 Tetrachloro-m-xylene

R.T.: 3.704 min
Delta R.T.: -0.006 min
Response: 197482179
Conc: 22.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2024
Supervised By :Ankita Jodhani 12/27/2024

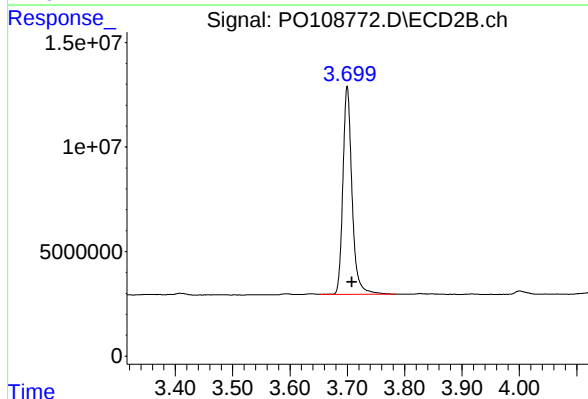


#1 Tetrachloro-m-xylene

R.T.: 3.700 min
Delta R.T.: -0.008 min
Response: 110477504
Conc: 21.79 ng/ml

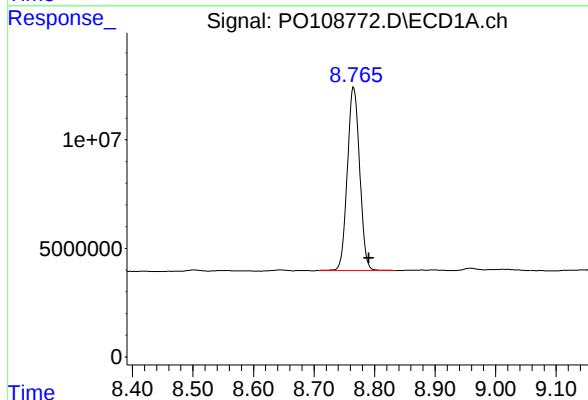

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.025 min
Response: 119717697
Conc: 16.39 ng/ml

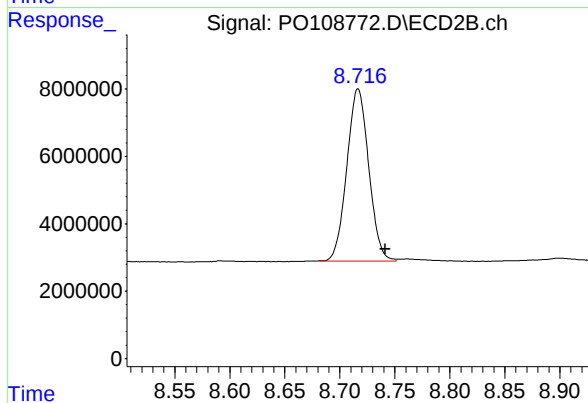

#2 Decachlorobiphenyl

R.T.: 8.716 min
Delta R.T.: -0.025 min
Response: 70687977
Conc: 18.24 ng/ml m



CALIBRATION SUMMARY

GC Column: ZB-MR1 ID: 0.32 (mm)

[illegible]

GC Column: ZB-MR2 ID: 0.32 (mm)

[illegible]

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: POWE02
Lab Code: CHEM **Case No.:** P5382 **SAS No.:** P5382 **SDG NO.:** P5382
Instrument ID: ECD_O
Calibration Date(s): 12/06/2024 12/06/2024
Calibration Times: 14:19 22:34
GC Column: ZB-MR1 **ID:** 0.32 (mm)

LAB FILE ID:		CF 1000 =	PO108362.D	CF 750 =	PO108363.D			
CF 500 =		PO108364.D	CF 250 =	PO108365.D	CF 050 =	PO108366.D		
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	CF	% RSD
Aroclor-1016-1	(1)	291946997	297743768	310620664	319628964	322276700	308443419	4
Aroclor-1016-2	(2)	404548343	410201719	419086158	434302728	418957120	417419214	3
Aroclor-1016-3	(3)	276313882	283350735	295214768	305005424	303271420	292631246	4
Aroclor-1016-4	(4)	219460370	224028880	231955104	239248200	241192240	231176959	4
Aroclor-1016-5	(5)	230837381	238568924	249276722	260302648	279364560	251670047	8
Aroclor-1260-1	(1)	430087746	435401064	458150304	486996644	475087940	457144740	5
Aroclor-1260-2	(2)	526959551	526383048	555764632	590931960	578558580	555719554	5
Aroclor-1260-3	(3)	436965341	443883275	464184392	487588856	485769460	463678265	5
Aroclor-1260-4	(4)	403312630	406530869	426472890	444299896	446086500	425340557	5
Aroclor-1260-5	(5)	957132439	955503789	984649950	1000570432	961557080	971882738	2
Decachlorobiphenyl		7019975940	7102279760	7343195240	7645101200	7409935200	7304097468	3
Tetrachloro-m-xylene		8754554380	8783699800	8926447760	8858353120	8177601800	8700131372	3
Decachlorobiphenyl		7151632520	7167100640	7259242160	7695082840	7616154000	7377842432	4
Tetrachloro-m-xylene		8921368150	8691850413	8750108140	8842570400	8500038400	8741187101	2
Decachlorobiphenyl		7041971050	7340001867	7677772660	8334328560	8377267200	7754268267	8
Tetrachloro-m-xylene		8742483090	9116744787	9342439560	9446963040	8577776400	9045281375	4
Aroclor-1254-1	(1)	463230517	487037587	512031514	533861324	572040640	513640316	8
Aroclor-1254-2	(2)	407035308	429134731	452892530	476390932	511836900	455458080	9
Aroclor-1254-3	(3)	665923649	695083201	726473802	743208540	769953480	720128534	6
Aroclor-1254-4	(4)	404280854	421077525	444268156	458648100	465789400	438812807	6
Aroclor-1254-5	(5)	578915300	604639081	636092894	662542188	693421140	635122121	7
Decachlorobiphenyl		7146512650	7451889427	7845842200	8029803560	8289288000	7752667167	6
Tetrachloro-m-xylene		8916956510	9205112240	9483653100	9313097600	8995829000	9182929690	3
Decachlorobiphenyl		13116054520	12684928373	12985206200	13660251040	13550255000	13199339027	3
Tetrachloro-m-xylene		9439924600	8926085107	9366220020	9585299080	8679584000	9199422561	4



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

Instrument ID: ECD_O

Calibration Date(s): 12/06/2024 12/06/2024

Calibration Times: 14:19 22:34

GC Column: ZB-MR2 ID: 0.32 (mm)

LAB FILE ID:		CF 1000 =	PO108362.D	CF 750 =	PO108363.D			
CF 500 =		PO108364.D	CF 250 =	PO108365.D	CF 050 =	PO108366.D		
COMPOUND		CF 1000	CF 750	CF 500	CF 250	CF 050	CF	% RSD
Aroclor-1016-1	(1)	153895169	156728372	161981056	169073964	160692820	160474276	4
Aroclor-1016-2	(2)	216342839	218481491	224728354	232664856	218246400	222092788	3
Aroclor-1016-3	(3)	120117826	122069885	126984464	131660600	128335340	125833623	4
Aroclor-1016-4	(4)	96843518	100727947	106065160	112123848	108269060	104805907	6
Aroclor-1016-5	(5)	124135109	128707045	133919966	139473364	149819760	135211049	7
Aroclor-1260-1	(1)	220557751	224688929	233372252	247245708	244312440	234035416	5
Aroclor-1260-2	(2)	265498816	268435476	278836448	291165028	298902840	280567722	5
Aroclor-1260-3	(3)	247895049	250737920	258985508	271036448	289186460	263568277	6
Aroclor-1260-4	(4)	206205103	207830825	214807128	221847076	213061100	212750246	3
Aroclor-1260-5	(5)	485216265	483370987	491130416	498849136	461100640	483933489	3
Decachlorobiphenyl		3766442770	3798929547	3925647180	4081005080	3802565400	3874917995	3
Tetrachloro-m-xylene		5125815400	5157614040	5227779180	5235220160	4600485000	5069382756	5
Decachlorobiphenyl		3837824030	3881889067	3932164520	4142632320	3981873600	3955276707	3
Tetrachloro-m-xylene		5175637870	5056121747	5062590080	5077379040	4694060200	5013157787	4
Decachlorobiphenyl		3812249930	3973614533	4145380680	4445118560	4295672800	4134407301	6
Tetrachloro-m-xylene		4965646150	5143987440	5236574340	5255843080	4633325600	5047075322	5
Aroclor-1254-1	(1)	245816740	256457156	269229946	279215328	303441080	270832050	8
Aroclor-1254-2	(2)	215464605	225390397	238770420	248817564	271658880	240020373	9
Aroclor-1254-3	(3)	351887512	364509791	380441060	386791796	393925500	375511132	5
Aroclor-1254-4	(4)	202983022	209924784	220508360	226093392	228876240	217677160	5
Aroclor-1254-5	(5)	301571990	312619885	327015726	332817532	339773740	322759775	5
Decachlorobiphenyl		3941299730	4071714027	4258931580	4374402200	4331619600	4195593427	4
Tetrachloro-m-xylene		5092418740	5228867107	5367266300	5227916200	4998387200	5182971109	3
Decachlorobiphenyl		7216327300	6964723040	7142803680	7406390760	7194775600	7185004076	2
Tetrachloro-m-xylene		5353757740	5060175947	5259788400	5326606440	4764065600	5152878825	5



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

Instrument ID: _____ Date(s) Analyzed: _____

GC Column: _____ ID: _____ (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
		1				
		2				
		3				
		4				
		5				

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 14:19
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 01:46:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 01:45:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.710	3.708	875.5E6	512.6E6	98.074	98.050
2) SA Decachlor...	8.791	8.741	702.0E6	376.6E6	95.598	95.945
Target Compounds						
3) L1 AR-1016-1	4.810	4.798	291.9E6	153.9E6	939.883	950.081
4) L1 AR-1016-2	4.830	4.818	404.5E6	216.3E6	965.311	962.686
5) L1 AR-1016-3	4.885	4.994	276.3E6	120.1E6	935.976	945.925
6) L1 AR-1016-4	5.007	5.036	219.5E6	96843518	946.133	913.057
7) L1 AR-1016-5	5.265	5.250	230.8E6	124.1E6	926.029	926.935
31) L7 AR-1260-1	6.310	6.286	430.1E6	220.6E6	938.748	945.090
32) L7 AR-1260-2	6.498	6.473	527.0E6	265.5E6	948.170	952.167
33) L7 AR-1260-3	6.869	6.628	437.0E6	247.9E6	941.362	957.177
34) L7 AR-1260-4	7.129	7.100	403.3E6	206.2E6	945.693	959.955
35) L7 AR-1260-5	7.370	7.340	957.1E6	485.2E6	972.054	987.958



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 14:19
Operator : YP/AJ
Sample : AR1660ICC1000
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 01:46:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 01:45:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

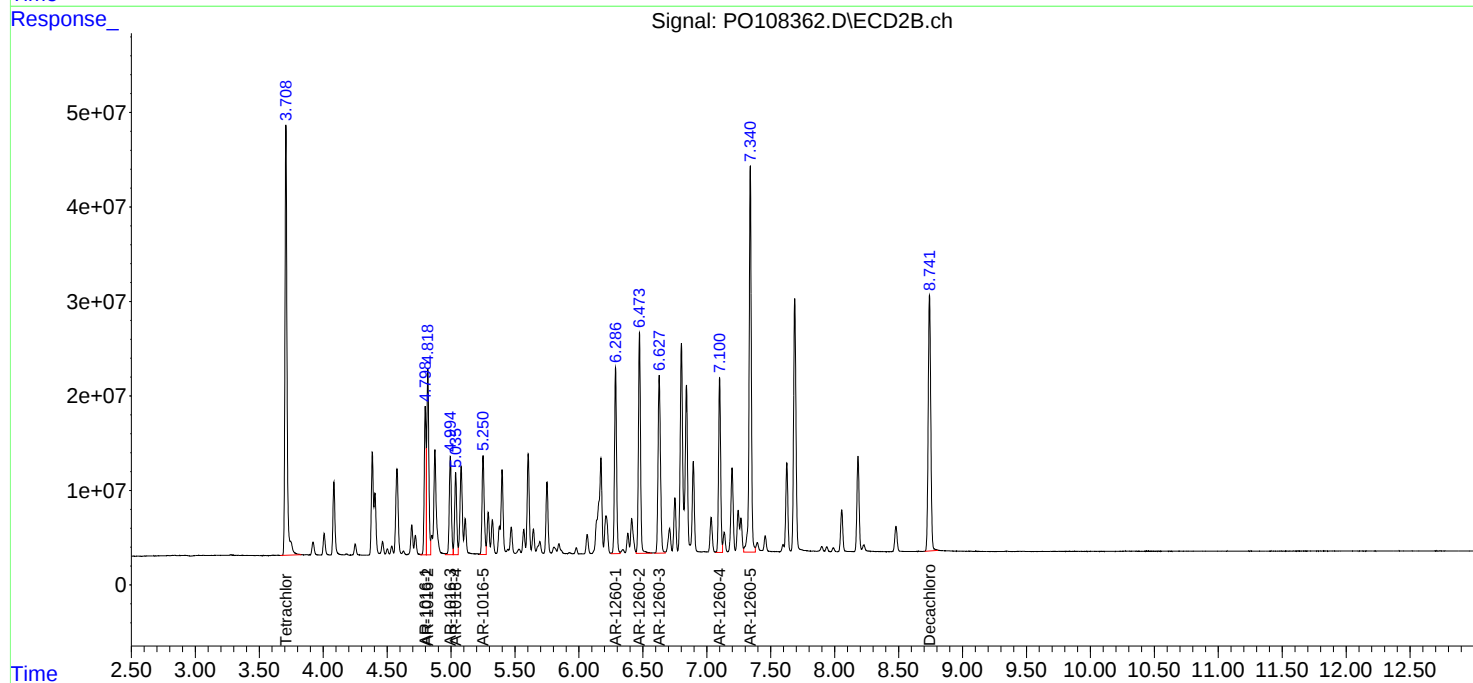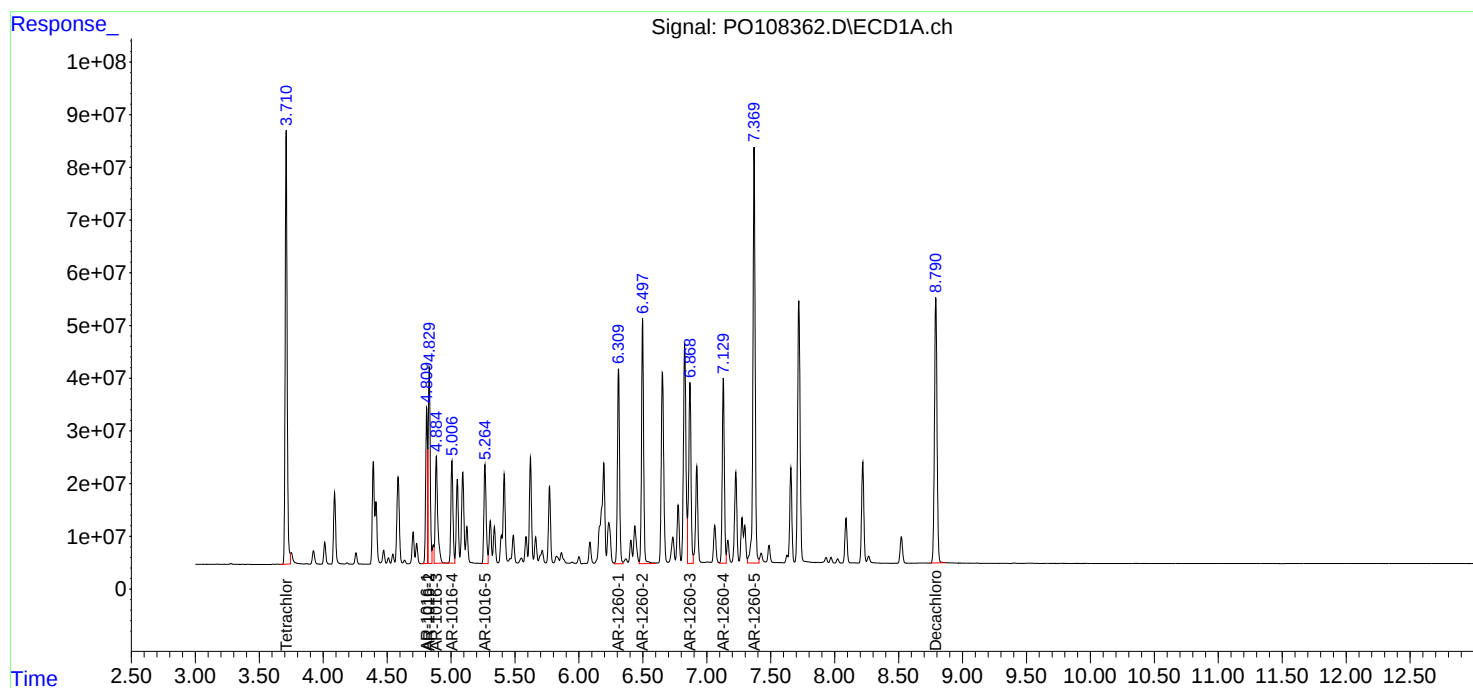

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 14:38
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 01:46:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 01:45:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.710	3.709	658.8E6	386.8E6	73.801	73.993
2) SA Decachlor...	8.790	8.741	532.7E6	284.9E6	72.539	72.579
Target Compounds						
3) L1 AR-1016-1	4.810	4.799	223.3E6	117.5E6	718.908	725.679
4) L1 AR-1016-2	4.829	4.818	307.7E6	163.9E6	734.100	729.152
5) L1 AR-1016-3	4.885	4.994	212.5E6	91552414	719.859	720.973
6) L1 AR-1016-4	5.007	5.036	168.0E6	75545960	724.371	712.260
7) L1 AR-1016-5	5.265	5.250	178.9E6	96530284	717.783	720.806
31) L7 AR-1260-1	6.309	6.287	326.6E6	168.5E6	712.759	722.094
32) L7 AR-1260-2	6.498	6.474	394.8E6	201.3E6	710.350	722.024
33) L7 AR-1260-3	6.869	6.628	332.9E6	188.1E6	717.199	726.116
34) L7 AR-1260-4	7.129	7.101	304.9E6	155.9E6	714.930	725.642
35) L7 AR-1260-5	7.370	7.340	716.6E6	362.5E6	727.800	738.151



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 14:38
Operator : YP/AJ
Sample : AR1660ICC750
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 01:46:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 01:45:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

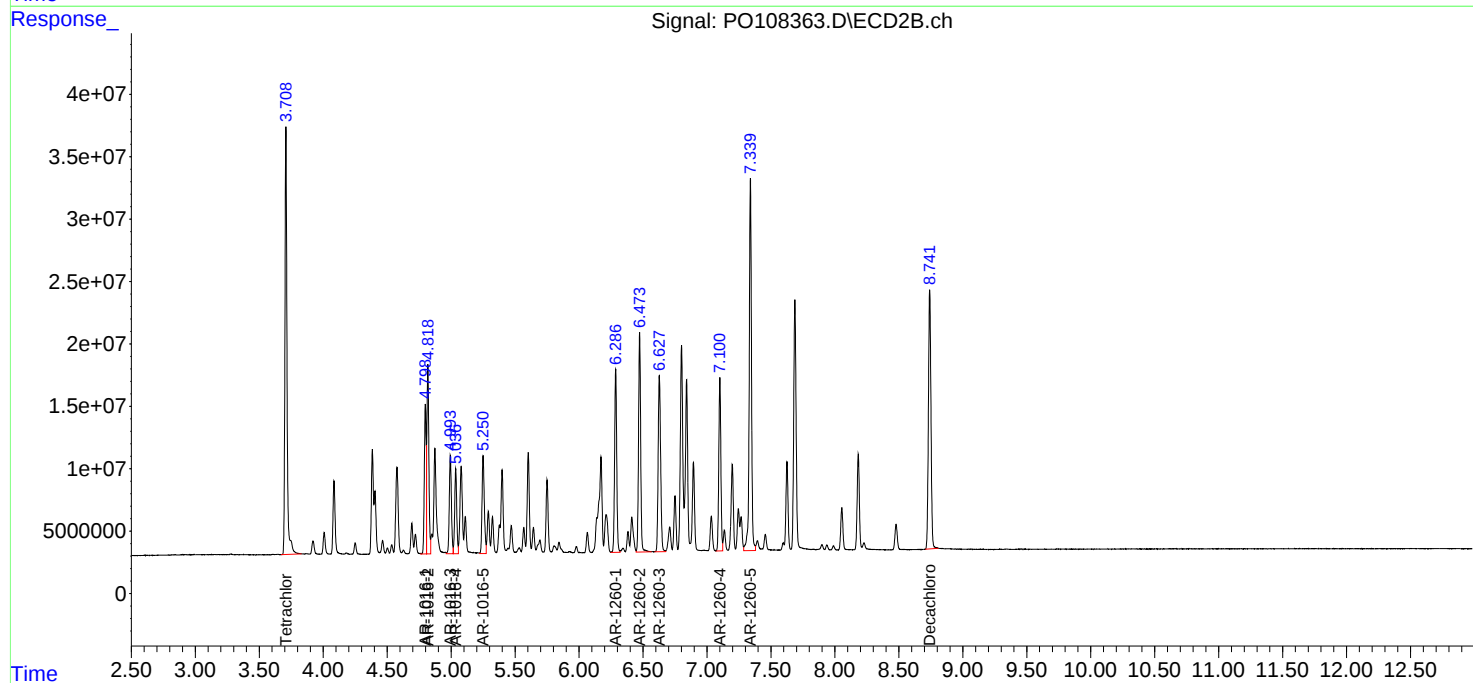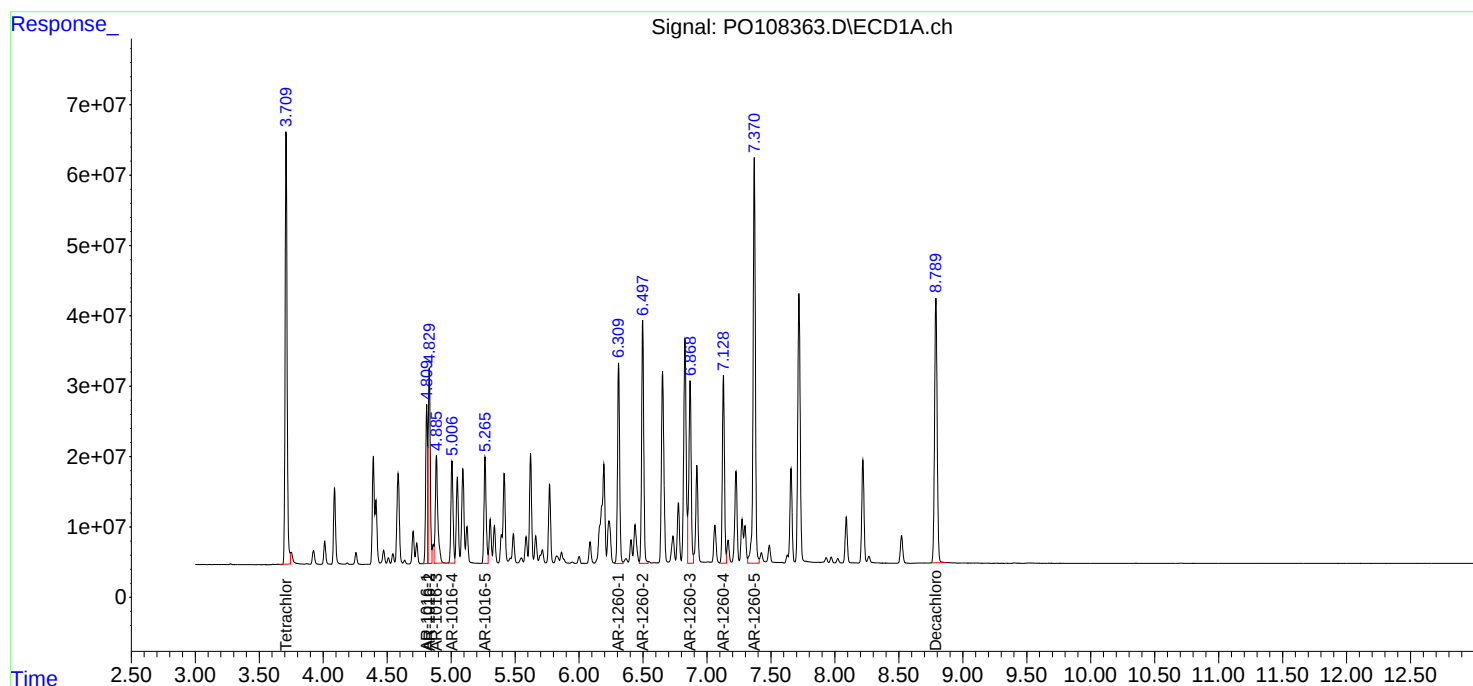

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 14:56
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 01:47:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 01:45:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.710	3.708	446.3E6	261.4E6	50.000	50.000
2) SA Decachlor...	8.791	8.741	367.2E6	196.3E6	50.000	50.000
Target Compounds						
3) L1 AR-1016-1	4.809	4.798	155.3E6	80990528	500.000	500.000
4) L1 AR-1016-2	4.829	4.818	209.5E6	112.4E6	500.000	500.000
5) L1 AR-1016-3	4.885	4.994	147.6E6	63492232	500.000	500.000
6) L1 AR-1016-4	5.007	5.035	116.0E6	53032580	500.000	500.000
7) L1 AR-1016-5	5.265	5.250	124.6E6	66959983	500.000	500.000
31) L7 AR-1260-1	6.310	6.286	229.1E6	116.7E6	500.000	500.000
32) L7 AR-1260-2	6.498	6.473	277.9E6	139.4E6	500.000	500.000
33) L7 AR-1260-3	6.869	6.627	232.1E6	129.5E6	500.000	500.000
34) L7 AR-1260-4	7.129	7.100	213.2E6	107.4E6	500.000	500.000
35) L7 AR-1260-5	7.370	7.339	492.3E6	245.6E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108364.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 14:56
Operator : YP/AJ
Sample : AR1660ICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 01:47:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 01:45:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

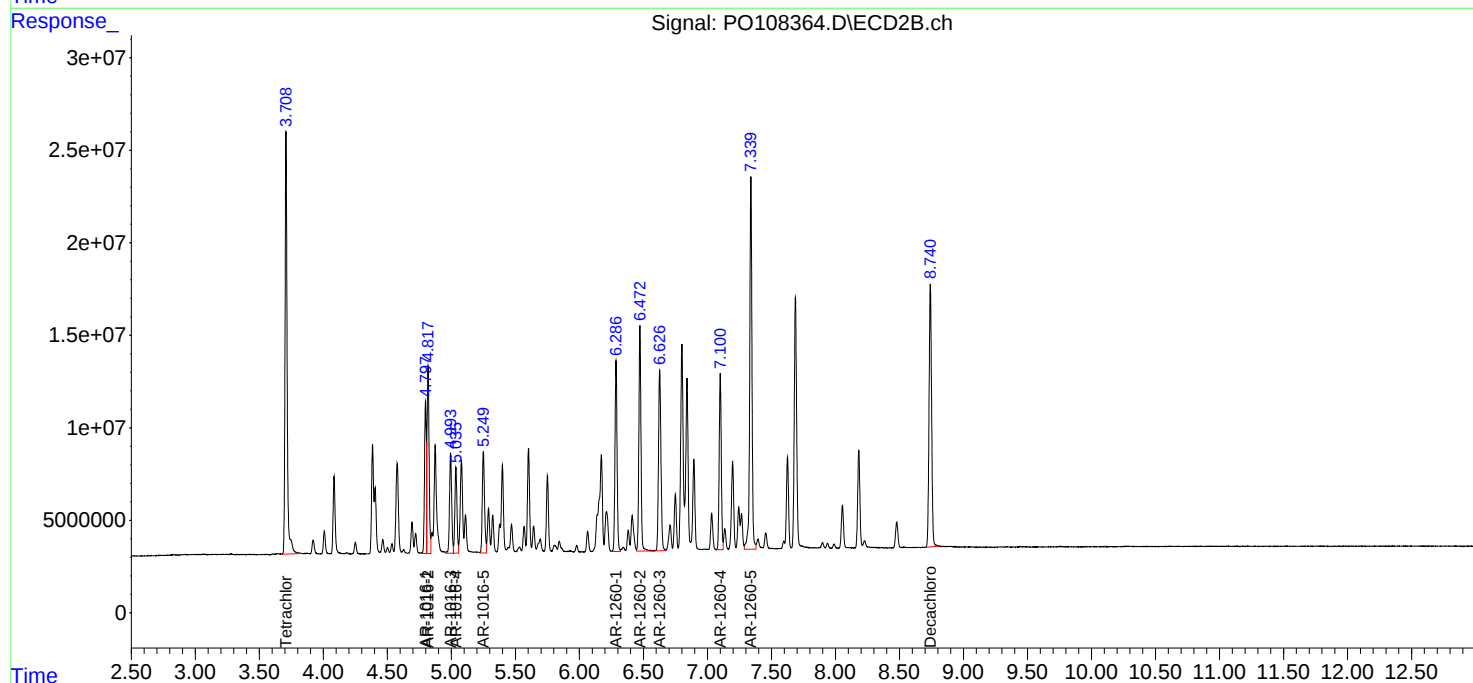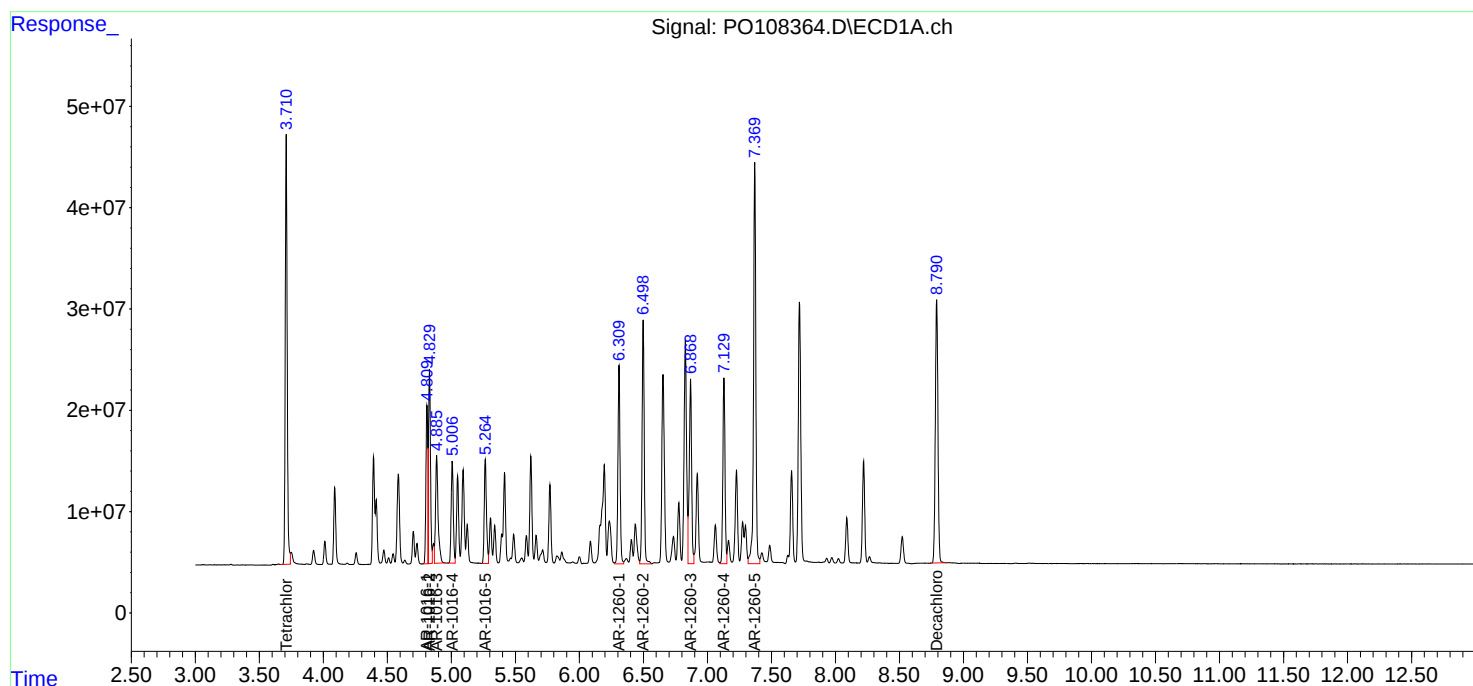

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 15:14
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 01:47:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 01:45:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.710	3.708	221.5E6	130.9E6	24.809	25.036
2) SA Decachlor...	8.790	8.741	191.1E6	102.0E6	26.028	25.989
Target Compounds						
3) L1 AR-1016-1	4.809	4.798	79907241	42268491	257.250	260.947
4) L1 AR-1016-2	4.829	4.818	108.6E6	58166214	259.077	258.829
5) L1 AR-1016-3	4.885	4.994	76251356	32915150	258.291	259.206
6) L1 AR-1016-4	5.007	5.035	59812050	28030962	257.860	264.281
7) L1 AR-1016-5	5.265	5.250	65075662	34868341	261.058	260.367
31) L7 AR-1260-1	6.309	6.286	121.7E6	61811427	265.741	264.862
32) L7 AR-1260-2	6.497	6.473	147.7E6	72791257	265.819	261.054
33) L7 AR-1260-3	6.868	6.627	121.9E6	67759112	262.605	261.633
34) L7 AR-1260-4	7.129	7.100	111.1E6	55461769	260.450	258.193
35) L7 AR-1260-5	7.370	7.339	250.1E6	124.7E6	254.042	253.929



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 15:14
Operator : YP/AJ
Sample : AR1660ICC250
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 01:47:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 01:45:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

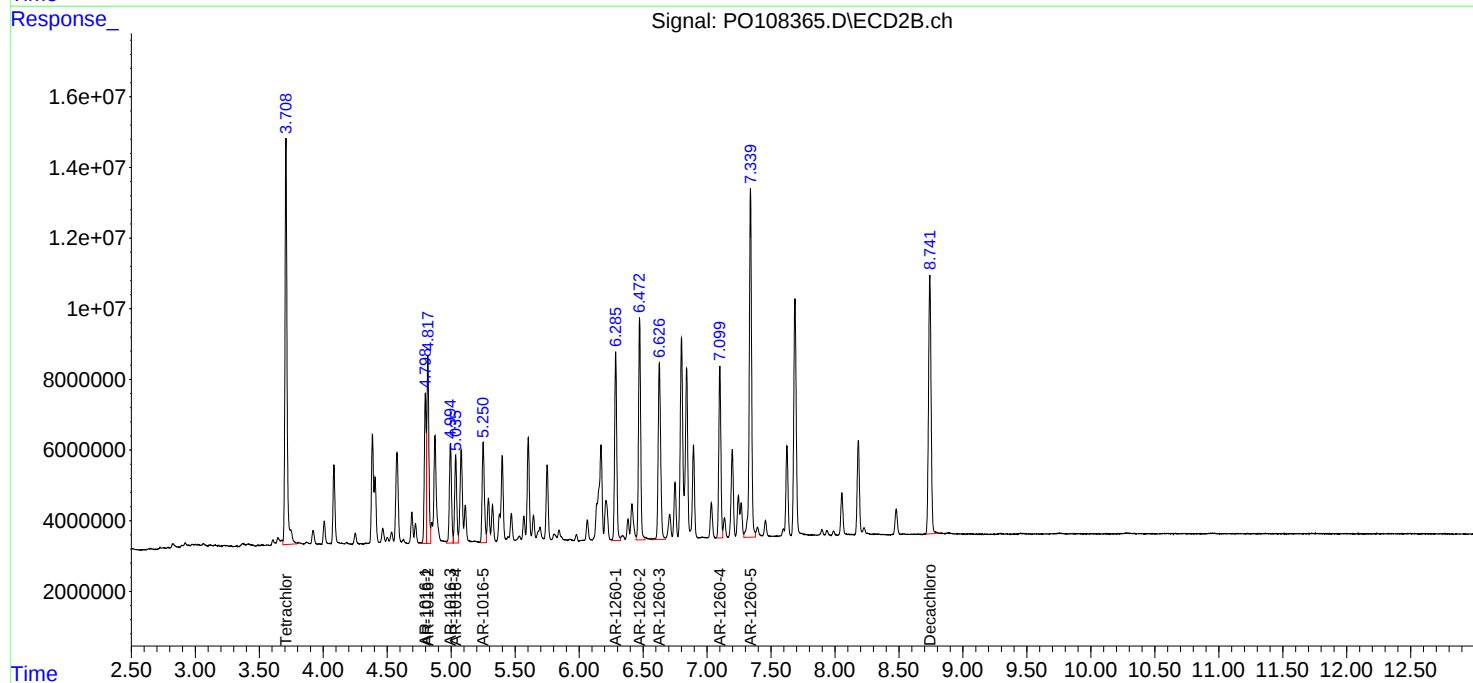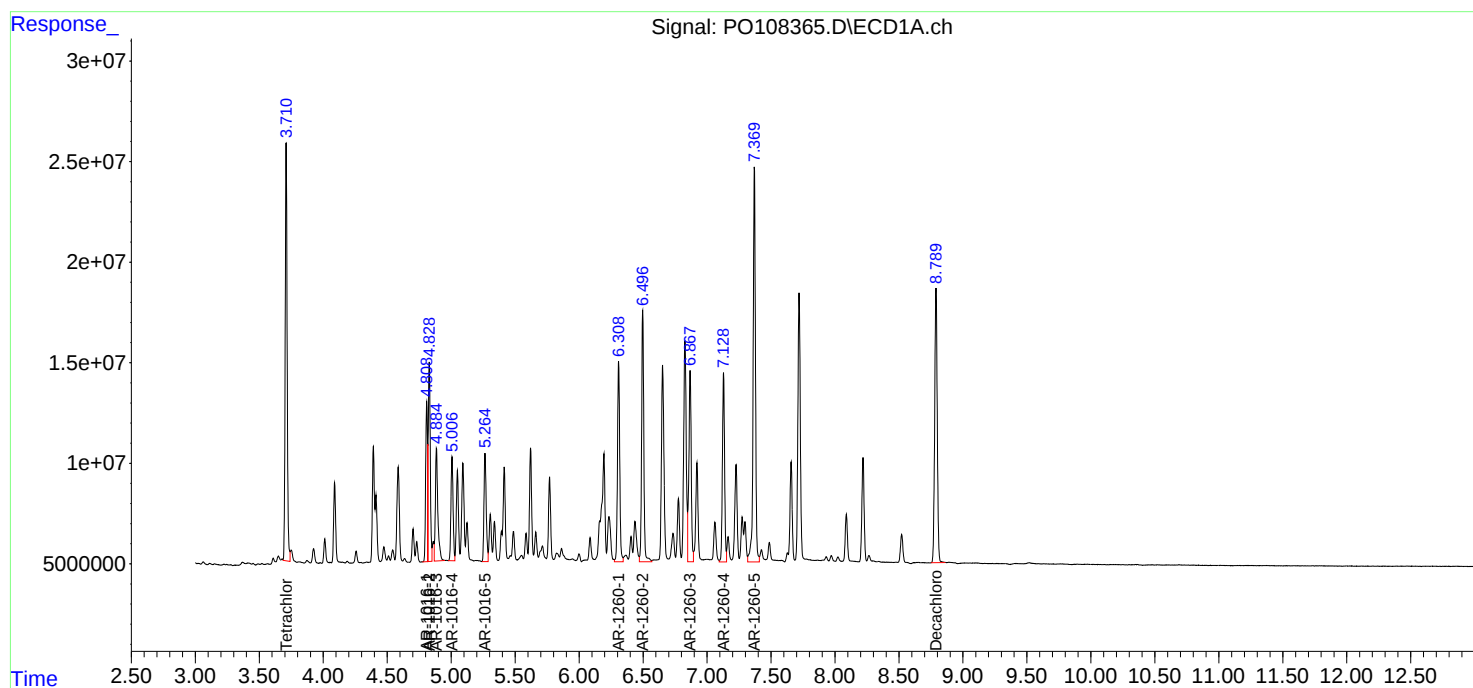

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO120624\
 Data File : PO108366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 15:33
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1660ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/09/2024
 Supervised By :Ankita Jodhani 12/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 01:47:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 01:45:35 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.710	3.708	40888009	23002425	4.581	4.400
2) SA Decachlor...	8.790	8.741	37049676	19012827	5.045	4.843
Target Compounds						
3) L1 AR-1016-1	4.809	4.797	16113835	8034641	51.876	49.602m
4) L1 AR-1016-2	4.829	4.818	20947856	10912320	49.985	48.558m
5) L1 AR-1016-3	4.885	4.993	15163571	6416767	51.365	50.532m
6) L1 AR-1016-4	5.006	5.035	12059612	5413453	51.991	51.039m
7) L1 AR-1016-5	5.265	5.249	13968228	7490988	56.035	55.936
31) L7 AR-1260-1	6.308	6.285	23754397	12215622	51.848m	52.344m
32) L7 AR-1260-2	6.497	6.472	28927929	14945142	52.051m	53.598m
33) L7 AR-1260-3	6.866	6.627	24288473	14459323	52.325m	55.831
34) L7 AR-1260-4	7.128	7.100	22304325	10653055	52.300	49.594
35) L7 AR-1260-5	7.369	7.339	48077854	23055032	48.827	46.943

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108366.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 15:33
Operator : YP/AJ
Sample : AR1660ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2024
Supervised By :Ankita Jodhani 12/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 01:47:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 01:45:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

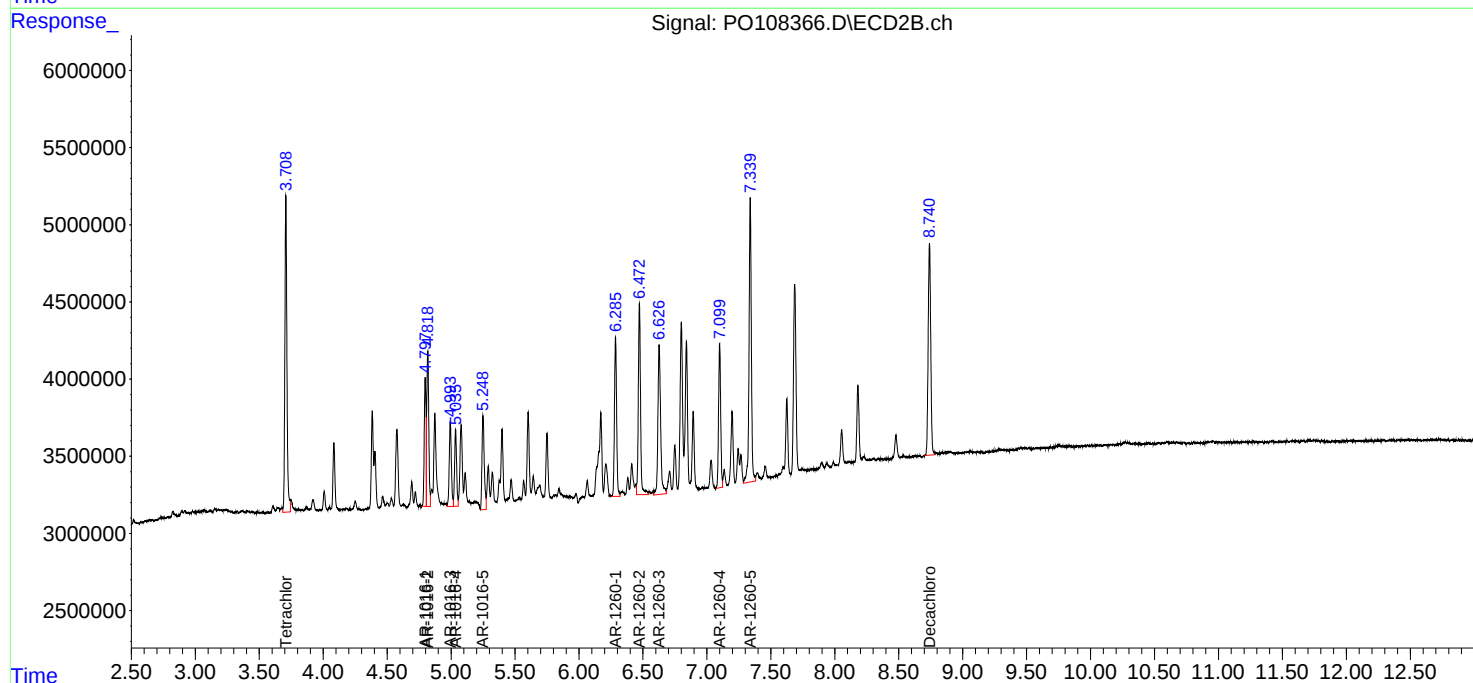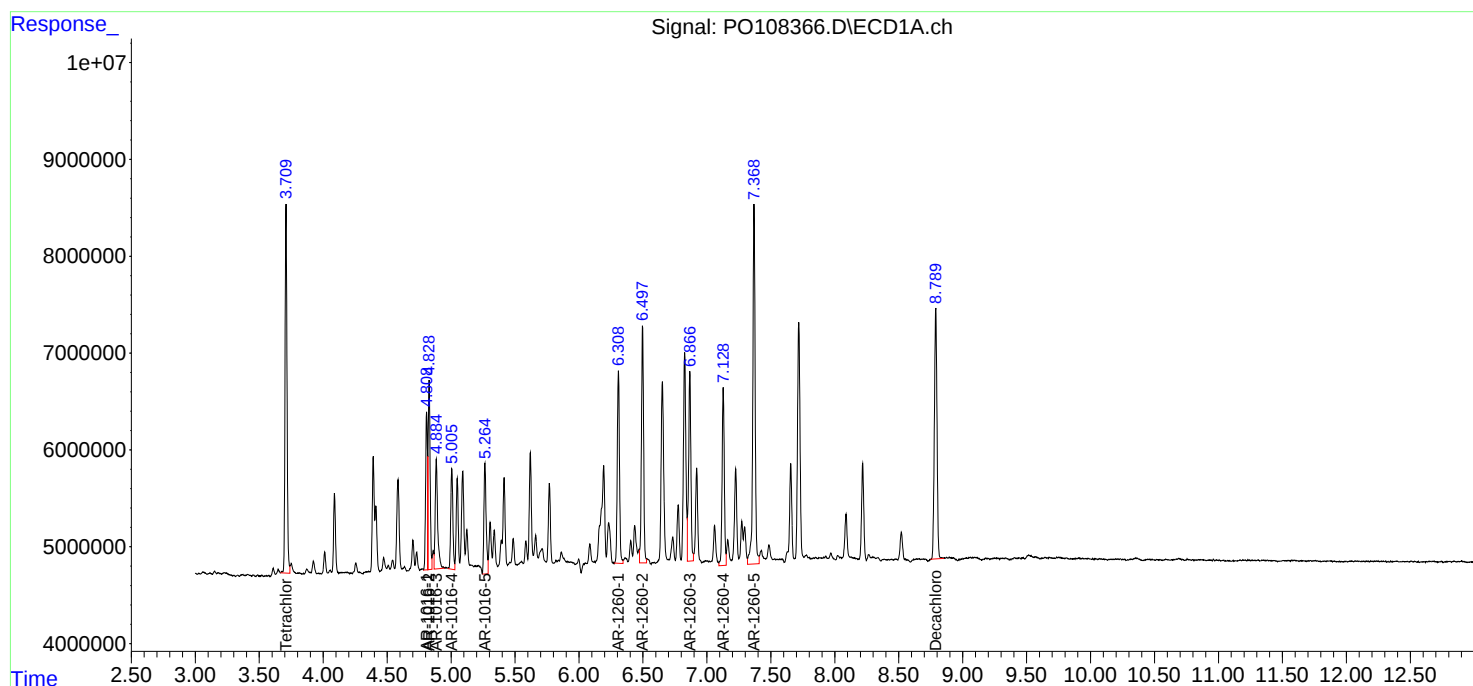

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 15:51
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 02:45:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 02:44:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.710	3.708	457.2E6	254.8E6	50.000	50.000
2)	SA Decachlor...	8.788	8.741	384.3E6	206.2E6	50.000	50.000
Target Compounds							
8)	L2 AR-1221-1	3.925	3.922	56571909	31061265	500.000	500.000
9)	L2 AR-1221-2	4.012	4.007	43360161	23722482	500.000	500.000
10)	L2 AR-1221-3	4.089	4.084	127.1E6	70293463	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 15:51
Operator : YP/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 02:45:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 02:44:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

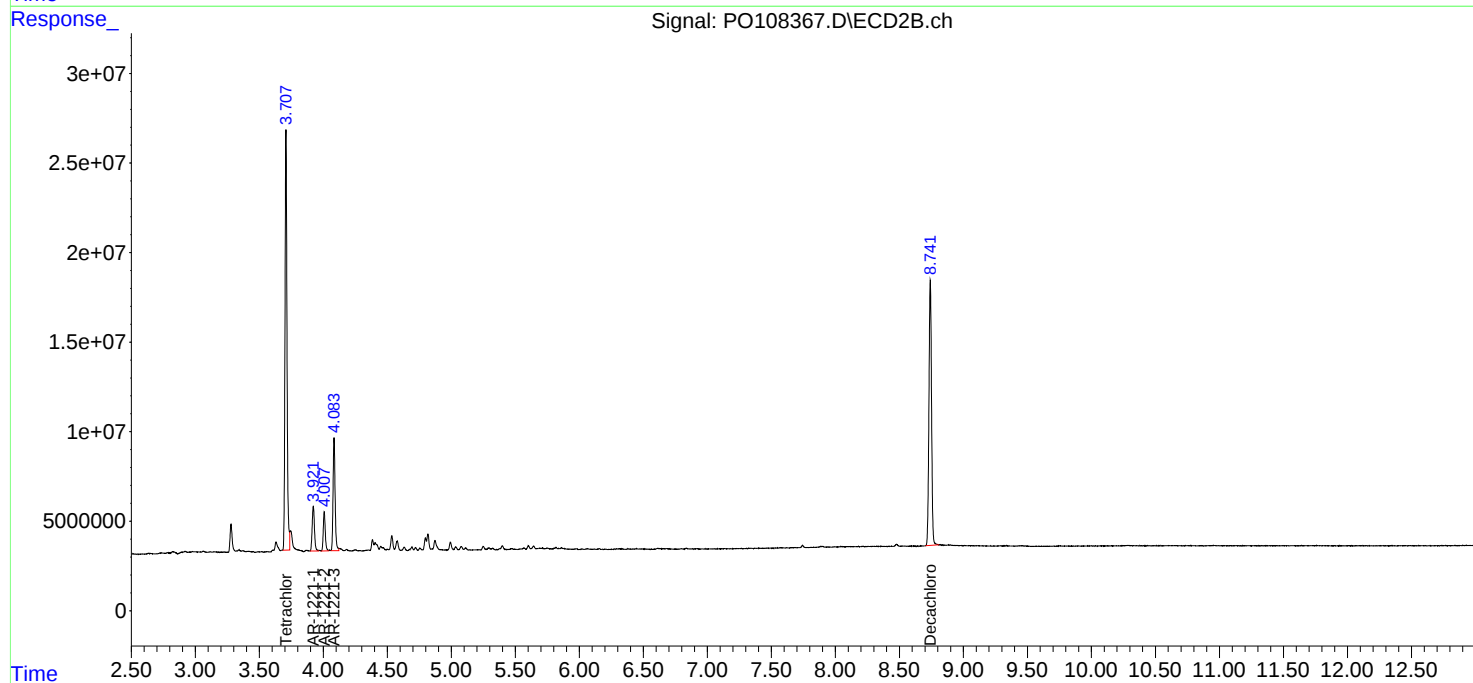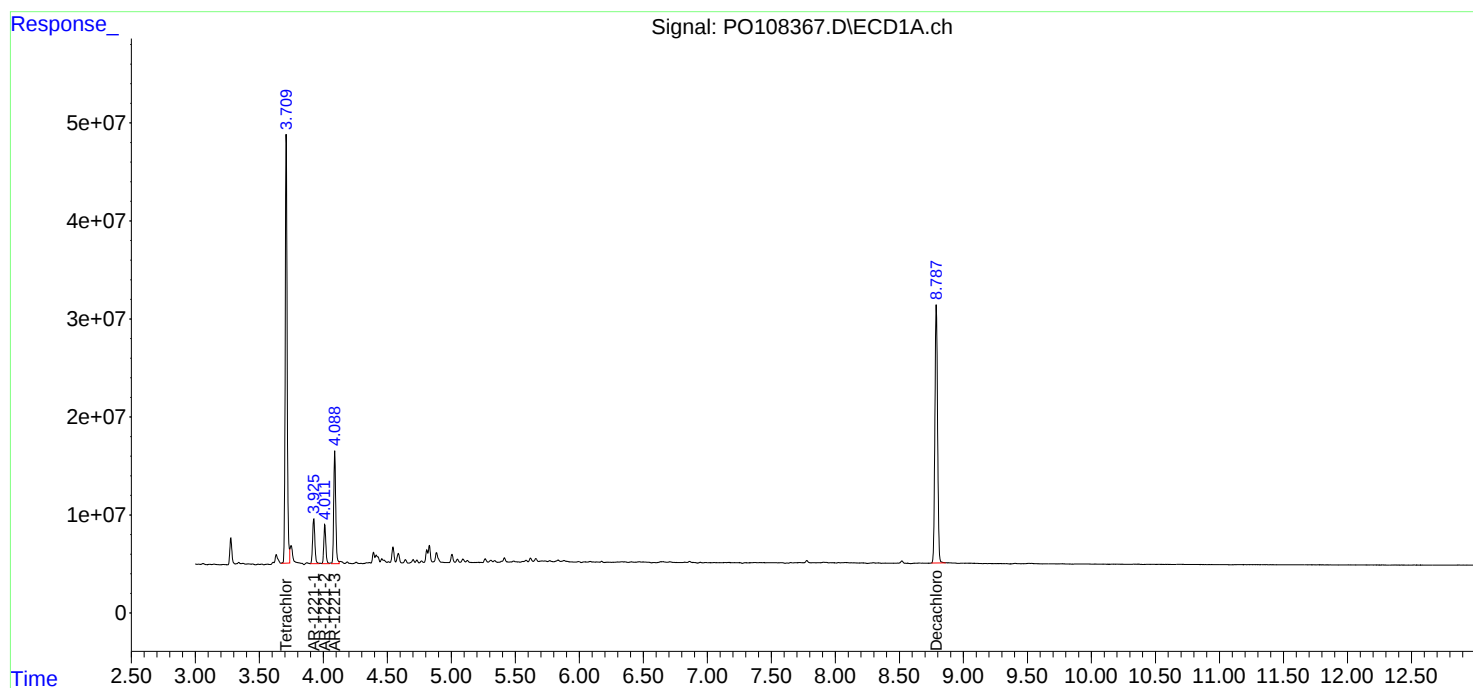

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 16:09
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:22:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 03:22:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.710	3.708	444.2E6	248.7E6	50.000	50.000
2) SA Decachlor...	8.789	8.741	367.4E6	196.5E6	50.000	50.000
Target Compounds						
11) L3 AR-1232-1	4.089	4.084	102.4E6	56025919	500.000	500.000
12) L3 AR-1232-2	4.586	4.817	57176726	52877010	500.000	500.000
13) L3 AR-1232-3	4.829	4.994	98738250	30173584	500.000	500.000
14) L3 AR-1232-4	5.005	5.078	54189863	27778236	500.000	500.000
15) L3 AR-1232-5	5.048	5.249	39164726	28788093	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 16:09
Operator : YP/AJ
Sample : AR1232ICC500
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:22:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:22:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

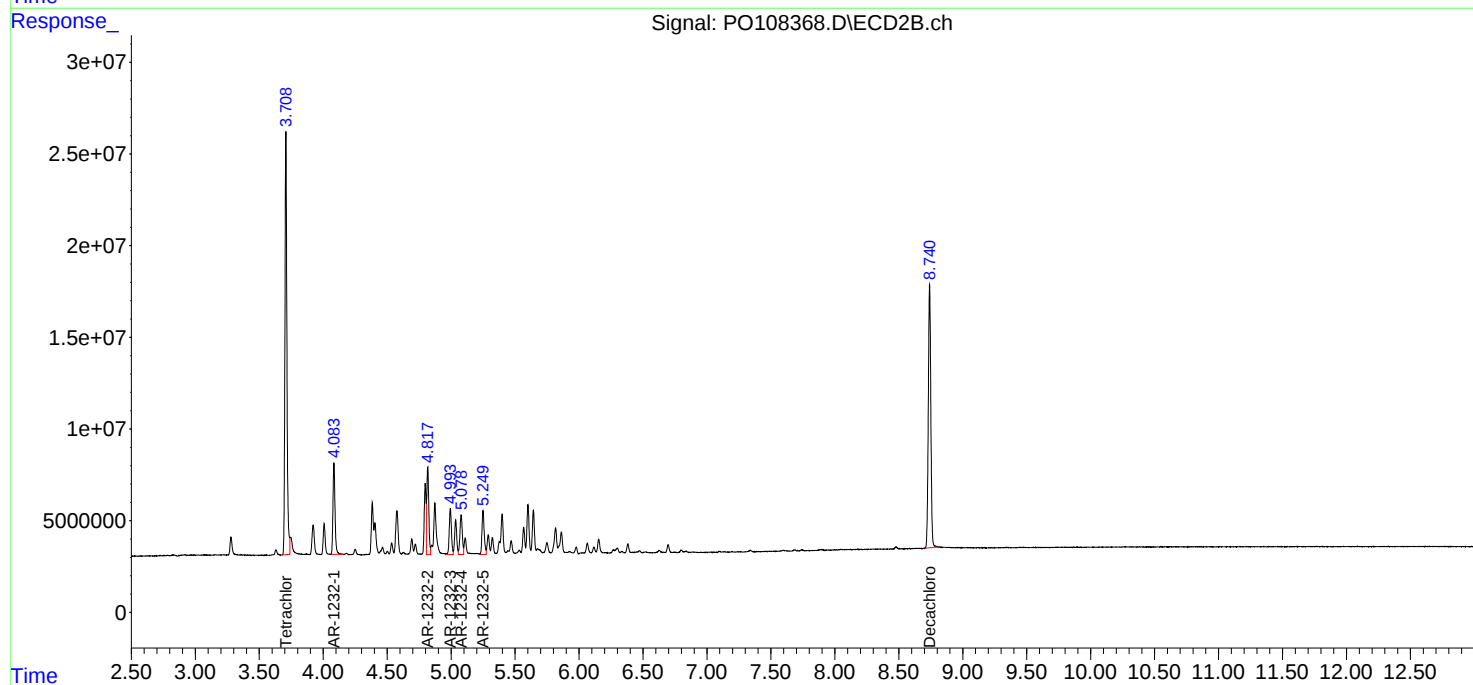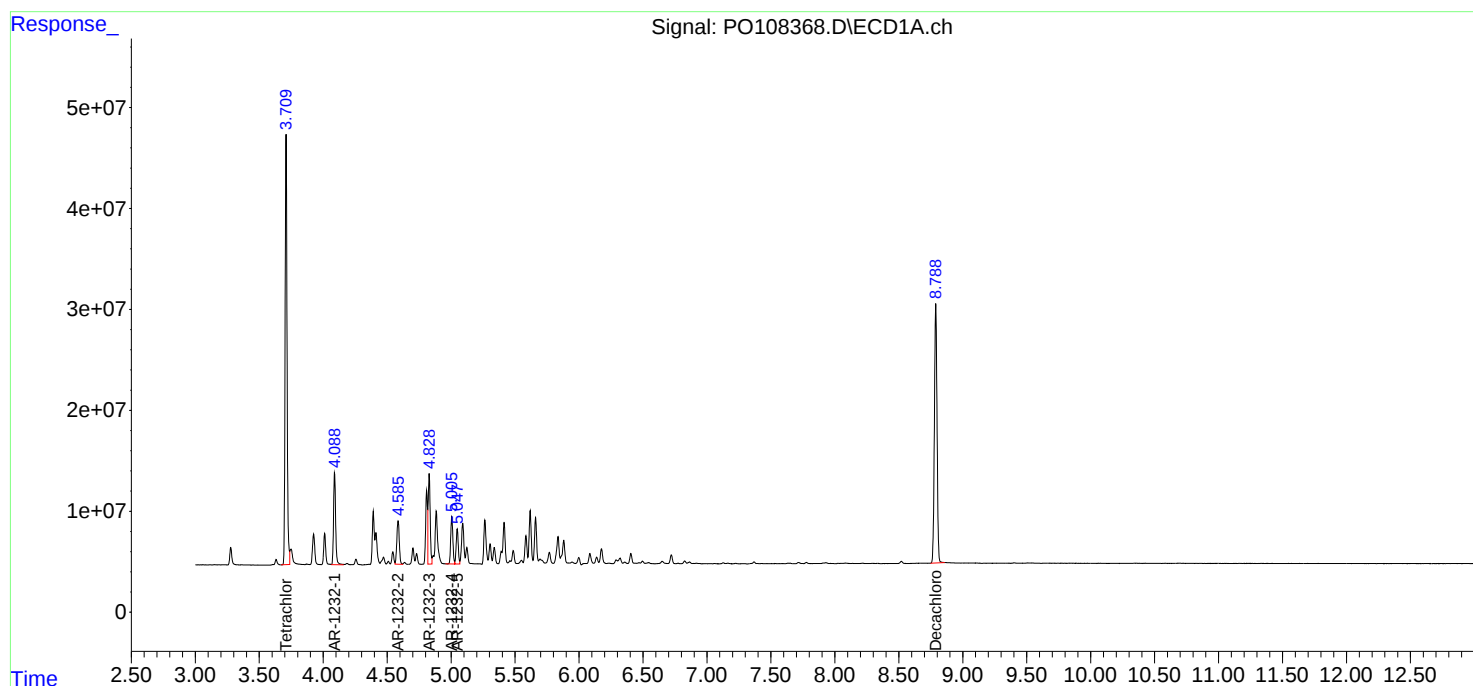

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 16:28
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:28:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 03:28:21 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	892.1E6	517.6E6	101.957	102.233
2) SA Decachlor...	8.787	8.740	715.2E6	383.8E6	98.518	97.601
Target Compounds						
16) L4 AR-1242-1	4.808	4.798	247.1E6	129.5E6	986.267	975.957
17) L4 AR-1242-2	4.828	4.818	337.8E6	181.1E6	994.614	988.288
18) L4 AR-1242-3	4.884	4.993	232.4E6	100.9E6	976.542	980.579
19) L4 AR-1242-4	5.005	5.078	184.2E6	100.4E6	985.499	961.375
20) L4 AR-1242-5	5.660	5.601	194.0E6	119.2E6	982.463	977.241


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 16:28
Operator : YP/AJ
Sample : AR1242ICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:28:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:28:21 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

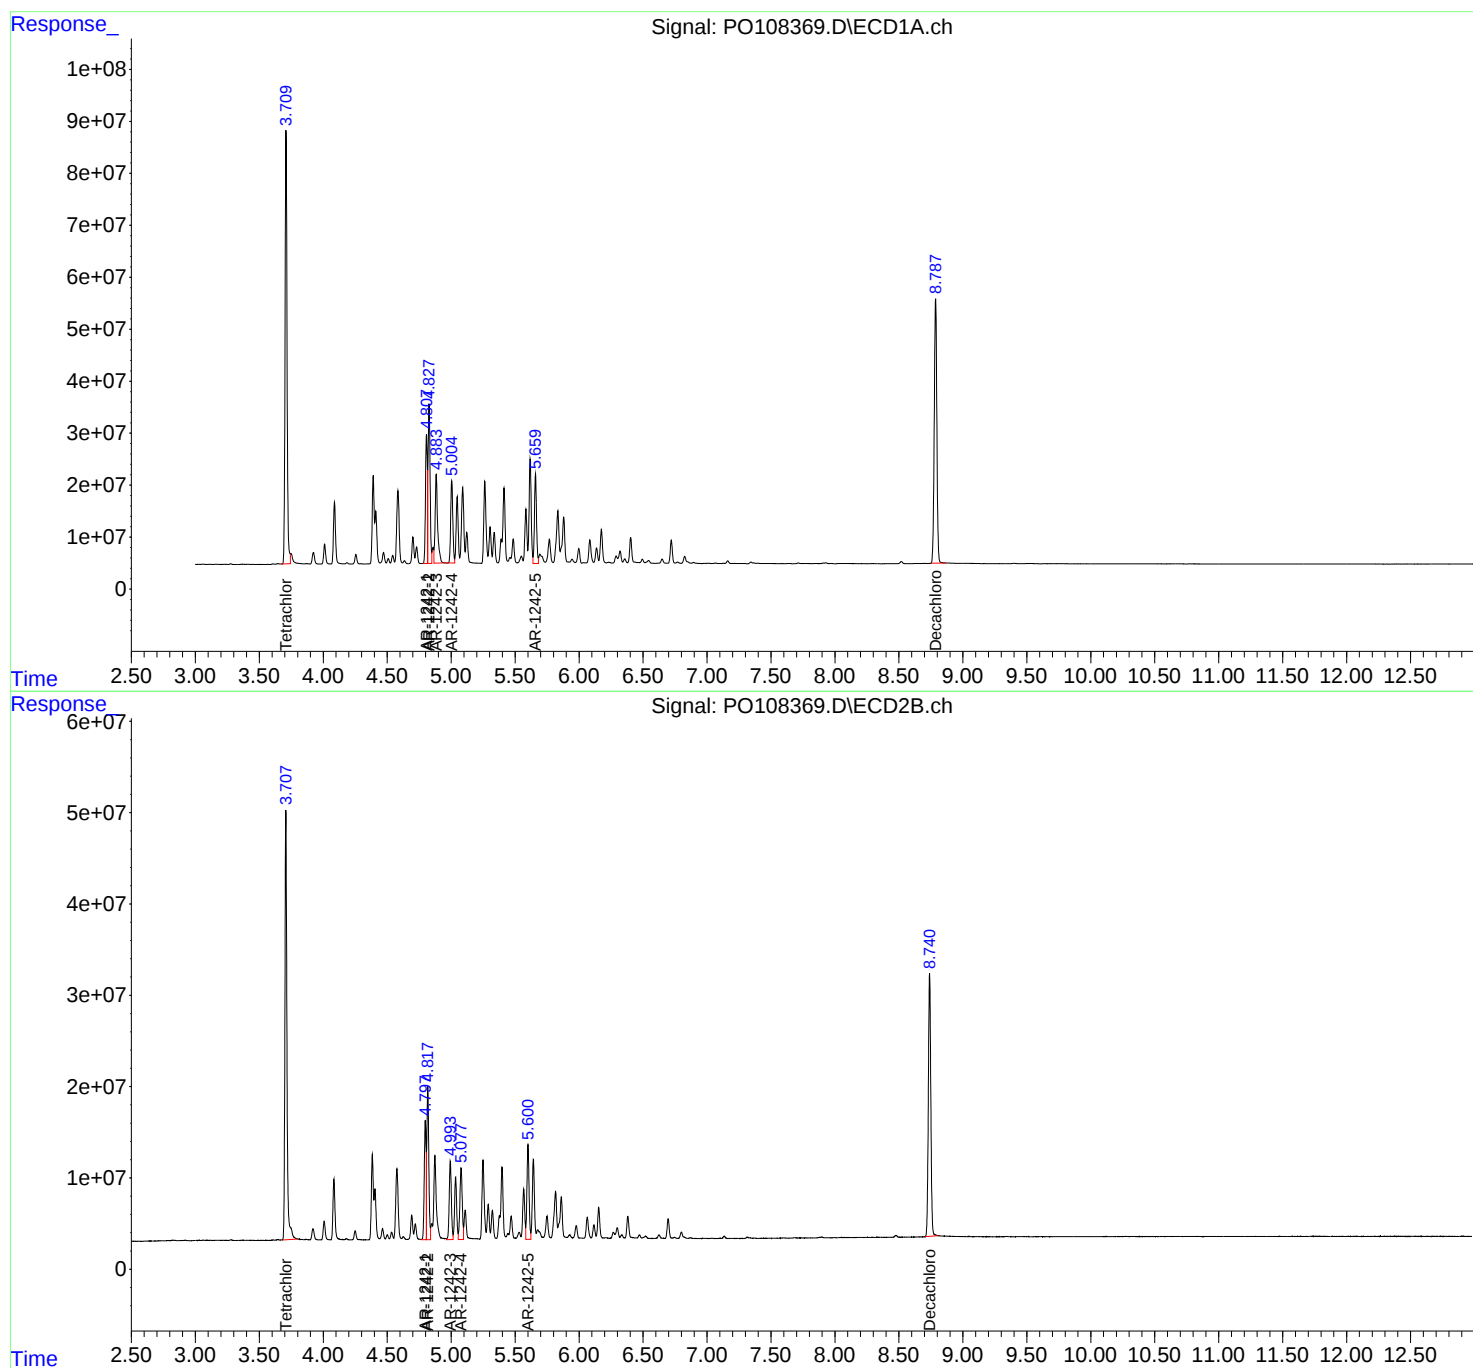

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 16:46
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:29:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 03:28:21 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	651.9E6	379.2E6	74.501	74.904
2) SA Decachlor...	8.787	8.741	537.5E6	291.1E6	74.048	74.041
Target Compounds						
16) L4 AR-1242-1	4.808	4.797	183.3E6	96799225	731.717	729.672
17) L4 AR-1242-2	4.828	4.817	249.4E6	135.2E6	734.320	737.938
18) L4 AR-1242-3	4.883	4.993	171.7E6	75364148	721.601	732.062
19) L4 AR-1242-4	5.005	5.078	134.3E6	75299205	718.502	721.202
20) L4 AR-1242-5	5.660	5.601	146.1E6	89249979	739.628	731.432



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 16:46
Operator : YP/AJ
Sample : AR1242ICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:29:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:28:21 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

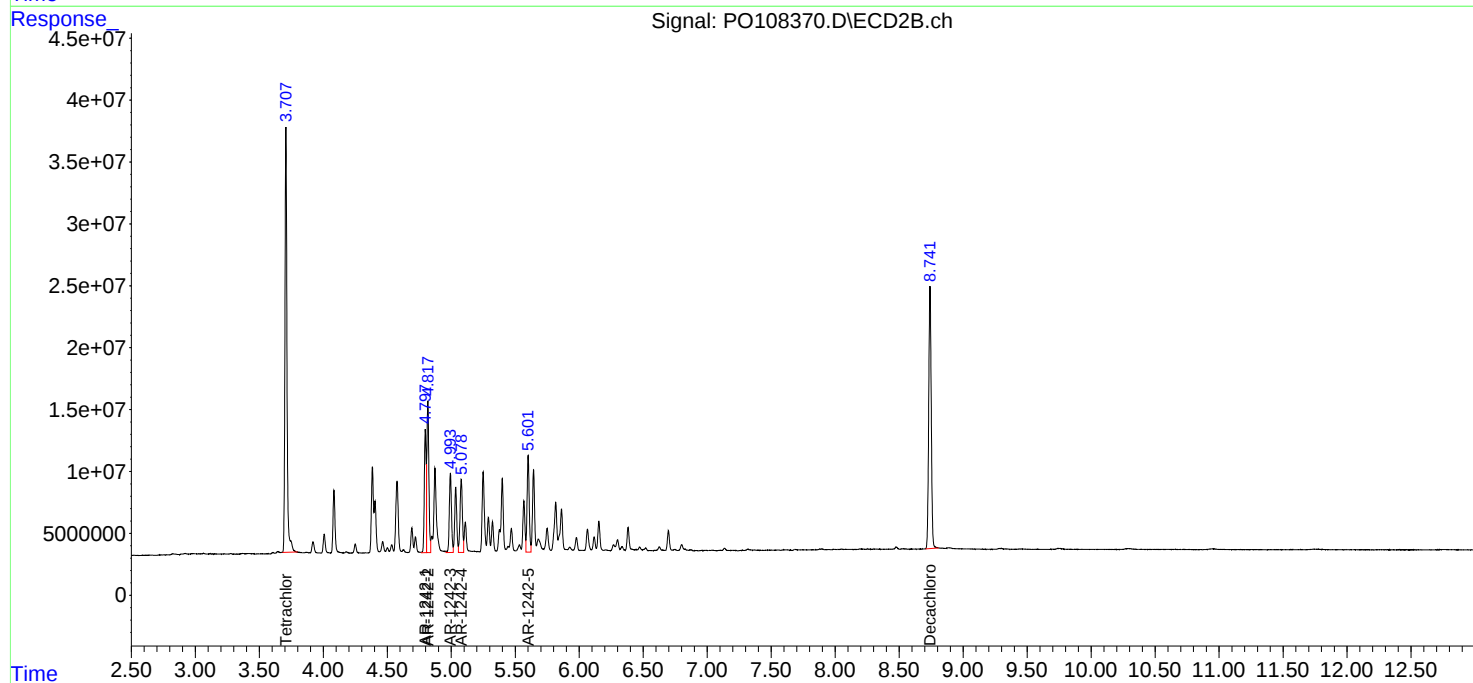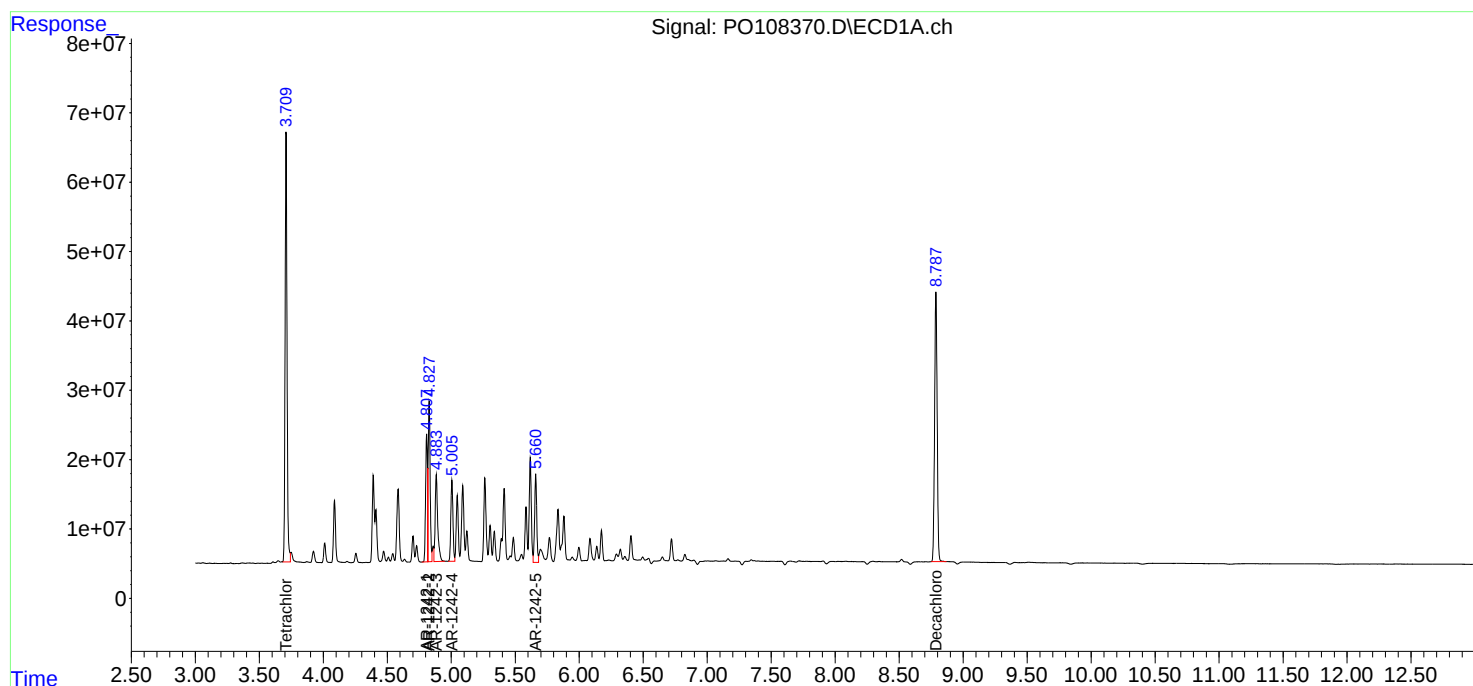

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 17:04
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:29:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 03:28:21 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.710	3.708	437.5E6	253.1E6	50.000	50.000
2) SA Decachlor...	8.788	8.740	363.0E6	196.6E6	50.000	50.000
Target Compounds						
16) L4 AR-1242-1	4.808	4.797	125.3E6	66330645	500.000	500.000
17) L4 AR-1242-2	4.828	4.817	169.8E6	91631995	500.000	500.000
18) L4 AR-1242-3	4.884	4.993	119.0E6	51473854	500.000	500.000
19) L4 AR-1242-4	5.005	5.078	93477622	52203987	500.000	500.000
20) L4 AR-1242-5	5.660	5.601	98737288	61010454	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 17:04
Operator : YP/AJ
Sample : AR1242ICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:29:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:28:21 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

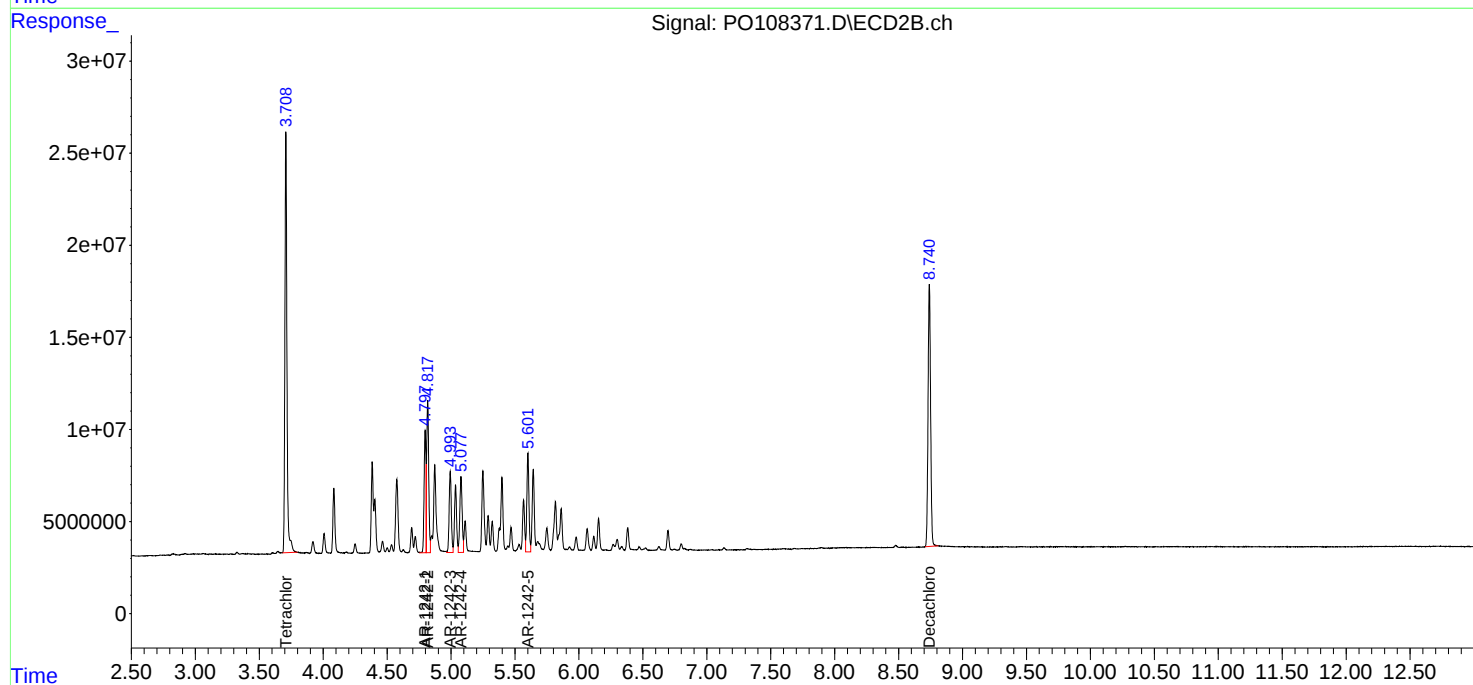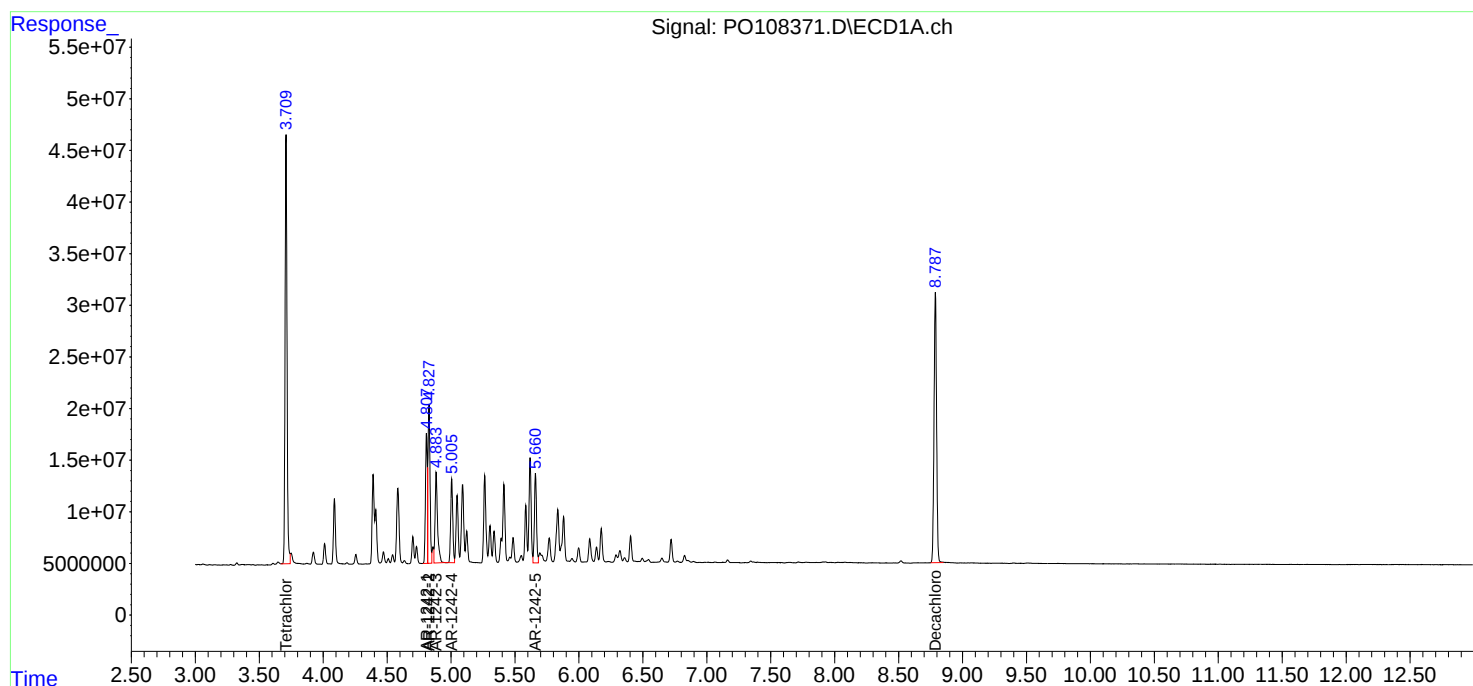

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 17:23
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:29:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 03:28:21 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	221.1E6	126.9E6	25.264	25.073
2) SA Decachlor...	8.787	8.740	192.4E6	103.6E6	26.501	26.338
Target Compounds						
16) L4 AR-1242-1	4.808	4.797	67263038	35363657	268.444	266.571
17) L4 AR-1242-2	4.828	4.817	89248071	47903183	262.765	261.389
18) L4 AR-1242-3	4.883	4.993	62854493	27129555	264.126	263.528
19) L4 AR-1242-4	5.004	5.078	49135003	27967035	262.817	267.863
20) L4 AR-1242-5	5.660	5.600	54535027	32733791	276.162	268.264



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 17:23
Operator : YP/AJ
Sample : AR1242ICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:29:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:28:21 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

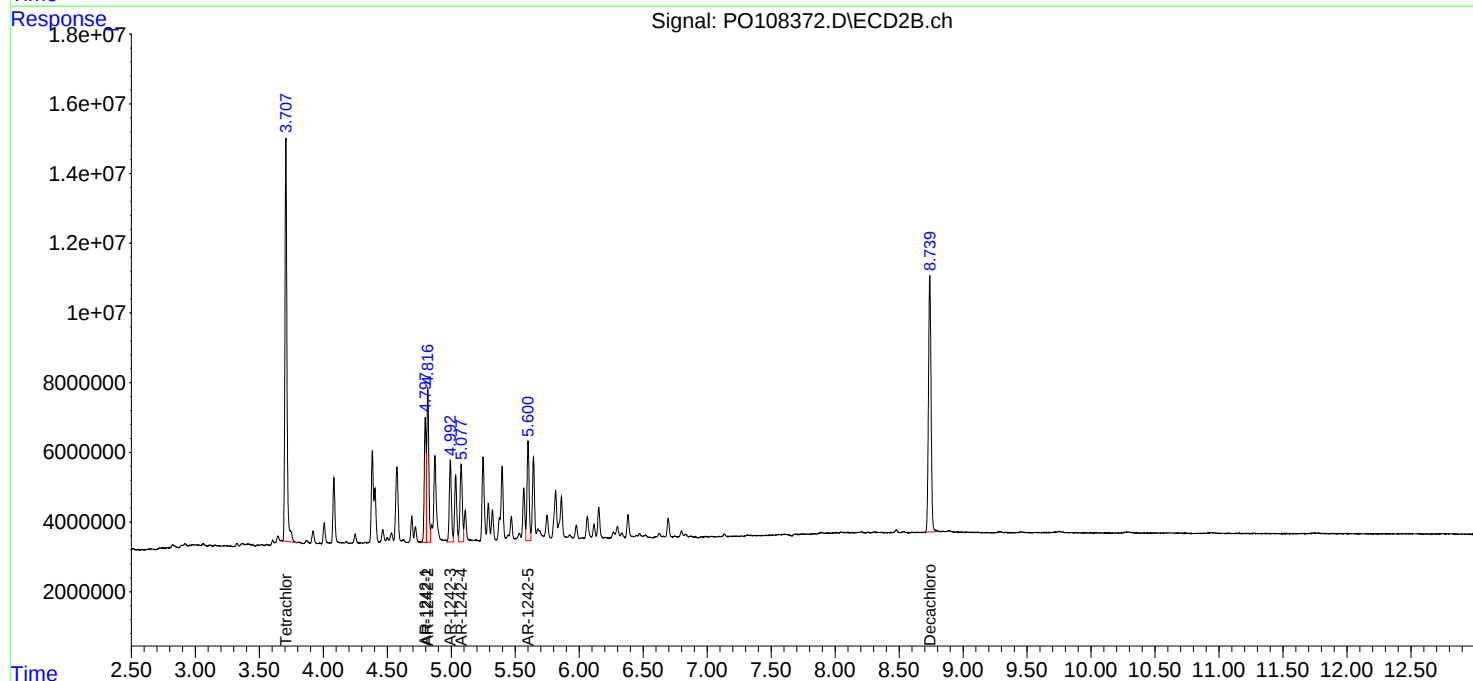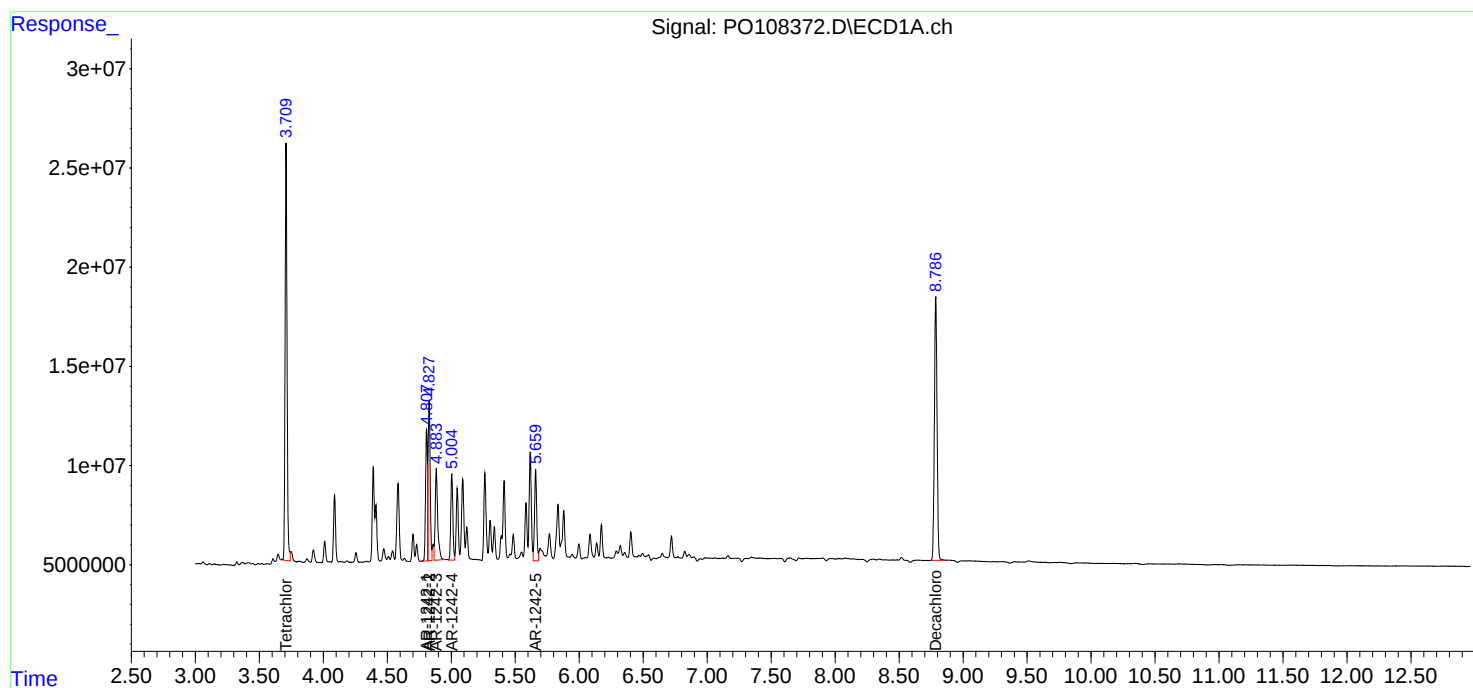

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 17:41
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/09/2024
 Supervised By :Ankita Jodhani 12/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:30:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 03:28:21 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.708	3.707	42500192	23470301	4.857	4.636
2)	SA Decachlor...	8.786	8.739	38080770	19909368	5.246	5.063
Target Compounds							
16)	L4 AR-1242-1	4.806	4.796	13771137	7309320	54.960	55.098
17)	L4 AR-1242-2	4.826	4.816	17939884	9549021	52.819	52.105
18)	L4 AR-1242-3	4.882	4.992	12765923	5700607	53.645	55.374
19)	L4 AR-1242-4	5.004	5.077	10336411	5979654	55.288	57.272
20)	L4 AR-1242-5	5.658	5.599	11699197	7040034	59.244m	57.695

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 17:41
Operator : YP/AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2024
Supervised By :Ankita Jodhani 12/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:30:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:28:21 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

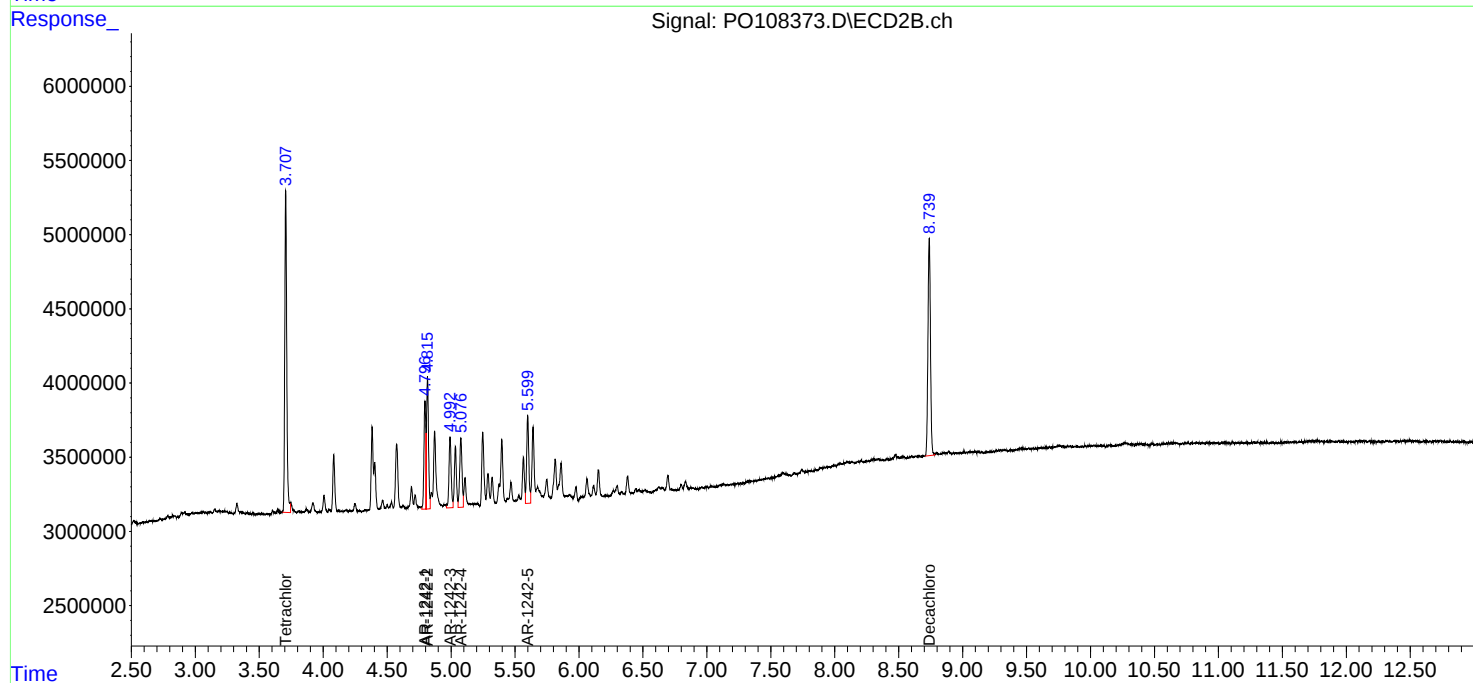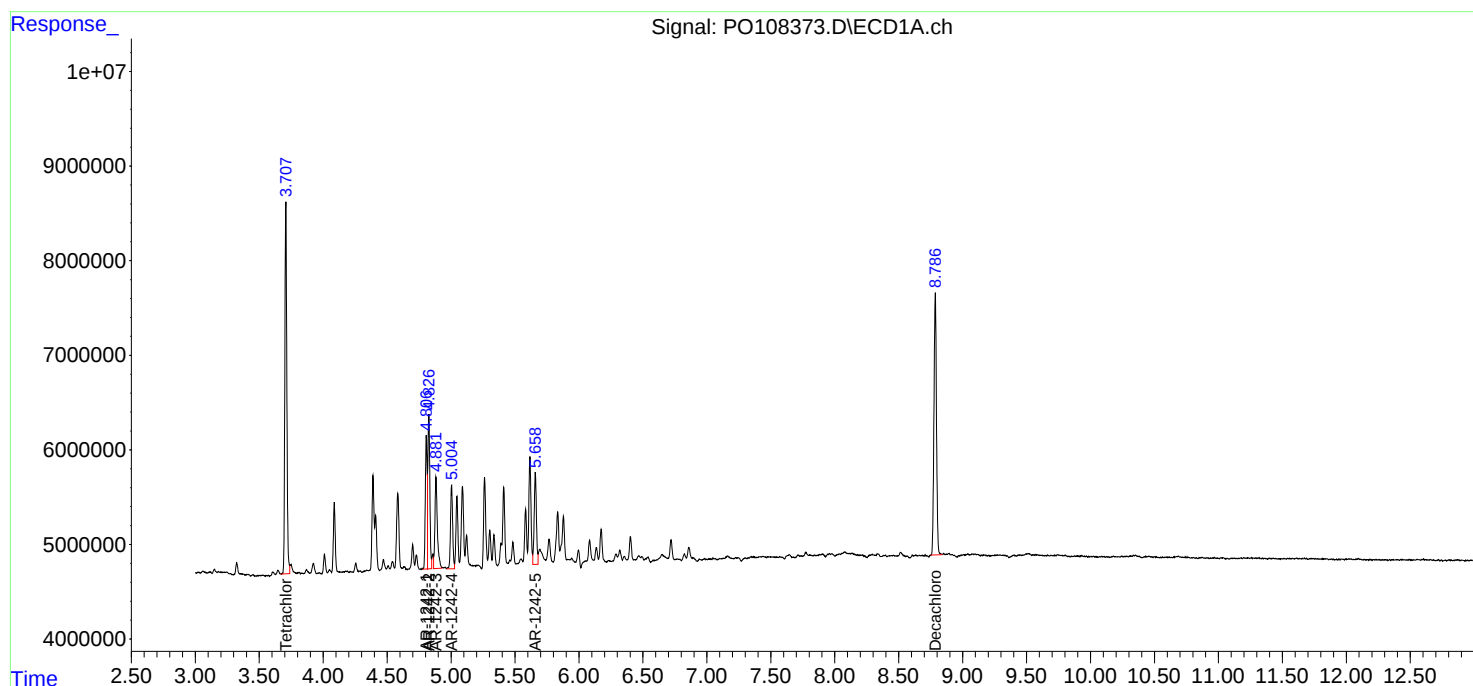

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108374.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 17:59
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:53:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 03:53:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	874.2E6	496.6E6	93.578	94.826
2) SA Decachlor...	8.786	8.739	704.2E6	381.2E6	91.719	91.964
Target Compounds						
21) L5 AR-1248-1	4.807	4.797	180.4E6	96151235	902.658	905.308
22) L5 AR-1248-2	5.047	5.035	246.3E6	134.5E6	889.469	895.026
23) L5 AR-1248-3	5.263	5.077	307.8E6	143.3E6	899.086	897.430
24) L5 AR-1248-4	5.618	5.249	437.7E6	168.4E6	912.944	911.152
25) L5 AR-1248-5	5.660	5.643	308.8E6	162.2E6	910.430	920.672



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108374.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 17:59
Operator : YP/AJ
Sample : AR1248ICC1000
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:53:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:53:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

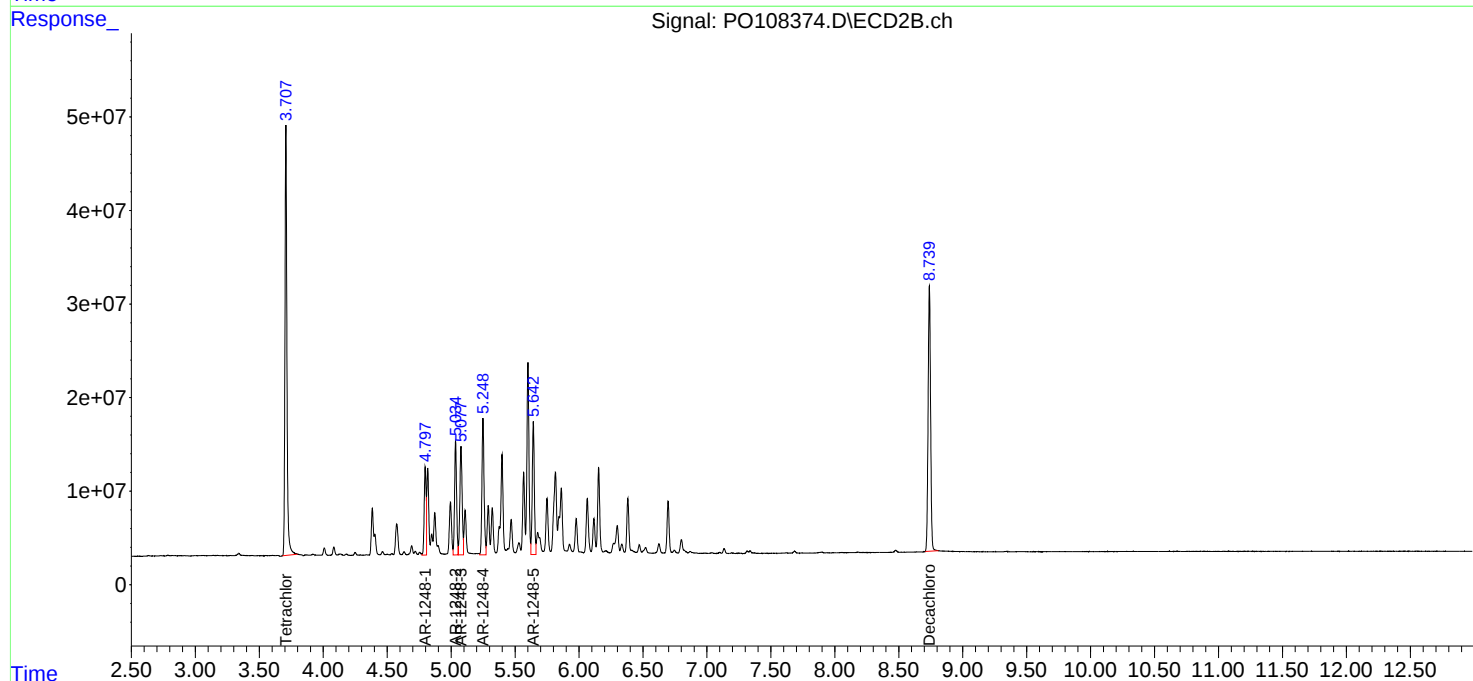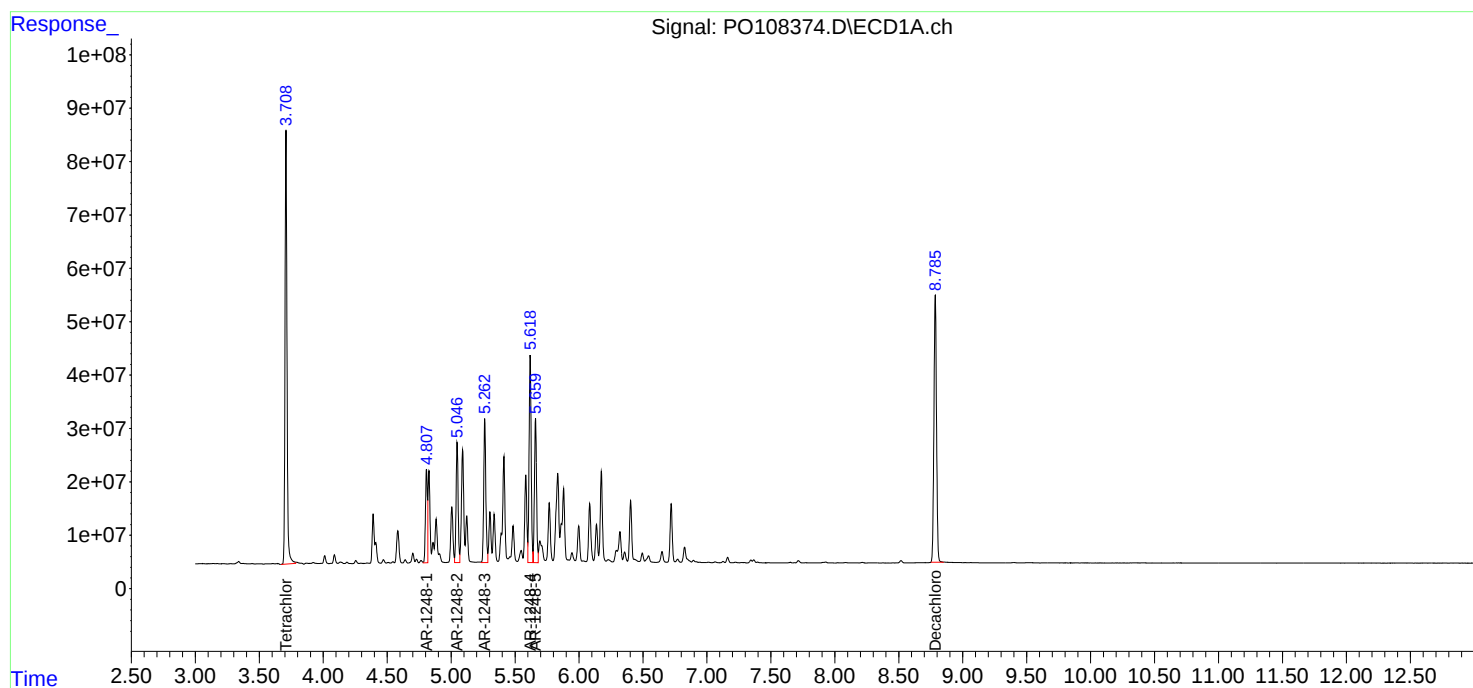

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 18:18
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:54:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 03:53:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	683.8E6	385.8E6	73.188	73.674
2) SA Decachlor...	8.787	8.739	550.5E6	298.0E6	71.701	71.892
Target Compounds						
21) L5 AR-1248-1	4.807	4.797	143.2E6	75879957	716.165	714.444
22) L5 AR-1248-2	5.047	5.035	196.8E6	106.9E6	710.590	711.516
23) L5 AR-1248-3	5.263	5.077	244.9E6	113.3E6	715.291	709.469
24) L5 AR-1248-4	5.617	5.249	343.4E6	133.0E6	716.151	719.504
25) L5 AR-1248-5	5.660	5.643	242.5E6	126.2E6	714.899	716.296



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 18:18
Operator : YP/AJ
Sample : AR1248ICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:54:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:53:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

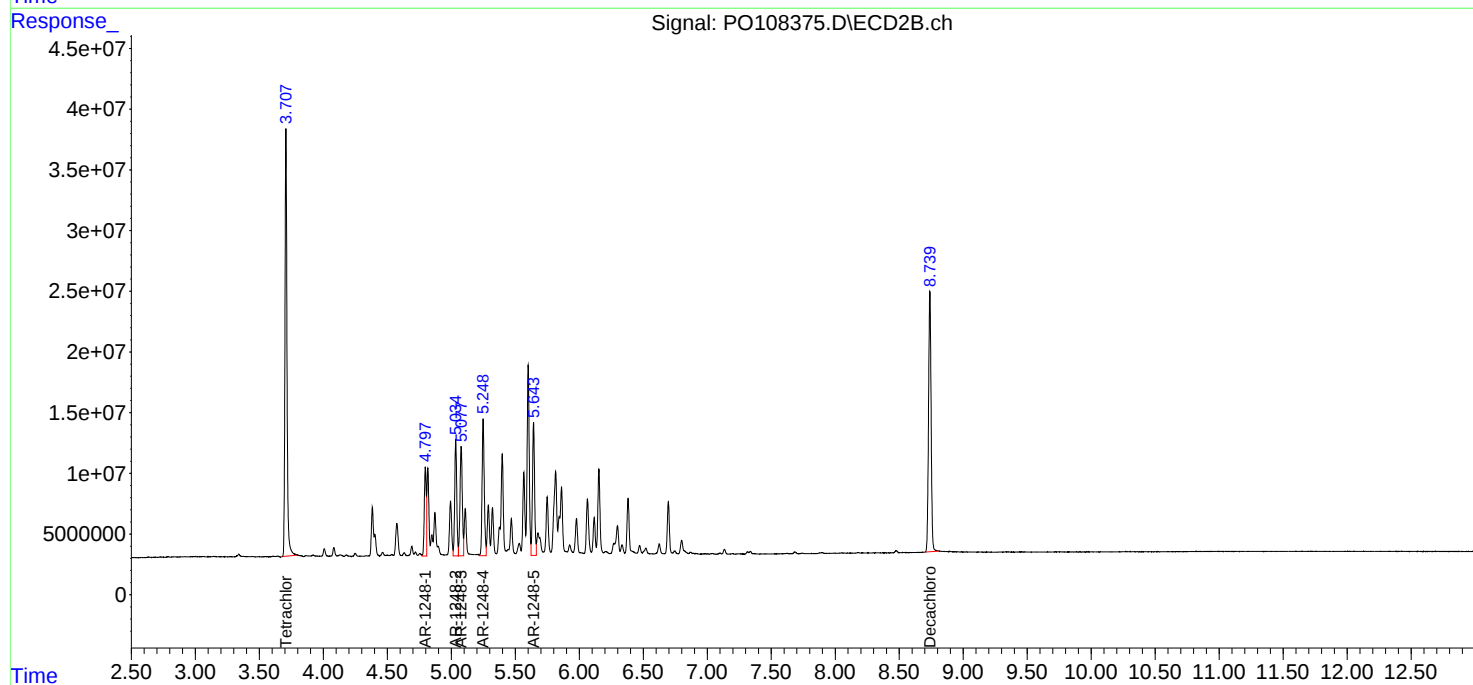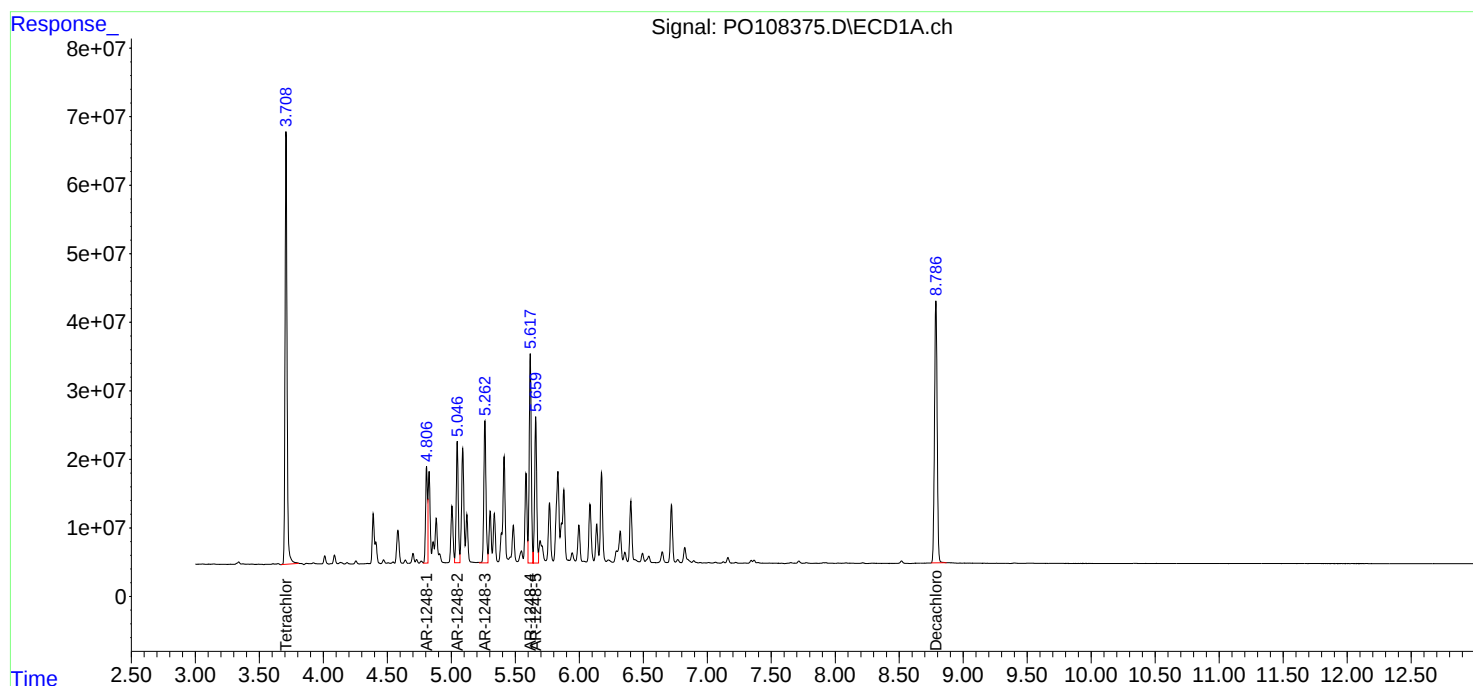

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 18:36
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:54:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 03:53:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	467.1E6	261.8E6	50.000	50.000
2) SA Decachlor...	8.786	8.740	383.9E6	207.3E6	50.000	50.000
Target Compounds						
21) L5 AR-1248-1	4.808	4.797	99951066	53104178	500.000	500.000
22) L5 AR-1248-2	5.047	5.034	138.5E6	75113048	500.000	500.000
23) L5 AR-1248-3	5.263	5.077	171.2E6	79857015	500.000	500.000
24) L5 AR-1248-4	5.618	5.249	239.7E6	92406937	500.000	500.000
25) L5 AR-1248-5	5.660	5.642	169.6E6	88072281	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 18:36
Operator : YP/AJ
Sample : AR1248ICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:54:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:53:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

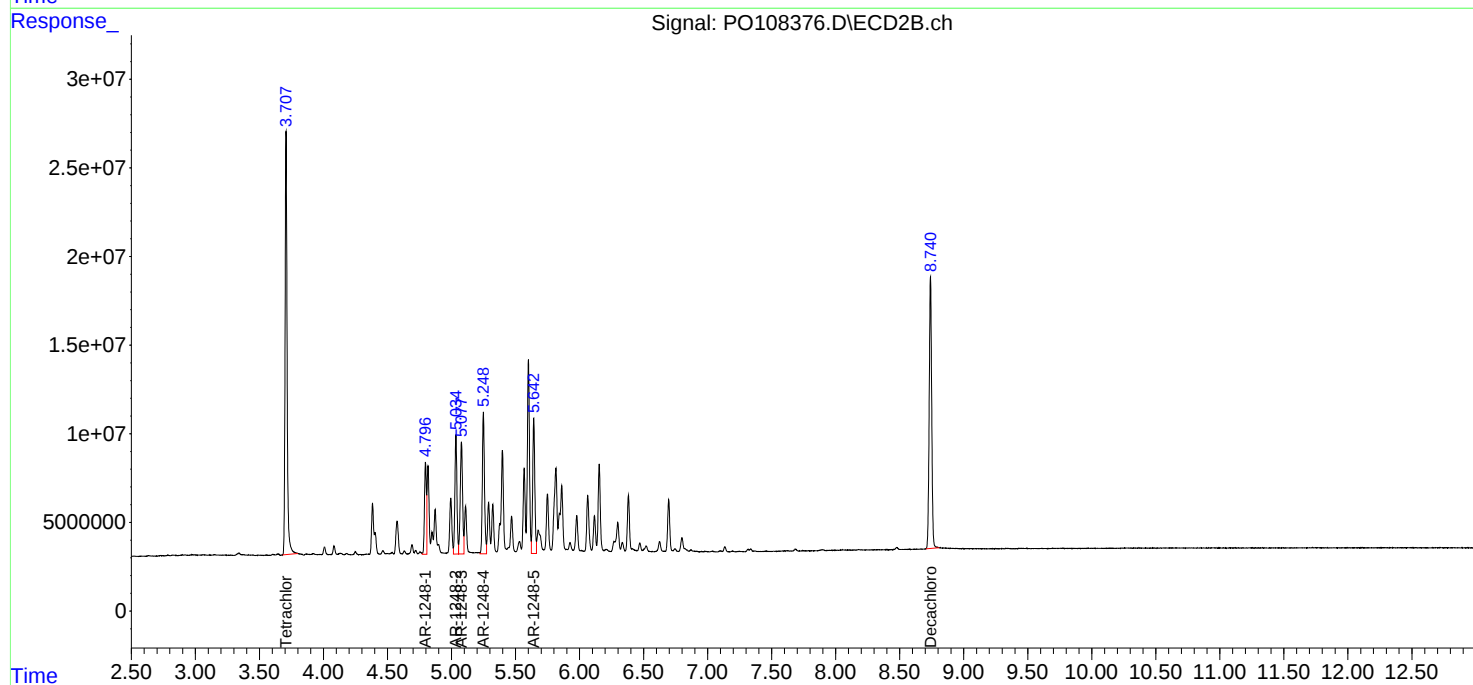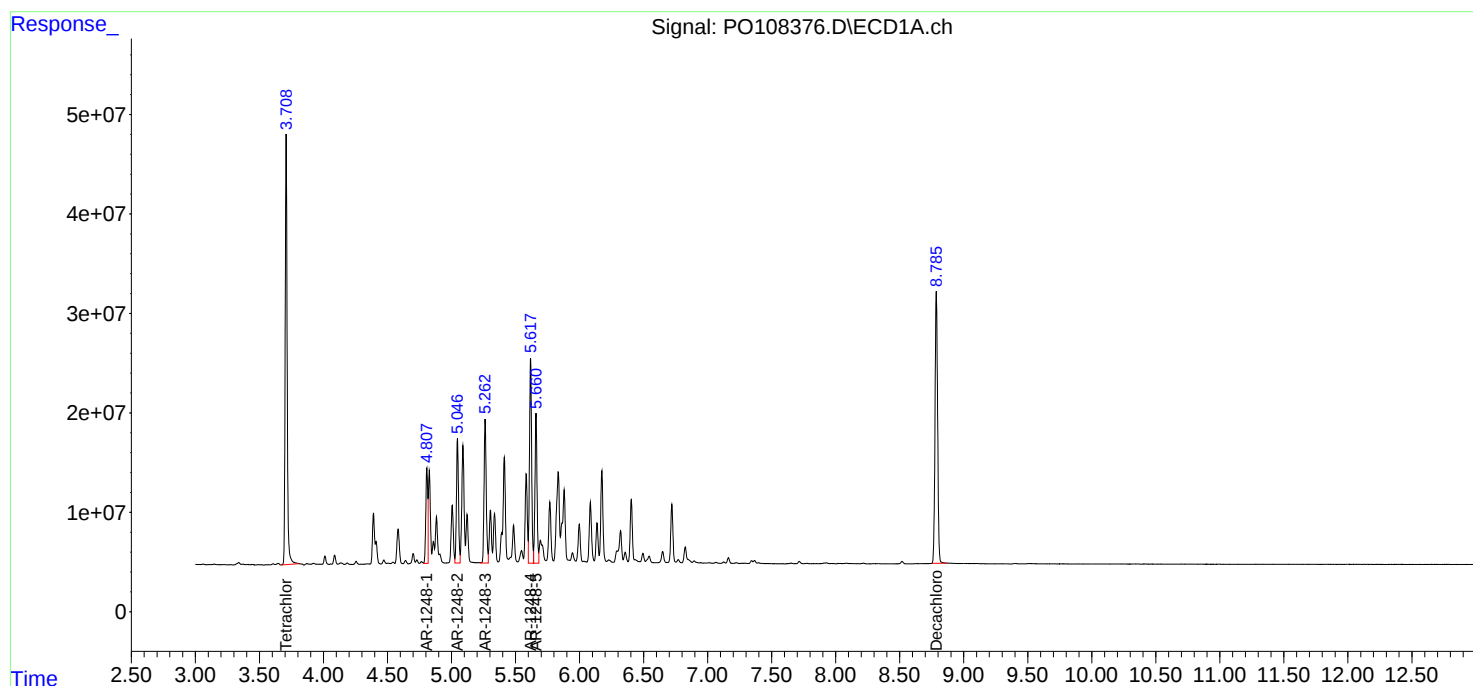

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 18:54
Operator : YP/AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:54:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:53:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.708	3.707	236.2E6	131.4E6	25.280	25.092
2)	SA Decachlor...	8.785	8.738	208.4E6	111.1E6	27.138	26.808
Target Compounds							
21)	L5 AR-1248-1	4.806	4.796	53325996	27878130	266.761	262.485
22)	L5 AR-1248-2	5.046	5.034	74645599	39915010	269.568	265.700
23)	L5 AR-1248-3	5.261	5.076	90583311	42267651	264.615	264.646
24)	L5 AR-1248-4	5.616	5.247	125.7E6	48425304	262.162	262.022
25)	L5 AR-1248-5	5.659	5.641	89499607	45702270	263.899	259.459



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 18:54
Operator : YP/AJ
Sample : AR1248ICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:54:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:53:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

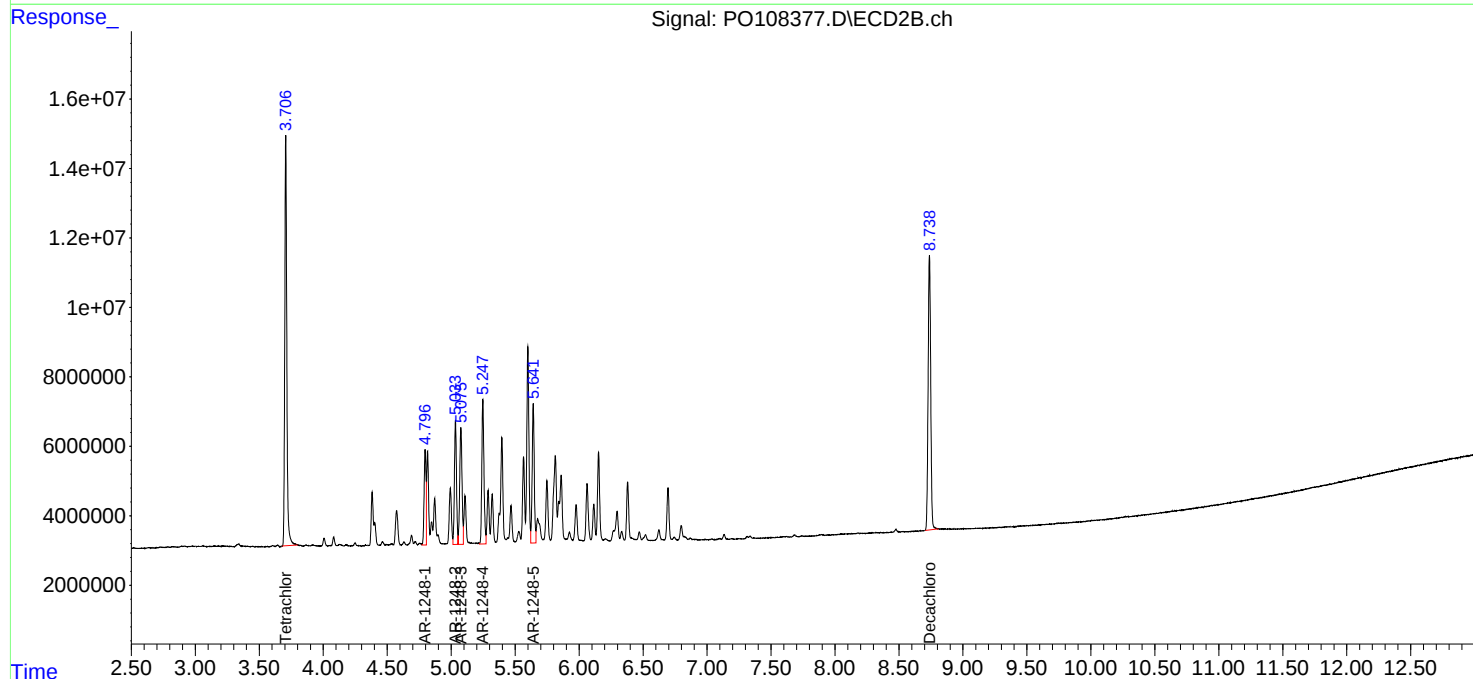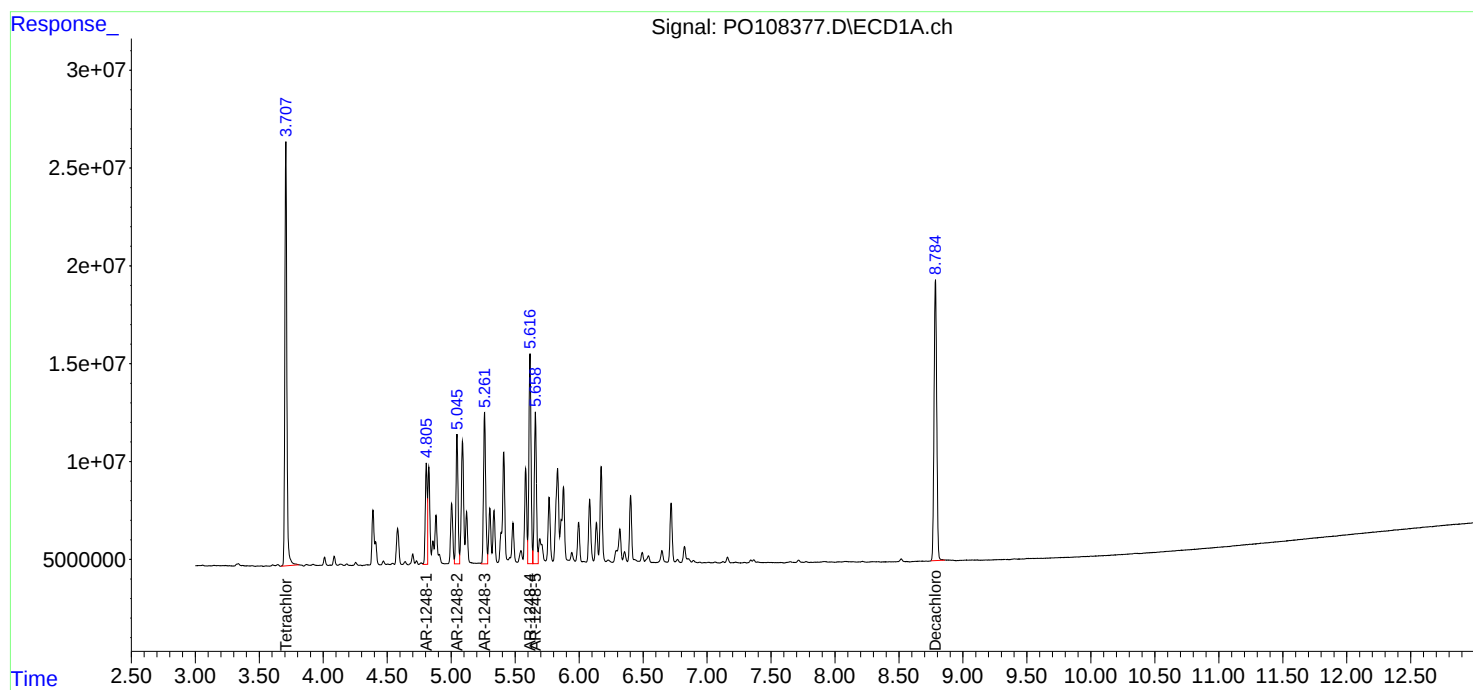

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 19:13
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/09/2024
 Supervised By :Ankita Jodhani 12/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:54:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 03:53:05 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.707	42888882	23166628	4.591	4.424
2) SA Decachlor...	8.785	8.739	41886336	21478364	5.456	5.181
Target Compounds						
21) L5 AR-1248-1	4.807	4.797	10841588	5527464	54.234	52.044
22) L5 AR-1248-2	5.047	5.035	15088946	7988873	54.491	53.179
23) L5 AR-1248-3	5.262	5.077	18304358	8442914	53.471m	52.863
24) L5 AR-1248-4	5.617	5.249	25239791	9427231	52.641m	51.009
25) L5 AR-1248-5	5.659	5.643	18193699	9433171	53.646m	53.554

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 19:13
Operator : YP/AJ
Sample : AR1248ICC050
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2024
Supervised By :Ankita Jodhani 12/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:54:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:53:05 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

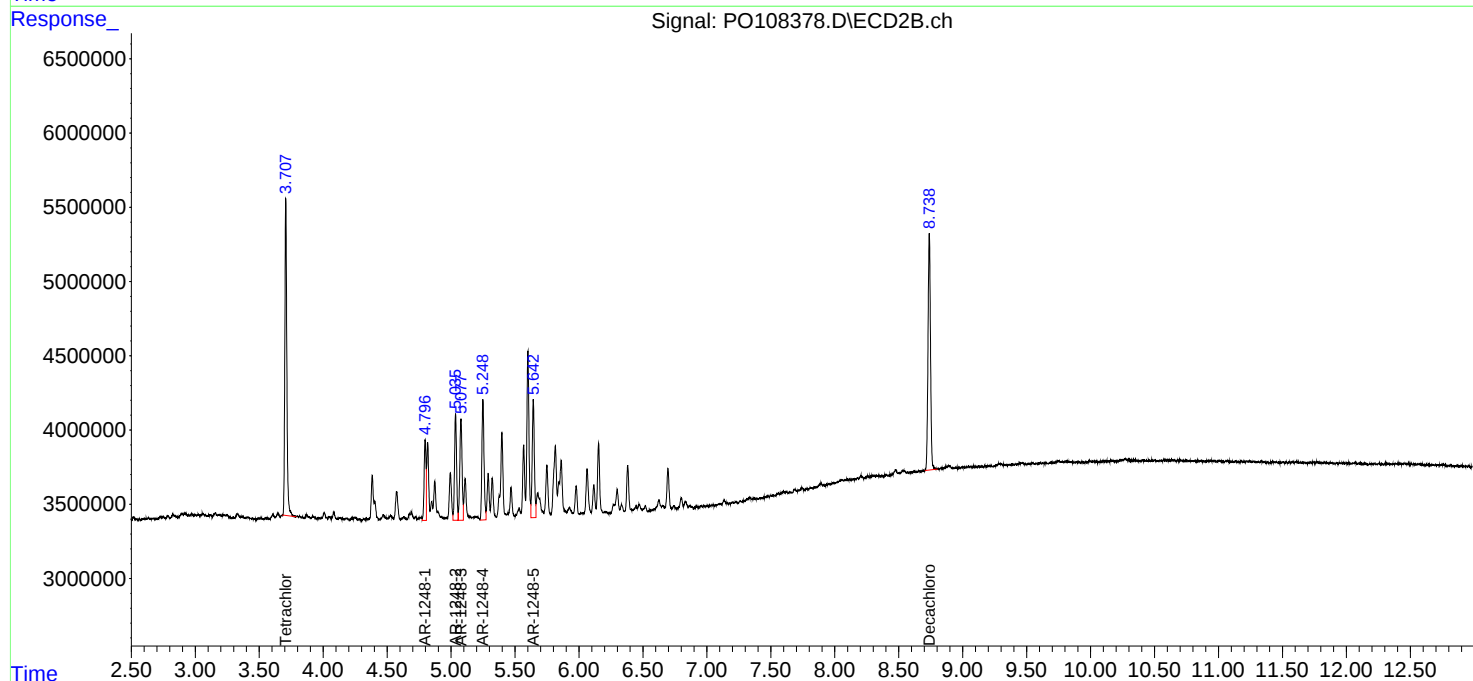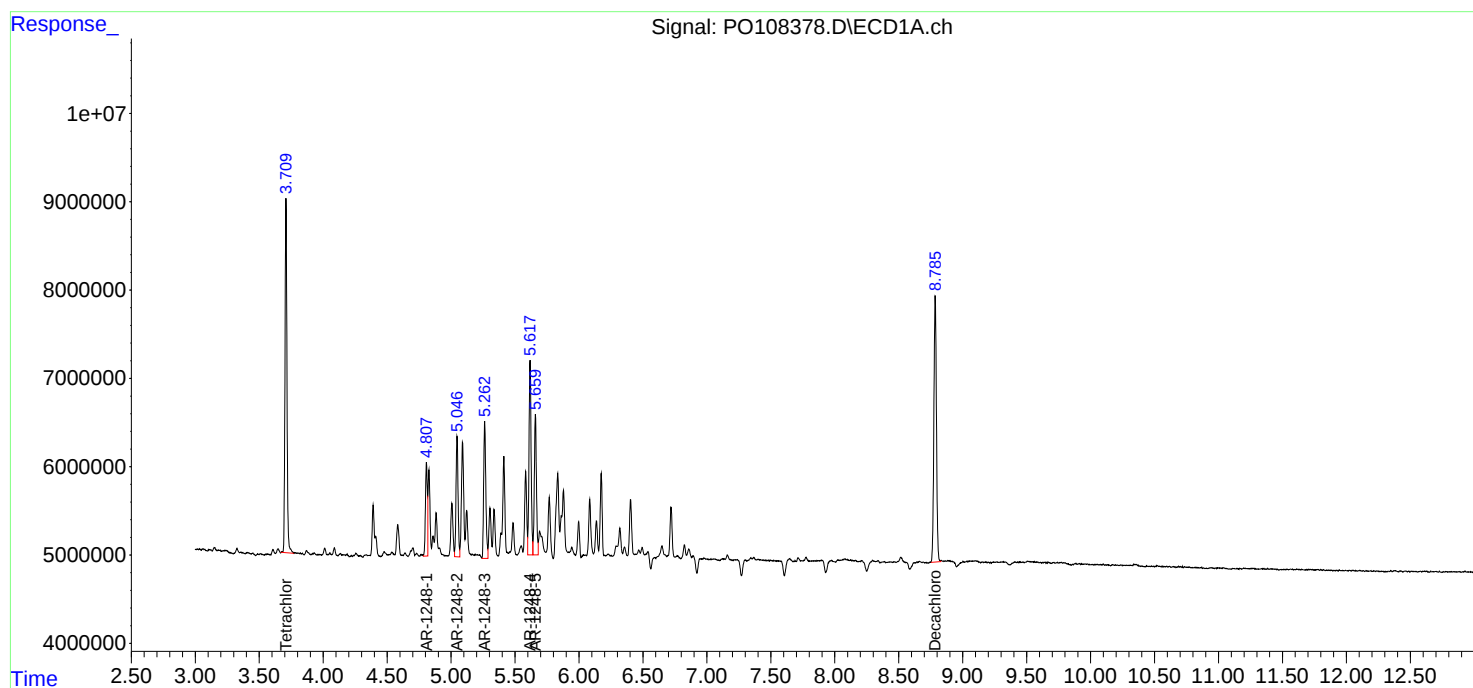

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108379.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 19:31
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 04:54:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 04:53:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	891.7E6	509.2E6	94.024	94.879
2) SA Decachlor...	8.788	8.740	714.7E6	394.1E6	91.087	92.542
Target Compounds						
26) L6 AR-1254-1	5.619	5.602	463.2E6	245.8E6	904.691	913.036
27) L6 AR-1254-2	5.768	5.749	407.0E6	215.5E6	898.746	902.392
28) L6 AR-1254-3	6.175	6.154	665.9E6	351.9E6	916.652	924.946
29) L6 AR-1254-4	6.404	6.382	404.3E6	203.0E6	909.993	920.523
30) L6 AR-1254-5	6.826	6.800	578.9E6	301.6E6	910.111	922.194



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108379.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 19:31
Operator : YP/AJ
Sample : AR1254ICC1000
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 04:54:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 04:53:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

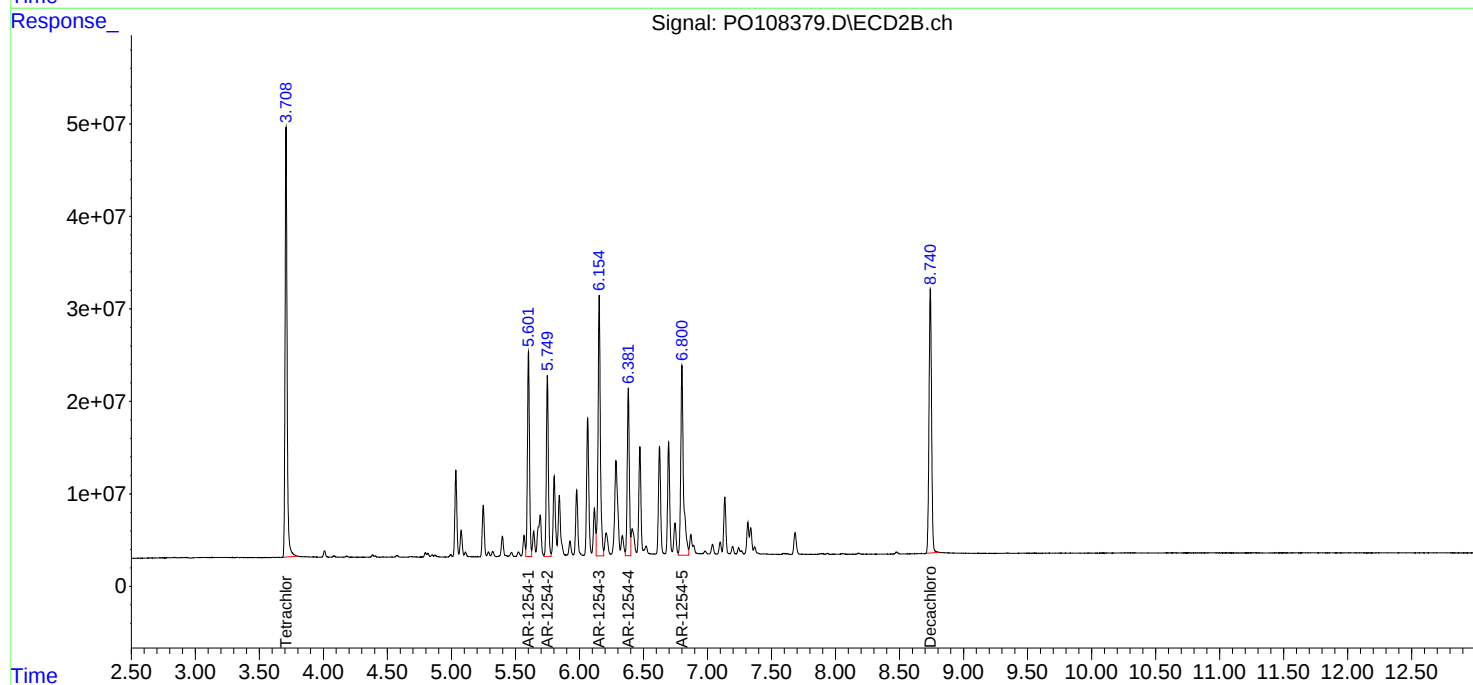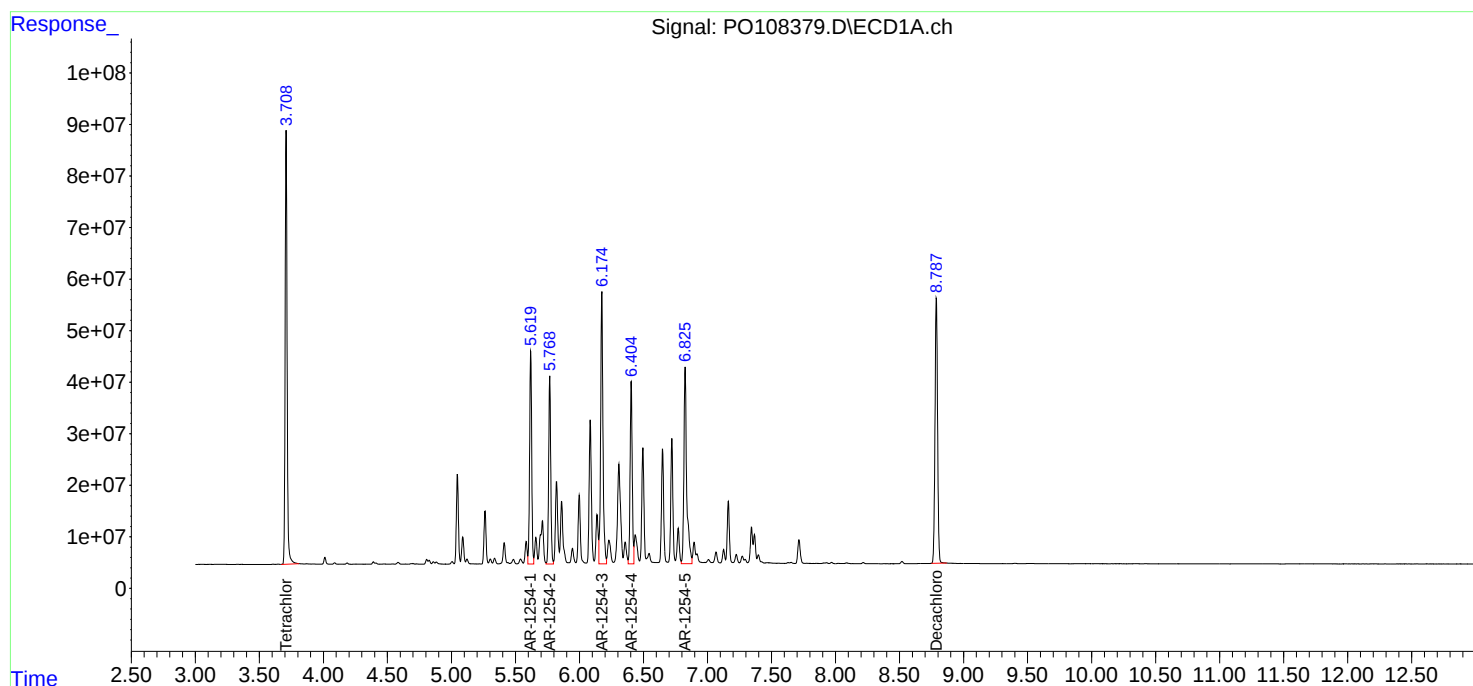

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 19:49
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 04:54:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 04:53:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	690.4E6	392.2E6	72.797	73.066
2) SA Decachlor...	8.786	8.740	558.9E6	305.4E6	71.234	71.703
Target Compounds						
26) L6 AR-1254-1	5.619	5.602	365.3E6	192.3E6	713.390	714.419
27) L6 AR-1254-2	5.768	5.749	321.9E6	169.0E6	710.657	707.972
28) L6 AR-1254-3	6.174	6.153	521.3E6	273.4E6	717.593	718.593
29) L6 AR-1254-4	6.404	6.380	315.8E6	157.4E6	710.850	714.003
30) L6 AR-1254-5	6.826	6.800	453.5E6	234.5E6	712.914	716.984



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 19:49
Operator : YP/AJ
Sample : AR1254ICC750
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 04:54:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 04:53:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

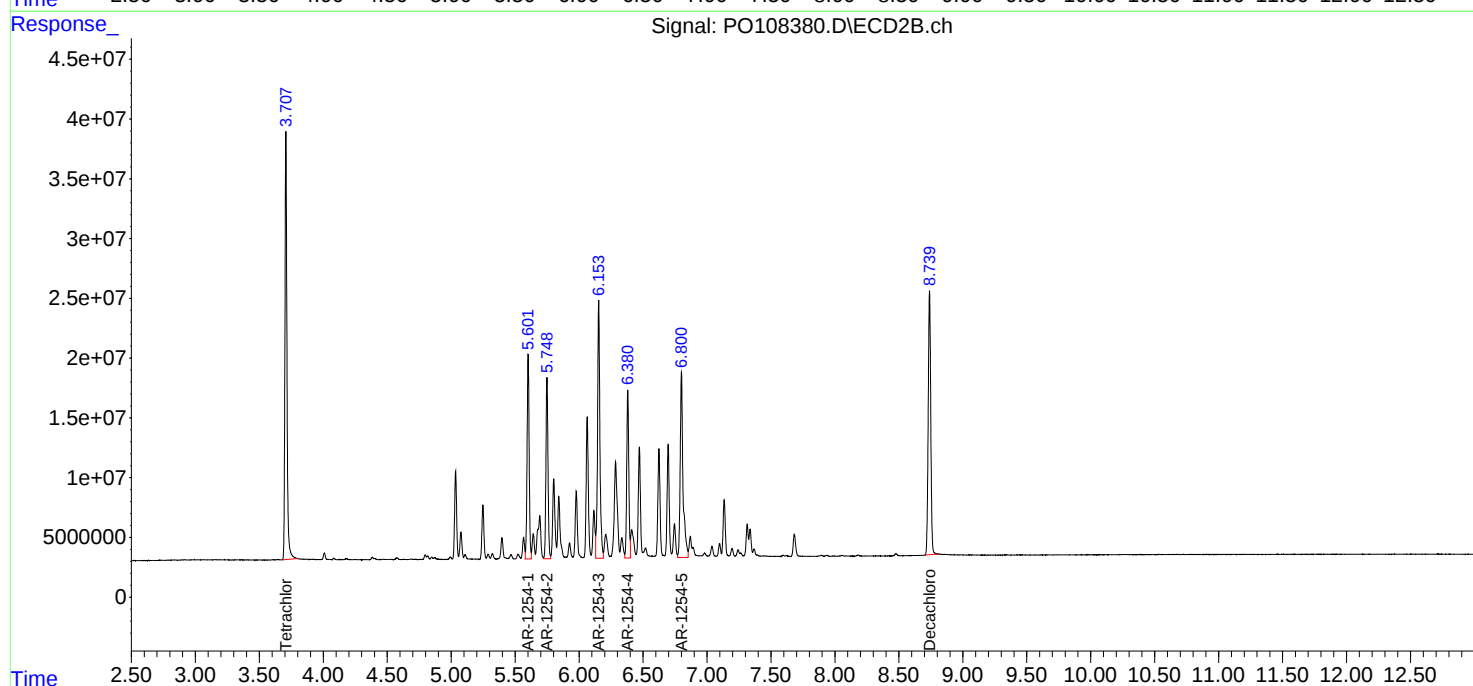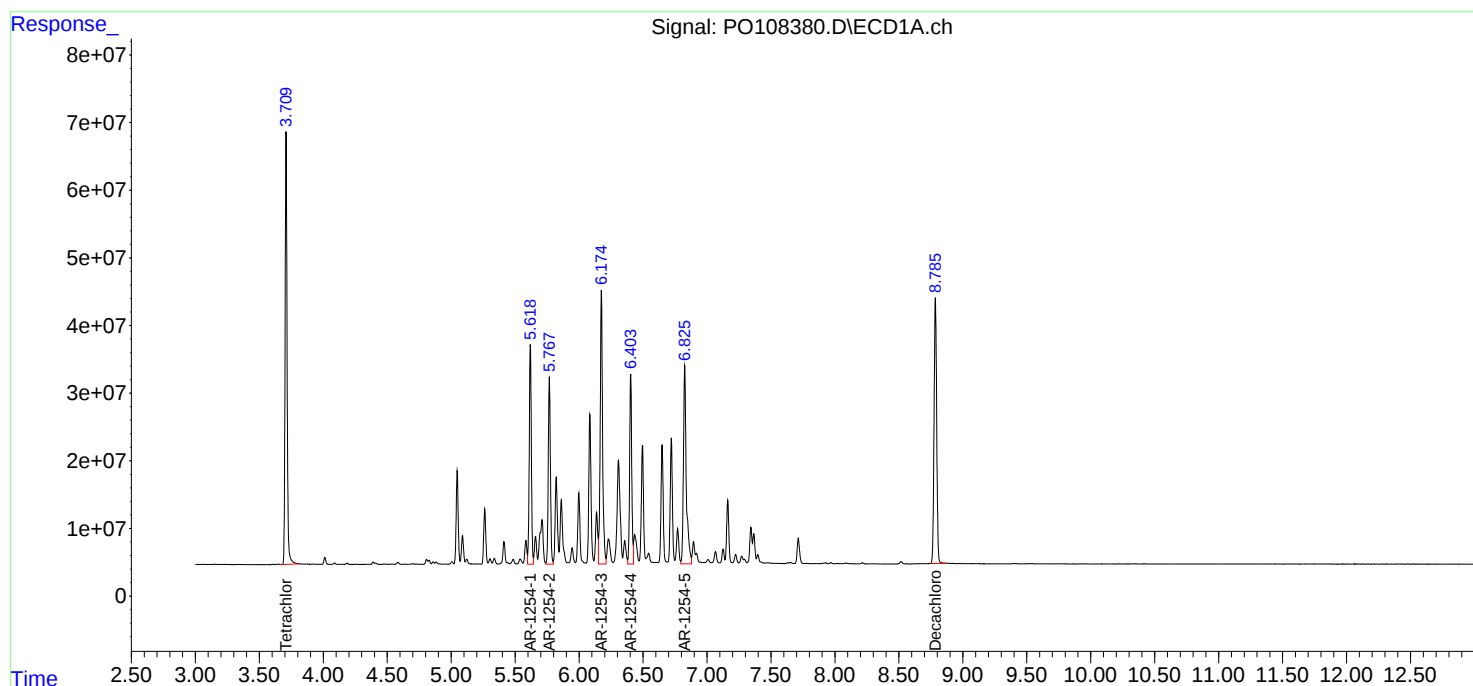

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 20:08
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 04:55:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 04:53:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.707	474.2E6	268.4E6	50.000	50.000
2) SA Decachlor...	8.786	8.738	392.3E6	212.9E6	50.000	50.000
Target Compounds						
26) L6 AR-1254-1	5.619	5.601	256.0E6	134.6E6	500.000	500.000
27) L6 AR-1254-2	5.768	5.749	226.4E6	119.4E6	500.000	500.000
28) L6 AR-1254-3	6.174	6.153	363.2E6	190.2E6	500.000	500.000
29) L6 AR-1254-4	6.404	6.381	222.1E6	110.3E6	500.000	500.000
30) L6 AR-1254-5	6.825	6.799	318.0E6	163.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 20:08
Operator : YP/AJ
Sample : AR1254ICC500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 04:55:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 04:53:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

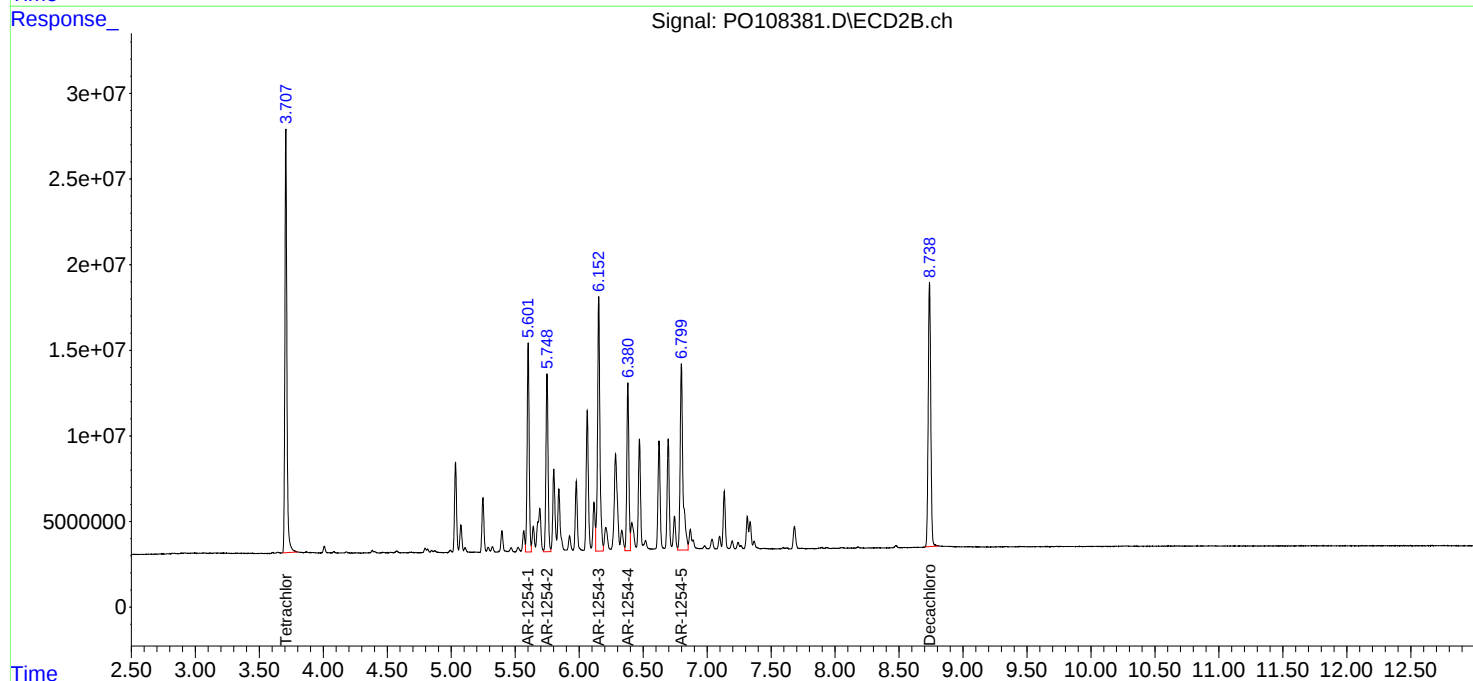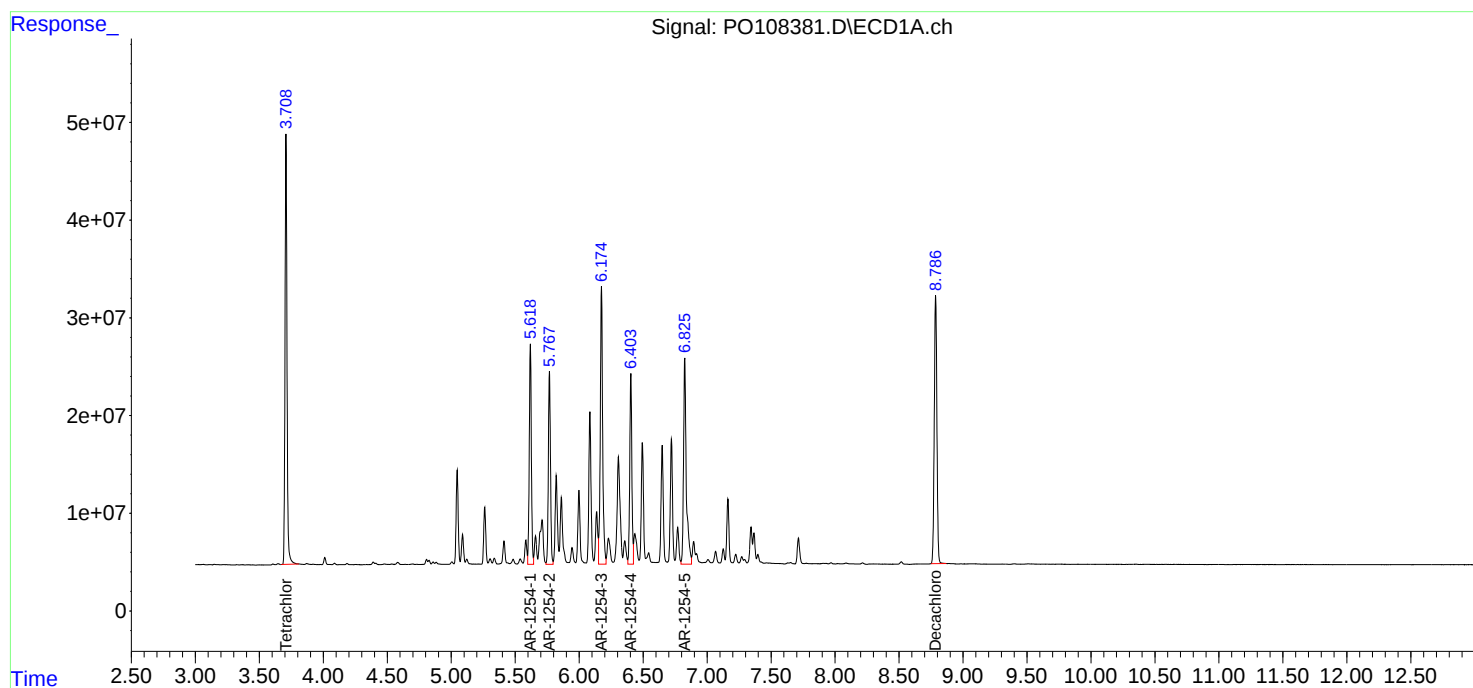

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 20:26
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 04:55:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 04:53:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.710	3.708	232.8E6	130.7E6	24.550	24.351
2)	SA Decachlor...	8.785	8.738	200.7E6	109.4E6	25.586	25.678
Target Compounds							
26)	L6 AR-1254-1	5.619	5.602	133.5E6	69803832	260.658	259.272
27)	L6 AR-1254-2	5.767	5.749	119.1E6	62204391	262.971	260.520
28)	L6 AR-1254-3	6.174	6.153	185.8E6	96697949	255.759	254.173
29)	L6 AR-1254-4	6.404	6.381	114.7E6	56523348	258.092	256.332
30)	L6 AR-1254-5	6.825	6.799	165.6E6	83204383	260.395	254.435



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 20:26
Operator : YP/AJ
Sample : AR1254ICC250
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 04:55:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 04:53:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

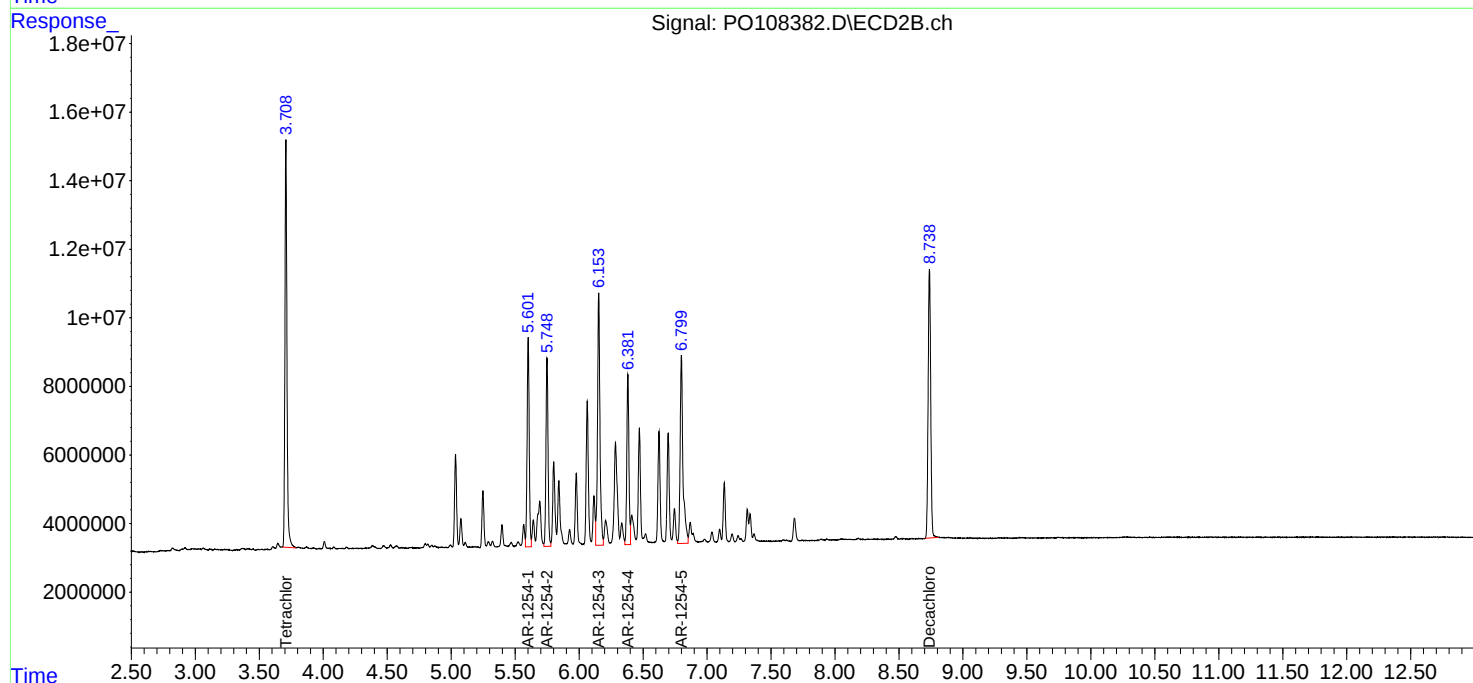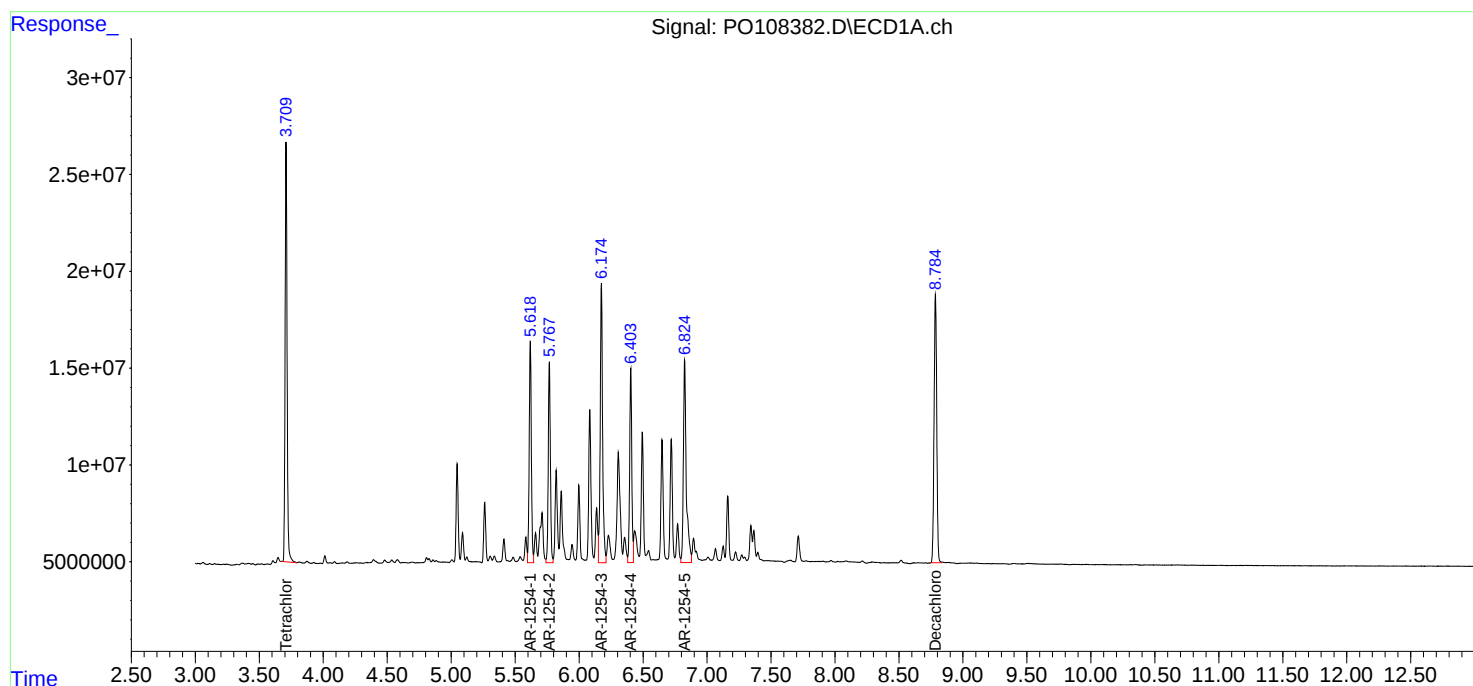

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108383.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 20:44
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/09/2024
 Supervised By :Ankita Jodhani 12/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 04:55:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 04:53:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	44979145	24991936	4.743	4.656
2) SA Decachlor...	8.786	8.738	41446440	21658098	5.283	5.085
Target Compounds						
26) L6 AR-1254-1	5.618	5.602	28602032	15172054	55.860m	56.354
27) L6 AR-1254-2	5.767	5.749	25591845	13582944	56.508m	56.887
28) L6 AR-1254-3	6.174	6.153	38497674	19696275	52.993m	51.772
29) L6 AR-1254-4	6.404	6.380	23289470	11443812	52.422m	51.897
30) L6 AR-1254-5	6.826	6.799	34671057	16988687	54.506	51.951

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108383.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 20:44
Operator : YP/AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/09/2024
Supervised By :Ankita Jodhani 12/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 04:55:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 04:53:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

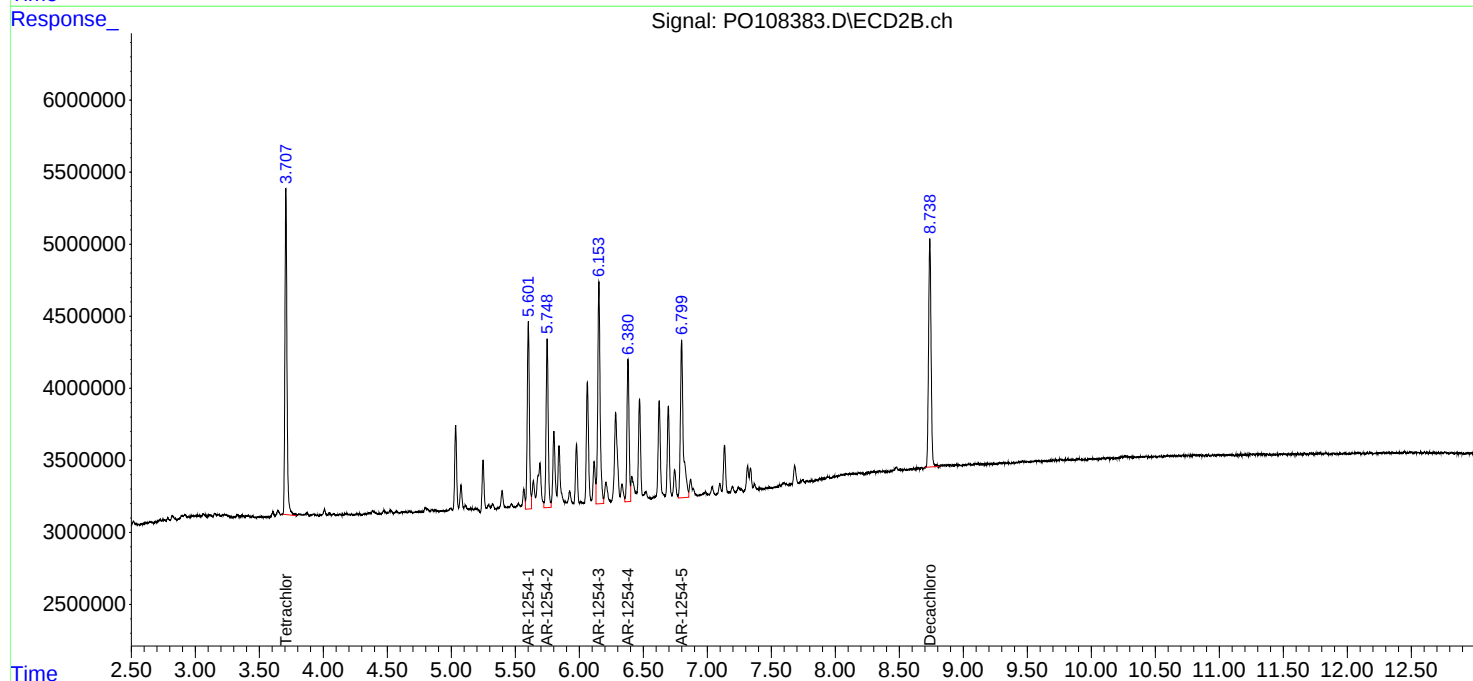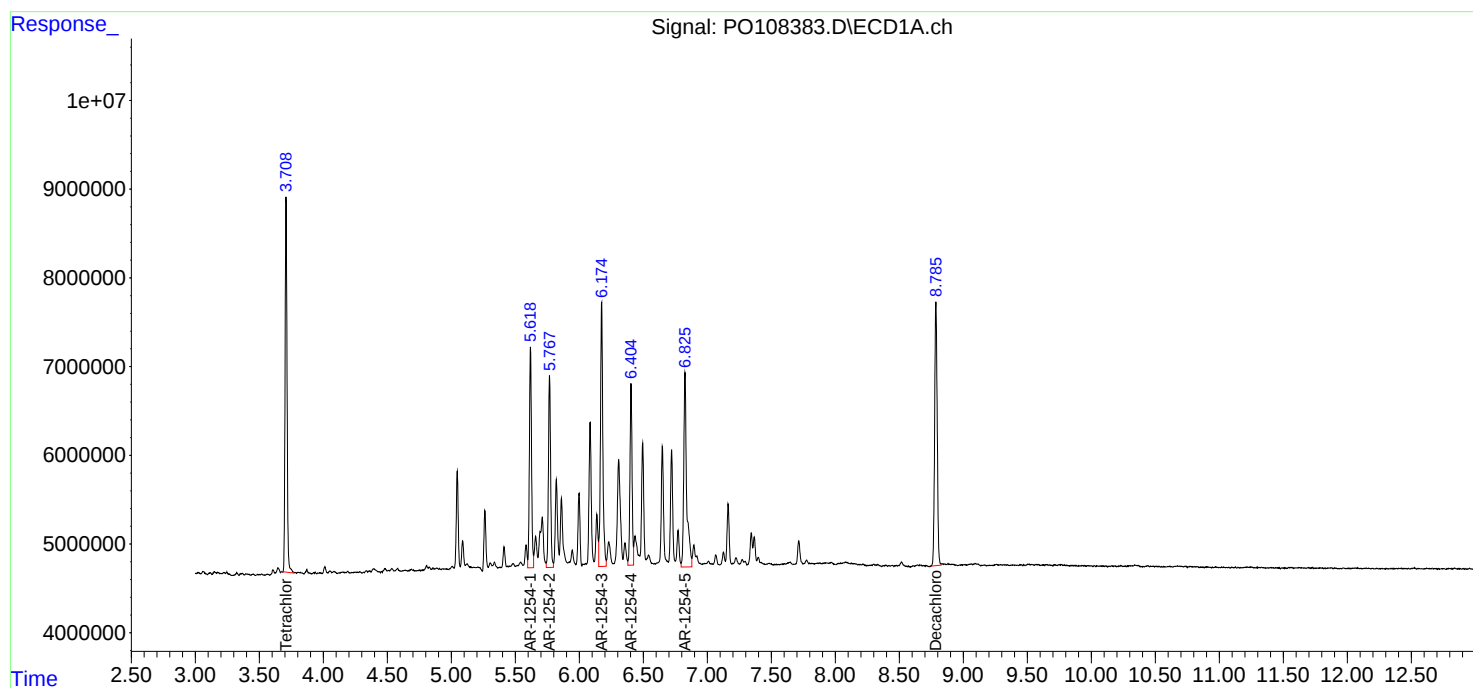

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 21:03
Operator : YP/AJ
Sample : AR1262ICC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 05:34:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:33:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.709	3.708	464.9E6	262.4E6	50.000	50.000
2)	SA Decachlor...	8.786	8.739	386.0E6	210.6E6	50.000	50.000
Target Compounds							
36)	L8 AR-1262-1	6.865	6.840	329.2E6	169.0E6	500.000	500.000
37)	L8 AR-1262-2	7.367	7.338	555.9E6	285.9E6	500.000	500.000
38)	L8 AR-1262-3	7.654	7.624	218.4E6	112.2E6	500.000	500.000
39)	L8 AR-1262-4	7.717	7.686	403.1E6	204.8E6	500.000	500.000
40)	L8 AR-1262-5	8.216	8.180	177.5E6	92414014	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO120624\
Data File : PO108384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 21:03
Operator : YP/AJ
Sample : AR1262ICC500
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 05:34:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:33:35 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

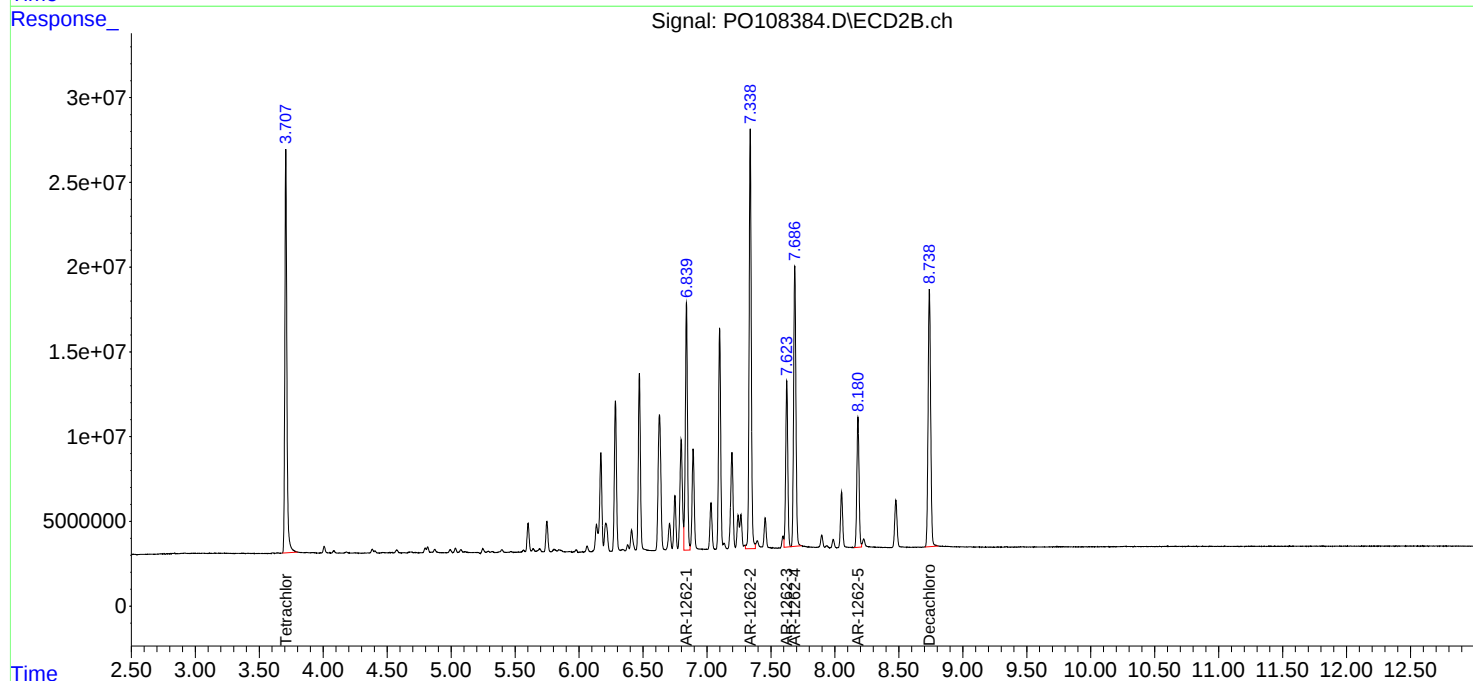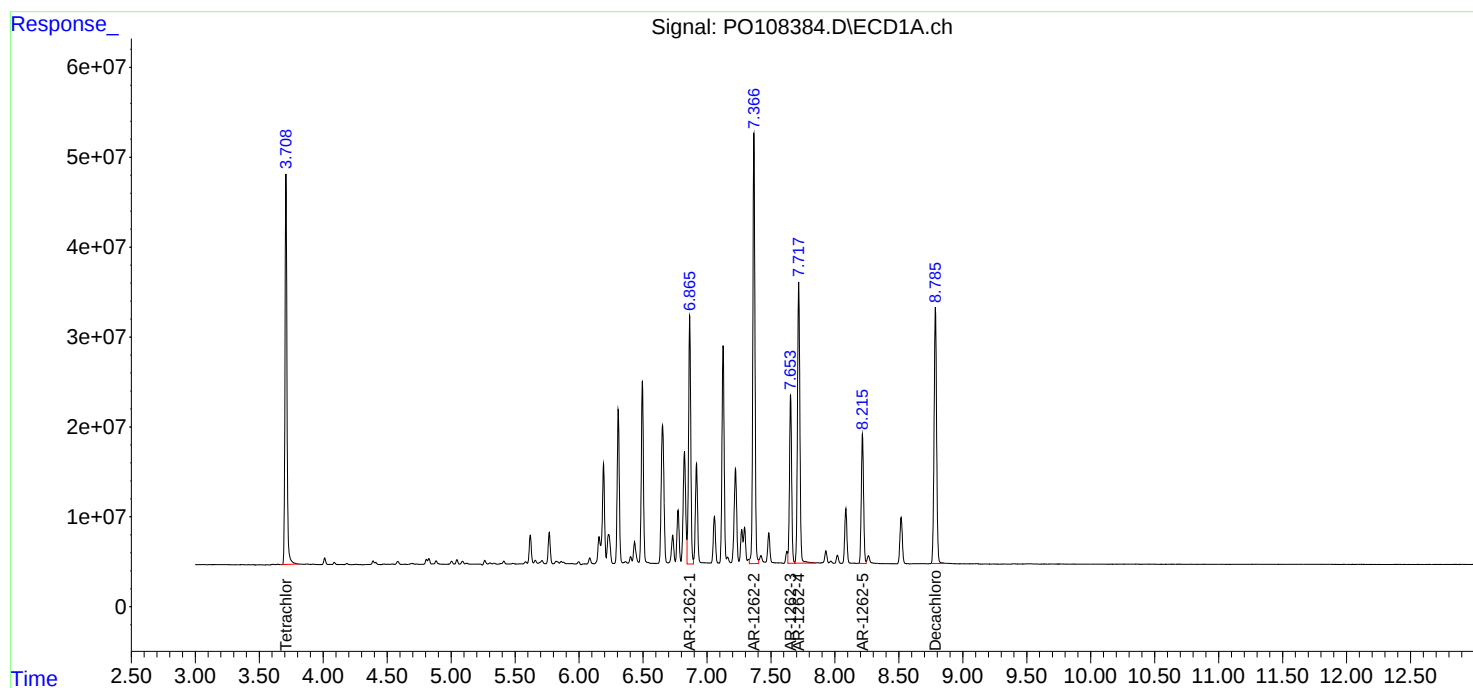

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 21:21
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 05:38:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:37:26 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.708	3.707	944.0E6	535.4E6	100.787	101.787
2) SA Decachlor...	8.785	8.738	1311.6E6	721.6E6	101.008	101.029
Target Compounds						
41) L9 AR-1268-1	7.653	7.623	1246.1E6	656.7E6	1009.703	1016.722
42) L9 AR-1268-2	7.718	7.688	1144.2E6	598.9E6	1028.743	1029.699
43) L9 AR-1268-3	7.929	7.898	941.0E6	514.1E6	1023.522	1023.269
44) L9 AR-1268-4	8.215	8.180	385.9E6	204.5E6	1004.849	1009.851
45) L9 AR-1268-5	8.517	8.477	2890.0E6	1554.5E6	1041.955	1041.780



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 21:21
Operator : YP/AJ
Sample : AR1268ICC1000
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 05:38:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:37:26 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

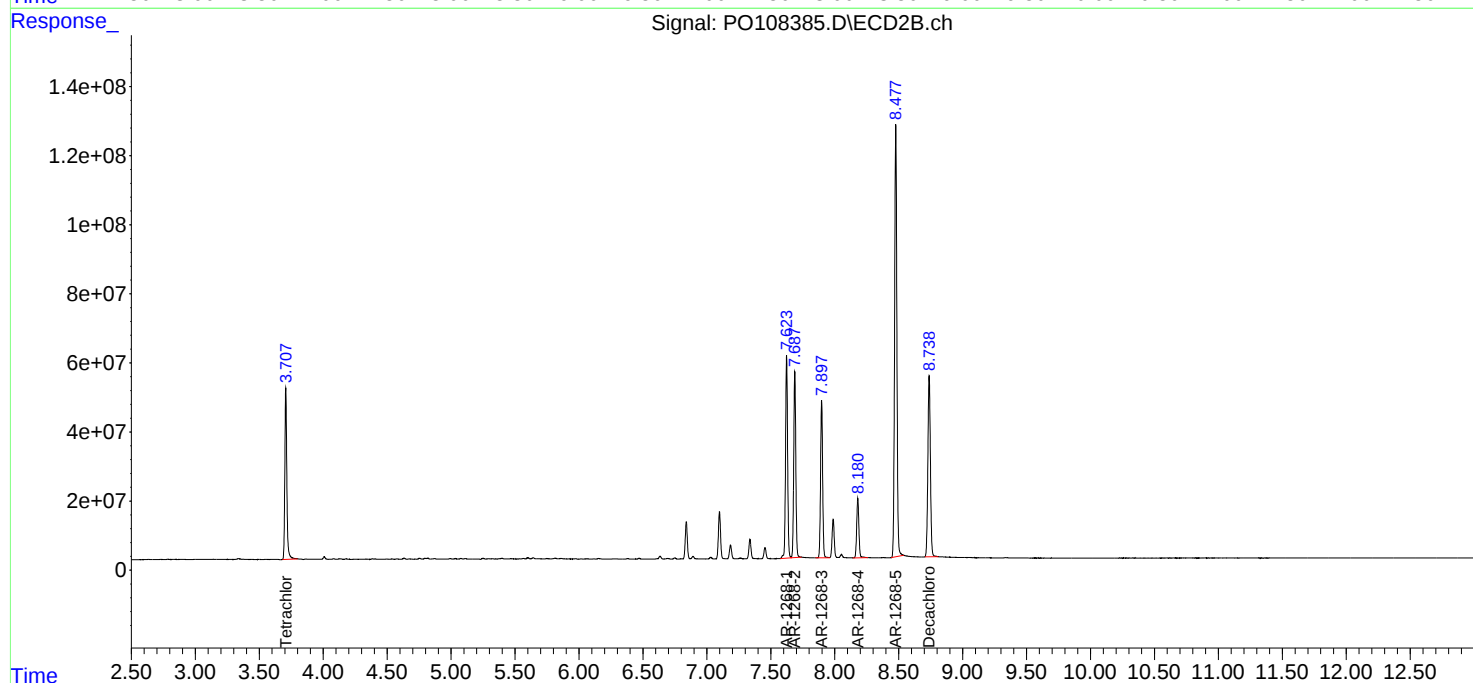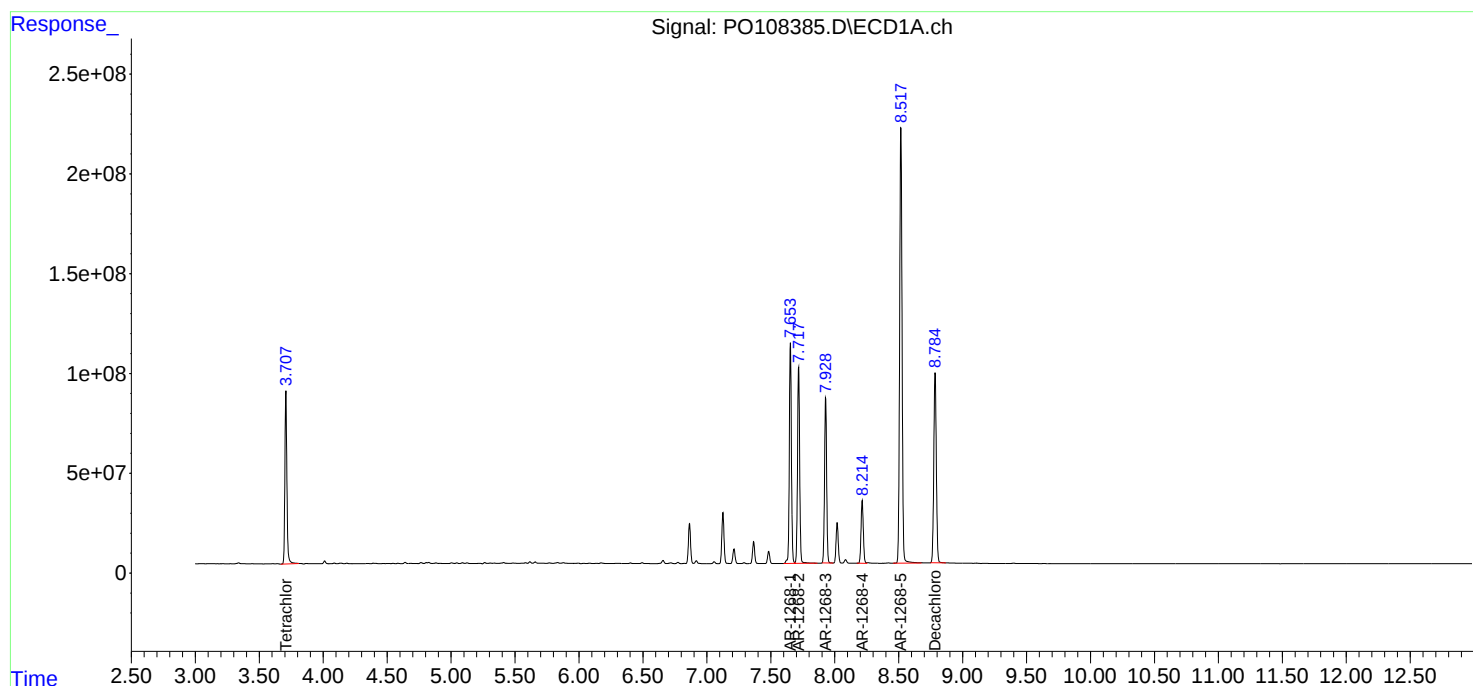

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 21:39
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 05:38:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:37:26 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	669.5E6	379.5E6	71.476	72.154
2) SA Decachlor...	8.785	8.737	951.4E6	522.4E6	73.266	73.130
Target Compounds						
41) L9 AR-1268-1	7.654	7.624	898.9E6	471.8E6	728.384	730.420
42) L9 AR-1268-2	7.719	7.686	816.4E6	430.2E6	734.013	739.705
43) L9 AR-1268-3	7.930	7.897	624.3E6	355.3E6	679.030	707.248
44) L9 AR-1268-4	8.217	8.180	277.7E6	146.2E6	723.017	721.624
45) L9 AR-1268-5	8.519	8.477	2067.2E6	1116.5E6	745.303	748.294



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 21:39
Operator : YP/AJ
Sample : AR1268ICC750
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 05:38:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:37:26 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

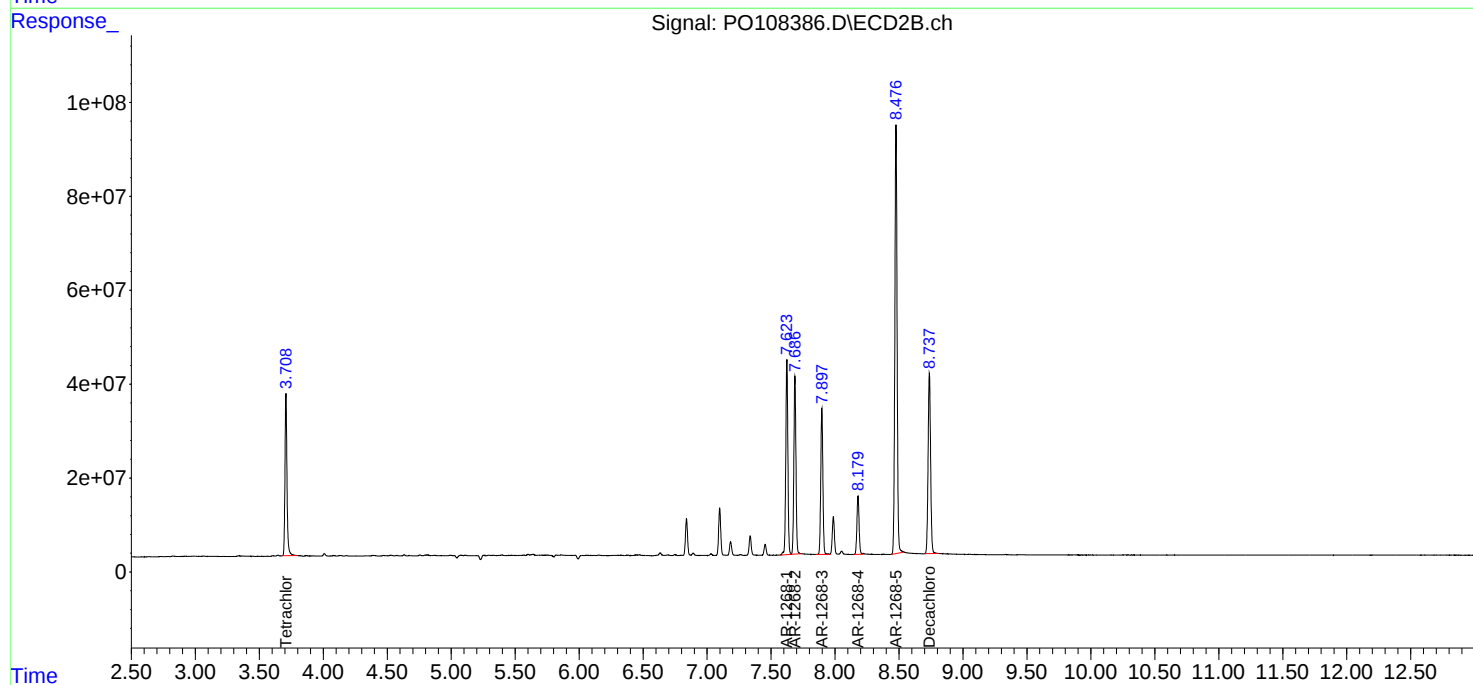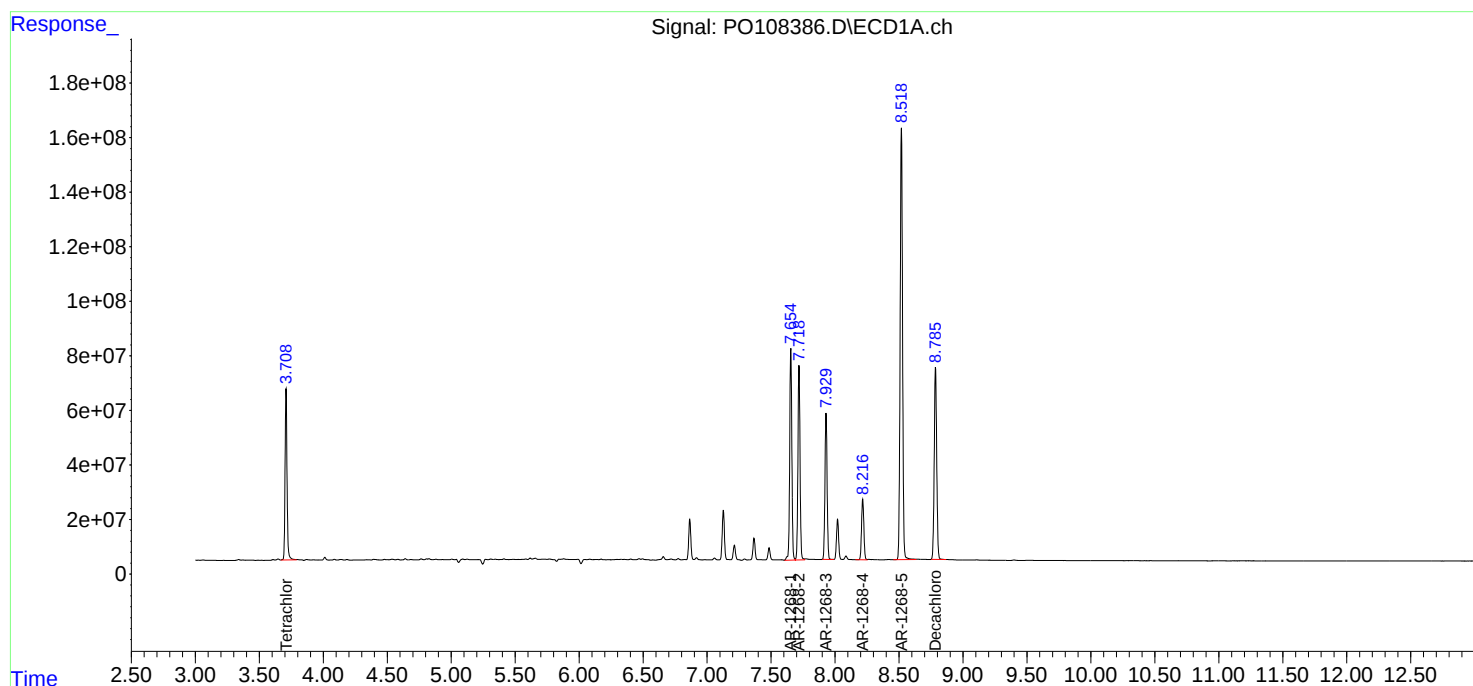

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 21:58
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 05:38:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:37:26 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	468.3E6	263.0E6	50.000	50.000
2) SA Decachlor...	8.786	8.739	649.3E6	357.1E6	50.000	50.000
Target Compounds						
41) L9 AR-1268-1	7.654	7.624	617.1E6	323.0E6	500.000	500.000
42) L9 AR-1268-2	7.718	7.687	556.1E6	290.8E6	500.000	500.000
43) L9 AR-1268-3	7.929	7.898	459.7E6	251.2E6	500.000	500.000
44) L9 AR-1268-4	8.216	8.181	192.0E6	101.3E6	500.000	500.000
45) L9 AR-1268-5	8.519	8.477	1386.8E6	746.1E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 21:58
Operator : YP/AJ
Sample : AR1268ICC500
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 05:38:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:37:26 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

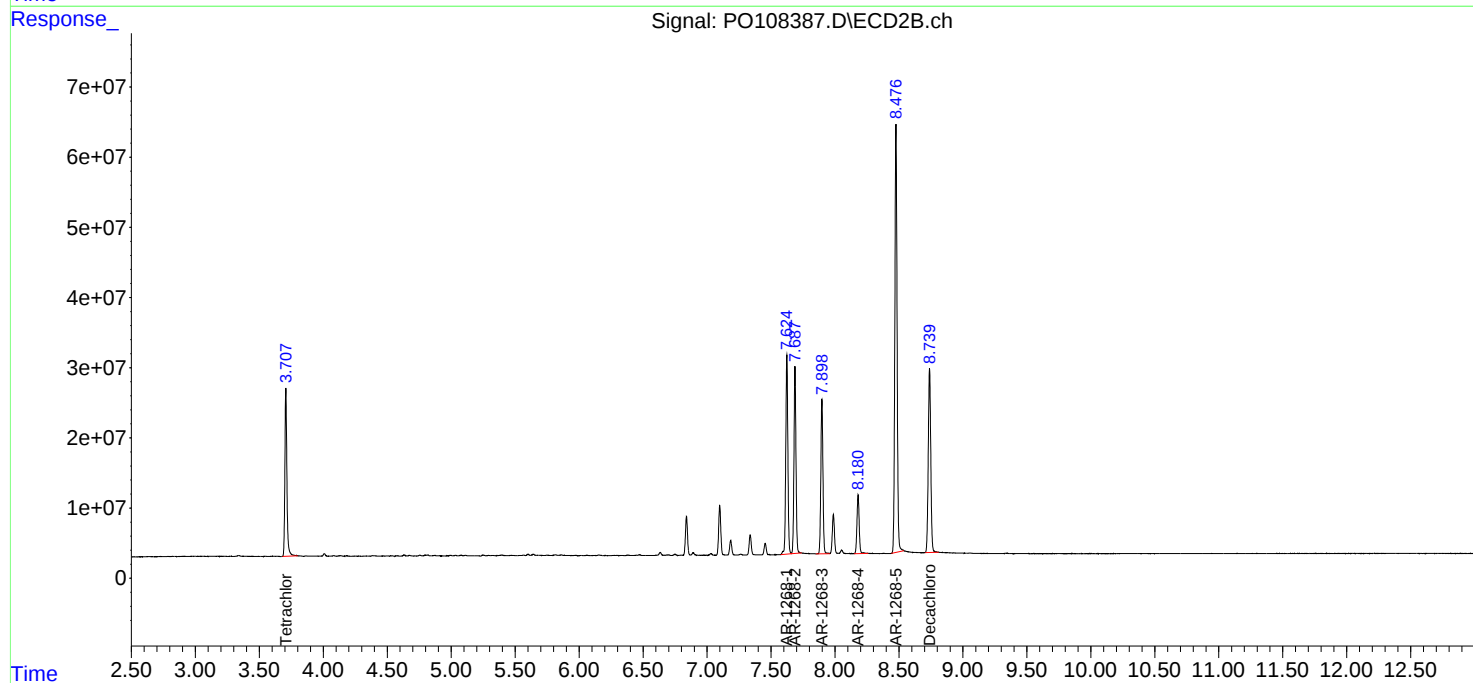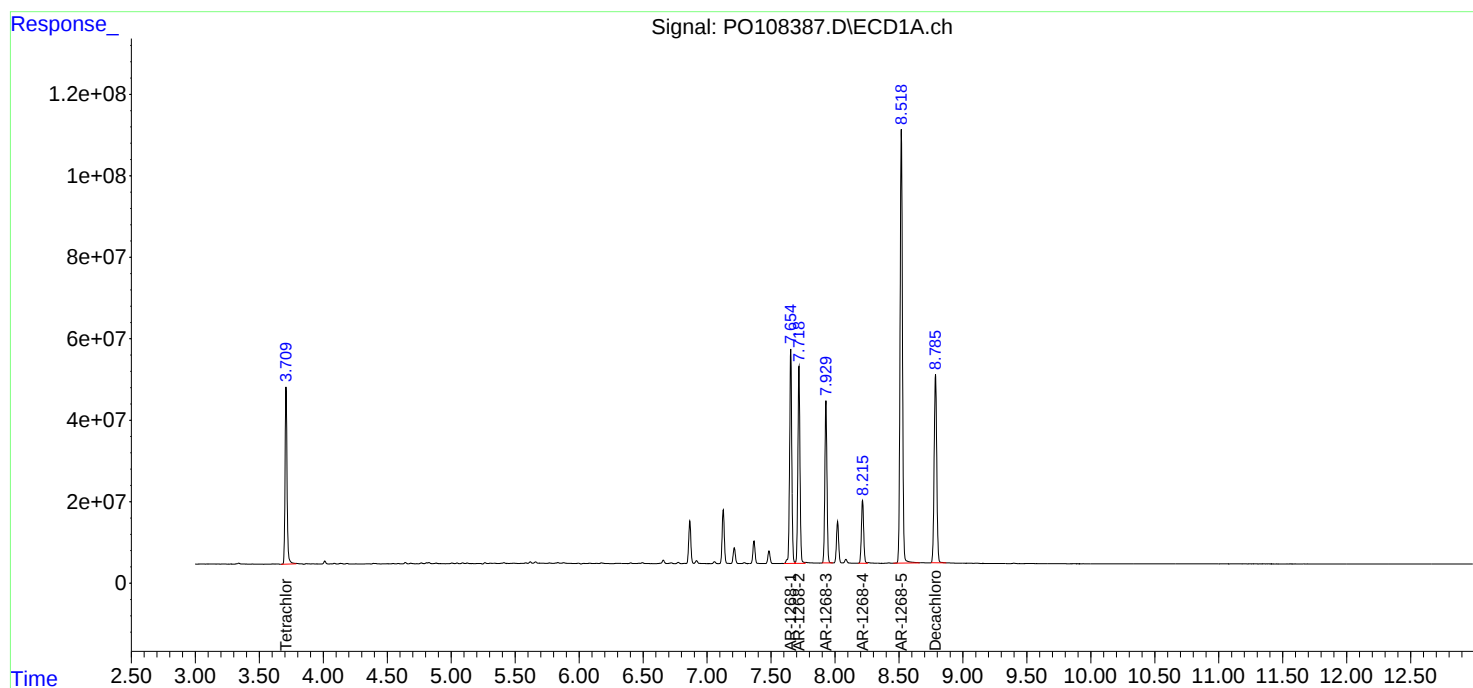

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 22:16
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 05:39:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:37:26 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.707	239.6E6	133.2E6	25.585	25.318
2) SA Decachlor...	8.785	8.739	341.5E6	185.2E6	26.300	25.923
Target Compounds						
41) L9 AR-1268-1	7.655	7.624	319.2E6	165.5E6	258.653	256.236
42) L9 AR-1268-2	7.719	7.688	286.9E6	148.5E6	257.913	255.365
43) L9 AR-1268-3	7.930	7.898	238.3E6	128.8E6	259.252	256.422
44) L9 AR-1268-4	8.216	8.181	101.2E6	53037702	263.394	261.855
45) L9 AR-1268-5	8.519	8.478	703.8E6	375.1E6	253.757	251.417



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 22:16
Operator : YP/AJ
Sample : AR1268ICC250
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 05:39:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:37:26 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

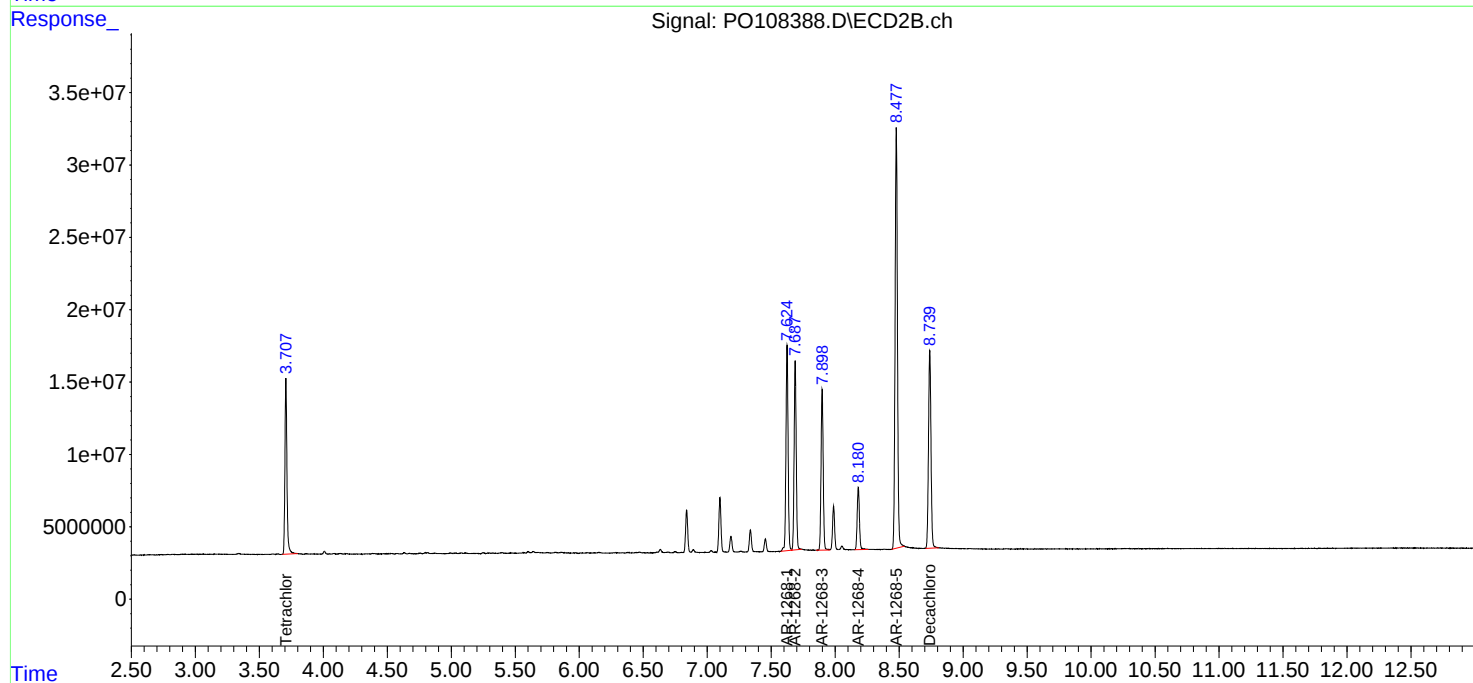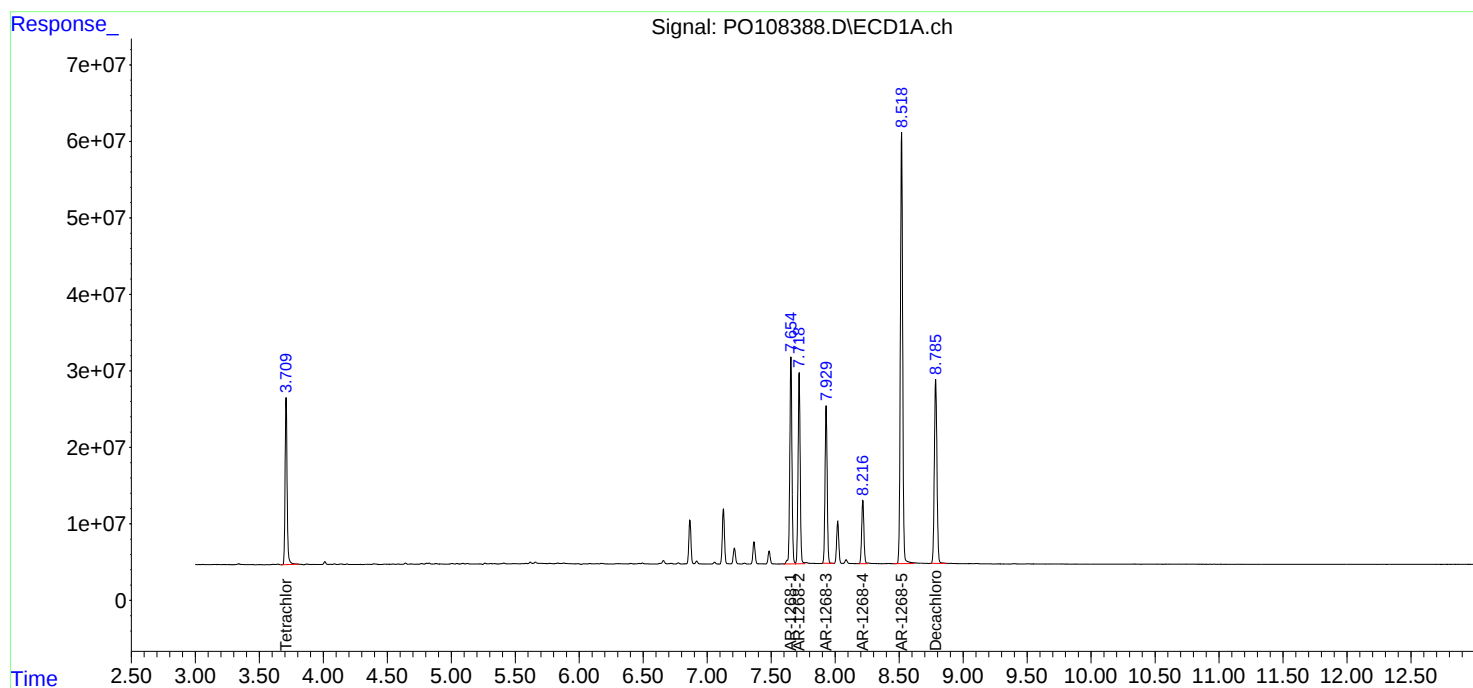

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108389.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 22:34
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 05:39:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:37:26 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.707	43397920	23820328	4.633	4.529
2) SA Decachlor...	8.787	8.739	67751275	35973878	5.218	5.036
Target Compounds						
41) L9 AR-1268-1	7.655	7.623	63224905	31796488	51.231	49.227
42) L9 AR-1268-2	7.719	7.687	55796192	27976696	50.166	48.104
43) L9 AR-1268-3	7.930	7.898	44249311	24435743	48.132	48.636
44) L9 AR-1268-4	8.217	8.180	19477210	10053726	50.710	49.637
45) L9 AR-1268-5	8.519	8.477	131.2E6	69412663	47.313	46.520



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108389.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 22:34
Operator : YP/AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 05:39:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:37:26 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

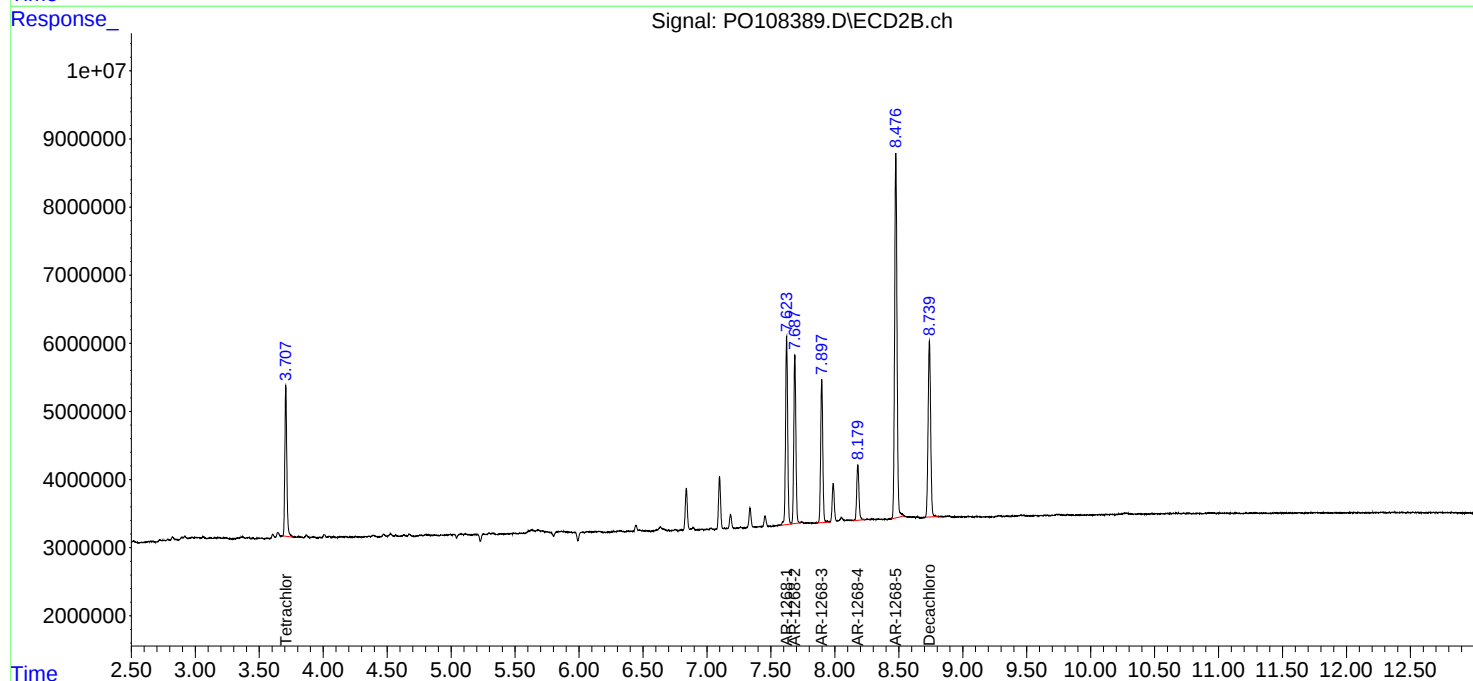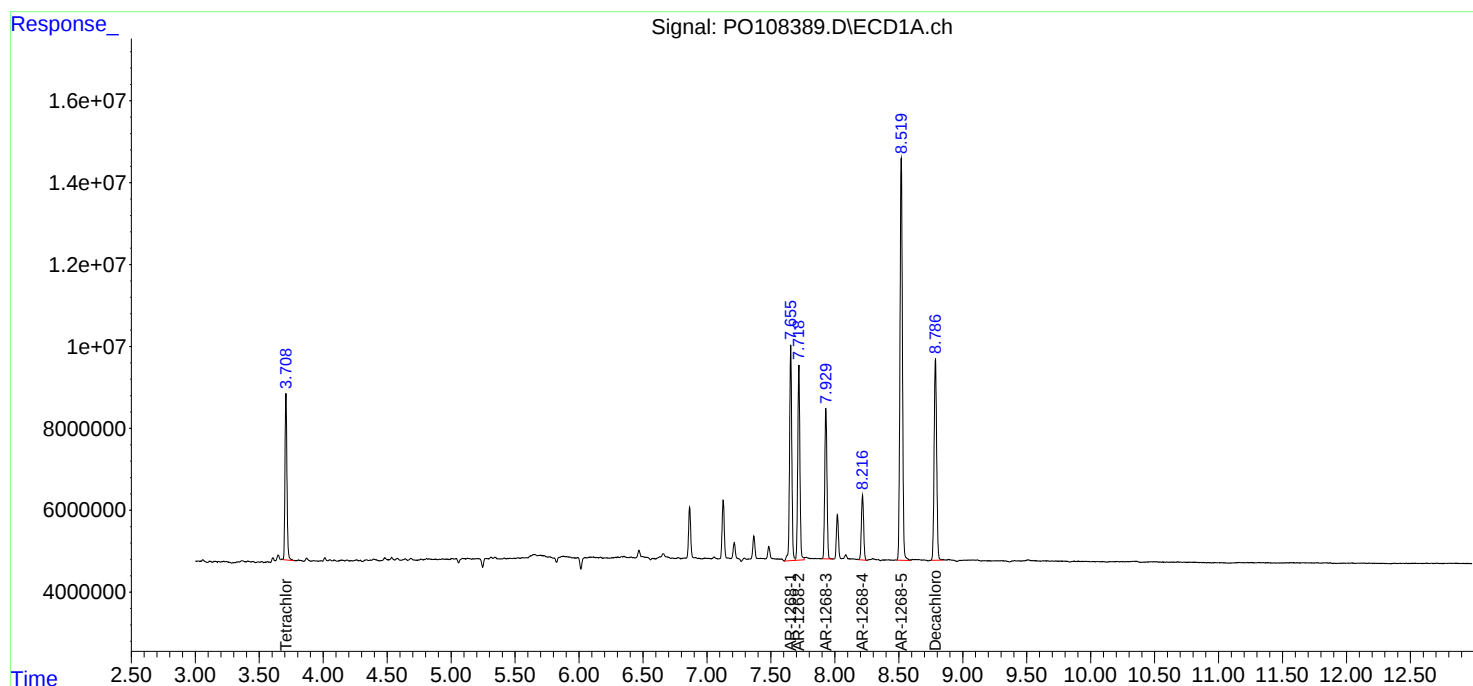

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 22:53
 Operator : YP/AJ
 Sample : PO120624ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO120624

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 02:30:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 02:28:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.708	3.707	433.5E6	256.1E6	49.827	50.509
2) SA Decachlor...	8.786	8.738	367.7E6	200.0E6	50.336	51.625
Target Compounds						
3) L1 AR-1016-1	4.807	4.796	152.4E6	80878936	494.032	503.999
4) L1 AR-1016-2	4.827	4.816	207.8E6	112.0E6	497.935	504.290
5) L1 AR-1016-3	4.883	4.992	146.3E6	63403102	499.921	503.865
6) L1 AR-1016-4	5.004	5.033	114.7E6	53092959	496.317	506.584
7) L1 AR-1016-5	5.262	5.248	123.4E6	67028787	490.414	495.735
31) L7 AR-1260-1	6.306	6.283	226.4E6	118.0E6	495.314	504.236
32) L7 AR-1260-2	6.495	6.470	272.5E6	141.0E6	490.407	502.514
33) L7 AR-1260-3	6.865	6.625	230.1E6	131.5E6	496.219	498.757
34) L7 AR-1260-4	7.126	7.098	210.3E6	109.4E6	494.415	514.366
35) L7 AR-1260-5	7.366	7.337	486.3E6	250.1E6	500.346	516.847



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 22:53
Operator : YP/AJ
Sample : PO120624ICV500
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO120624

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 02:30:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 02:28:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

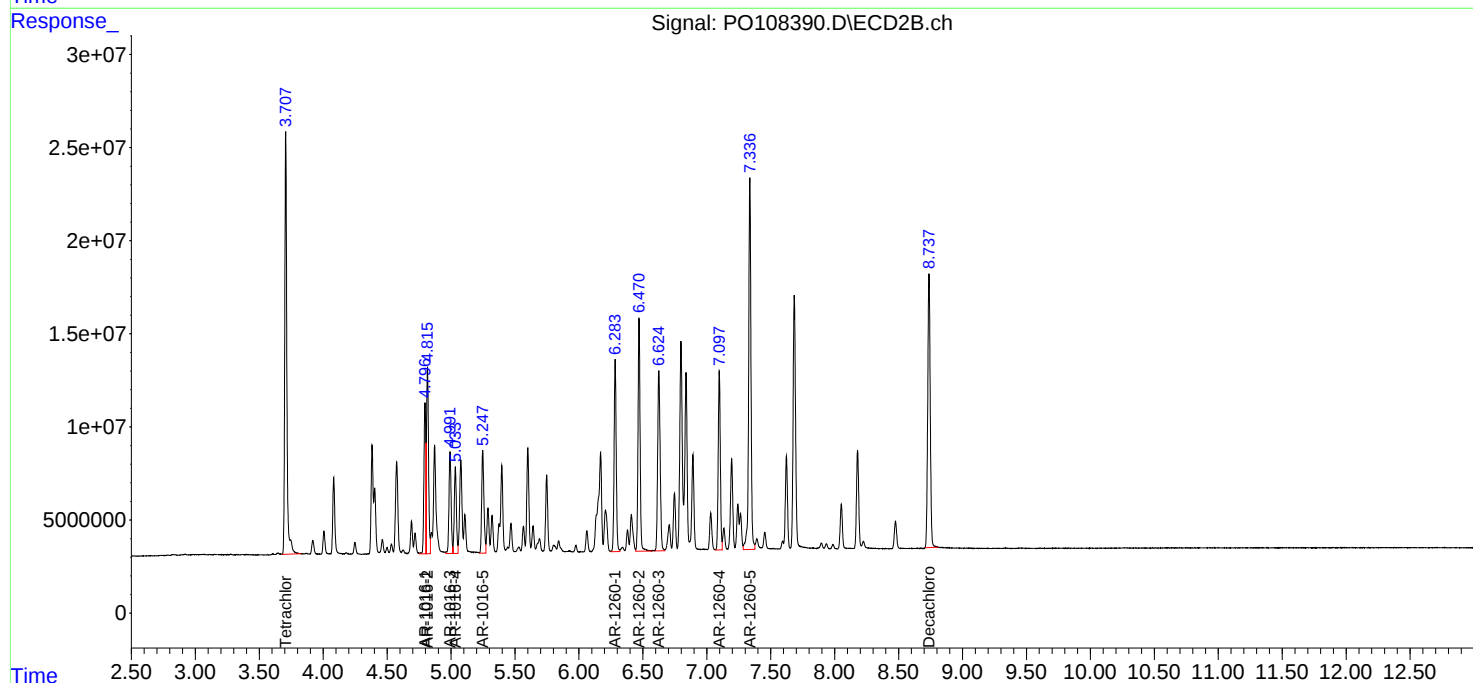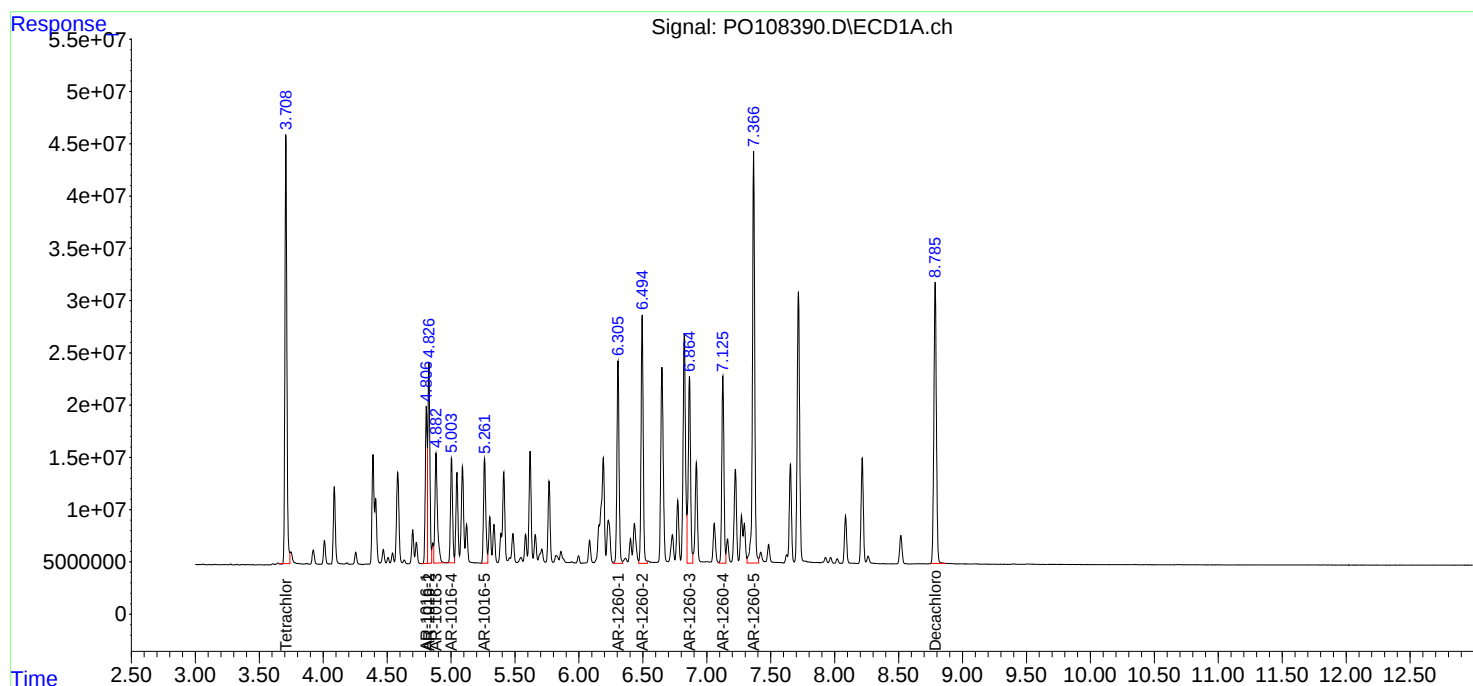

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 23:11
 Operator : YP/AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO120624AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 03:47:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 03:45:26 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.707	473.2E6	274.6E6	54.132	54.770
2) SA Decachlor...	8.787	8.739	400.3E6	218.3E6	54.256	55.188
Target Compounds						
16) L4 AR-1242-1	4.808	4.797	136.2E6	72198817	529.129	531.781
17) L4 AR-1242-2	4.828	4.817	185.7E6	100.0E6	538.138	539.407
18) L4 AR-1242-3	4.884	4.993	130.0E6	56871808	538.888	539.671
19) L4 AR-1242-4	5.005	5.077	102.2E6	57541113	535.754	536.121
20) L4 AR-1242-5	5.660	5.600	109.7E6	67632185	528.454	535.064



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 23:11
Operator : YP/AJ
Sample : AR1242ICV500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO120624AR1242

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 03:47:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 03:45:26 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

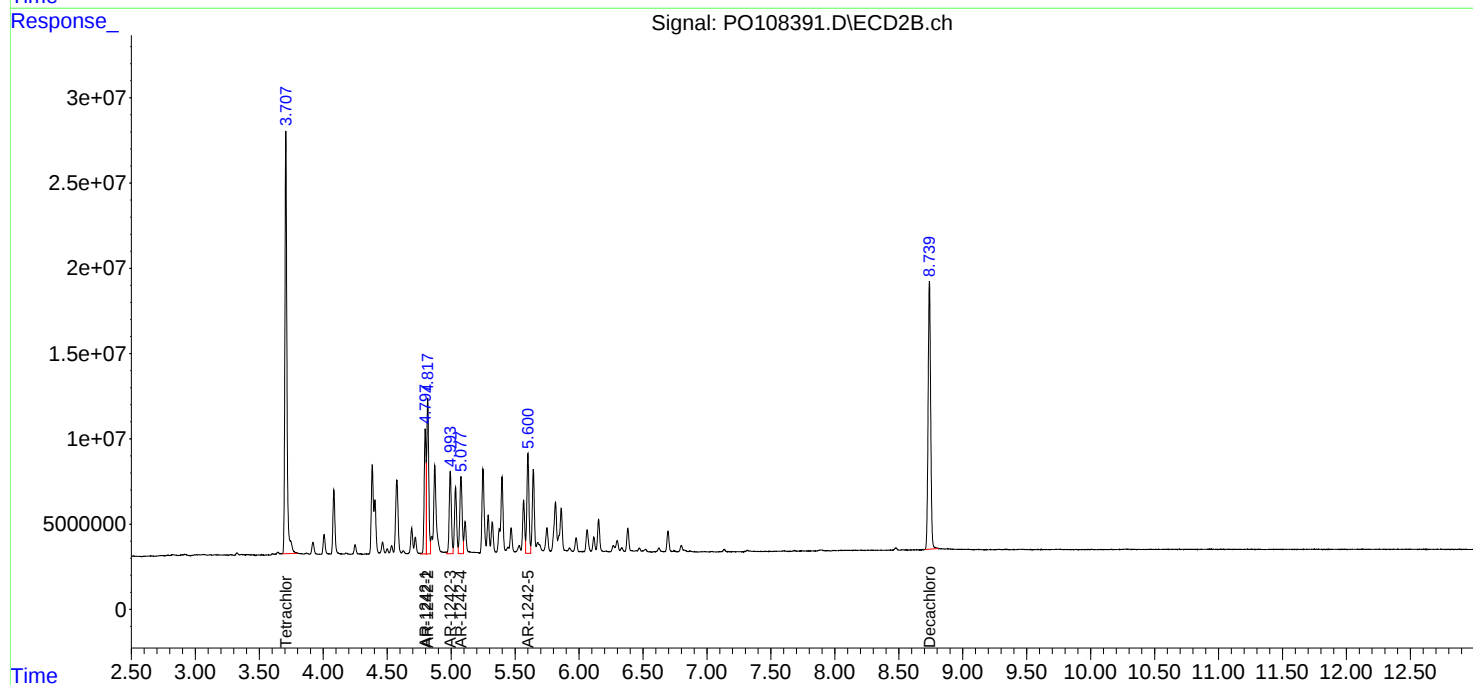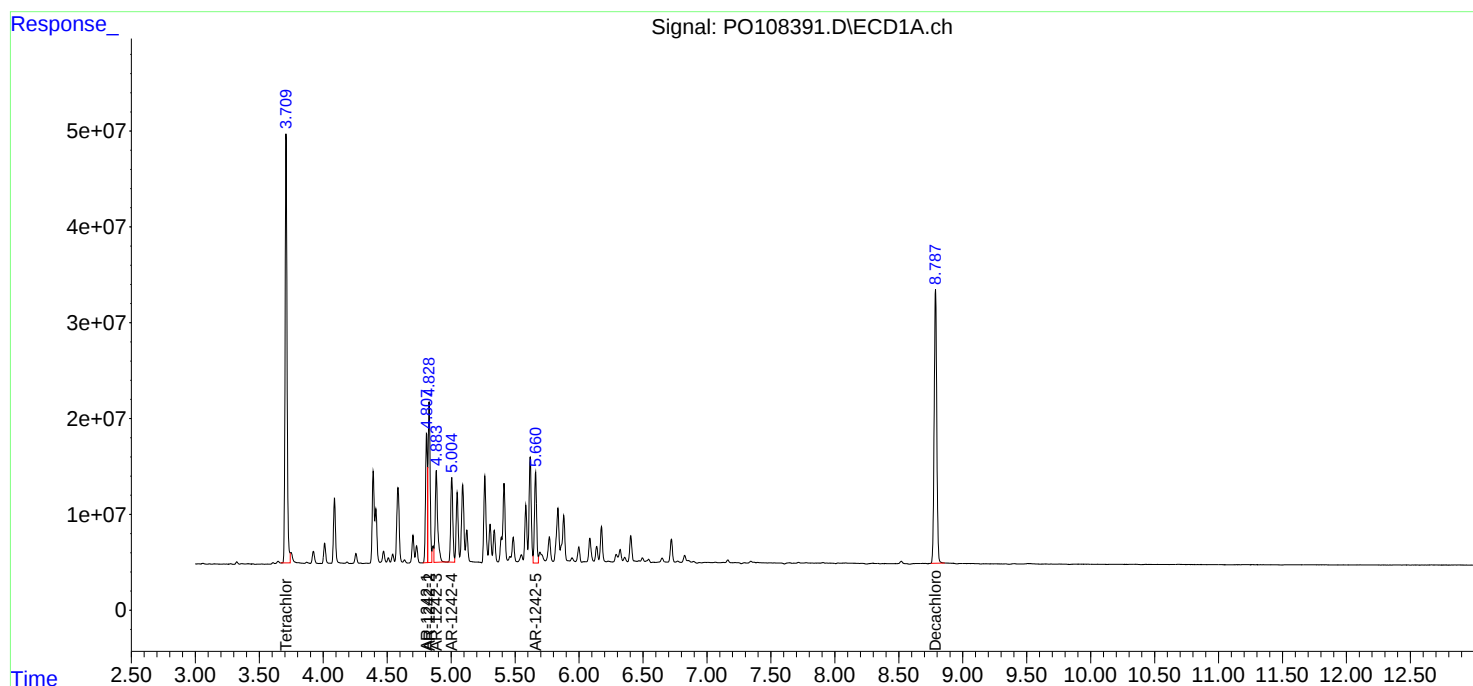

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 23:29
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO120624AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 05:15:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:15:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.710	3.708	494.8E6	277.9E6	54.702	55.064
2) SA Decachlor...	8.787	8.739	408.5E6	223.3E6	52.675	53.999
Target Compounds						
21) L5 AR-1248-1	4.808	4.797	106.4E6	56795368	531.289	540.296
22) L5 AR-1248-2	5.048	5.034	146.8E6	80058605	529.599	536.128
23) L5 AR-1248-3	5.264	5.077	180.4E6	84835876	528.911	535.541
24) L5 AR-1248-4	5.619	5.248	255.1E6	98531455	535.318	539.749
25) L5 AR-1248-5	5.661	5.643	180.4E6	94191450	532.664	536.387



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 23:29
Operator : YP/AJ
Sample : AR1248ICV500
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO120624AR1248

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 05:15:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:15:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

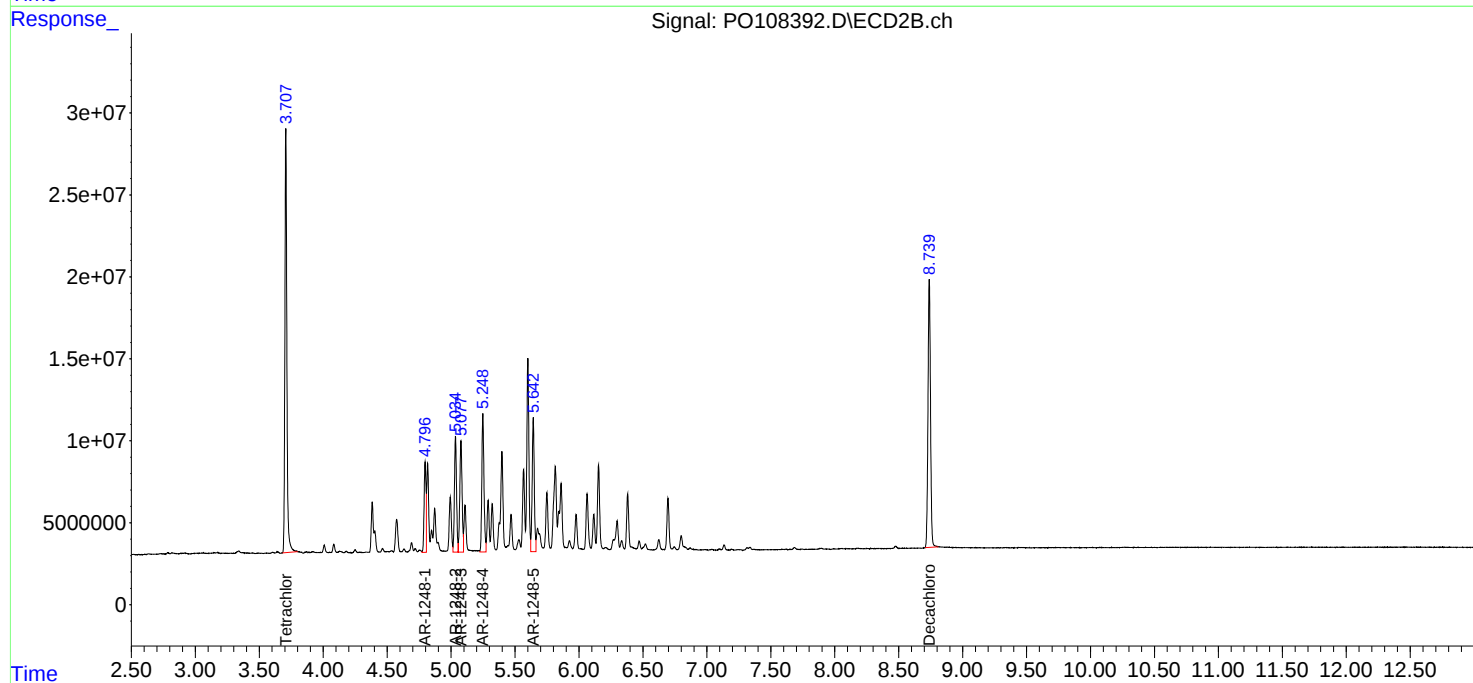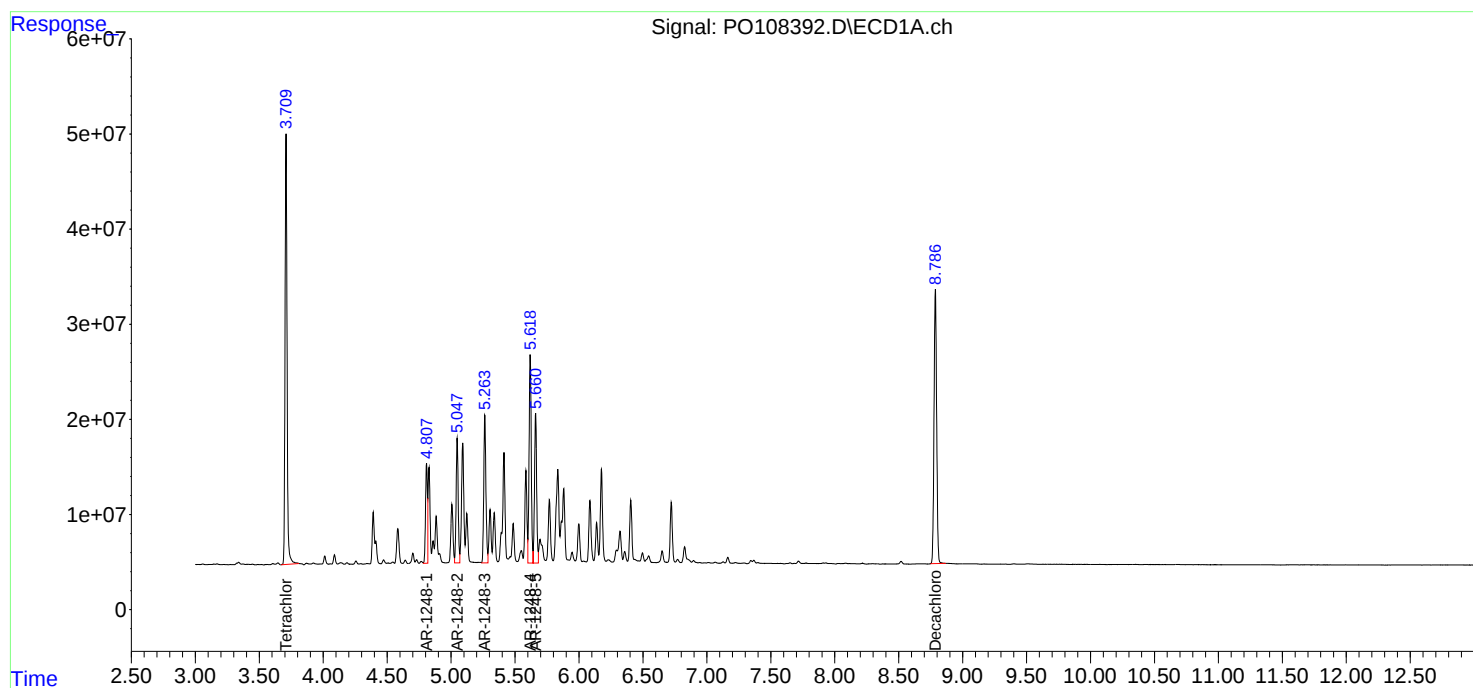

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108393.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 23:48
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO120624AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 05:09:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:08:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.707	496.6E6	280.8E6	54.077	54.172
2) SA Decachlor...	8.788	8.740	411.8E6	224.2E6	53.122	53.431
Target Compounds						
26) L6 AR-1254-1	5.620	5.601	273.4E6	144.3E6	532.286	532.859
27) L6 AR-1254-2	5.768	5.749	242.1E6	127.8E6	531.623	532.309
28) L6 AR-1254-3	6.175	6.153	387.5E6	203.0E6	538.152	540.509
29) L6 AR-1254-4	6.405	6.381	237.3E6	117.8E6	540.738	541.351
30) L6 AR-1254-5	6.827	6.800	339.7E6	174.8E6	534.857	541.443



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108393.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 23:48
Operator : YP/AJ
Sample : AR1254ICV500
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO120624AR1254

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 05:09:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:08:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

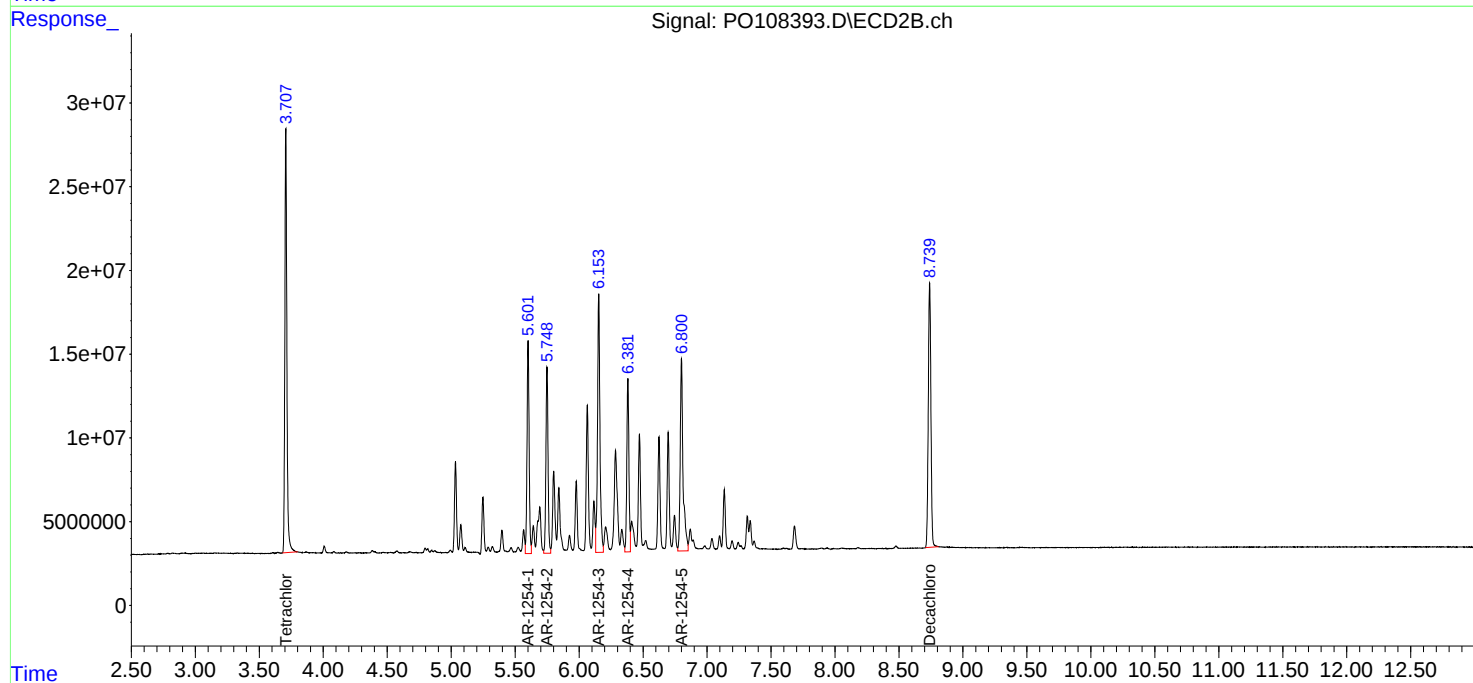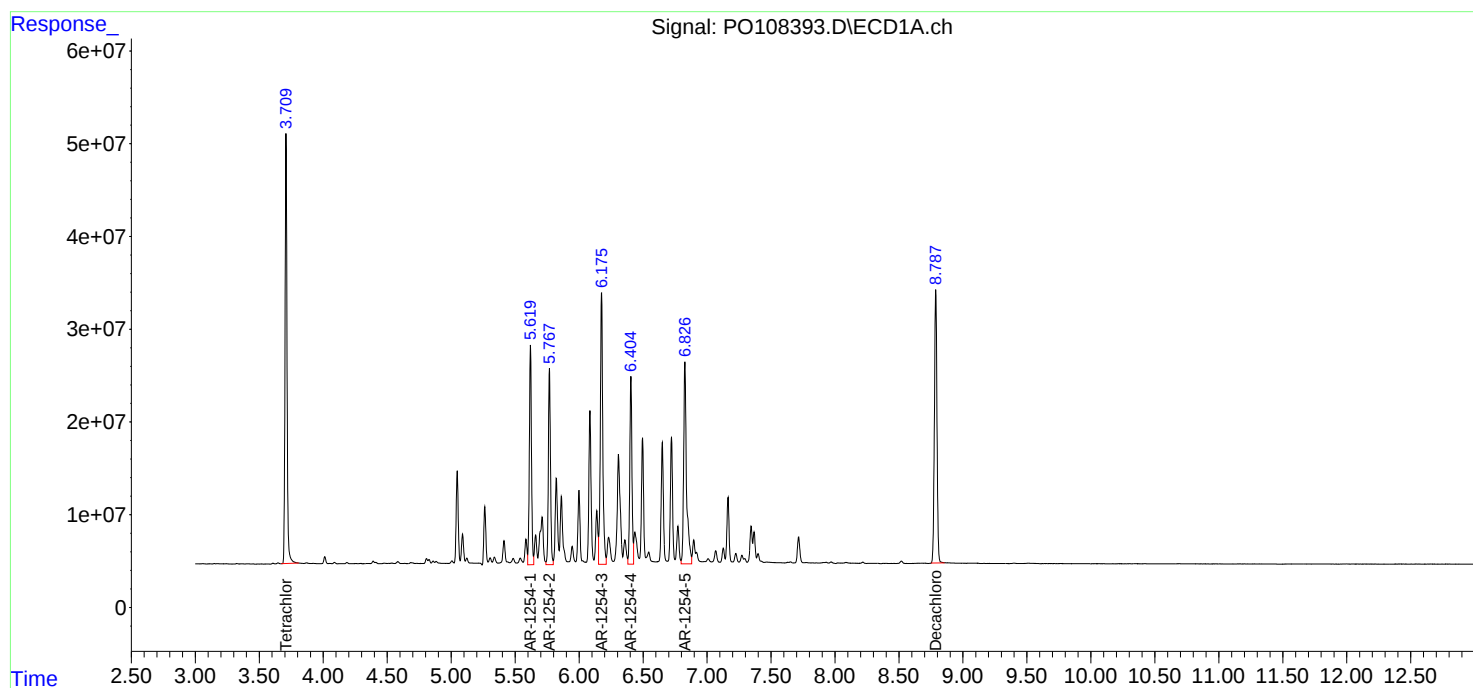

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2024 00:06
 Operator : YP/AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO120624AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 05:47:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:46:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.709	3.708	445.9E6	250.8E6	48.476	48.664
2) SA Decachlor...	8.786	8.739	629.8E6	343.6E6	47.715	47.815
Target Compounds						
41) L9 AR-1268-1	7.655	7.624	596.7E6	310.0E6	479.624	479.987
42) L9 AR-1268-2	7.719	7.688	536.9E6	279.8E6	478.639	481.104
43) L9 AR-1268-3	7.931	7.898	429.9E6	238.3E6	474.352	477.608
44) L9 AR-1268-4	8.217	8.181	185.6E6	97713362	479.679	481.254
45) L9 AR-1268-5	8.519	8.477	1339.4E6	717.3E6	483.179	483.115



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2024 00:06
Operator : YP/AJ
Sample : AR1268ICV500
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO120624AR1268

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 05:47:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:46:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

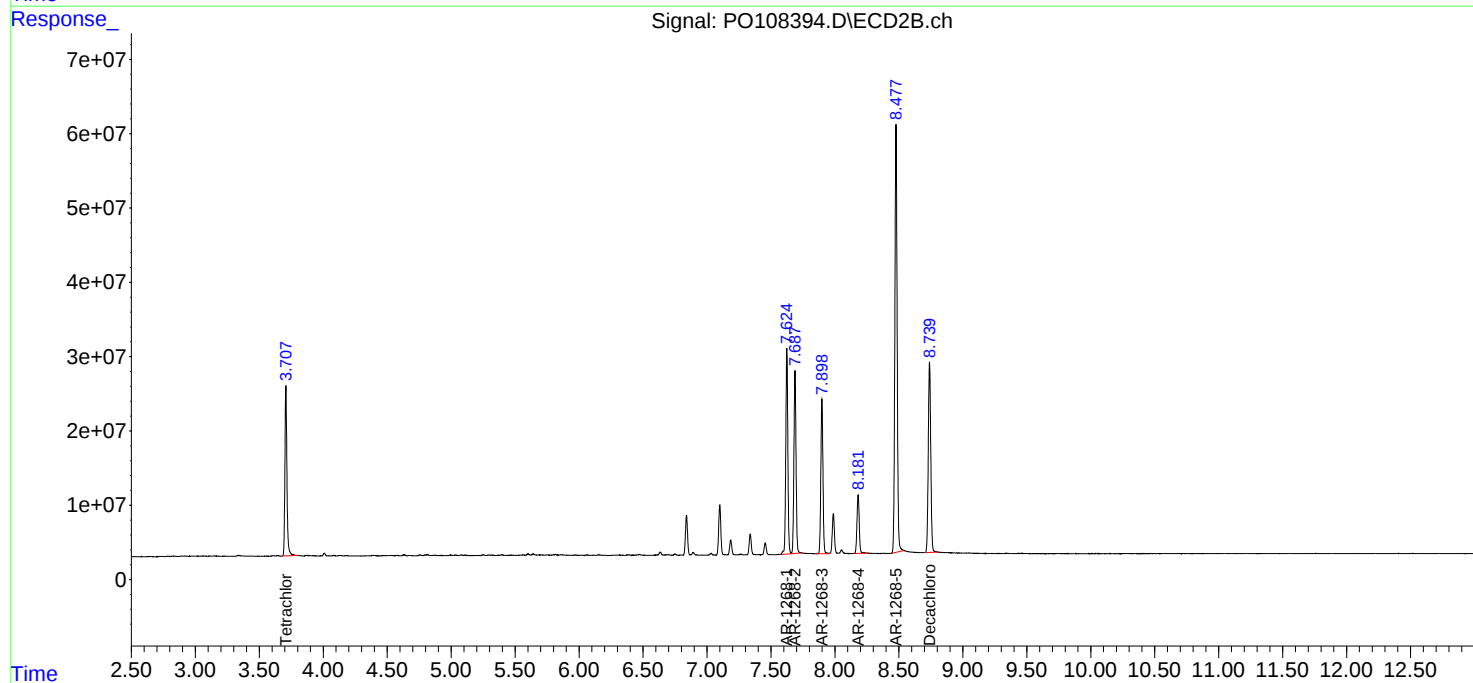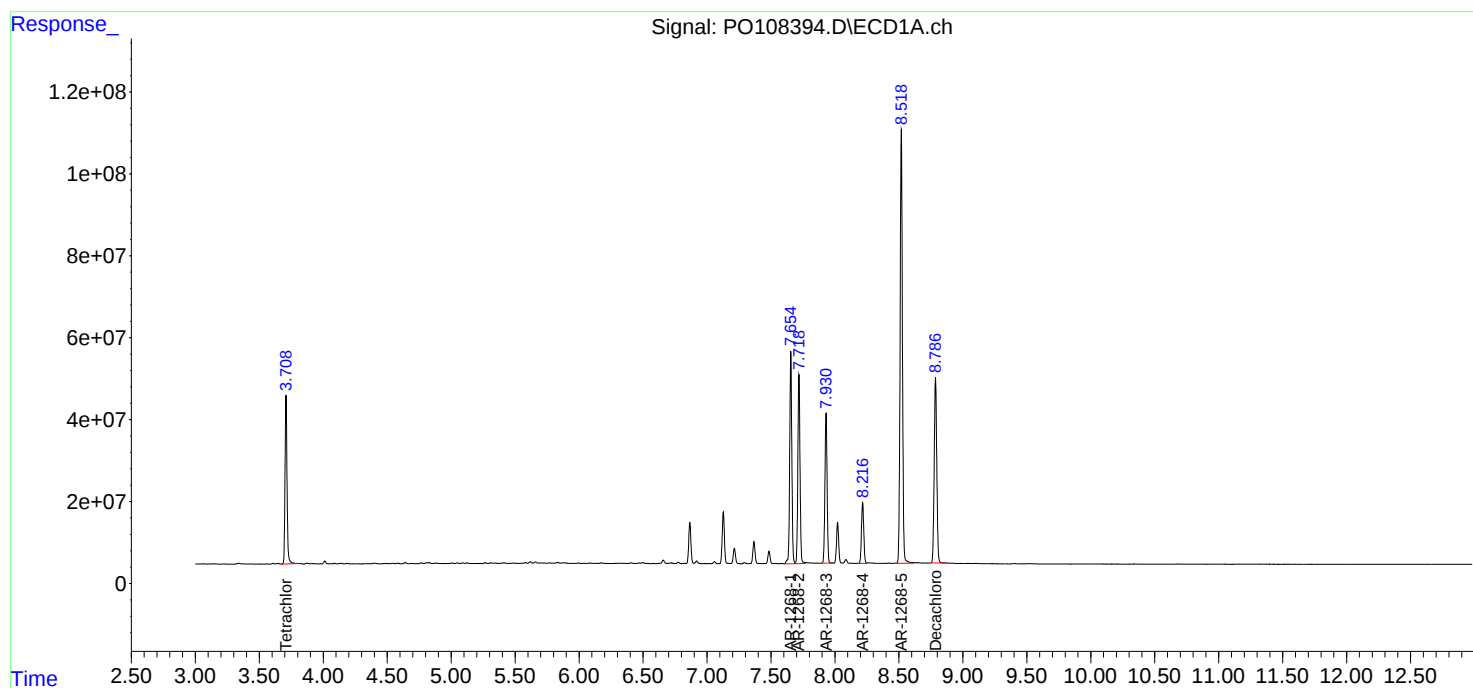



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

Continuing Calib Date: 12/26/2024 Initial Calibration Date(s): 12/06/2024 12/06/2024

Continuing Calib Time: 09:31 Initial Calibration Time(s): 14:19 22:34

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Aroclor-1016-1	(1)	4.80	4.81	4.71	4.91	0.01
Aroclor-1016-2	(2)	4.82	4.83	4.73	4.93	0.01
Aroclor-1016-3	(3)	4.88	4.89	4.79	4.99	0.01
Aroclor-1016-4	(4)	5.00	5.01	4.91	5.11	0.01
Aroclor-1016-5	(5)	5.25	5.27	5.17	5.37	0.02
Aroclor-1260-1	(1)	6.30	6.31	6.21	6.41	0.01
Aroclor-1260-2	(2)	6.48	6.50	6.40	6.60	0.02
Aroclor-1260-3	(3)	6.85	6.87	6.77	6.97	0.02
Aroclor-1260-4	(4)	7.11	7.13	7.03	7.23	0.02
Aroclor-1260-5	(5)	7.36	7.37	7.27	7.47	0.01
Tetrachloro-m-xylene		3.70	3.71	3.61	3.81	0.01
Decachlorobiphenyl		8.77	8.79	8.69	8.89	0.02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

Continuing Calib Date: 12/26/2024 Initial Calibration Date(s): 12/06/2024 12/06/2024

Continuing Calib Time: 09:31 Initial Calibration Time(s): 14:19 22:34

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Aroclor-1016-1	(1)	4.79	4.80	4.70	4.90	0.02
Aroclor-1016-2	(2)	4.81	4.82	4.72	4.92	0.02
Aroclor-1016-3	(3)	4.98	4.99	4.89	5.09	0.01
Aroclor-1016-4	(4)	5.02	5.04	4.94	5.14	0.02
Aroclor-1016-5	(5)	5.24	5.25	5.15	5.35	0.01
Aroclor-1260-1	(1)	6.27	6.29	6.19	6.39	0.02
Aroclor-1260-2	(2)	6.46	6.47	6.37	6.57	0.01
Aroclor-1260-3	(3)	6.61	6.63	6.53	6.73	0.02
Aroclor-1260-4	(4)	7.08	7.10	7.00	7.20	0.02
Aroclor-1260-5	(5)	7.32	7.34	7.24	7.44	0.02
Tetrachloro-m-xylene		3.70	3.71	3.61	3.81	0.01
Decachlorobiphenyl		8.72	8.74	8.64	8.84	0.02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 12/06/2024 12/06/2024

Client Sample No.: CCAL01 Date Analyzed: 12/26/2024

Lab Sample No.: AR1660CCC500 Data File : PO108758.D Time Analyzed: 09:31

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.798	4.709	4.909	492.260	500.000	-1.5
Aroclor-1016-2	4.819	4.729	4.929	555.520	500.000	11.1
Aroclor-1016-3	4.875	4.785	4.985	566.500	500.000	13.3
Aroclor-1016-4	4.996	4.907	5.107	554.660	500.000	10.9
Aroclor-1016-5	5.254	5.165	5.365	545.160	500.000	9.0
Aroclor-1260-1	6.296	6.210	6.410	532.910	500.000	6.6
Aroclor-1260-2	6.484	6.398	6.598	520.070	500.000	4.0
Aroclor-1260-3	6.854	6.769	6.969	508.280	500.000	1.7
Aroclor-1260-4	7.114	7.029	7.229	500.340	500.000	0.1
Aroclor-1260-5	7.355	7.270	7.470	505.130	500.000	1.0
Decachlorobiphenyl	8.768	8.691	8.891	48.400	50.000	-3.2
Tetrachloro-m-xylene	3.703	3.610	3.810	58.440	50.000	16.9



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 12/06/2024 12/06/2024

Client Sample No.: CCAL01 Date Analyzed: 12/26/2024

Lab Sample No.: AR1660CCC500 Data File : PO108758.D Time Analyzed: 09:31

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.785	4.698	4.898	523.530	500.000	4.7
Aroclor-1016-2	4.805	4.718	4.918	530.700	500.000	6.1
Aroclor-1016-3	4.981	4.894	5.094	521.170	500.000	4.2
Aroclor-1016-4	5.022	4.935	5.135	517.040	500.000	3.4
Aroclor-1016-5	5.236	5.150	5.350	538.660	500.000	7.7
Aroclor-1260-1	6.269	6.186	6.386	539.930	500.000	8.0
Aroclor-1260-2	6.456	6.373	6.573	533.550	500.000	6.7
Aroclor-1260-3	6.610	6.527	6.727	525.430	500.000	5.1
Aroclor-1260-4	7.081	7.000	7.200	541.640	500.000	8.3
Aroclor-1260-5	7.321	7.239	7.439	544.970	500.000	9.0
Decachlorobiphenyl	8.717	8.641	8.841	51.720	50.000	3.4
Tetrachloro-m-xylene	3.700	3.608	3.808	54.500	50.000	9.0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
 Data File : PO108758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 09:31
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/27/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 13:17:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.703	3.700	508.4E6	276.3E6	58.439	54.502
2) SA Decachlor...	8.768	8.717	353.5E6	200.4E6	48.402	51.717
Target Compounds						
3) L1 AR-1016-1	4.798	4.785	151.8E6	84012877	492.259m	523.529m
4) L1 AR-1016-2	4.819	4.805	231.9E6	117.9E6	555.516	530.698
5) L1 AR-1016-3	4.875	4.981	165.8E6	65581081	566.504	521.173
6) L1 AR-1016-4	4.996	5.022	128.2E6	54189024	554.665	517.042
7) L1 AR-1016-5	5.254	5.236	137.2E6	72832421	545.163	538.657
31) L7 AR-1260-1	6.296	6.269	243.6E6	126.4E6	532.907	539.927
32) L7 AR-1260-2	6.484	6.456	289.0E6	149.7E6	520.068	533.551
33) L7 AR-1260-3	6.854	6.610	235.7E6	138.5E6	508.278	525.428
34) L7 AR-1260-4	7.114	7.081	212.8E6	115.2E6	500.338	541.645m
35) L7 AR-1260-5	7.355	7.321	490.9E6	263.7E6	505.135	544.966

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
Data File : PO108758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 09:31
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2024
Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 13:17:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

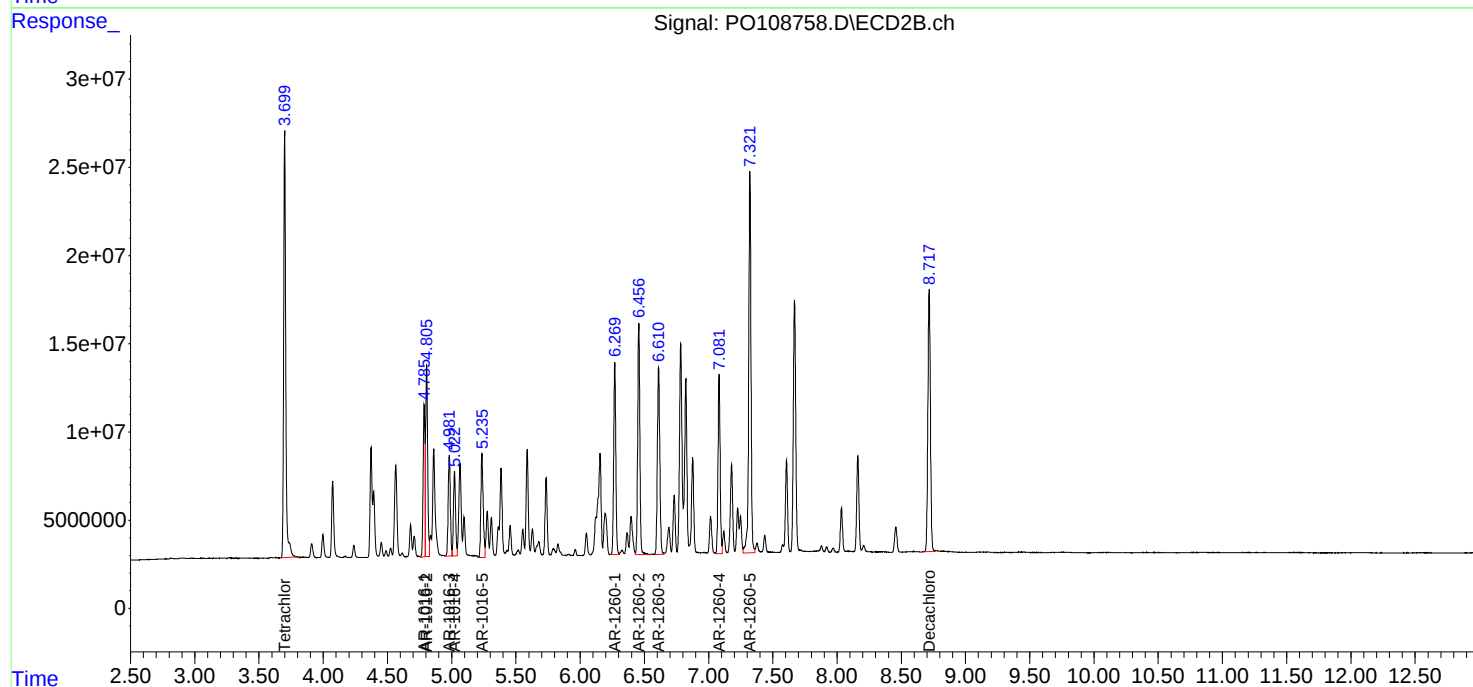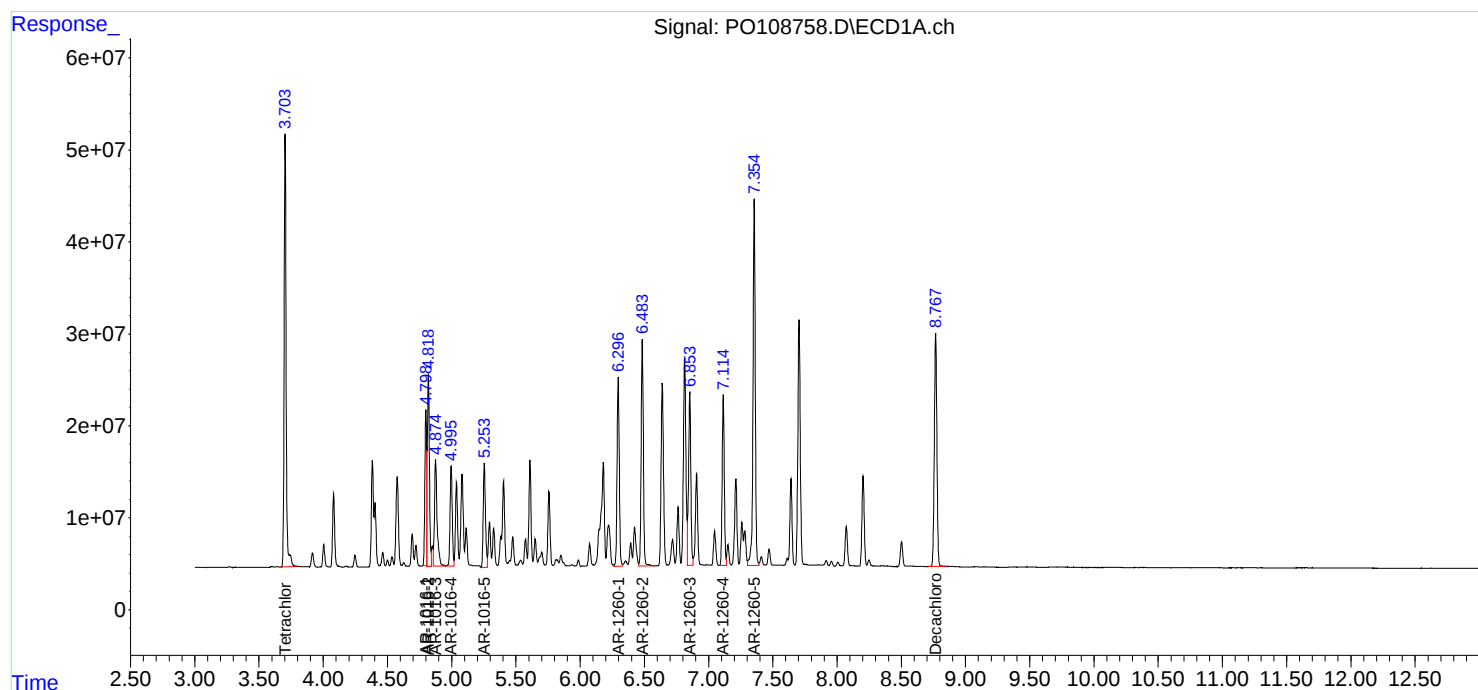



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

Continuing Calib Date: 12/26/2024 Initial Calibration Date(s): 12/06/2024 12/06/2024

Continuing Calib Time: 16:10 Initial Calibration Time(s): 14:19 22:34

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.80	4.81	4.71	4.91	0.01
Aroclor-1016-2	(2)	4.82	4.83	4.73	4.93	0.01
Aroclor-1016-3	(3)	4.87	4.89	4.79	4.99	0.02
Aroclor-1016-4	(4)	5.00	5.01	4.91	5.11	0.01
Aroclor-1016-5	(5)	5.25	5.27	5.17	5.37	0.02
Aroclor-1260-1	(1)	6.30	6.31	6.21	6.41	0.01
Aroclor-1260-2	(2)	6.48	6.50	6.40	6.60	0.02
Aroclor-1260-3	(3)	6.85	6.87	6.77	6.97	0.02
Aroclor-1260-4	(4)	7.11	7.13	7.03	7.23	0.02
Aroclor-1260-5	(5)	7.35	7.37	7.27	7.47	0.02
Tetrachloro-m-xylene		3.70	3.71	3.61	3.81	0.01
Decachlorobiphenyl		8.77	8.79	8.69	8.89	0.02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

Continuing Calib Date: 12/26/2024 Initial Calibration Date(s): 12/06/2024 12/06/2024

Continuing Calib Time: 16:10 Initial Calibration Time(s): 14:19 22:34

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND		CCAL RT	AVG RT	RT WINDOW		DIFF RT
				FROM	TO	
Aroclor-1016-1	(1)	4.79	4.80	4.70	4.90	0.02
Aroclor-1016-2	(2)	4.81	4.82	4.72	4.92	0.01
Aroclor-1016-3	(3)	4.98	4.99	4.89	5.09	0.01
Aroclor-1016-4	(4)	5.02	5.04	4.94	5.14	0.02
Aroclor-1016-5	(5)	5.24	5.25	5.15	5.35	0.01
Aroclor-1260-1	(1)	6.27	6.29	6.19	6.39	0.02
Aroclor-1260-2	(2)	6.46	6.47	6.37	6.57	0.01
Aroclor-1260-3	(3)	6.61	6.63	6.53	6.73	0.02
Aroclor-1260-4	(4)	7.08	7.10	7.00	7.20	0.02
Aroclor-1260-5	(5)	7.32	7.34	7.24	7.44	0.02
Tetrachloro-m-xylene		3.70	3.71	3.61	3.81	0.01
Decachlorobiphenyl		8.72	8.74	8.64	8.84	0.02



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 12/06/2024 12/06/2024

Client Sample No.: CCAL02 Date Analyzed: 12/26/2024

Lab Sample No.: AR1660CCC500 Data File : PO108773.D Time Analyzed: 16:10

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
Aroclor-1016-1	4.798	4.709	4.909	500.920	500.000	0.2
Aroclor-1016-2	4.819	4.729	4.929	536.280	500.000	7.3
Aroclor-1016-3	4.874	4.785	4.985	543.260	500.000	8.7
Aroclor-1016-4	4.996	4.907	5.107	553.060	500.000	10.6
Aroclor-1016-5	5.254	5.165	5.365	531.340	500.000	6.3
Aroclor-1260-1	6.296	6.210	6.410	460.940	500.000	-7.8
Aroclor-1260-2	6.484	6.398	6.598	500.470	500.000	0.1
Aroclor-1260-3	6.853	6.769	6.969	489.770	500.000	-2.0
Aroclor-1260-4	7.113	7.029	7.229	448.450	500.000	-10.3
Aroclor-1260-5	7.354	7.270	7.470	434.300	500.000	-13.1
Decachlorobiphenyl	8.766	8.691	8.891	41.820	50.000	-16.4
Tetrachloro-m-xylene	3.703	3.610	3.810	55.860	50.000	11.7



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 12/06/2024 12/06/2024

Client Sample No.: CCAL02 Date Analyzed: 12/26/2024

Lab Sample No.: AR1660CCC500 Data File : PO108773.D Time Analyzed: 16:10

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Aroclor-1016-1	4.785	4.698	4.898	546.650	500.000	9.3
Aroclor-1016-2	4.806	4.718	4.918	538.450	500.000	7.7
Aroclor-1016-3	4.981	4.894	5.094	528.610	500.000	5.7
Aroclor-1016-4	5.022	4.935	5.135	515.360	500.000	3.1
Aroclor-1016-5	5.236	5.150	5.350	549.390	500.000	9.9
Aroclor-1260-1	6.270	6.186	6.386	508.560	500.000	1.7
Aroclor-1260-2	6.457	6.373	6.573	501.550	500.000	0.3
Aroclor-1260-3	6.610	6.527	6.727	500.950	500.000	0.2
Aroclor-1260-4	7.083	7.000	7.200	502.140	500.000	0.4
Aroclor-1260-5	7.322	7.239	7.439	505.850	500.000	1.2
Decachlorobiphenyl	8.716	8.641	8.841	47.280	50.000	-5.4
Tetrachloro-m-xylene	3.700	3.608	3.808	53.750	50.000	7.5

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
 Data File : PO108773.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 16:10
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/27/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 20:27:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.703	3.700	486.0E6	272.5E6	55.863	53.753
2) SA Decachlor...	8.766	8.716	305.4E6	183.2E6	41.816	47.280
Target Compounds						
3) L1 AR-1016-1	4.798	4.785	154.5E6	87723512	500.915m	546.652m
4) L1 AR-1016-2	4.819	4.806	223.9E6	119.6E6	536.279	538.453
5) L1 AR-1016-3	4.874	4.981	159.0E6	66516293	543.263m	528.605
6) L1 AR-1016-4	4.996	5.022	127.9E6	54012709	553.059	515.359
7) L1 AR-1016-5	5.254	5.236	133.7E6	74283899	531.341	549.392
31) L7 AR-1260-1	6.296	6.270	210.7E6	119.0E6	460.941	508.557
32) L7 AR-1260-2	6.484	6.457	278.1E6	140.7E6	500.474	501.547
33) L7 AR-1260-3	6.853	6.610	227.1E6	132.0E6	489.769	500.953
34) L7 AR-1260-4	7.113	7.083	190.7E6	106.8E6	448.454	502.137
35) L7 AR-1260-5	7.354	7.322	422.1E6	244.8E6	434.304	505.851

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
Data File : PO108773.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 16:10
Operator : YP/AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

AR1660CCC500

Manual Integrations



APPROVED

Reviewed By :Yogesh Patel 12/27/2024

Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 20:27:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

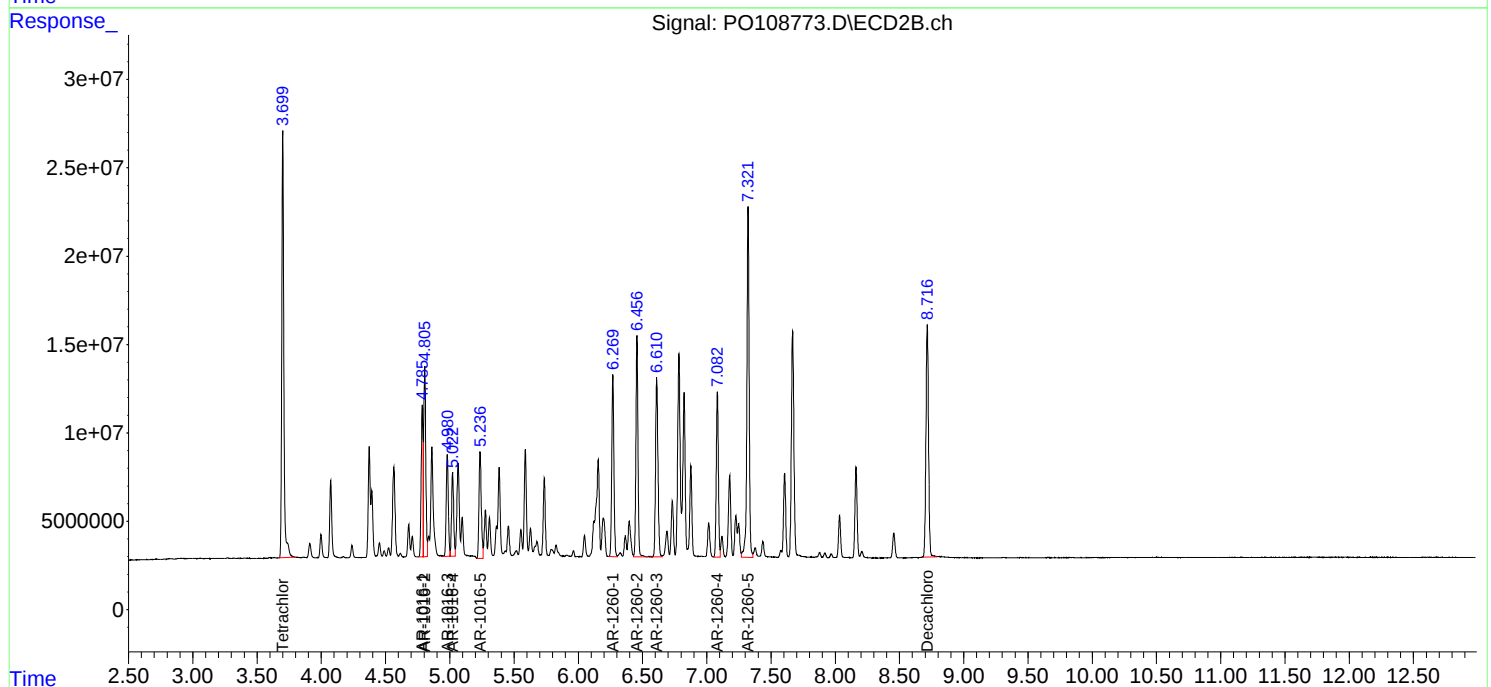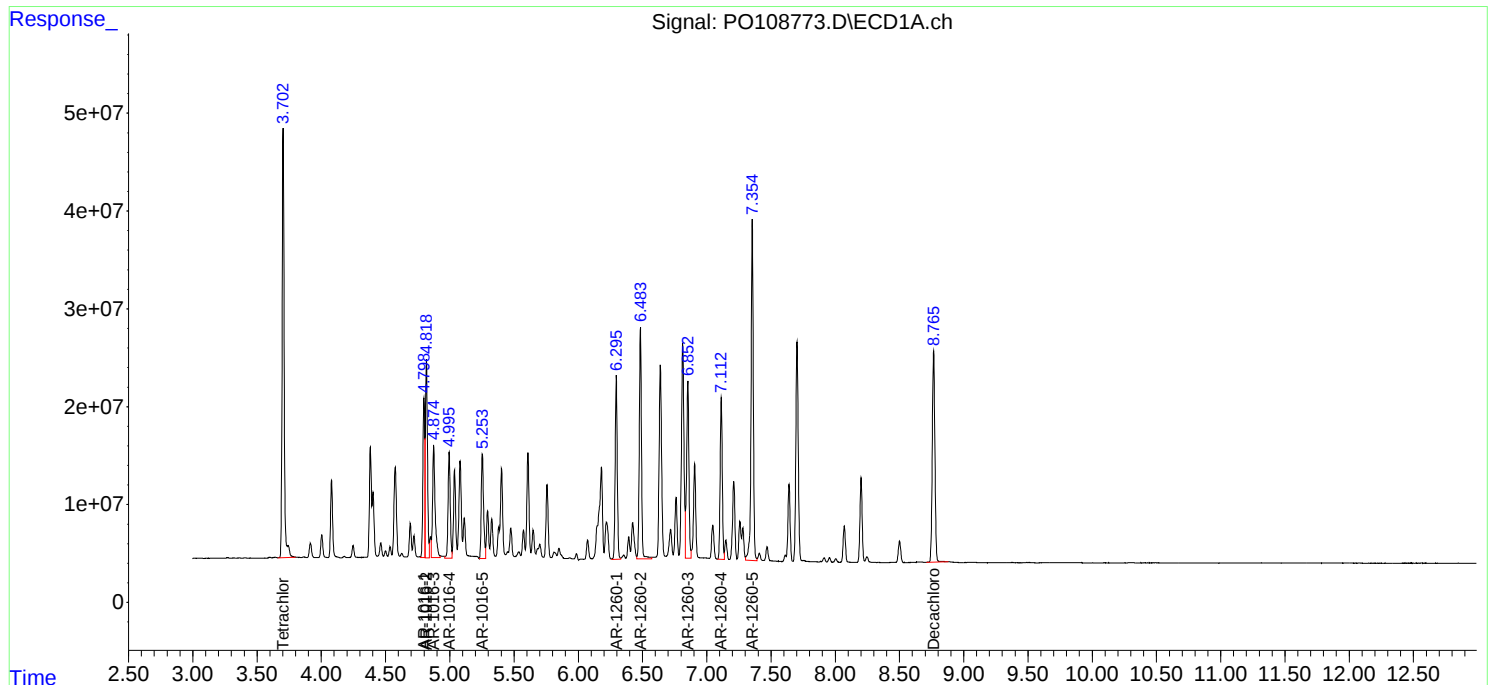

Analytical Sequence

Client: Kleinfelder

SDG No.: P5382

Project: Comegys School

Instrument ID: ECD_O

GC Column: ZB-MR1

ID: 0.32 (mm)

Inst. Calib. Date(s): 12/06/2024

12/06/2024

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
1.BLK	1.BLK	12/06/2024	14:01	PO108361.D	8.79	3.71
AR1660ICC1000	AR1660ICC1000	12/06/2024	14:19	PO108362.D	8.79	3.71
AR1660ICC750	AR1660ICC750	12/06/2024	14:38	PO108363.D	8.79	3.71
AR1660ICC500	AR1660ICC500	12/06/2024	14:56	PO108364.D	8.79	3.71
AR1660ICC250	AR1660ICC250	12/06/2024	15:14	PO108365.D	8.79	3.71
AR1660ICC050	AR1660ICC050	12/06/2024	15:33	PO108366.D	8.79	3.71
AR1221ICC500	AR1221ICC500	12/06/2024	15:51	PO108367.D	8.79	3.71
AR1232ICC500	AR1232ICC500	12/06/2024	16:09	PO108368.D	8.79	3.71
AR1242ICC1000	AR1242ICC1000	12/06/2024	16:28	PO108369.D	8.79	3.71
AR1242ICC750	AR1242ICC750	12/06/2024	16:46	PO108370.D	8.79	3.71
AR1242ICC500	AR1242ICC500	12/06/2024	17:04	PO108371.D	8.79	3.71
AR1242ICC250	AR1242ICC250	12/06/2024	17:23	PO108372.D	8.79	3.71
AR1242ICC050	AR1242ICC050	12/06/2024	17:41	PO108373.D	8.79	3.71
AR1248ICC1000	AR1248ICC1000	12/06/2024	17:59	PO108374.D	8.79	3.71
AR1248ICC750	AR1248ICC750	12/06/2024	18:18	PO108375.D	8.79	3.71
AR1248ICC500	AR1248ICC500	12/06/2024	18:36	PO108376.D	8.79	3.71
AR1248ICC250	AR1248ICC250	12/06/2024	18:54	PO108377.D	8.79	3.71
AR1248ICC050	AR1248ICC050	12/06/2024	19:13	PO108378.D	8.79	3.71
AR1254ICC1000	AR1254ICC1000	12/06/2024	19:31	PO108379.D	8.79	3.71
AR1254ICC750	AR1254ICC750	12/06/2024	19:49	PO108380.D	8.79	3.71
AR1254ICC500	AR1254ICC500	12/06/2024	20:08	PO108381.D	8.79	3.71
AR1254ICC250	AR1254ICC250	12/06/2024	20:26	PO108382.D	8.79	3.71
AR1254ICC050	AR1254ICC050	12/06/2024	20:44	PO108383.D	8.79	3.71
AR1262ICC500	AR1262ICC500	12/06/2024	21:03	PO108384.D	8.79	3.71
AR1268ICC1000	AR1268ICC1000	12/06/2024	21:21	PO108385.D	8.79	3.71
AR1268ICC750	AR1268ICC750	12/06/2024	21:39	PO108386.D	8.79	3.71
AR1268ICC500	AR1268ICC500	12/06/2024	21:58	PO108387.D	8.79	3.71
AR1268ICC250	AR1268ICC250	12/06/2024	22:16	PO108388.D	8.79	3.71
AR1268ICC050	AR1268ICC050	12/06/2024	22:34	PO108389.D	8.79	3.71
AR1660CCC500	AR1660CCC500	12/26/2024	09:31	PO108758.D	8.77	3.70
1.BLK	1.BLK	12/26/2024	11:32	PO108762.D	8.77	3.70
PB165843BL	PB165843BL	12/26/2024	12:21	PO108763.D	8.77	3.70
PB165843BS	PB165843BS	12/26/2024	12:39	PO108764.D	8.77	3.70
AU-06-122024MS	P5318-01MS	12/26/2024	13:34	PO108767.D	8.77	3.70
AU-06-122024MSD	P5318-01MSD	12/26/2024	13:52	PO108768.D	8.77	3.70
COMP-1	P5382-01	12/26/2024	14:29	PO108770.D	8.77	3.70
COMP-2	P5382-02	12/26/2024	14:47	PO108771.D	8.77	3.70
COMP-3	P5382-03	12/26/2024	15:05	PO108772.D	8.77	3.70
AR1660CCC500	AR1660CCC500	12/26/2024	16:10	PO108773.D	8.77	3.70
1.BLK	1.BLK	12/26/2024	17:24	PO108777.D	8.77	3.70

Analytical Sequence

Client: Kleinfelder

SDG No.: P5382

Project: Comegys School

Instrument ID: ECD_O

GC Column: ZB-MR2

ID: 0.32 (mm)

Inst. Calib. Date(s): 12/06/2024

12/06/2024

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

EPA SAMPLE NO.	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	12/06/2024	14:01	PO108361.D	8.74	3.71
AR1660ICC1000	AR1660ICC1000	12/06/2024	14:19	PO108362.D	8.74	3.71
AR1660ICC750	AR1660ICC750	12/06/2024	14:38	PO108363.D	8.74	3.71
AR1660ICC500	AR1660ICC500	12/06/2024	14:56	PO108364.D	8.74	3.71
AR1660ICC250	AR1660ICC250	12/06/2024	15:14	PO108365.D	8.74	3.71
AR1660ICC050	AR1660ICC050	12/06/2024	15:33	PO108366.D	8.74	3.71
AR1221ICC500	AR1221ICC500	12/06/2024	15:51	PO108367.D	8.74	3.71
AR1232ICC500	AR1232ICC500	12/06/2024	16:09	PO108368.D	8.74	3.71
AR1242ICC1000	AR1242ICC1000	12/06/2024	16:28	PO108369.D	8.74	3.71
AR1242ICC750	AR1242ICC750	12/06/2024	16:46	PO108370.D	8.74	3.71
AR1242ICC500	AR1242ICC500	12/06/2024	17:04	PO108371.D	8.74	3.71
AR1242ICC250	AR1242ICC250	12/06/2024	17:23	PO108372.D	8.74	3.71
AR1242ICC050	AR1242ICC050	12/06/2024	17:41	PO108373.D	8.74	3.71
AR1248ICC1000	AR1248ICC1000	12/06/2024	17:59	PO108374.D	8.74	3.71
AR1248ICC750	AR1248ICC750	12/06/2024	18:18	PO108375.D	8.74	3.71
AR1248ICC500	AR1248ICC500	12/06/2024	18:36	PO108376.D	8.74	3.71
AR1248ICC250	AR1248ICC250	12/06/2024	18:54	PO108377.D	8.74	3.71
AR1248ICC050	AR1248ICC050	12/06/2024	19:13	PO108378.D	8.74	3.71
AR1254ICC1000	AR1254ICC1000	12/06/2024	19:31	PO108379.D	8.74	3.71
AR1254ICC750	AR1254ICC750	12/06/2024	19:49	PO108380.D	8.74	3.71
AR1254ICC500	AR1254ICC500	12/06/2024	20:08	PO108381.D	8.74	3.71
AR1254ICC250	AR1254ICC250	12/06/2024	20:26	PO108382.D	8.74	3.71
AR1254ICC050	AR1254ICC050	12/06/2024	20:44	PO108383.D	8.74	3.71
AR1262ICC500	AR1262ICC500	12/06/2024	21:03	PO108384.D	8.74	3.71
AR1268ICC1000	AR1268ICC1000	12/06/2024	21:21	PO108385.D	8.74	3.71
AR1268ICC750	AR1268ICC750	12/06/2024	21:39	PO108386.D	8.74	3.71
AR1268ICC500	AR1268ICC500	12/06/2024	21:58	PO108387.D	8.74	3.71
AR1268ICC250	AR1268ICC250	12/06/2024	22:16	PO108388.D	8.74	3.71
AR1268ICC050	AR1268ICC050	12/06/2024	22:34	PO108389.D	8.74	3.71
AR1660CCC500	AR1660CCC500	12/26/2024	09:31	PO108758.D	8.72	3.70
IBLK	IBLK	12/26/2024	11:32	PO108762.D	8.72	3.70
PB165843BL	PB165843BL	12/26/2024	12:21	PO108763.D	8.72	3.70
PB165843BS	PB165843BS	12/26/2024	12:39	PO108764.D	8.72	3.70
AU-06-122024MS	P5318-01MS	12/26/2024	13:34	PO108767.D	8.72	3.70
AU-06-122024MSD	P5318-01MSD	12/26/2024	13:52	PO108768.D	8.72	3.70
COMP-1	P5382-01	12/26/2024	14:29	PO108770.D	8.72	3.70
COMP-2	P5382-02	12/26/2024	14:47	PO108771.D	8.72	3.70
COMP-3	P5382-03	12/26/2024	15:05	PO108772.D	8.72	3.70
AR1660CCC500	AR1660CCC500	12/26/2024	16:10	PO108773.D	8.72	3.70
IBLK	IBLK	12/26/2024	17:24	PO108777.D	8.72	3.70

COMPOUND DETECTION SUMMARY

CLIENT SAMPLE NO.

Contract: POWE02

Lab Code: CHEM **Case No.:** P5382 **SAS No.:** P5382 **SDG NO.:** P5382

Lab Sample ID: _____ **Date(s) Analyzed:** _____

Instrument ID (1): _____ **Instrument ID (2):** _____

GC Column: (1): _____ **ID:** _____ **(mm)** **GC Column:(2):** _____ **ID:** _____ **(mm)**

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	%RPD
			FROM	TO		
	1					
	2					



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB165843BS

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

Lab Sample ID: PB165843BS Date(s) Analyzed: 12/26/2024 12/26/2024

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO108764.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.798	4.748	4.848	157	165	4.33
COLUMN 1	2	4.818	4.768	4.868	160		
	3	4.874	4.824	4.924	173		
	4	4.996	4.946	5.046	171		
	5	5.253	5.203	5.303	163		
	1	4.786	4.736	4.836	156		
COLUMN 2	2	4.806	4.756	4.856	161	158	
	3	4.981	4.931	5.031	159		
	4	5.023	4.973	5.073	158		
	5	5.237	5.187	5.287	157		
Aroclor-1260	1	6.296	6.246	6.346	173	159	4.31
COLUMN 1	2	6.484	6.434	6.534	173		
	3	6.853	6.803	6.903	148		
	4	7.114	7.064	7.164	150		
	5	7.354	7.304	7.404	151		
	1	6.27	6.22	6.32	172		
COLUMN 2	2	6.456	6.406	6.506	172	166	
	3	6.61	6.56	6.66	171		
	4	7.082	7.032	7.132	156		
	5	7.321	7.271	7.371	158		

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

AU-06-122024MS

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

Lab Sample ID: P5318-01MS Date(s) Analyzed: 12/26/2024 12/26/2024

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO108767.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.799	4.749	4.849	140	128	7.52
COLUMN 1	2	4.819	4.769	4.869	129		
	3	4.874	4.824	4.924	134		
	4	4.995	4.945	5.045	131		
	5	5.253	5.203	5.303	109		
	1	4.786	4.736	4.836	139		
COLUMN 2	2	4.805	4.755	4.855	139	138	
	3	4.982	4.932	5.032	146		
	4	5.023	4.973	5.073	145		
	5	5.236	5.186	5.286	119		
Aroclor-1254	1	5.61	5.56	5.66	62.9	63.0	6.15
COLUMN 1	2	5.758	5.708	5.808	61.1		
	3	6.18	6.13	6.23	47.4		
	4	6.394	6.344	6.444	18.9		
	5	6.813	6.763	6.863	125		
	1	5.589	5.539	5.639	64.1		
COLUMN 2	2	5.735	5.685	5.785	60.2	67.0	
	3	6.155	6.105	6.205	43.5		
	4	6.367	6.317	6.417	22.0		
	5	6.784	6.734	6.834	145		

IDENTIFICATION SUMMARY FOR MULTICOMPONENT ANALYTES

Aroclor-1260	1	6.296	6.246	6.346	121		
	2	6.485	6.435	6.535	115		
	3	6.854	6.804	6.904	87.1		
	4	7.113	7.063	7.163	90.3		
	5	7.355	7.305	7.405	89.9		
COLUMN 1						101	
	1	6.27	6.22	6.32	137		
	2	6.457	6.407	6.507	134		
	3	6.61	6.56	6.66	132		
	4	7.081	7.031	7.131	107		
COLUMN 2	5	7.321	7.271	7.371	107	124	20.44

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

AU-06-122024MSD

Contract: POWE02

Lab Code: CHEM Case No.: P5382 SAS No.: P5382 SDG NO.: P5382

Lab Sample ID: P5318-01MSD Date(s) Analyzed: 12/26/2024 12/26/2024

Instrument ID (1): ECD_O Instrument ID (2): ECD_O

GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)

Data file PO108768.D

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	MEAN CONCENTRATION	%RPD
			FROM	TO			
Aroclor-1016	1	4.798	4.748	4.848	137	131	2.26
COLUMN 1	2	4.817	4.767	4.867	132		
	3	4.873	4.823	4.923	138		
	4	4.995	4.945	5.045	133		
	5	5.253	5.203	5.303	114		
	1	4.785	4.735	4.835	131		
COLUMN 2	2	4.805	4.755	4.855	140	134	
	3	4.981	4.931	5.031	138		
	4	5.022	4.972	5.072	139		
	5	5.236	5.186	5.286	124		
Aroclor-1254	1	5.609	5.559	5.659	59.0	62.3	19.94
COLUMN 1	2	5.757	5.707	5.807	56.7		
	3	6.179	6.129	6.229	46.4		
	4	6.393	6.343	6.443	18.3		
	5	6.813	6.763	6.863	131		
	1	5.589	5.539	5.639	65.5		
COLUMN 2	2	5.735	5.685	5.785	63.2	76.1	
	3	6.155	6.105	6.205	50.9		
	4	6.397	6.347	6.447	48.0		
	5	6.783	6.733	6.833	153		



Aroclor-1260	1	6.295	6.245	6.345	121	104	19.91	
	2	6.484	6.434	6.534	113			
	3	6.853	6.803	6.903	93.1			
	4	7.113	7.063	7.163	98.5			
	5	7.354	7.304	7.404	94.9			
COLUMN 1						127		19.91
	1	6.27	6.22	6.32	138			
	2	6.456	6.406	6.506	134			
	3	6.61	6.56	6.66	131			
	4	7.081	7.031	7.131	118			
COLUMN 2	5	7.321	7.271	7.371	114	127	19.91	



QC SAMPLE DATA

Report of Analysis

Client:	Kleinfelder	Date Collected:	
Project:	Comegys School	Date Received:	
Client Sample ID:	PB165843BL	SDG No.:	P5382
Lab Sample ID:	PB165843BL	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	100
Sample Wt/Vol:	30.02 Units: g	Decanted:	
Soil Aliquot Vol:	uL	Final Vol:	10000 uL
Extraction Type:		Test:	PCB Group1
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108763.D	1	12/26/24 08:30	12/26/24 12:21	PB165843

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	3.40	U	3.40	17.0	ug/kg
11097-69-1	Aroclor-1254	2.70	U	2.70	17.0	ug/kg
11096-82-5	Aroclor-1260	2.90	U	2.90	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	22.0		32 - 144	110%	SPK: 20
2051-24-3	Decachlorobiphenyl	22.9		32 - 175	115%	SPK: 20

Comments:

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 E = Value Exceeds Calibration Range
 P = Indicates >25% difference for detected concentrations between the two GC columns
 Q = indicates LCS control criteria did not meet requirements
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 N = Presumptive Evidence of a Compound
 * = Values outside of QC limits
 D = Dilution
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
 Data File : PO108763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 12:21
 Operator : YP/AJ
 Sample : PB165843BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB165843BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 13:20:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.703	3.700	191.6E6	101.5E6	22.018	20.013
2) SA Decachlor...	8.768	8.717	161.9E6	88829372	22.168	22.924

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
Data File : PO108763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 12:21
Operator : YP/AJ
Sample : PB165843BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB165843BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 13:20:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

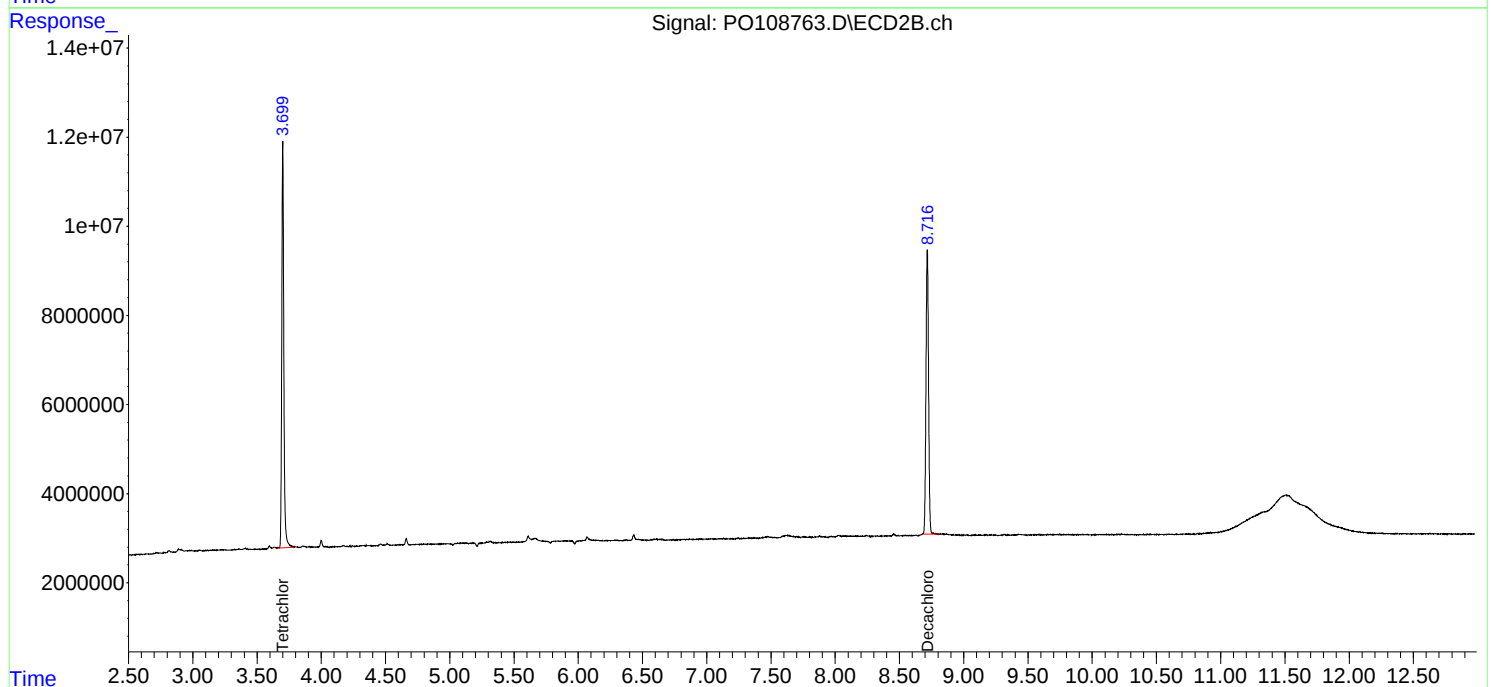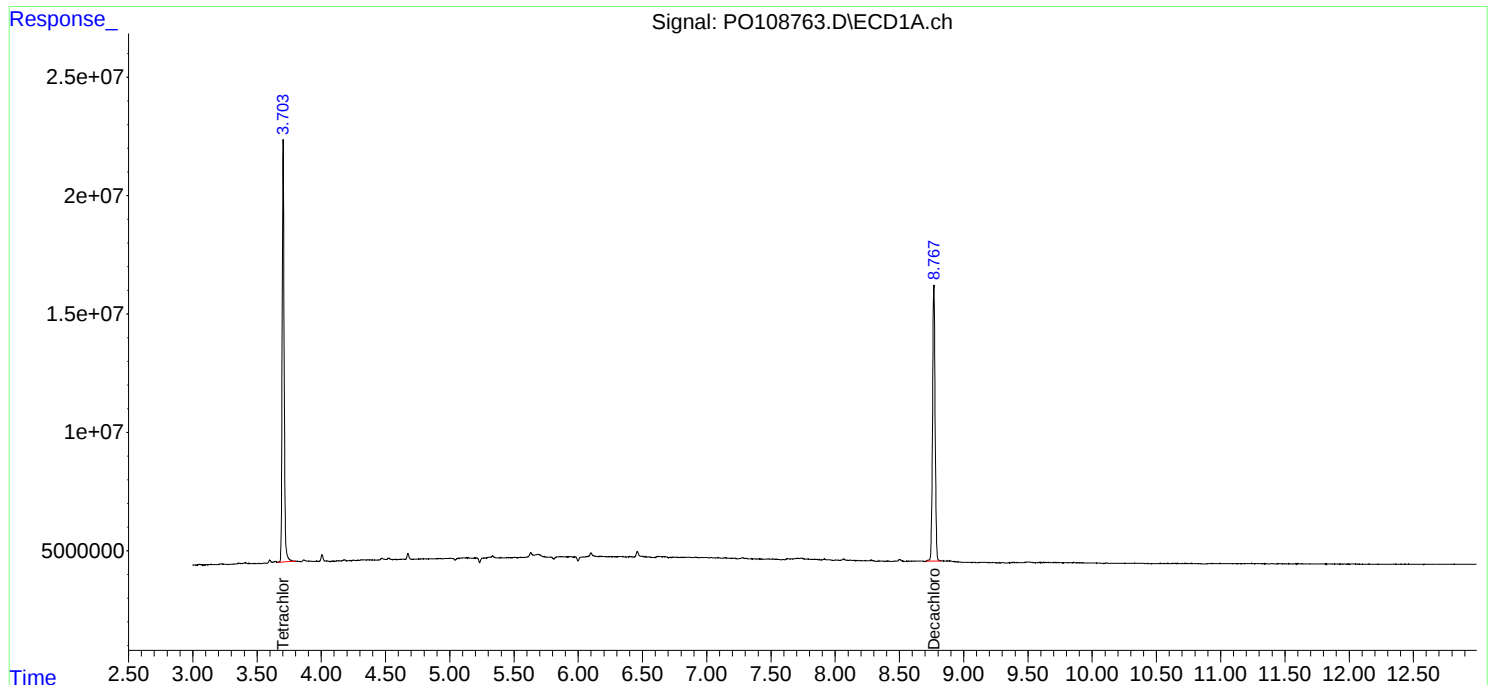


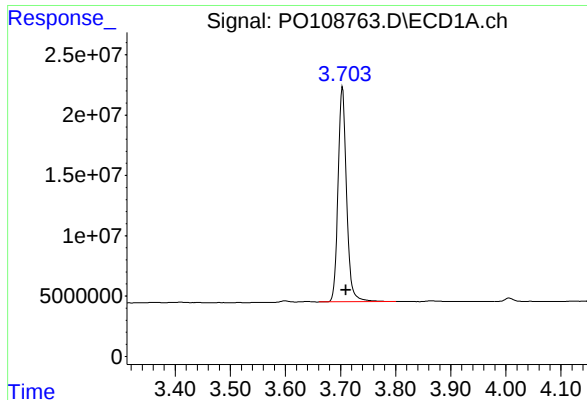

#1 Tetrachloro-m-xylene


R.T.: 3.703 min
Delta R.T.: -0.007 min
Response: 191560666
Conc: 22.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB165843BL

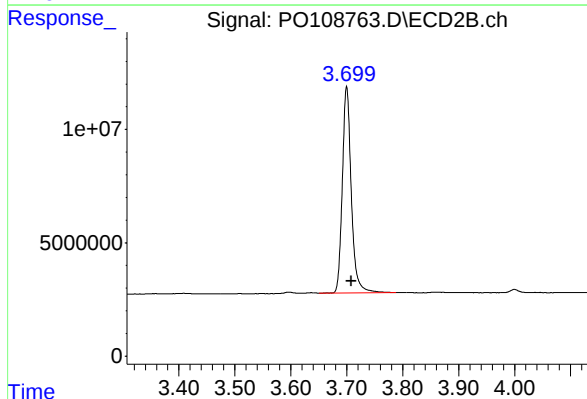


#1 Tetrachloro-m-xylene

R.T.: 3.700 min
Delta R.T.: -0.009 min
Response: 101451572
Conc: 20.01 ng/ml

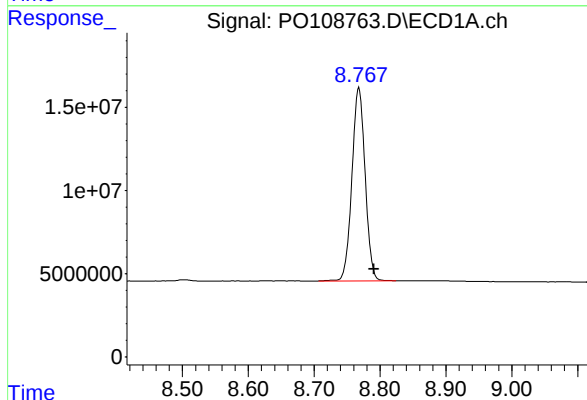

#2 Decachlorobiphenyl

R.T.: 8.768 min
Delta R.T.: -0.023 min
Response: 161918151
Conc: 22.17 ng/ml

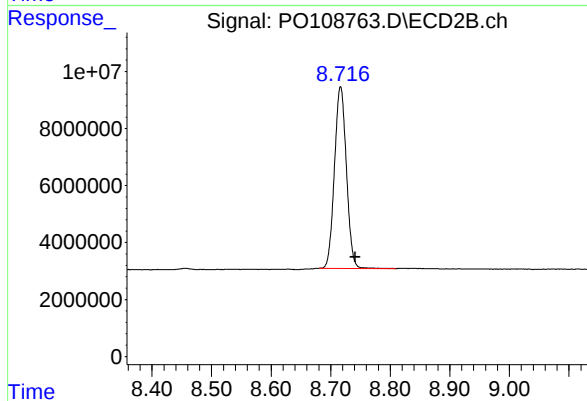

#2 Decachlorobiphenyl

R.T.: 8.717 min
Delta R.T.: -0.025 min
Response: 88829372
Conc: 22.92 ng/ml

Report of Analysis

Client:	Kleinfelder	Date Collected:	12/06/24
Project:	Comegys School	Date Received:	12/06/24
Client Sample ID:	PIBLK-PO108361.D	SDG No.:	P5382
Lab Sample ID:	I.BLK-PO108361.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB Group1
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108361.D	1		12/06/24	PO120624

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.6		60 - 140	108%	SPK: 20
2051-24-3	Decachlorobiphenyl	23.6		60 - 140	118%	SPK: 20

Comments:

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 E = Value Exceeds Calibration Range
 P = Indicates >25% difference for detected concentrations between the two GC columns
 Q = indicates LCS control criteria did not meet requirements
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 N = Presumptive Evidence of a Compound
 * = Values outside of QC limits
 D = Dilution
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
 Data File : PO108361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Dec 2024 14:01
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 06:00:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.711	3.708	199.9E6	109.7E6	22.973	21.649
2) SA Decachlor...	8.790	8.741	172.3E6	91294392	23.583	23.560

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120624\
Data File : PO108361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Dec 2024 14:01
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 06:00:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

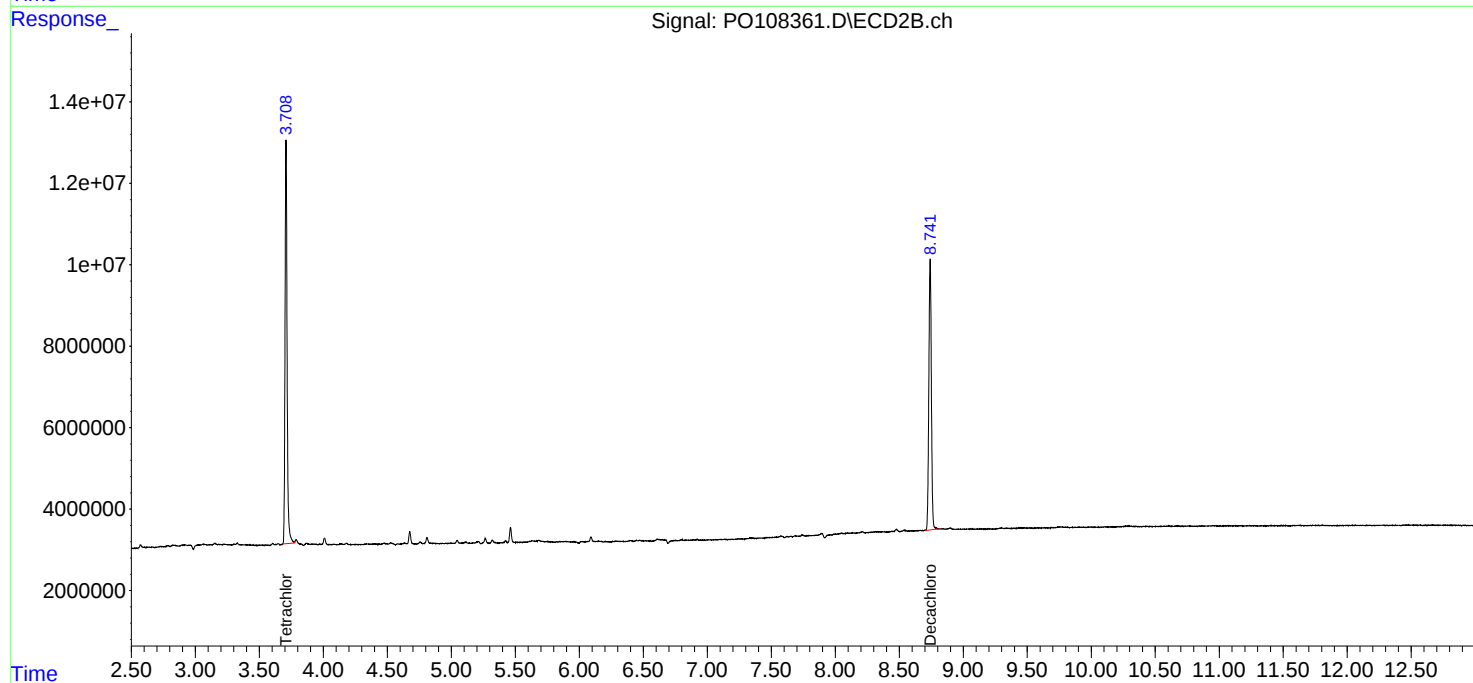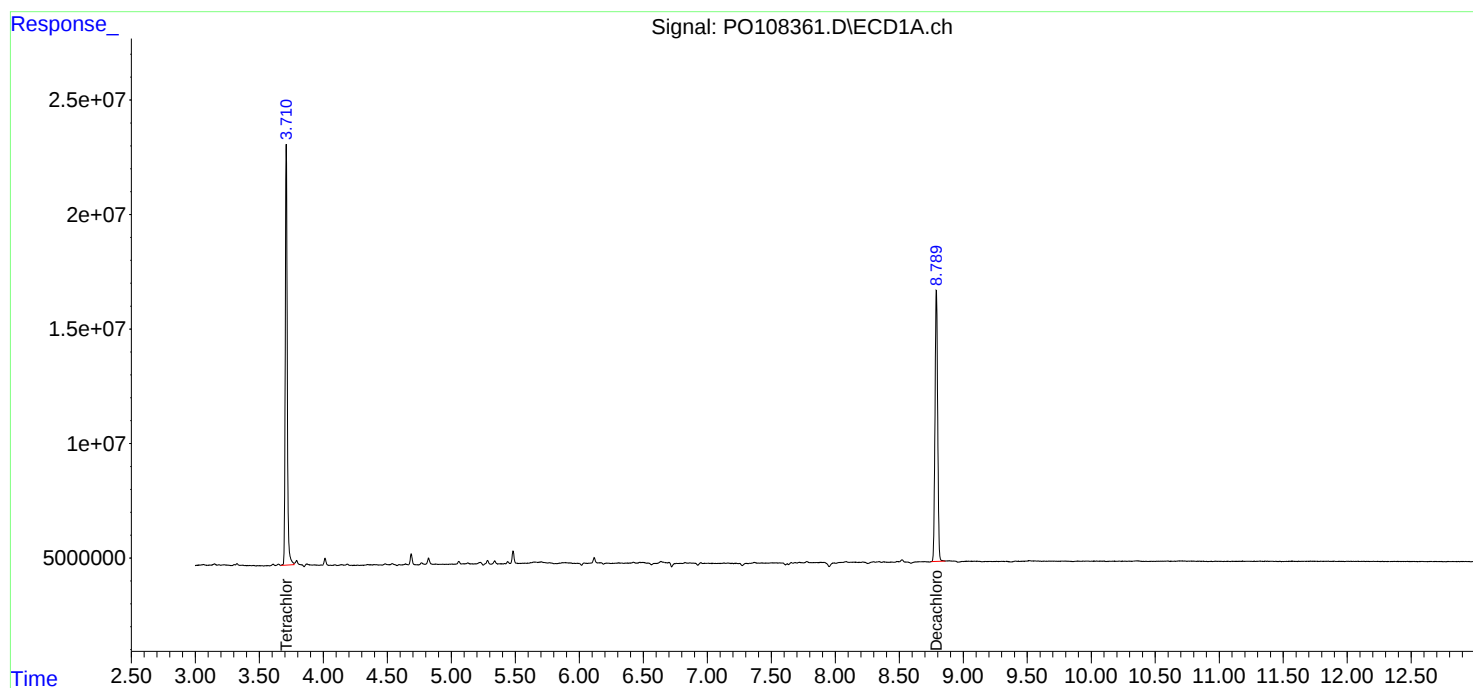


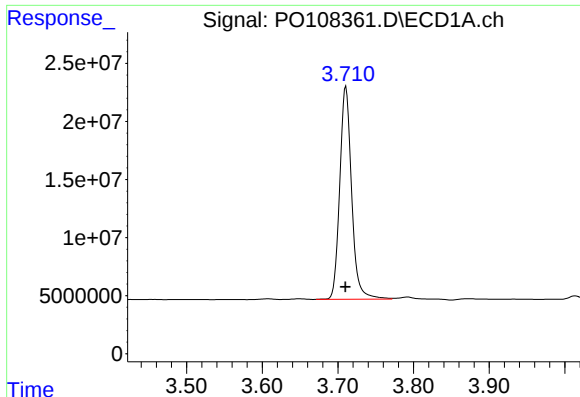

#1 Tetrachloro-m-xylene


R.T.: 3.711 min
Delta R.T.: 0.000 min
Response: 199870010
Conc: 22.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

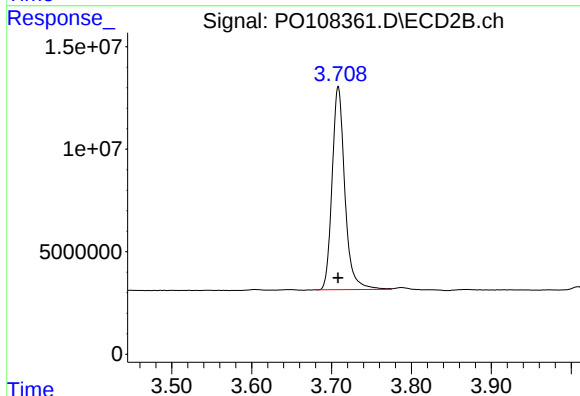


#1 Tetrachloro-m-xylene

R.T.: 3.708 min
Delta R.T.: 0.000 min
Response: 109748107
Conc: 21.65 ng/ml

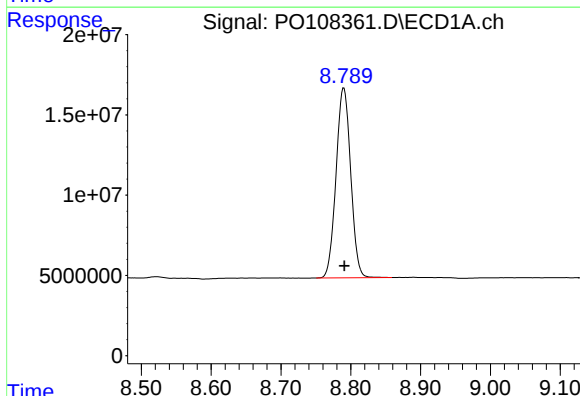

#2 Decachlorobiphenyl

R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 172254353
Conc: 23.58 ng/ml

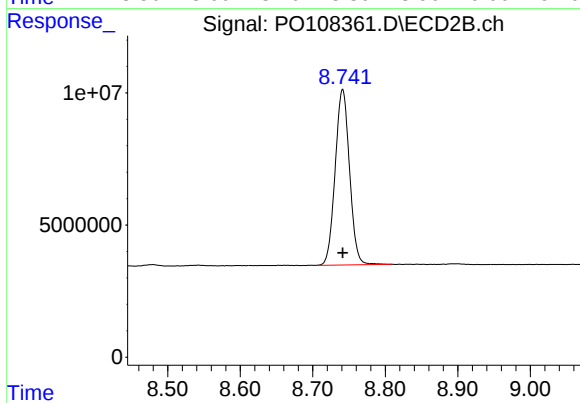

#2 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: 0.000 min
Response: 91294392
Conc: 23.56 ng/ml

Report of Analysis

Client:	Kleinfelder	Date Collected:	12/26/24
Project:	Comegys School	Date Received:	12/26/24
Client Sample ID:	PIBLK-PO108762.D	SDG No.:	P5382
Lab Sample ID:	I.BLK-PO108762.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB Group1
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108762.D	1		12/26/24	PO122624

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	20.0		60 - 140	100%	SPK: 20
2051-24-3	Decachlorobiphenyl	21.3		60 - 140	107%	SPK: 20

Comments:

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 E = Value Exceeds Calibration Range
 P = Indicates >25% difference for detected concentrations between the two GC columns
 Q = indicates LCS control criteria did not meet requirements
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 N = Presumptive Evidence of a Compound
 * = Values outside of QC limits
 D = Dilution
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
 Data File : PO108762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 11:32
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 13:19:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.703	3.700	189.6E6	101.4E6	21.795	20.001
2) SA Decachlor...	8.767	8.716	155.7E6	85520616	21.316	22.070

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
Data File : PO108762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 11:32
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 13:19:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

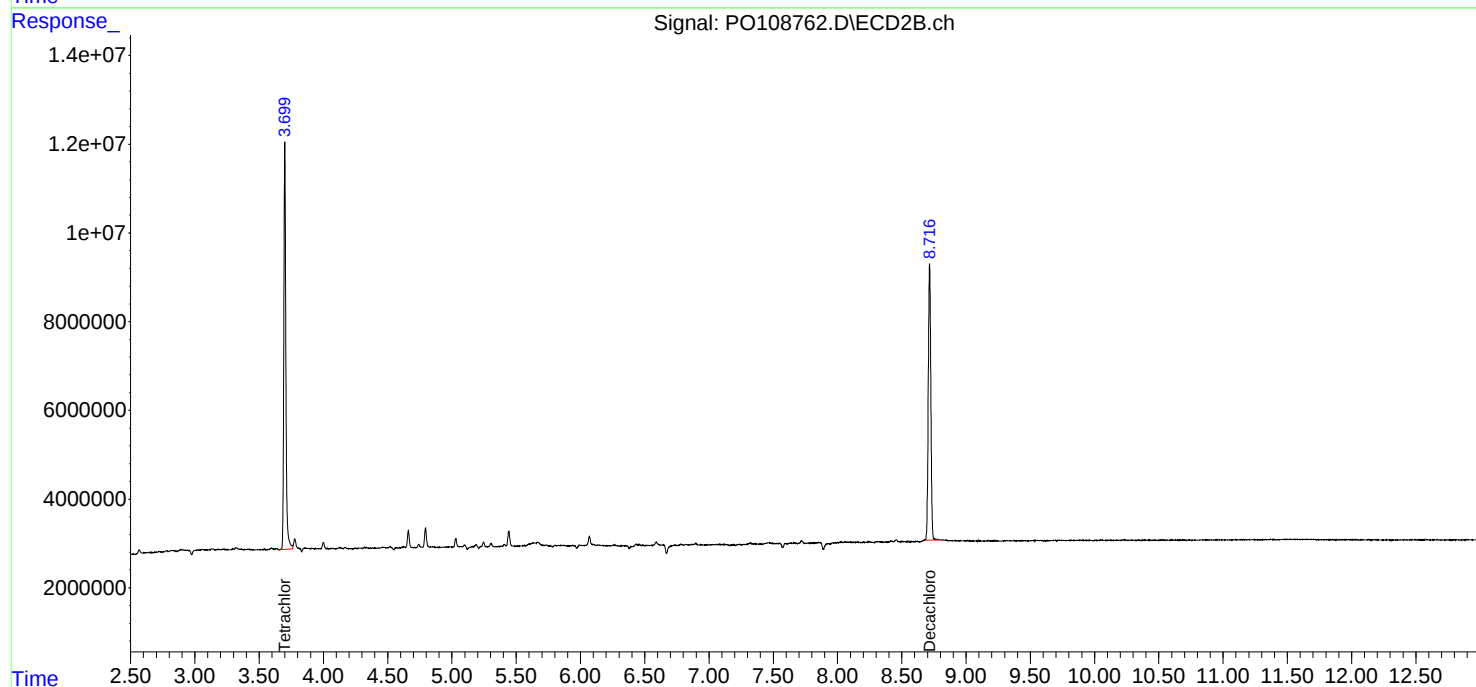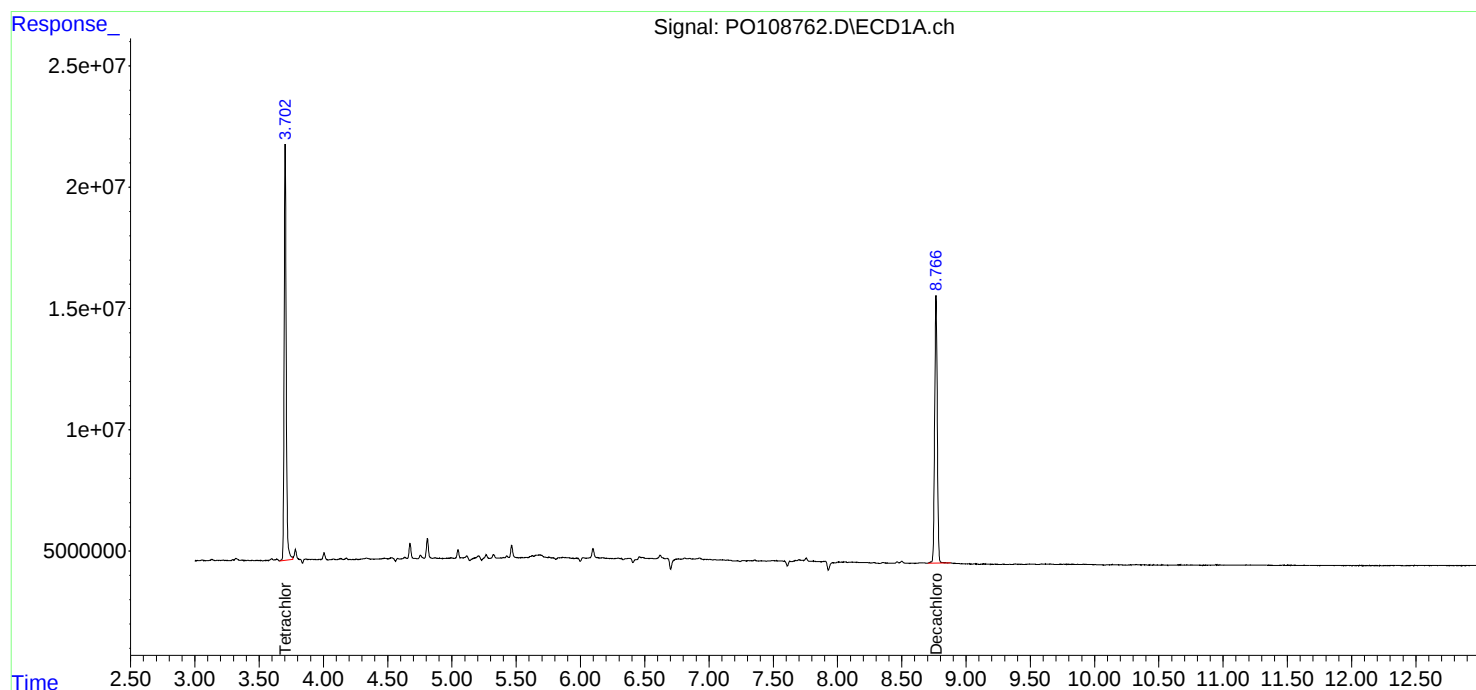


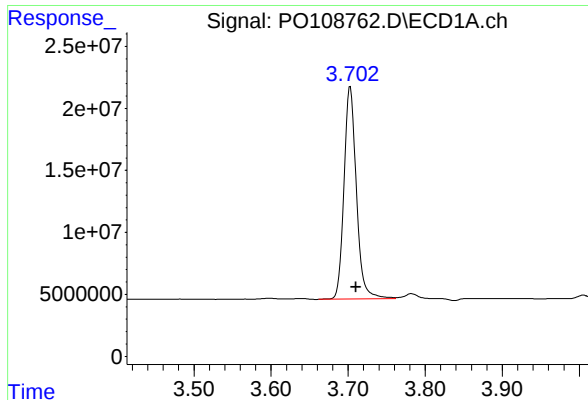

#1 Tetrachloro-m-xylene


R.T.: 3.703 min
Delta R.T.: -0.007 min
Response: 189622024
Conc: 21.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

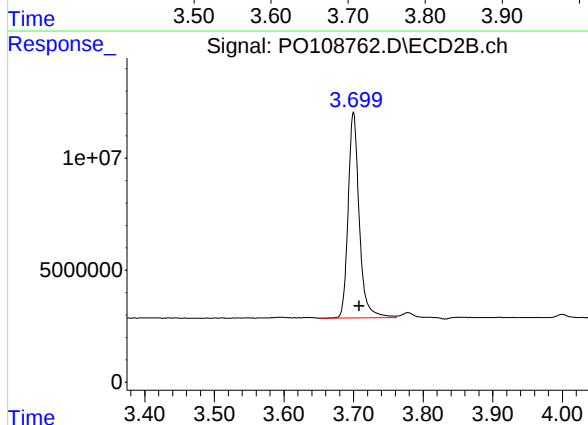


#1 Tetrachloro-m-xylene

R.T.: 3.700 min
Delta R.T.: -0.009 min
Response: 101391275
Conc: 20.00 ng/ml

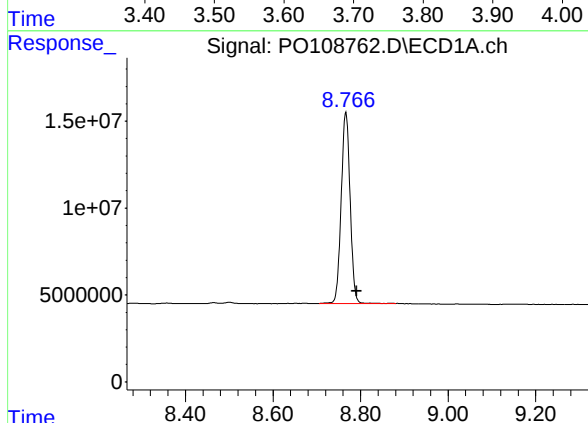

#2 Decachlorobiphenyl

R.T.: 8.767 min
Delta R.T.: -0.024 min
Response: 155695866
Conc: 21.32 ng/ml

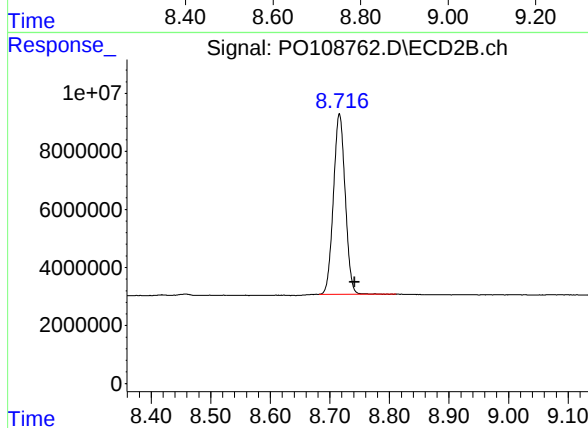

#2 Decachlorobiphenyl

R.T.: 8.716 min
Delta R.T.: -0.025 min
Response: 85520616
Conc: 22.07 ng/ml

Report of Analysis

Client:	Kleinfelder	Date Collected:	12/26/24
Project:	Comegys School	Date Received:	12/26/24
Client Sample ID:	PIBLK-PO108777.D	SDG No.:	P5382
Lab Sample ID:	I.BLK-PO108777.D	Matrix:	WATER
Analytical Method:	SW8082A	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB Group1
GPC Factor :	1.0	PH :	
Prep Method :	5030	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108777.D	1		12/26/24	PO122624

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
12674-11-2	Aroclor-1016	0.15	U	0.15	0.50	ug/L
11097-69-1	Aroclor-1254	0.11	U	0.11	0.50	ug/L
11096-82-5	Aroclor-1260	0.15	U	0.15	0.50	ug/L
SURROGATES						
877-09-8	Tetrachloro-m-xylene	19.4		60 - 140	97%	SPK: 20
2051-24-3	Decachlorobiphenyl	18.1		60 - 140	90%	SPK: 20

Comments:

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 E = Value Exceeds Calibration Range
 P = Indicates >25% difference for detected concentrations between the two GC columns
 Q = indicates LCS control criteria did not meet requirements
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 N = Presumptive Evidence of a Compound
 * = Values outside of QC limits
 D = Dilution
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
 Data File : PO108777.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 17:24
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 20:28:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.703	3.701	178.1E6	98099223	20.469	19.351
2) SA Decachlor...	8.765	8.716	131.9E6	77109959	18.060	19.900

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
Data File : PO108777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 17:24
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 20:28:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

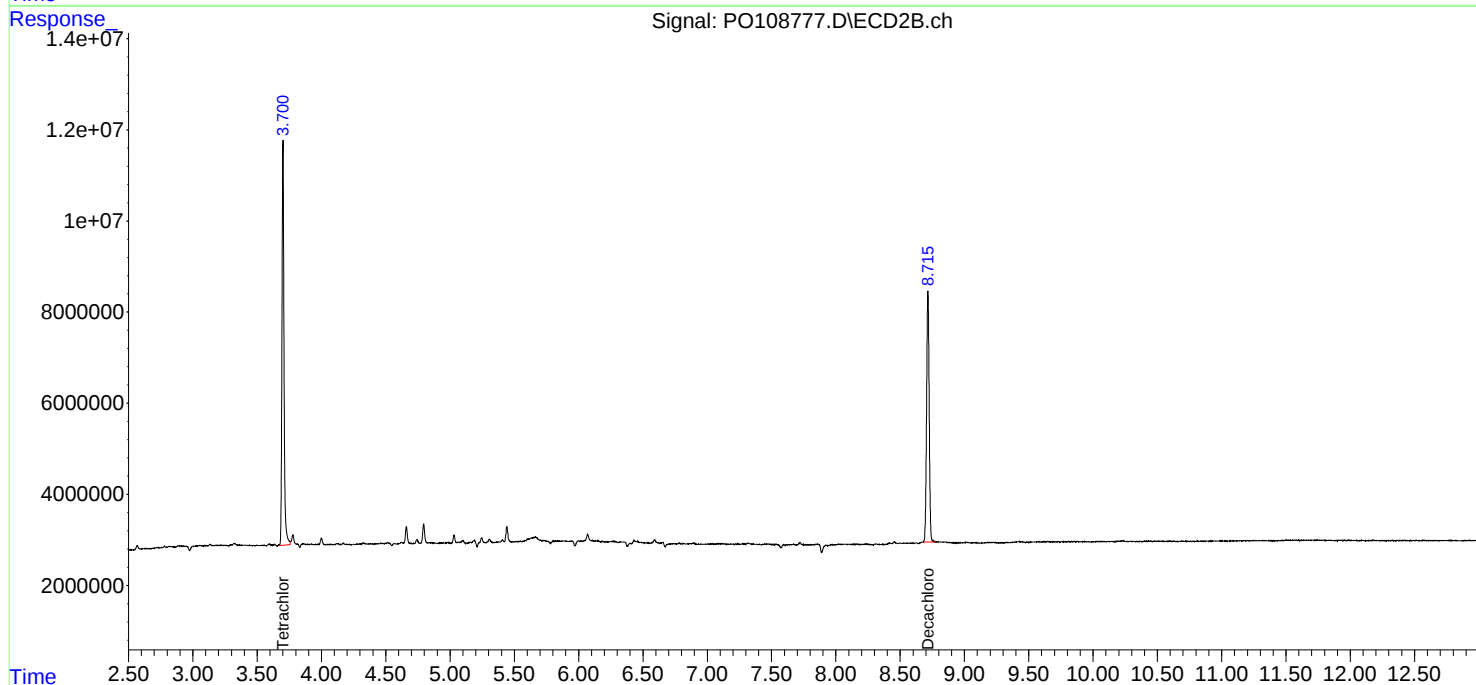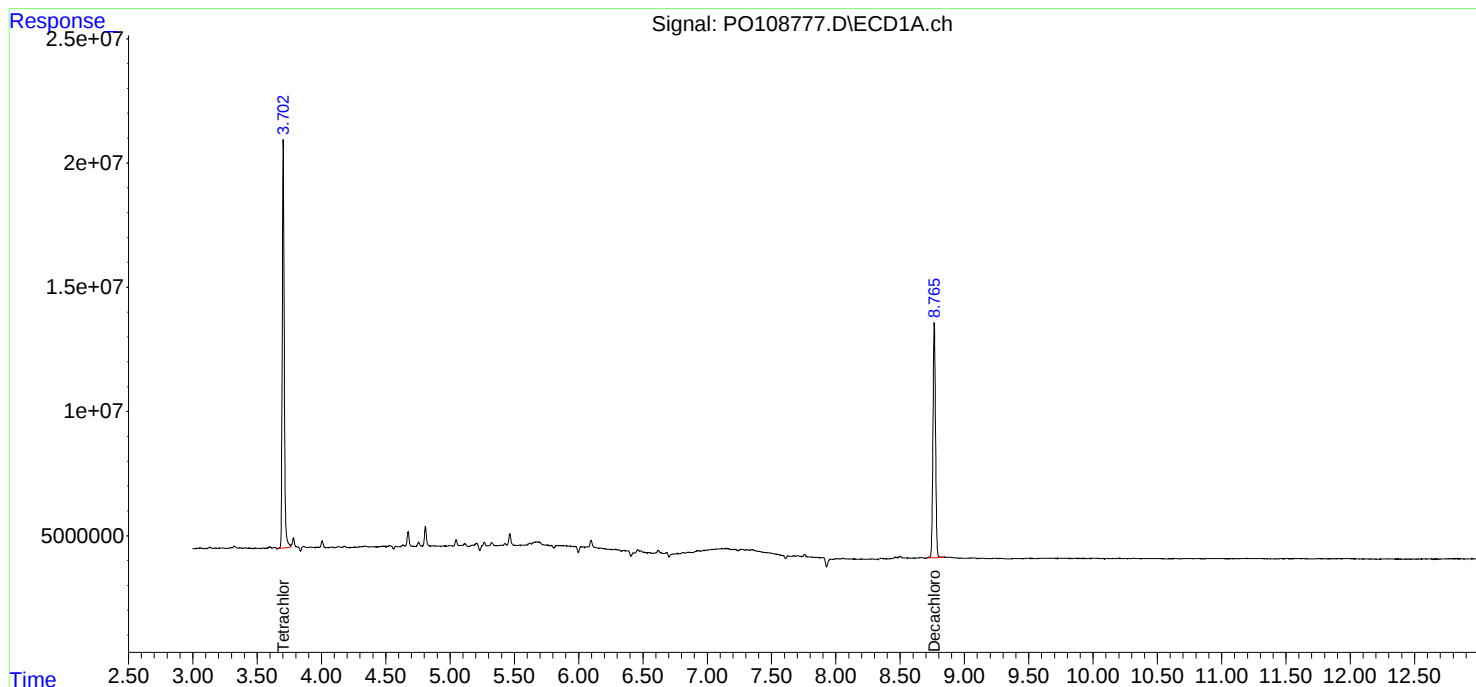


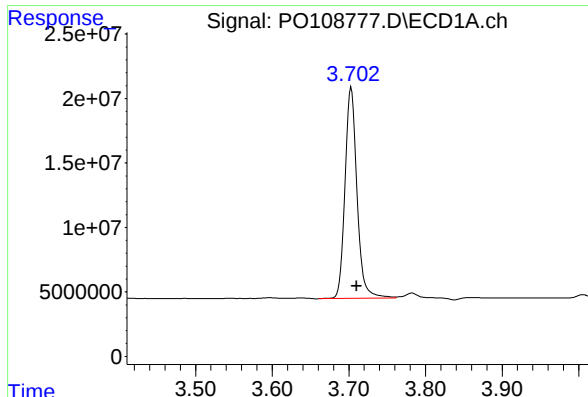

#1 Tetrachloro-m-xylene


R.T.: 3.703 min
Delta R.T.: -0.007 min
Response: 178086317
Conc: 20.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

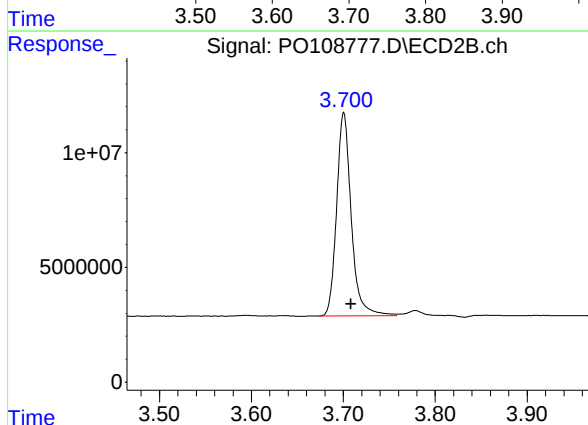


#1 Tetrachloro-m-xylene

R.T.: 3.701 min
Delta R.T.: -0.008 min
Response: 98099223
Conc: 19.35 ng/ml

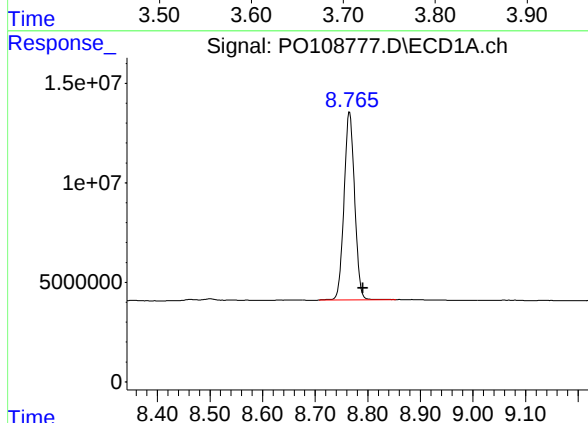

#2 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: -0.026 min
Response: 131912093
Conc: 18.06 ng/ml

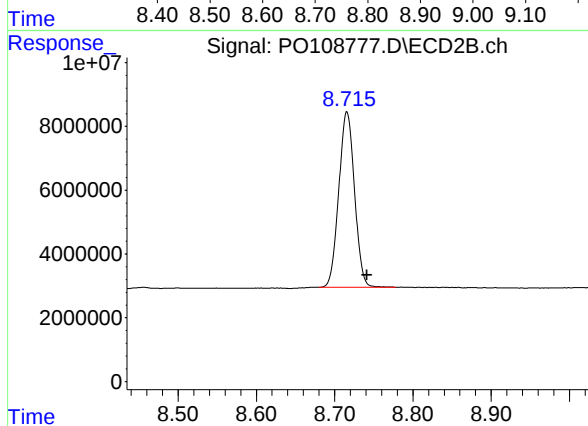

#2 Decachlorobiphenyl

R.T.: 8.716 min
Delta R.T.: -0.026 min
Response: 77109959
Conc: 19.90 ng/ml

Report of Analysis

Client:	Kleinfelder	Date Collected:	
Project:	Comegys School	Date Received:	
Client Sample ID:	PB165843BS	SDG No.:	P5382
Lab Sample ID:	PB165843BS	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	100 Decanted:
Sample Wt/Vol:	30.01 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PCB Group1
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108764.D	1	12/26/24 08:30	12/26/24 12:39	PB165843

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	165		3.40	17.0	ug/kg
11097-69-1	Aroclor-1254	2.70	U	2.70	17.0	ug/kg
11096-82-5	Aroclor-1260	166		2.90	17.0	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	21.2		32 - 144	106%	SPK: 20
2051-24-3	Decachlorobiphenyl	23.2		32 - 175	116%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
 Data File : PO108764.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 12:39
 Operator : YP/AJ
 Sample : PB165843BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

PB165843BS

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 12/27/2024

Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 13:21:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.704	3.700	184.5E6	97355081	21.201	19.205
2) SA Decachlor...	8.766	8.717	158.3E6	89764925	21.679m	23.166
Target Compounds						
3) L1 AR-1016-1	4.798	4.786	145.4E6	75056310	471.504m	467.716m
4) L1 AR-1016-2	4.818	4.806	199.8E6	107.0E6	478.763m	481.828
5) L1 AR-1016-3	4.874	4.981	152.2E6	59862847	520.119	475.730
6) L1 AR-1016-4	4.996	5.023	118.6E6	49759685	513.098	474.779
7) L1 AR-1016-5	5.253	5.237	123.4E6	63807633	490.468	471.911
31) L7 AR-1260-1	6.296	6.270	237.4E6	120.8E6	519.356	516.062
32) L7 AR-1260-2	6.484	6.456	287.7E6	144.5E6	517.757	514.849
33) L7 AR-1260-3	6.853	6.610	205.6E6	135.4E6	443.461	513.878
34) L7 AR-1260-4	7.114	7.082	191.7E6	99875620	450.665	469.450m
35) L7 AR-1260-5	7.354	7.321	440.1E6	228.9E6	452.843	473.004

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
Data File : PO108764.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 12:39
Operator : YP/AJ
Sample : PB165843BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

PB165843BS



Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 12/27/2024
Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 13:21:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

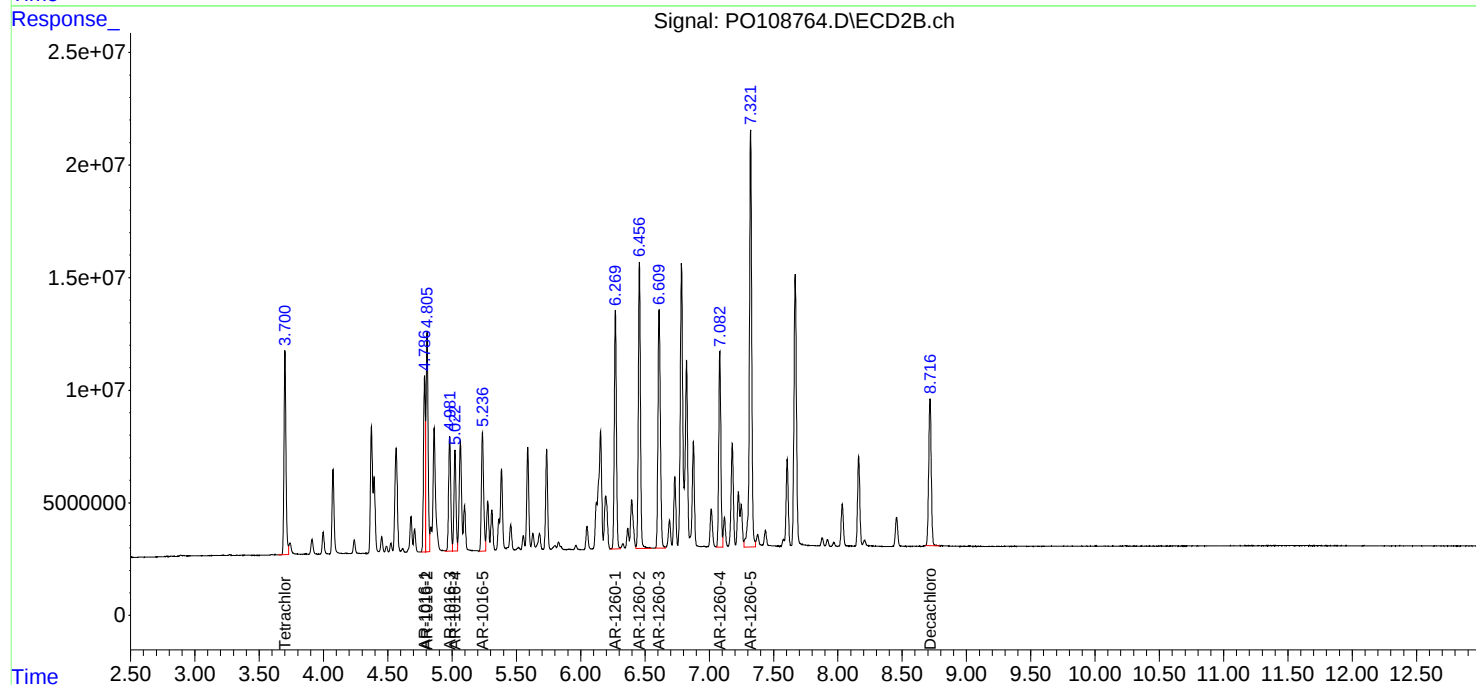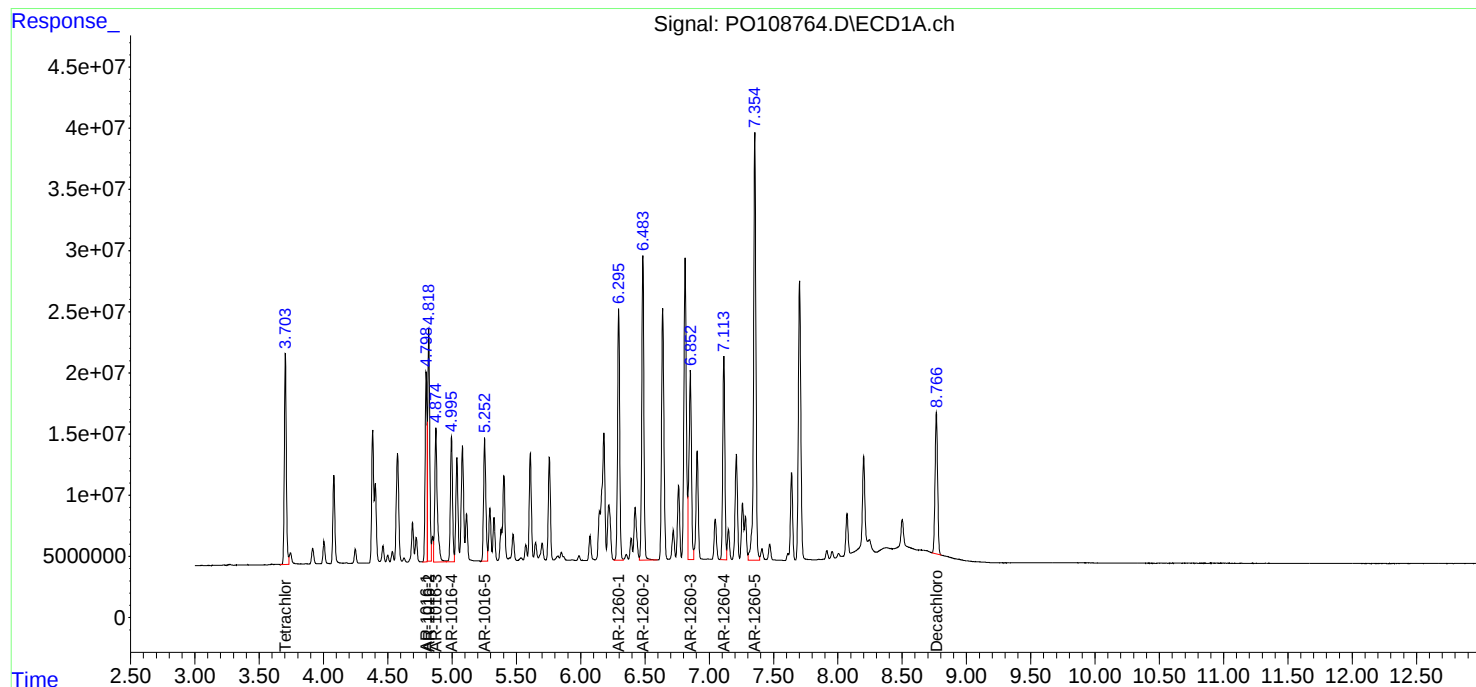

Report of Analysis

Client:	Kleinfelder	Date Collected:	12/20/24
Project:	Comegys School	Date Received:	12/20/24
Client Sample ID:	AU-06-122024MS	SDG No.:	P5382
Lab Sample ID:	P5318-01MS	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	86.2
Sample Wt/Vol:	30.02	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB Group1
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108767.D	1	12/26/24 08:30	12/26/24 13:34	PB165843

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	138		3.90	19.7	ug/kg
11097-69-1	Aroclor-1254	67.0		3.20	19.7	ug/kg
11096-82-5	Aroclor-1260	124		3.40	19.7	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	13.5		32 - 144	67%	SPK: 20
2051-24-3	Decachlorobiphenyl	12.1		32 - 175	61%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
 Data File : PO108767.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 13:34
 Operator : YP/AJ
 Sample : P5318-01MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-06-122024MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/27/2024
 Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 20:25:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.703	3.700	117.1E6	63005635	13.465	12.429
2) SA Decachlor...	8.767	8.716	79994059	47034703	10.952	12.138
Target Compounds						
3) L1 AR-1016-1	4.799	4.786	111.4E6	57738215	361.068m	359.797m
4) L1 AR-1016-2	4.819	4.805	139.2E6	79882192	333.477m	359.679m
5) L1 AR-1016-3	4.874	4.982	101.6E6	47595257	347.045m	378.240
6) L1 AR-1016-4	4.995	5.023	78285027	39357397	338.637m	375.527
7) L1 AR-1016-5	5.253	5.236	70709034	41496048	280.959	306.898
26) L6 AR-1254-1	5.610	5.589	83640162	44889774	162.838	165.748m
27) L6 AR-1254-2	5.758	5.735	72002105	37409671	158.087	155.860m
28) L6 AR-1254-3	6.180	6.155	88420672	42236300	122.785m	112.477m
29) L6 AR-1254-4	6.394	6.367	21409815	12408858	48.790	57.006
30) L6 AR-1254-5	6.813	6.784	205.2E6	121.2E6	323.152	375.633
31) L7 AR-1260-1	6.296	6.270	143.5E6	82940985	313.875	354.395
32) L7 AR-1260-2	6.485	6.457	165.4E6	97504750	297.586	347.527
33) L7 AR-1260-3	6.854	6.610	104.5E6	90045747	225.333	341.641 #
34) L7 AR-1260-4	7.113	7.081	99412583	58853339	233.725	276.631m
35) L7 AR-1260-5	7.355	7.321	226.1E6	134.4E6	232.673	277.749

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
Data File : PO108767.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 13:34
Operator : YP/AJ
Sample : P5318-01MS
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AU-06-122024MS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2024
Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 20:25:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

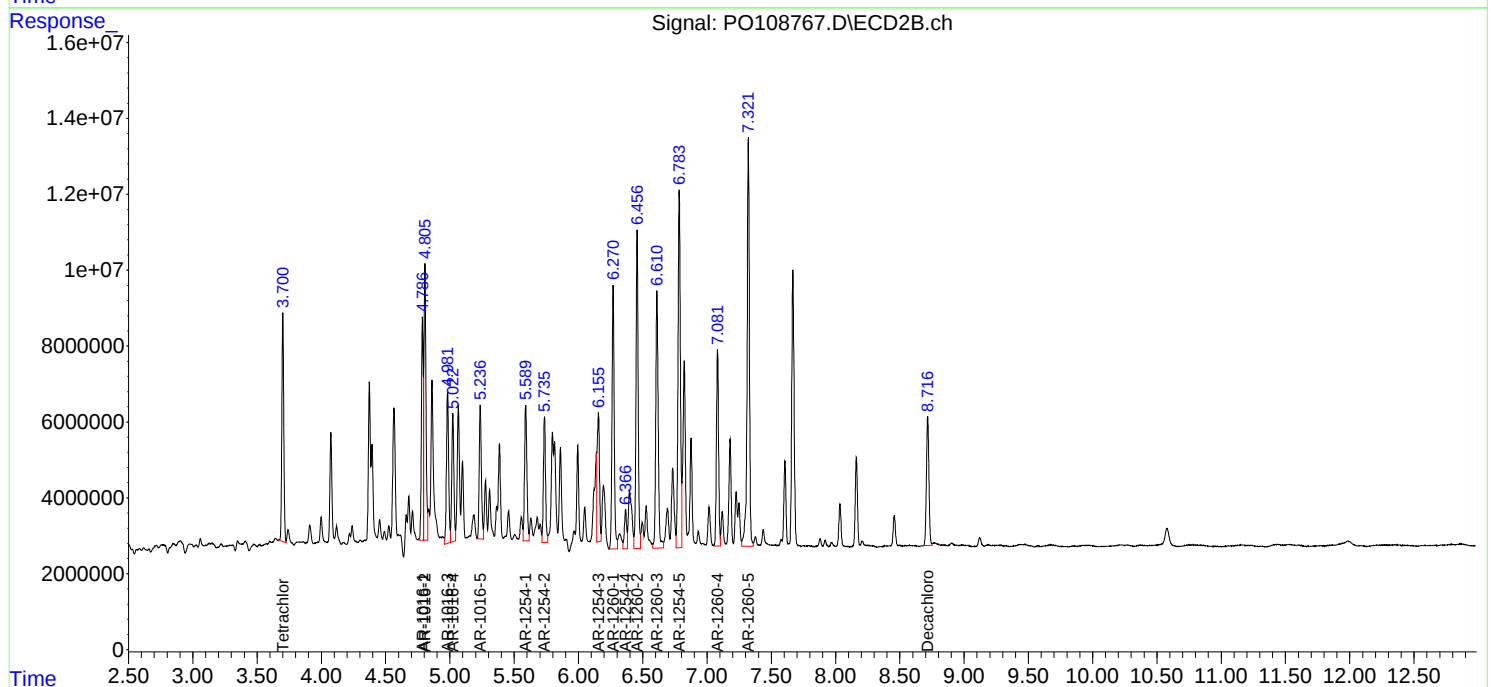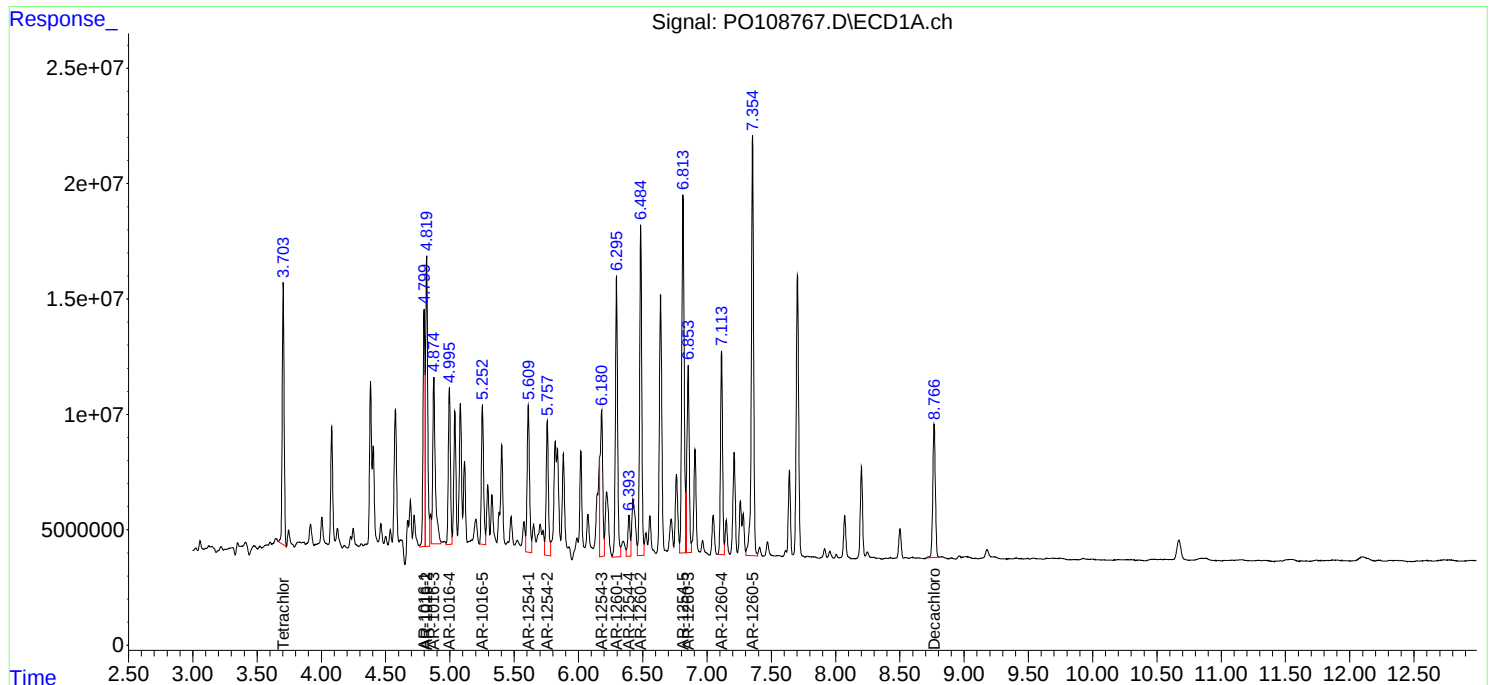

Report of Analysis

Client:	Kleinfelder	Date Collected:	12/20/24
Project:	Comegys School	Date Received:	12/20/24
Client Sample ID:	AU-06-122024MSD	SDG No.:	P5382
Lab Sample ID:	P5318-01MSD	Matrix:	SOIL
Analytical Method:	SW8082A	% Solid:	86.2
Sample Wt/Vol:	30.04	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PCB Group1
GPC Factor :	1.0	PH :	
Prep Method :	SW3541B	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PO108768.D	1	12/26/24 08:30	12/26/24 13:52	PB165843

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
12674-11-2	Aroclor-1016	134		3.90	19.7	ug/kg
11097-69-1	Aroclor-1254	76.1		3.20	19.7	ug/kg
11096-82-5	Aroclor-1260	127		3.40	19.7	ug/kg
SURROGATES						
877-09-8	Tetrachloro-m-xylene	13.9		32 - 144	70%	SPK: 20
2051-24-3	Decachlorobiphenyl	13.3		32 - 175	66%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
 Data File : PO108768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Dec 2024 13:52
 Operator : YP/AJ
 Sample : P5318-01MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :

ECD_O

ClientSampleId :

AU-06-122024MSD

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 12/27/2024

Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 26 20:25:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 07 05:58:15 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.703	3.700	121.3E6	68967710	13.944	13.605
2) SA Decachlor...	8.765	8.716	86238901	51471776	11.807	13.283
Target Compounds						
3) L1 AR-1016-1	4.798	4.785	109.7E6	54581003	355.566m	340.123m
4) L1 AR-1016-2	4.817	4.805	142.3E6	80430843	340.987m	362.150m
5) L1 AR-1016-3	4.873	4.981	104.7E6	44950074	357.771m	357.218
6) L1 AR-1016-4	4.995	5.022	79714078	37634335	344.818m	359.086
7) L1 AR-1016-5	5.253	5.236	74494284	43370701	296.000	320.763
26) L6 AR-1254-1	5.609	5.589	78456670	45901974	152.746	169.485
27) L6 AR-1254-2	5.757	5.735	66871719	39255320	146.823	163.550
28) L6 AR-1254-3	6.179	6.155	86582522	49540869	120.232m	131.929m
29) L6 AR-1254-4	6.393	6.397	20748526	27048501	47.283	124.260 #
30) L6 AR-1254-5	6.813	6.783	215.8E6	127.8E6	339.800	395.945
31) L7 AR-1260-1	6.295	6.270	143.2E6	83772123	313.266	357.946
32) L7 AR-1260-2	6.484	6.456	162.1E6	97069129	291.727	345.974
33) L7 AR-1260-3	6.853	6.610	111.8E6	89688226	241.075	340.285 #
34) L7 AR-1260-4	7.113	7.081	108.5E6	65021372	255.080	305.623m
35) L7 AR-1260-5	7.354	7.321	238.7E6	142.9E6	245.648	295.381

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO122624\
Data File : PO108768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Dec 2024 13:52
Operator : YP/AJ
Sample : P5318-01MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AU-06-122024MSD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/27/2024
Supervised By :Ankita Jodhani 12/27/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 26 20:25:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120624.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 07 05:58:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

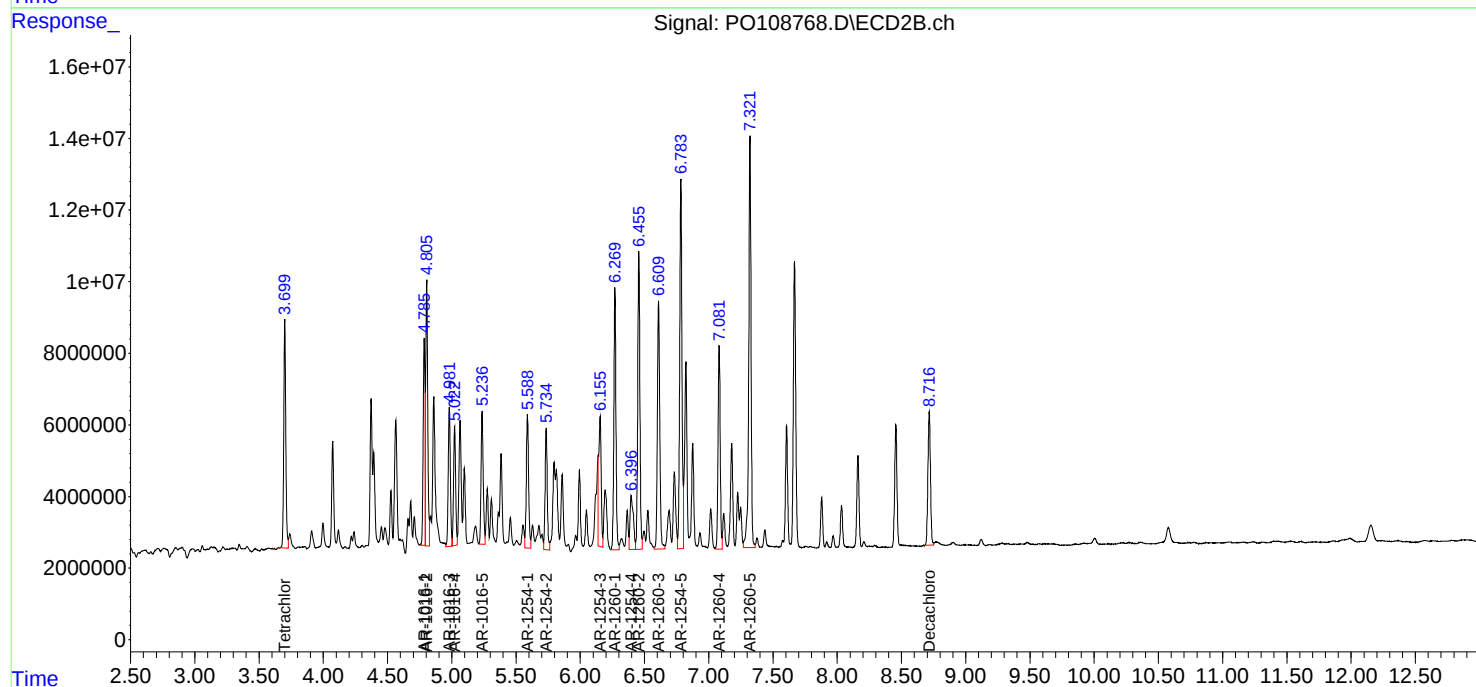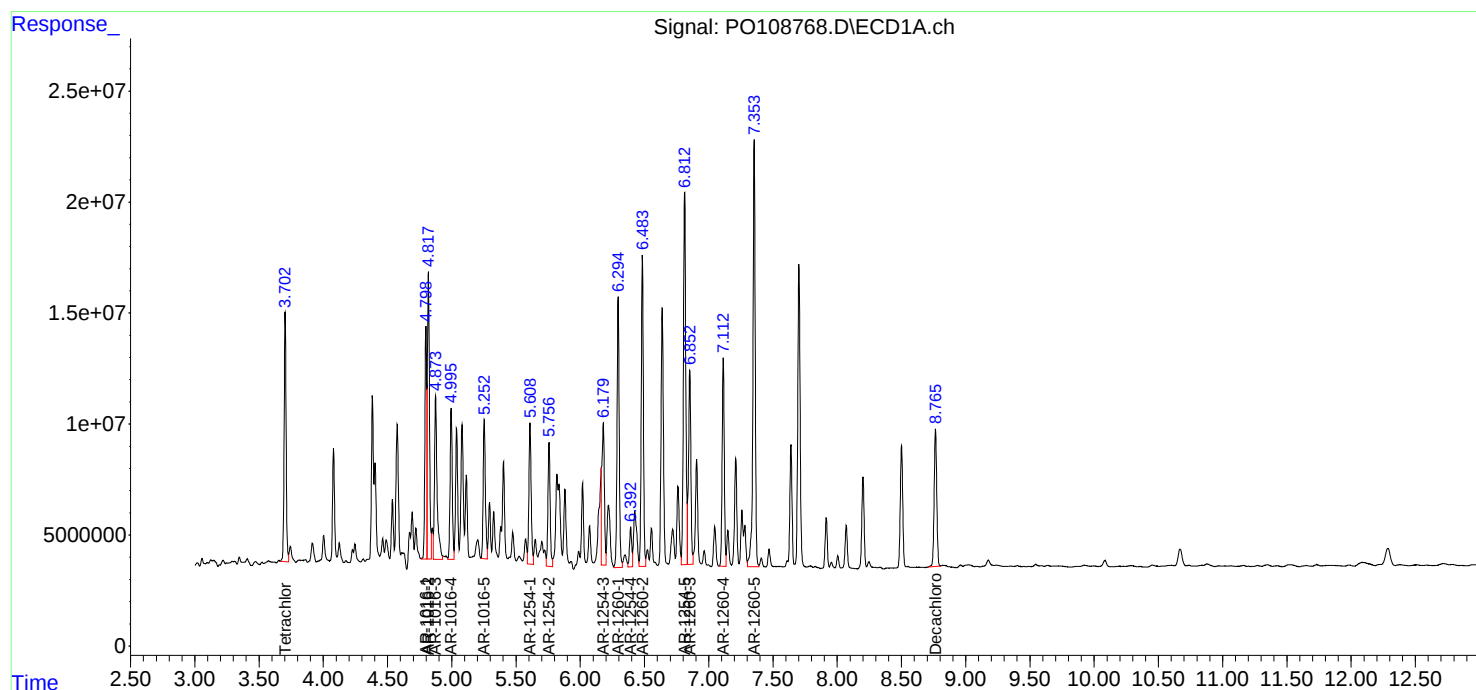

Manual Integration Report

Sequence:	PO120624	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660ICC050	PO108366.D	AR-1016-1 #2	yogesh	12/9/2024 10:59:43 AM	Ankita	12/9/2024 11:02:57	Peak Integrated by Software
AR1660ICC050	PO108366.D	AR-1016-2 #2	yogesh	12/9/2024 10:59:43 AM	Ankita	12/9/2024 11:02:57	Peak Integrated by Software
AR1660ICC050	PO108366.D	AR-1016-3 #2	yogesh	12/9/2024 10:59:43 AM	Ankita	12/9/2024 11:02:57	Peak Integrated by Software
AR1660ICC050	PO108366.D	AR-1016-4 #2	yogesh	12/9/2024 10:59:43 AM	Ankita	12/9/2024 11:02:57	Peak Integrated by Software
AR1660ICC050	PO108366.D	AR-1260-1	yogesh	12/9/2024 10:59:43 AM	Ankita	12/9/2024 11:02:57	Peak Integrated by Software
AR1660ICC050	PO108366.D	AR-1260-1 #2	yogesh	12/9/2024 10:59:43 AM	Ankita	12/9/2024 11:02:57	Peak Integrated by Software
AR1660ICC050	PO108366.D	AR-1260-2	yogesh	12/9/2024 10:59:43 AM	Ankita	12/9/2024 11:02:57	Peak Integrated by Software
AR1660ICC050	PO108366.D	AR-1260-2 #2	yogesh	12/9/2024 10:59:43 AM	Ankita	12/9/2024 11:02:57	Peak Integrated by Software
AR1660ICC050	PO108366.D	AR-1260-3	yogesh	12/9/2024 10:59:43 AM	Ankita	12/9/2024 11:02:57	Peak Integrated by Software
AR1242ICC050	PO108373.D	AR-1242-5	yogesh	12/9/2024 10:59:45 AM	Ankita	12/9/2024 11:02:58	Peak Integrated by Software
AR1248ICC050	PO108378.D	AR-1248-3	yogesh	12/9/2024 10:59:47 AM	Ankita	12/9/2024 11:02:59	Peak Integrated by Software
AR1248ICC050	PO108378.D	AR-1248-4	yogesh	12/9/2024 10:59:47 AM	Ankita	12/9/2024 11:02:59	Peak Integrated by Software
AR1248ICC050	PO108378.D	AR-1248-5	yogesh	12/9/2024 10:59:47 AM	Ankita	12/9/2024 11:02:59	Peak Integrated by Software

Manual Integration Report

Sequence:	PO120624	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1254ICC050	PO108383.D	AR-1254-1	yogesh	12/9/2024 10:59:49 AM	Ankita	12/9/2024 11:03:01	Peak Integrated by Software
AR1254ICC050	PO108383.D	AR-1254-2	yogesh	12/9/2024 10:59:49 AM	Ankita	12/9/2024 11:03:01	Peak Integrated by Software
AR1254ICC050	PO108383.D	AR-1254-3	yogesh	12/9/2024 10:59:49 AM	Ankita	12/9/2024 11:03:01	Peak Integrated by Software
AR1254ICC050	PO108383.D	AR-1254-4	yogesh	12/9/2024 10:59:49 AM	Ankita	12/9/2024 11:03:01	Peak Integrated by Software

Manual Integration Report

Sequence:	PO122624	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1660CCC500	PO108758.D	AR-1260-4 #2	yogesh	12/27/2024 7:58:23 AM	Ankita	12/27/2024 8:14:08	Peak Integrated by Software
AR1242CCC500	PO108759.D	AR-1242-2	yogesh	12/27/2024 7:58:25 AM	Ankita	12/27/2024 8:14:10	Peak Integrated by Software
AR1242CCC500	PO108759.D	AR-1242-3	yogesh	12/27/2024 7:58:25 AM	Ankita	12/27/2024 8:14:10	Peak Integrated by Software
AR1254CCC500	PO108761.D	AR-1254-3 #2	yogesh	12/27/2024 8:00:52 AM	Ankita	12/27/2024 8:14:12	Peak Integrated by Software
PB165843BS	PO108764.D	AR-1016-2	yogesh	12/27/2024 8:00:54 AM	Ankita	12/27/2024 8:14:18	Peak Integrated by Software
PB165843BS	PO108764.D	AR-1260-4 #2	yogesh	12/27/2024 8:00:54 AM	Ankita	12/27/2024 8:14:18	Peak Integrated by Software
PB165843BS	PO108764.D	Decachlorobiphenyl	yogesh	12/27/2024 8:00:54 AM	Ankita	12/27/2024 8:14:18	Peak Integrated by Software
P5318-01MS	PO108767.D	AR-1016-1	yogesh	12/27/2024 8:01:00 AM	Ankita	12/27/2024 8:14:24	Peak Integrated by Software
P5318-01MS	PO108767.D	AR-1016-1 #2	yogesh	12/27/2024 8:01:00 AM	Ankita	12/27/2024 8:14:24	Peak Integrated by Software
P5318-01MS	PO108767.D	AR-1016-2	yogesh	12/27/2024 8:01:00 AM	Ankita	12/27/2024 8:14:24	Peak Integrated by Software
P5318-01MS	PO108767.D	AR-1016-2 #2	yogesh	12/27/2024 8:01:00 AM	Ankita	12/27/2024 8:14:24	Peak Integrated by Software
P5318-01MS	PO108767.D	AR-1016-3	yogesh	12/27/2024 8:01:00 AM	Ankita	12/27/2024 8:14:24	Peak Integrated by Software
P5318-01MS	PO108767.D	AR-1016-4	yogesh	12/27/2024 8:01:00 AM	Ankita	12/27/2024 8:14:24	Peak Integrated by Software

Manual Integration Report

Sequence:	PO122624	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
P5318-01MS	PO108767.D	AR-1254-1 #2	yogesh	12/27/2024 8:01:00 AM	Ankita	12/27/2024 8:14:24	Peak Integrated by Software
P5318-01MS	PO108767.D	AR-1254-2 #2	yogesh	12/27/2024 8:01:00 AM	Ankita	12/27/2024 8:14:24	Peak Integrated by Software
P5318-01MS	PO108767.D	AR-1254-3	yogesh	12/27/2024 8:01:00 AM	Ankita	12/27/2024 8:14:24	Peak Integrated by Software
P5318-01MS	PO108767.D	AR-1254-3 #2	yogesh	12/27/2024 8:01:00 AM	Ankita	12/27/2024 8:14:24	Peak Integrated by Software
P5318-01MS	PO108767.D	AR-1260-4 #2	yogesh	12/27/2024 8:01:00 AM	Ankita	12/27/2024 8:14:24	Peak Integrated by Software
P5318-01MSD	PO108768.D	AR-1016-1	yogesh	12/27/2024 8:01:02 AM	Ankita	12/27/2024 8:14:26	Peak Integrated by Software
P5318-01MSD	PO108768.D	AR-1016-1 #2	yogesh	12/27/2024 8:01:02 AM	Ankita	12/27/2024 8:14:26	Peak Integrated by Software
P5318-01MSD	PO108768.D	AR-1016-2	yogesh	12/27/2024 8:01:02 AM	Ankita	12/27/2024 8:14:26	Peak Integrated by Software
P5318-01MSD	PO108768.D	AR-1016-2 #2	yogesh	12/27/2024 8:01:02 AM	Ankita	12/27/2024 8:14:26	Peak Integrated by Software
P5318-01MSD	PO108768.D	AR-1016-3	yogesh	12/27/2024 8:01:02 AM	Ankita	12/27/2024 8:14:26	Peak Integrated by Software
P5318-01MSD	PO108768.D	AR-1016-4	yogesh	12/27/2024 8:01:02 AM	Ankita	12/27/2024 8:14:26	Peak Integrated by Software
P5318-01MSD	PO108768.D	AR-1254-3	yogesh	12/27/2024 8:01:02 AM	Ankita	12/27/2024 8:14:26	Peak Integrated by Software
P5318-01MSD	PO108768.D	AR-1254-3 #2	yogesh	12/27/2024 8:01:02 AM	Ankita	12/27/2024 8:14:26	Peak Integrated by Software

Manual Integration Report

Sequence:	PO122624	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
P5318-01MSD	PO108768.D	AR-1260-4 #2	yogesh	12/27/2024 8:01:02 AM	Ankita	12/27/2024 8:14:26	Peak Integrated by Software
P5382-01	PO108770.D	Decachlorobiphenyl #2	yogesh	12/27/2024 8:01:05 AM	Ankita	12/27/2024 8:14:30	Peak Integrated by Software
P5382-02	PO108771.D	Decachlorobiphenyl #2	yogesh	12/27/2024 8:01:06 AM	Ankita	12/27/2024 8:14:31	Peak Integrated by Software
P5382-03	PO108772.D	Decachlorobiphenyl #2	yogesh	12/27/2024 8:01:08 AM	Ankita	12/27/2024 8:14:33	Peak Integrated by Software
AR1660CCC50 0	PO108773.D	AR-1016-1	yogesh	12/27/2024 8:01:10 AM	Ankita	12/27/2024 8:14:35	Peak Integrated by Software
AR1660CCC50 0	PO108773.D	AR-1016-1 #2	yogesh	12/27/2024 8:01:10 AM	Ankita	12/27/2024 8:14:35	Peak Integrated by Software
AR1660CCC50 0	PO108773.D	AR-1016-3	yogesh	12/27/2024 8:01:10 AM	Ankita	12/27/2024 8:14:35	Peak Integrated by Software
AR1242CCC50 0	PO108774.D	AR-1242-1	yogesh	12/27/2024 10:18:03 AM	Ankita	12/27/2024 10:18:33	Peak Integrated by Software
AR1242CCC50 0	PO108774.D	AR-1242-1 #2	yogesh	12/27/2024 10:18:03 AM	Ankita	12/27/2024 10:18:33	Peak Integrated by Software
AR1242CCC50 0	PO108774.D	AR-1242-2	yogesh	12/27/2024 10:18:03 AM	Ankita	12/27/2024 10:18:33	Peak Integrated by Software
AR1242CCC50 0	PO108774.D	AR-1242-2 #2	yogesh	12/27/2024 10:18:03 AM	Ankita	12/27/2024 10:18:33	Peak Integrated by Software
AR1242CCC50 0	PO108774.D	AR-1242-3	yogesh	12/27/2024 10:18:03 AM	Ankita	12/27/2024 10:18:33	Peak Integrated by Software
AR1242CCC50 0	PO108774.D	AR-1242-4	yogesh	12/27/2024 10:18:03 AM	Ankita	12/27/2024 10:18:33	Peak Integrated by Software

Manual Integration Report

Sequence:	PO122624	Instrument	ECD_o
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
AR1248CCC500	PO108775.D	AR-1248-1 #2	yogesh	12/27/2024 8:01:13 AM	Ankita	12/27/2024 8:14:38	Peak Integrated by Software
AR1254CCC500	PO108776.D	AR-1254-3 #2	yogesh	12/27/2024 8:01:14 AM	Ankita	12/27/2024 8:14:40	Peak Integrated by Software
AR1254CCC500	PO108776.D	AR-1254-5	yogesh	12/27/2024 8:01:14 AM	Ankita	12/27/2024 8:14:40	Peak Integrated by Software
AR1660CCC500	PO108782.D	AR-1016-1	yogesh	12/27/2024 8:01:19 AM	Ankita	12/27/2024 8:14:48	Peak Integrated by Software
AR1660CCC500	PO108782.D	AR-1016-1 #2	yogesh	12/27/2024 8:01:19 AM	Ankita	12/27/2024 8:14:48	Peak Integrated by Software
AR1660CCC500	PO108782.D	AR-1260-4 #2	yogesh	12/27/2024 8:01:19 AM	Ankita	12/27/2024 8:14:48	Peak Integrated by Software
AR1242CCC500	PO108783.D	AR-1242-1	yogesh	12/27/2024 8:01:21 AM	Ankita	12/27/2024 8:14:50	Peak Integrated by Software
AR1242CCC500	PO108783.D	AR-1242-1 #2	yogesh	12/27/2024 8:01:21 AM	Ankita	12/27/2024 8:14:50	Peak Integrated by Software
AR1242CCC500	PO108783.D	AR-1242-2 #2	yogesh	12/27/2024 8:01:21 AM	Ankita	12/27/2024 8:14:50	Peak Integrated by Software
AR1242CCC500	PO108783.D	AR-1242-3	yogesh	12/27/2024 8:01:21 AM	Ankita	12/27/2024 8:14:50	Peak Integrated by Software
AR1248CCC500	PO108784.D	AR-1248-1 #2	yogesh	12/27/2024 8:01:23 AM	Ankita	12/27/2024 8:14:52	Peak Integrated by Software
AR1254CCC500	PO108785.D	AR-1254-3 #2	yogesh	12/27/2024 8:01:25 AM	Ankita	12/27/2024 8:14:54	Peak Integrated by Software
AR1254CCC500	PO108785.D	AR-1254-5	yogesh	12/27/2024 8:01:25 AM	Ankita	12/27/2024 8:14:54	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:

PO122624

Instrument

ECD_o

Sample ID

File ID

Parameter

Review By

Review On

Supervised
By

Supervised On

Reason

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO120624

Review By	yogesh	Review On	12/9/2024 11:00:19 AM
Supervise By	Ankita	Supervise On	12/9/2024 11:03:08 AM
SubDirectory	PO120624	HP Acquire Method	HP Processing Method PO120624
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO108360.D	06 Dec 2024 13:43	YP/AJ	Ok
2	I.BLK	PO108361.D	06 Dec 2024 14:01	YP/AJ	Ok
3	AR1660ICC1000	PO108362.D	06 Dec 2024 14:19	YP/AJ	Ok
4	AR1660ICC750	PO108363.D	06 Dec 2024 14:38	YP/AJ	Ok
5	AR1660ICC500	PO108364.D	06 Dec 2024 14:56	YP/AJ	Ok
6	AR1660ICC250	PO108365.D	06 Dec 2024 15:14	YP/AJ	Ok
7	AR1660ICC050	PO108366.D	06 Dec 2024 15:33	YP/AJ	Ok,M
8	AR1221ICC500	PO108367.D	06 Dec 2024 15:51	YP/AJ	Ok
9	AR1232ICC500	PO108368.D	06 Dec 2024 16:09	YP/AJ	Ok
10	AR1242ICC1000	PO108369.D	06 Dec 2024 16:28	YP/AJ	Ok
11	AR1242ICC750	PO108370.D	06 Dec 2024 16:46	YP/AJ	Ok
12	AR1242ICC500	PO108371.D	06 Dec 2024 17:04	YP/AJ	Ok
13	AR1242ICC250	PO108372.D	06 Dec 2024 17:23	YP/AJ	Ok
14	AR1242ICC050	PO108373.D	06 Dec 2024 17:41	YP/AJ	Ok,M
15	AR1248ICC1000	PO108374.D	06 Dec 2024 17:59	YP/AJ	Ok
16	AR1248ICC750	PO108375.D	06 Dec 2024 18:18	YP/AJ	Ok
17	AR1248ICC500	PO108376.D	06 Dec 2024 18:36	YP/AJ	Ok
18	AR1248ICC250	PO108377.D	06 Dec 2024 18:54	YP/AJ	Ok
19	AR1248ICC050	PO108378.D	06 Dec 2024 19:13	YP/AJ	Ok,M
20	AR1254ICC1000	PO108379.D	06 Dec 2024 19:31	YP/AJ	Ok
21	AR1254ICC750	PO108380.D	06 Dec 2024 19:49	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO120624

Review By	yogesh	Review On	12/9/2024 11:00:19 AM
Supervise By	Ankita	Supervise On	12/9/2024 11:03:08 AM
SubDirectory	PO120624	HP Acquire Method	HP Processing Method PO120624
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	AR1254ICC500	PO108381.D	06 Dec 2024 20:08	YP/AJ	Ok
23	AR1254ICC250	PO108382.D	06 Dec 2024 20:26	YP/AJ	Ok
24	AR1254ICC050	PO108383.D	06 Dec 2024 20:44	YP/AJ	Ok,M
25	AR1262ICC500	PO108384.D	06 Dec 2024 21:03	YP/AJ	Ok
26	AR1268ICC1000	PO108385.D	06 Dec 2024 21:21	YP/AJ	Ok
27	AR1268ICC750	PO108386.D	06 Dec 2024 21:39	YP/AJ	Ok
28	AR1268ICC500	PO108387.D	06 Dec 2024 21:58	YP/AJ	Ok
29	AR1268ICC250	PO108388.D	06 Dec 2024 22:16	YP/AJ	Ok
30	AR1268ICC050	PO108389.D	06 Dec 2024 22:34	YP/AJ	Ok
31	PO120624ICV500	PO108390.D	06 Dec 2024 22:53	YP/AJ	Ok
32	AR1242ICV500	PO108391.D	06 Dec 2024 23:11	YP/AJ	Ok
33	AR1248ICV500	PO108392.D	06 Dec 2024 23:29	YP/AJ	Ok
34	AR1254ICV500	PO108393.D	06 Dec 2024 23:48	YP/AJ	Ok
35	AR1268ICV500	PO108394.D	07 Dec 2024 00:06	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO122624

Review By	yogesh	Review On	12/26/2024 11:43:31 AM
Supervise By	Ankita	Supervise On	12/27/2024 8:15:18 AM
SubDirectory	PO122624	HP Acquire Method	HP Processing Method PO120624
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PO108757.D	26 Dec 2024 09:13	YP/AJ	Ok
2	AR1660CCC500	PO108758.D	26 Dec 2024 09:31	YP/AJ	Ok,M
3	AR1242CCC500	PO108759.D	26 Dec 2024 09:49	YP/AJ	Ok,M
4	AR1248CCC500	PO108760.D	26 Dec 2024 10:08	YP/AJ	Ok
5	AR1254CCC500	PO108761.D	26 Dec 2024 10:26	YP/AJ	Ok,M
6	I.BLK	PO108762.D	26 Dec 2024 11:32	YP/AJ	Ok
7	PB165843BL	PO108763.D	26 Dec 2024 12:21	YP/AJ	Ok
8	PB165843BS	PO108764.D	26 Dec 2024 12:39	YP/AJ	Ok,M
9	P5383-01	PO108765.D	26 Dec 2024 12:57	YP/AJ	Ok,M
10	P5318-01	PO108766.D	26 Dec 2024 13:15	YP/AJ	Ok,M
11	P5318-01MS	PO108767.D	26 Dec 2024 13:34	YP/AJ	Ok,M
12	P5318-01MSD	PO108768.D	26 Dec 2024 13:52	YP/AJ	Ok,M
13	P5380-01	PO108769.D	26 Dec 2024 14:10	YP/AJ	Ok,M
14	P5382-01	PO108770.D	26 Dec 2024 14:29	YP/AJ	Ok,M
15	P5382-02	PO108771.D	26 Dec 2024 14:47	YP/AJ	Ok,M
16	P5382-03	PO108772.D	26 Dec 2024 15:05	YP/AJ	Ok,M
17	AR1660CCC500	PO108773.D	26 Dec 2024 16:10	YP/AJ	Ok,M
18	AR1242CCC500	PO108774.D	26 Dec 2024 16:29	YP/AJ	Ok,M
19	AR1248CCC500	PO108775.D	26 Dec 2024 16:47	YP/AJ	Ok,M
20	AR1254CCC500	PO108776.D	26 Dec 2024 17:05	YP/AJ	Ok,M
21	I.BLK	PO108777.D	26 Dec 2024 17:24	YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO122624

Review By	yogesh	Review On	12/26/2024 11:43:31 AM
Supervise By	Ankita	Supervise On	12/27/2024 8:15:18 AM
SubDirectory	PO122624	HP Acquire Method	HP Processing Method PO120624
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	PB165855BL	PO108778.D	26 Dec 2024 17:42	YP/AJ	Ok
23	PB165855BS	PO108779.D	26 Dec 2024 18:00	YP/AJ	Ok,M
24	PB165855BSD	PO108780.D	26 Dec 2024 18:18	YP/AJ	Ok,M
25	P5377-02	PO108781.D	26 Dec 2024 18:37	YP/AJ	ReRun
26	AR1660CCC500	PO108782.D	26 Dec 2024 19:56	YP/AJ	Ok,M
27	AR1242CCC500	PO108783.D	26 Dec 2024 20:14	YP/AJ	Ok,M
28	AR1248CCC500	PO108784.D	26 Dec 2024 20:32	YP/AJ	Ok,M
29	AR1254CCC500	PO108785.D	26 Dec 2024 20:51	YP/AJ	Ok,M
30	I.BLK	PO108786.D	26 Dec 2024 21:09	YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO120624

Review By	yogesh	Review On	12/9/2024 11:00:19 AM
Supervise By	Ankita	Supervise On	12/9/2024 11:03:08 AM
SubDirectory	PO120624	HP Acquire Method	HP Processing Method PO120624

STD. NAME	STD REF.#
Tune/Reschk	
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773
Internal Standard/PEM	
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO108360.D	06 Dec 2024 13:43		YP/AJ	Ok
2	I.BLK	I.BLK	PO108361.D	06 Dec 2024 14:01		YP/AJ	Ok
3	AR1660ICC1000	AR1660ICC1000	PO108362.D	06 Dec 2024 14:19		YP/AJ	Ok
4	AR1660ICC750	AR1660ICC750	PO108363.D	06 Dec 2024 14:38		YP/AJ	Ok
5	AR1660ICC500	AR1660ICC500	PO108364.D	06 Dec 2024 14:56		YP/AJ	Ok
6	AR1660ICC250	AR1660ICC250	PO108365.D	06 Dec 2024 15:14		YP/AJ	Ok
7	AR1660ICC050	AR1660ICC050	PO108366.D	06 Dec 2024 15:33		YP/AJ	Ok,M
8	AR1221ICC500	AR1221ICC500	PO108367.D	06 Dec 2024 15:51		YP/AJ	Ok
9	AR1232ICC500	AR1232ICC500	PO108368.D	06 Dec 2024 16:09		YP/AJ	Ok
10	AR1242ICC1000	AR1242ICC1000	PO108369.D	06 Dec 2024 16:28		YP/AJ	Ok
11	AR1242ICC750	AR1242ICC750	PO108370.D	06 Dec 2024 16:46		YP/AJ	Ok
12	AR1242ICC500	AR1242ICC500	PO108371.D	06 Dec 2024 17:04		YP/AJ	Ok
13	AR1242ICC250	AR1242ICC250	PO108372.D	06 Dec 2024 17:23		YP/AJ	Ok
14	AR1242ICC050	AR1242ICC050	PO108373.D	06 Dec 2024 17:41		YP/AJ	Ok,M
15	AR1248ICC1000	AR1248ICC1000	PO108374.D	06 Dec 2024 17:59		YP/AJ	Ok
16	AR1248ICC750	AR1248ICC750	PO108375.D	06 Dec 2024 18:18		YP/AJ	Ok
17	AR1248ICC500	AR1248ICC500	PO108376.D	06 Dec 2024 18:36		YP/AJ	Ok
18	AR1248ICC250	AR1248ICC250	PO108377.D	06 Dec 2024 18:54		YP/AJ	Ok

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO120624

Review By	yogesh	Review On	12/9/2024 11:00:19 AM
Supervise By	Ankita	Supervise On	12/9/2024 11:03:08 AM
SubDirectory	PO120624	HP Acquire Method	HP Processing Method PO120624
STD. NAME	STD REF.#		
Tune/Reschk	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775 PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773 PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Initial Calibration Stds			
CCC			
Internal Standard/PEM			
ICV/I.BLK			
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248ICC050	AR1248ICC050	PO108378.D	06 Dec 2024 19:13		YP/AJ	Ok,M
20	AR1254ICC1000	AR1254ICC1000	PO108379.D	06 Dec 2024 19:31		YP/AJ	Ok
21	AR1254ICC750	AR1254ICC750	PO108380.D	06 Dec 2024 19:49		YP/AJ	Ok
22	AR1254ICC500	AR1254ICC500	PO108381.D	06 Dec 2024 20:08		YP/AJ	Ok
23	AR1254ICC250	AR1254ICC250	PO108382.D	06 Dec 2024 20:26		YP/AJ	Ok
24	AR1254ICC050	AR1254ICC050	PO108383.D	06 Dec 2024 20:44		YP/AJ	Ok,M
25	AR1262ICC500	AR1262ICC500	PO108384.D	06 Dec 2024 21:03		YP/AJ	Ok
26	AR1268ICC1000	AR1268ICC1000	PO108385.D	06 Dec 2024 21:21		YP/AJ	Ok
27	AR1268ICC750	AR1268ICC750	PO108386.D	06 Dec 2024 21:39		YP/AJ	Ok
28	AR1268ICC500	AR1268ICC500	PO108387.D	06 Dec 2024 21:58		YP/AJ	Ok
29	AR1268ICC250	AR1268ICC250	PO108388.D	06 Dec 2024 22:16		YP/AJ	Ok
30	AR1268ICC050	AR1268ICC050	PO108389.D	06 Dec 2024 22:34		YP/AJ	Ok
31	PO120624ICV500	ICVPO120624	PO108390.D	06 Dec 2024 22:53		YP/AJ	Ok
32	AR1242ICV500	ICVPO120624AR1242	PO108391.D	06 Dec 2024 23:11		YP/AJ	Ok
33	AR1248ICV500	ICVPO120624AR1248	PO108392.D	06 Dec 2024 23:29		YP/AJ	Ok
34	AR1254ICV500	ICVPO120624AR1254	PO108393.D	06 Dec 2024 23:48		YP/AJ	Ok
35	AR1268ICV500	ICVPO120624AR1268	PO108394.D	07 Dec 2024 00:06		YP/AJ	Ok

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO122624

Review By	yogesh	Review On	12/26/2024 11:43:31 AM
Supervise By	Ankita	Supervise On	12/27/2024 8:15:18 AM
SubDirectory	PO122624	HP Acquire Method	HP Processing Method PO120624
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PO108757.D	26 Dec 2024 09:13		YP/AJ	Ok
2	AR1660CCC500	AR1660CCC500	PO108758.D	26 Dec 2024 09:31		YP/AJ	Ok,M
3	AR1242CCC500	AR1242CCC500	PO108759.D	26 Dec 2024 09:49		YP/AJ	Ok,M
4	AR1248CCC500	AR1248CCC500	PO108760.D	26 Dec 2024 10:08		YP/AJ	Ok
5	AR1254CCC500	AR1254CCC500	PO108761.D	26 Dec 2024 10:26		YP/AJ	Ok,M
6	I.BLK	I.BLK	PO108762.D	26 Dec 2024 11:32		YP/AJ	Ok
7	PB165843BL	PB165843BL	PO108763.D	26 Dec 2024 12:21		YP/AJ	Ok
8	PB165843BS	PB165843BS	PO108764.D	26 Dec 2024 12:39		YP/AJ	Ok,M
9	P5383-01	OK-02-12232024	PO108765.D	26 Dec 2024 12:57		YP/AJ	Ok,M
10	P5318-01	AU-06-122024	PO108766.D	26 Dec 2024 13:15	AR1254 + AR1260 Hit	YP/AJ	Ok,M
11	P5318-01MS	AU-06-122024MS	PO108767.D	26 Dec 2024 13:34		YP/AJ	Ok,M
12	P5318-01MSD	AU-06-122024MSD	PO108768.D	26 Dec 2024 13:52		YP/AJ	Ok,M
13	P5380-01	TAPIAL3-IDW-SOIL-12	PO108769.D	26 Dec 2024 14:10		YP/AJ	Ok,M
14	P5382-01	COMP-1	PO108770.D	26 Dec 2024 14:29		YP/AJ	Ok,M
15	P5382-02	COMP-2	PO108771.D	26 Dec 2024 14:47		YP/AJ	Ok,M
16	P5382-03	COMP-3	PO108772.D	26 Dec 2024 15:05		YP/AJ	Ok,M
17	AR1660CCC500	AR1660CCC500	PO108773.D	26 Dec 2024 16:10		YP/AJ	Ok,M
18	AR1242CCC500	AR1242CCC500	PO108774.D	26 Dec 2024 16:29		YP/AJ	Ok,M

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QC Batch ID # PO122624

Review By	yogesh	Review On	12/26/2024 11:43:31 AM
Supervise By	Ankita	Supervise On	12/27/2024 8:15:18 AM
SubDirectory	PO122624	HP Acquire Method	HP Processing Method PO120624
STD. NAME	STD REF.#		
Tune/Reschk			
Initial Calibration Stds	PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,P P23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP 23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775		
CCC	PP23737,PP23742,PP23749,PP23754,PP23758,PP23763,PP23768,PP23773		
Internal Standard/PEM			
ICV/I.BLK	PP23778,PP23780,PP23783,PP23784,PP23786,PP23788,PP23790,PP23947		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	AR1248CCC500	AR1248CCC500	PO108775.D	26 Dec 2024 16:47		YP/AJ	Ok,M
20	AR1254CCC500	AR1254CCC500	PO108776.D	26 Dec 2024 17:05		YP/AJ	Ok,M
21	I.BLK	I.BLK	PO108777.D	26 Dec 2024 17:24		YP/AJ	Ok
22	PB165855BL	PB165855BL	PO108778.D	26 Dec 2024 17:42		YP/AJ	Ok
23	PB165855BS	PB165855BS	PO108779.D	26 Dec 2024 18:00		YP/AJ	Ok,M
24	PB165855BSD	PB165855BSD	PO108780.D	26 Dec 2024 18:18		YP/AJ	Ok,M
25	P5377-02	GAS-TRE-1114	PO108781.D	26 Dec 2024 18:37	DCB and TCMX low in both column	YP/AJ	ReRun
26	AR1660CCC500	AR1660CCC500	PO108782.D	26 Dec 2024 19:56		YP/AJ	Ok,M
27	AR1242CCC500	AR1242CCC500	PO108783.D	26 Dec 2024 20:14		YP/AJ	Ok,M
28	AR1248CCC500	AR1248CCC500	PO108784.D	26 Dec 2024 20:32		YP/AJ	Ok,M
29	AR1254CCC500	AR1254CCC500	PO108785.D	26 Dec 2024 20:51		YP/AJ	Ok,M
30	I.BLK	I.BLK	PO108786.D	26 Dec 2024 21:09		YP/AJ	Ok

M : Manual Integration



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 12/27/2024

OVENTEMP IN Celsius(°C): 106
Time IN: 17:15
In Date: 12/26/2024
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 103
Time OUT: 08:15
Out Date: 12/27/2024
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID- OVEN

QC:LB134080

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
P5380-01	TAPIAL3-IDW-SOIL-122024-T1	1	1.15	8.48	9.63	8.47	86.3	
P5382-01	COMP-1	2	1.19	8.60	9.79	8.31	82.8	
P5382-02	COMP-2	3	1.15	8.82	9.97	8.43	82.5	
P5382-03	COMP-3	4	1.16	8.76	9.92	8.41	82.8	
P5382-04	SB-1	5	1.15	8.80	9.95	8.47	83.2	
P5382-05	SB-2	6	1.18	8.75	9.93	8.4	82.5	
P5382-06	SB-3	7	1.17	8.80	9.97	8.27	80.7	
P5382-07	SB-4	8	1.19	8.53	9.72	8.02	80.1	
P5382-08	SB-5	9	1.15	8.80	9.95	8.73	86.1	
P5382-09	SB-6	10	1.19	8.50	9.69	7.75	77.2	
P5382-10	SB-7	11	1.14	8.69	9.83	7.86	77.3	
P5382-11	SB-8	12	1.13	8.82	9.95	8.55	84.1	
P5382-12	SB-9	13	1.11	8.73	9.84	8.29	82.2	
P5382-13	SB-10	14	1.19	8.78	9.97	8.16	79.4	
P5382-14	SB-11	15	1.19	8.40	9.59	7.98	80.8	
P5382-15	SB-12	16	1.19	8.51	9.7	8.28	83.3	
P5383-01	OK-02-12232024	17	1.15	8.82	9.97	9.3	92.4	
P5383-02	OK-02-12232024-E2	18	1.13	8.81	9.94	9.54	95.5	
P5384-01	ORA-2066	19	1.00	1.00	2.00	2.00	100.0	wipe sample
P5384-02	ORA-2067	20	1.00	1.00	2.00	2.00	100.0	wipe sample
P5386-01	MOO-24-00398	21	1.15	8.44	9.59	8.99	92.9	
P5386-03	MOO-24-00395-96	22	1.00	1.00	2.00	2.00	100.0	debris
P5387-01	TR-05-122624	23	1.13	8.66	9.79	8.86	89.3	
P5387-02	TR-05-122624-E2	24	1.14	8.80	9.94	8.91	88.3	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

JB 134020

WorkList Name : %1-122624

WorkList ID : 186590

Department : Wet-Chemistry

Date : 12-26-2024 07:48:31

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P5380-01	TAPIAL3-IDW-SOIL-122024-T1	Solid	Percent Solids	Cool 4 deg C	WEST04	N31	12/20/2024	Chemtech -SO
P5382-01	COMP-1	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-02	COMP-2	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-03	COMP-3	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-04	SB-1	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-05	SB-2	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-06	SB-3	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-07	SB-4	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-08	SB-5	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-09	SB-6	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-10	SB-7	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-11	SB-8	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-12	SB-9	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-13	SB-10	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-14	SB-11	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5382-15	SB-12	Solid	Percent Solids	Cool 4 deg C	POWE02	N31	12/20/2024	Chemtech -SO
P5383-01	OK-02-12232024	Solid	Percent Solids	Cool 4 deg C	PSEG05	K31	12/23/2024	Chemtech -SO
P5383-02	OK-02-12232024-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	K31	12/23/2024	Chemtech -SO
P5384-01	ORA-2066	Solid	Percent Solids	Cool 4 deg C	PSEG03	N31	12/26/2024	Chemtech -SO
P5384-02	ORA-2067	Solid	Percent Solids	Cool 4 deg C	PSEG03	N31	12/26/2024	Chemtech -SO
P5386-01	MOO-24-00398	Solid	Percent Solids	Cool 4 deg C	PSEG03	N31	12/26/2024	Chemtech -SO

Date/Time 12/26/24 16:00
 Raw Sample Received by: JB WWC
 Raw Sample Relinquished by: JB WWC

WORKLIST(Hardcopy Internal Chain)

JB 134080

WorkList Name : %1-122624 WorkList ID : 186590 Department : Wet-Chemistry Date : 12-26-2024 07:48:31

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P5386-03	MOO-24-00395-96	Solid	Percent Solids	Cool 4 deg C	PSEG03	N31	12/26/2024	Chemtech -SO
P5387-01	TR-05-122624	Solid	Percent Solids	Cool 4 deg C	PSEG05	N41	12/26/2024	Chemtech -SO
P5387-02	TR-05-122624-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	N41	12/26/2024	Chemtech -SO

Date/Time 12/26/24
 Raw Sample Received by: JB WEL
 Raw Sample Relinquished by: JB WEL

Date/Time 12/26/24
 Raw Sample Received by: JB WEL
 Raw Sample Relinquished by: JB WEL

SOP ID: M3541-ASE Extraction-14

Clean Up SOP #: Acid Cleanup

Matrix : Solid

Weigh By: RJ

Balance check: RJ

Balance ID: EX-SC-2

pH Strip Lot#: N/A

Extraction By: RJ

Filter By: RJ

pH Meter ID: N/A

Hood ID: 3,7

Extraction Start Date : 12/26/2024

Extraction Start Time : 08:30

Extraction End Date : 12/26/2024

Extraction End Time : 11:30

Concentration By: EH

Supervisor By : rajesh

Extraction Method: ☐ Separatory Funnel ☐ Continuous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☒ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP23913
Surrogate	1.0ML	200 PPB	PP23985
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Hexane/Acetone/1:1	N/A	EP2561
Baked Na2SO4	N/A	EP2573
Sand	N/A	E2865
Hexane	N/A	E3847
H2SO4 1:1	N/A	EP2565
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40 ML Vial lot# 03-40 BTS721.

KD Bath ID: N/A

KD Bath Temperature: N/A

Envap ID: NEVAP-02

Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
12/26/24	RP (Ext. Lab)	Y.P. Pestil/42
11:35	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-14

Concentration Date: 12/26/2024

Sample ID	Client Sample ID	Test	g/mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB165843BL	ABLK843	PCB	30.02	N/A	ritesh	Evelyn	10			U7-1
PB165843BS	ALCS843	PCB	30.01	N/A	ritesh	Evelyn	10			2
P5318-01	AU-06-122024	PCB	30.05	N/A	ritesh	Evelyn	10	E		3
P5318-01MS	AU-06-122024MS	PCB	30.02	N/A	ritesh	Evelyn	10	E		4
P5318-01MS	AU-06-122024MSD	PCB	30.04	N/A	ritesh	Evelyn	10	E		5
P5380-01	TAPIAL3-IDW-SOIL-1220 24-T1	PCB	30.06	N/A	ritesh	Evelyn	10	B		6
P5382-01	COMP-1	PCB Group1	30.08	N/A	ritesh	Evelyn	10	D		U6-1
P5382-02	COMP-2	PCB Group1	30.03	N/A	ritesh	Evelyn	10	D		2
P5382-03	COMP-3	PCB Group1	30.01	N/A	ritesh	Evelyn	10	D		3
P5383-01	OK-02-12232024	PCB	30.05	N/A	ritesh	Evelyn	10	E		4

* Extracts relinquished on the same date as received.



WORKLIST(Hardcopy Internal Chain)

WorkList Name : p5318pcb WorkList ID : 186610 Department : Extraction Date : 12-26-2024 08:26:46

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
P5318-01	AU-06-122024	Solid	PCB	Cool 4 deg C	PSEG05	N31	12/20/2024	8082A
P5380-01	TAPIAL3-IDW-SOIL-122024-T1	Solid	PCB	Cool 4 deg C	WEST04	N31	12/20/2024	8082A
P5382-01	COMP-1	Solid	PCB Group1	Cool 4 deg C	POWE02	N31	12/20/2024	8082A
P5382-02	COMP-2	Solid	PCB Group1	Cool 4 deg C	POWE02	N31	12/20/2024	8082A
P5382-03	COMP-3	Solid	PCB Group1	Cool 4 deg C	POWE02	N31	12/20/2024	8082A
P5383-01	OK-02-12232024	Solid	PCB	Cool 4 deg C	PSEG05	K31	12/23/2024	8082A

Date/Time 12/26/24 8:28
Raw Sample Received by: RY (Set Lab)
Raw Sample Relinquished by: JD (SM)

Date/Time 12/26/24 9:00
Raw Sample Received by: JD (SM)
Raw Sample Relinquished by: RY (Set Lab)

Prep Standard - Chemical Standard Summary

Order ID : P5382

Test : PCB Group1

Prepbatch ID : PB165843,

Sequence ID/Qc Batch ID: PO122624,

Standard ID :

EP2561,EP2565,EP2573,PP23733,PP23735,PP23736,PP23737,PP23738,PP23739,PP23740,PP23741,PP23742,PP23743,PP23744,PP23745,PP23747,PP23748,PP23749,PP23750,PP23751,PP23752,PP23753,PP23754,PP23755,PP23756,PP23757,PP23758,PP23759,PP23760,PP23761,PP23762,PP23763,PP23764,PP23765,PP23766,PP23767,PP23768,PP23769,PP23770,PP23771,PP23772,PP23773,PP23774,PP23775,PP23776,PP23777,PP23778,PP23779,PP23780,PP23781,PP23782,PP23783,PP23784,PP23785,PP23786,PP23787,PP23788,PP23789,PP23790,PP23913,PP23946,PP23947,PP23985,

Chemical ID :

E2865,E3551,E3804,E3805,E3822,E3825,E3826,E3827,E3847,M5173,P10483,P10500,P11507,P11512,P11521,P11581,P11587,P11590,P11597,P12698,P12929,P12934,P12947,P12957,P13033,P13104,P13109,P13350,P13352,P13372,W3112,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	EP2561	11/14/2024	05/08/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 11/14/2024

FROM 8000.00000ml of E3826 + 8000.00000ml of E3827 = Final Quantity: 8000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
314	1.1 H2SO4 SOLN	EP2565	11/20/2024	05/20/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 11/20/2024

FROM 1000.00000ml of M5173 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2573	12/16/2024	06/16/2025	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	RUPESHKUMAR SHAH 12/16/2024
<u>FROM</u> 4000.00000gram of E3551 = Final Quantity: 4000.000 gram								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP23733	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel 10/03/2024
<u>FROM</u> 1.00000ml of P13350 + 9.00000ml of E3805 = Final Quantity: 10.000 ml								

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
202	AR1660 1000/100 ppb working solution 1st source	PP23735	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P10483 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
203	AR1660 750 PPB STD	PP23736	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23735 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
204	AR1660 500 PPB STD	PP23737	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23735 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
205	AR1660 250 PPB STD	PP23738	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23735 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
206	AR1660 50 PPB STD	PP23739	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23737 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
213	AR1221 1000 PPB WORKING SOLUTION	PP23740	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11581 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1079	AR1221 750 PPB STD	PP23741	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23740 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
222	AR1221 500 PPB STD	PP23742	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23740 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1080	AR1221 250 PPB STD	PP23743	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23740 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1081	AR1221 50 PPB STD	PP23744	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23742 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
214	AR1232 1000 PPB WORKING SOLUTION	PP23745	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11587 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1063	AR1232 750 PPB STD	PP23747	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23745 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
223	AR1232 500 PPB STD	PP23748	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23745 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1064	AR1232 250 PPB STD	PP23749	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23745 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1065	AR1232 50 PPB STD	PP23750	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23748 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
215	AR1242 1000 PPB WORKING STD	PP23751	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P12929 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1067	AR1242 750 PPB STD	PP23752	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23751 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
224	AR1242 500 PPB STD	PP23753	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23751 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1068	AR1242 250 PPB STD	PP23754	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23751 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1069	AR1242 50 PPB STD	PP23755	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23753 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
216	AR1248 1000 PPB WORKING STD	PP23756	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P12934 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1075	AR1248 750 PPB STD	PP23757	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23756 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
225	AR1248 500 PPB STD	PP23758	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23756 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1076	AR1248 250 PPB STD	PP23759	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23756 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1077	AR1248 50 PPB STD	PP23760	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23758 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
217	AR1254 1000 PPB WORKING STD	PP23761	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11590 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1071	AR1254 750 PPB STD	PP23762	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23761 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
226	AR1254 500 PPB STD	PP23763	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23761 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1072	AR1254 250 PPB STD	PP23764	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23761 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1073	AR1254 50 PPB STD	PP23765	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23763 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1529	AR1262 1000 PPB Working Solution	PP23766	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P10500 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3753	AR1262 750 PPB STD	PP23767	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23766 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1530	AR1262 500 PPB STD	PP23768	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23766 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3754	AR1262 250 PPB STD	PP23769	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23766 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3755	AR1262 50 PPB STD	PP23770	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23768 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1532	AR1268 1000 PPB Working Solution	PP23771	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11597 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3820	AR1268 750 PPB STD	PP23772	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.25000ml of E3805 + 0.75000ml of PP23771 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1533	AR1268 500 PPB STD	PP23773	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23771 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3821	AR1268 250 PPB STD	PP23774	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.75000ml of E3805 + 0.25000ml of PP23771 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3822	AR1268 50 PPB STD	PP23775	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.90000ml of E3805 + 0.10000ml of PP23773 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
404	AR1660 100 PPM Stock Solution 2nd Source	PP23776	10/03/2024	04/01/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12947 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
405	AR1660 1000/100 PPB ICV STD	PP23777	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 98.50000ml of E3805 + 0.50000ml of PP23733 + 1.00000ml of PP23776 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
406	AR1660 500 PPB ICV	PP23778	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23777 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3789	AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT)	PP23779	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P13372 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3790	AR1221 500 PPB ICV(AGILENT)	PP23780	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23779 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1887	AR1232 1000 PPB Working Sol. 2nd Source	PP23781	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12698 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1889	AR1242 1000 PPB Working Sol. 2nd Source	PP23782	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P11507 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1888	AR1232 500 PPB ICV	PP23783	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23781 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1891	AR1242 500 PPB ICV	PP23784	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23782 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1890	AR1248 1000 PPB Working Sol. 2nd Source	PP23785	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P11512 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1892	AR1248 500 PPB ICV	PP23786	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23785 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1893	AR1254 1000 PPB Working Sol. 2nd Source	PP23787	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 1.00000ml of P12957 + 98.50000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1894	AR1254 500 PPB ICV	PP23788	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23787 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3757	AR1262 1000 PPB Working Solution second source	PP23789	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.10000ml of P13033 + 99.40000ml of E3805 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3758	AR1262 500 PPB STD ICV	PP23790	10/03/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel
								10/03/2024

FROM 0.50000ml of E3805 + 0.50000ml of PP23789 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3609	20 PPM DRO SPIKE SOLUTION (RESTEK)	PP23913	10/25/2024	04/23/2025	Yogesh Patel	None	None	Ankita Jodhani
								10/25/2024

FROM 1.00000ml of P13104 + 1.00000ml of P13109 + 48.00000ml of E3822 = Final Quantity: 50.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3817	AR1268 1000 ppb Working Soln. 2nd source	PP23946	11/07/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel 11/13/2024

FROM 1.00000ml of P11521 + 98.50000ml of E3825 + 0.50000ml of PP23733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3823	AR1268 500 PPB STD ICV	PP23947	11/07/2024	03/30/2025	Ankita Jodhani	None	None	Yogesh Patel 11/13/2024

FROM 0.50000ml of E3825 + 0.50000ml of PP23946 = Final Quantity: 1.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP23985	11/15/2024	05/08/2025	Ankita Jodhani	None	None	Yogesh Patel
<u>FROM</u> 1.00000ml of P13352 + 999.00000ml of E3827 = Final Quantity: 1000.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	06/30/2025	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	07/01/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	24E0761004	11/05/2025	10/01/2024 / Rajesh	09/25/2024 / Rajesh	E3804

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24C1862008	03/30/2025	09/30/2024 / Rajesh	09/25/2024 / Rajesh	E3805

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24I2662006	04/23/2025	10/24/2024 / Rajesh	10/24/2024 / Rajesh	E3822

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	11/06/2025	11/06/2024 / Rajesh	11/01/2024 / Rajesh	E3825

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	05/09/2025	11/09/2024 / Rajesh	11/07/2024 / Rajesh	E3826

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	05/08/2025	11/08/2024 / Rajesh	11/07/2024 / Rajesh	E3827

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	06/16/2025	12/16/2024 / Rajesh	12/13/2024 / Rajesh	E3847

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	0000281827	06/02/2025	06/01/2022 /	04/05/2022 / william	M5173

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul	A0163157	04/03/2025	10/03/2024 / Ankita	03/19/2021 / Abdul	P10483

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane	A0167722	04/03/2025	10/03/2024 / Ankita	03/19/2021 / Ankita	P10500

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-312-1 / Aroclor 1242	0006665550	04/03/2025	10/03/2024 / Ankita	02/21/2022 / Ankita	P11507

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-342-1 / Aroclor 1248	0006626997	04/03/2025	10/03/2024 / Ankita	02/21/2022 / Ankita	P11512

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-382-1 / Aroclor 1268	0006587800	05/07/2025	11/07/2024 / Ankita	02/21/2022 / Ankita	P11521

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul	A0175456	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11581

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul	A0173309	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11587

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul	A0175403	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11590

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane	A0181782	04/03/2025	10/03/2024 / Ankita	03/18/2022 / Abdul	P11597

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	91867 / Aroclor 1232 100 ug/mL	020823	04/03/2025	10/03/2024 / Ankita	08/07/2023 / Ankita	P12698

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul	a0203672	04/03/2025	10/03/2024 / Ankita	12/07/2023 / Ankita	P12929

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul	a0202803	04/03/2025	10/03/2024 / Ankita	12/07/2023 / Ankita	P12934

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	20064 / Aroclor 1016/1260	022023	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12947

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ Aroclor 1254	121823	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P12957

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc	90165 / Aroclor 1262	112322	04/03/2025	10/03/2024 / Ankita	12/20/2023 / Yogesh	P13033

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0204859	04/25/2025	10/25/2024 / yogesh	01/12/2024 / Yogesh	P13104

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0204859	04/25/2025	10/25/2024 / yogesh	01/12/2024 / Yogesh	P13109

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	04/03/2025	10/03/2024 / Ankita	04/22/2024 / Abdul	P13350

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	05/15/2025	11/15/2024 / Ankita	04/22/2024 / Abdul	P13352

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	PP-292-1 / Aroclor 1221	0006783205	04/03/2025	10/03/2024 / Ankita	05/02/2024 / Ankita	P13372

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1


Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865

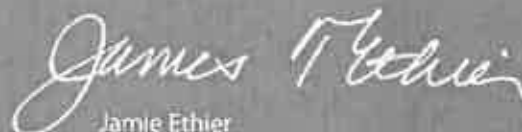
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	3.6 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	7.9 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	8 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

Acetone
CMOS

 **avantor™**



Material No.: 9005-05
Batch No.: 24E0761004

Test	Specification	Result
------	---------------	--------

For Microelectronic Use

Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC



Michelle Bales
Sr. Manager, Quality Assurance

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9262-03
Batch No.: 24C1862008
Manufactured Date: 2024-01-30
Expiration Date: 2025-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.4 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 9/25/24

E 3805

Jamie Croak
Director Quality Operations, Bioscience Production

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4

Batch No.: 24I2662006

Manufactured Date: 2024-08-29

Expiration Date: 2025-11-28

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	3
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8\%$	99.9%
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	≤ 10 ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02\%$	$< 0.01\%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3822

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

£3825

Jamie Croak
Director Quality Operations, Bioscience Production

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3826

Rec'd by RP on 11/7/24

Jamie Croak
Director Quality Operations, Bioscience Production

Acetone

BAKER RESI-ANALYZED® Reagent

For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E 3827

Rec'd by RS on ~~11/8/24~~ 11/7/24
RS
11/7

Jamie Croak

Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 12/13/24

E3847



Jamie Croak
Director Quality Operations, Bioscience Production

Hydrochloric Acid, 36.5–38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis



Material No.: 9530-33
Batch No.: 0000281827
Manufactured Date: 2021/03/30
Retest Date: 2026/03/29
Revision No: 1

Certificate of Analysis

Test	Specification	Result
ACS – Assay (as HCl) (by acid–base titrn)	36.5 – 38.0 %	37.6
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	1
ACS – Specific Gravity at 60°/60°F	1.185 – 1.192	1.189
ACS – Bromide (Br)	<= 0.005 %	< 0.005
ACS – Extractable Organic Substances	<= 5 ppm	< 1
ACS – Free Chlorine (as Cl ₂)	<= 0.5 ppm	< 0.5
Phosphate (PO ₄)	<= 0.05 ppm	< 0.03
Sulfate (SO ₄)	<= 0.5 ppm	< 0.3
Sulfite (SO ₃)	<= 0.8 ppm	0.3
Ammonium (NH ₄)	<= 3 ppm	< 1
Trace Impurities – Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities – Aluminum (Al)	<= 10.0 ppb	0.5
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities – Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities – Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities – Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities – Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities – Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities – Calcium (Ca)	<= 50.0 ppb	15.0
Trace Impurities – Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities – Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities – Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities – Gallium (Ga)	<= 1.0 ppb	< 0.2

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	3.0
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	1.0
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	< 0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	< 0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	0.2
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	18.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	< 0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.4
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use

Product Information (not specifications):

Appearance (clear, fuming liquid)

Meets ACS Specifications

Country of Origin: US

Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32039 **Lot No.:** A0163157

Description : Aroclor® 1016/1260 Mix
Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2026 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1016 CAS # 12674-11-2 (Lot 04) Purity ----%	1,007.0 µg/mL	+/- 5.8683 µg/mL Gravimetric +/- 31.9082 µg/mL Unstressed +/- 41.6868 µg/mL Stressed
2	Aroclor 1260 CAS # 11096-82-5 (Lot 07) Purity ----%	1,008.0 µg/mL	+/- 5.8741 µg/mL Gravimetric +/- 31.9399 µg/mL Unstressed +/- 41.7282 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 10476

P 10480

AR
02/19/21

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

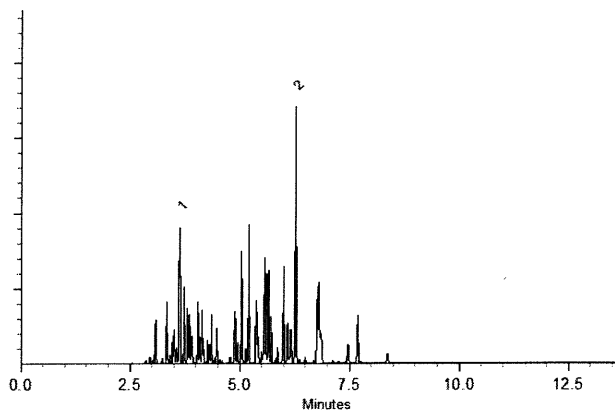

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Tom Suckar - Mix Technician

Date Mixed: 03-Aug-2020

Balance: B442140311

Justine Albertson - Operations Tech-ARM QC

Date Passed: 05-Aug-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32409 Lot No.: A0167722
Description : Aroclor® 1262 Standard
Aroclor® 1262 Standard 1,000 µg/mL, 1mL/ampul, Hexane
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : April 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1262	1,004.0 µg/mL	+/- 5.9635 µg/mL Gravimetric
	CAS # 37324-23-5 (Lot 10849100)		+/- 31.8340 µg/mL Unstressed
	Purity ----%		+/- 41.5787 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P10496
↓
P10500

AJ
09/19/21

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

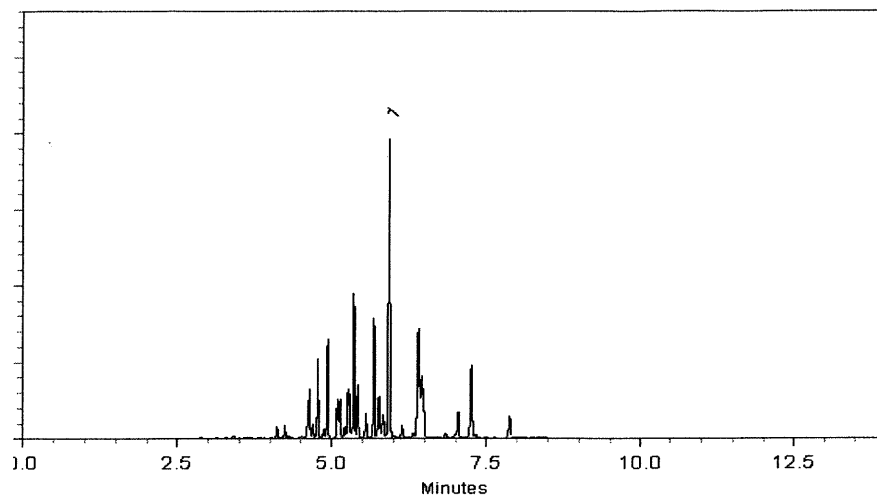

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 03-Jan-2021


Balance: B707717271

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 05-Jan-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1242 Standard

Lot Number: 0006665550

Product Number: PP-312-1

Lot Issue Date: 08-Feb-2022

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 31-Jan-2027

Component Name	CERTIFIED VALUES			CAS#	Analyte Lot
	Concentration	Expanded Uncertainty			
Aroclor 1242	100.4	± 0.5 µg/mL		053469-21-9	NT01020

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P11503
↓
P11507

AJ
02/21/22

Page: 1 of 2

CSD-QA-015.1

ISO 17034



Agilent

Trusted Answers

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2


www.agilent.com/quality/

CSD-QA-015.1



ISO 17025
Cert No. AT-

ISO 17034



Agilent

Trusted Answers

Reference Material Certificate

Product Name: Aroclor 1248 Standard

Lot Number: 0006626997

Product Number: PP-342-1

Lot Issue Date: 17-Aug-2021

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 30-Sep-2025

Component Name	CERTIFIED VALUES		CAS#	Analyte Lot
	Concentration	Expanded Uncertainty		
Aroclor 1248	100.3	± 0.5 µg/mL	012672-29-6	NT01582

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.


P11508

↓
P11512

AJ

2/21/22

ISO 17034



Agilent

Trusted Answers

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



Certificate of Analysis

P11518
↓
P11522
AJ
02/21/22

Product Name: Aroclor 1268 Standard

Product Number: PP-382-1

Lot Issue Date: 09-Feb-2021

Lot Number: 0006587800

Expiration Date: 31-Mar-2029

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration ± Uncertainty
Aroclor 1268	011100-14-4	RM00937	100.0 ± 0.5 µg/mL

Matrix: isooctane (2,2,4-trimethylpentane)

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.


Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026
Page: 1 of 1

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32007 Lot No.: A0175456
Description : Aroclor® 1221 Standard
Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1221 CAS # 11104-28-2 (Lot 10210500) Purity ----%	1,002.0 µg/mL	+/- 5.9516 µg/mL Gravimetric +/- 31.7706 µg/mL Unstressed +/- 41.4958 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 11578
↓
P 11582 / (S)

AR
04/30/22

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

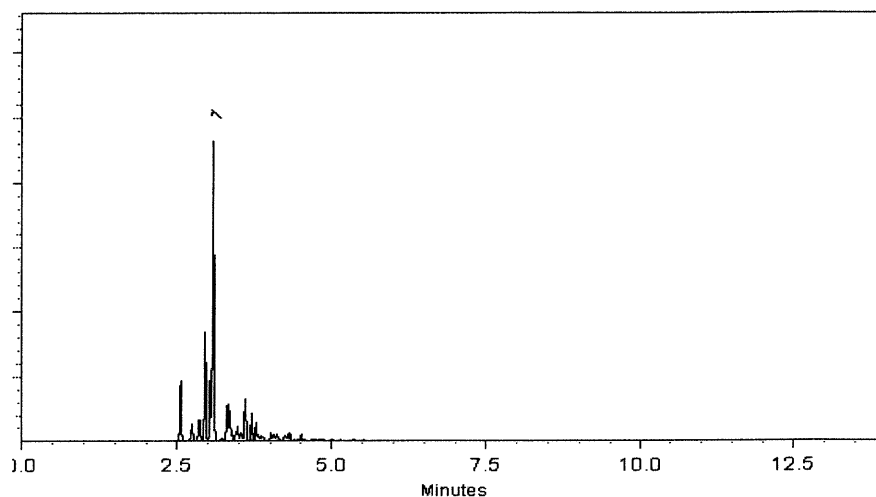

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 16-Aug-2021 Balance: B442140311

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 18-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11578
↓
P11582 / (S)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32008 Lot No.: A0173309
Description : Aroclor® 1232 Standard
Aroclor® 1232 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : September 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1232	1,001.0 µg/mL	+/- 5.9456 µg/mL Gravimetric
	CAS # 11141-16-5 (Lot 15665-01)		+/- 31.7389 µg/mL Unstressed
	Purity ----%		+/- 41.4544 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11583
↓
P11587 / (S)

AR
04/30/22

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

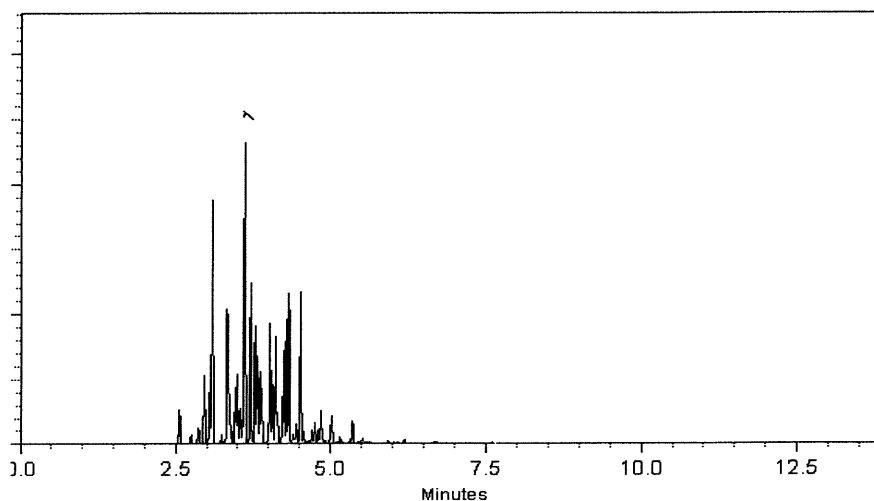

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 13-Jun-2021 **Balance:** B442140311

Alexis Shelow
Alexis Shelow - Operations Tech I

Date Passed: 16-Jun-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11583
↓
P11587 (5)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011 Lot No.: A0175403
Description : Aroclor® 1254 Standard
Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : November 30, 2027 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1254 CAS # 11097-69-1 (Lot 124-191-B) Purity ----%	1,000.7 µg/mL	+/- 5.9437 µg/mL Gravimetric +/- 31.7284 µg/mL Unstressed +/- 41.4406 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P11588
↓
P11592 / (S)

AR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

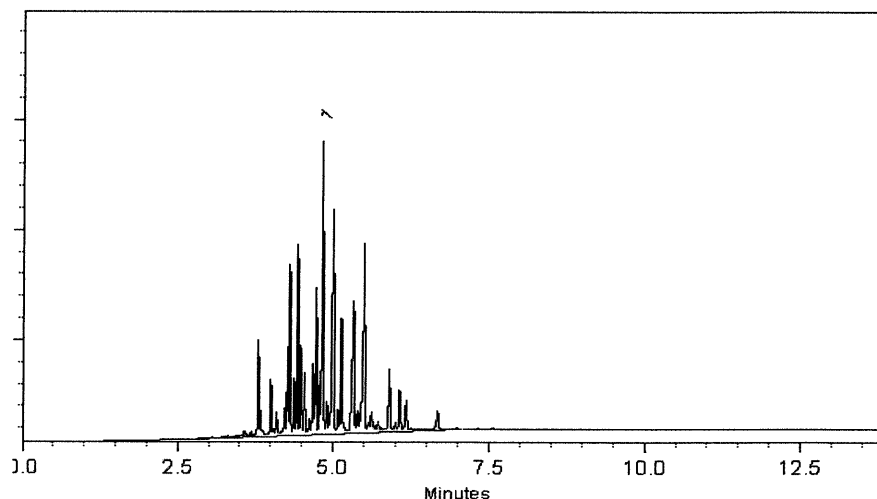

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Cathleen Soltis

Cathleen Soltis - Mix Technician

Date Mixed: 15-Aug-2021

Balance: 1128360905

Alexis Shelow

Alexis Shelow - Operations Tech I

Date Passed: 17-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11588
↓
P11592 / (5)

AR
04/30/22



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32410 Lot No.: A0181782
Description : Aroclor® 1268 Standard
Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : May 31, 2028 Storage: 25°C nominal
Handling: This product contains PCBs. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Aroclor 1268 CAS # 11100-14-4 Purity ----%	1,001.4 µg/mL (Lot 10947000)	+/- 5.9480 µg/mL Gravimetric +/- 31.7516 µg/mL Unstressed +/- 41.4710 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 11593
↓
P 11597
⑤

UAR
04/30/2022

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

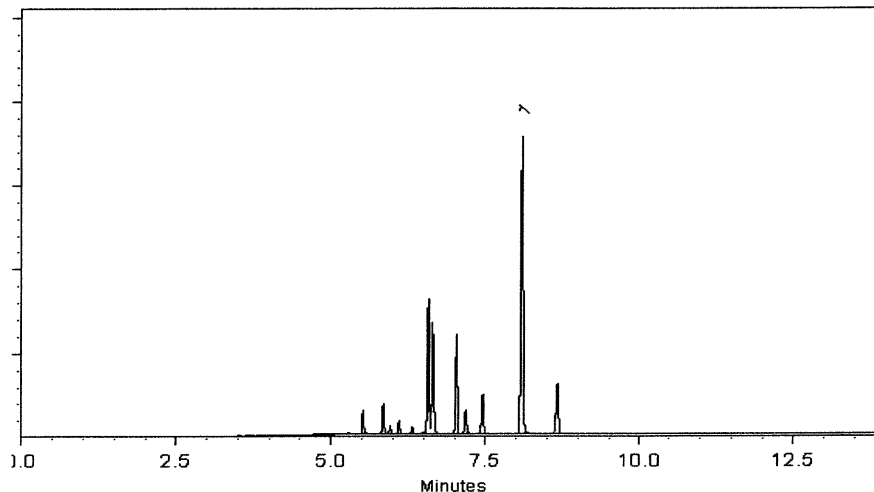

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Penelope S. Riglin
Penelope Riglin - Operations Tech I

Date Mixed: 14-Feb-2022

Balance: 1128360905

Clara Windle
Clara Windle - Operations Technician I

Date Passed: 17-Feb-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 11593 / (5)
↓
P 11597
[Signature]
04/30/2022



CERTIFIED WEIGHT REPORT

Part Number: **91867**
 Lot Number: **020823**
 Description: **WP 037 - Aroclor 1232**
PCB Technical Mixture
 Expiration Date: **020833**
 Recommended Storage: **Ambient (20 °C)**
 Nominal Concentration ($\mu\text{g/mL}$): **100**
 NIST Test ID#: **6UTB**

Solvent(
Aceton


Weight(s) shown below were combined and diluted to (mL): **100.0**
 5E-05 Balance Uncertainty
 0.057 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc ($\mu\text{g/mL}$)	Purity (%)	Uncertainty Purity	Target Weight (g)
1. Aroclor 1232	17	45-6A	100	100	0.5	0.01000

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measure Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stonier
 Column ID SPB-608 30 meter X 0.53mm X 5 μm film thickness
 Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
 Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
 Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
 Rate = 8°C/min, Total run time = 35 min
 Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
 Standard injection = 1.5 μL , Range=3

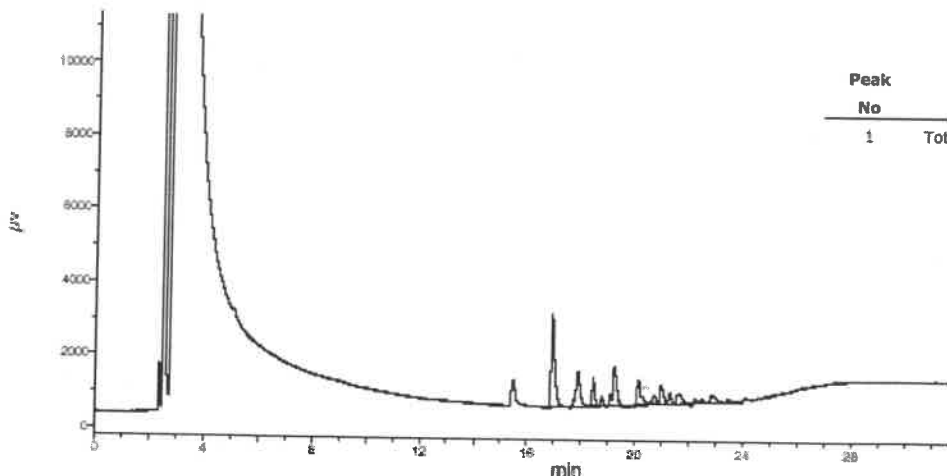




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32009 **Lot No.:** A0203672

Description: Aroclor® 1242 Standard

Aroclor® 1242 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

p12928

→

p12932

AJ

12/27/23

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Aroclor 1242	53469-21-9	01141	—%	1,004.7 µg/mL	+/- 55.7515

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

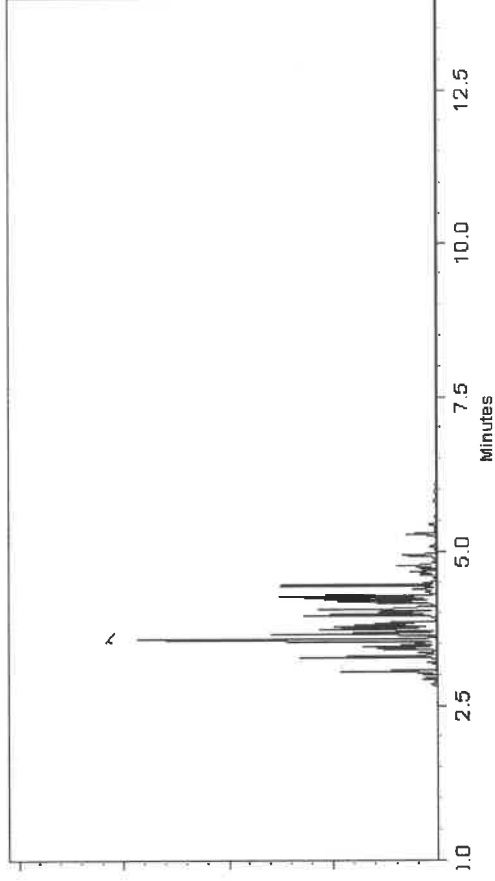

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Boothamer

Russ Boothamer - Operations Technician I

Date Mixed: 26-Oct-2023

Balance Serial #

B442140311

Jennifer Polino

Jennifer Polino - Operations Tech III - APM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32010 **Lot No.:** A0202803

Description: Aroclor® 1248 Standard

Aroclor® 1248 Standard 1,000µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: January 31, 2030 **Storage:** 25°C nominal

Handling: This product contains PCBs. **Ship:** Ambient

P1210967
P1210977
P1210977
P1210977

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Aroclor 1248	12672-29-6	13897600	---%	1,001.7 µg/mL	+/- 55.5850

Solvent: Hexane

CAS # 110-54-3

Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2ul

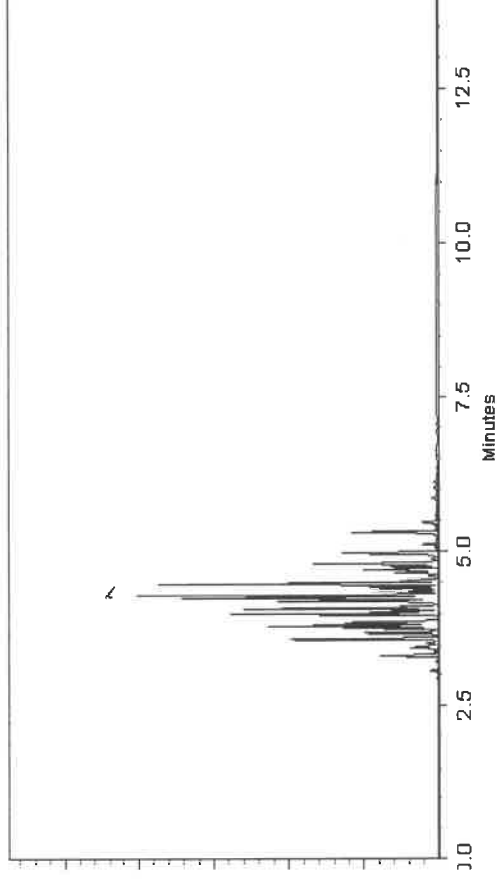

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

[Signature]
Laith Clemente - Operations Technician I

Date Mixed: 03-Oct-2023

Balance Serial # 1128360905

[Signature]
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FW 80397



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT

Part Number:
20064

Solvent(s):
Hexane

Lot#
273615

Lot Number:
022023

Formulated By:
Benson Chan

DATE
022023

Description:
CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260

Reviewed By:
Pedro L. Rentas

DATE
022023

Expiration Date:
022033

Expanded
Uncertainty
(+/-) (µg/mL)

4.0

Recommended Storage:
Ambient (20 °C)

Actual
Conc (µg/mL)

1002.8

Nominal Concentration (µg/mL):
1000

Actual
Weight(g)

0.20060

NIST Test ID#:
6UTB

Target
Weight(g)

0.20004

Weight(s) shown below were combined and diluted to (mL.):
200.0

Purity
(%)

100

5E-05 Balance Uncertainty
0.010 Flask Uncertainty

Conc (µg/mL)

1000

SDS Information
(Solvent Safety Info. On Attached pg.)

OSHA PEL (TWA)


LD50

PR2946 718
↓
12/20/23
P12955

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. Aroclor 1016	15	020491JC	1000	100	0.2	0.20004	0.20060	1002.8	4.0	12674-11-2	N/A	N/A
2. Aroclor 1260	21	020491JC	1000	100	0.2	0.20004	0.20081	1003.9	4.0	11086-82-5	0.5mg/m3	orl-rat 1315mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stortier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 280°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Etdaq Channel 1
Standard Injection = 1.5µL, Range=3

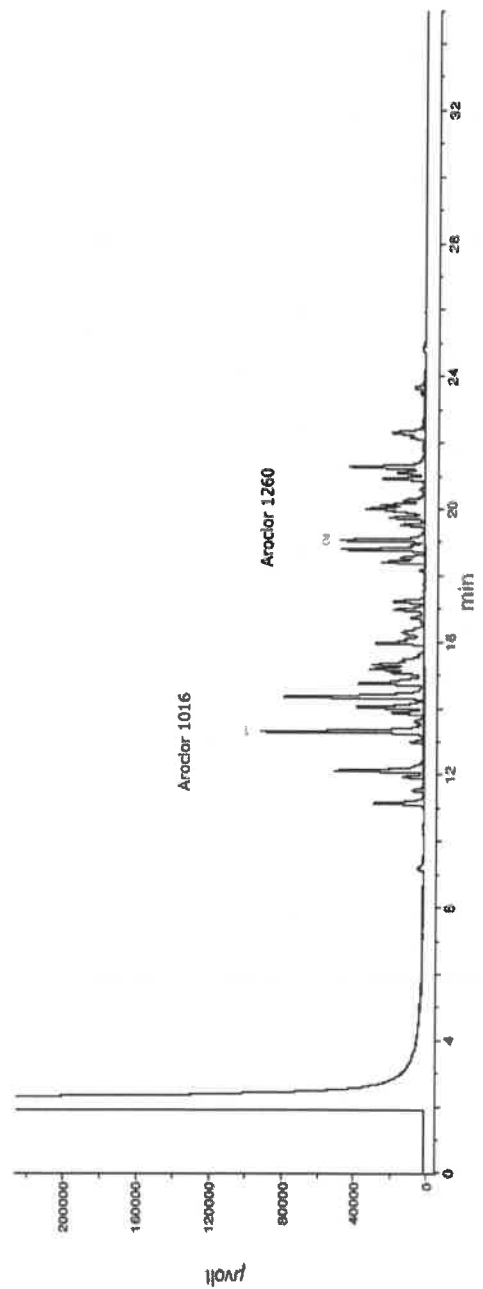



CERTIFIED WEIGHT REPORT

Part Number: 99139
Lot Number: 121823
Description: Aroclor 1254

Expiration Date: 121833
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 100
NIST Test ID#: 6UTB

Volume(s) shown below were combined and diluted to (mL): 20.0
Note: Aroclor 1254 is a mix of isomers.

Solvent(s): Iso-octane
Lot#: 82227

Formulated By: Anthony Mahoney	121823	DATE
Reviewed By: Pedro L. Rentas	121823	DATE


P12956 / Y.P.
12/18/23
P12957

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Initial Uncertainty	Pipette (mL)	Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information		
											(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA) LD50
1. Aroclor 1254	79100	121823	0.10	2.00	0.017	0.017	1003.3	100.1	1.8	11097-69-1	0.5mg/m3 (skin)		or-rat 1295mg/kg

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments
GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X 5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150 °C (Time 1 = 4 min), Temp 2 = 280 °C (Time 2 = 13.5 min)
Rate = 8 °C/min, Total run time = 35 min
Injector temp. = 200 °C, FID Temp. = 300 °C, FID Signal = Etdaq Channel 1
Standard injection = 1.5µL, Range=3

Peak No.	Name	FID RT (min.)
1	Total Aroclor 1254	18.12

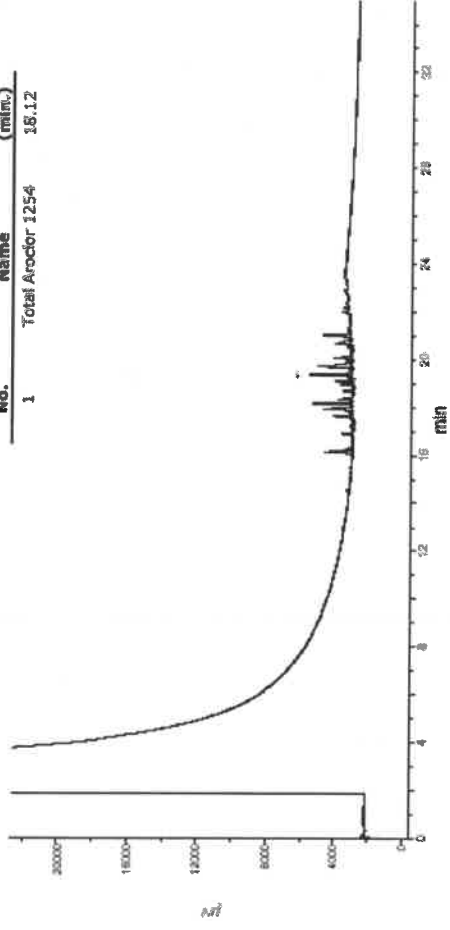



CERTIFIED WEIGHT REPORT

Part Number: 90165
Lot Number: 112322
Description: Atrocior 1262
Expiration Date: 112332
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 6LUTB
Weight(s) shown were combined and diluted to (mL): 50.0

Solvent(s): Hexane
Lot# 273615


SE-05 Balance Uncertainty
0.005 Flask Uncertainty

Formulated By:	Prashant Chauhan	112322	DATE
Reviewed By:	Pedro L. Rentes	112322	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
----------	-----	------------	----------------------	------------	--------------------	-------------------	-------------------	---------------------	----------------------------------	------	----------------	------

1. Atrocior 1262 444 W-130-05 1000 100 0.2 0.05003 0.05016 1002.7 4.5 37324-23-5 N/A or-ral 11300mg/kg

Method GC/MSD-7.M: Column:(30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (0min.), Temp 2 = 290°C (12.5 min.), Rate = 8°C/min., Injector B = 200°C, Detector B = 290°C.

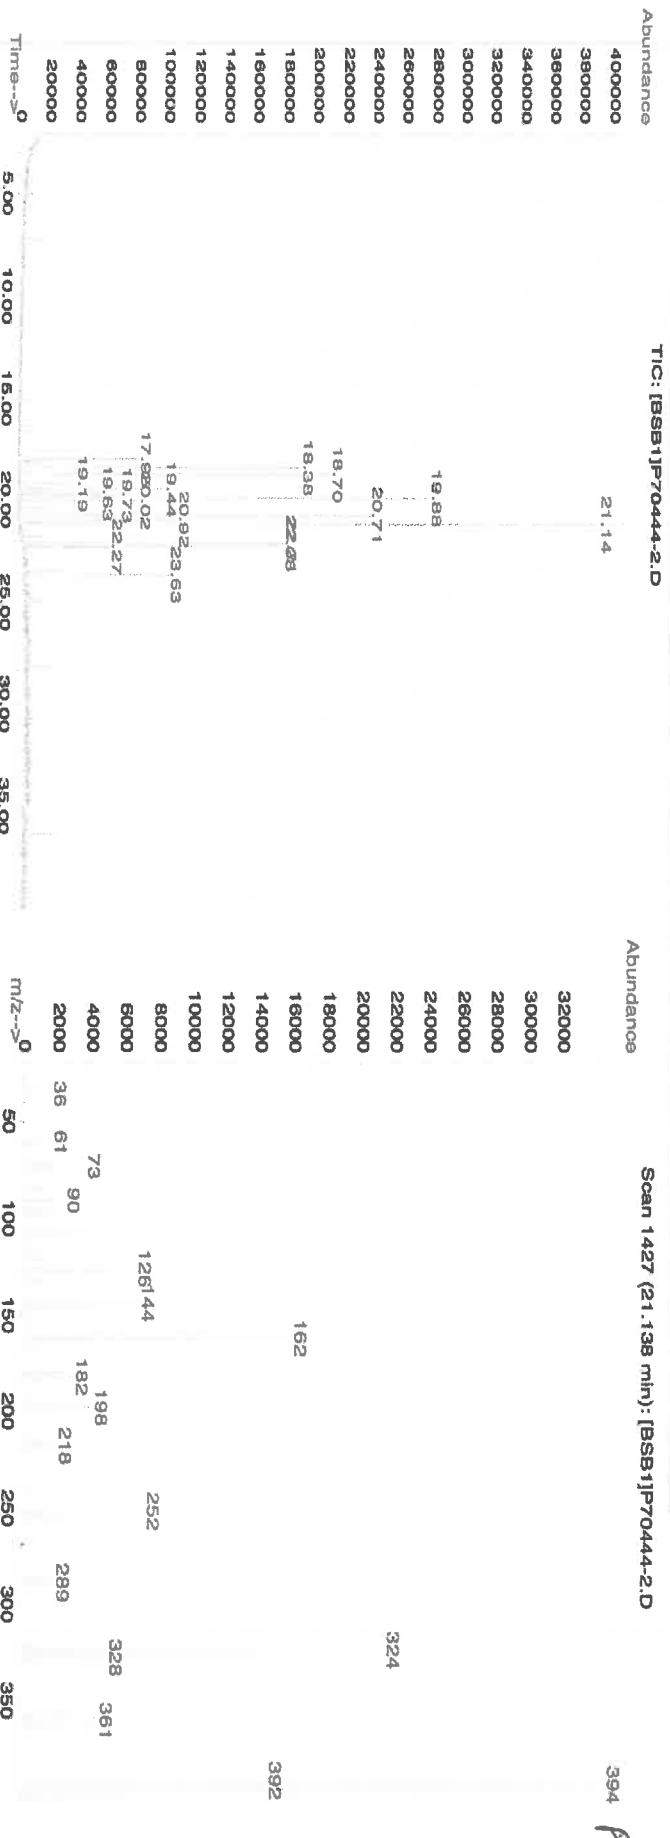

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




Run 20, "P90165 L112322 [1000µg/mL in hexane]"

Run Length: 35.00 min, 21000 points at 10 points/second.
Created: Thu, Dec 8, 2022 at 2:31:02 AM.
Sampled: Sequence "120722-GC3M1", Method "GC3-M1".
Analyzed using Method "GC3-M1".

Comments

GC3-M1 Analysis by Melissa Stonier
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
Standard injection = 1.5µL, Range=3

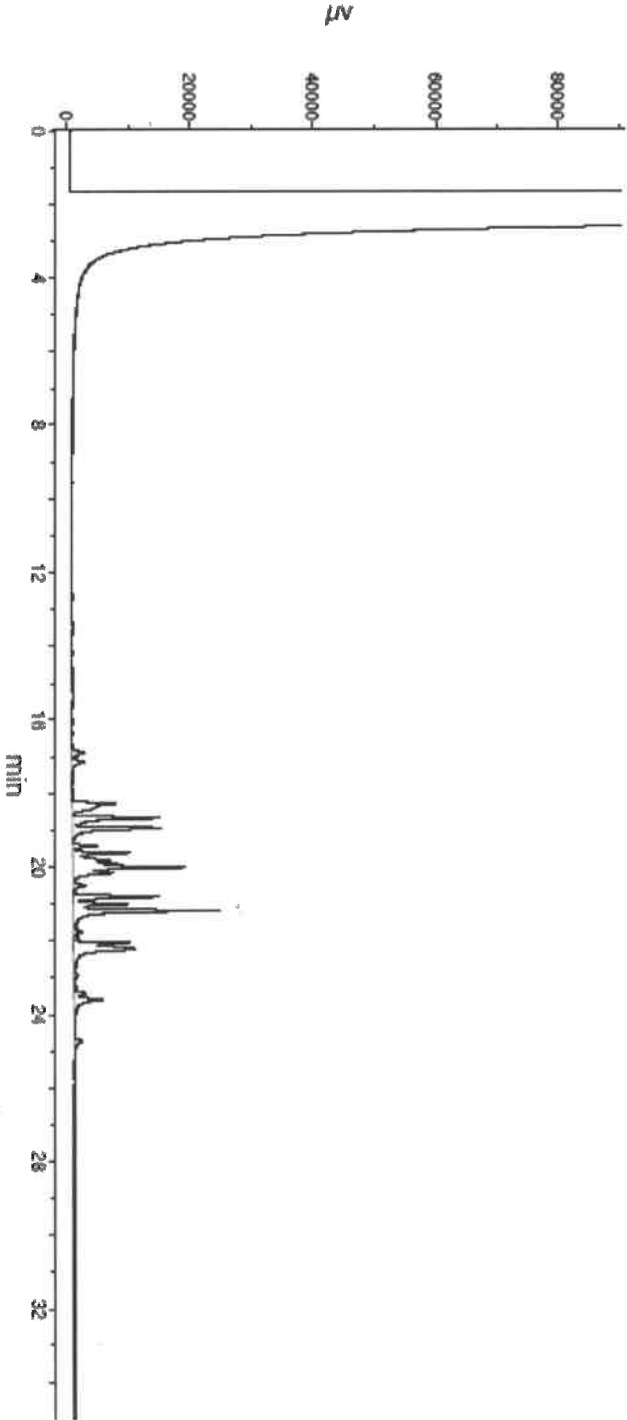



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266 **Lot No.:** A0204859

Description : Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2030 **Storage:** 25°C nominal

Handling: Sonicate prior to use. **Ship:** Ambient

P13103 } Y.P.
↓
P13112 } 01/12/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Octane (C8)	111-65-9	SHBP9758	99%	504.4 µg/mL	+/- 13.0305
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	503.6 µg/mL	+/- 13.0098
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	503.6 µg/mL	+/- 13.0098
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	504.0 µg/mL	+/- 13.0201
5	n-Hexadecane (C16)	544-76-3	SHBP8192	99%	504.0 µg/mL	+/- 13.0201
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	504.1 µg/mL	+/- 13.0230
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	504.0 µg/mL	+/- 13.0204
8	n-Docosane (C22)	629-97-0	MKQC3882	99%	503.6 µg/mL	+/- 13.0098
9	n-Tetracosane (C24)	646-31-1	MKQC8345	99%	504.0 µg/mL	+/- 13.0201
10	n-Hexacosane (C26)	630-01-3	MKQC4814	99%	504.0 µg/mL	+/- 13.0201
11	n-Octacosane (C28)	630-02-4	BCCG0084	99%	504.0 µg/mL	+/- 13.0201
12	n-Triacontane (C30)	638-68-6	MKQC9436	97%	504.0 µg/mL	+/- 13.0204
13	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	504.0 µg/mL	+/- 13.0201
14	n-Tetratriacontane (C34)	14167-59-0	OML4N	99%	504.4 µg/mL	+/- 13.0305
15	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	504.0 µg/mL	+/- 13.0201
16	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	503.8 µg/mL	+/- 13.0152
17	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	503.6 µg/mL	+/- 13.0098

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

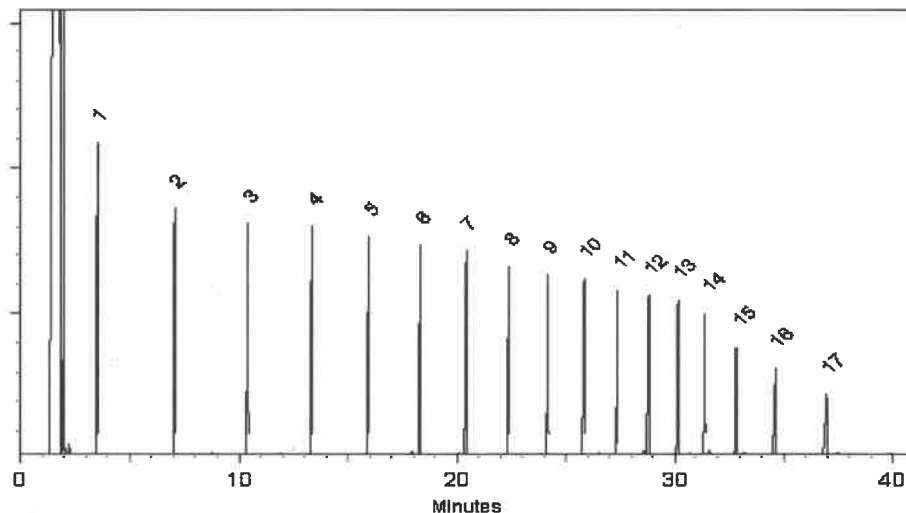


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 29-Nov-2023

Balance Serial # B442140311


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Dec-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266 **Lot No.:** A0204859

Description : Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2030 **Storage:** 25°C nominal

Handling: Sonicate prior to use. **Ship:** Ambient

P13103 } Y.P.
↓
P13112 } 01/12/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Octane (C8)	111-65-9	SHBP9758	99%	504.4 µg/mL	+/- 13.0305
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	503.6 µg/mL	+/- 13.0098
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	503.6 µg/mL	+/- 13.0098
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	504.0 µg/mL	+/- 13.0201
5	n-Hexadecane (C16)	544-76-3	SHBP8192	99%	504.0 µg/mL	+/- 13.0201
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	504.1 µg/mL	+/- 13.0230
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	504.0 µg/mL	+/- 13.0204
8	n-Docosane (C22)	629-97-0	MKCQ3882	99%	503.6 µg/mL	+/- 13.0098
9	n-Tetracosane (C24)	646-31-1	MKCQ8345	99%	504.0 µg/mL	+/- 13.0201
10	n-Hexacosane (C26)	630-01-3	MKCQ4814	99%	504.0 µg/mL	+/- 13.0201
11	n-Octacosane (C28)	630-02-4	BCCG0084	99%	504.0 µg/mL	+/- 13.0201
12	n-Triacontane (C30)	638-68-6	MKCQ9436	97%	504.0 µg/mL	+/- 13.0204
13	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	504.0 µg/mL	+/- 13.0201
14	n-Tetratriacontane (C34)	14167-59-0	OML4N	99%	504.4 µg/mL	+/- 13.0305
15	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	504.0 µg/mL	+/- 13.0201
16	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	503.8 µg/mL	+/- 13.0152
17	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	503.6 µg/mL	+/- 13.0098

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

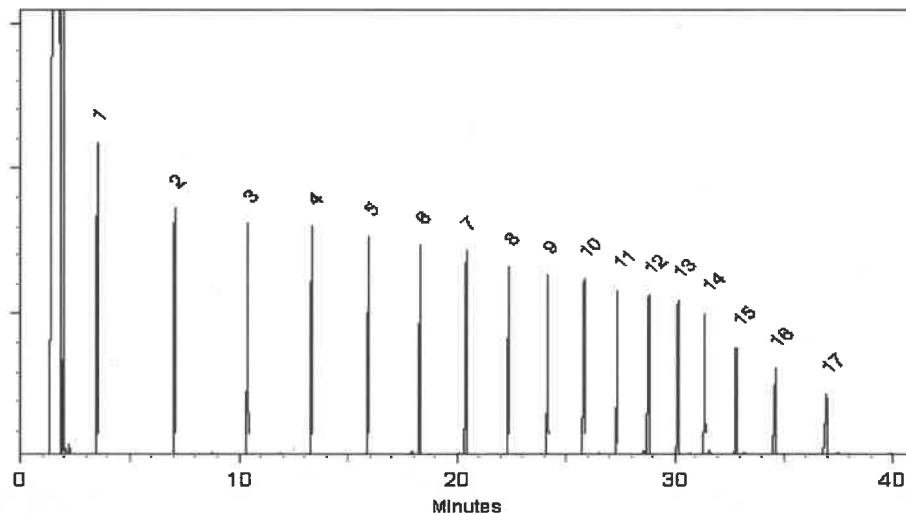


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 29-Nov-2023

Balance Serial # B442140311


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Dec-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

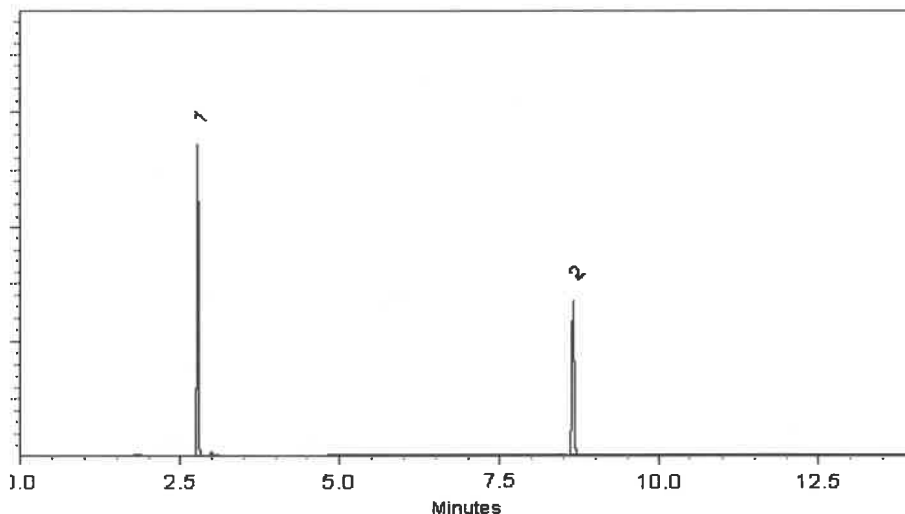


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

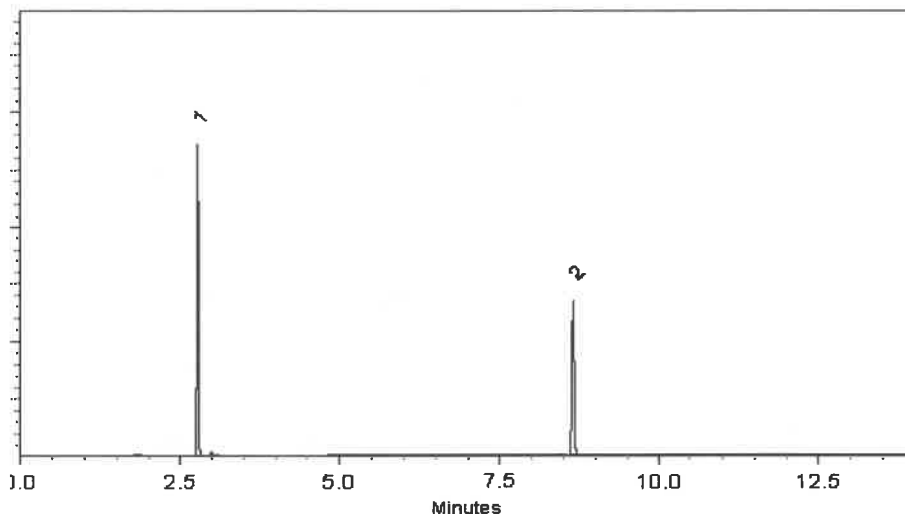


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



ISO 17034

Reference Material Certificate

Product Information Sheet

Product Name: Aroclor 1221 Standard
Product Number: PP-292-1
Storage Conditions: Store at Room Temperature (15° to 30°C).

Lot Number: 0006783205
Lot Issue Date: 20-Feb-2024
Expiration Date: 31-Mar-2032

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
Aroclor 1221	100.3 ±	0.5 µg/mL	011104-28-2	NT01017

Matrix: isooctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13342
AJ
05106124
P13343

Page: 1 of 2

CSD-QA-015.2

ISO 17025

Cert No. AT-1937


250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.2

ISO 17025
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



SHIPPING DOCUMENTS

CLIENT INFORMATION

REPORT TO BE SENT TO:

COMPANY: Kleinfelder
 ADDRESS: 25 Gold Drive
 CITY: Hamilton STATE: NJ ZIP: 08691
 ATTENTION: Mark Warchol
 PHONE: 484-883-3892 FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME: ~~Mountaintop~~ Comegys School
 PROJECT NO.: 1400513.001 LOCATION: Philadelphia, PA
 PROJECT MANAGER: Mark Warchol
 e-mail: mwarchol@kleinfelder.com
 PHONE: 484-883-3892 FAX:

CLIENT BILLING INFORMATION

BILL TO: PO#:
 ADDRESS: Same
 CITY: STATE: ZIP:
 ATTENTION: PHONE:

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) 5 DAYS*
 HARDCOPY (DATA PACKAGE): 5 DAYS*
 EDD: 5 DAYS*

*TO BE APPROVED BY CHEMTECH

STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS DAYS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☒ Level 2 (Results + QC) ☐ NJ Reduced ☐ US EPA CLP
☐ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
 + Raw Data ☐ Other
☐ EDD FORMAT

1 2 3 4 5 6 7 8 9
 PAPER LIST: Fill
 Level 2: Fill
 On Hold

PRESERVATIVES

COMMENTS

CHEMTECH SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES										COMMENTS
			COMP	GRAB	DATE	TIME		E	E								
1.	COMP-1	Soil	✓		12/20/24	9:15	3	✓									* 1
2.	COMP-2					9:50											* 5
3.	COMP-3		↓			10:35	↓	↓									* 4
4.	SB-1			✓		9:25	1		✓								
5.	SB-2					9:00											
6.	SB-3					9:30											
7.	SB-4					9:10											
8.	SB-5					9:05											
9.	SB-6					8:30											
10.	SB-7					9:40											

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER: 1. <i>[Signature]</i>	DATE/TIME: 12/20/24 12:45	RECEIVED BY: 1. <i>[Signature]</i>	Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP 1.6°C °C
RELINQUISHED BY SAMPLER: 2. FedEx	DATE/TIME: 1128 12/23/24	RECEIVED BY: 2. <i>[Signature]</i>	Comments:
RELINQUISHED BY SAMPLER: 3.	DATE/TIME:	RECEIVED BY: 3.	Page 1 of 2 CLIENT: ☐ Hand Delivered ☒ Other FedEx CHEMTECH: ☐ Picked Up ☐ Field Sampling Shipment Complete ☐ YES ☐ NO

CLIENT INFORMATION

REPORT TO BE SENT TO:

COMPANY: Kleinfelder
 ADDRESS: 2 S Gold Drive
 CITY: Hamilton STATE: NJ ZIP: 08691
 ATTENTION: Mark Warchol
 PHONE: 484-883-3892 FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME: Comegys School
 PROJECT NO.: 24005163.001A LOCATION: Philadelphia, PA
 PROJECT MANAGER: Marks Warchol
 e-mail: mwarchol@kleinfelder.com
 PHONE: 484-883-3892 FAX:

CLIENT BILLING INFORMATION

BILL TO: PO#: Same
 ADDRESS: Same
 CITY: Same STATE: Same ZIP: Same
 ATTENTION: PHONE:

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) 5 DAYS*
 HARDCOPY (DATA PACKAGE): 5 DAYS*
 EDD: 5 DAYS*

*TO BE APPROVED BY CHEMTECH

STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS DAYS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☒ Level 2 (Results + QC) ☐ NJ Reduced ☐ US EPA CLP
☐ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
 + Raw Data ☐ Other _____
☐ EDD FORMAT _____

On Hold

1	2	3	4	5	6	7	8	9
---	---	---	---	---	---	---	---	---

CHEMTECH SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									COMMENTS		
			COMP	GRAB	DATE	TIME		F	1	2	3	4	5	6	7	8	9	← Specify Preservatives	
																		A-HCl	D-NaOH
																		B-HNO3	E-ICE
																		C-H2SO4	F-OTHER
1.	SB-8	Soil		✓	12/20/24	9:45	1	✓											
2.	SB-9	↓		↓	↓	10:00	↓	↓											
3.	SB-10	↓		↓	↓	10:15	↓	↓											
4.	SB-11	↓		↓	↓	10:30	↓	↓											
5.	SB-12	↓		↓	↓	10:05	↓	↓											
6.																			
7.																			
8.																			
9.																			
10.																			

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:	Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP <u>1.6°C</u> °C
1. <u>Jul</u>	<u>12/20/24 12:45</u>	1. <u>[Signature]</u>	Comments:
RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:	
2. <u>FedEx</u>	<u>12/23/24</u>	2. <u>[Signature]</u>	
RELINQUISHED BY SAMPLER:	DATE/TIME:	RECEIVED BY:	
3.		3.	

Page 2 of 2 CLIENT: ☐ Hand Delivered ☒ Other FedEx Shipment Complete ☐ YES ☐ NO
 CHEMTECH: ☐ Picked Up ☐ Field Sampling



284 Sheffield Street, Mountainside NJ 07092 (908)-789-8900 Fax : 908 789 8922

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488