


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122724\
Data File : BF140980.D
Acq On : 27 Dec 2024 07:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 27 00:31:16 2024

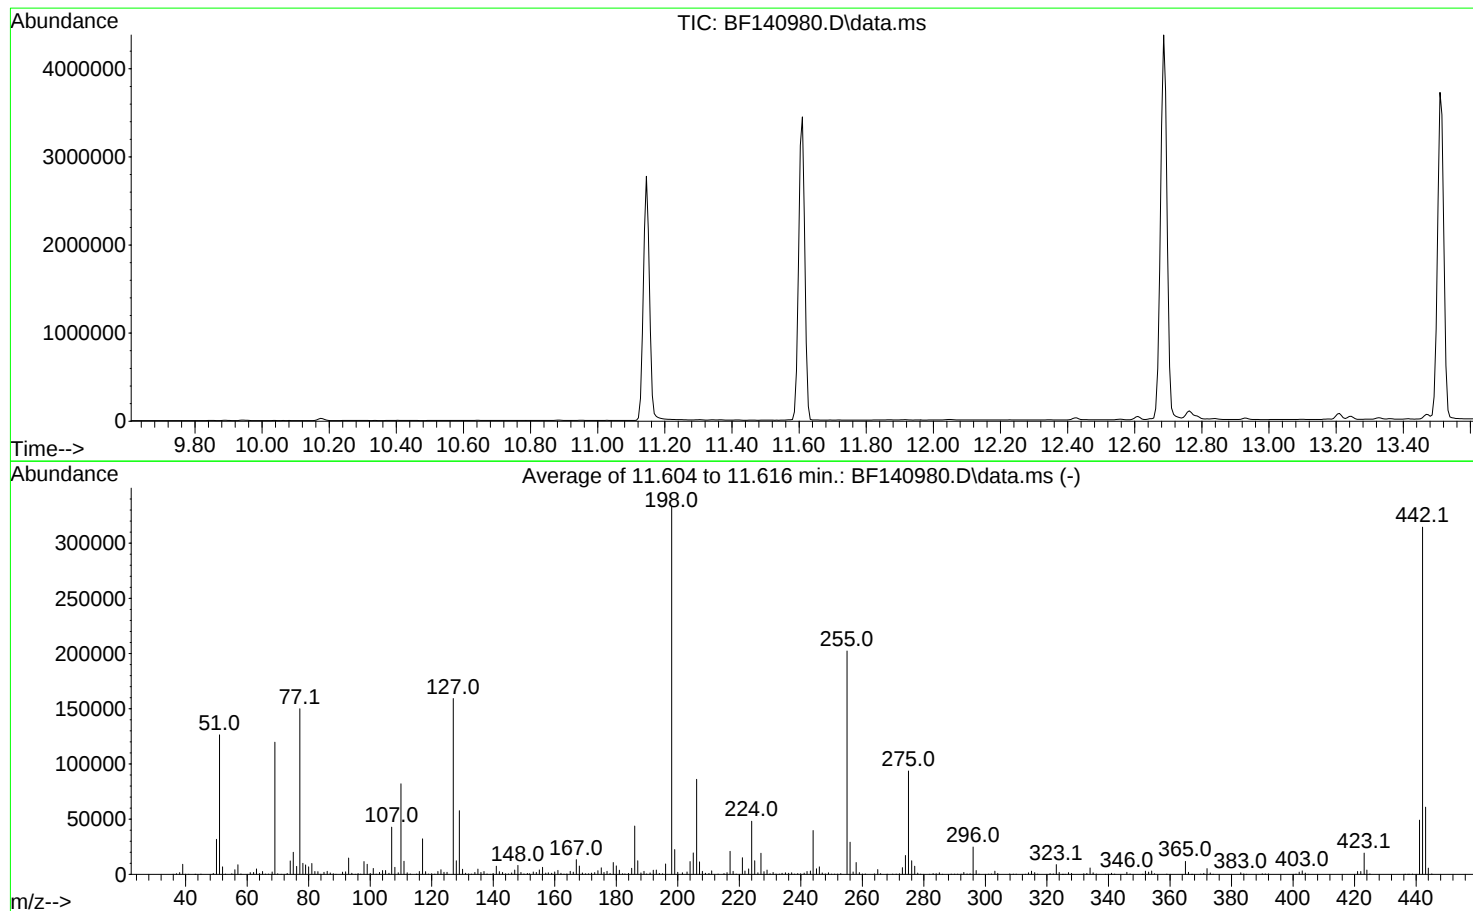

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	126454	PASS
68	69	0.00	2	1.9	2252	PASS
69	198	0.00	100	35.9	119774	PASS
70	69	0.00	2	0.5	554	PASS
127	198	10	80	47.8	159248	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	333248	PASS
199	198	5	9	6.7	22432	PASS
275	198	10	60	28.1	93632	PASS
365	198	1	100	3.5	11781	PASS
441	198	0.01	100	14.8	49179	PASS
442	442	50	100	100.0	314603	PASS
443	442	15	24	19.3	60859	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/27/2024	BNA_F	<u>BF140980.D</u>
Compound Name	Response	Retention Time
DDT	889651	13.51
DDD	23327	13.21
DDE	233	12.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23560	913211	2.58

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122724\
Data File : BF140980.D
Acq On : 27 Dec 2024 07:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 27 10:40:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

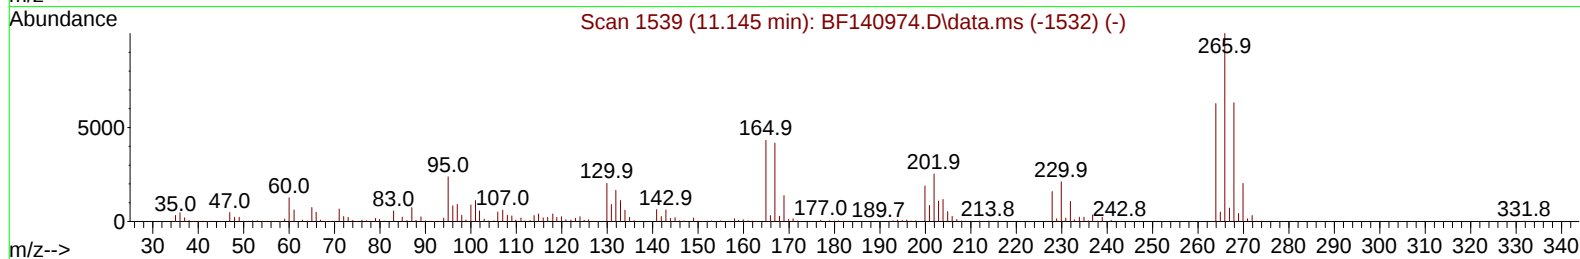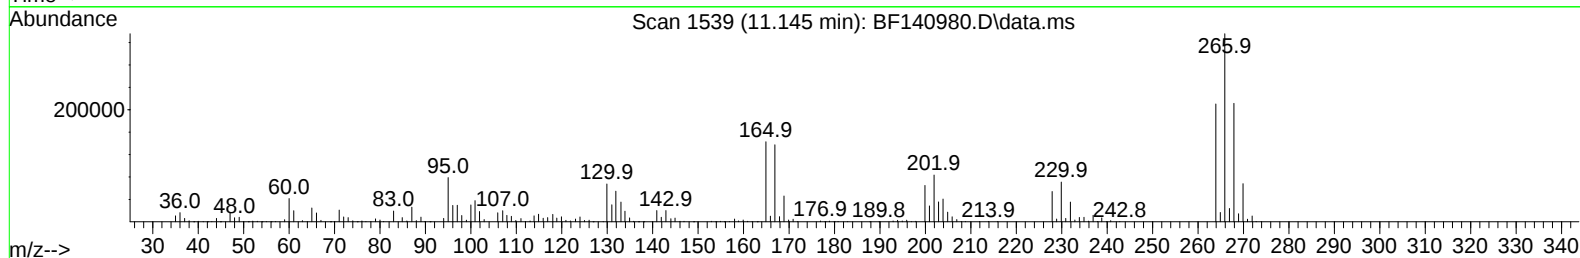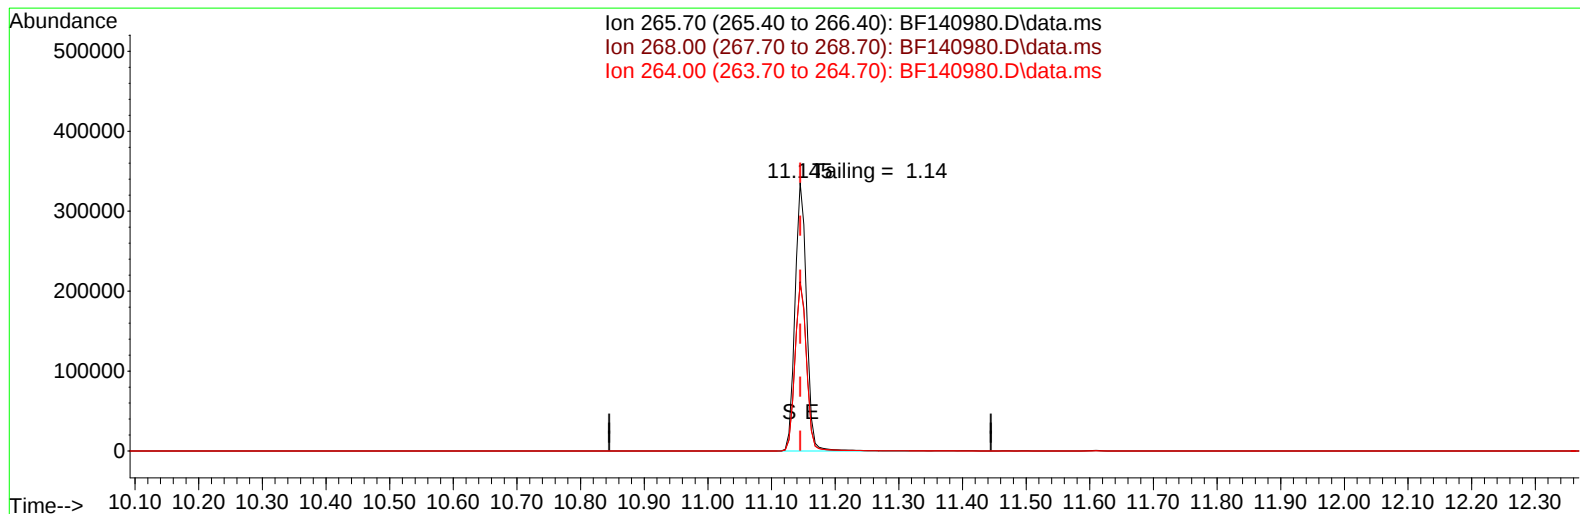

TIC: BF140980.D\data.ms

(70) Pentachlorophenol (C)

11.145min (-0.000) 34975.88 ng




response 426475

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.00
264.00	62.80	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122724\
Data File : BF140980.D
Acq On : 27 Dec 2024 07:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 27 10:40:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

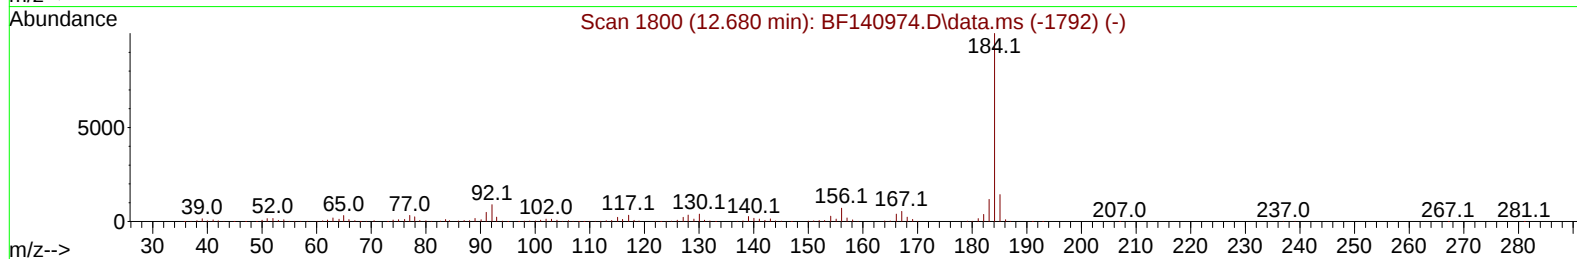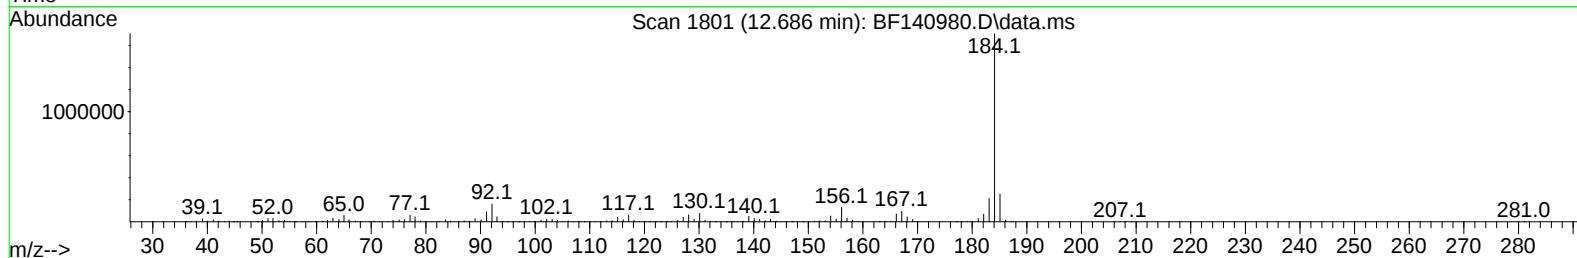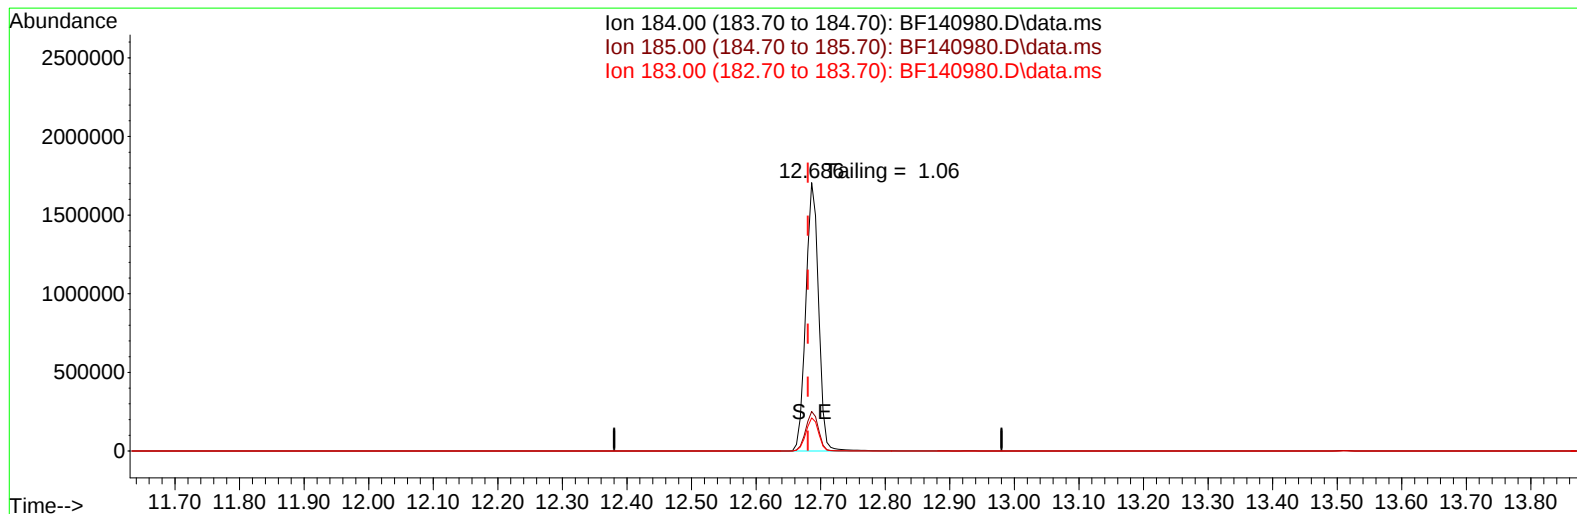

TIC: BF140980.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 38443.56 ng

response 2340716

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.75
183.00	11.70	12.36
0.00	0.00	0.00