
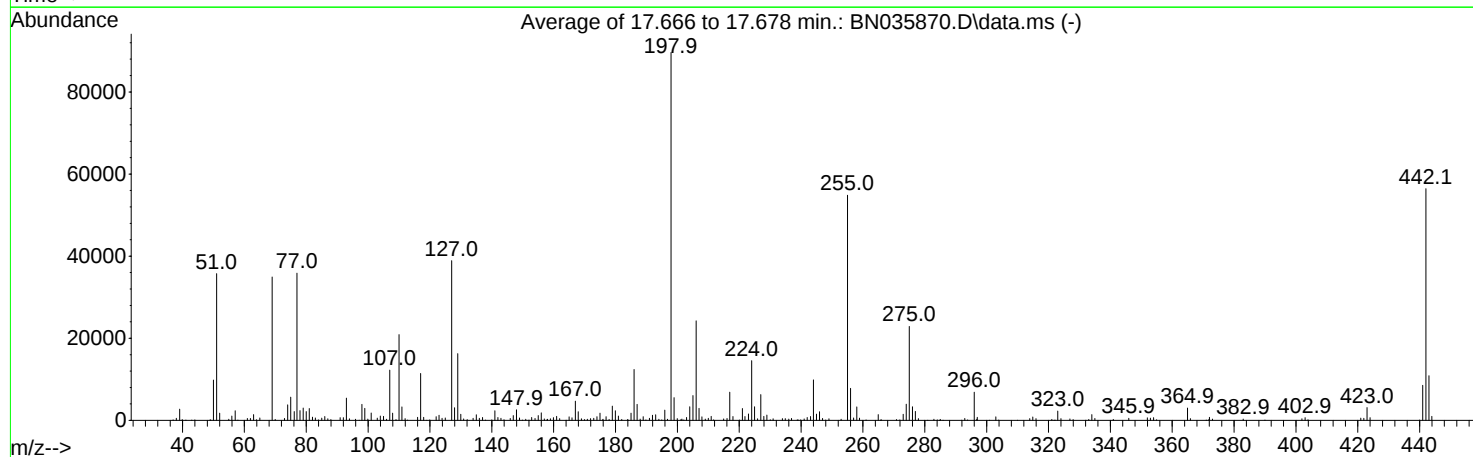


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010225\
Data File : BN035870.D
Acq On : 02 Jan 2025 10:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN010225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 02 15:39:17 2025

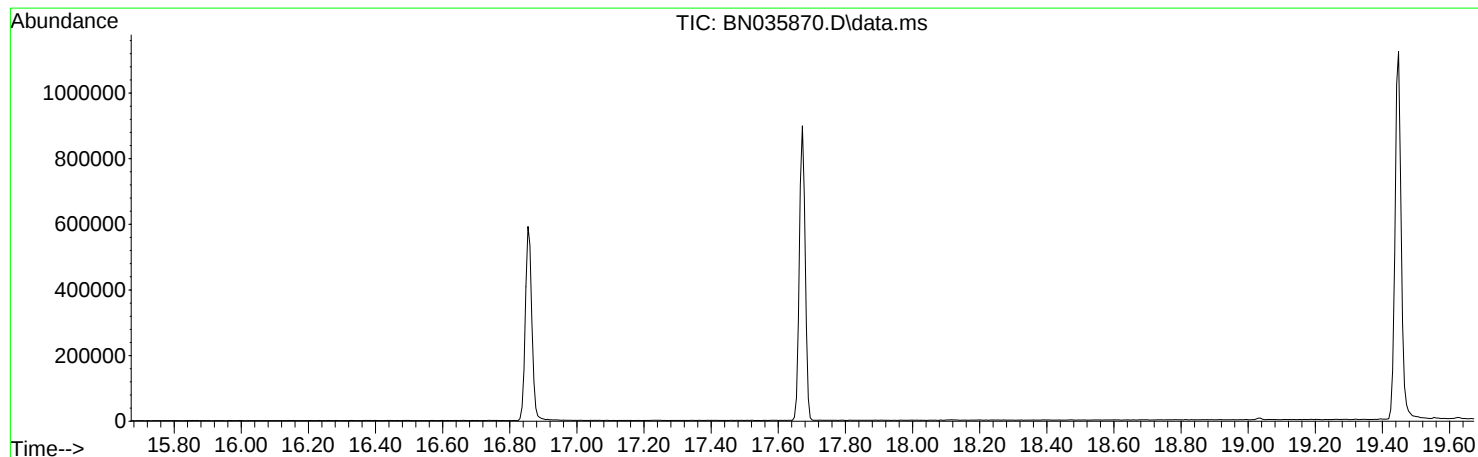

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	35733	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.0	34920	PASS
70	69	0.00	2	0.7	232	PASS
127	198	10	80	43.4	38907	PASS
197	198	0.00	2	0.3	256	PASS
198	198	100	100	100.0	89616	PASS
199	198	5	9	6.2	5523	PASS
275	198	10	60	25.6	22899	PASS
365	198	1	100	3.3	2996	PASS
441	198	0.01	100	9.5	8544	PASS
442	442	50	100	100.0	56448	PASS
443	442	15	24	19.3	10868	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/2/2025	BNA_N	<u>BN035870.D</u>
Compound Name	Response	Retention Time
DDT	243994	20.695
DDD	3023	20.307
DDE	79	19.748
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3102	247096	1.26

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010225\
Data File : BN035870.D
Acq On : 02 Jan 2025 10:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 02 12:15:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

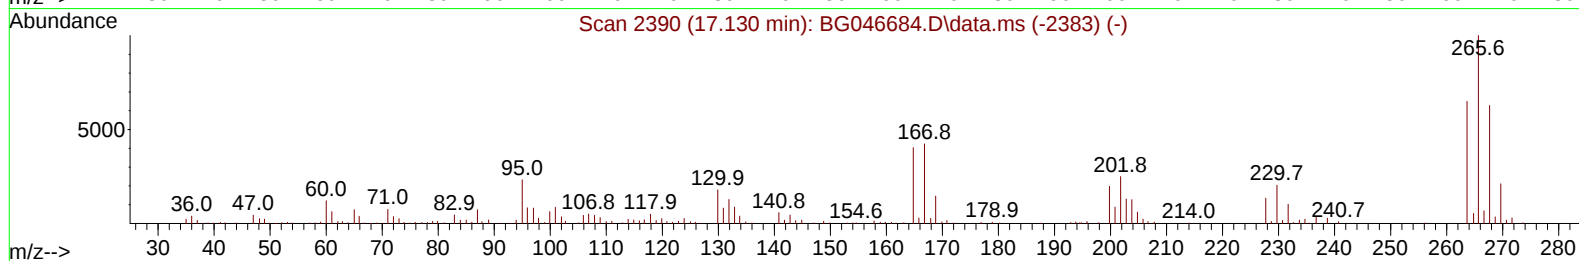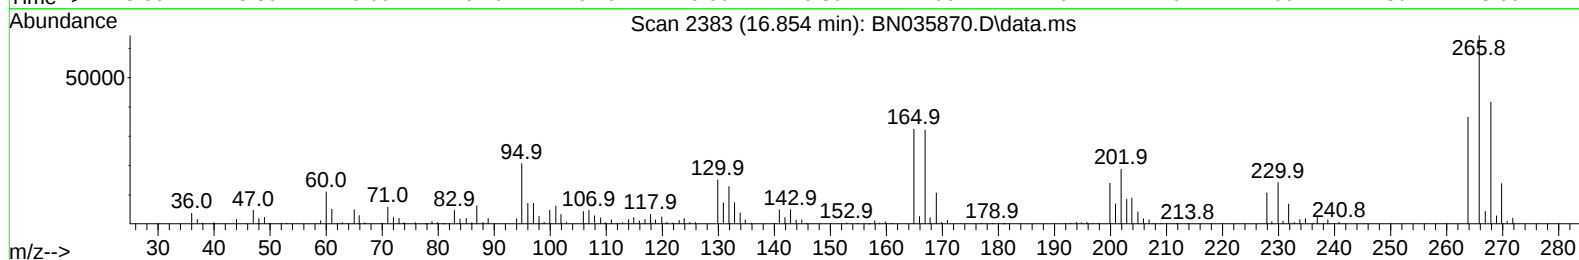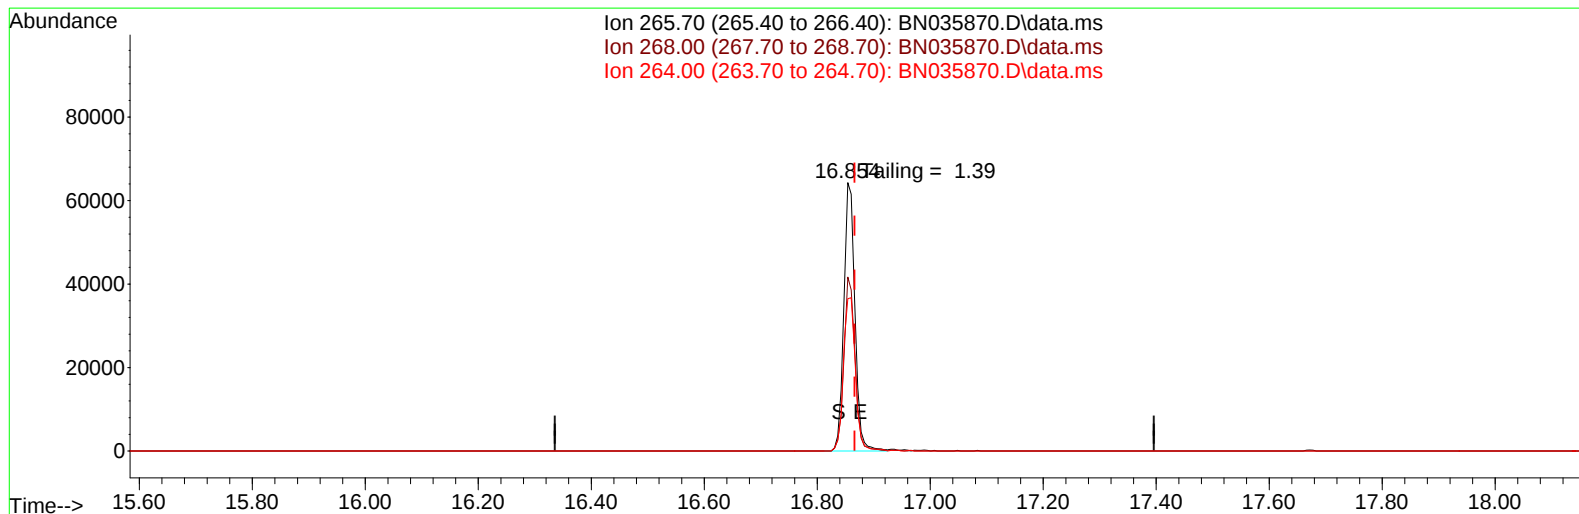

TIC: BN035870.D\data.ms

(70) Pentachlorophenol (C)

16.854min (-0.012) 32111.49 ng




response 87193

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.79
264.00	61.60	56.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010225\
Data File : BN035870.D
Acq On : 02 Jan 2025 10:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 02 12:15:33 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

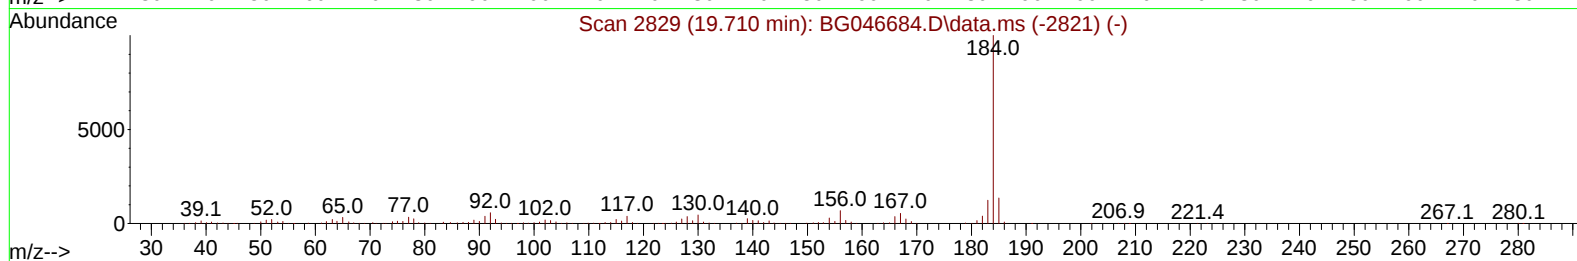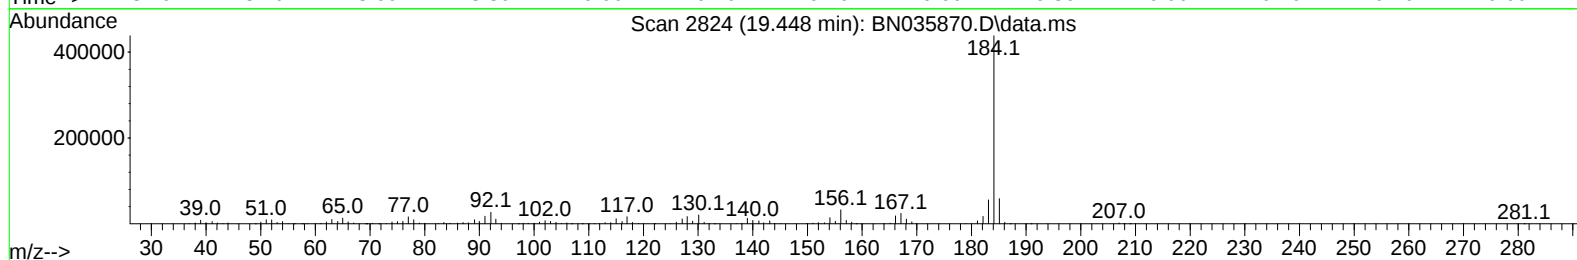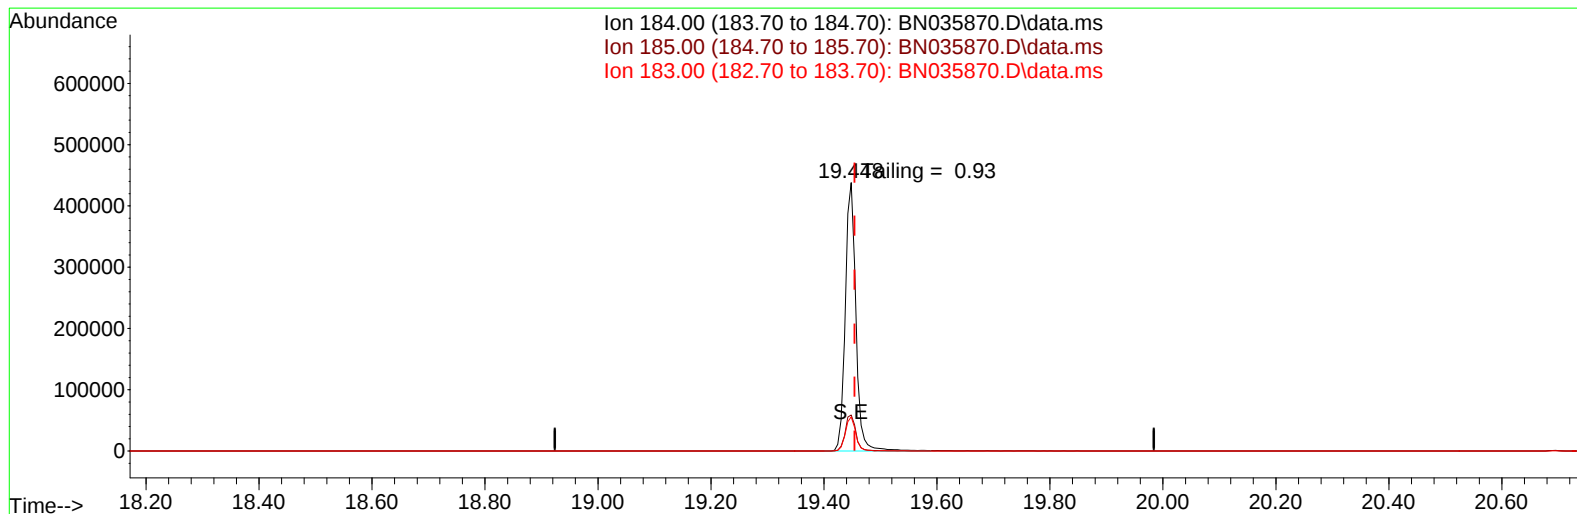

TIC: BN035870.D\data.ms

(77) Benzidine

19.448min (-0.006) 0.00 ng

response 567773

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.41
183.00	13.20	12.73
0.00	0.00	0.00