


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010625\
Data File : BN035888.D
Acq On : 06 Jan 2025 09:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN010225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 02 15:39:17 2025

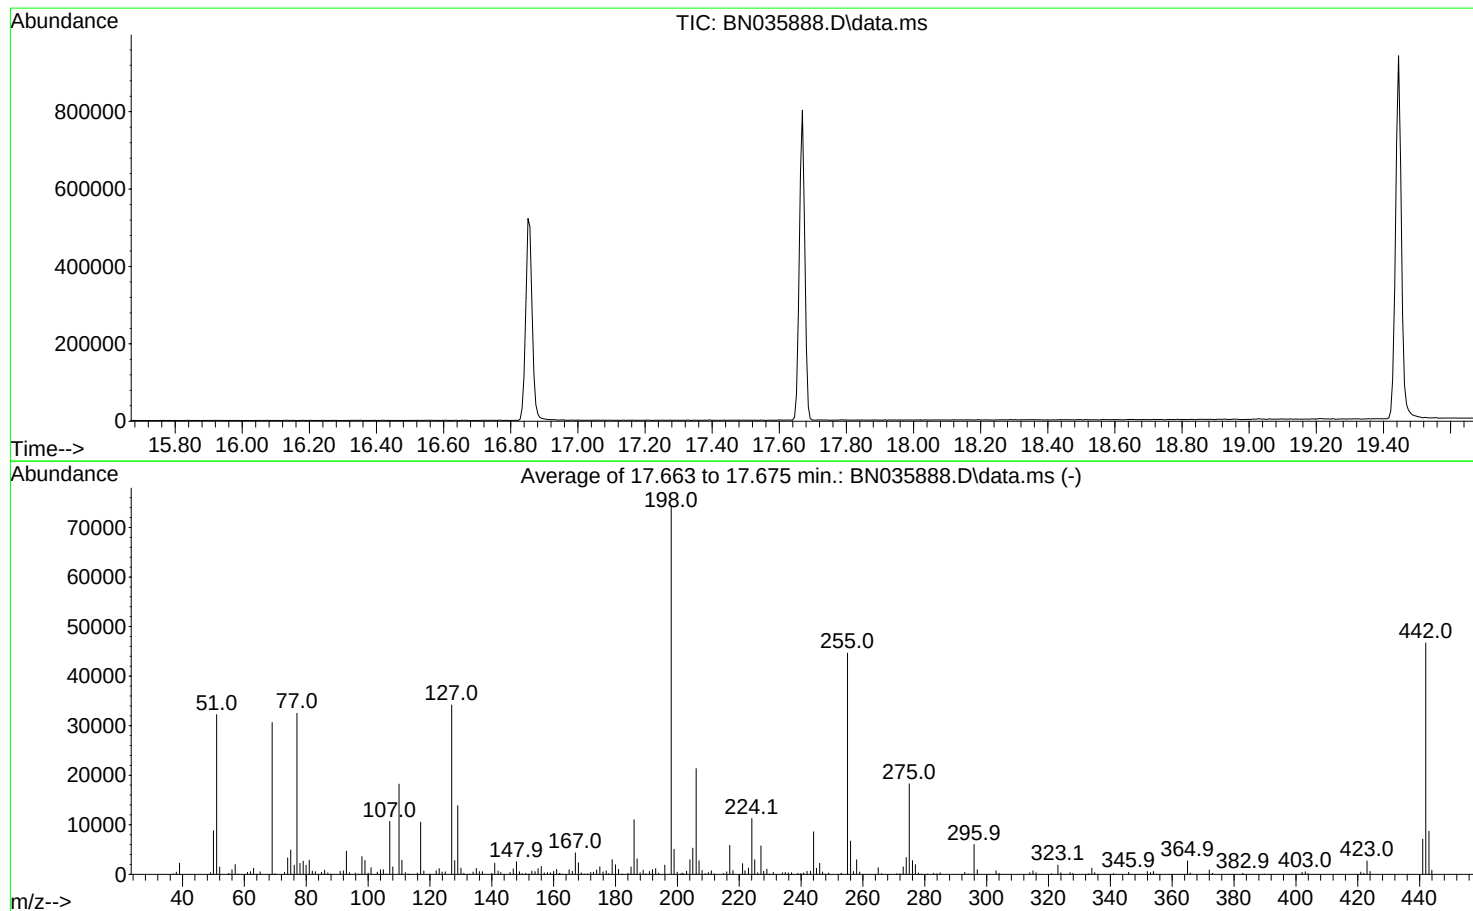

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	32224	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.3	30653	PASS
70	69	0.00	2	0.4	134	PASS
127	198	10	80	46.0	34168	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74227	PASS
199	198	5	9	6.8	5079	PASS
275	198	10	60	24.6	18271	PASS
365	198	1	100	3.6	2705	PASS
441	198	0.01	100	9.6	7094	PASS
442	442	50	100	100.0	46680	PASS
443	442	15	24	18.6	8694	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/6/2025	BNA_N	<u>BN035888.D</u>
Compound Name	Response	Retention Time
DDT	192811	20.692
DDD	2725	20.251
DDE	146	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2871	195682	1.47

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010625\
Data File : BN035888.D
Acq On : 06 Jan 2025 09:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 06 13:15:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

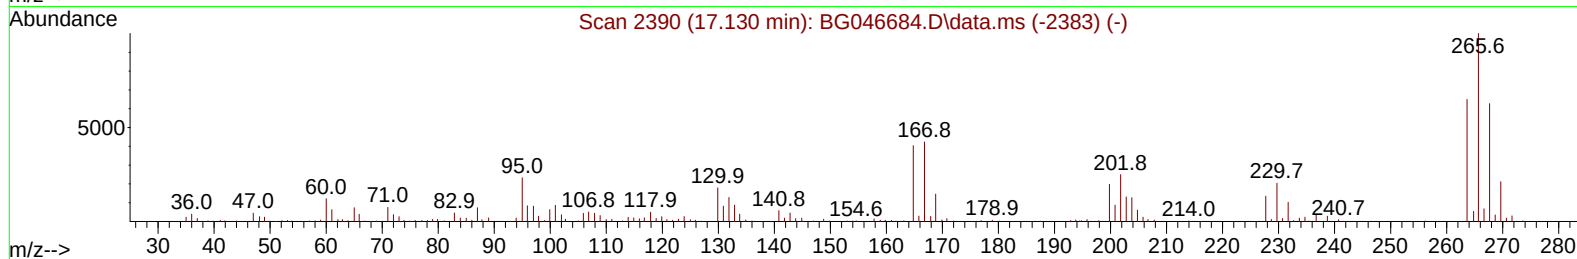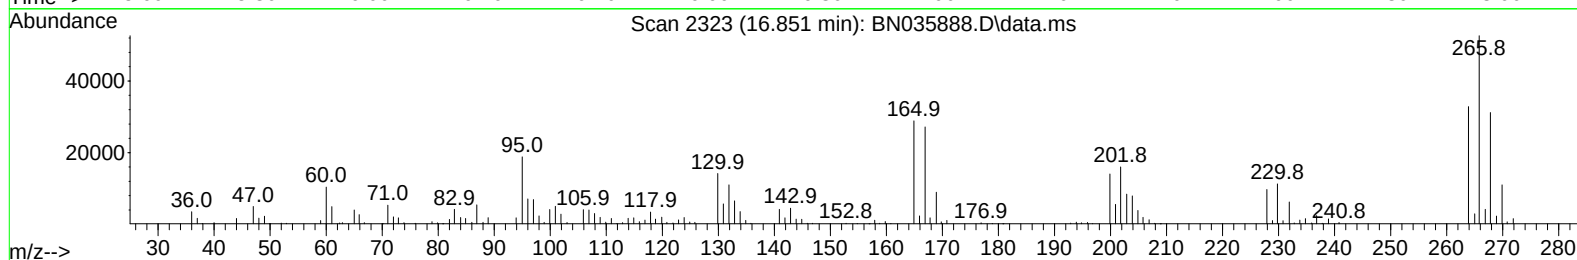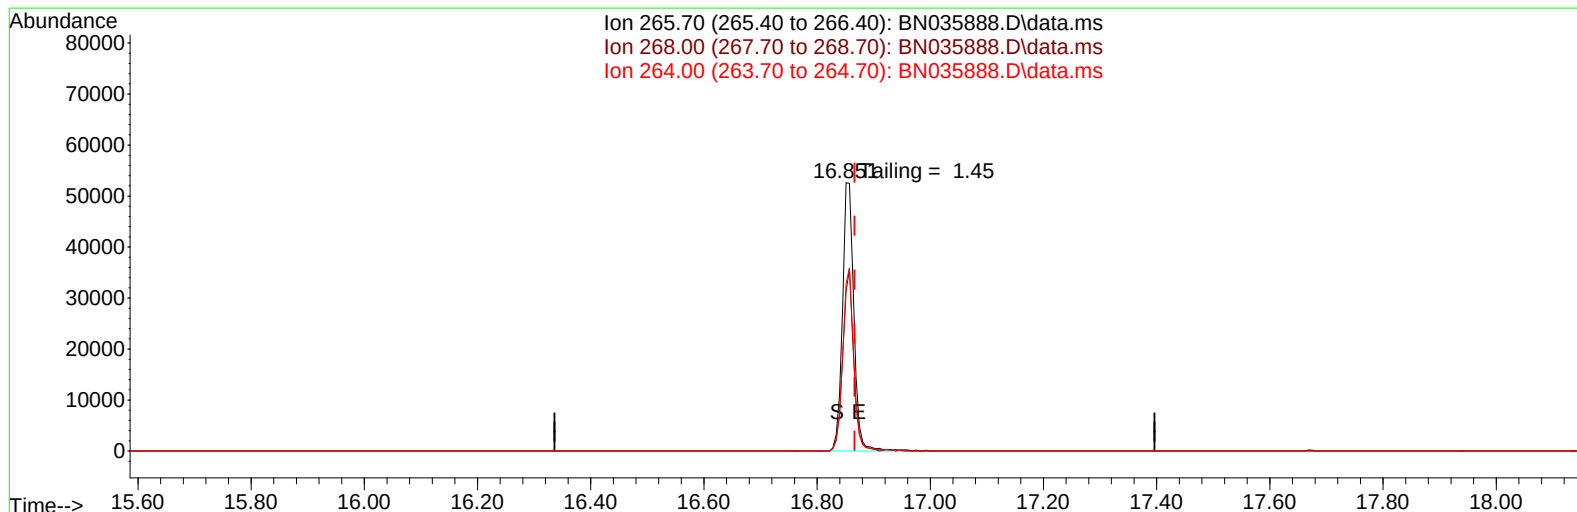

TIC: BN035888.D\data.ms

(70) Pentachlorophenol (C)

16.851min (-0.015) 21827.15 ng




response 73999

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.23
264.00	61.60	62.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010625\
Data File : BN035888.D
Acq On : 06 Jan 2025 09:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 06 13:15:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

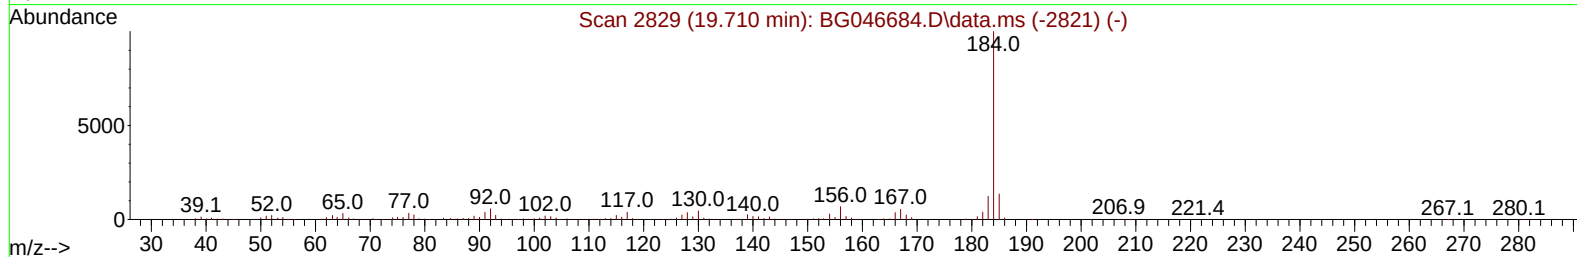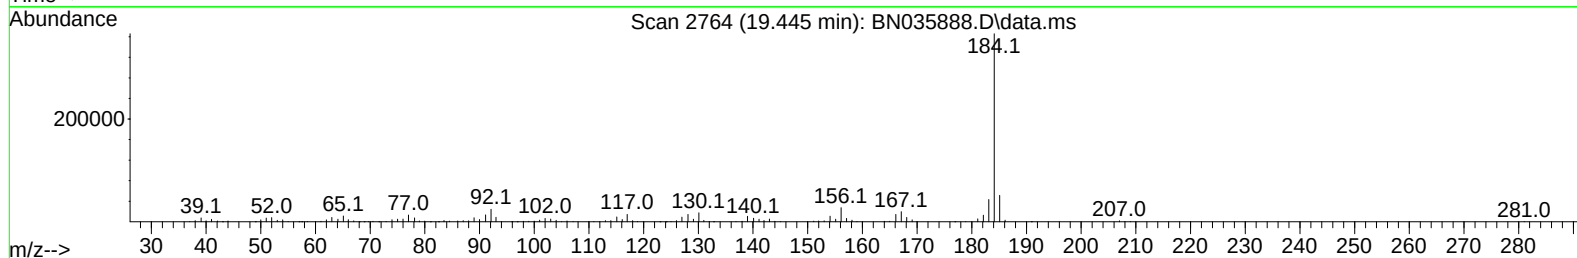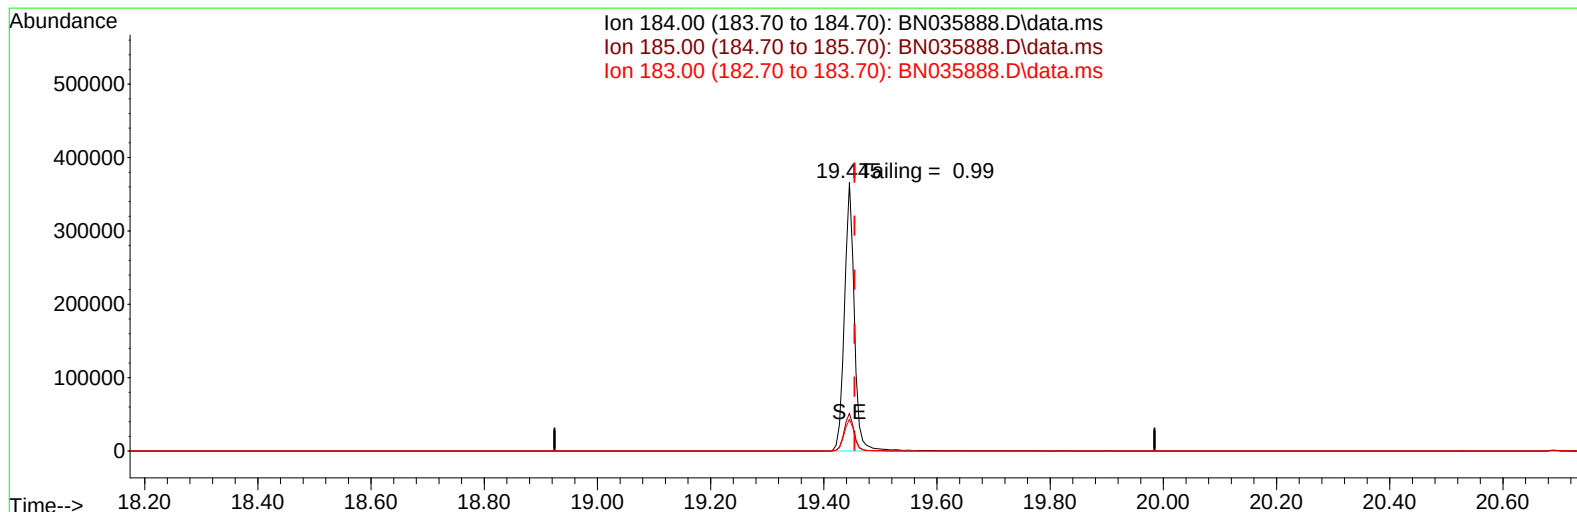

TIC: BN035888.D\data.ms

(77) Benzidine

19.445min (-0.009) 0.00 ng

response 444563

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	11.86
0.00	0.00	0.00